

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 11:44
 Operator : UA
 Sample : J3465-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 13:19:56 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.825	11.198	104.9E6	95526323	297.207	304.125
Target Compounds							
2) T	3,5-DICHL...	0.000	9.282	0	4110519	N.D.	9.310 #
3) T	4-Nitroph...	11.484	10.355	4914251	4903159	21.098	26.328
5) T	DICAMBA	0.000	11.443	0	5240237	N.D.	4.737 #
6) T	MCP	12.524	0.000	3075674	0	2.755	N.D. #
11) T	2,4,5-TP ...	0.000	14.182	0	23122766	N.D.	13.443 #
15) T	Picloram	0.000	17.153	0	1018862	N.D.	0.478 #
16) T	DCPA	0.000	17.153	0	1018862	N.D.	0.493 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 11:44
Operator : UA
Sample : J3465-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 13:19:56 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

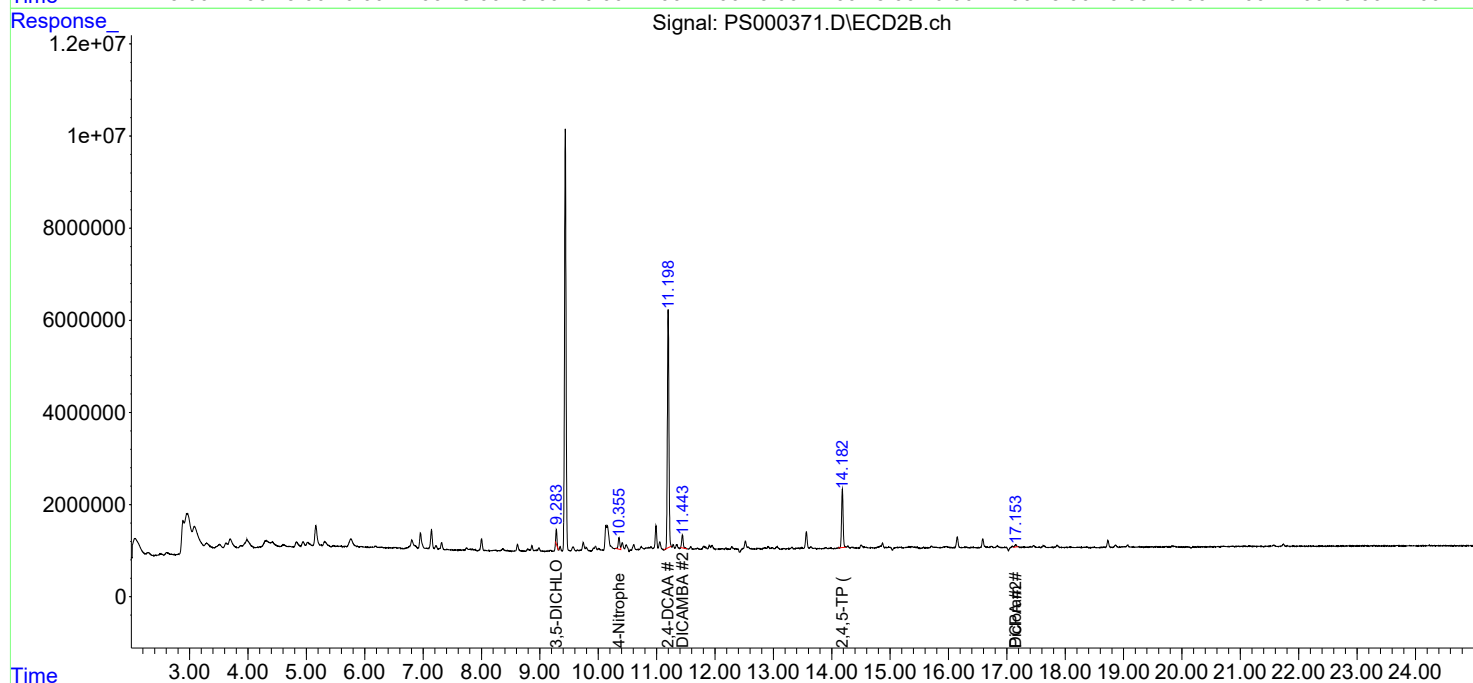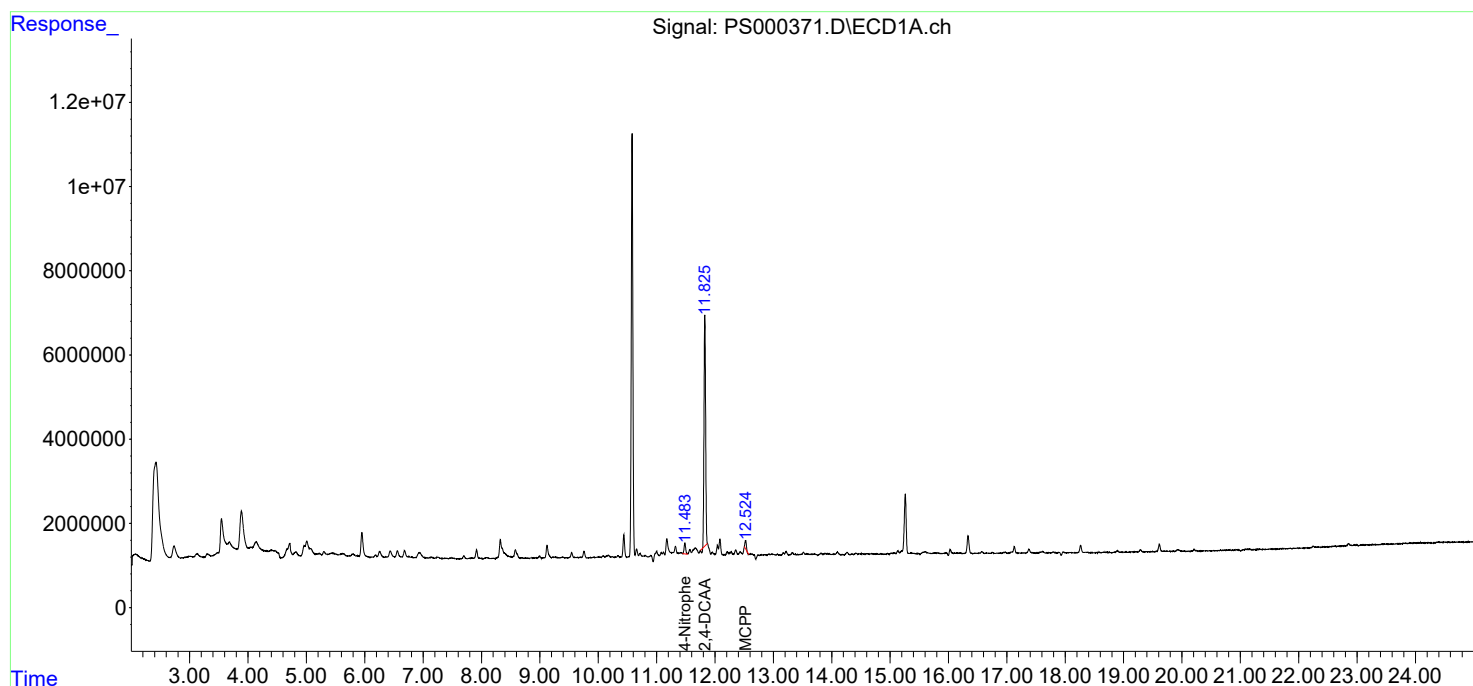


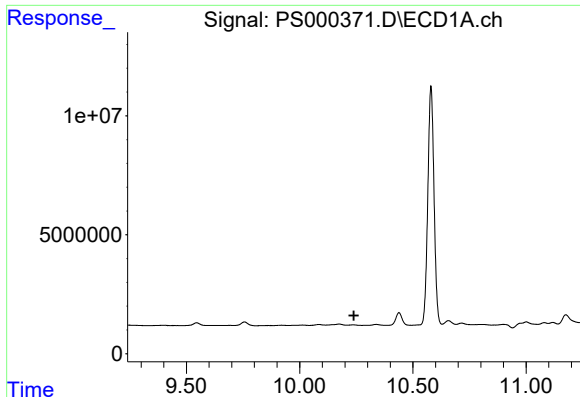

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

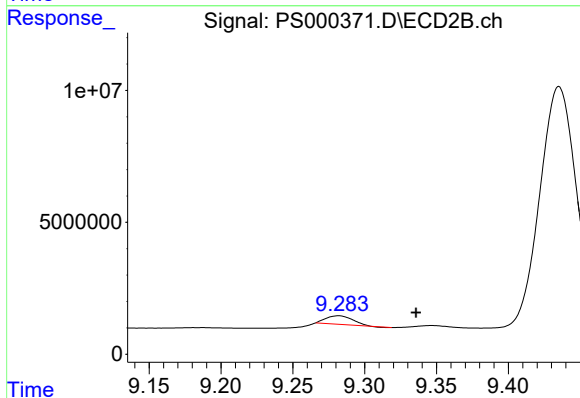


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.282 min
Delta R.T.: -0.054 min
Response: 4110519
Conc: 9.31 ng/ml

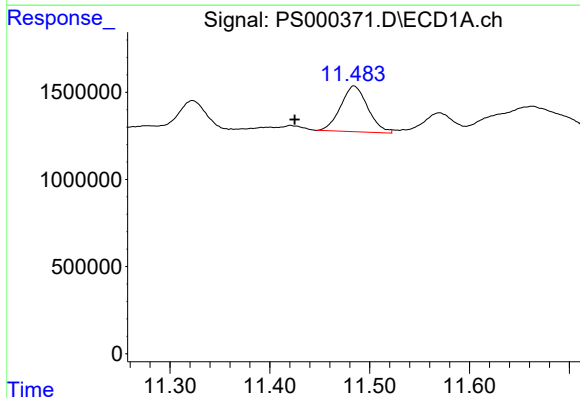


#3 4-Nitrophenol

R.T.: 11.484 min
Delta R.T.: 0.059 min
Response: 4914251
Conc: 21.10 ng/ml

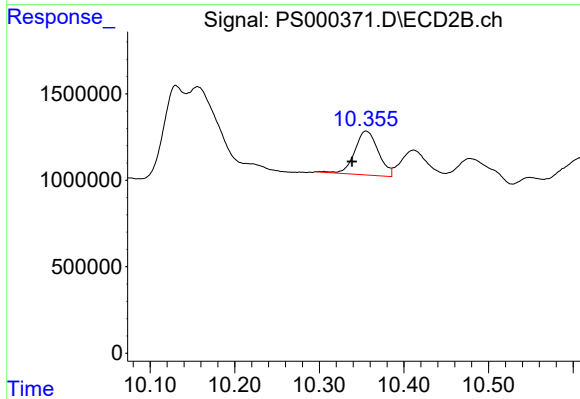

#3 4-Nitrophenol


R.T.: 10.355 min
Delta R.T.: 0.017 min
Response: 4903159
Conc: 26.33 ng/ml

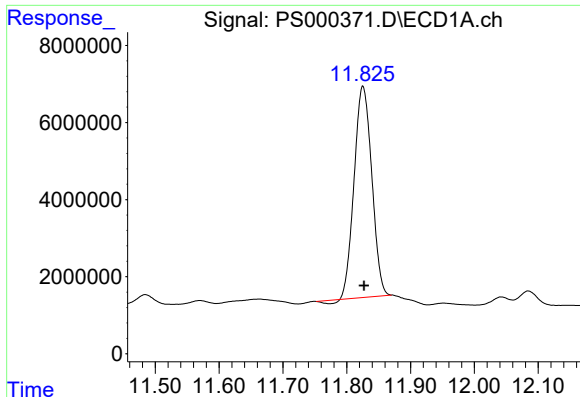

#4 2,4-DCAA


R.T.: 11.825 min
Delta R.T.: -0.002 min
Response: 104936648
Conc: 297.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

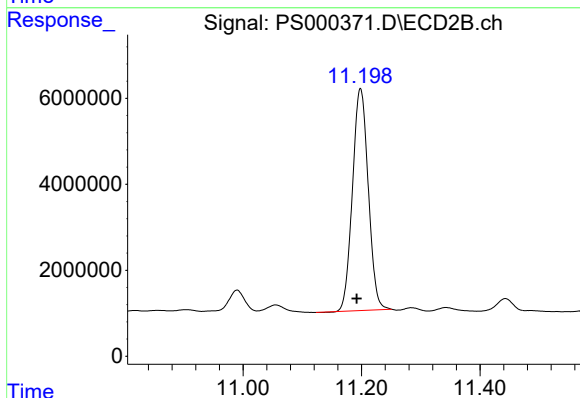


#4 2,4-DCAA

R.T.: 11.198 min
Delta R.T.: 0.006 min
Response: 95526323
Conc: 304.13 ng/ml

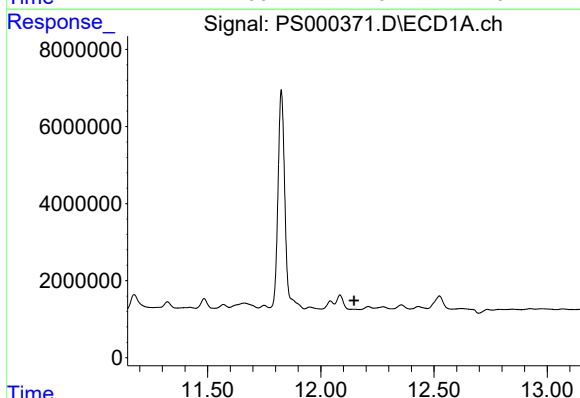


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.147 min
Response: 0
Conc: N.D.

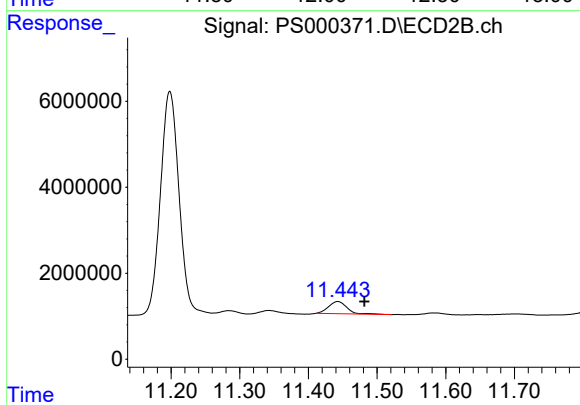

#5 DICAMBA


R.T.: 11.443 min
Delta R.T.: -0.039 min
Response: 5240237
Conc: 4.74 ng/ml

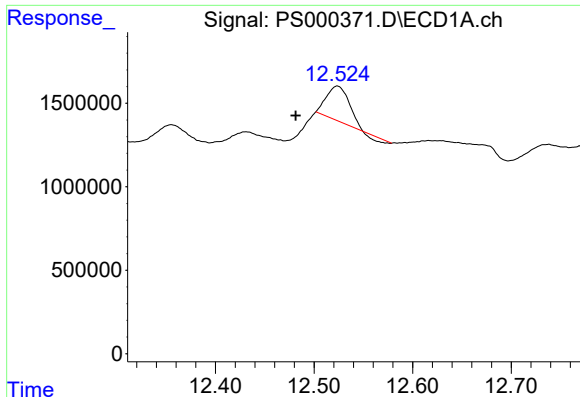

#6 MCP


R.T.: 12.524 min
Delta R.T.: 0.042 min
Response: 3075674
Conc: 2.76 ug/ml

Instrument :
ECD_S
ClientSampleId :

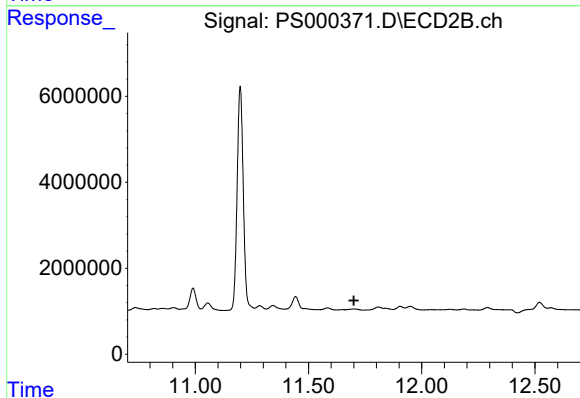


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.700 min
Response: 0
Conc: N.D.

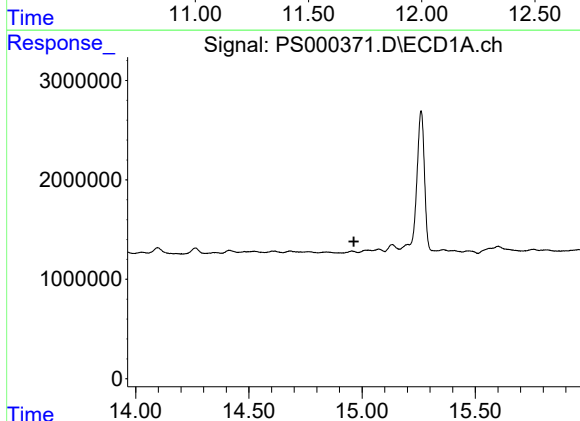


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.964 min
Response: 0
Conc: N.D.

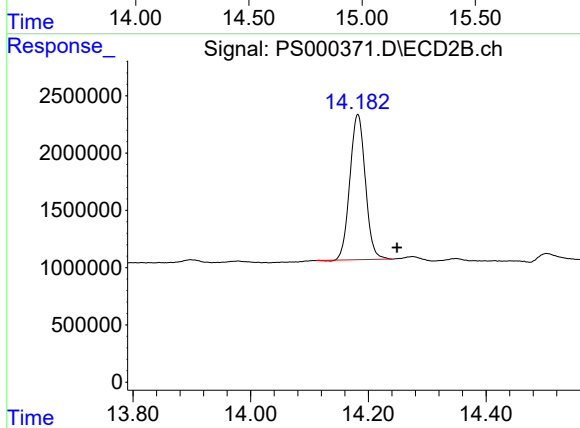

#11 2,4,5-TP (SILVEX)


R.T.: 14.182 min
Delta R.T.: -0.067 min
Response: 23122766
Conc: 13.44 ng/ml

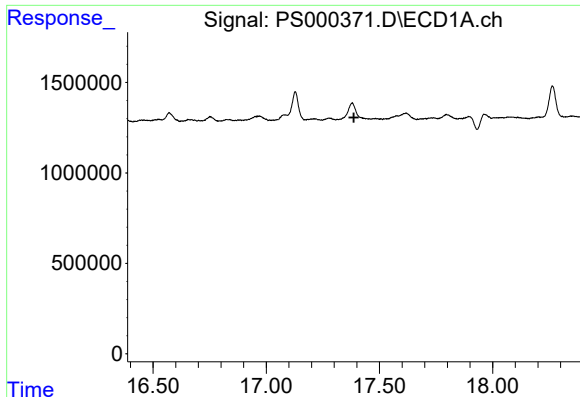

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

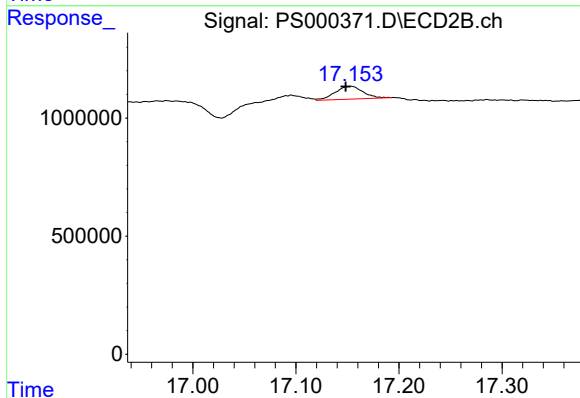


#15 Picloram

R.T.: 17.153 min
Delta R.T.: 0.005 min
Response: 1018862
Conc: 0.48 ng/ml

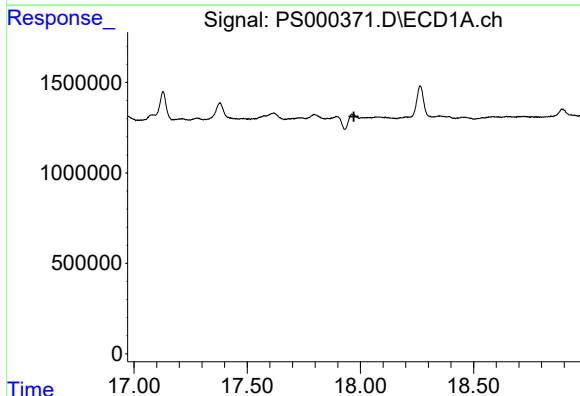

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.971 min
Response: 0
Conc: N.D.

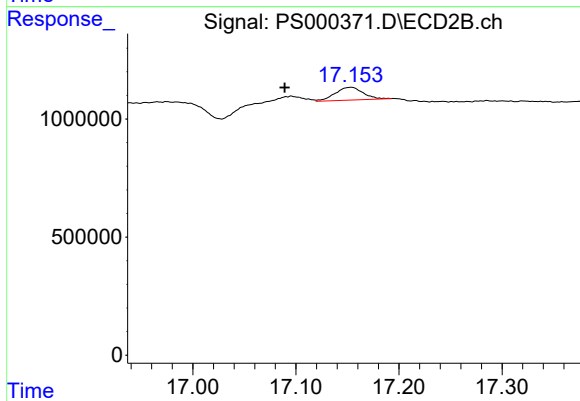

#16 DCPA

R.T.: 17.153 min
Delta R.T.: 0.064 min
Response: 1018862
Conc: 0.49 ng/ml