

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 16:22
 Operator : UA
 Sample : J3241-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 22:52:02 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.857	11.232	79017114	52959479	223.796	168.606
Target Compounds							
2) T	3,5-DICHL...	0.000	9.316	0	6908804	N.D.	15.648 #
3) T	4-Nitroph...	0.000	10.389	0	4208943	N.D.	22.600 #
5) T	DICAMBA	0.000	11.476	0	4954197	N.D.	4.478 #
6) T	MCP	12.551	0.000	8844876	0	7.923	N.D. #
10) T	Pentachlo...	0.000	13.598	0	8301791	N.D.	1.884 #
11) T	2,4,5-TP ...	0.000	14.215	0	20776382	N.D.	12.079 #
13) T	2,4-DB	16.063	0.000	3148309	0	11.579	N.D. #
15) T	Picloram	0.000	17.187	0	583698	N.D.	0.274 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 16:22
Operator : UA
Sample : J3241-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 22:52:02 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

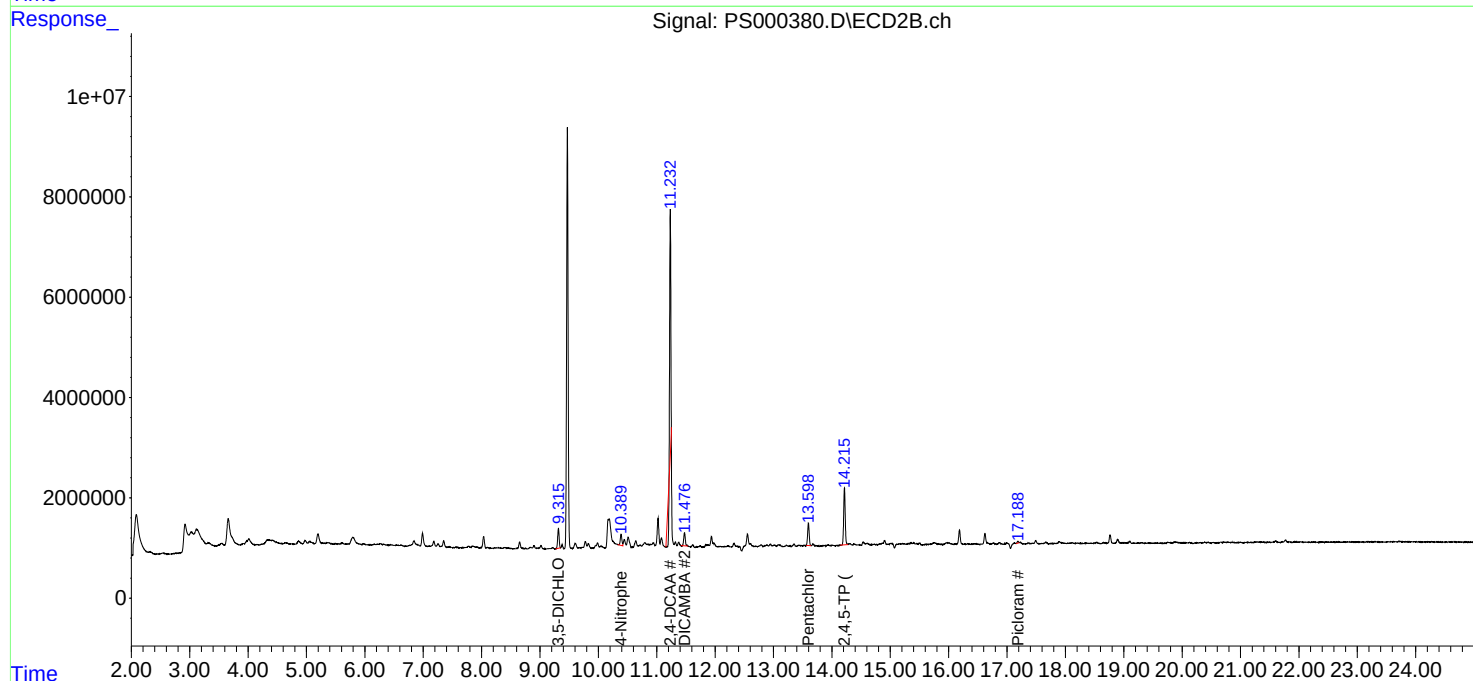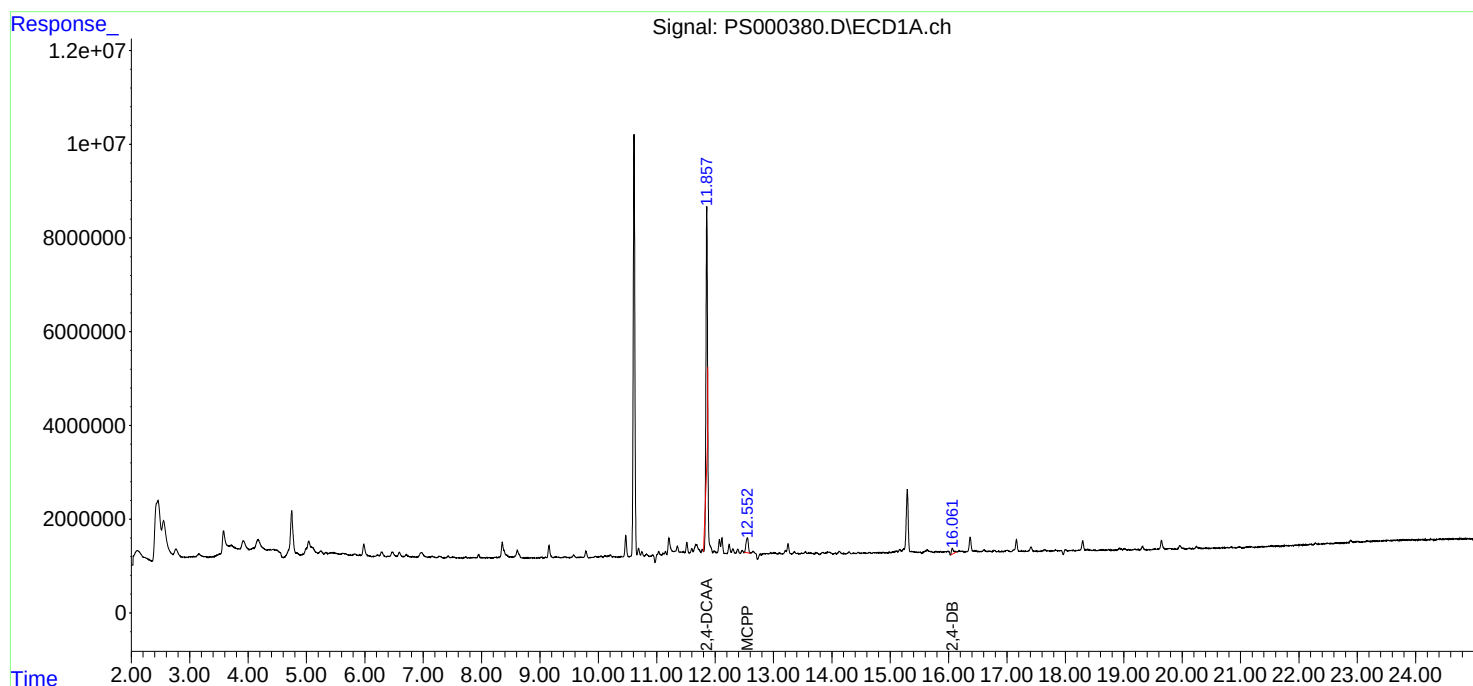


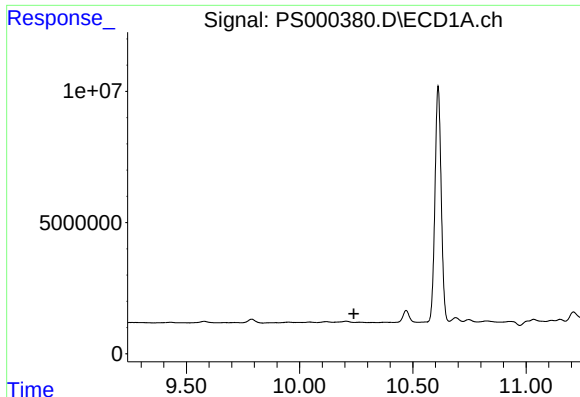

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

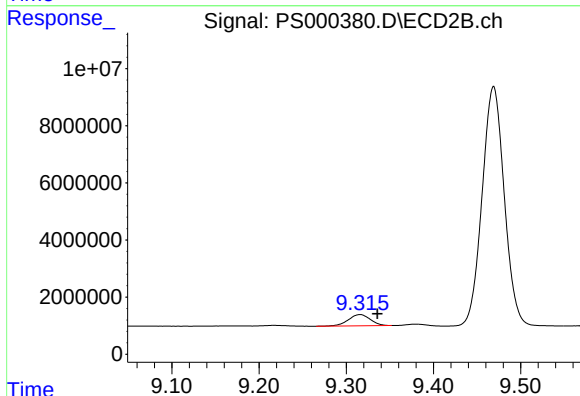


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.316 min
Delta R.T.: -0.020 min
Response: 6908804
Conc: 15.65 ng/ml

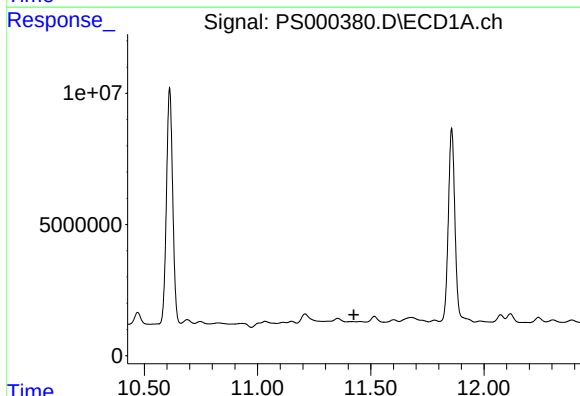


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.425 min
Response: 0
Conc: N.D.

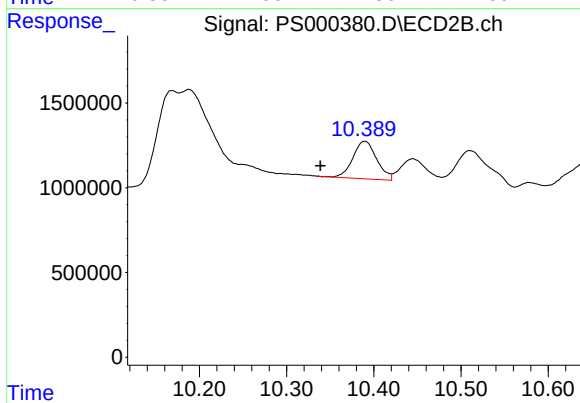

#3 4-Nitrophenol


R.T.: 10.389 min
Delta R.T.: 0.051 min
Response: 4208943
Conc: 22.60 ng/ml

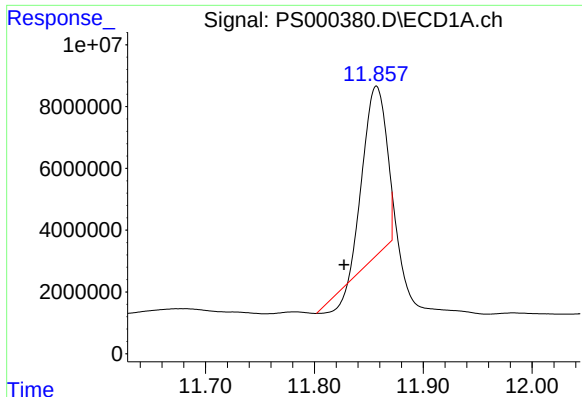

#4 2,4-DCAA


R.T.: 11.857 min
Delta R.T.: 0.030 min
Response: 79017114
Conc: 223.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

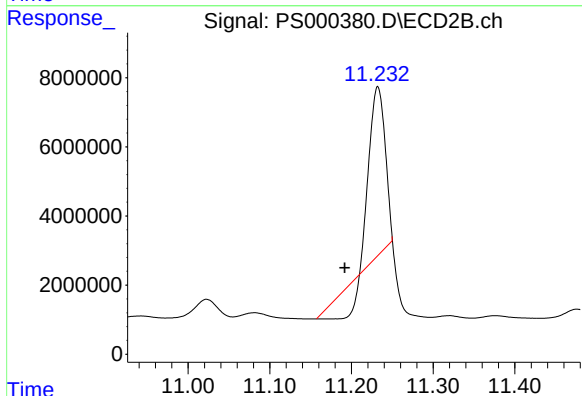


#4 2,4-DCAA

R.T.: 11.232 min
Delta R.T.: 0.040 min
Response: 52959479
Conc: 168.61 ng/ml

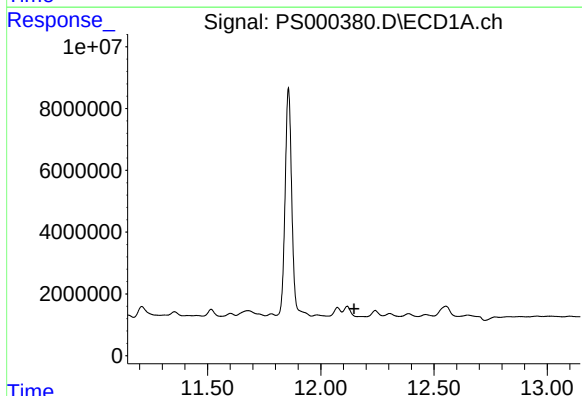


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.147 min
Response: 0
Conc: N.D.

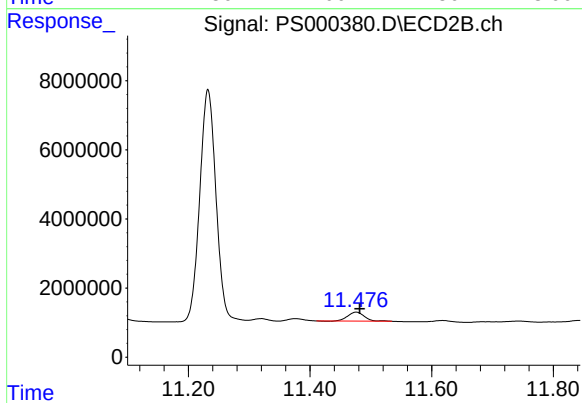

#5 DICAMBA


R.T.: 11.476 min
Delta R.T.: -0.006 min
Response: 4954197
Conc: 4.48 ng/ml

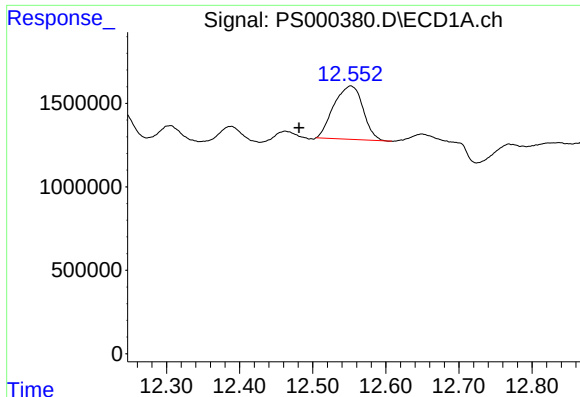

#6 MCP


R.T.: 12.551 min
Delta R.T.: 0.070 min
Response: 8844876
Conc: 7.92 ug/ml

Instrument :
ECD_S
ClientSampleId :

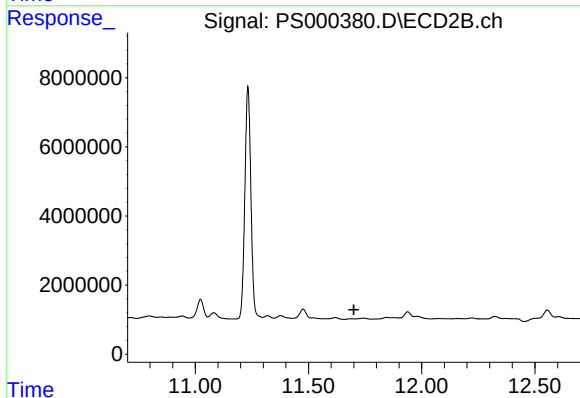


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.700 min
Response: 0
Conc: N.D.

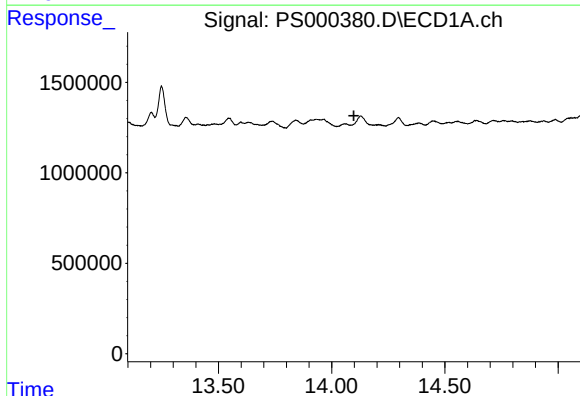


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 14.098 min
Response: 0
Conc: N.D.

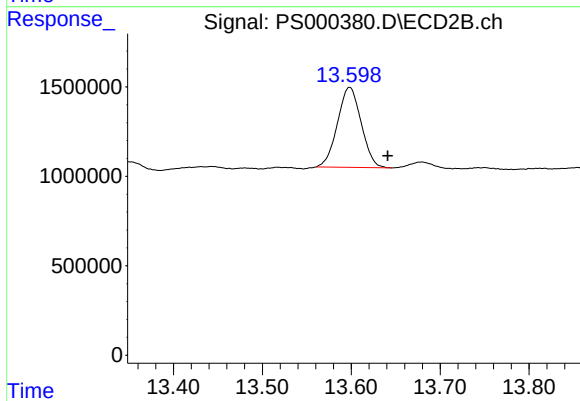

#10 Pentachlorophenol


R.T.: 13.598 min
Delta R.T.: -0.043 min
Response: 8301791
Conc: 1.88 ng/ml

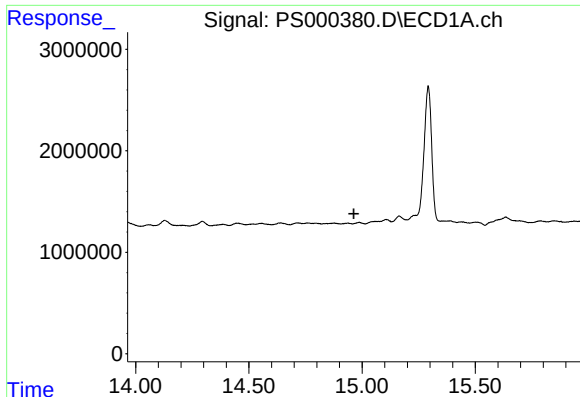

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

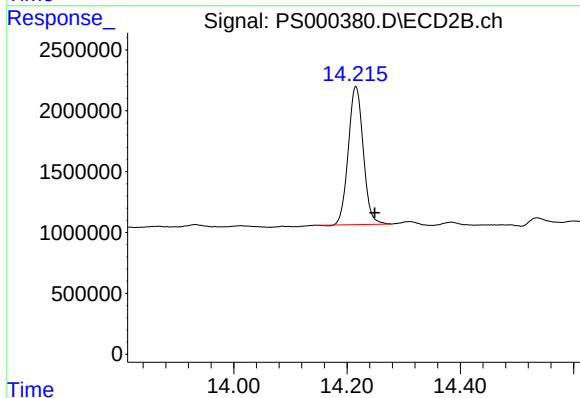


#11 2,4,5-TP (SILVEX)

R.T.: 14.215 min
Delta R.T.: -0.034 min
Response: 20776382
Conc: 12.08 ng/ml

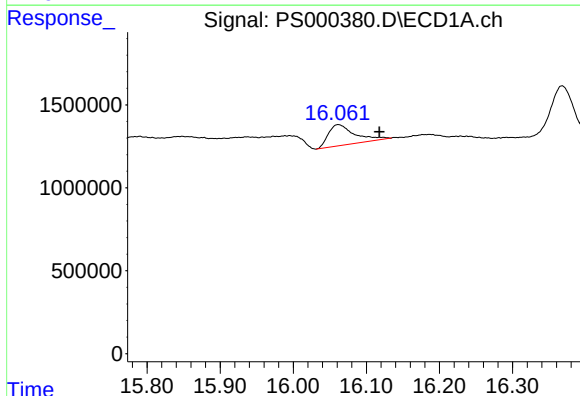


#13 2,4-DB

R.T.: 16.063 min
Delta R.T.: -0.055 min
Response: 3148309
Conc: 11.58 ng/ml

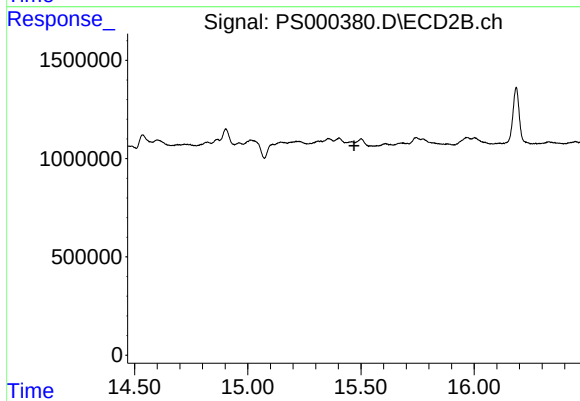

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.469 min
Response: 0
Conc: N.D.

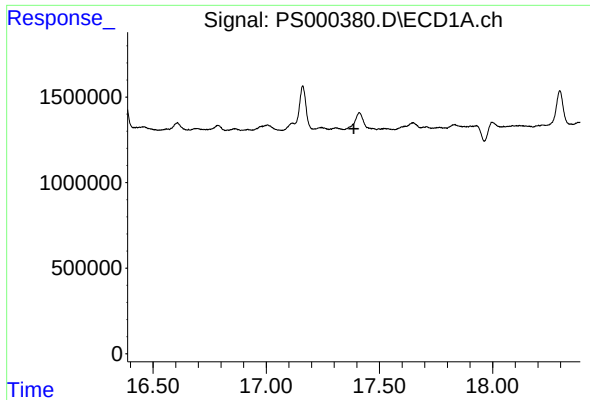

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

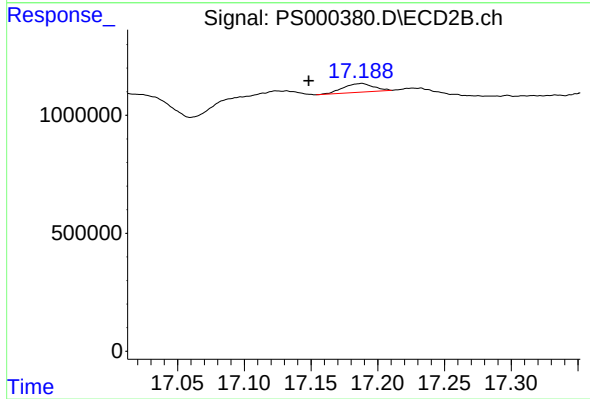

#15 Picloram

R.T.: 17.187 min
Delta R.T.: 0.039 min
Response: 583698
Conc: 0.27 ng/ml