

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 23:35
 Operator : UA
 Sample : J3498-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 02:05:52 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.791	11.167	152.6E6	131.3E6	432.137	417.929
Target Compounds							
2) T	3,5-DICHL...	0.000	9.403	0	124.7E6	N.D.	282.322 #
3) T	4-Nitroph...	11.450	10.324	5197836	5503064	22.315	29.549 #
6) T	MCP	12.472	0.000	8690561	0	7.785	N.D. #
10) T	Pentachlo...	14.060	13.615	3147857	2014103	0.630	0.457 #
12) T	2,4,5-T	0.000	14.837	0	2941234	N.D.	1.785 #
15) T	Picloram	0.000	17.162	0	3304891	N.D.	1.551 #
16) T	DCPA	17.937	17.060	164509	4055147	0.068	1.962 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 23:35
Operator : UA
Sample : J3498-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 02:05:52 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

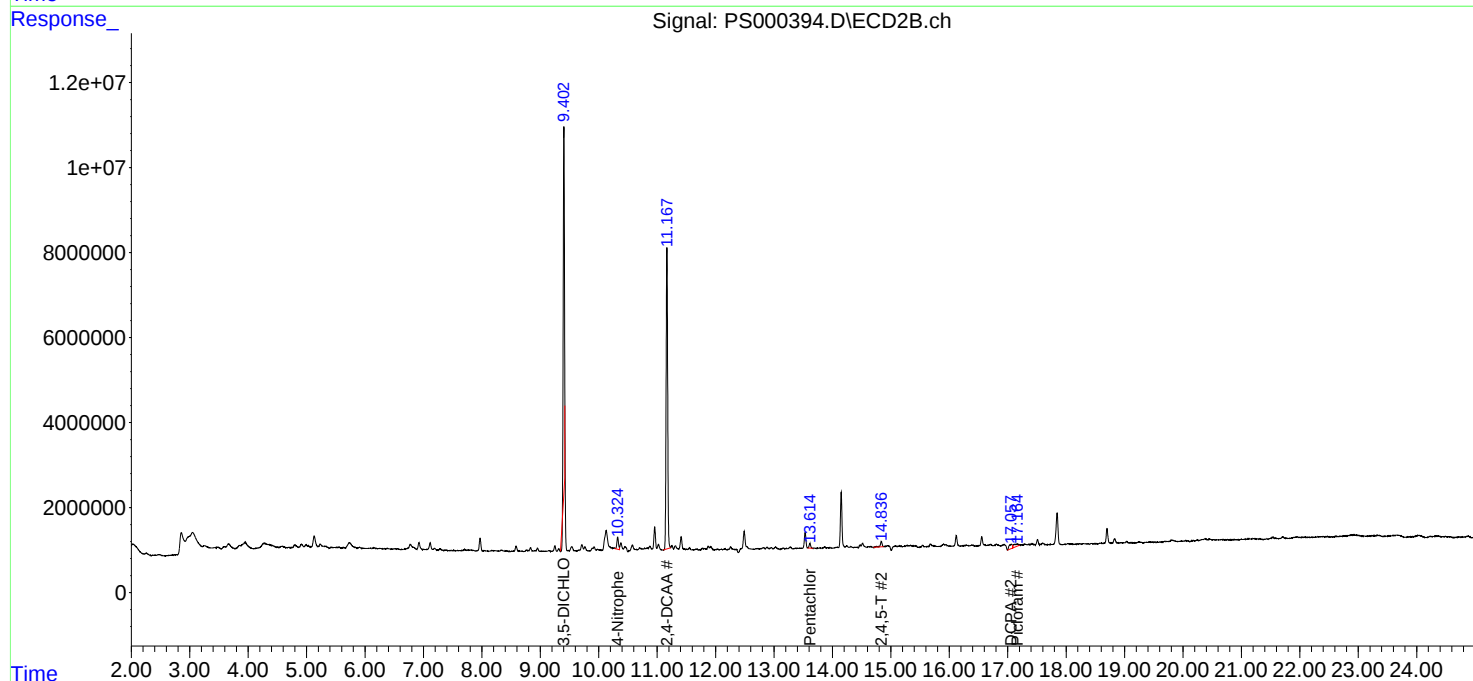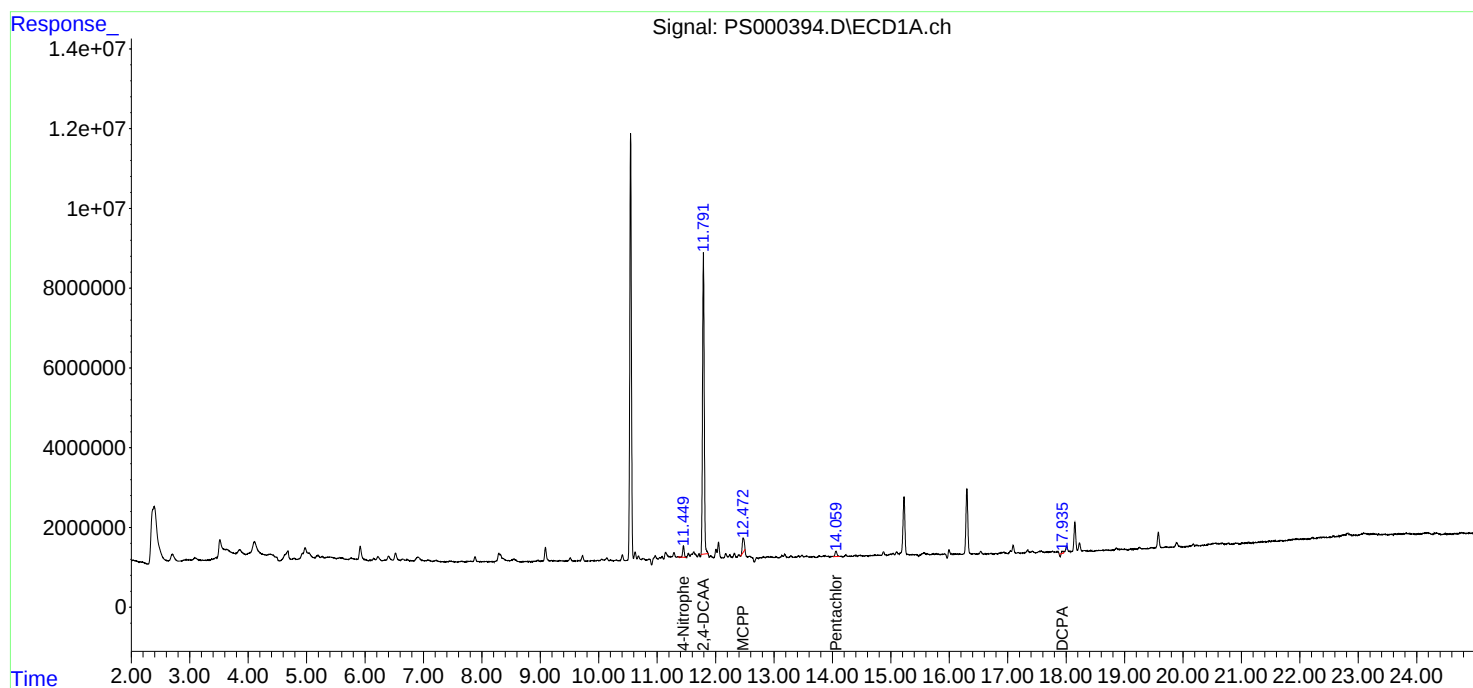


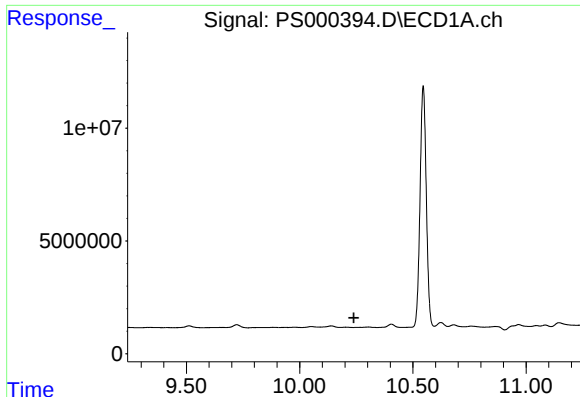

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

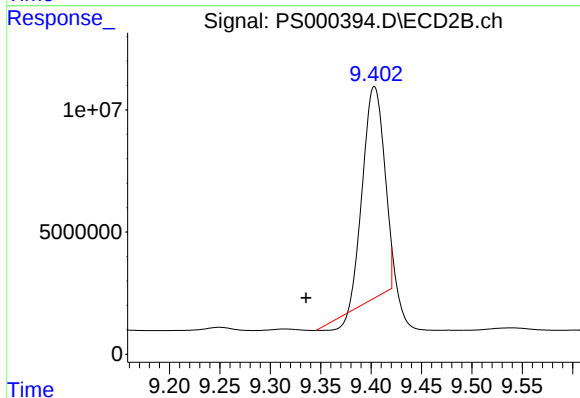


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.403 min
Delta R.T.: 0.068 min
Response: 124651737
Conc: 282.32 ng/ml

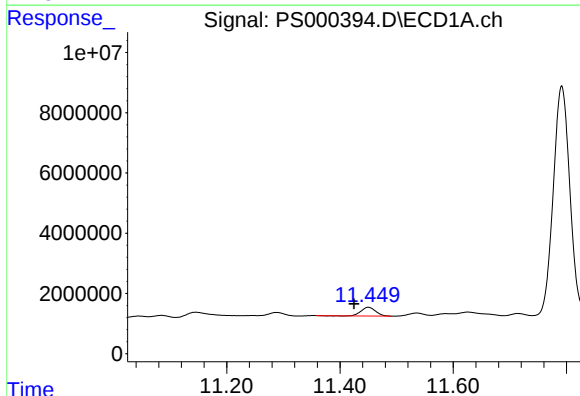


#3 4-Nitrophenol

R.T.: 11.450 min
Delta R.T.: 0.025 min
Response: 5197836
Conc: 22.32 ng/ml

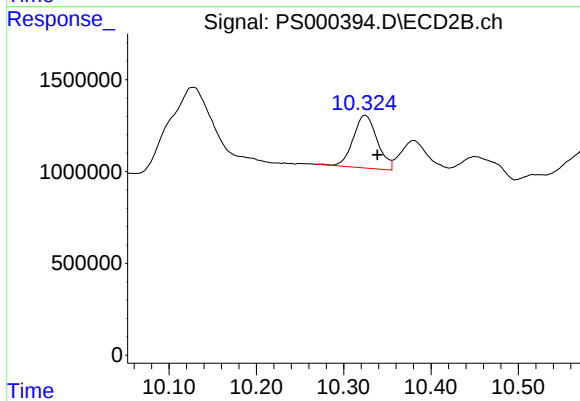

#3 4-Nitrophenol


R.T.: 10.324 min
Delta R.T.: -0.015 min
Response: 5503064
Conc: 29.55 ng/ml

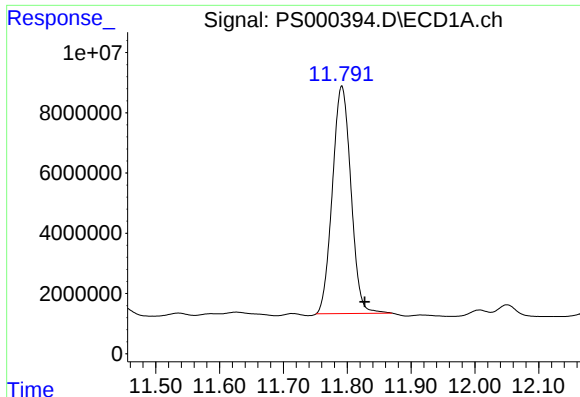

#4 2,4-DCAA


R.T.: 11.791 min
Delta R.T.: -0.036 min
Response: 152577392
Conc: 432.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

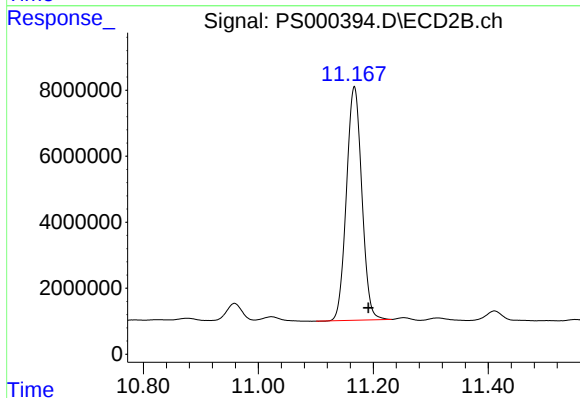


#4 2,4-DCAA

R.T.: 11.167 min
Delta R.T.: -0.025 min
Response: 131272347
Conc: 417.93 ng/ml

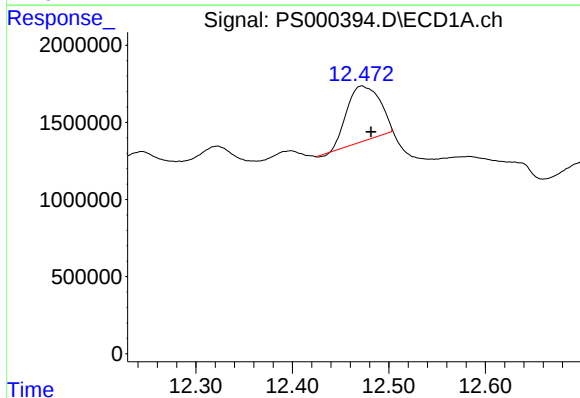


#6 MCP

R.T.: 12.472 min
Delta R.T.: -0.009 min
Response: 8690561
Conc: 7.78 ug/ml

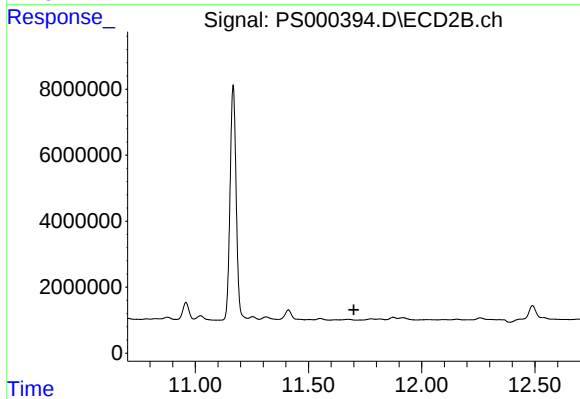

#6 MCP


R.T.: 0.000 min
Exp R.T. : 11.700 min
Response: 0
Conc: N.D.

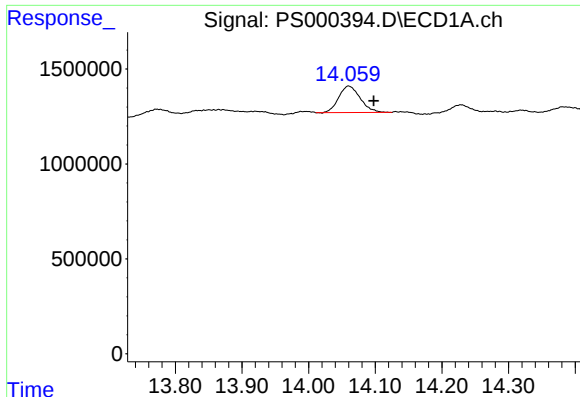

#10 Pentachlorophenol


R.T.: 14.060 min
Delta R.T.: -0.037 min
Response: 3147857
Conc: 0.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

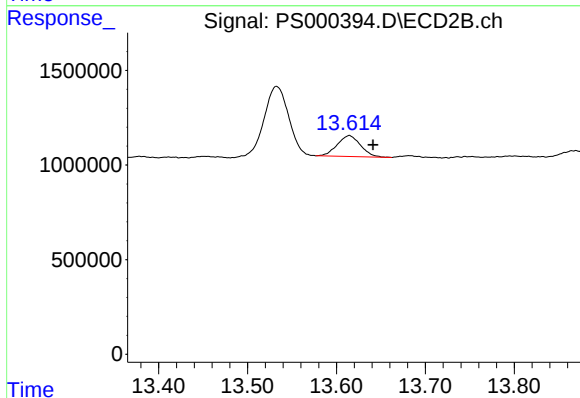


#10 Pentachlorophenol

R.T.: 13.615 min
Delta R.T.: -0.027 min
Response: 2014103
Conc: 0.46 ng/ml

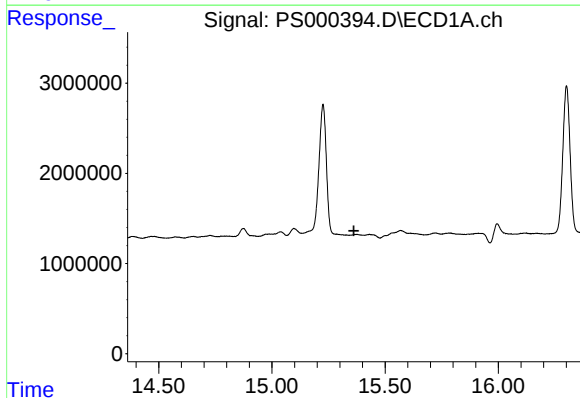


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.362 min
Response: 0
Conc: N.D.

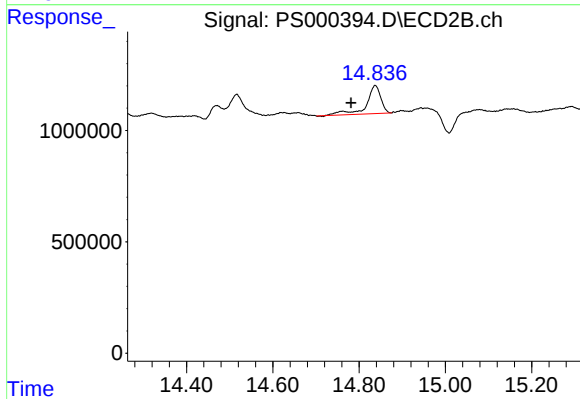

#12 2,4,5-T


R.T.: 14.837 min
Delta R.T.: 0.056 min
Response: 2941234
Conc: 1.78 ng/ml

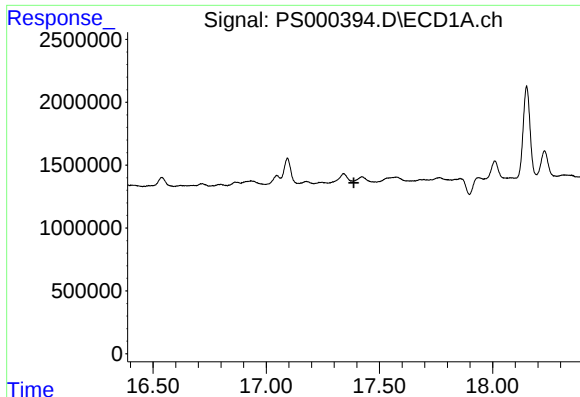

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

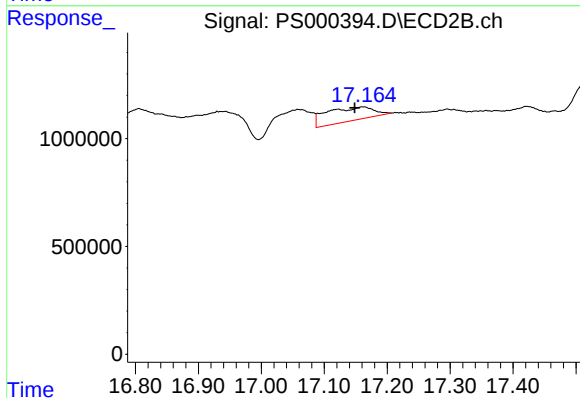


#15 Picloram

R.T.: 17.162 min
Delta R.T.: 0.013 min
Response: 3304891
Conc: 1.55 ng/ml

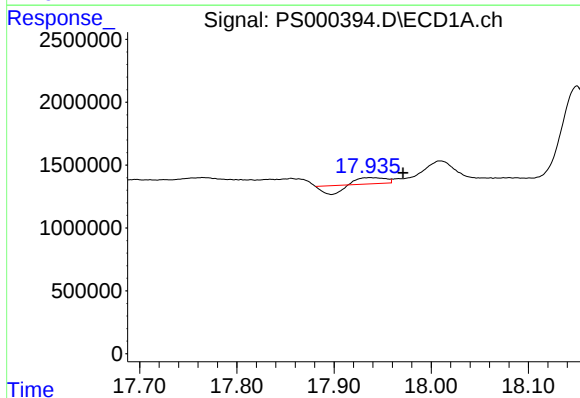

#16 DCPA

R.T.: 17.937 min
Delta R.T.: -0.034 min
Response: 164509
Conc: 0.07 ng/ml

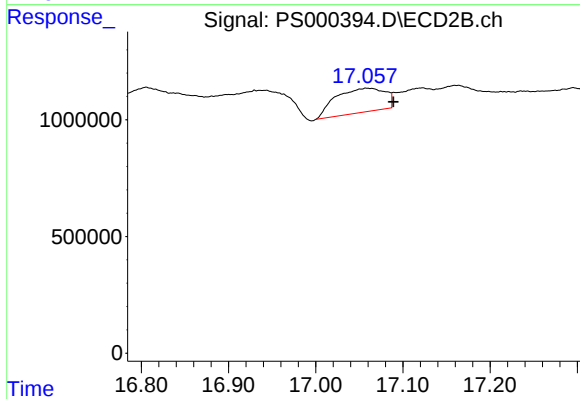

#16 DCPA

R.T.: 17.060 min
Delta R.T.: -0.029 min
Response: 4055147
Conc: 1.96 ng/ml