

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
 Data File : PS000376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2018 14:19
 Operator : UA
 Sample : J3490-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CONCRETE-BASE

Manual Integrations
 APPROVED

ugo
 6/18/2018 1:21:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 22:50:33 2018
 Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Thu May 31 04:46:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.825	11.199	148.3E6	125.6E6	420.118m	399.936m
Target Compounds							
9) T	2,4-D	13.695	13.083	77396091	64423734	171.612m	167.579m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS061518\
Data File : PS000376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2018 14:19
Operator : UA
Sample : J3490-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CONCRETE-BASE


Manual Integrations
APPROVED

ugo
6/18/2018 1:21:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 22:50:33 2018
Quant Method : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Thu May 31 04:46:50 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

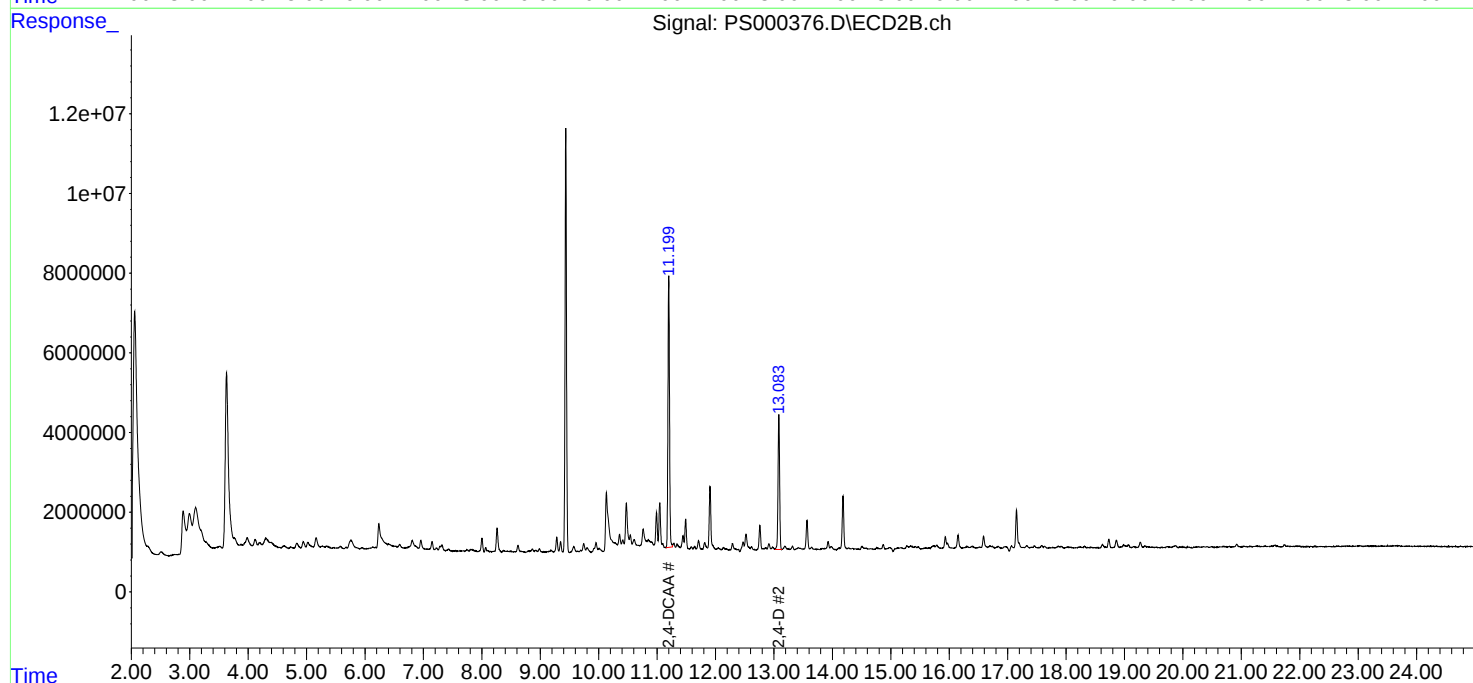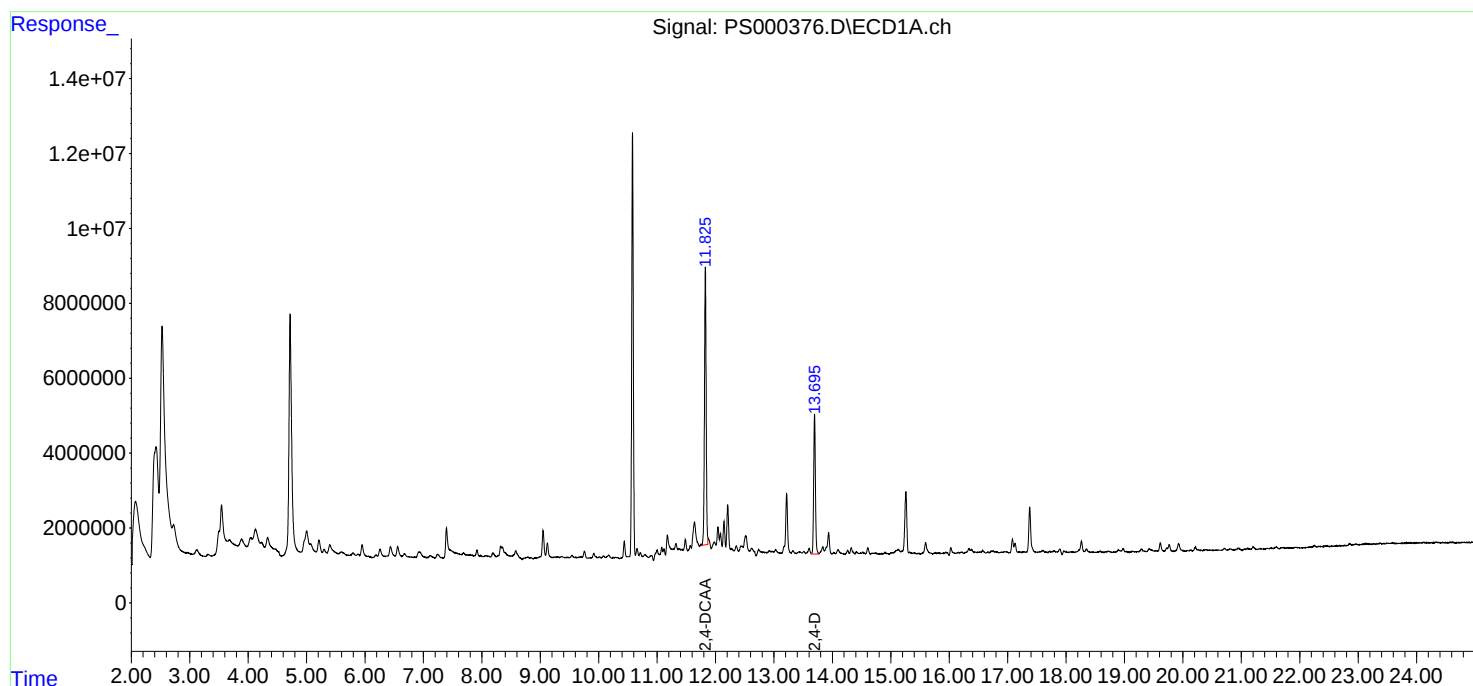

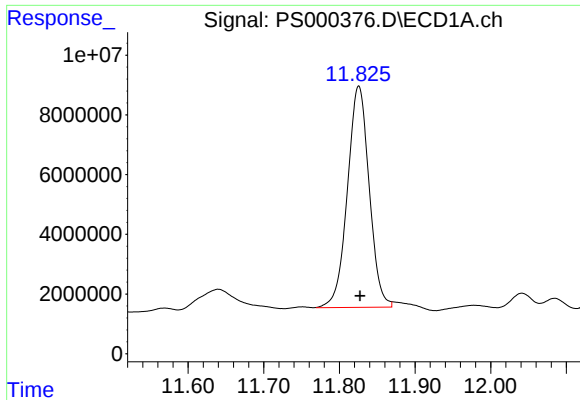


#4 2,4-DCAA

R.T.: 11.825 min
Delta R.T.: -0.002 min
Response: 148333842
Conc: 420.12 ng/ml m

Instrument :
ECD_S
ClientSampleId :
CONCRETE-BASE


Manual Integrations
APPROVED

ugo
6/18/2018 1:21:12 PM

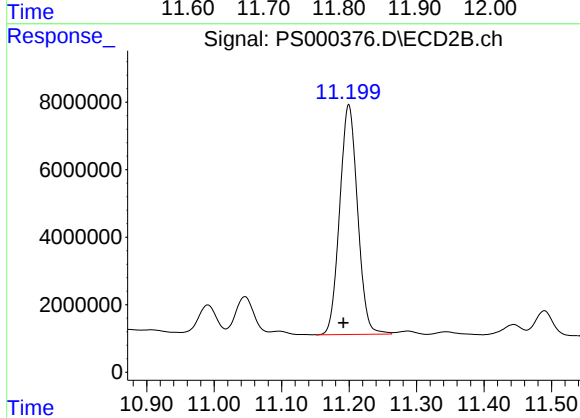


#4 2,4-DCAA

R.T.: 11.199 min
Delta R.T.: 0.007 min
Response: 125620708
Conc: 399.94 ng/ml m

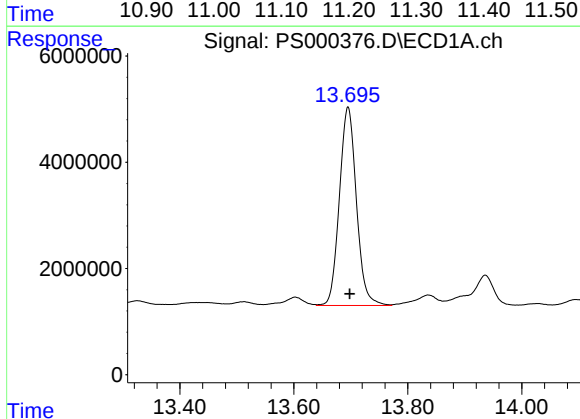

#9 2,4-D

R.T.: 13.695 min
Delta R.T.: -0.003 min
Response: 77396091
Conc: 171.61 ng/ml m

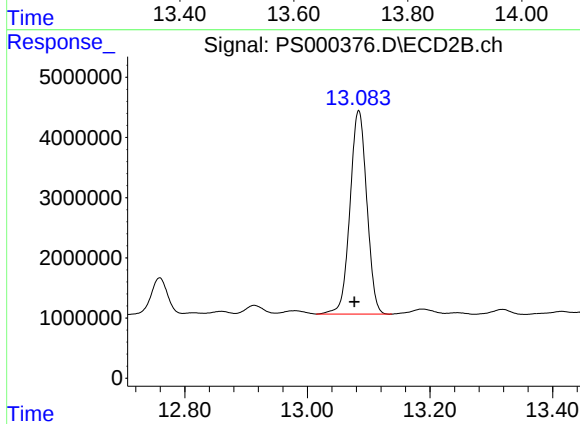

#9 2,4-D

R.T.: 13.083 min
Delta R.T.: 0.007 min
Response: 64423734
Conc: 167.58 ng/ml m