

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 08:00
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:54:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.953	0.000	2780.2E6	0	1383.391	N.D. #
5) T	DICAMBA	0.000	5.453	0	2011.5E6	N.D.	537.350
6) T	MCPD	0.000	5.453	0	2011.5E6	N.D.	722.129
7) T	MCPA	5.973	0.000	34171184	0	5.441	N.D. #
8) T	DICHLORPROP	0.000	5.987	0	41858467	N.D.	43.352
9) T	2,4-D	6.626	0.000	3460.3E6	0	2225.842	N.D. #
10) T	Pentachlo...	6.886	0.000	33024938	0	1.678	N.D. #
12) T	2,4,5-T	7.692	7.402	17798108	61199381	2.212	11.998 #
15) T	Picloram	9.126	9.110	1802.7E6	377.0E6	156.875	49.962 #
16) T	DCPA	0.000	9.110	0	377.0E6	N.D.	55.386



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 08:00
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:54:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

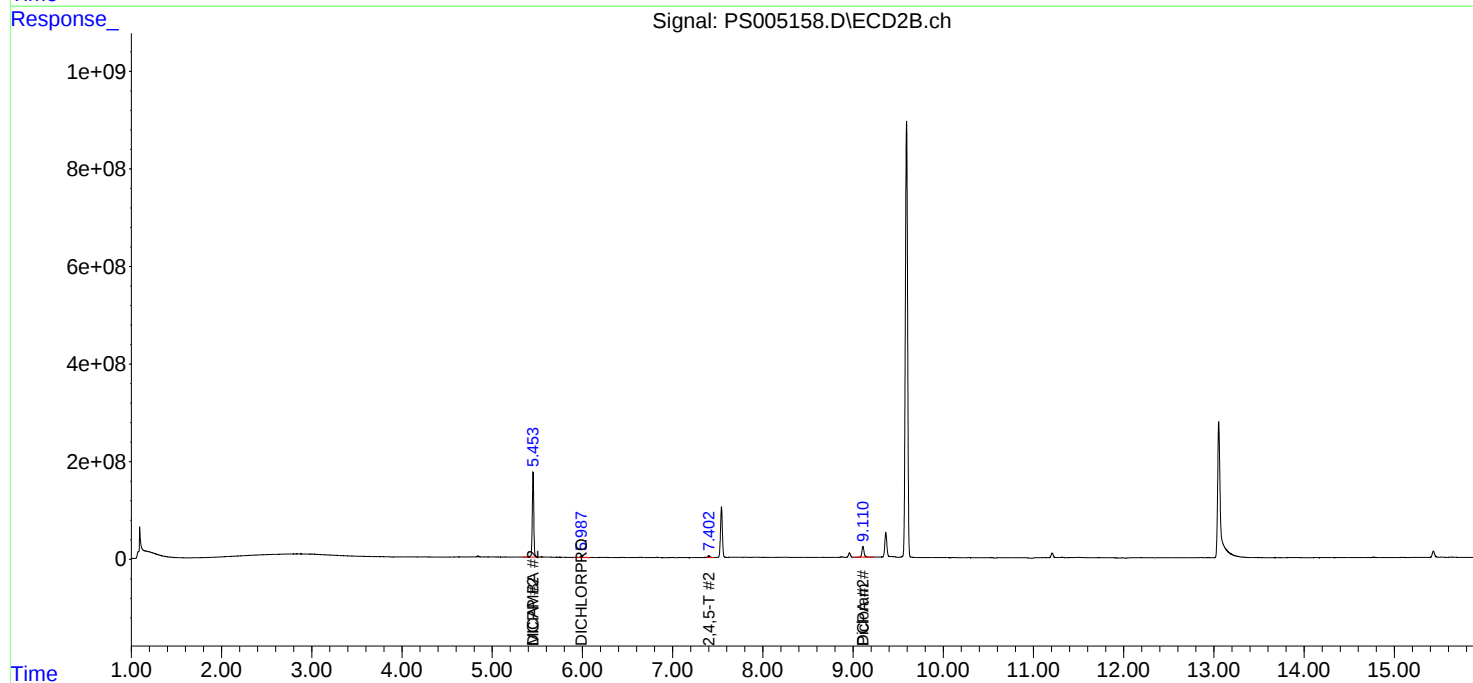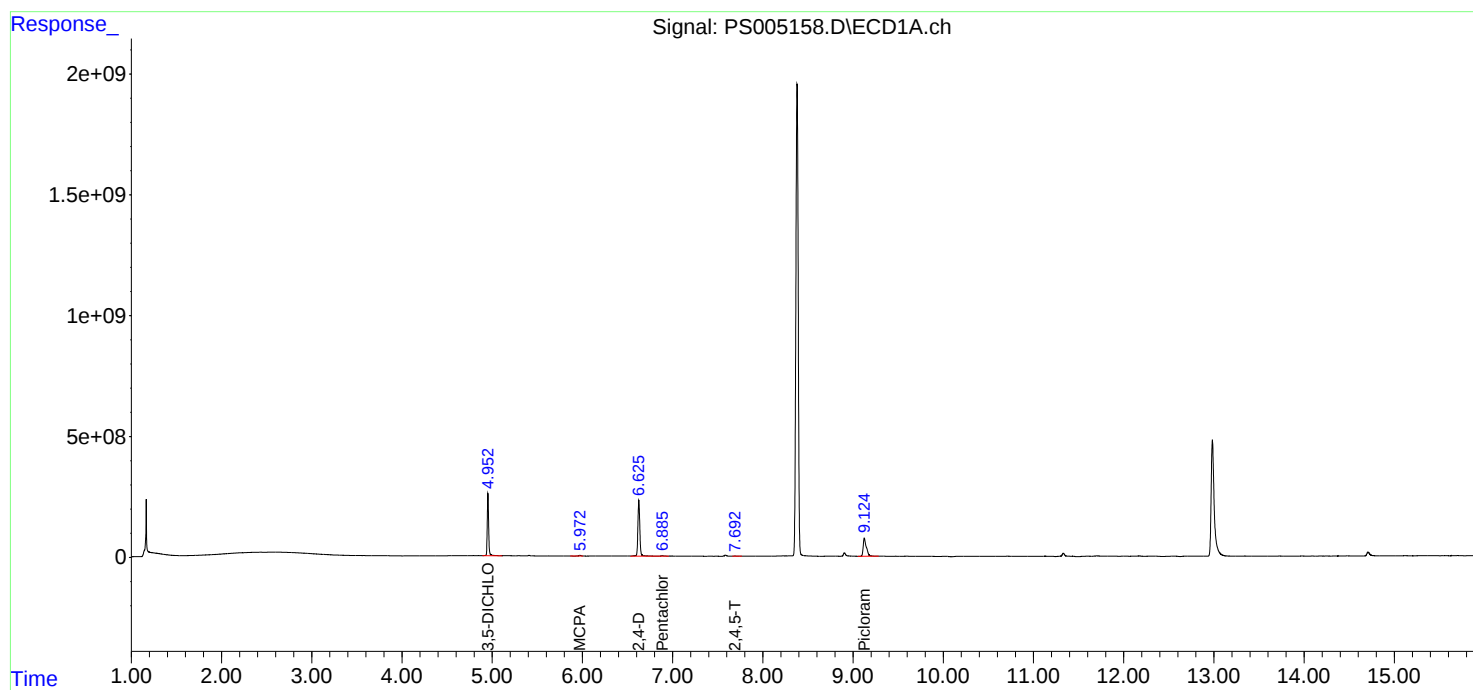


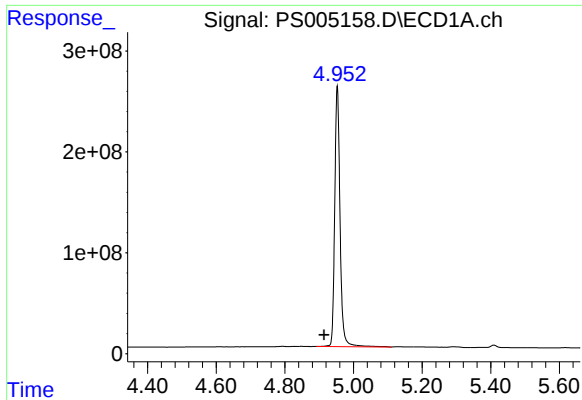

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.953 min
Delta R.T.: 0.039 min
Response: 2780226342
Conc: 1383.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

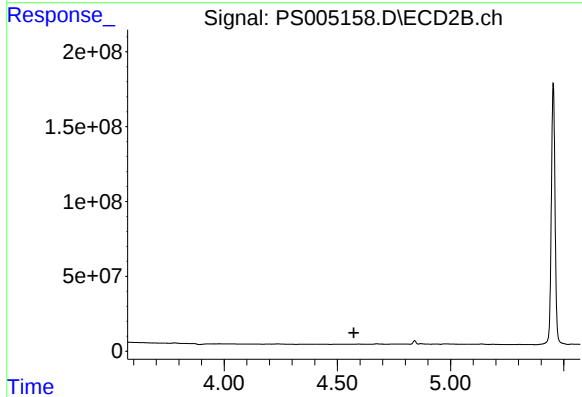


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

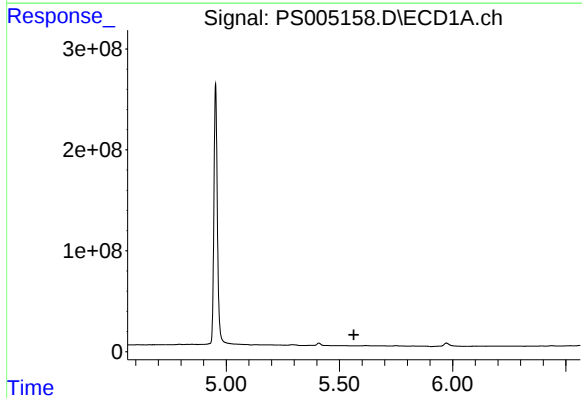


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

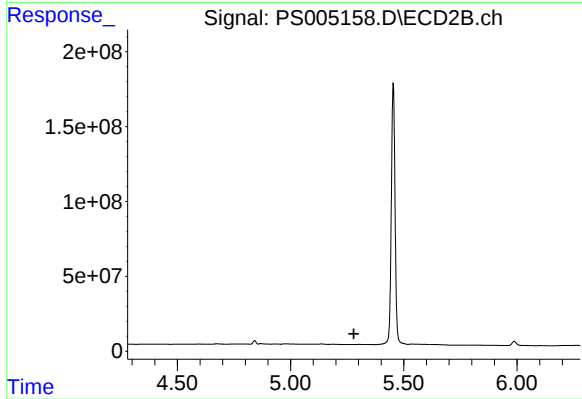

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

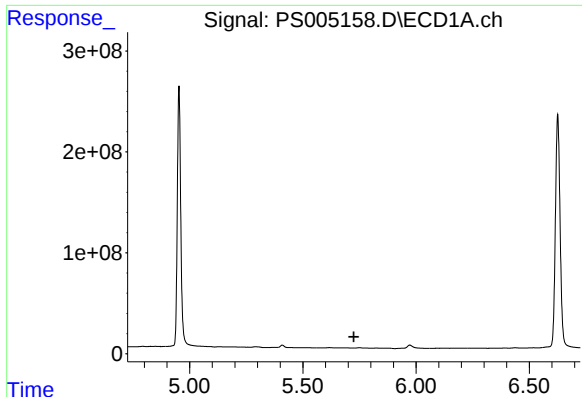

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

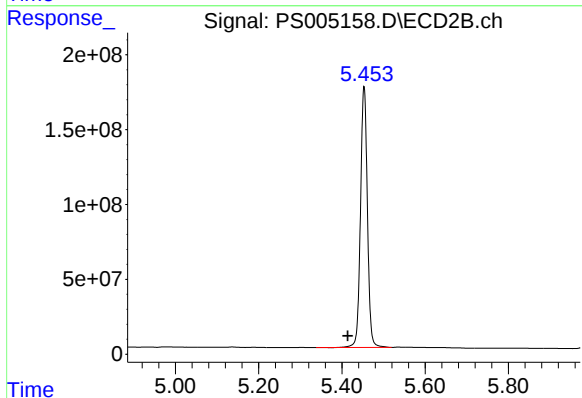


#5 DICAMBA

R.T.: 5.453 min
Delta R.T.: 0.039 min
Response: 2011474697
Conc: 537.35 ng/ml

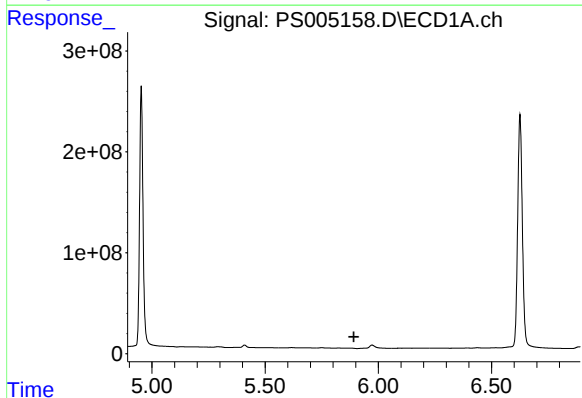


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

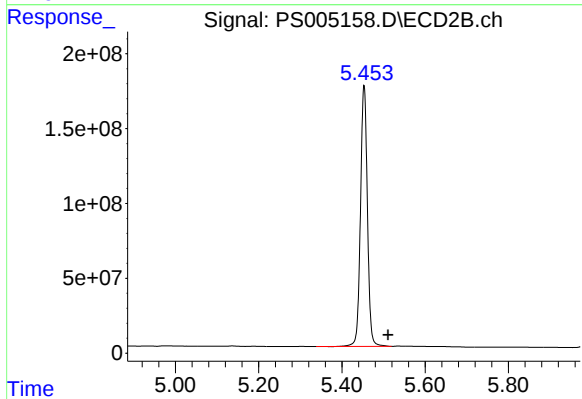

#6 MCP


R.T.: 5.453 min
Delta R.T.: -0.057 min
Response: 2011474697
Conc: 722.13 ug/ml

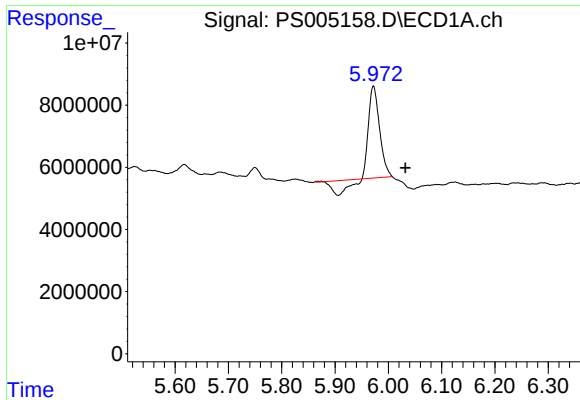

#7 MCPA


R.T.: 5.973 min
Delta R.T.: -0.059 min
Response: 34171184
Conc: 5.44 ug/ml

Instrument :
ECD_S
ClientSampleId :

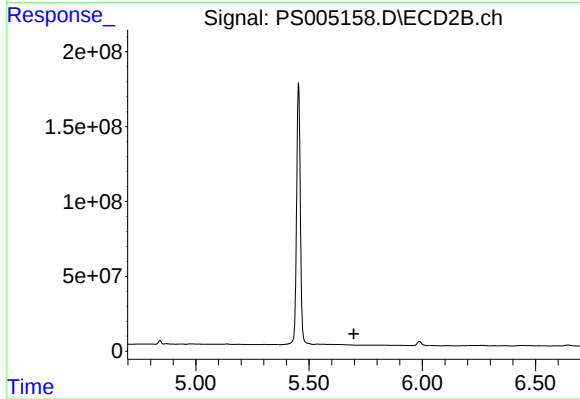


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.698 min
Response: 0
Conc: N.D.

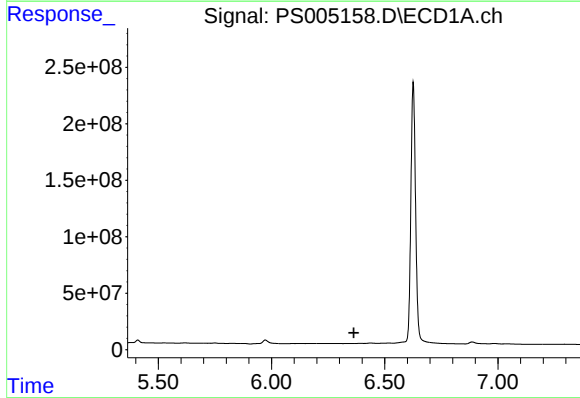


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

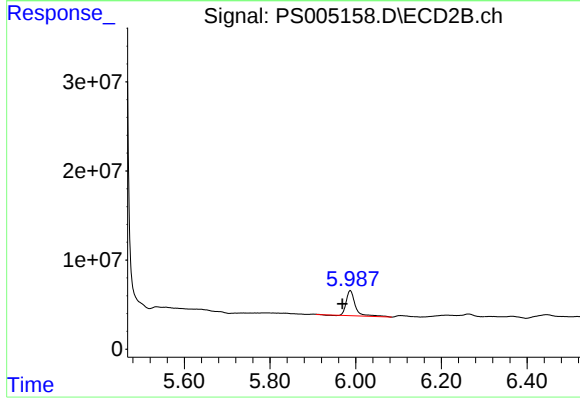

#8 DICHLORPROP


R.T.: 5.987 min
Delta R.T.: 0.018 min
Response: 41858467
Conc: 43.35 ng/ml

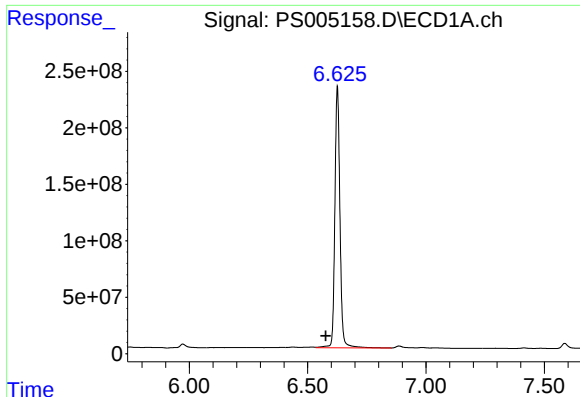

#9 2,4-D


R.T.: 6.626 min
Delta R.T.: 0.049 min
Response: 3460293559
Conc: 2225.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

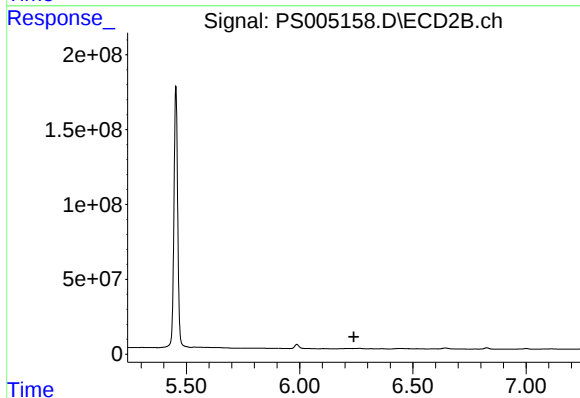


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

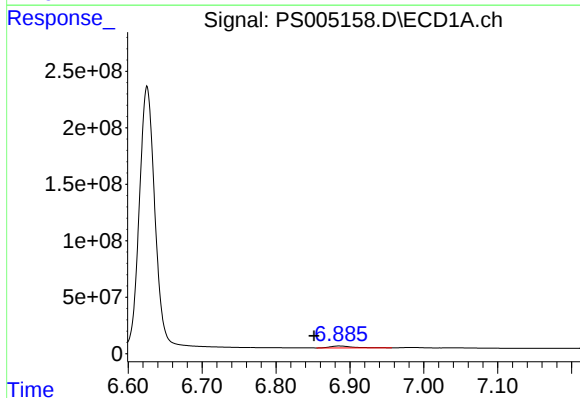


#10 Pentachlorophenol

R.T.: 6.886 min
Delta R.T.: 0.035 min
Response: 33024938
Conc: 1.68 ng/ml

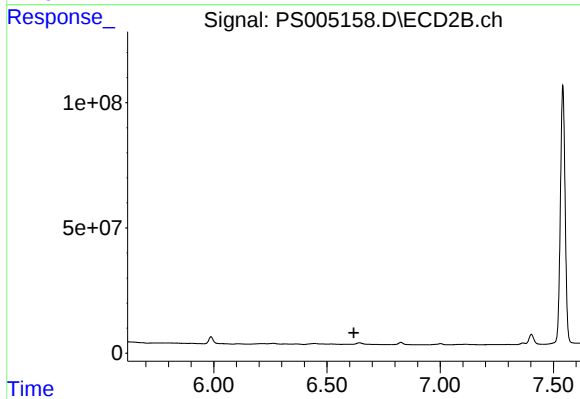

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.619 min
Response: 0
Conc: N.D.

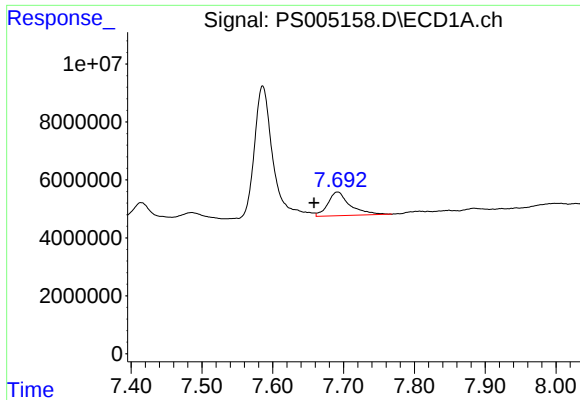

#12 2,4,5-T


R.T.: 7.692 min
Delta R.T.: 0.033 min
Response: 17798108
Conc: 2.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

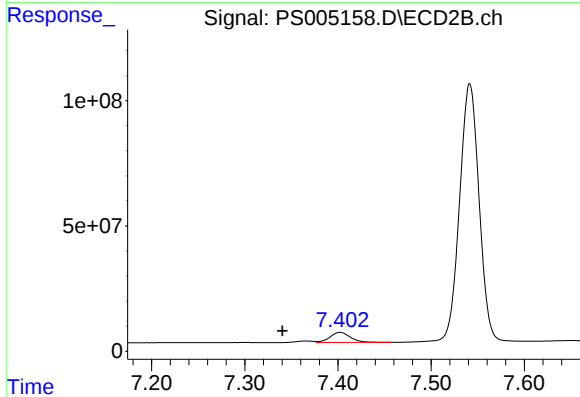


#12 2,4,5-T

R.T.: 7.402 min
Delta R.T.: 0.062 min
Response: 61199381
Conc: 12.00 ng/ml

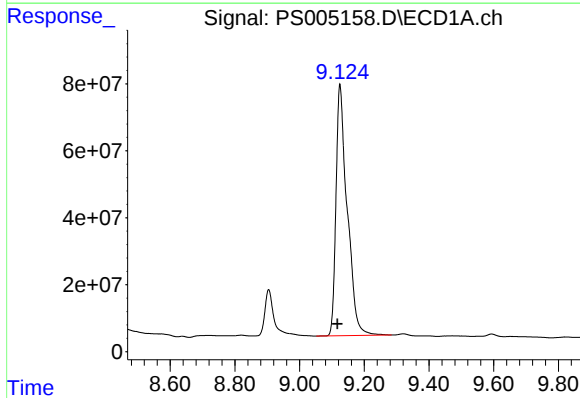


#15 Picloram

R.T.: 9.126 min
Delta R.T.: 0.009 min
Response: 1802668574
Conc: 156.87 ng/ml

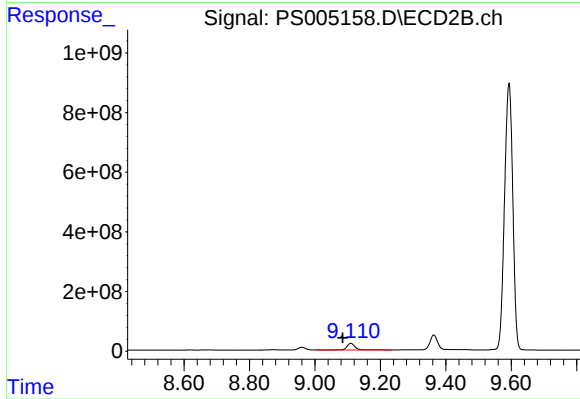

#15 Picloram


R.T.: 9.110 min
Delta R.T.: 0.025 min
Response: 377033233
Conc: 49.96 ng/ml

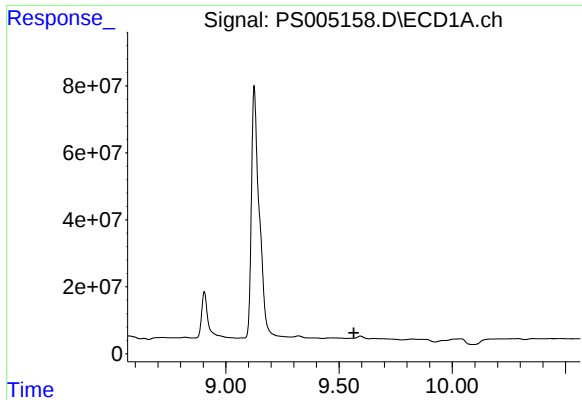

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

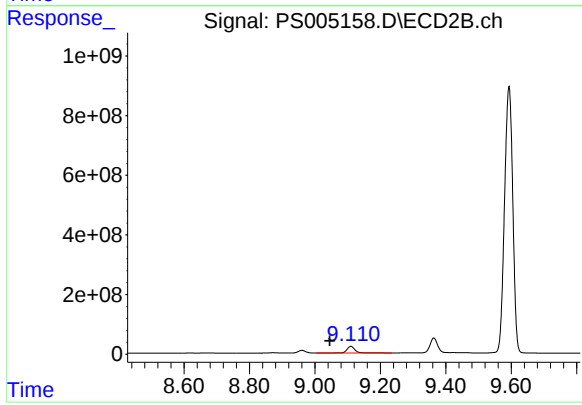

#16 DCPA

R.T.: 9.110 min
Delta R.T.: 0.064 min
Response: 377033233
Conc: 55.39 ng/ml