

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 12:37
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:55:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.585	5.295	573.8E6	393.2E6	390.917	392.269
Target Compounds							
12) T	2,4,5-T	7.690	7.401	18585905	72515660	2.309	14.216 #
15) T	Picloram	9.152	9.108	378.2E6	272.2E6	32.914	36.068
16) T	DCPA	0.000	9.108	0	272.2E6	N.D.	39.984



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 12:37
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:55:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

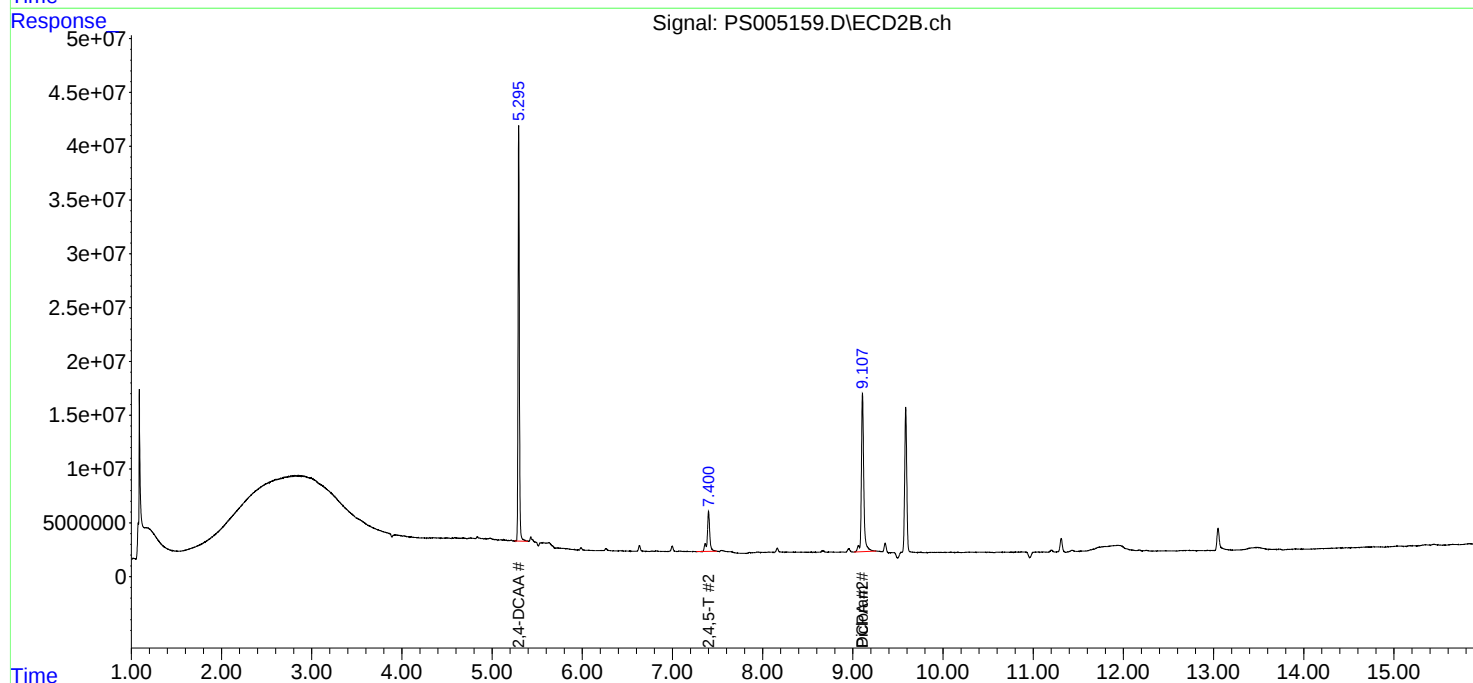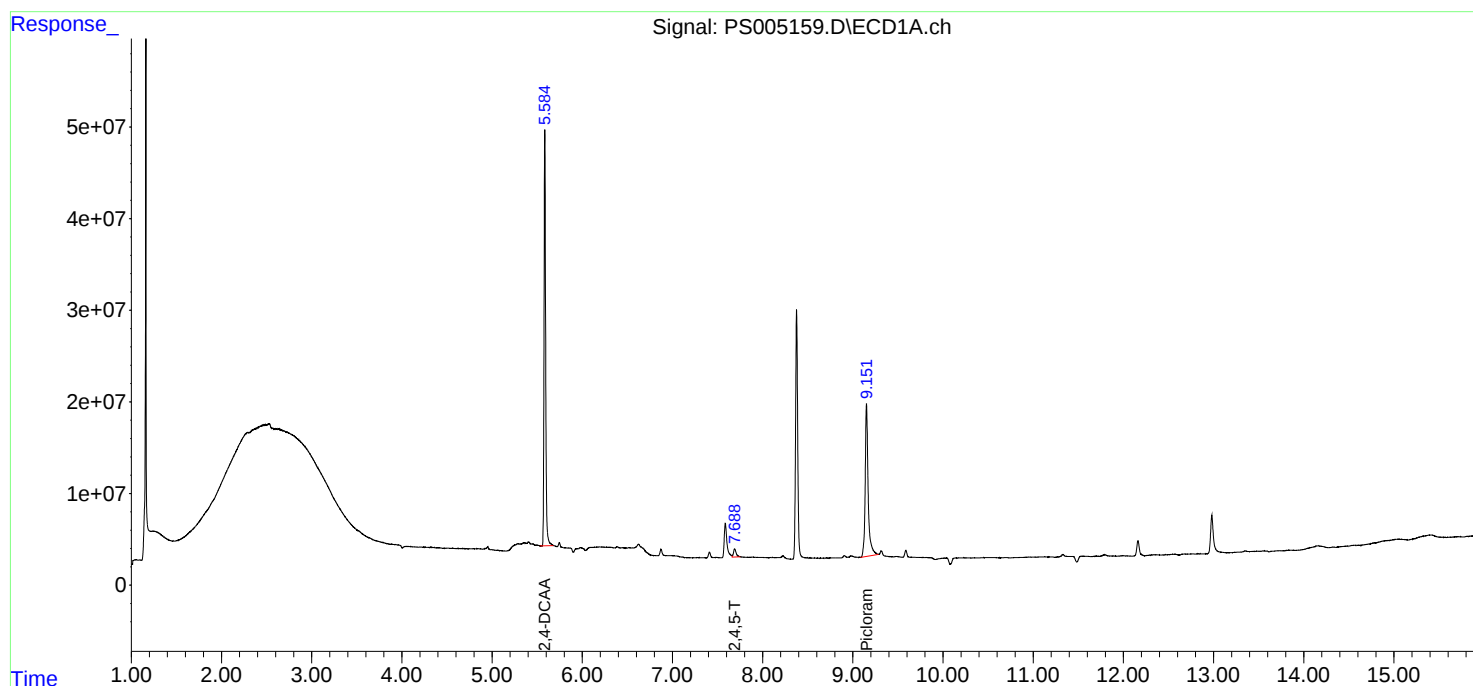


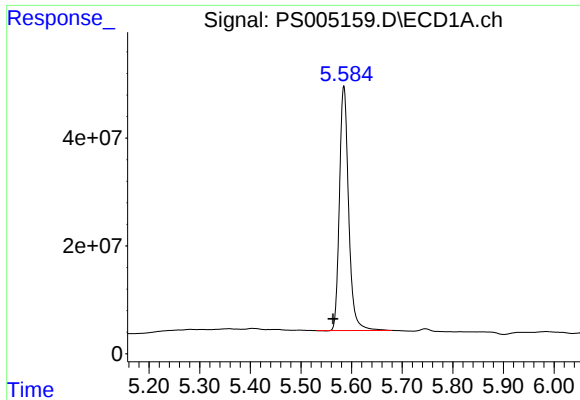

#4 2,4-DCAA


R.T.: 5.585 min
Delta R.T.: 0.021 min
Response: 573824318
Conc: 390.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

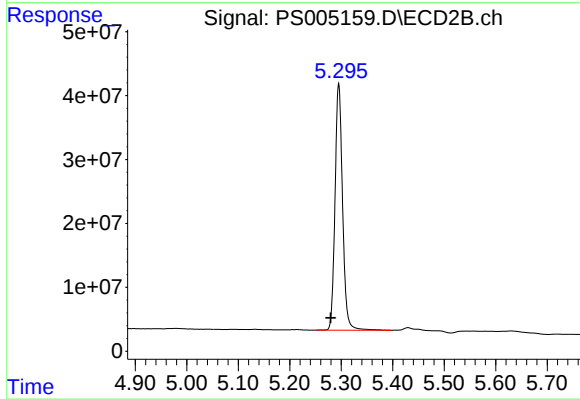


#4 2,4-DCAA

R.T.: 5.295 min
Delta R.T.: 0.016 min
Response: 393197691
Conc: 392.27 ng/ml

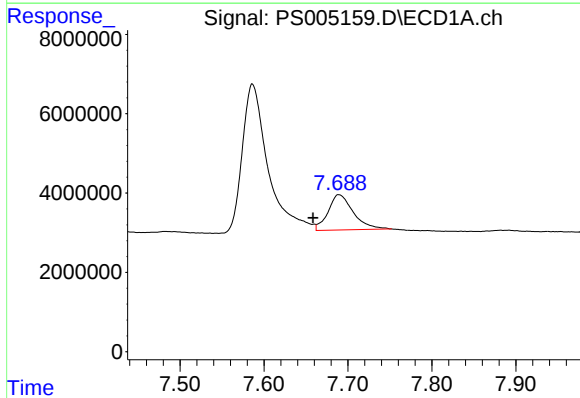


#12 2,4,5-T

R.T.: 7.690 min
Delta R.T.: 0.031 min
Response: 18585905
Conc: 2.31 ng/ml

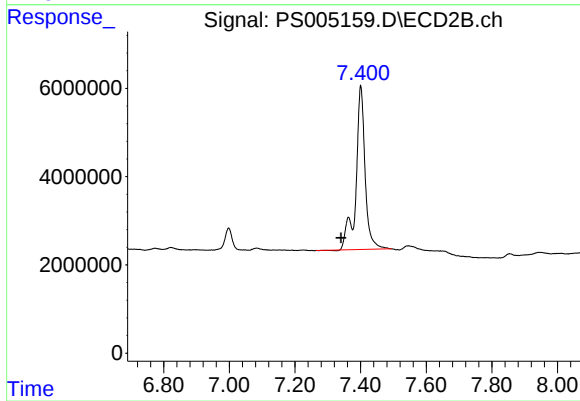

#12 2,4,5-T


R.T.: 7.401 min
Delta R.T.: 0.060 min
Response: 72515660
Conc: 14.22 ng/ml

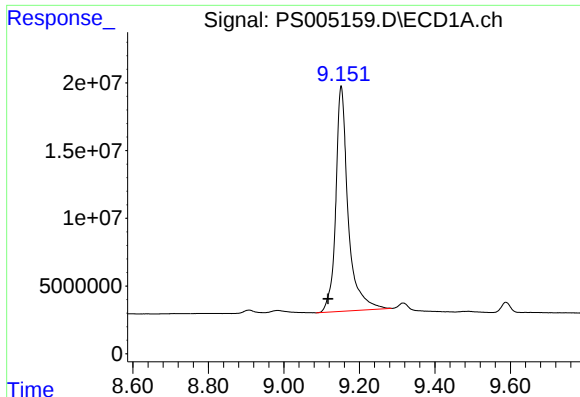

#15 Picloram


R.T.: 9.152 min
Delta R.T.: 0.035 min
Response: 378224720
Conc: 32.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

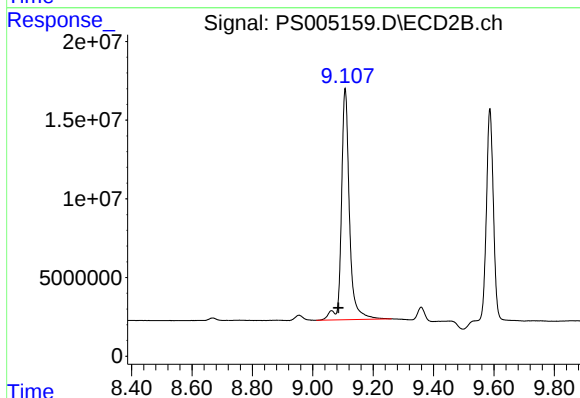


#15 Picloram

R.T.: 9.108 min
Delta R.T.: 0.023 min
Response: 272184969
Conc: 36.07 ng/ml

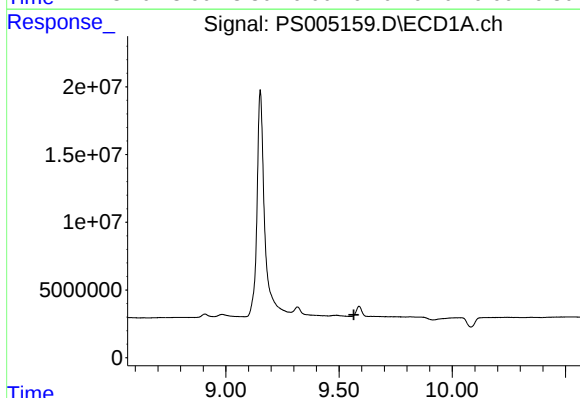

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

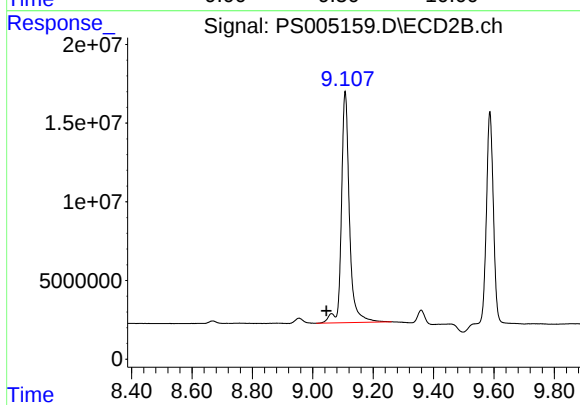

#16 DCPA

R.T.: 9.108 min
Delta R.T.: 0.062 min
Response: 272184969
Conc: 39.98 ng/ml