

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 15:20
 Operator : SM\AJ
 Sample : K3441-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:57:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.302	559.9E6	369.7E6	381.441	368.847
Target Compounds							
1) T	Dalapon	2.089	1.779	73612776	-4317026	39.935	N.D. #
2) T	3,5-DICHL...	0.000	4.579	0	10922683	N.D.	8.283
7) T	MCPA	5.978	5.631	16732487	20035998	2.665	4.946 #
8) T	DICHLORPROP	0.000	5.990	0	18322595	N.D.	18.977
9) T	2,4-D	0.000	6.250	0	20000119	N.D.	17.933
10) T	Pentachlo...	0.000	6.568	0	21984062	N.D.	1.710
12) T	2,4,5-T	7.602	0.000	34305200	0	4.263	N.D. #
15) T	Picloram	9.134	0.000	33620699	0	2.926	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 15:20
Operator : SM\AJ
Sample : K3441-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:57:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

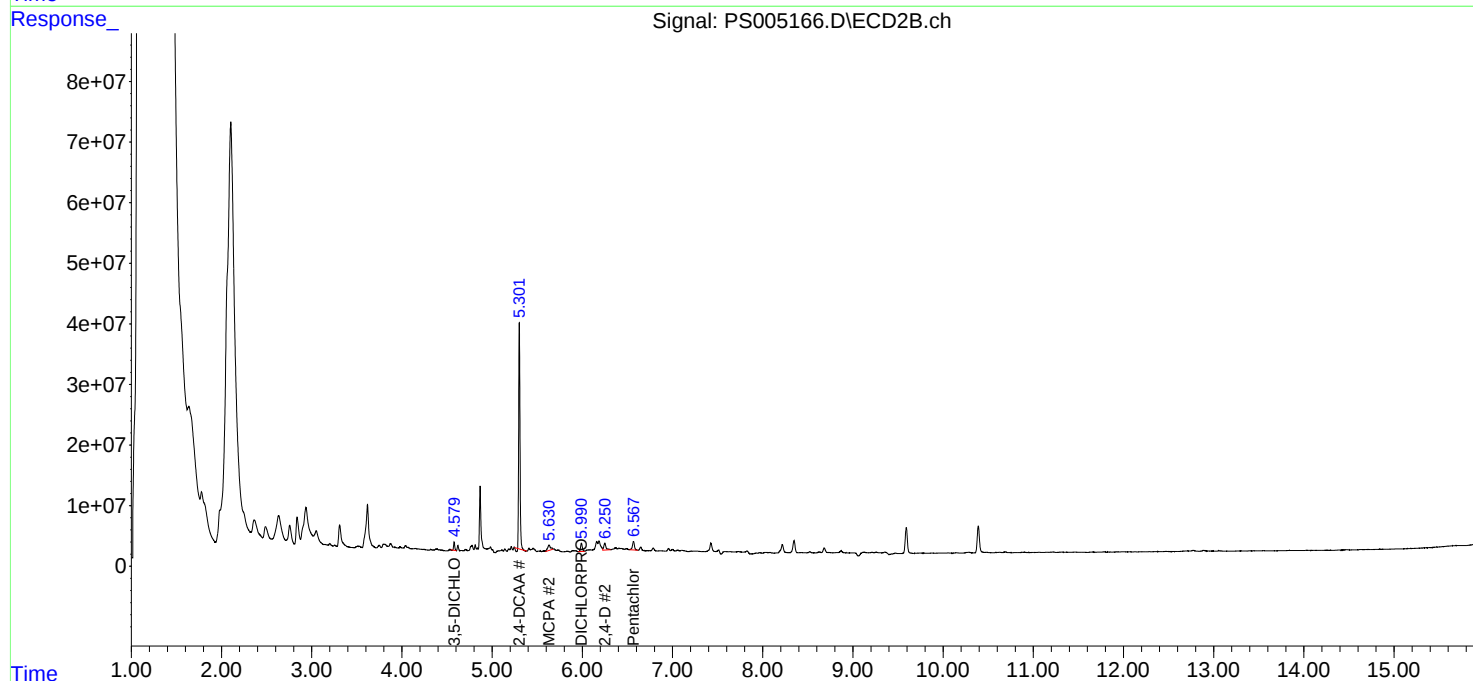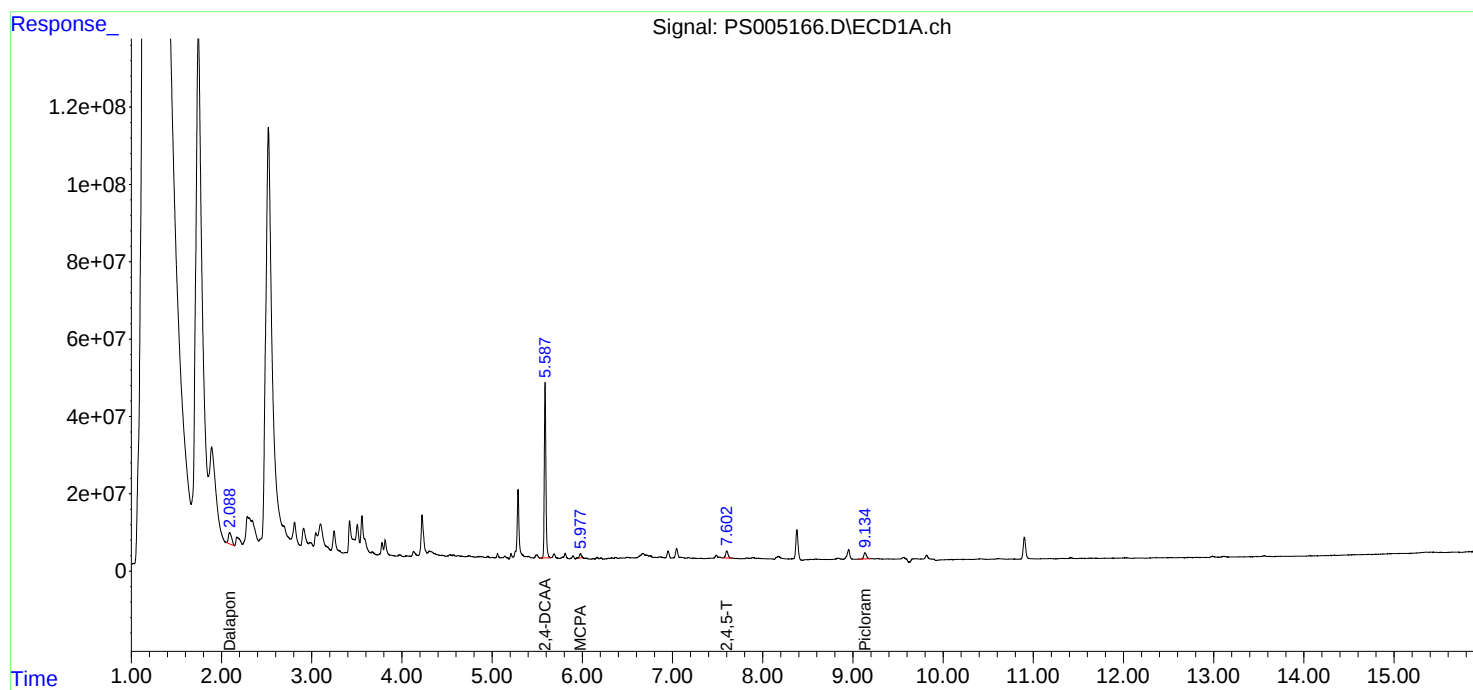


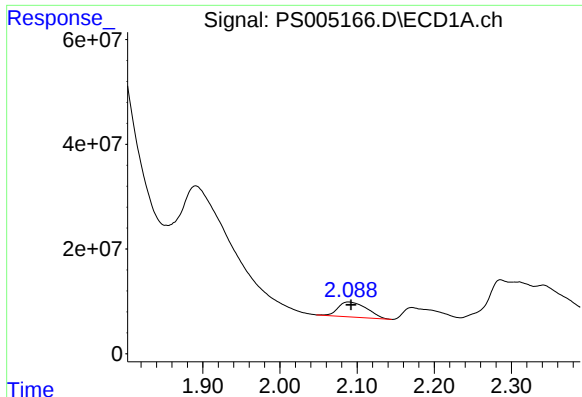

#1 Dalapon


R.T.: 2.089 min
Delta R.T.: -0.003 min
Response: 73612776
Conc: 39.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

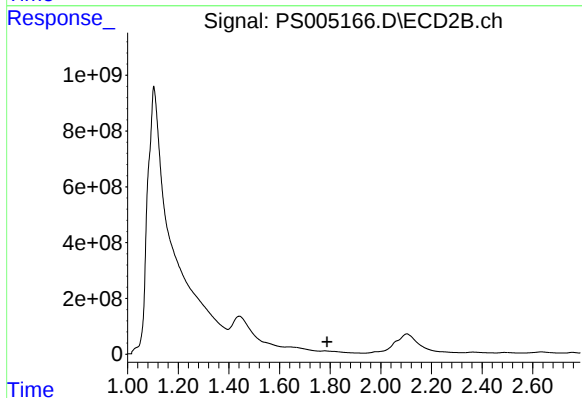


#1 Dalapon

R.T.: 1.779 min
Delta R.T.: -0.009 min
Response: -4317026
Conc: N.D.

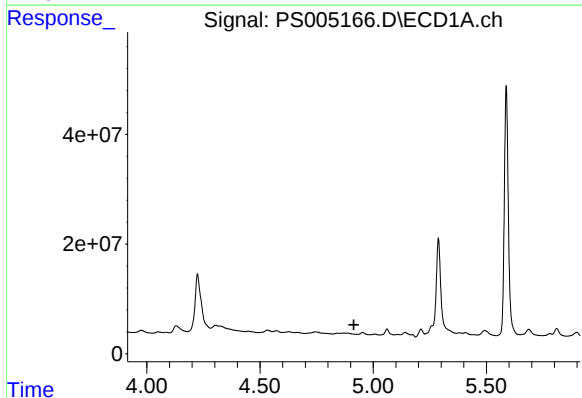


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

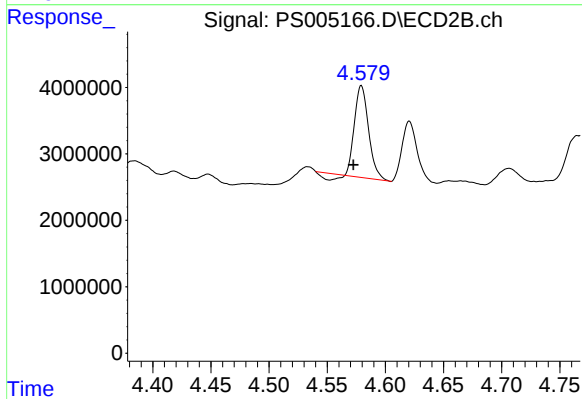

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.579 min
Delta R.T.: 0.007 min
Response: 10922683
Conc: 8.28 ng/ml

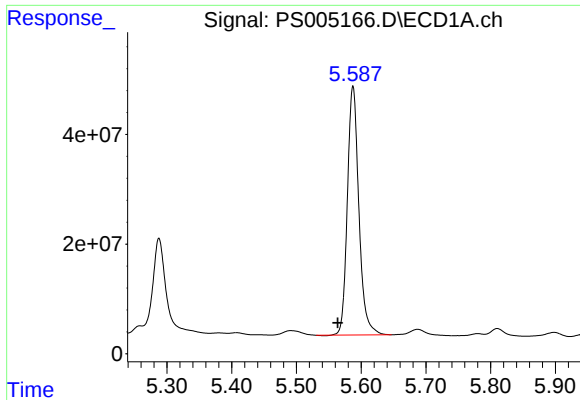

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.024 min
Response: 559914184
Conc: 381.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

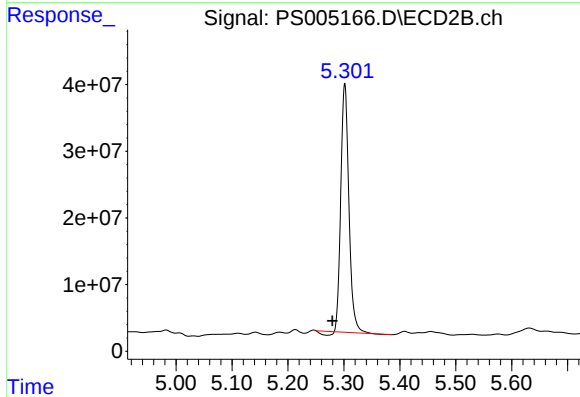


#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: 0.022 min
Response: 369720673
Conc: 368.85 ng/ml

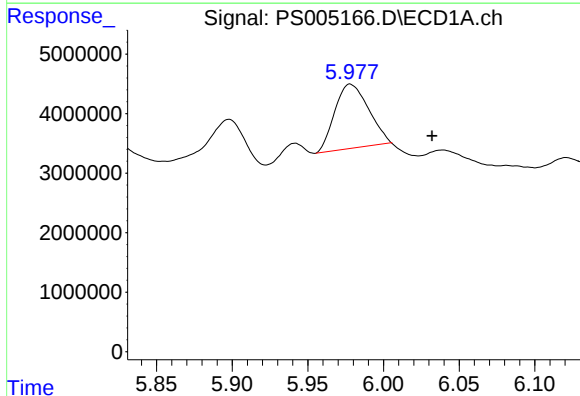


#7 MCPA

R.T.: 5.978 min
Delta R.T.: -0.054 min
Response: 16732487
Conc: 2.66 ug/ml

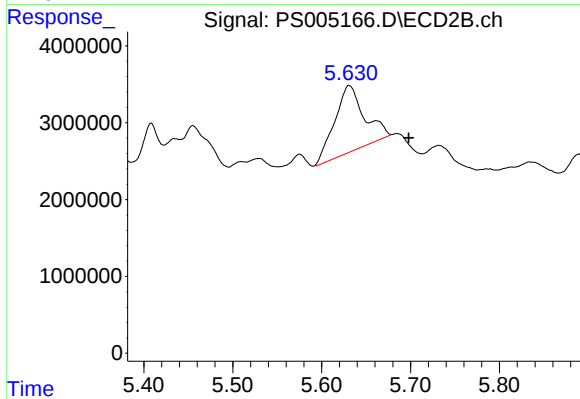

#7 MCPA


R.T.: 5.631 min
Delta R.T.: -0.067 min
Response: 20035998
Conc: 4.95 ug/ml

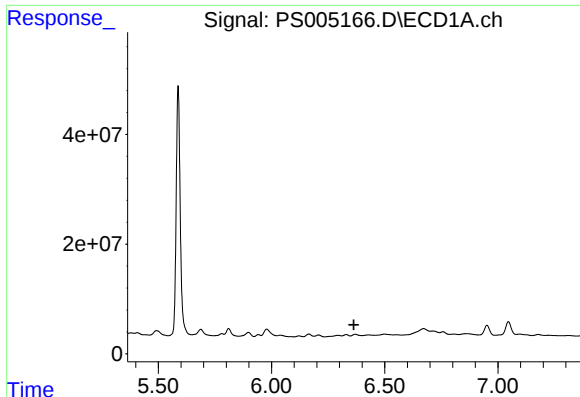

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

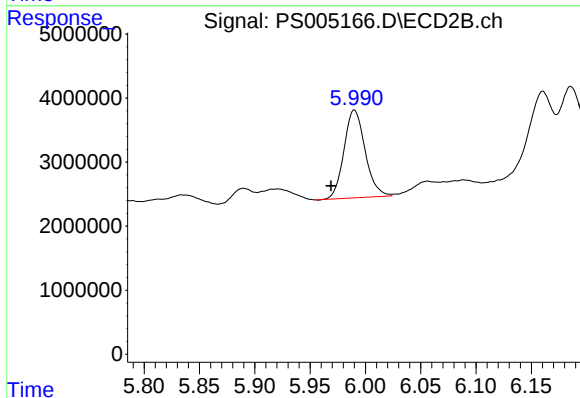


#8 DICHLORPROP

R.T.: 5.990 min
Delta R.T.: 0.021 min
Response: 18322595
Conc: 18.98 ng/ml

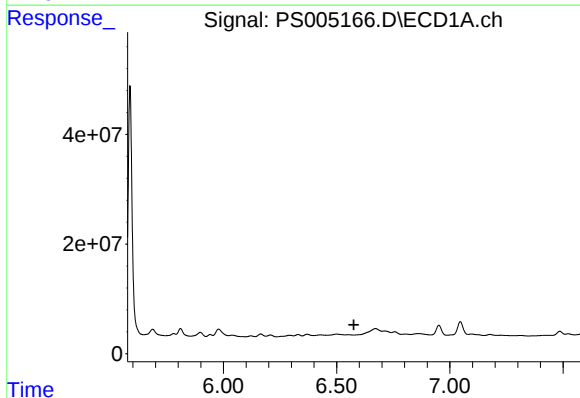


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

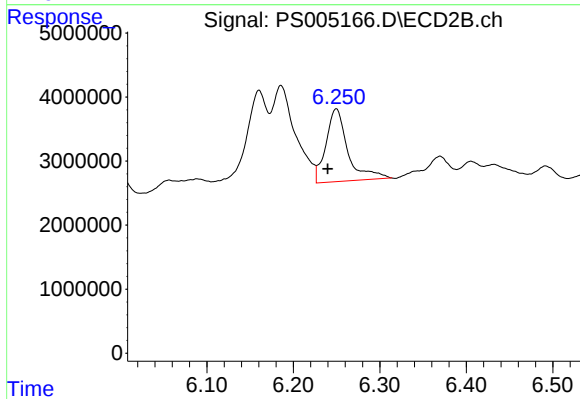

#9 2,4-D


R.T.: 6.250 min
Delta R.T.: 0.010 min
Response: 20000119
Conc: 17.93 ng/ml

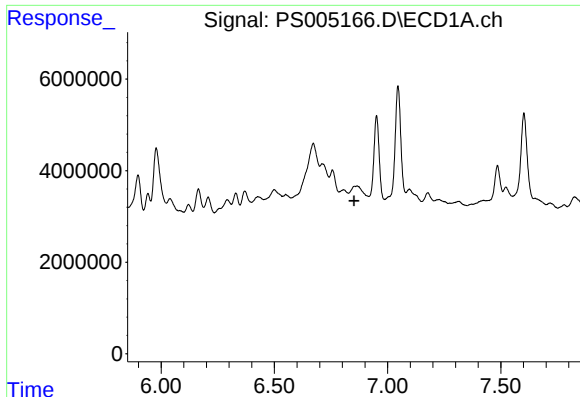

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

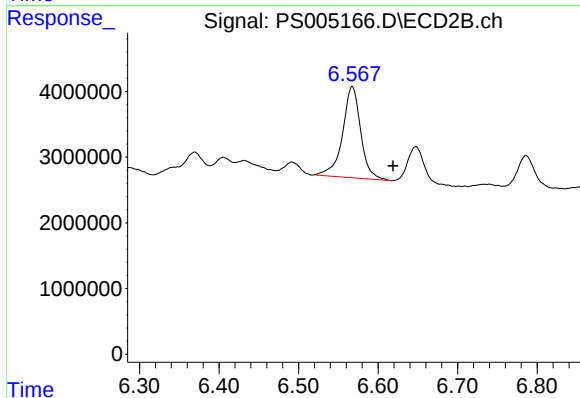


#10 Pentachlorophenol

R.T.: 6.568 min
Delta R.T.: -0.052 min
Response: 21984062
Conc: 1.71 ng/ml

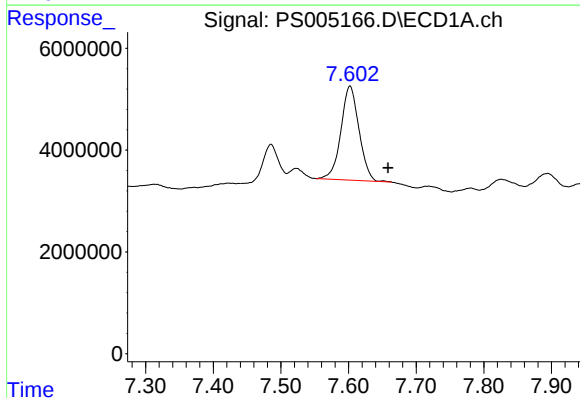


#12 2,4,5-T

R.T.: 7.602 min
Delta R.T.: -0.056 min
Response: 34305200
Conc: 4.26 ng/ml

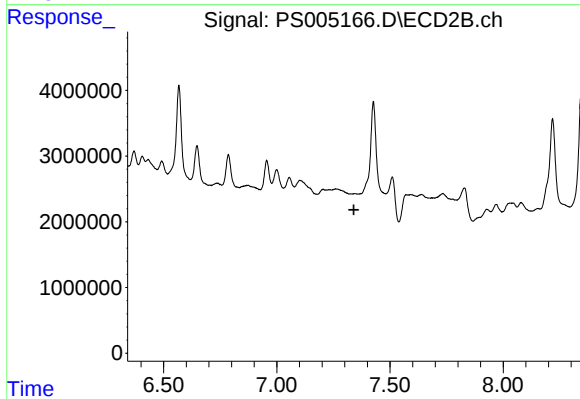

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.

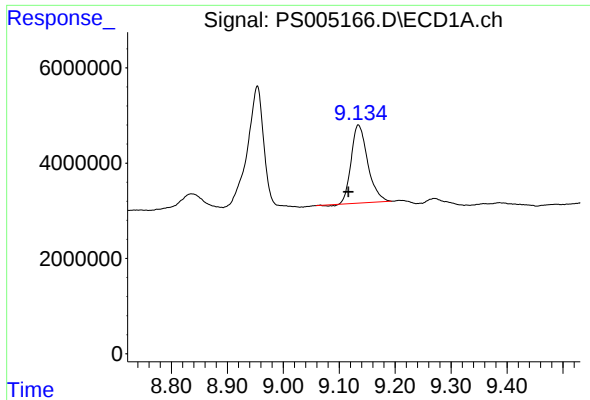

#15 Picloram

R.T.: 9.134 min
Delta R.T.: 0.018 min
Response: 33620699
Conc: 2.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

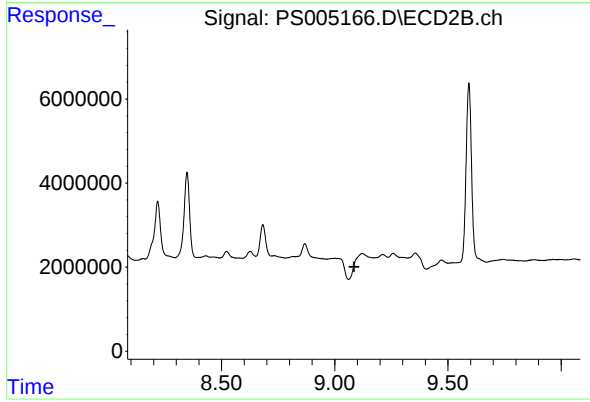

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.