

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 16:26
 Operator : SM\AJ
 Sample : K3455-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:59:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.286	480.1E6	338.3E6	327.051	337.519
Target Compounds							
1) T	Dalapon	2.077	0.000	71388268	0	38.729	N.D. #
2) T	3,5-DICHL...	0.000	4.563	0	13651978	N.D.	10.353
3) T	4-Nitroph...	5.364	0.000	12255311	0	16.920	N.D. #
5) T	DICAMBA	5.671	5.392	7308451	16009332	1.281	4.277 #
6) T	MCP	5.925	0.000	10723107	0	2.450	N.D. #
8) T	DICHLORPROP	6.313	0.000	8209918	0	5.741	N.D. #
9) T	2,4-D	0.000	6.234	0	17502704	N.D.	15.694
10) T	Pentachlo...	0.000	6.552	0	31288334	N.D.	2.434
11) T	2,4,5-TP ...	0.000	6.940	0	58327618	N.D.	10.953
12) T	2,4,5-T	7.593	0.000	144.1E6	0	17.900	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 16:26
Operator : SM\AJ
Sample : K3455-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:59:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

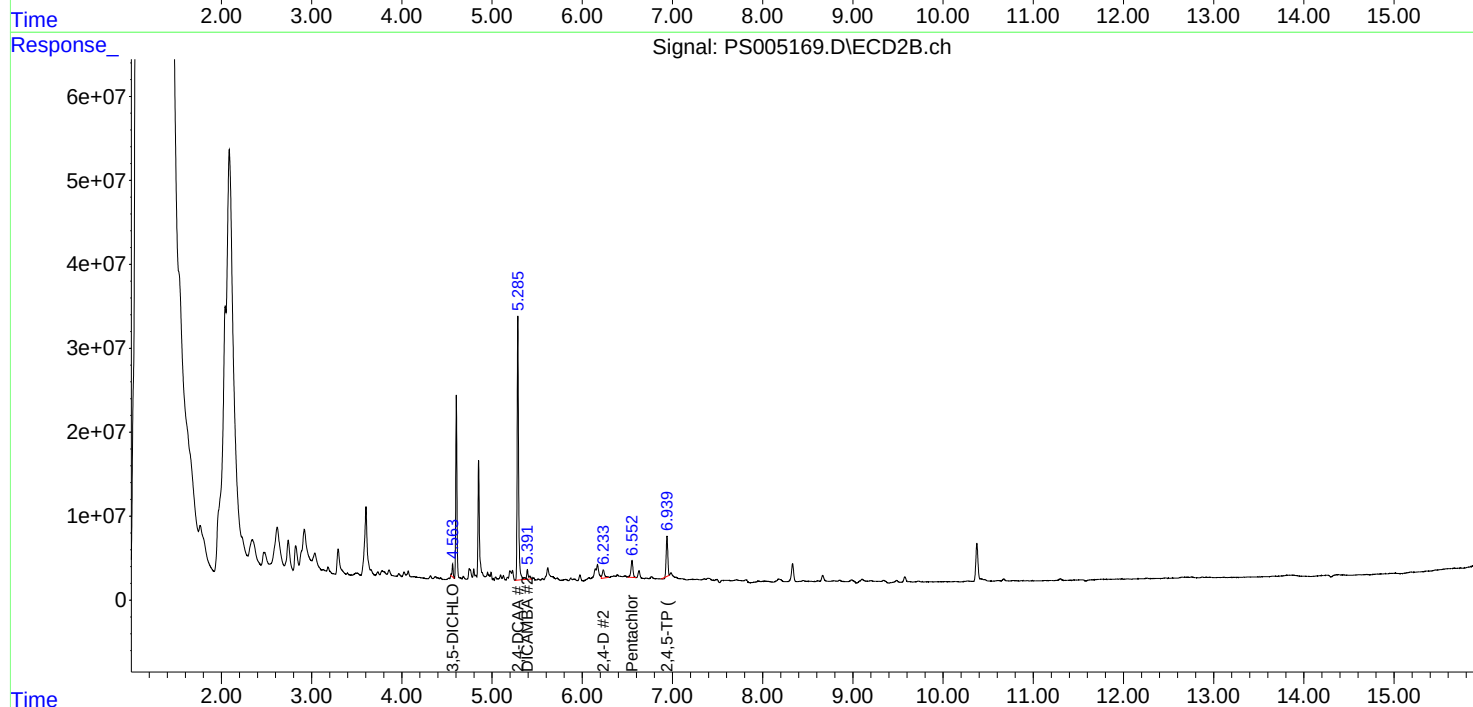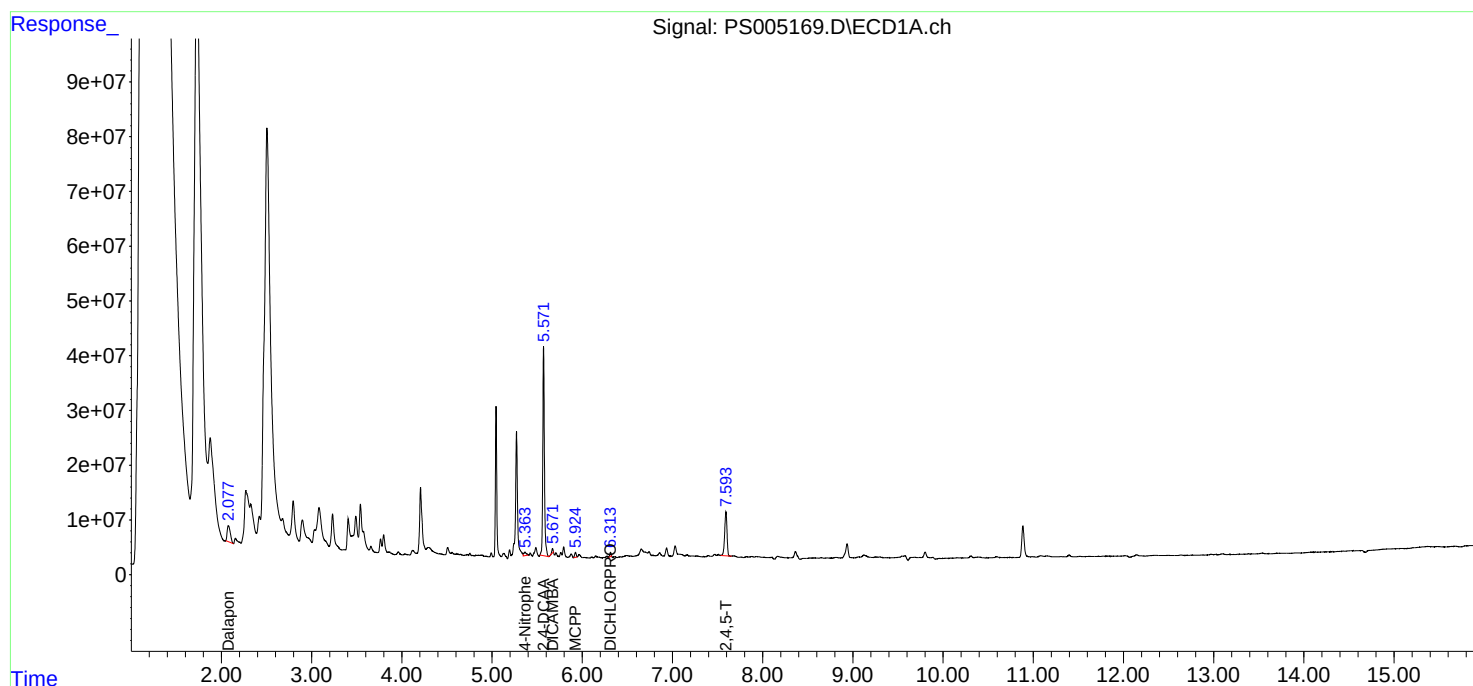


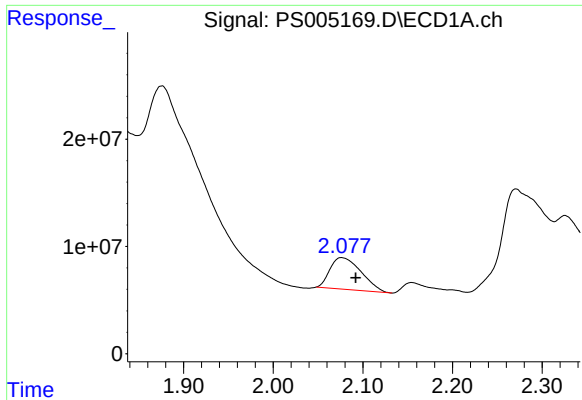

#1 Dalapon


R.T.: 2.077 min
Delta R.T.: -0.015 min
Response: 71388268
Conc: 38.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

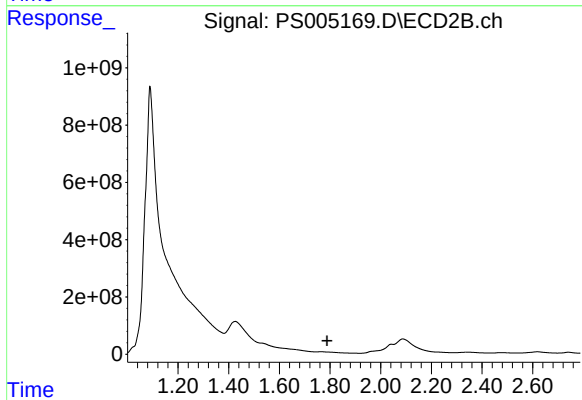


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

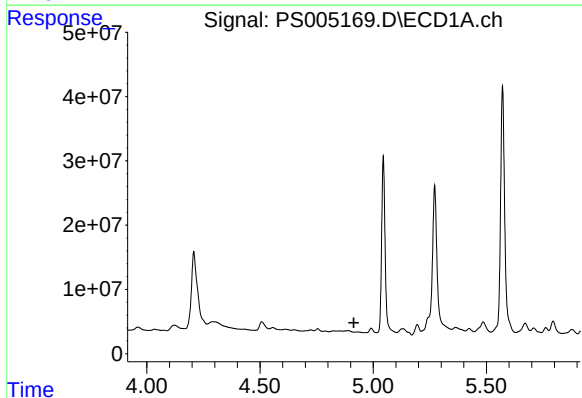


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

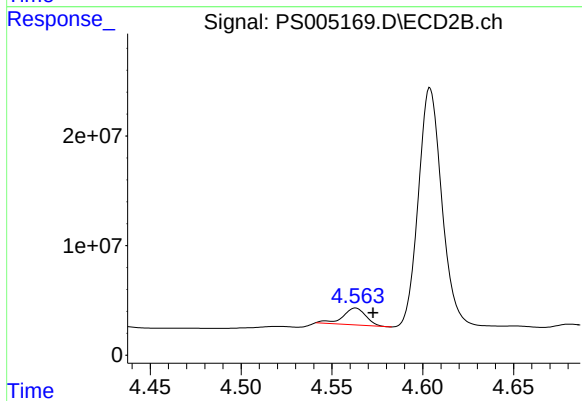

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.563 min
Delta R.T.: -0.010 min
Response: 13651978
Conc: 10.35 ng/ml

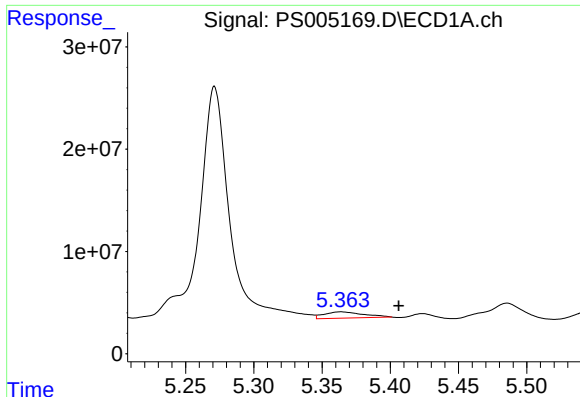

#3 4-Nitrophenol


R.T.: 5.364 min
Delta R.T.: -0.042 min
Response: 12255311
Conc: 16.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

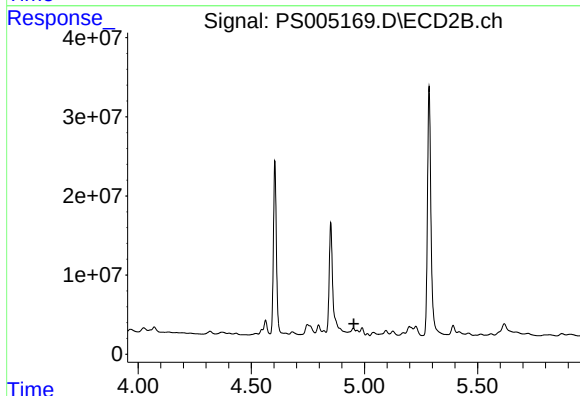


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

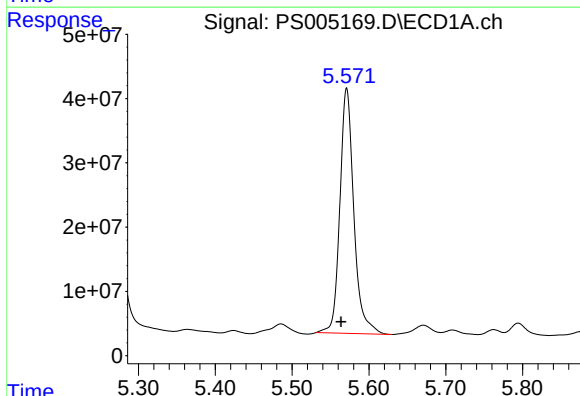


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: 0.007 min
Response: 480075476
Conc: 327.05 ng/ml

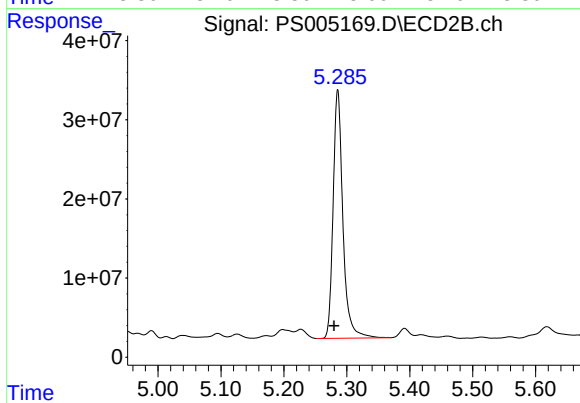

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: 0.006 min
Response: 338318253
Conc: 337.52 ng/ml

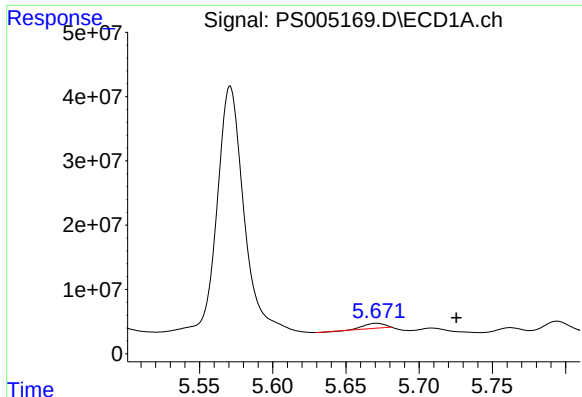

#5 DICAMBA


R.T.: 5.671 min
Delta R.T.: -0.055 min
Response: 7308451
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

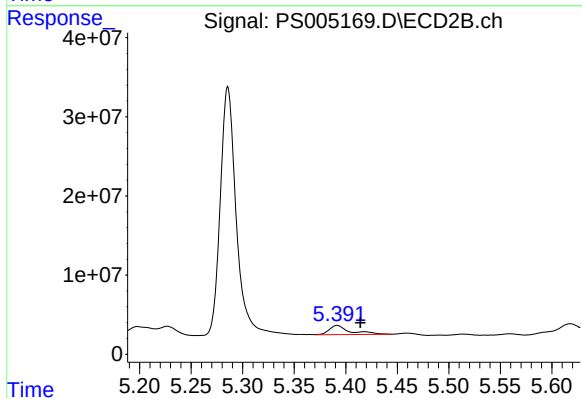


#5 DICAMBA

R.T.: 5.392 min
Delta R.T.: -0.022 min
Response: 16009332
Conc: 4.28 ng/ml

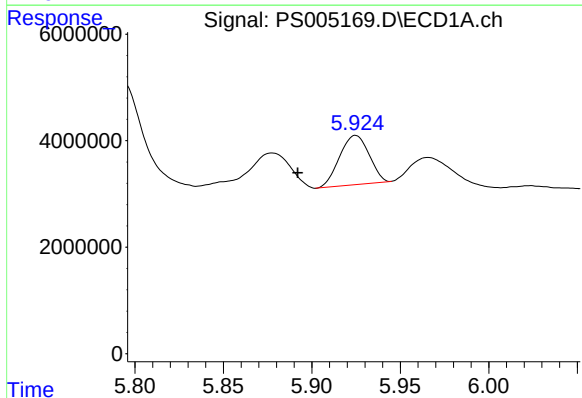


#6 MCP

R.T.: 5.925 min
Delta R.T.: 0.033 min
Response: 10723107
Conc: 2.45 ug/ml

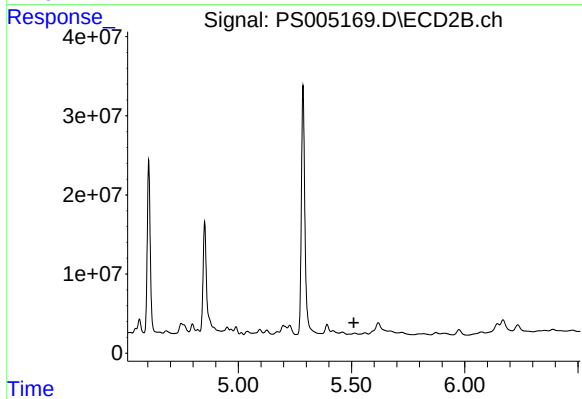

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

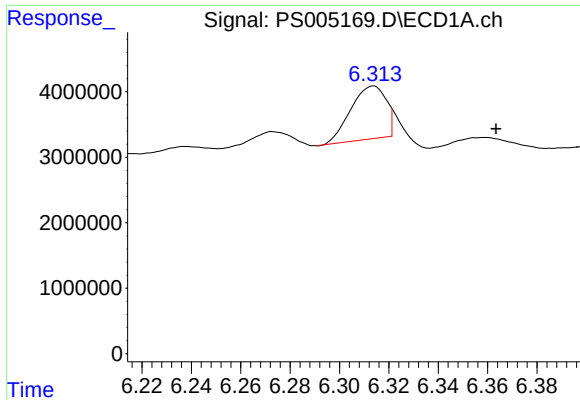

#8 DICHLORPROP


R.T.: 6.313 min
Delta R.T.: -0.050 min
Response: 8209918
Conc: 5.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

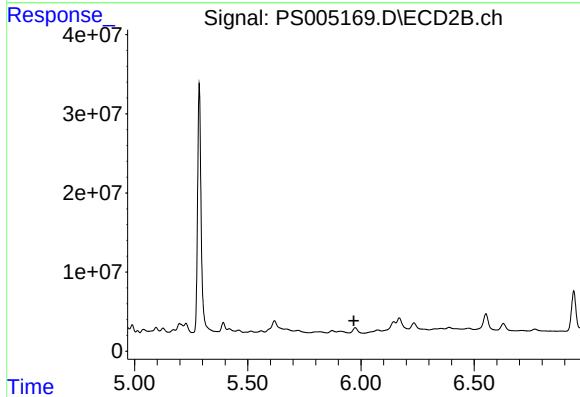


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.969 min
Response: 0
Conc: N.D.

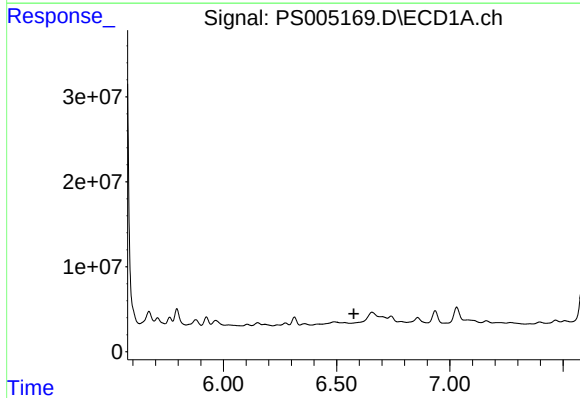


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.576 min
Response: 0
Conc: N.D.

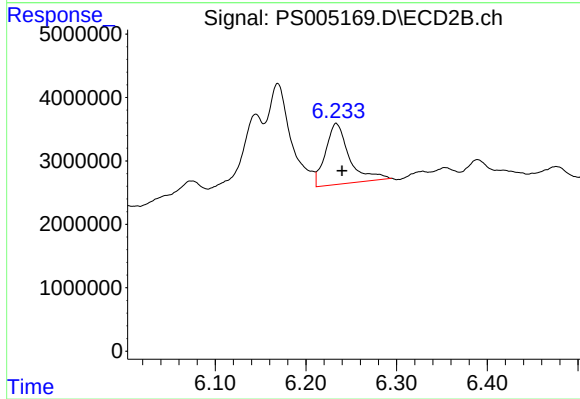

#9 2,4-D


R.T.: 6.234 min
Delta R.T.: -0.006 min
Response: 17502704
Conc: 15.69 ng/ml

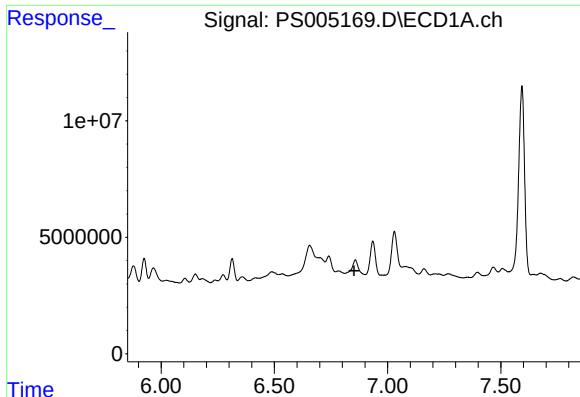

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

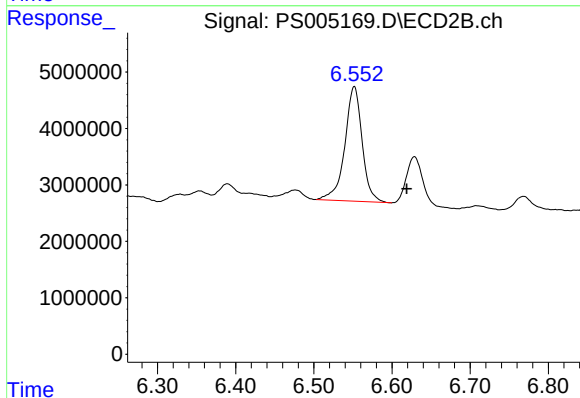


#10 Pentachlorophenol

R.T.: 6.552 min
Delta R.T.: -0.067 min
Response: 31288334
Conc: 2.43 ng/ml

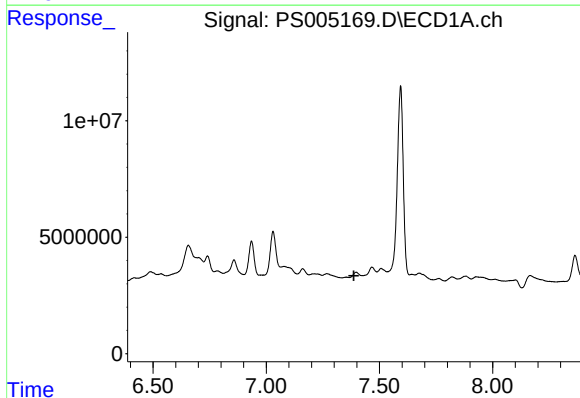


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

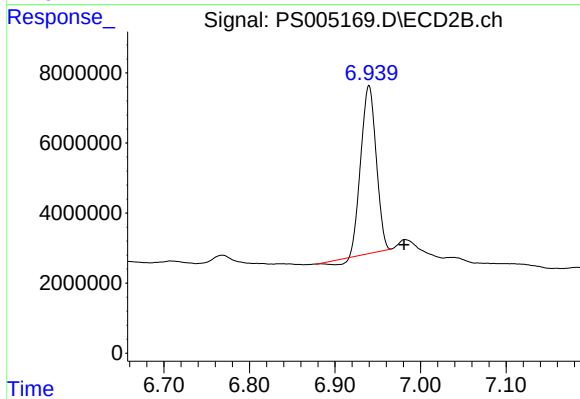

#11 2,4,5-TP (SILVEX)


R.T.: 6.940 min
Delta R.T.: -0.041 min
Response: 58327618
Conc: 10.95 ng/ml

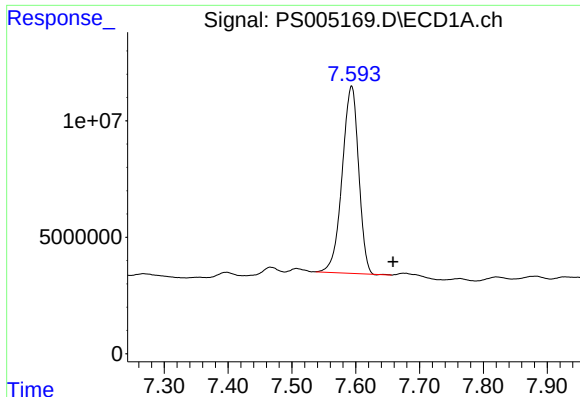

#12 2,4,5-T

R.T.: 7.593 min
Delta R.T.: -0.065 min
Response: 144052341
Conc: 17.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

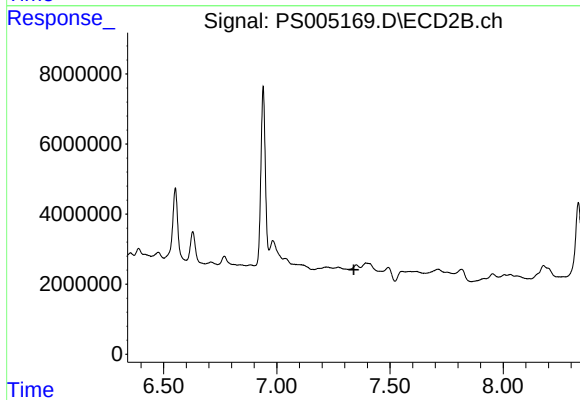

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.