

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 17:33
 Operator : SM\AJ
 Sample : K3455-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 23:00:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.570	5.284	469.4E6	336.0E6	319.764	335.195
Target Compounds							
1) T	Dalapon	2.073	0.000	69071133	0	37.472	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	211.8E6	N.D.	160.636
3) T	4-Nitroph...	5.362	0.000	13239561	0	18.279	N.D. #
5) T	DICAMBA	5.669	5.390	8492329	14097113	1.489	3.766 #
6) T	MCP	5.923	0.000	10895896	0	2.489	N.D. #
9) T	2,4-D	0.000	6.232	0	17803274	N.D.	15.963
10) T	Pentachlo...	0.000	6.550	0	24342625	N.D.	1.893
11) T	2,4,5-TP ...	0.000	6.938	0	68727451	N.D.	12.906
12) T	2,4,5-T	7.592	0.000	132.1E6	0	16.418	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 17:33
Operator : SM\AJ
Sample : K3455-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 23:00:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

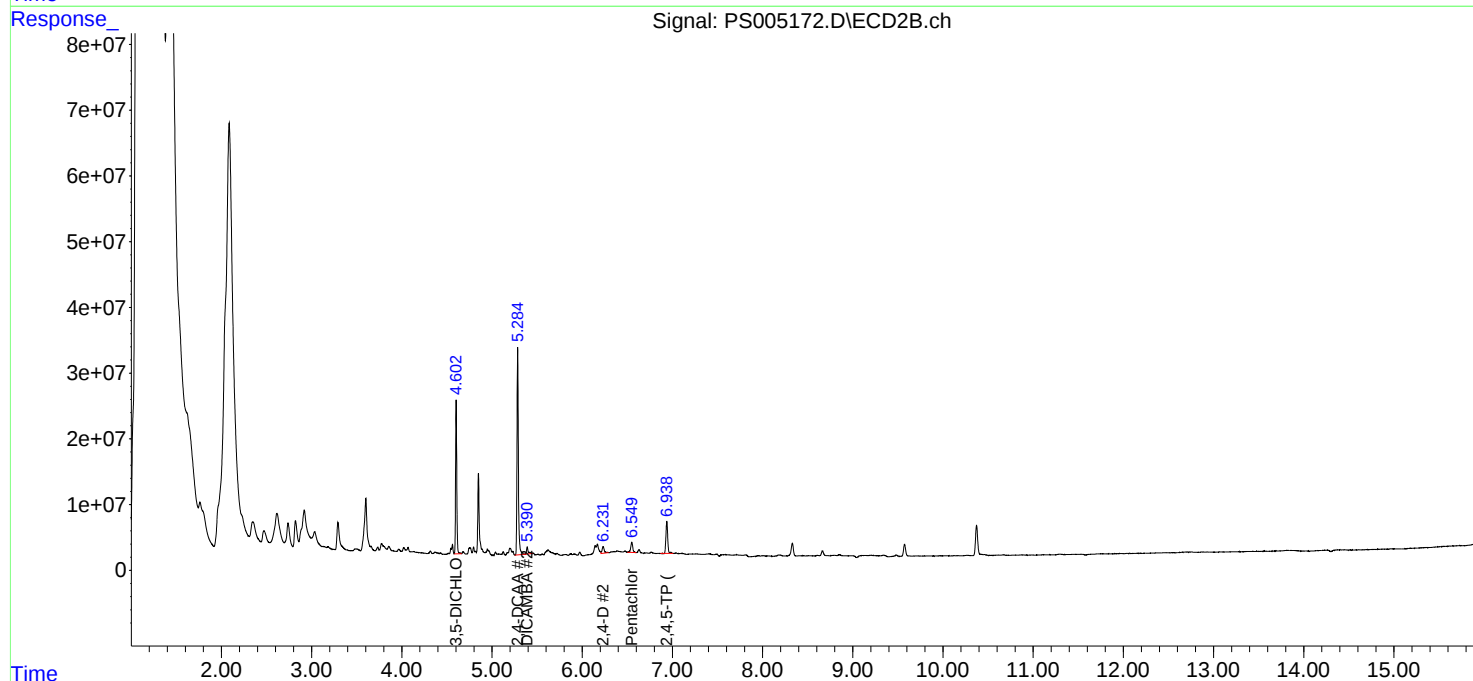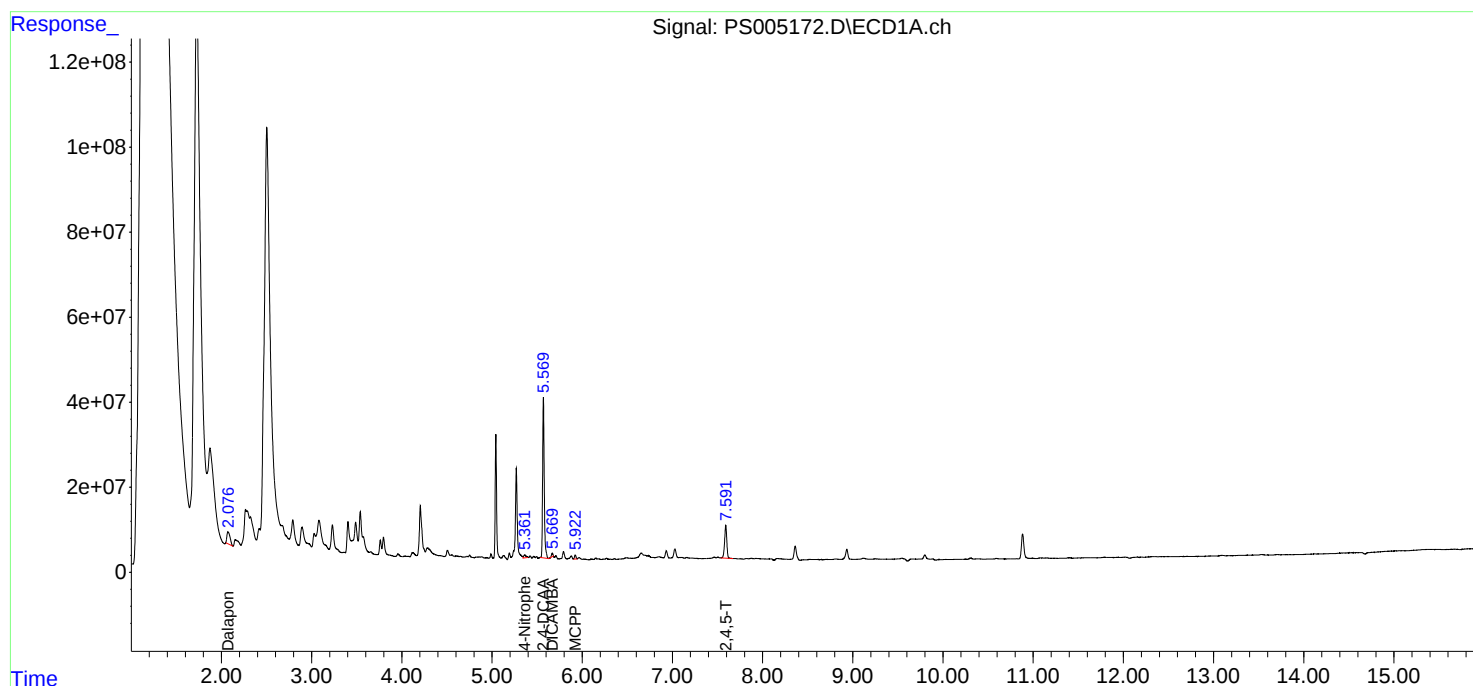


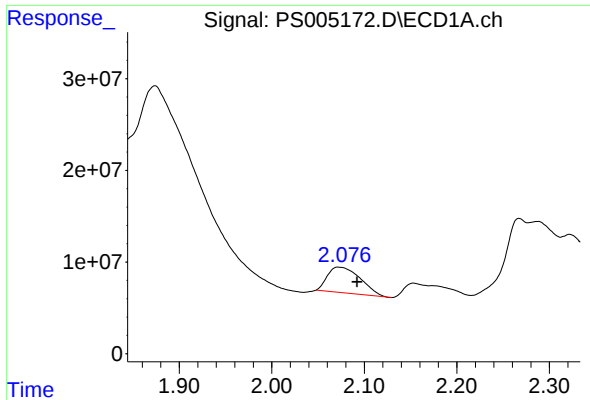

#1 Dalapon


R.T.: 2.073 min
Delta R.T.: -0.019 min
Response: 69071133
Conc: 37.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

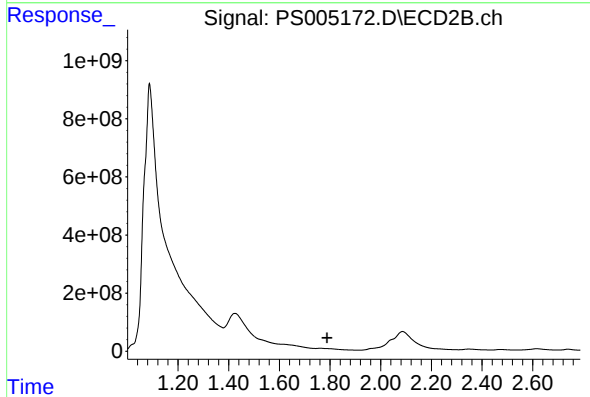


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

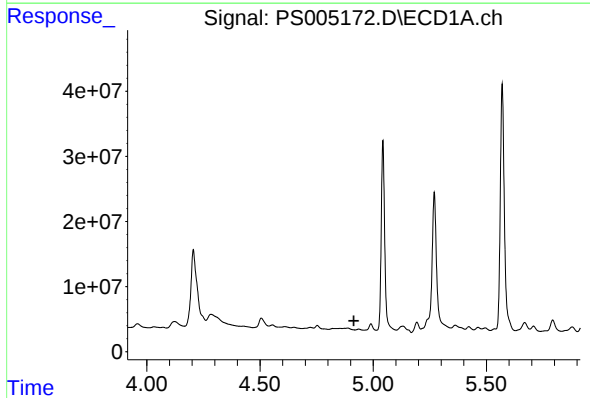


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

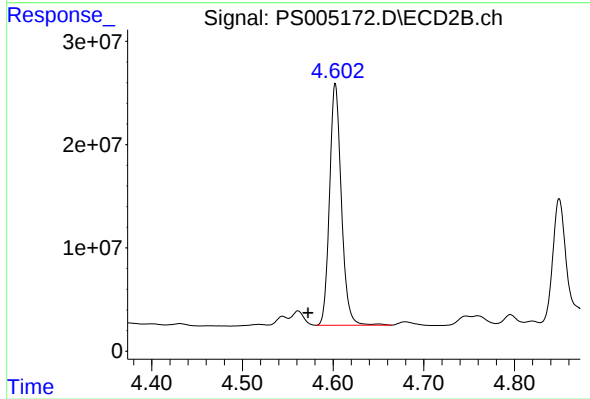

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.030 min
Response: 211832021
Conc: 160.64 ng/ml

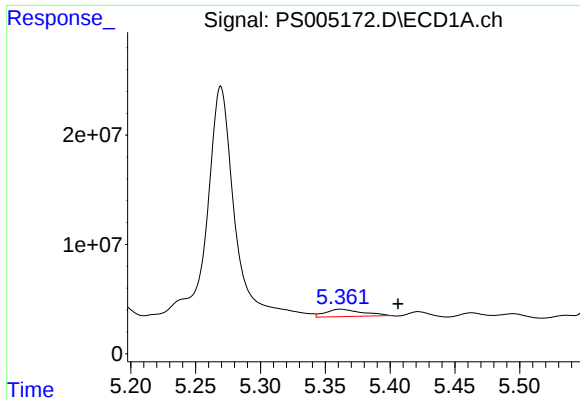

#3 4-Nitrophenol


R.T.: 5.362 min
Delta R.T.: -0.044 min
Response: 13239561
Conc: 18.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

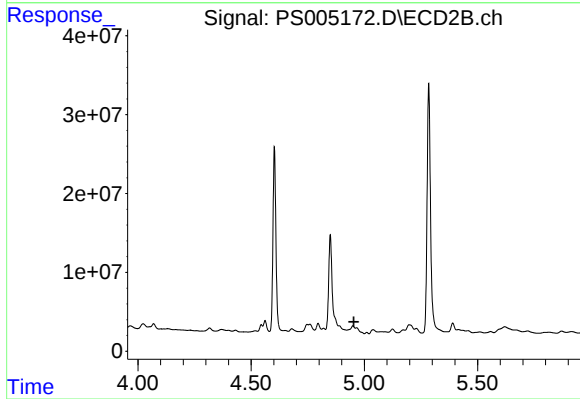


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

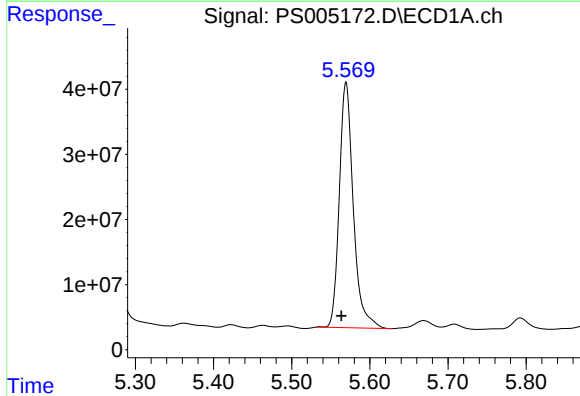


#4 2,4-DCAA

R.T.: 5.570 min
Delta R.T.: 0.006 min
Response: 469379174
Conc: 319.76 ng/ml

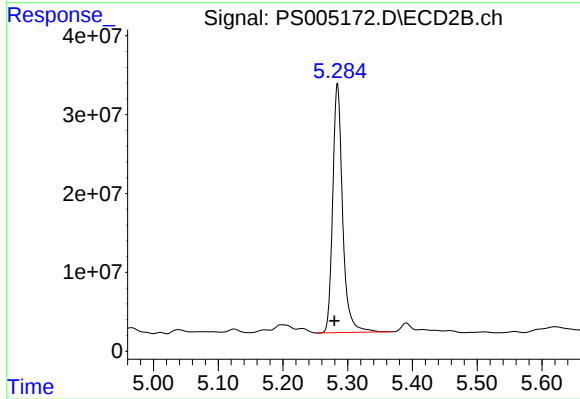

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: 0.005 min
Response: 335989170
Conc: 335.20 ng/ml

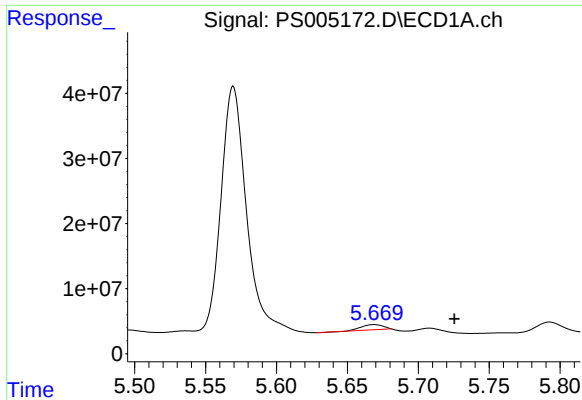

#5 DICAMBA


R.T.: 5.669 min
Delta R.T.: -0.057 min
Response: 8492329
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

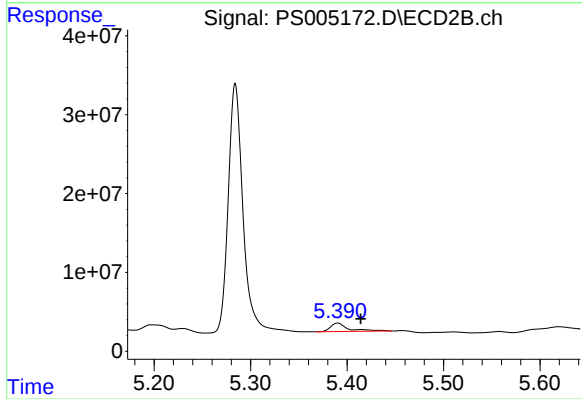


#5 DICAMBA

R.T.: 5.390 min
Delta R.T.: -0.024 min
Response: 14097113
Conc: 3.77 ng/ml

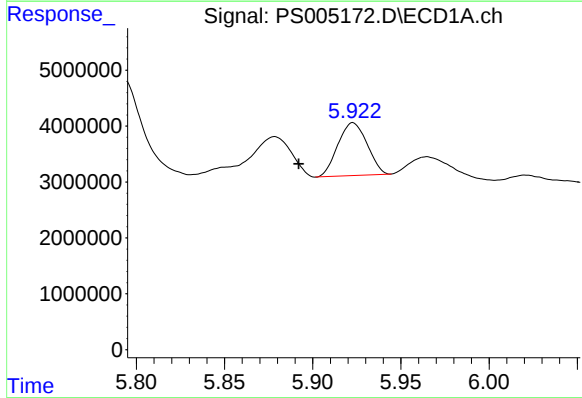


#6 MCP

R.T.: 5.923 min
Delta R.T.: 0.031 min
Response: 10895896
Conc: 2.49 ug/ml

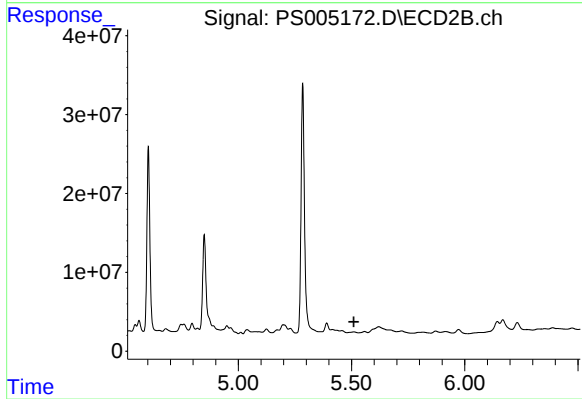

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

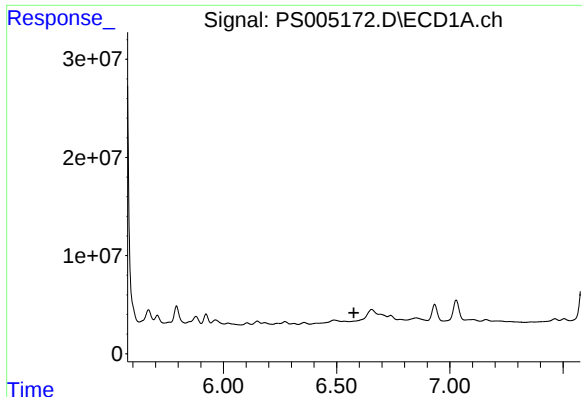

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

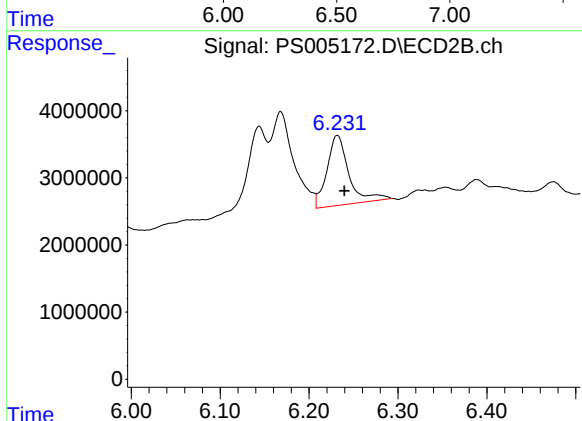


#9 2,4-D

R.T.: 6.232 min
Delta R.T.: -0.008 min
Response: 17803274
Conc: 15.96 ng/ml

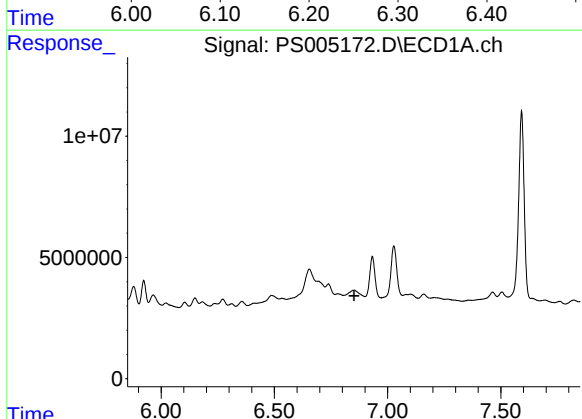


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

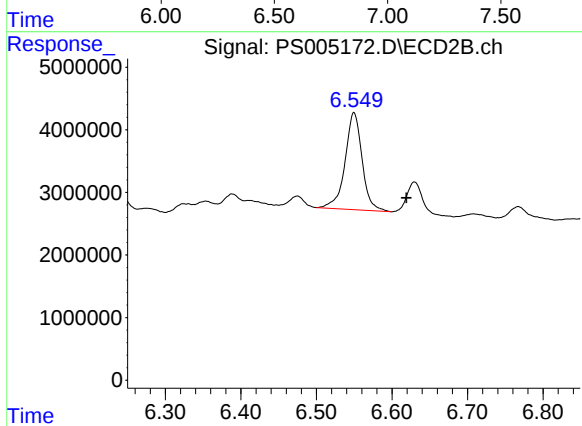

#10 Pentachlorophenol


R.T.: 6.550 min
Delta R.T.: -0.069 min
Response: 24342625
Conc: 1.89 ng/ml

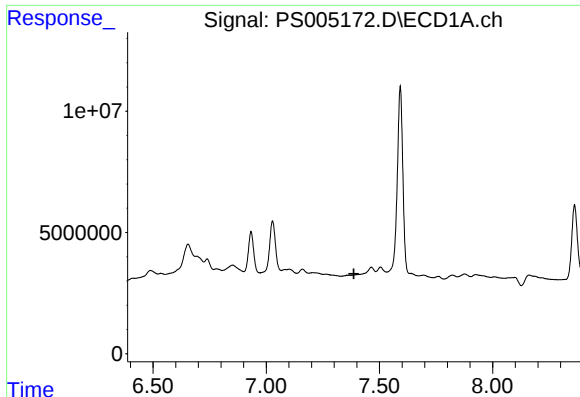

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

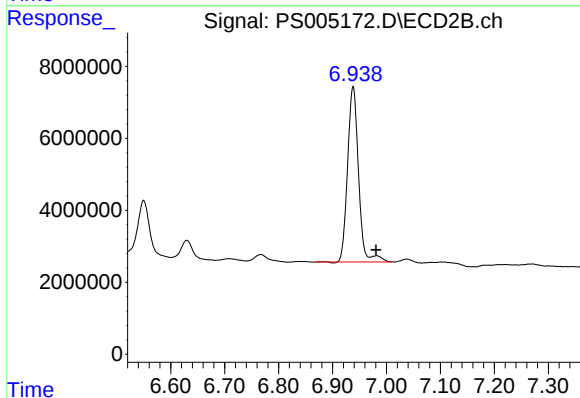


#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.042 min
Response: 68727451
Conc: 12.91 ng/ml

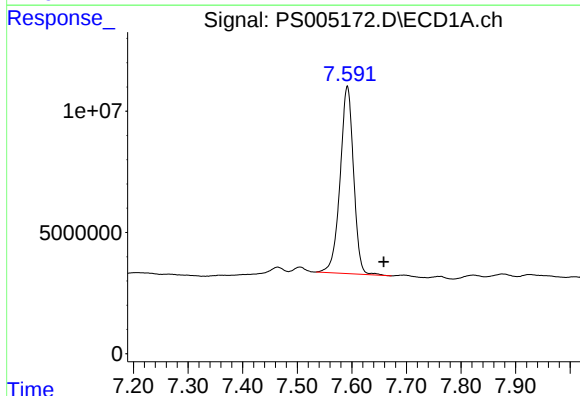

#12 2,4,5-T

R.T.: 7.592 min
Delta R.T.: -0.067 min
Response: 132132219
Conc: 16.42 ng/ml

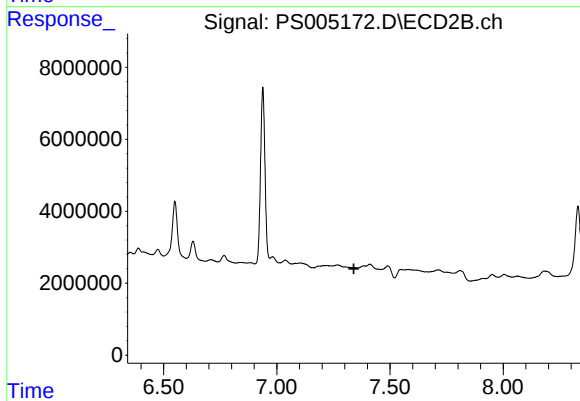

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.