

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 17:54
 Operator : SM\AJ
 Sample : K3455-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 23:00:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.302	443.0E6	303.6E6	301.780	302.919
Target Compounds							
1) T	Dalapon	2.093	0.000	71308540	0	38.685	N.D. #
2) T	3,5-DICHL...	0.000	4.579	0	17935986	N.D.	13.601
3) T	4-Nitroph...	5.380	0.000	5900400	0	8.146	N.D. #
5) T	DICAMBA	0.000	5.408	0	12929837	N.D.	3.454
6) T	MCP	5.942	0.000	11286697	0	2.578	N.D. #
9) T	2,4-D	0.000	6.250	0	11971019	N.D.	10.734
10) T	Pentachlo...	0.000	6.568	0	25632858	N.D.	1.994
11) T	2,4,5-TP ...	0.000	6.956	0	70219140	N.D.	13.186
12) T	2,4,5-T	7.610	0.000	143.1E6	0	17.776	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 17:54
Operator : SM\AJ
Sample : K3455-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 23:00:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

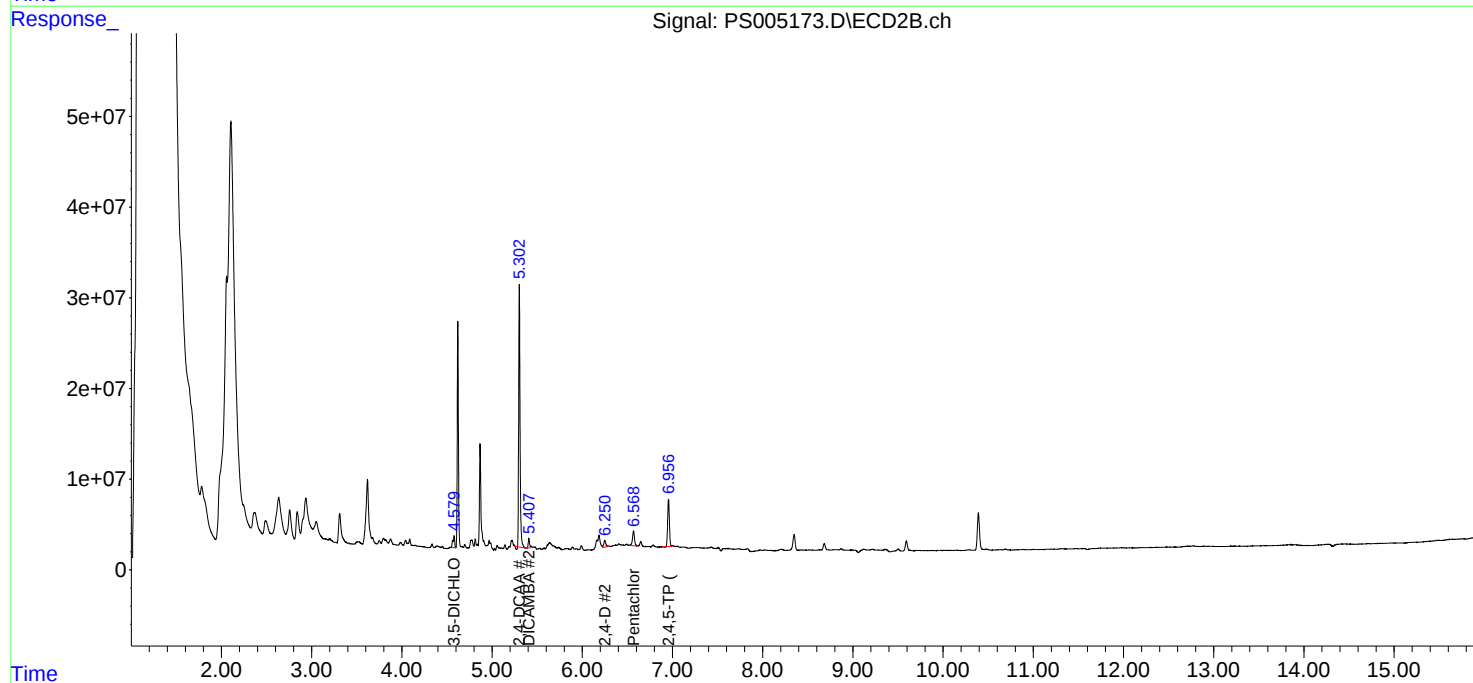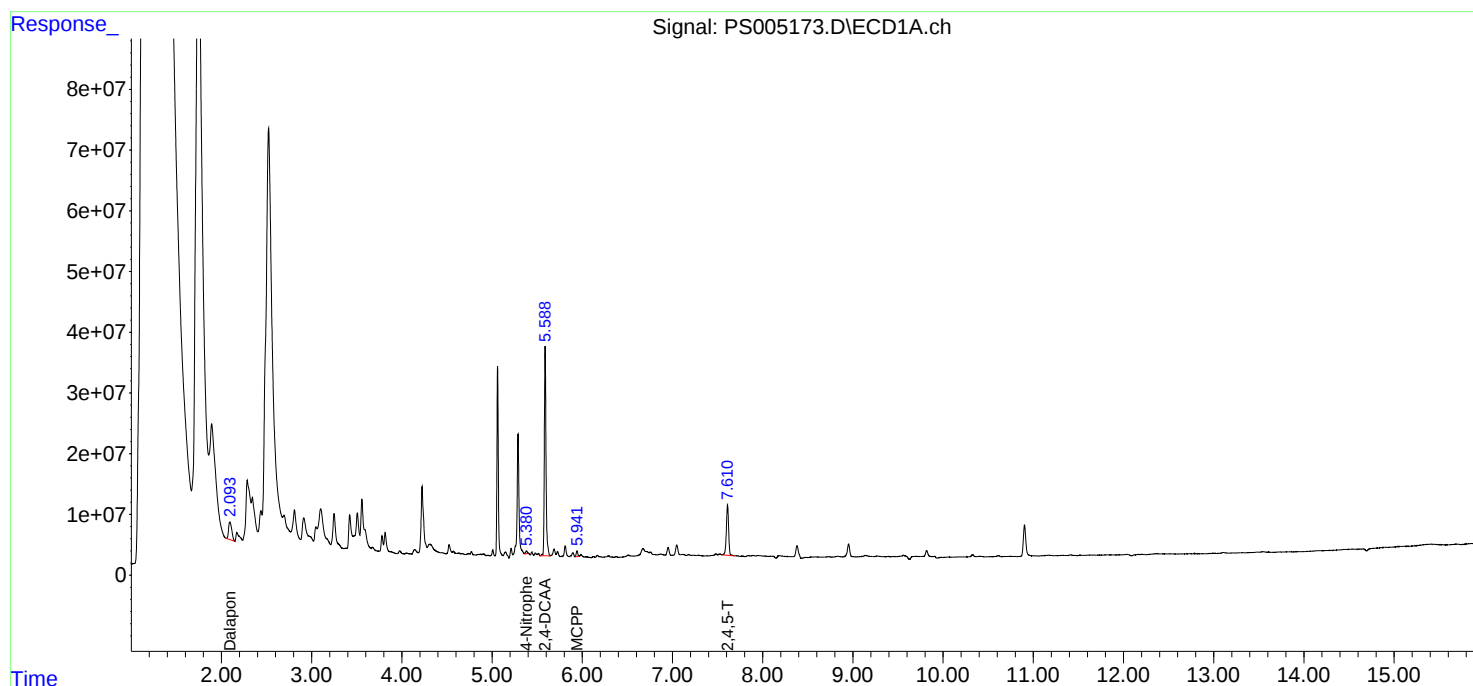


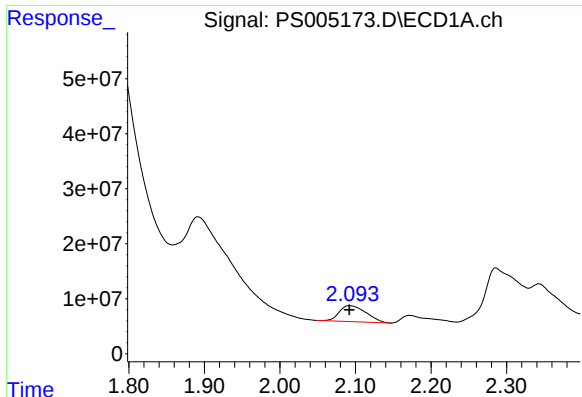

#1 Dalapon


R.T.: 2.093 min
Delta R.T.: 0.000 min
Response: 71308540
Conc: 38.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

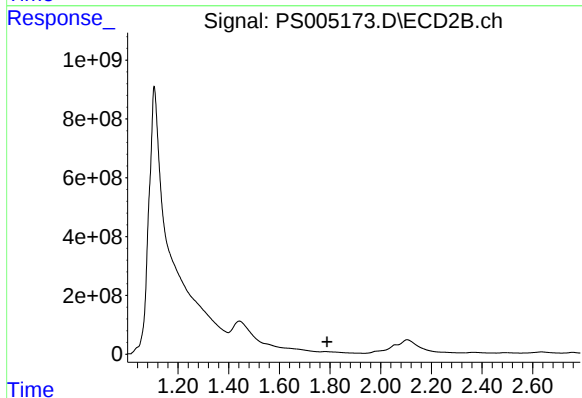


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

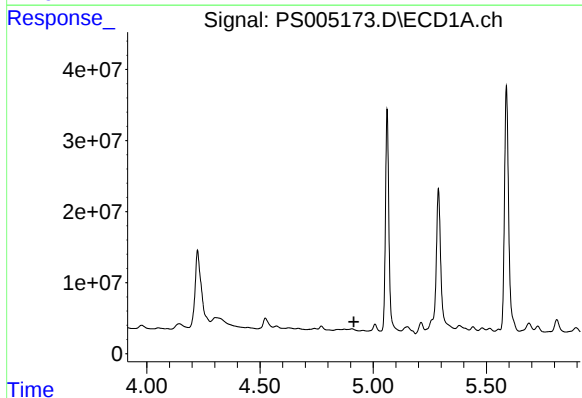


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

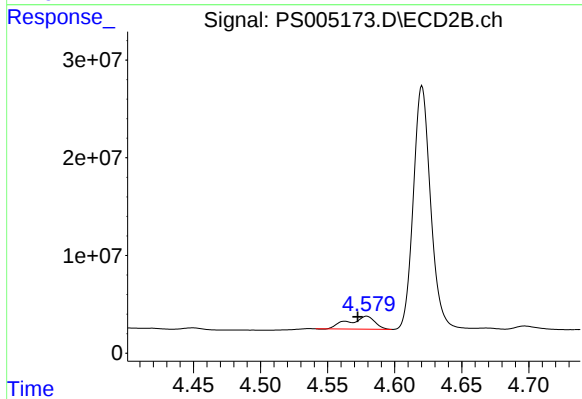

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.579 min
Delta R.T.: 0.006 min
Response: 17935986
Conc: 13.60 ng/ml

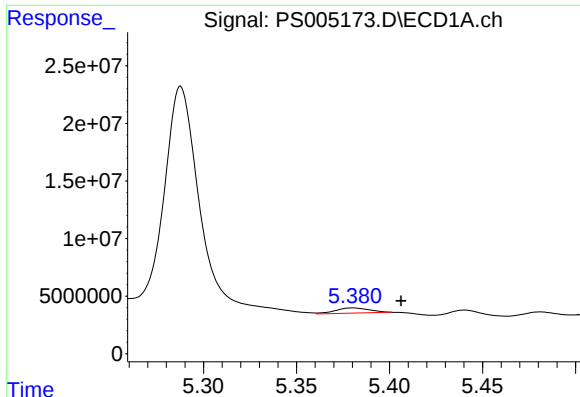

#3 4-Nitrophenol


R.T.: 5.380 min
Delta R.T.: -0.026 min
Response: 5900400
Conc: 8.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

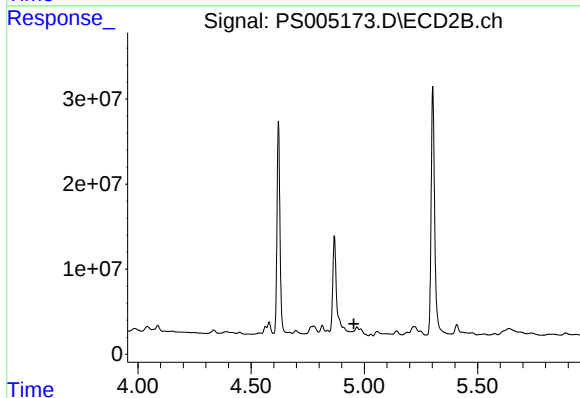


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

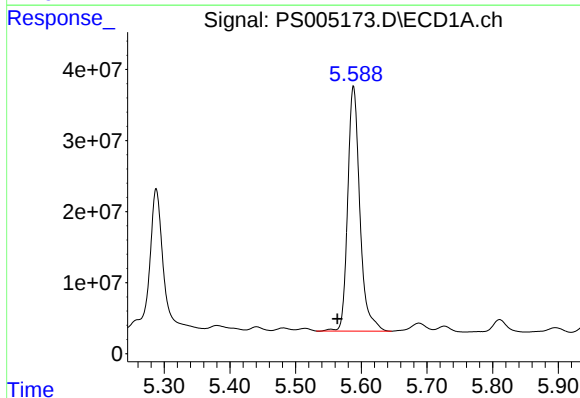


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: 0.025 min
Response: 442980638
Conc: 301.78 ng/ml

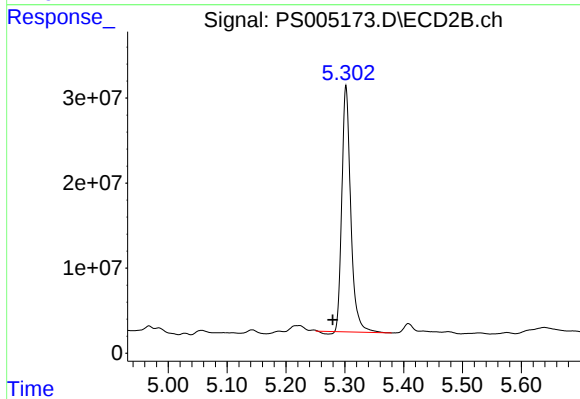

#4 2,4-DCAA


R.T.: 5.302 min
Delta R.T.: 0.023 min
Response: 303636894
Conc: 302.92 ng/ml

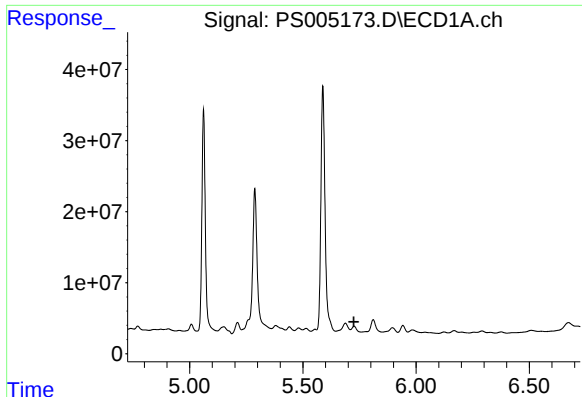

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

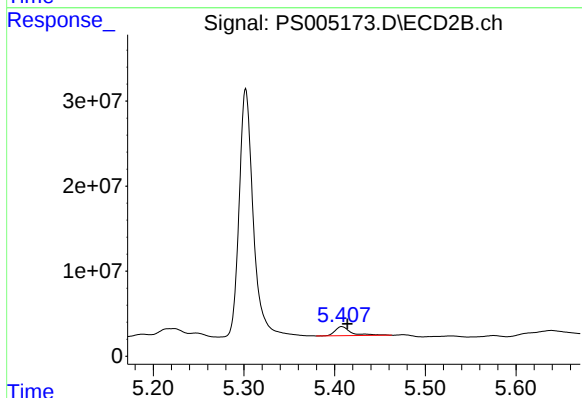


#5 DICAMBA

R.T.: 5.408 min
Delta R.T.: -0.006 min
Response: 12929837
Conc: 3.45 ng/ml

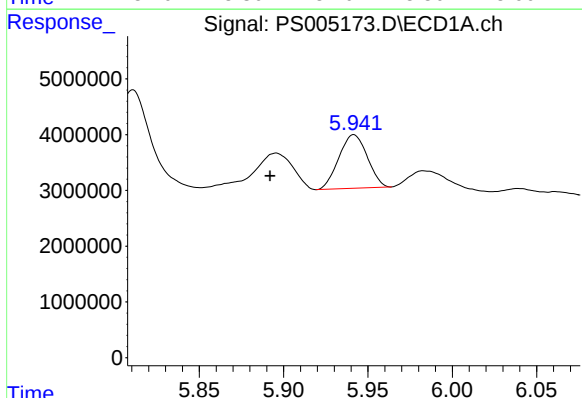


#6 MCP

R.T.: 5.942 min
Delta R.T.: 0.050 min
Response: 11286697
Conc: 2.58 ug/ml

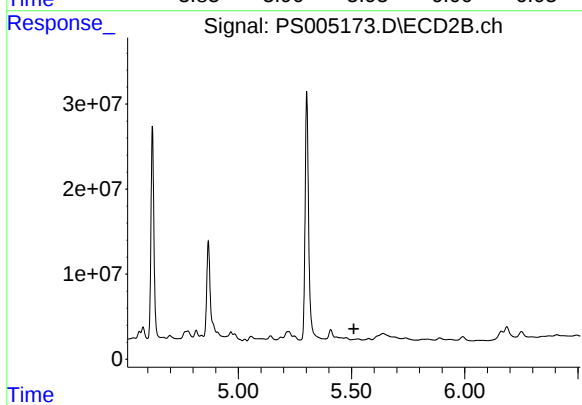

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

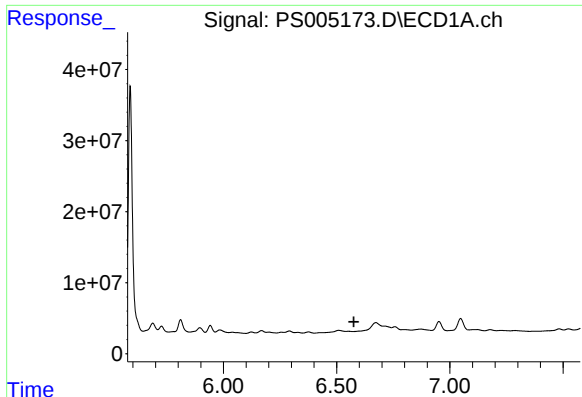

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

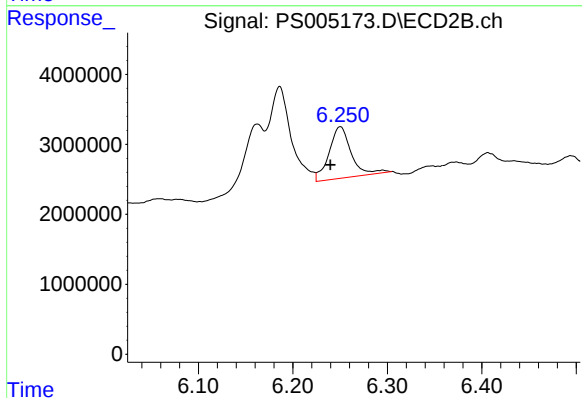


#9 2,4-D

R.T.: 6.250 min
Delta R.T.: 0.010 min
Response: 11971019
Conc: 10.73 ng/ml

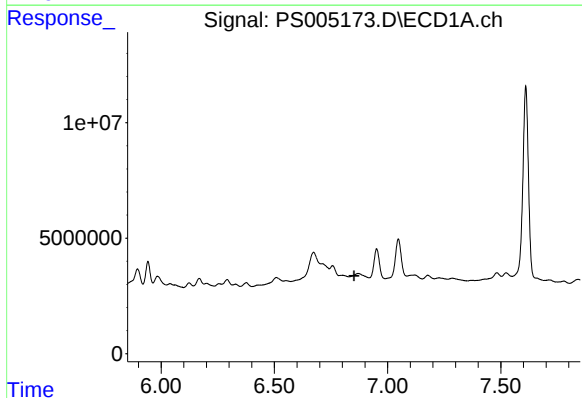


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

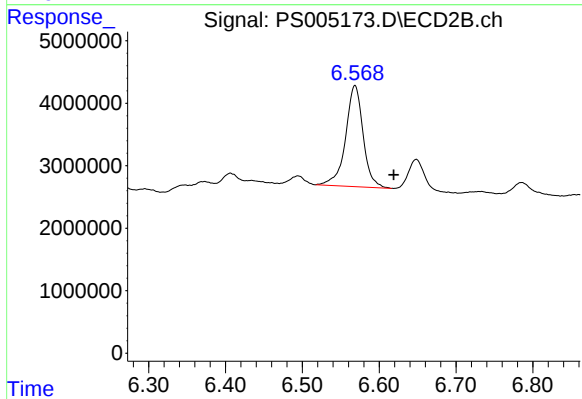

#10 Pentachlorophenol


R.T.: 6.568 min
Delta R.T.: -0.051 min
Response: 25632858
Conc: 1.99 ng/ml

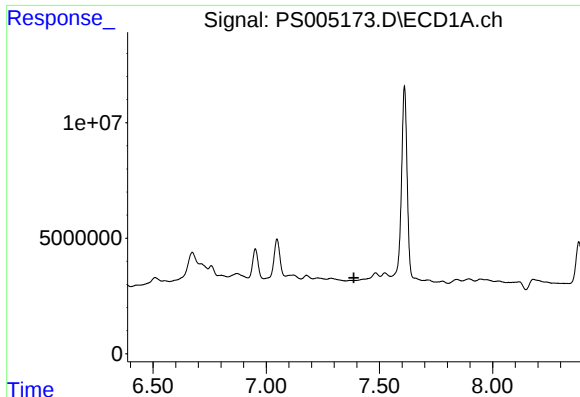

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

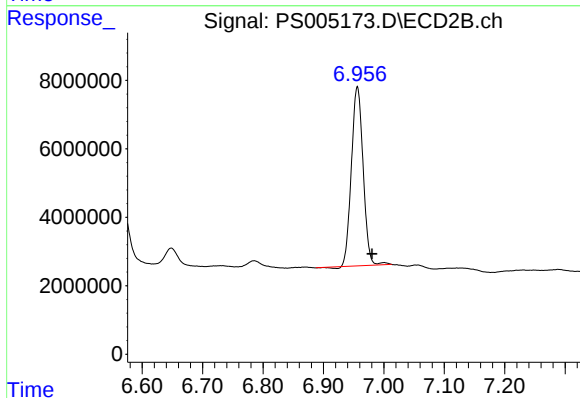


#11 2,4,5-TP (SILVEX)

R.T.: 6.956 min
Delta R.T.: -0.024 min
Response: 70219140
Conc: 13.19 ng/ml

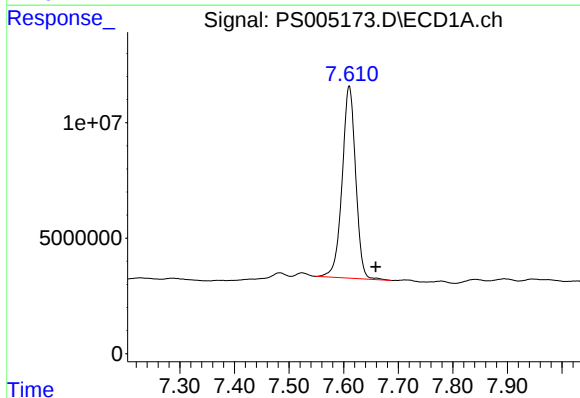

#12 2,4,5-T

R.T.: 7.610 min
Delta R.T.: -0.048 min
Response: 143055590
Conc: 17.78 ng/ml

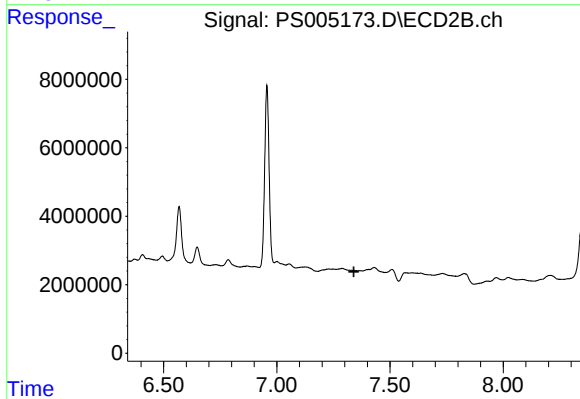

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.