

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
 Data File : PS005173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2019 17:54
 Operator : SM\AJ
 Sample : K3455-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5-DUCT-BANK

Manual Integrations
 APPROVED

Ankita
 6/24/2019 8:59:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 23:00:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.302	443.0E6	317.6E6	301.780	316.807m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062119\
Data File : PS005173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2019 17:54
Operator : SM\AJ
Sample : K3455-10
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-5-DUCT-BANK


Manual Integrations
APPROVED

Ankita
6/24/2019 8:59:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 23:00:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

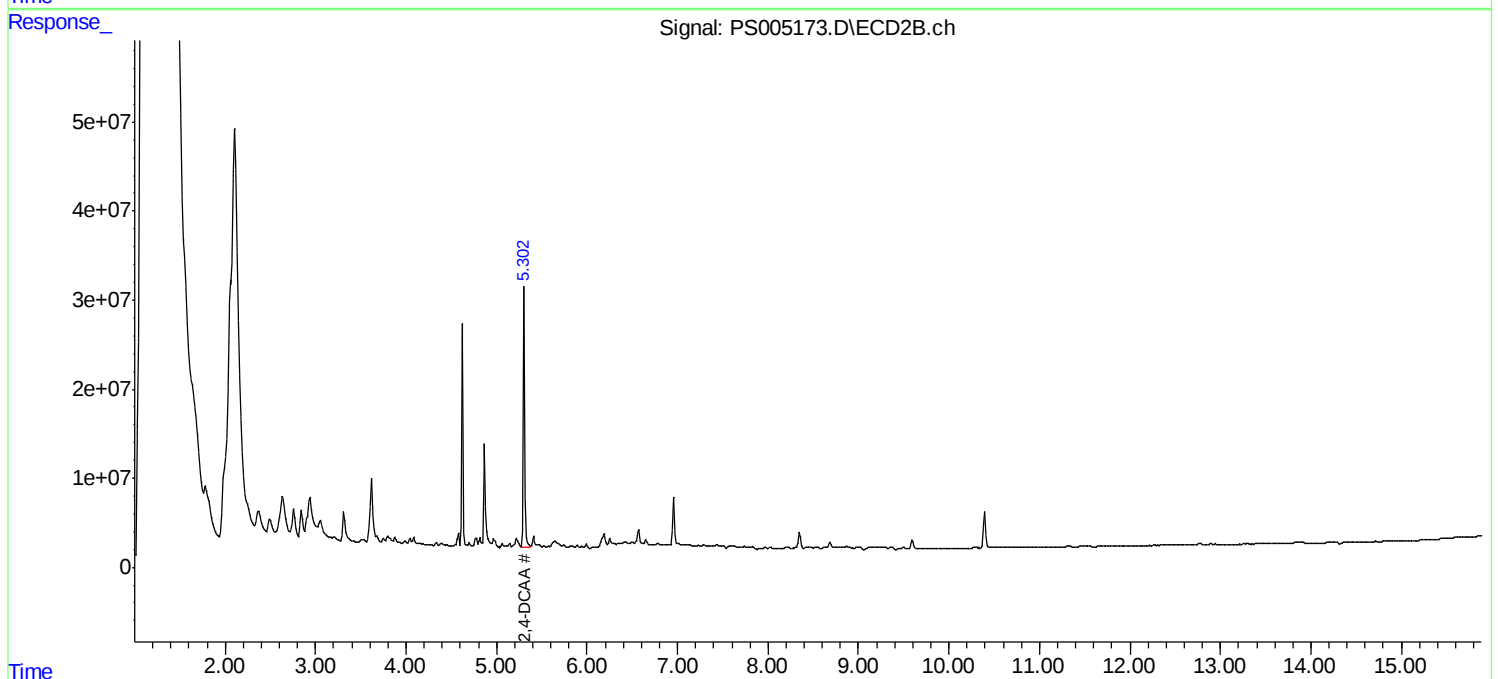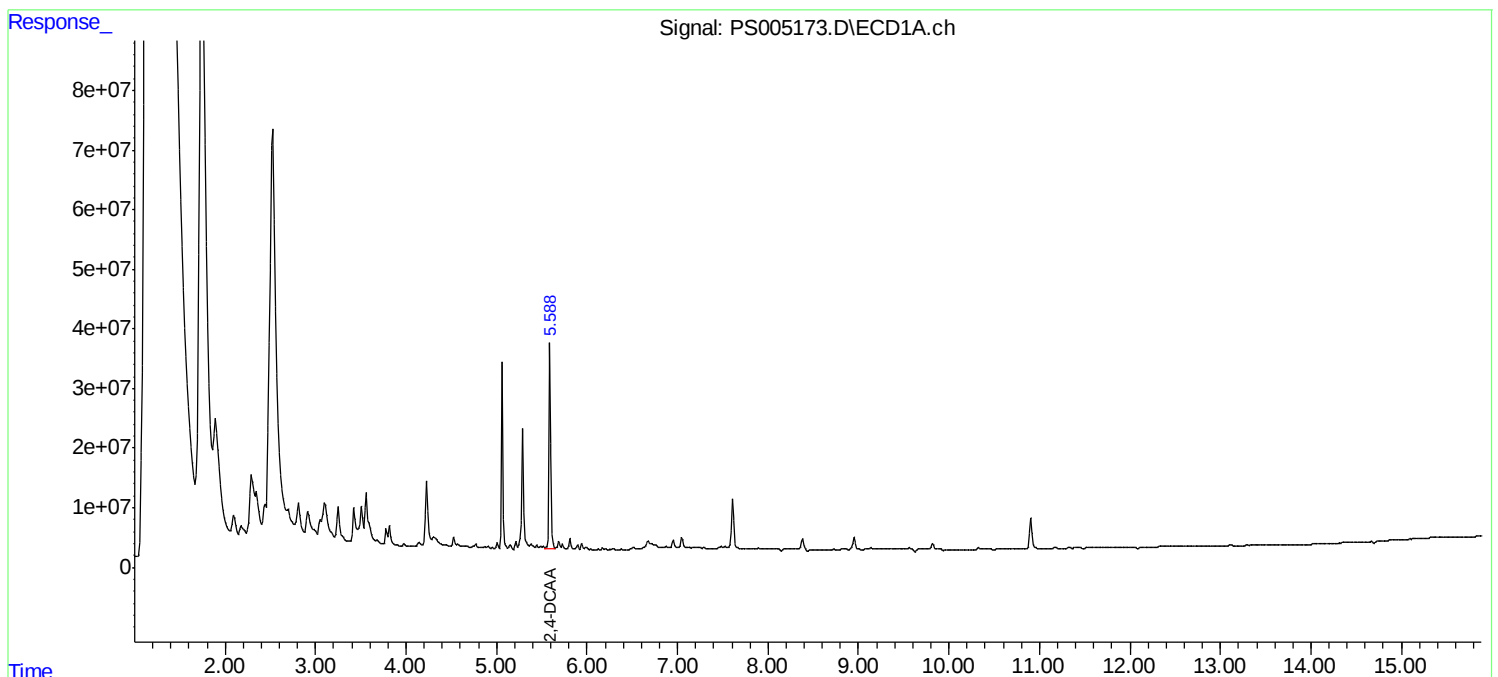

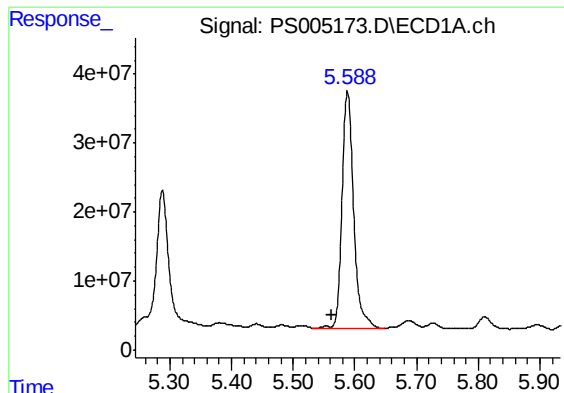


#4 2,4-DCAA

R.T.: 5.588 min
Delta R.T.: 0.025 min
Response: 442980638
Conc: 301.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-DUCT-BANK

Manual Integrations
APPROVED

Ankita
6/24/2019 8:59:29 AM

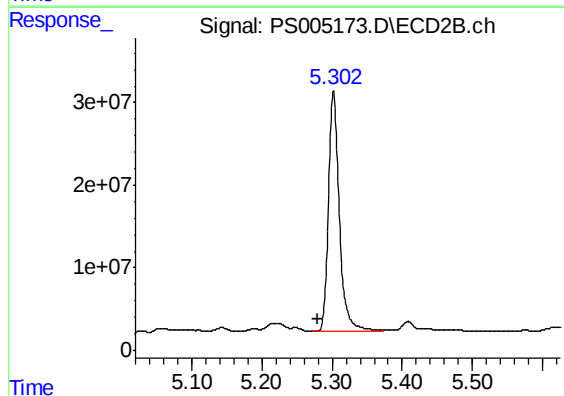

#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: 0.022 min
Response: 317557738
Conc: 316.81 ng/ml m