

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
 Data File : PS005202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2019 18:40
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:07:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	4.937	0.000	7672.7E6	0	3817.775	N.D. #
3) T	4-Nitroph...	5.391	0.000	14828194	0	20.473	N.D. #
5) T	DICAMBA	0.000	5.441	0	6082.0E6	N.D.	1624.764
6) T	MCP	5.957	0.000	106.8E6	0	24.391	N.D. #
8) T	DICHLORPROP	6.418	5.976	26696735	90233450	18.668	93.454 #
9) T	2,4-D	6.607	0.000	8756.1E6	0	5632.373	N.D. #
10) T	Pentachlo...	6.870	6.641	57071100	19265907	2.901	1.499 #
12) T	2,4,5-T	0.000	7.394	0	60099378	N.D.	11.782
15) T	Picloram	9.103	9.096	3487.2E6	179.3E6	303.465	23.765 #
16) T	DCPA	0.000	9.096	0	179.3E6	N.D.	26.344



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
Data File : PS005202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2019 18:40
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:07:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

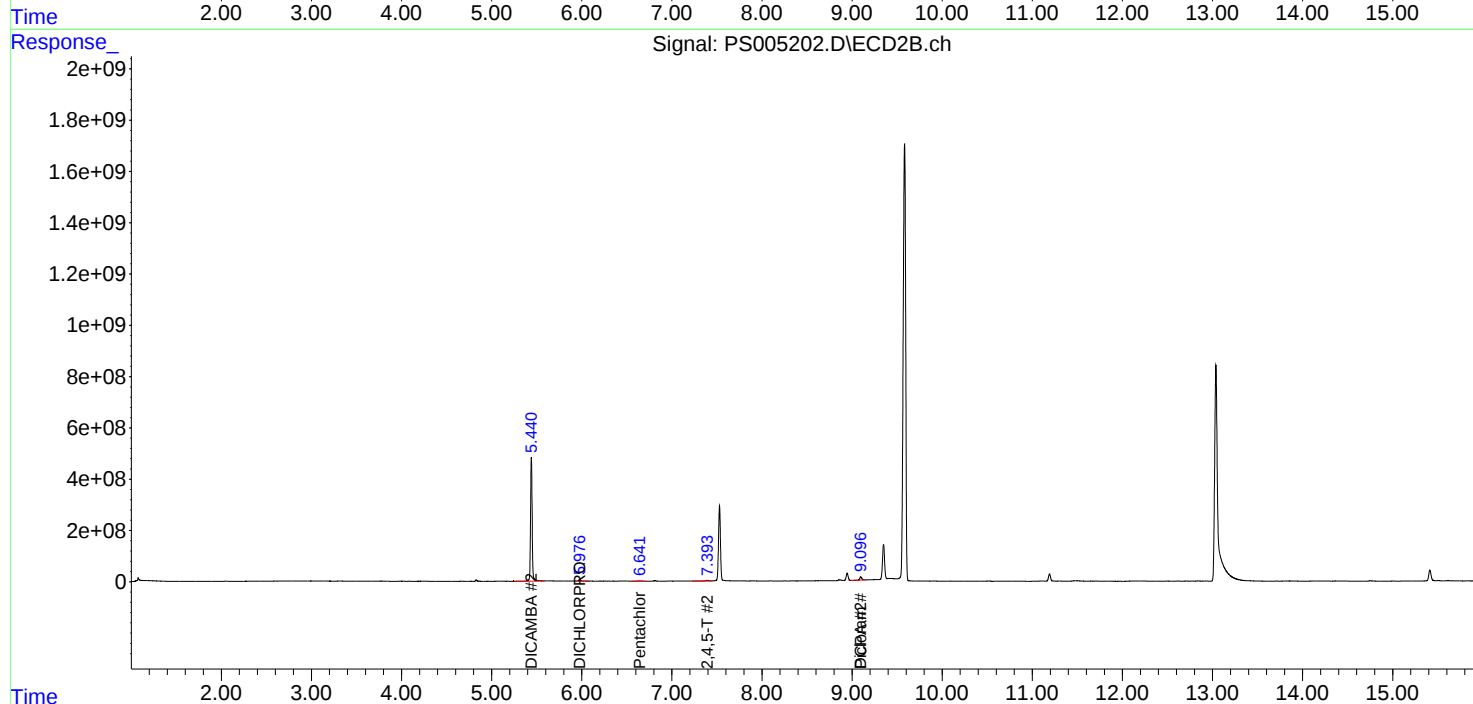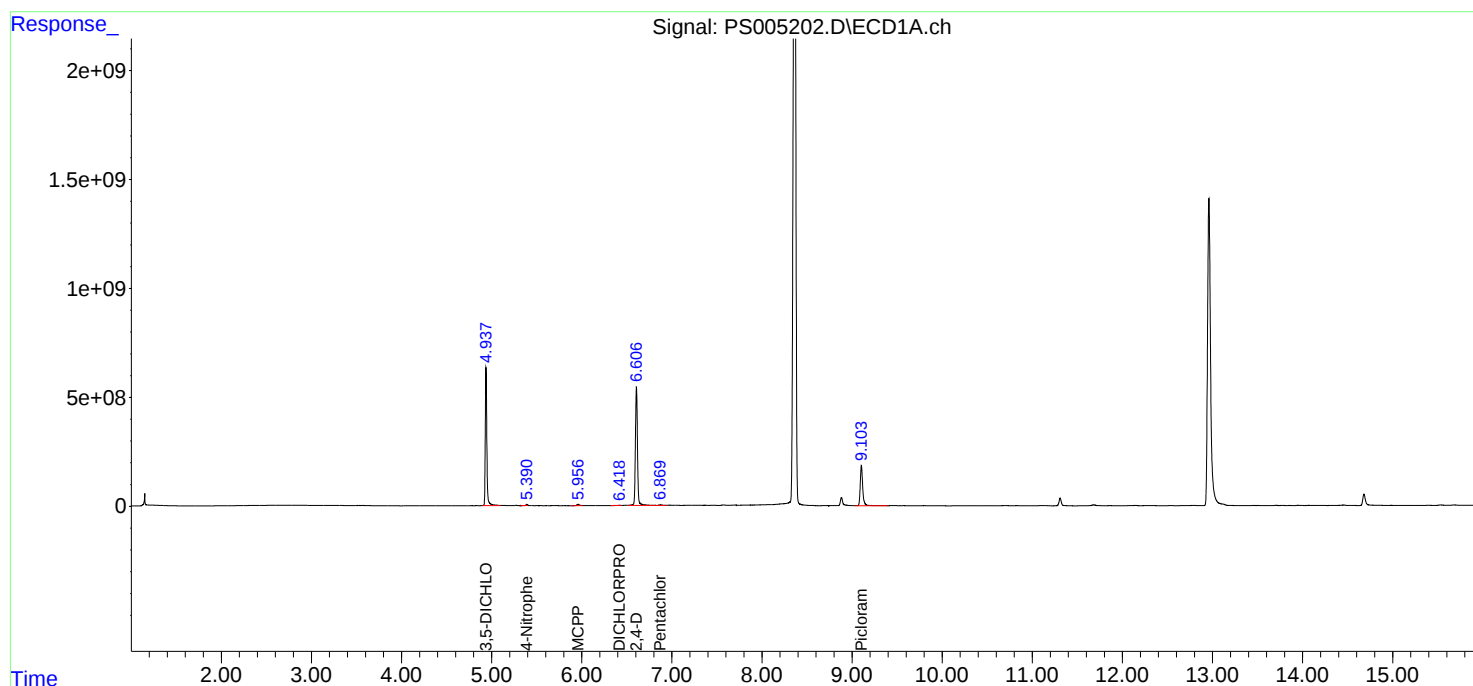


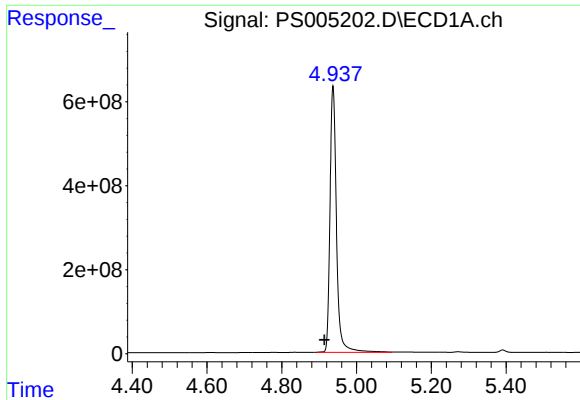

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.937 min
Delta R.T.: 0.023 min
Response: 7672652073
Conc: 3817.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

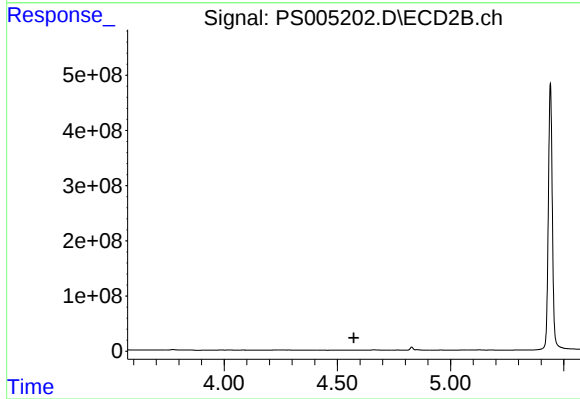


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

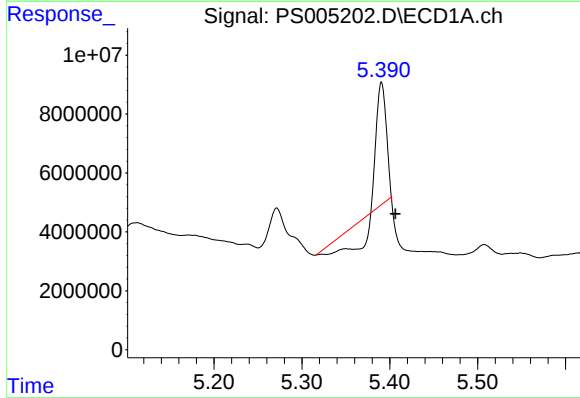


#3 4-Nitrophenol

R.T.: 5.391 min
Delta R.T.: -0.015 min
Response: 14828194
Conc: 20.47 ng/ml

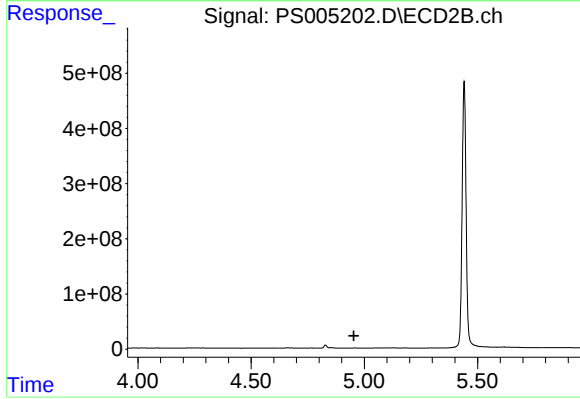

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

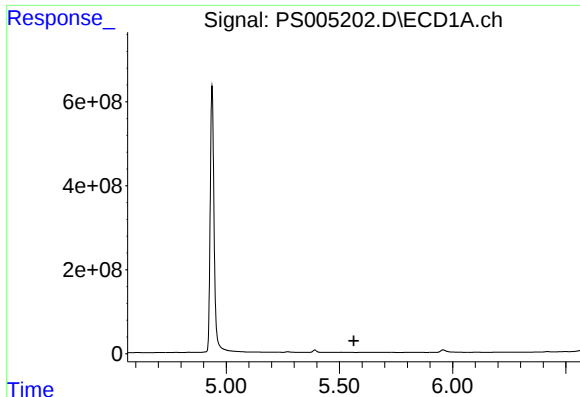

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.564 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

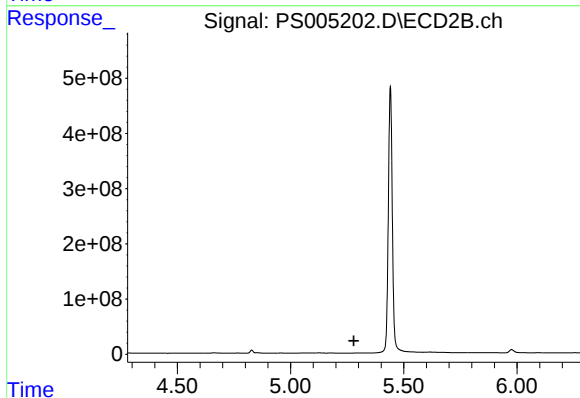


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.280 min
Response: 0
Conc: N.D.

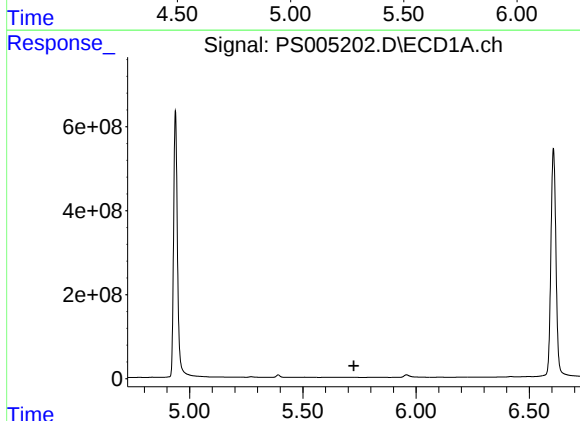


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

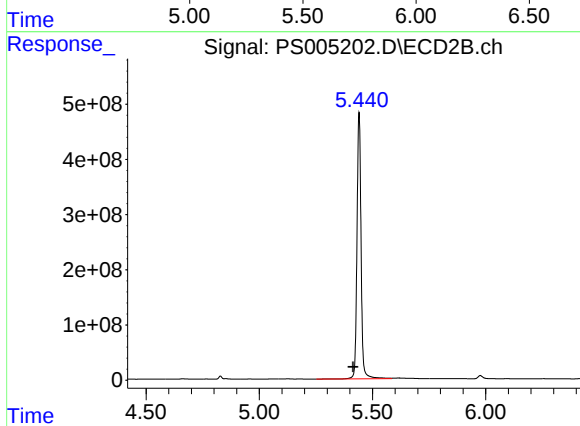

#5 DICAMBA


R.T.: 5.441 min
Delta R.T.: 0.027 min
Response: 6082019189
Conc: 1624.76 ng/ml

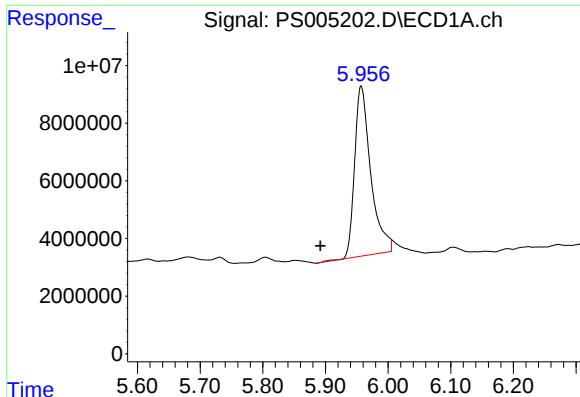

#6 MCP


R.T.: 5.957 min
Delta R.T.: 0.065 min
Response: 106773389
Conc: 24.39 ug/ml

Instrument :
ECD_S
ClientSampleId :

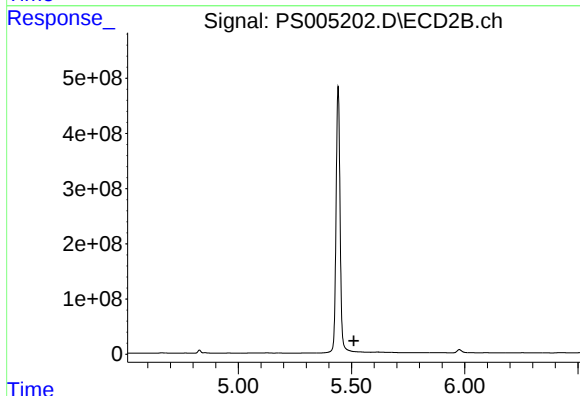


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

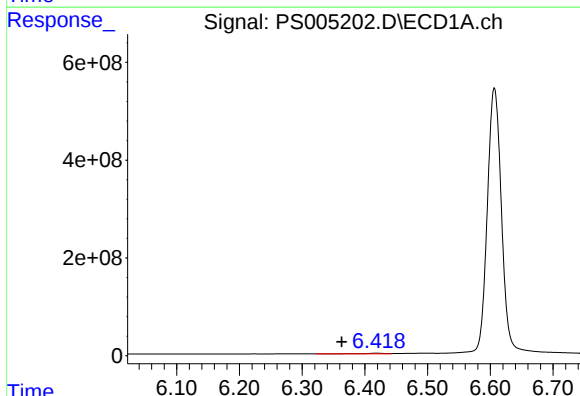


#8 DICHLORPROP

R.T.: 6.418 min
Delta R.T.: 0.055 min
Response: 26696735
Conc: 18.67 ng/ml

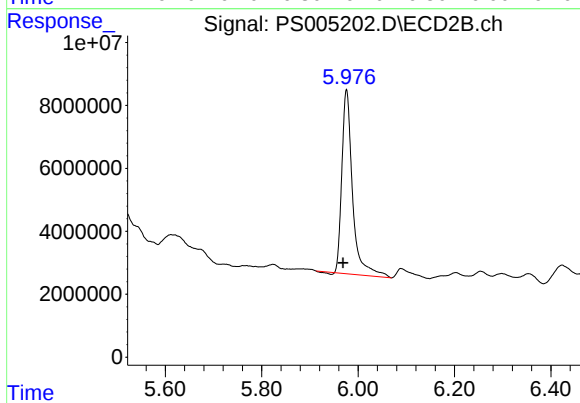

#8 DICHLORPROP


R.T.: 5.976 min
Delta R.T.: 0.007 min
Response: 90233450
Conc: 93.45 ng/ml

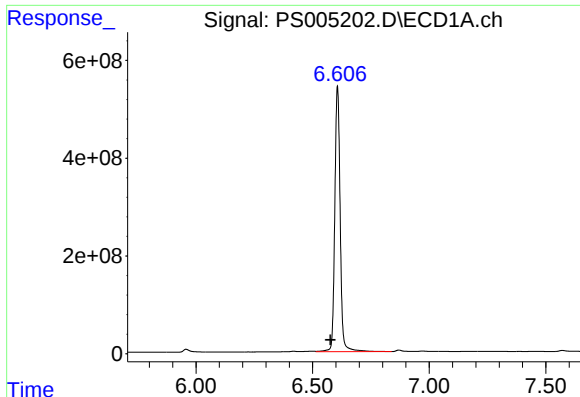

#9 2,4-D


R.T.: 6.607 min
Delta R.T.: 0.030 min
Response: 8756087495
Conc: 5632.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

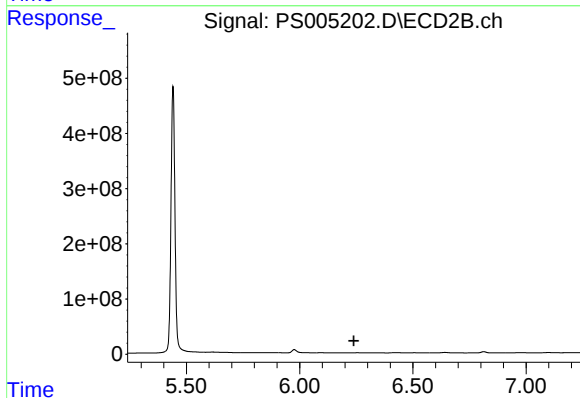


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

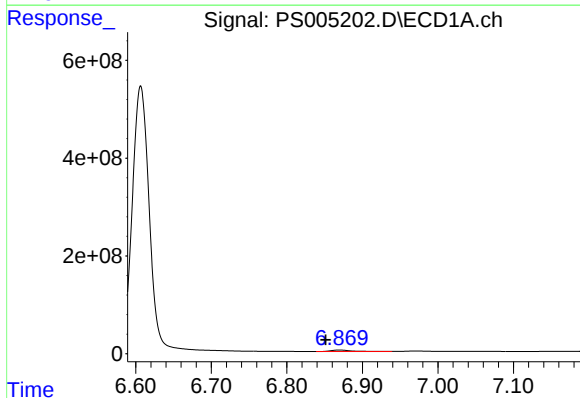


#10 Pentachlorophenol

R.T.: 6.870 min
Delta R.T.: 0.018 min
Response: 57071100
Conc: 2.90 ng/ml

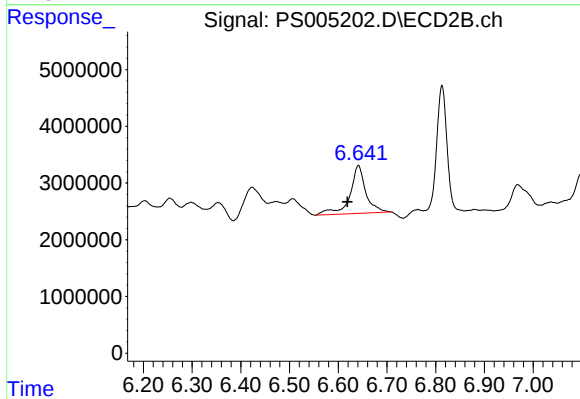

#10 Pentachlorophenol


R.T.: 6.641 min
Delta R.T.: 0.022 min
Response: 19265907
Conc: 1.50 ng/ml

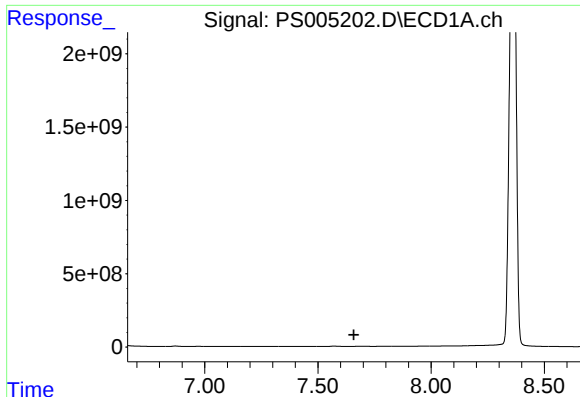

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

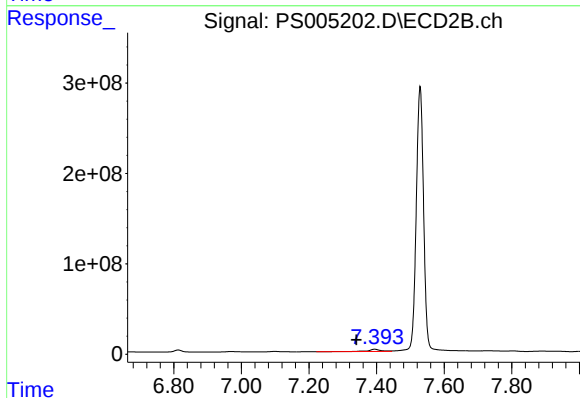


#12 2,4,5-T

R.T.: 7.394 min
Delta R.T.: 0.053 min
Response: 60099378
Conc: 11.78 ng/ml

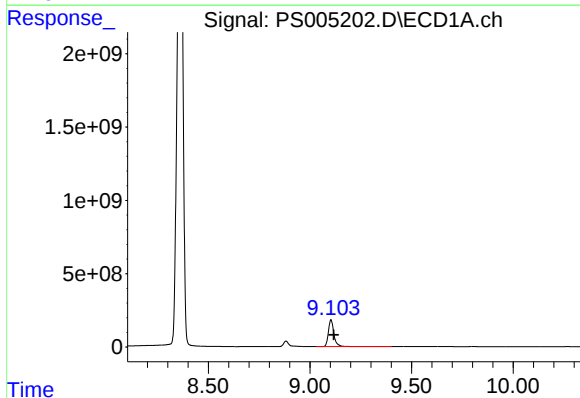


#15 Picloram

R.T.: 9.103 min
Delta R.T.: -0.013 min
Response: 3487156760
Conc: 303.47 ng/ml

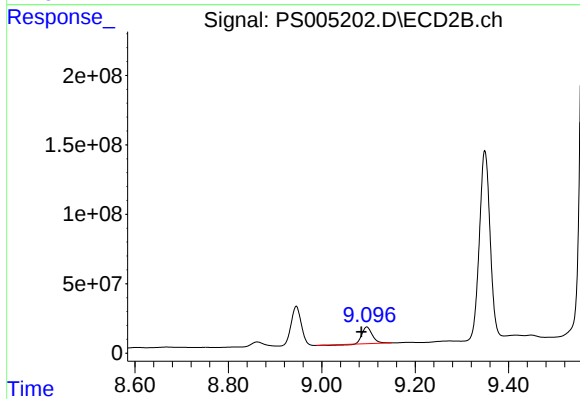

#15 Picloram


R.T.: 9.096 min
Delta R.T.: 0.011 min
Response: 179337282
Conc: 23.76 ng/ml

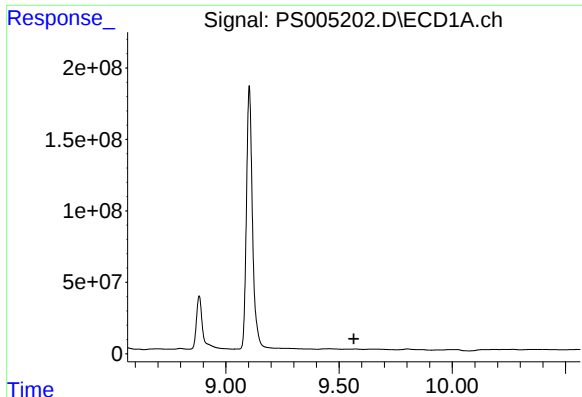

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

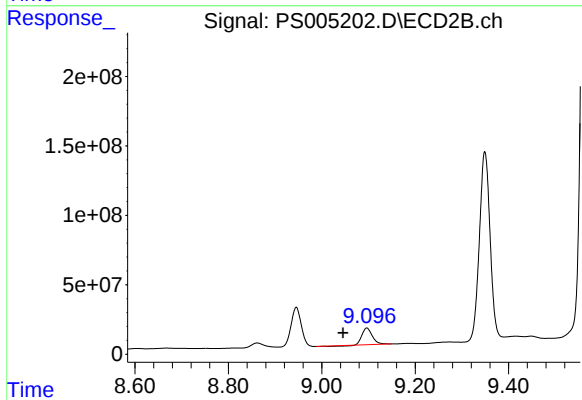

#16 DCPA

R.T.: 9.096 min
Delta R.T.: 0.051 min
Response: 179337282
Conc: 26.34 ng/ml