

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
 Data File : PS005209.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2019 21:14
 Operator : SM\AJ
 Sample : K3482-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:10:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.557	5.271	328.1E6	229.7E6	223.530	229.157
Target Compounds							
1) T	Dalapon	2.062	1.751	30936511	-274482	16.783	N.D. #
2) T	3,5-DICHL...	4.977	4.590	10658808	195.8E6	5.304	148.467 #
3) T	4-Nitroph...	5.350	0.000	16084788	0	22.208	N.D. #
5) T	DICAMBA	5.657	5.377	13899096	13420986	2.436	3.585 #
6) T	MCPD	5.910	0.000	8586365	0	1.961	N.D. #
7) T	MCPA	0.000	5.656	0	25612962	N.D.	6.323
8) T	DICHLORPROP	6.299	5.959	7817653	31184395	5.467	32.297 #
9) T	2,4-D	6.641	0.000	50954900	0	32.777	N.D. #
10) T	Pentachlo...	6.921	0.000	14799664	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.925	0	164.6E6	N.D.	30.916



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
Data File : PS005209.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2019 21:14
Operator : SM\AJ
Sample : K3482-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:10:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

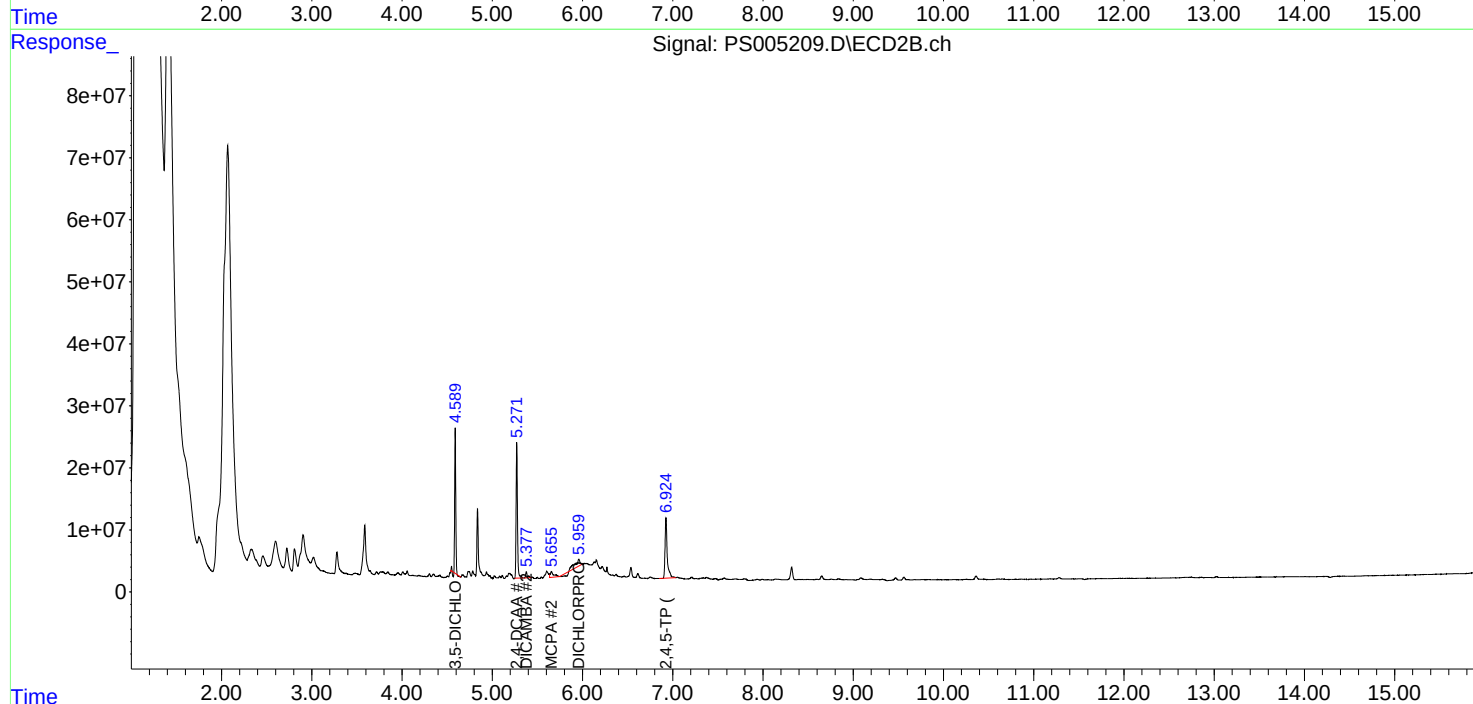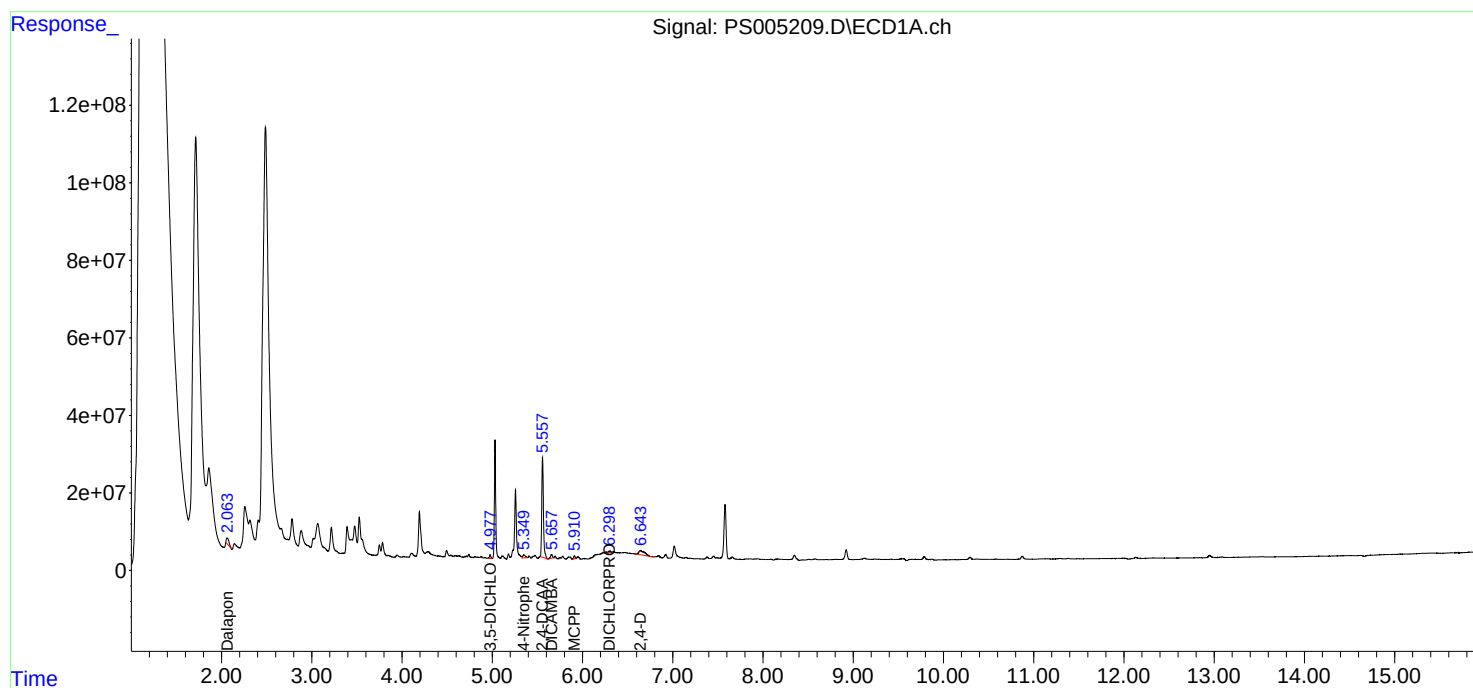


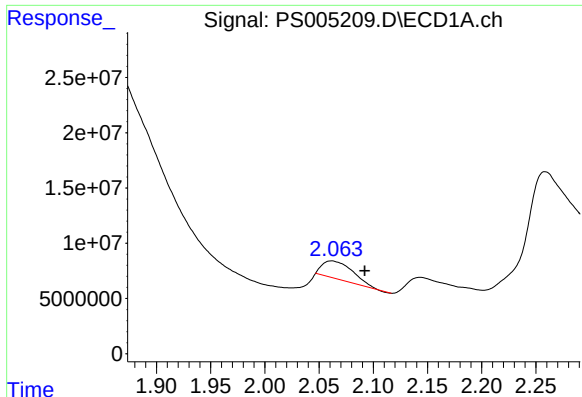

#1 Dalapon


R.T.: 2.062 min
Delta R.T.: -0.030 min
Response: 30936511
Conc: 16.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

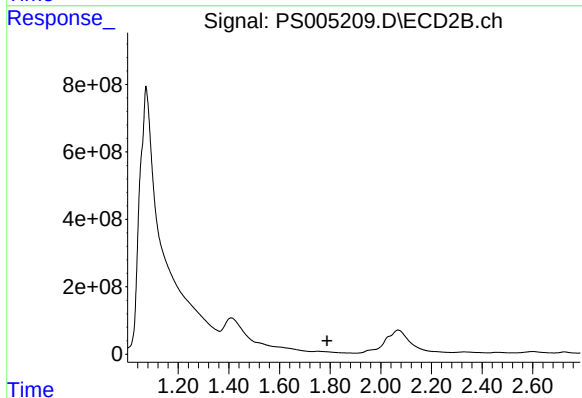


#1 Dalapon

R.T.: 1.751 min
Delta R.T.: -0.037 min
Response: -274482
Conc: N.D.

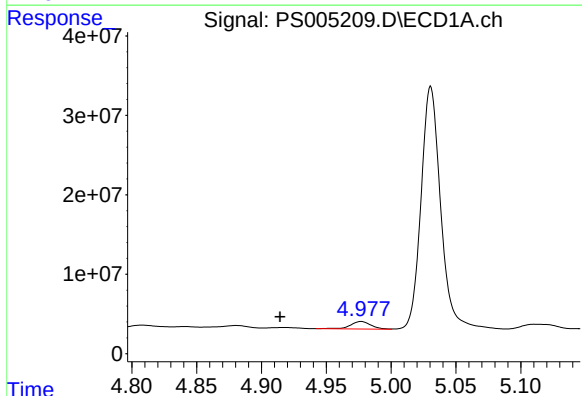


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.977 min
Delta R.T.: 0.063 min
Response: 10658808
Conc: 5.30 ng/ml

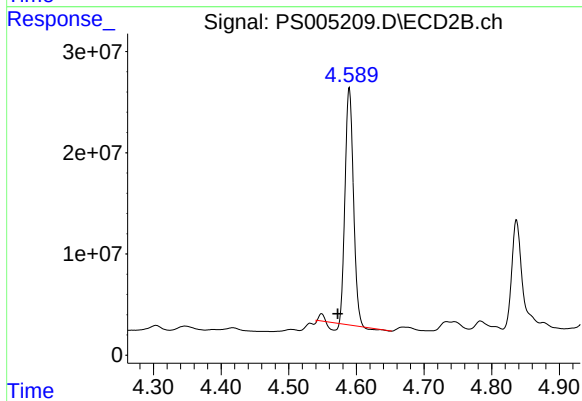

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.590 min
Delta R.T.: 0.017 min
Response: 195785167
Conc: 148.47 ng/ml

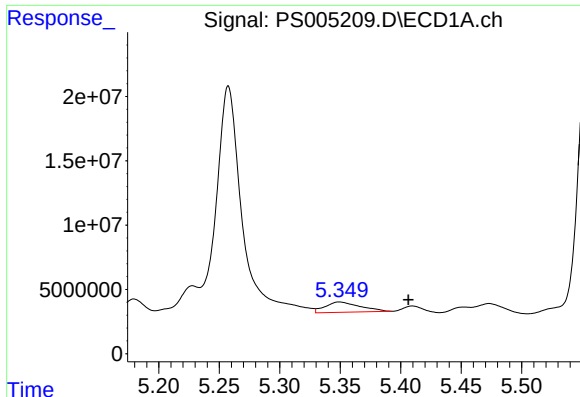

#3 4-Nitrophenol


R.T.: 5.350 min
Delta R.T.: -0.057 min
Response: 16084788
Conc: 22.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

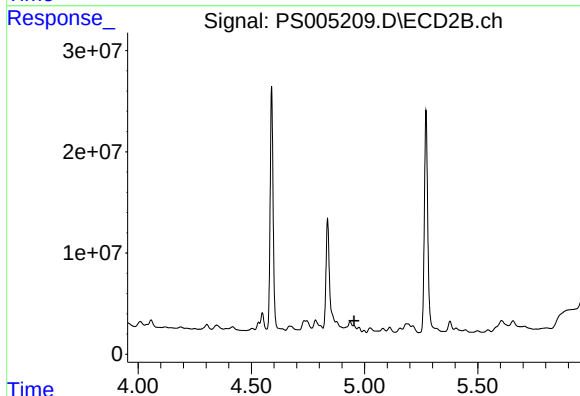


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

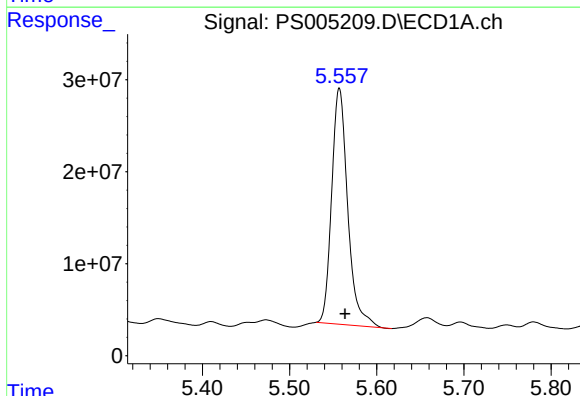


#4 2,4-DCAA

R.T.: 5.557 min
Delta R.T.: -0.007 min
Response: 328117911
Conc: 223.53 ng/ml

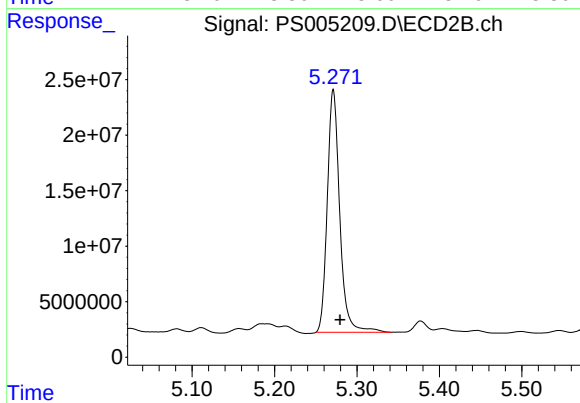

#4 2,4-DCAA


R.T.: 5.271 min
Delta R.T.: -0.008 min
Response: 229699418
Conc: 229.16 ng/ml

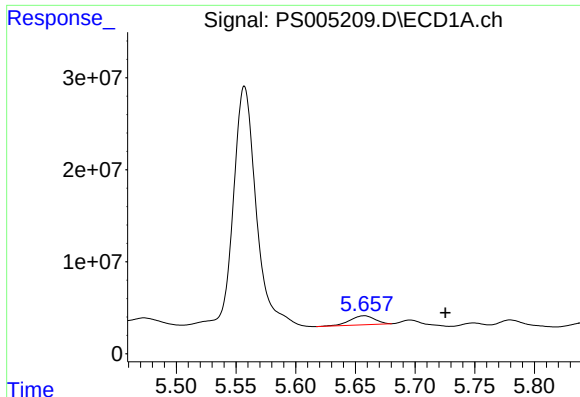

#5 DICAMBA


R.T.: 5.657 min
Delta R.T.: -0.068 min
Response: 13899096
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

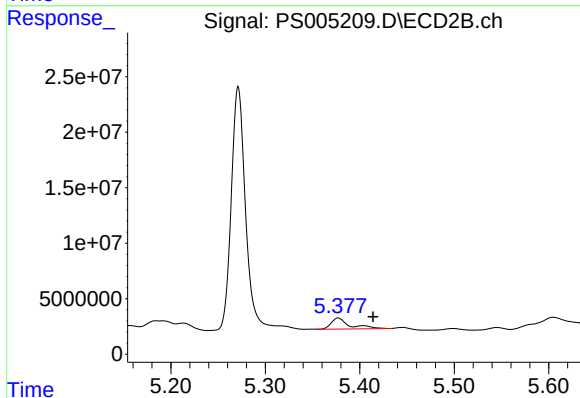


#5 DICAMBA

R.T.: 5.377 min
Delta R.T.: -0.037 min
Response: 13420986
Conc: 3.59 ng/ml

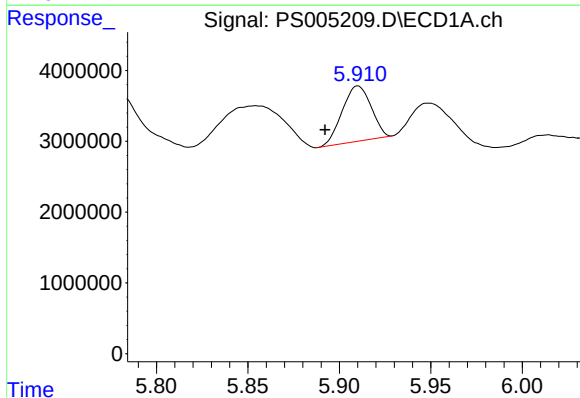


#6 MCP

R.T.: 5.910 min
Delta R.T.: 0.018 min
Response: 8586365
Conc: 1.96 ug/ml

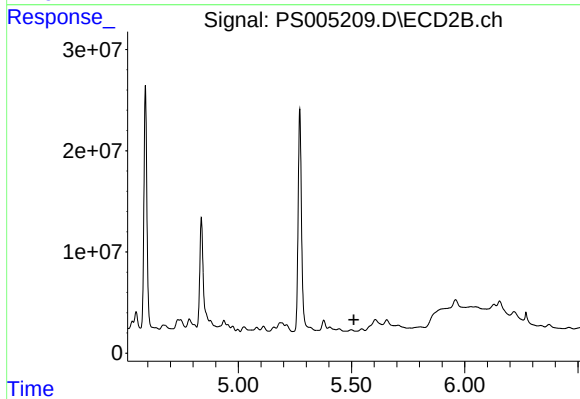

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

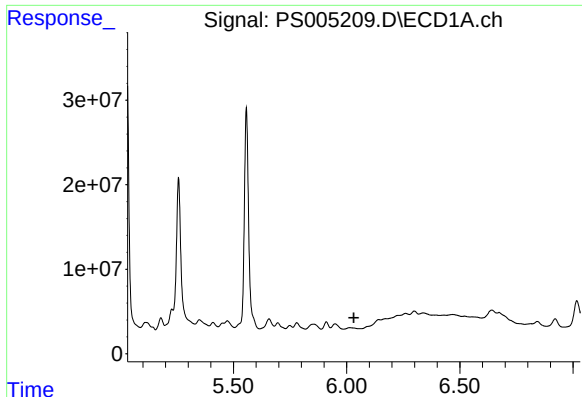

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

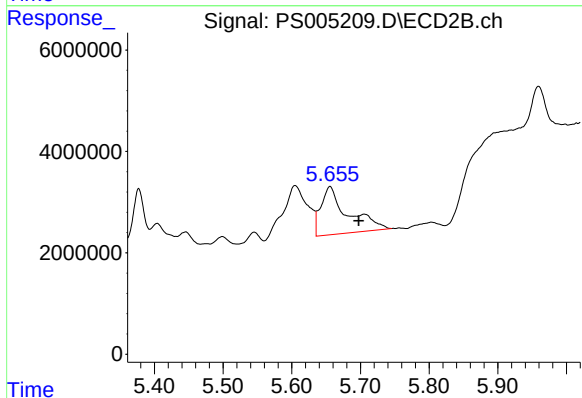


#7 MCPA

R.T.: 5.656 min
Delta R.T.: -0.042 min
Response: 25612962
Conc: 6.32 ug/ml

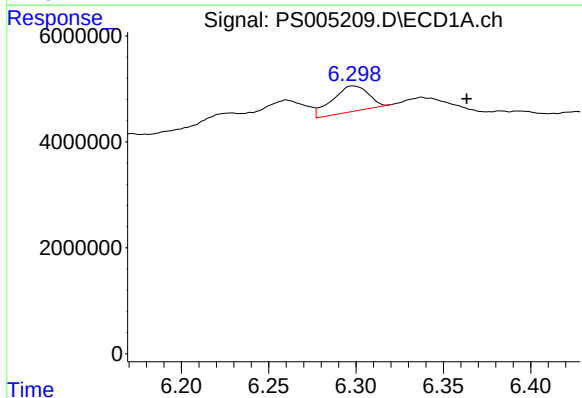


#8 DICHLORPROP

R.T.: 6.299 min
Delta R.T.: -0.065 min
Response: 7817653
Conc: 5.47 ng/ml

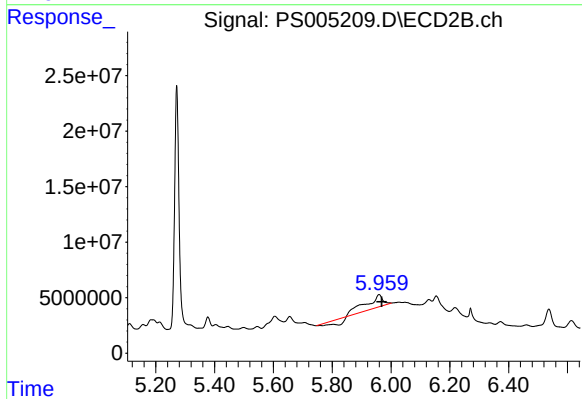

#8 DICHLORPROP


R.T.: 5.959 min
Delta R.T.: -0.010 min
Response: 31184395
Conc: 32.30 ng/ml

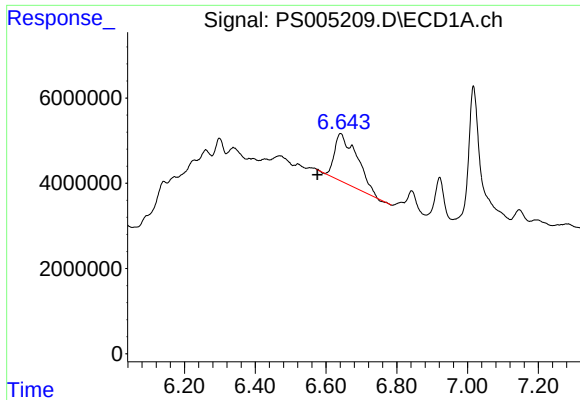

#9 2,4-D


R.T.: 6.641 min
Delta R.T.: 0.065 min
Response: 50954900
Conc: 32.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

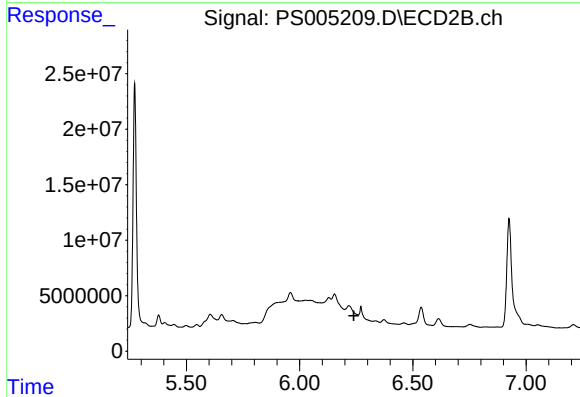


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.240 min
Response: 0
Conc: N.D.

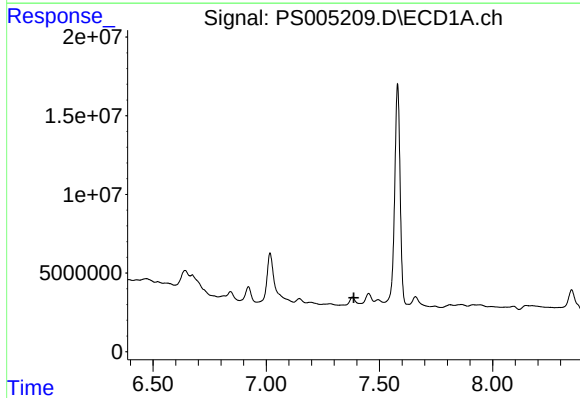

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

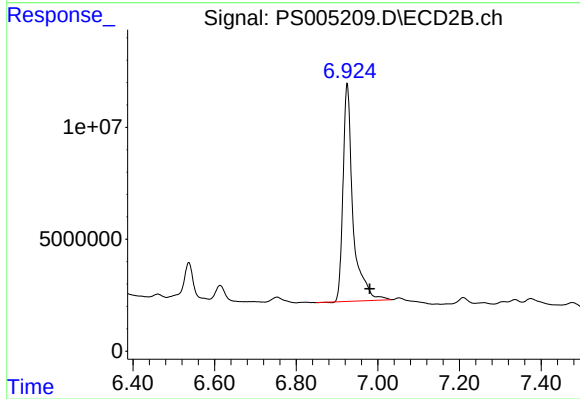

#11 2,4,5-TP (SILVEX)

R.T.: 6.925 min
Delta R.T.: -0.056 min
Response: 164636953
Conc: 30.92 ng/ml