

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
 Data File : PS005192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2019 11:10
 Operator : SM\AJ
 Sample : K2459-01 (Sig #1); K3459-01 (Sig #2)
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-04-002

Manual Integrations
 APPROVED

Ankita
 6/26/2019 1:10:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 12:07:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.569	5.284	384.6E6	255.2E6	262.040m	254.585

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062519\
Data File : PS005192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2019 11:10
Operator : SM\AJ
Sample : K2459-01 (Sig #1); K3459-01 (Sig #2)
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-BPM-04-002


Manual Integrations
APPROVED

Ankita
6/26/2019 1:10:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 12:07:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

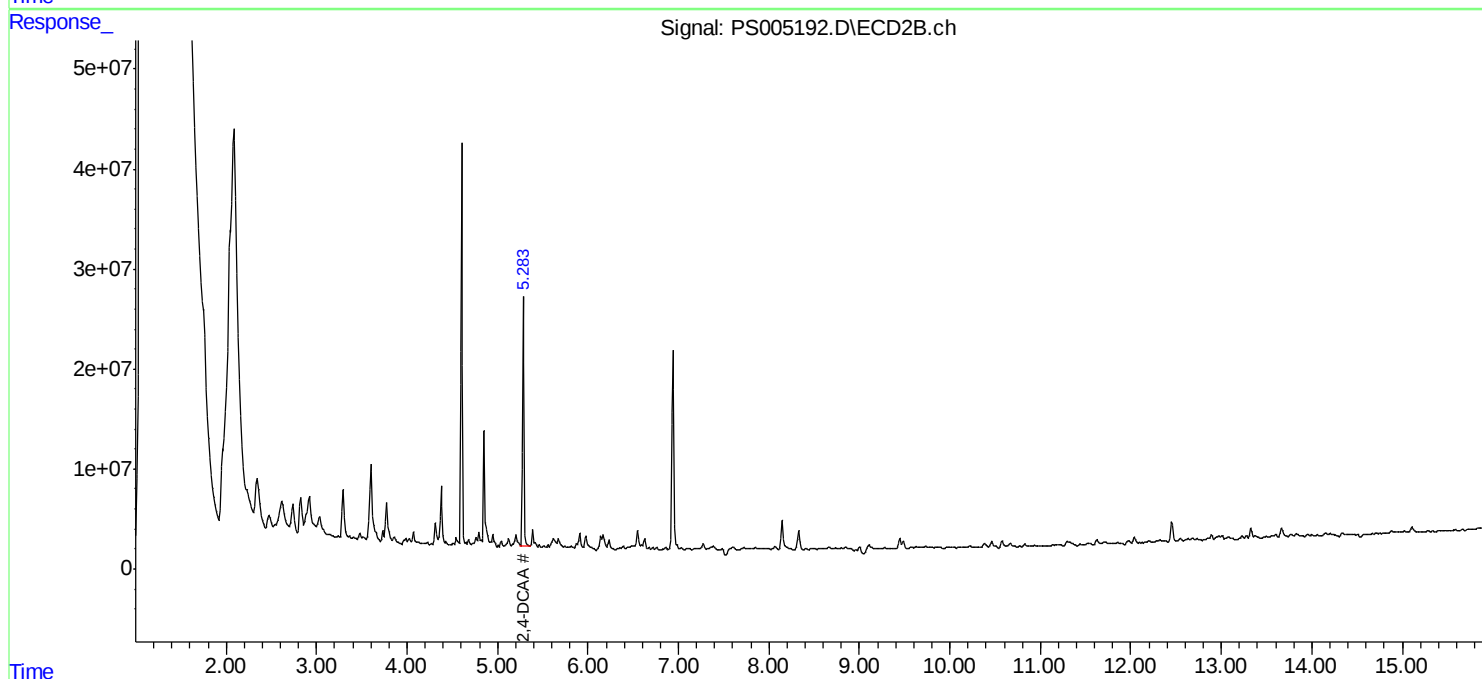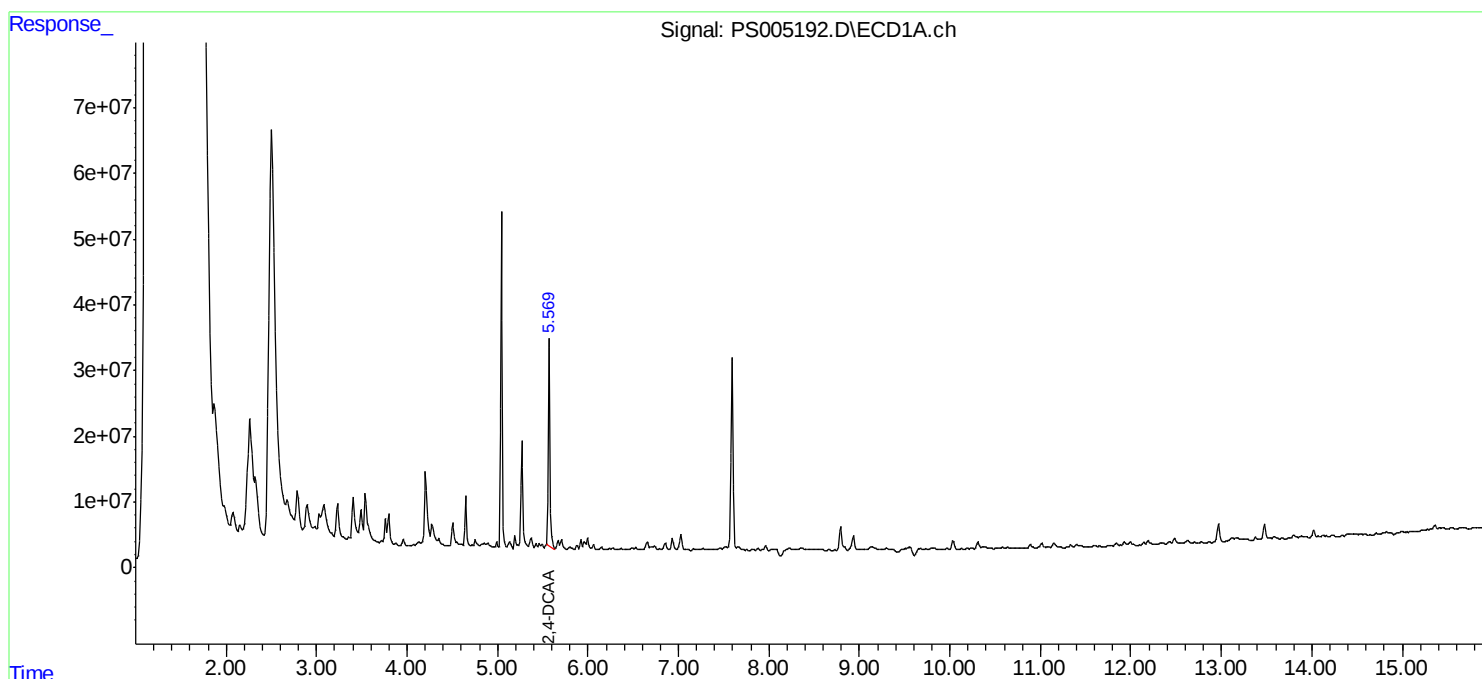

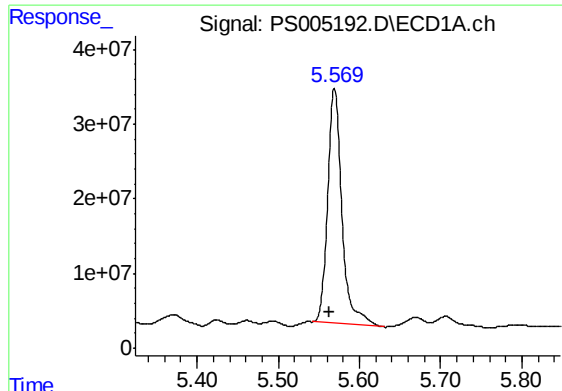


#4 2,4-DCAA

R.T.: 5.569 min
Delta R.T.: 0.005 min
Response: 384647208
Conc: 262.04 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-BPM-04-002

Manual Integrations
APPROVED

Ankita
6/26/2019 1:10:30 PM

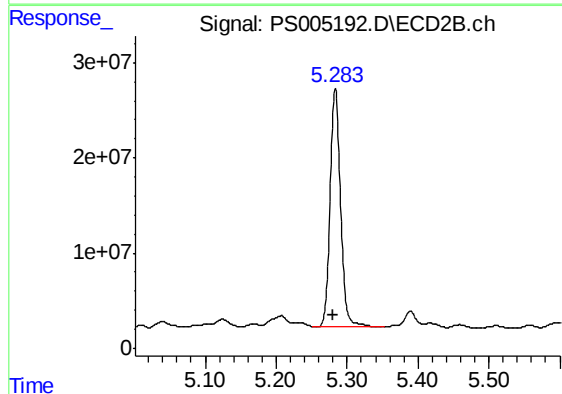

#4 2,4-DCAA

R.T.: 5.284 min
Delta R.T.: 0.004 min
Response: 255187945
Conc: 254.58 ng/ml