

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
 Data File : PS005247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 11:02
 Operator : SM\AJ
 Sample : K3511-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 13:28:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.281	651.4E6	448.2E6	443.795	447.147
Target Compounds							
1) T	Dalapon	2.075	0.000	35902743	0	19.477	N.D. #
2) T	3,5-DICHL...	0.000	4.599	0	197.5E6	N.D.	149.773
5) T	DICAMBA	0.000	5.387	0	6331779	N.D.	1.691
6) T	MCP	5.957	0.000	14391115	0	3.288	N.D. #
8) T	DICHLORPROP	0.000	5.970	0	16436931	N.D.	17.024
11) T	2,4,5-TP ...	0.000	6.934	0	121.1E6	N.D.	22.734
12) T	2,4,5-T	7.589	7.386	235.5E6	40928244	29.258	8.024 #
15) T	Picloram	9.131	9.093	184.6E6	130.7E6	16.060	17.317
16) T	DCPA	0.000	9.093	0	130.7E6	N.D.	19.197



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
Data File : PS005247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 11:02
Operator : SM\AJ
Sample : K3511-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 13:28:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

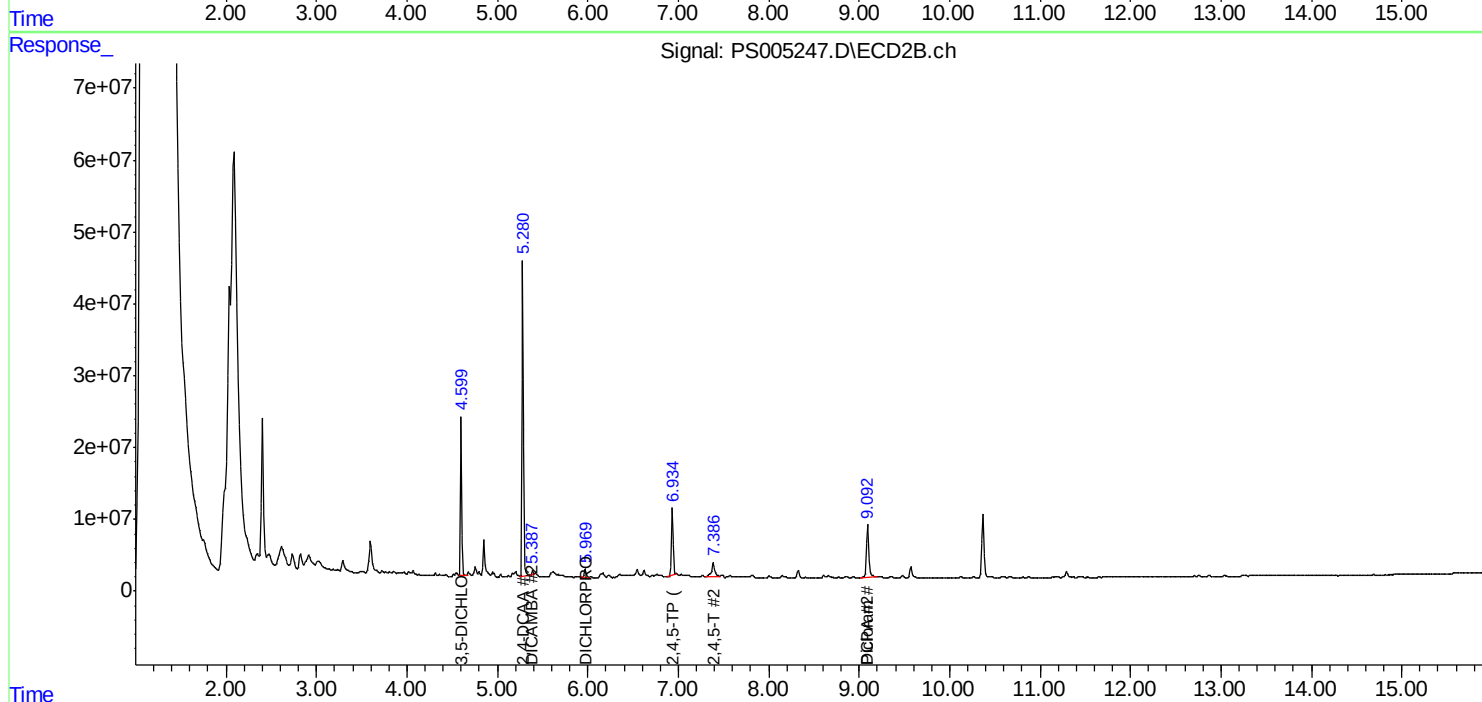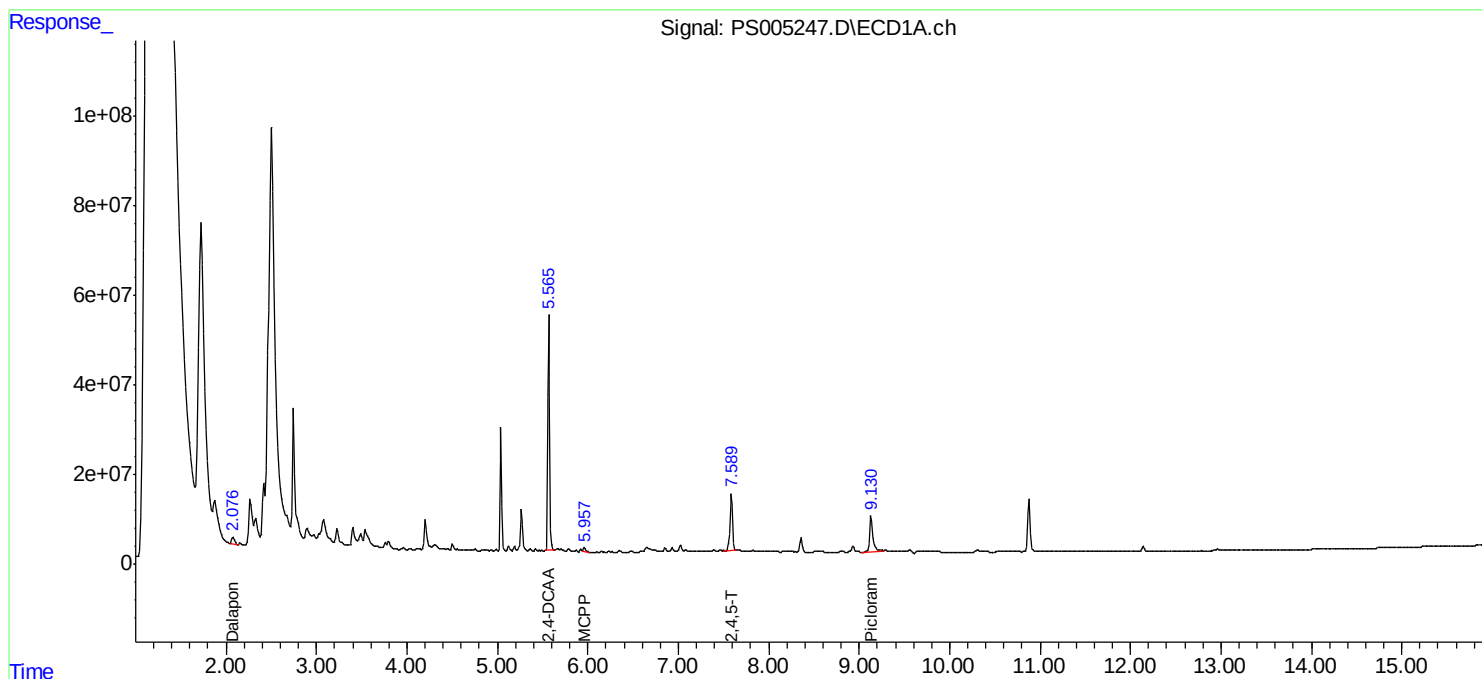


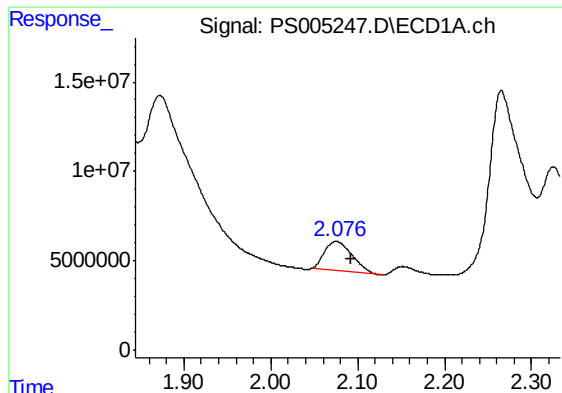

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.017 min
Response: 35902743
Conc: 19.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-1

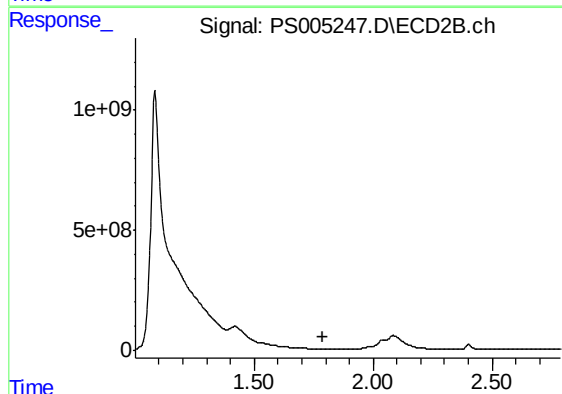


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

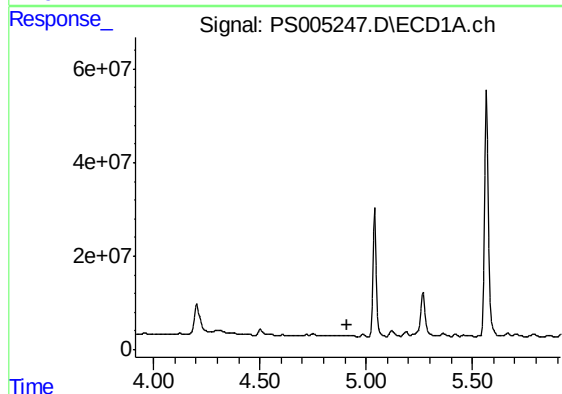


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

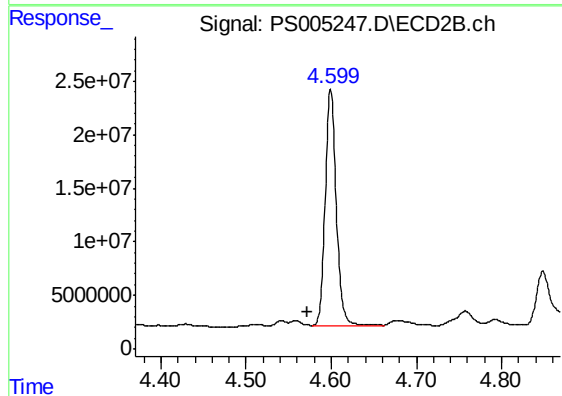

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.599 min
Delta R.T.: 0.027 min
Response: 197506443
Conc: 149.77 ng/ml

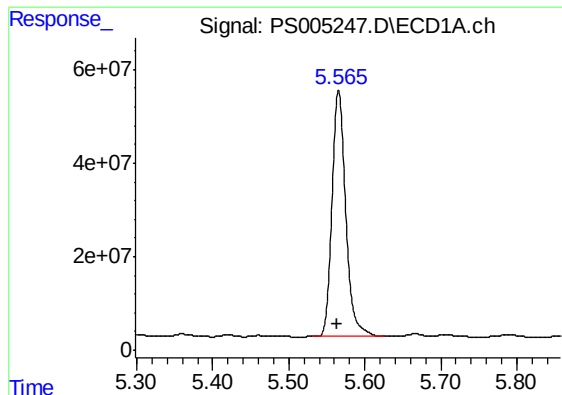

#4 2,4-DCAA


R.T.: 5.566 min
Delta R.T.: 0.002 min
Response: 651443058
Conc: 443.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-1

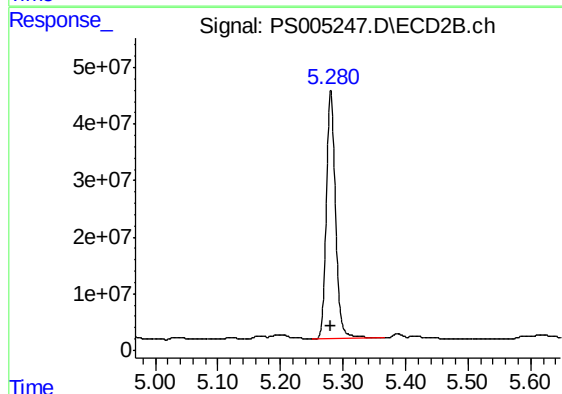


#4 2,4-DCAA

R.T.: 5.281 min
Delta R.T.: 0.001 min
Response: 448206129
Conc: 447.15 ng/ml

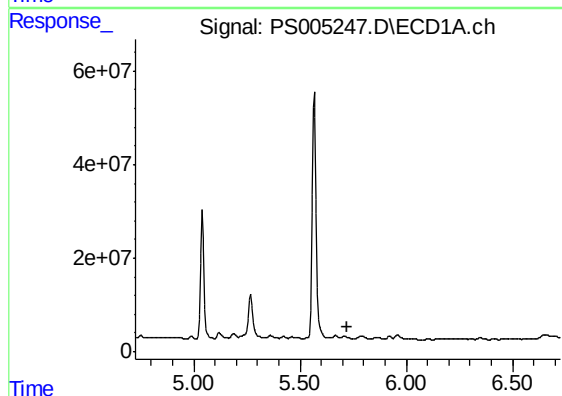


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

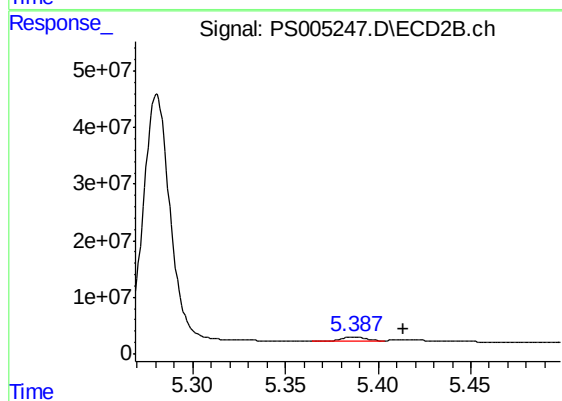

#5 DICAMBA


R.T.: 5.387 min
Delta R.T.: -0.027 min
Response: 6331779
Conc: 1.69 ng/ml

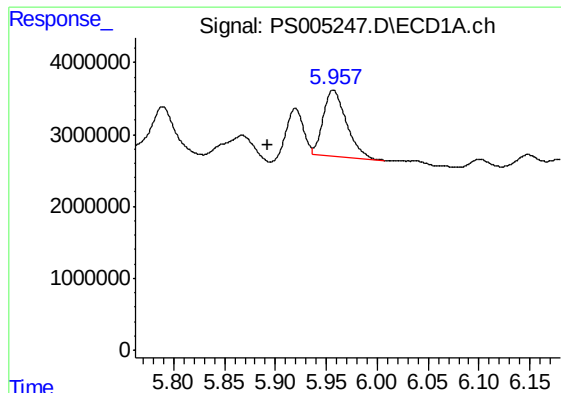

#6 MCPP


R.T.: 5.957 min
Delta R.T.: 0.065 min
Response: 14391115
Conc: 3.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-1

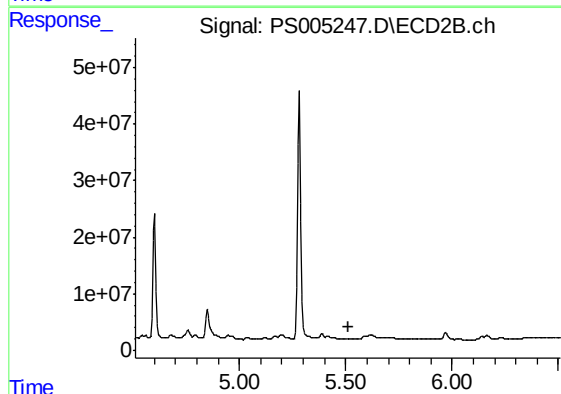


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

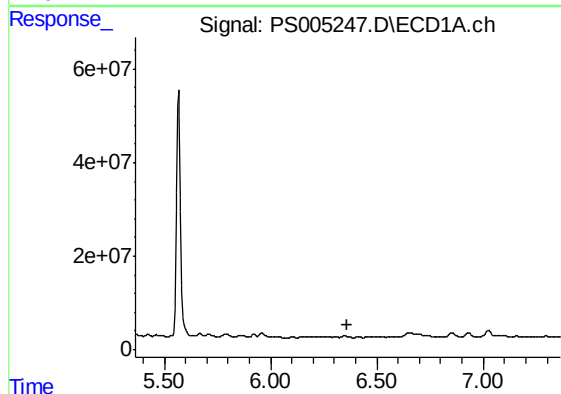


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

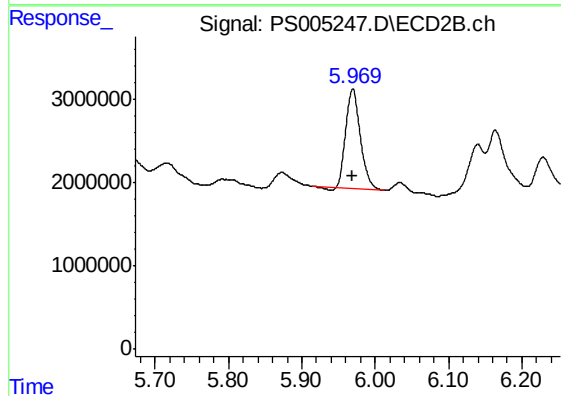

#8 DICHLORPROP


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 16436931
Conc: 17.02 ng/ml

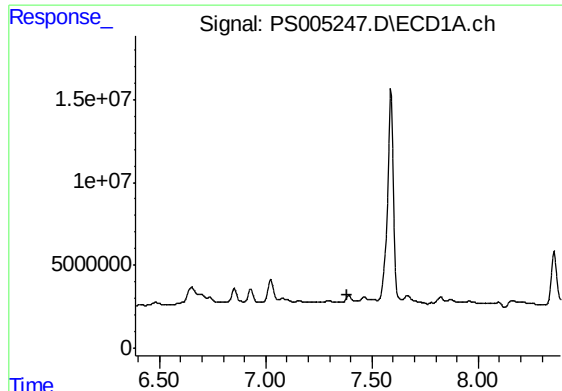

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-1

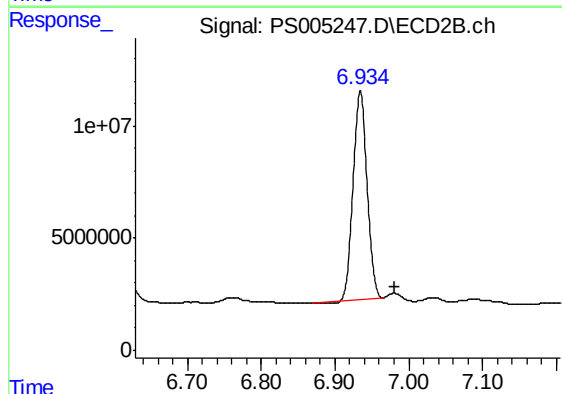


#11 2,4,5-TP (SILVEX)

R.T.: 6.934 min
Delta R.T.: -0.046 min
Response: 121062447
Conc: 22.73 ng/ml

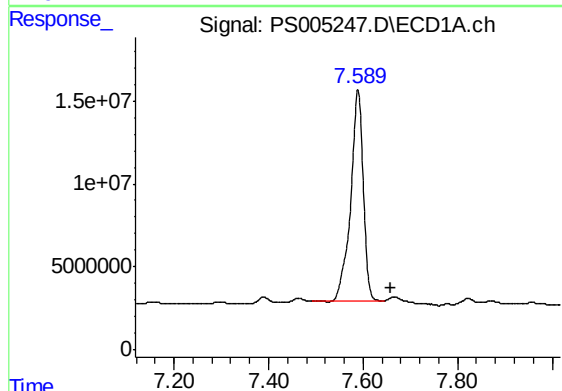


#12 2,4,5-T

R.T.: 7.589 min
Delta R.T.: -0.070 min
Response: 235461783
Conc: 29.26 ng/ml

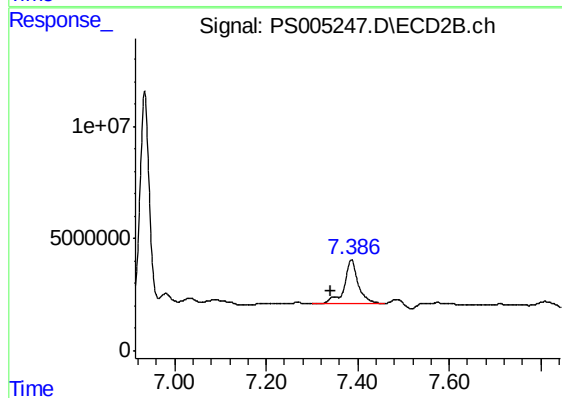

#12 2,4,5-T


R.T.: 7.386 min
Delta R.T.: 0.046 min
Response: 40928244
Conc: 8.02 ng/ml

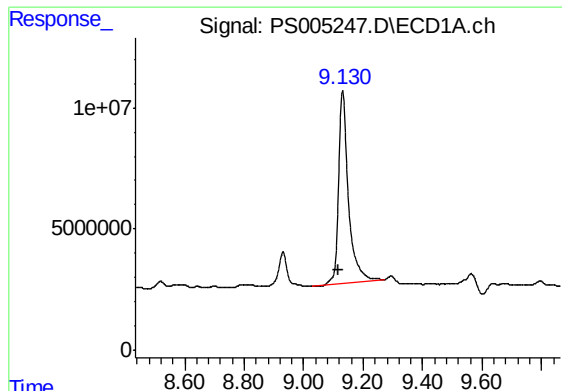

#15 Picloram


R.T.: 9.131 min
Delta R.T.: 0.014 min
Response: 184550783
Conc: 16.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-1

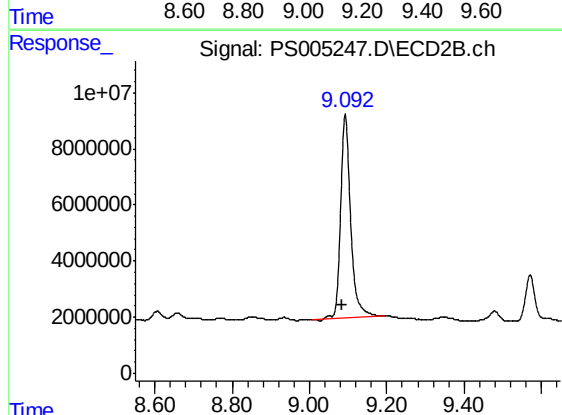


#15 Picloram

R.T.: 9.093 min
Delta R.T.: 0.008 min
Response: 130685076
Conc: 17.32 ng/ml

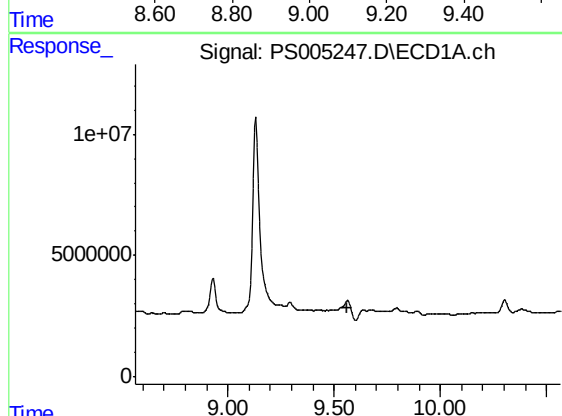

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

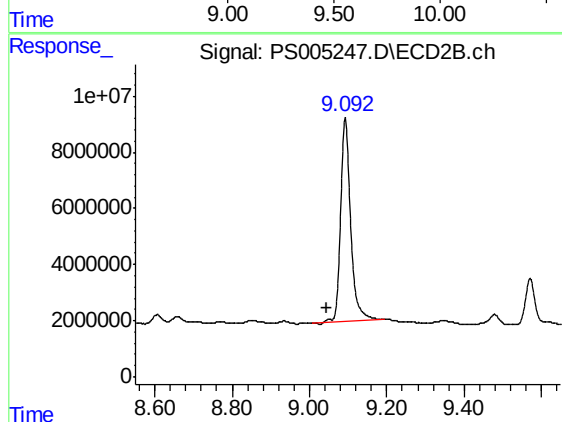

#16 DCPA

R.T.: 9.093 min
Delta R.T.: 0.047 min
Response: 130685076
Conc: 19.20 ng/ml