

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
 Data File : PS005248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 11:24
 Operator : SM\AJ
 Sample : K3510-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-062419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 13:10:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.281	854.9E6	581.4E6	582.382	580.070
Target Compounds							
1) T	Dalapon	2.075	0.000	51421381	0	27.896	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	162.8E6	N.D.	123.470
6) T	MCP	5.958	0.000	15347788	0	3.506	N.D. #
8) T	DICHLORPROP	0.000	5.970	0	9739496	N.D.	10.087
9) T	2,4-D	0.000	6.229	0	10721449	N.D.	9.613
11) T	2,4,5-TP ...	0.000	6.935	0	104.6E6	N.D.	19.644



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
Data File : PS005248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 11:24
Operator : SM\AJ
Sample : K3510-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 13:10:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

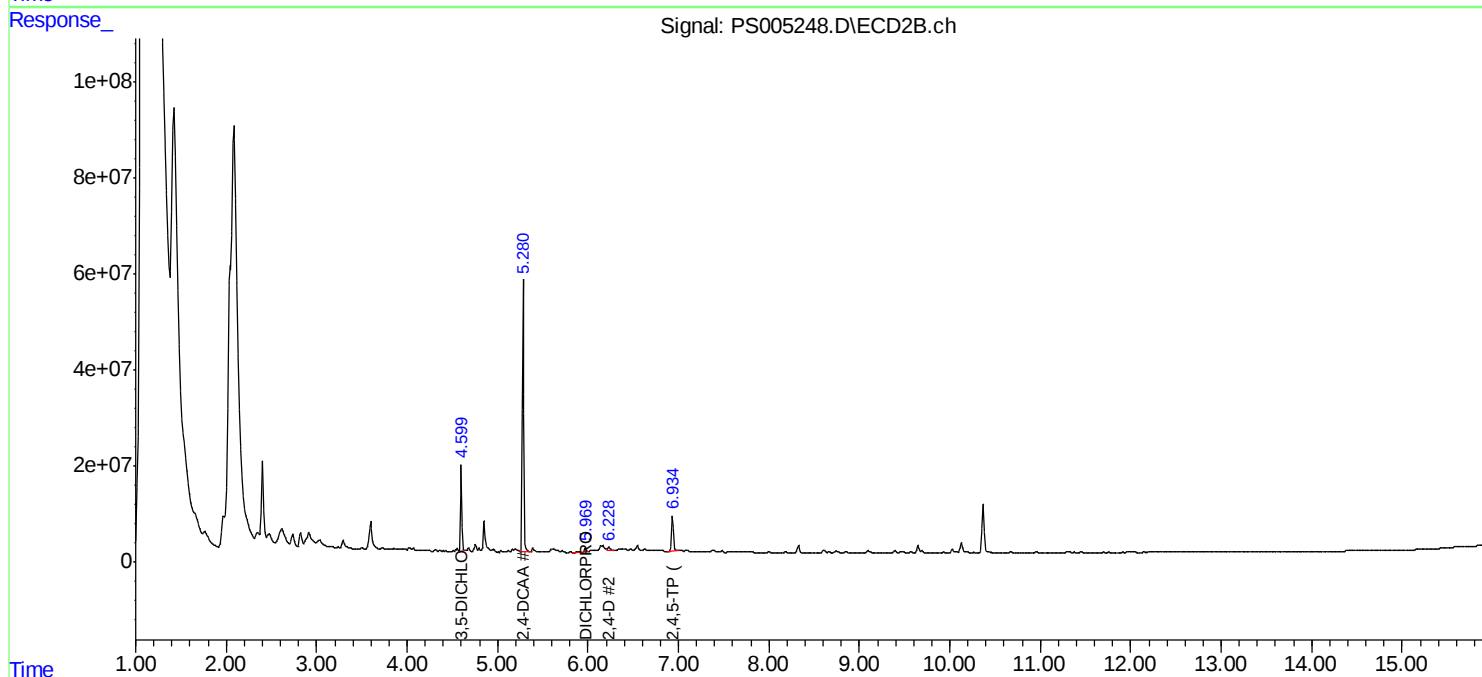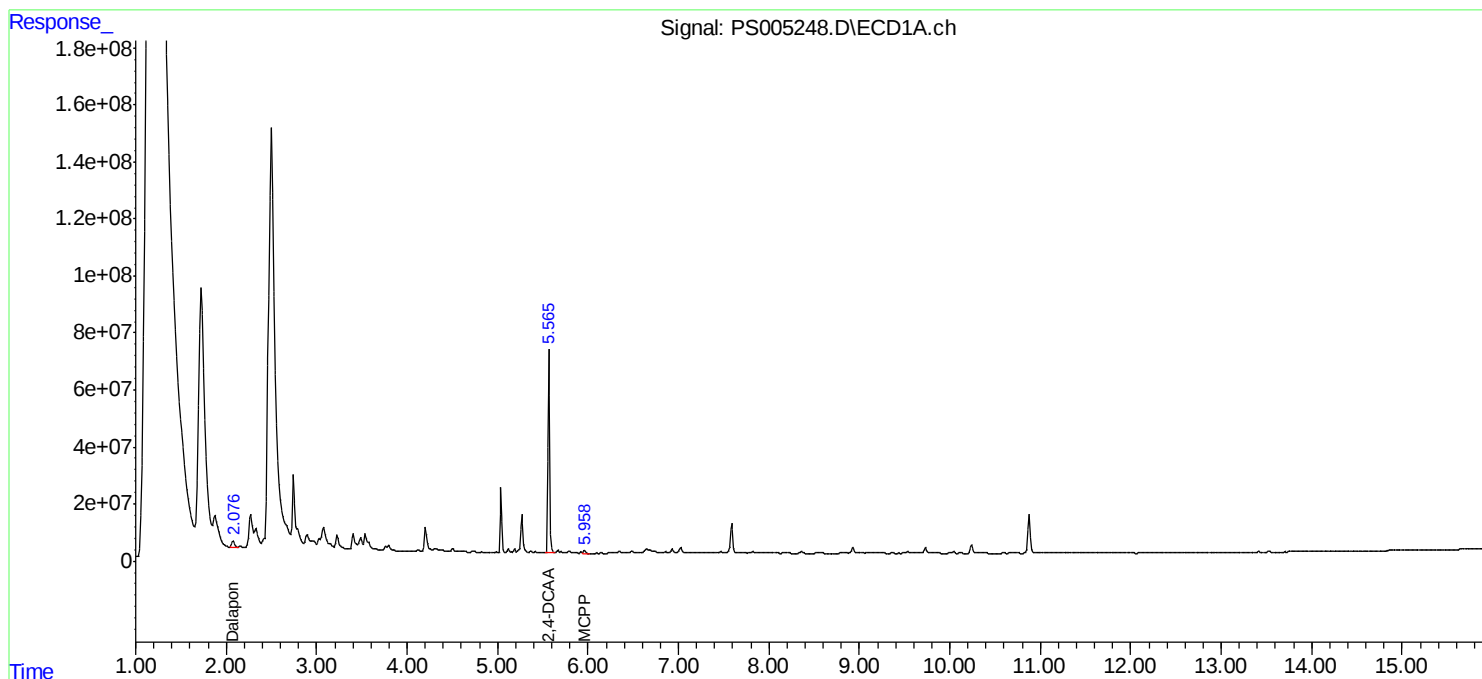


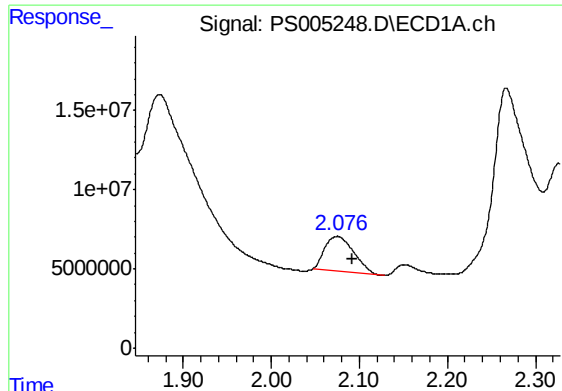

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.017 min
Response: 51421381
Conc: 27.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-062419

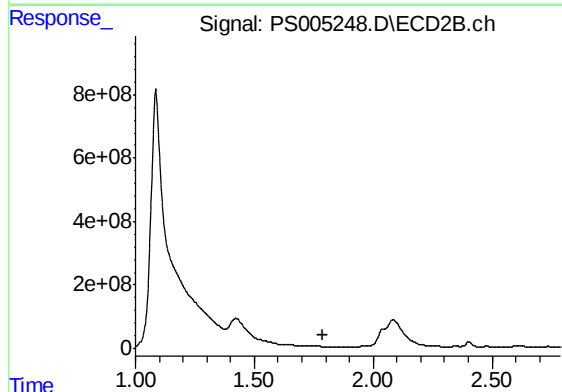


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

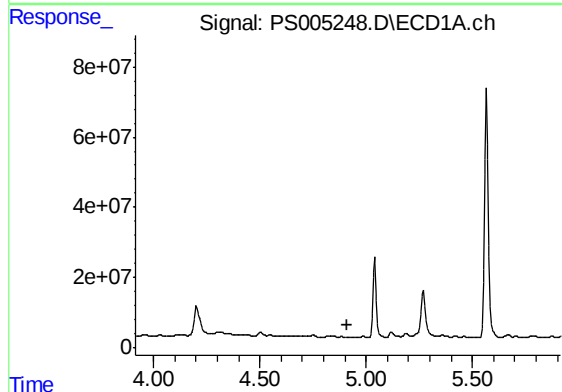


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

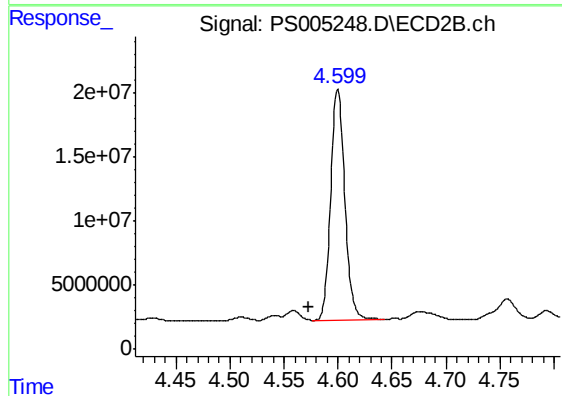

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.027 min
Response: 162821037
Conc: 123.47 ng/ml

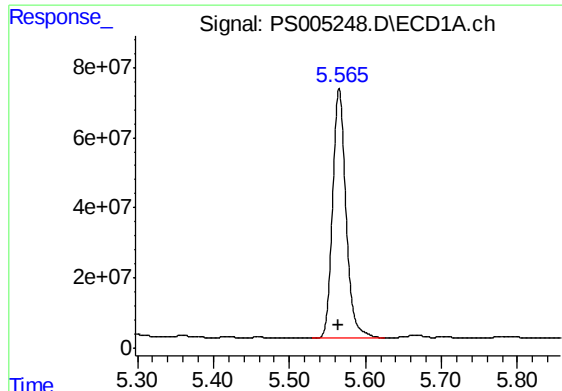

#4 2,4-DCAA


R.T.: 5.566 min
Delta R.T.: 0.002 min
Response: 854874250
Conc: 582.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-062419

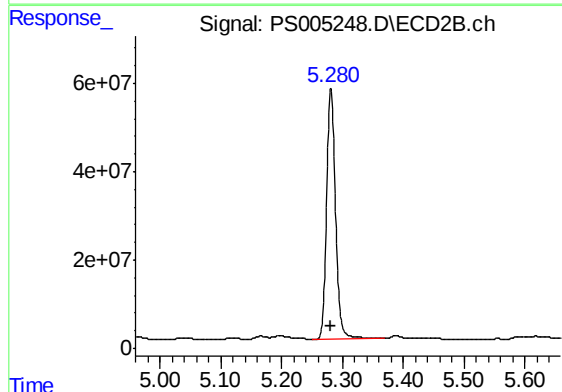


#4 2,4-DCAA

R.T.: 5.281 min
Delta R.T.: 0.001 min
Response: 581443408
Conc: 580.07 ng/ml

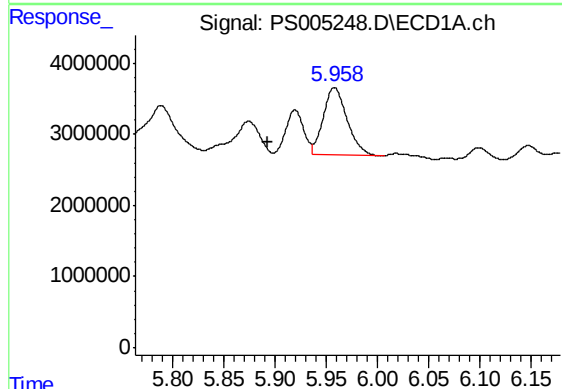


#6 MCP

R.T.: 5.958 min
Delta R.T.: 0.066 min
Response: 15347788
Conc: 3.51 ug/ml

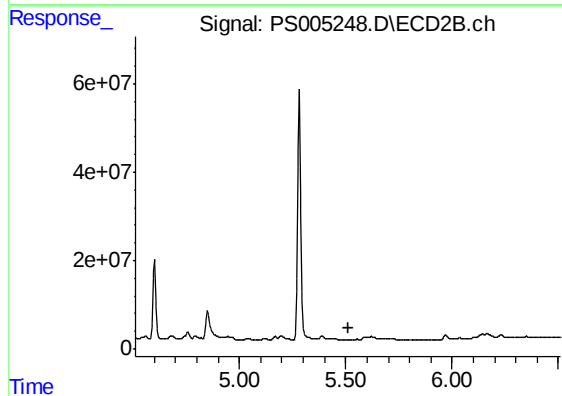

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

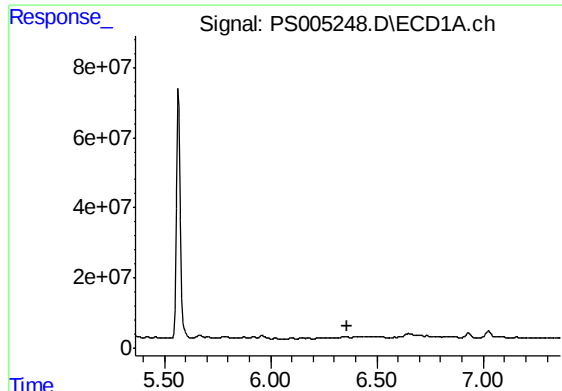

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-062419

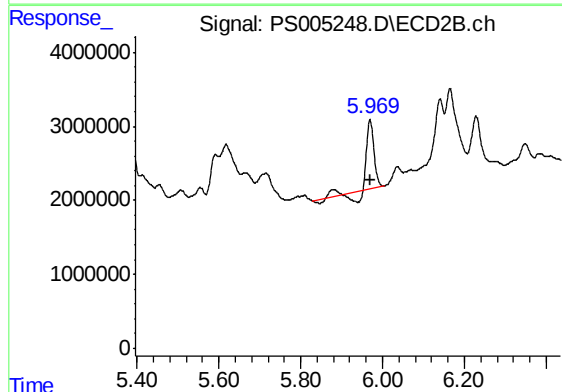


#8 DICHLORPROP

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 9739496
Conc: 10.09 ng/ml

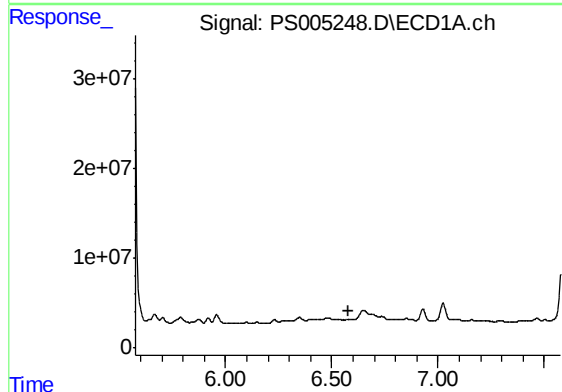


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

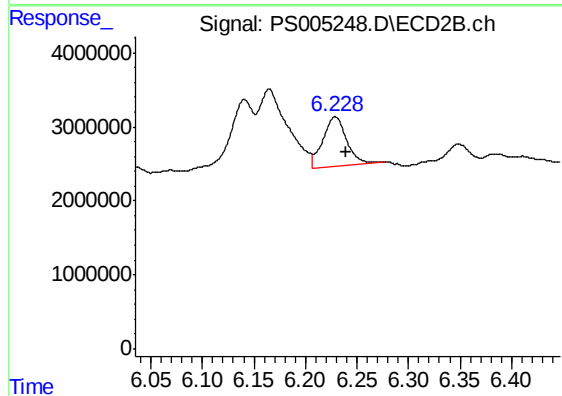

#9 2,4-D


R.T.: 6.229 min
Delta R.T.: -0.011 min
Response: 10721449
Conc: 9.61 ng/ml

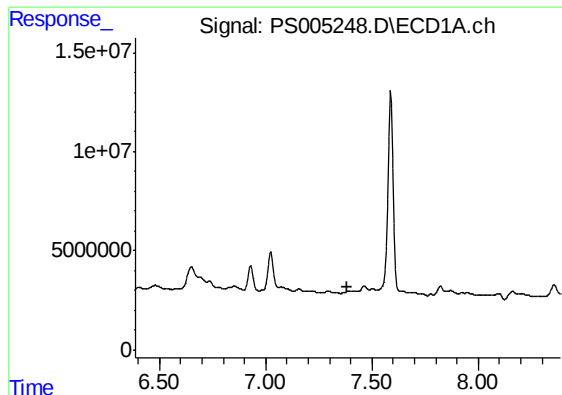

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-062419

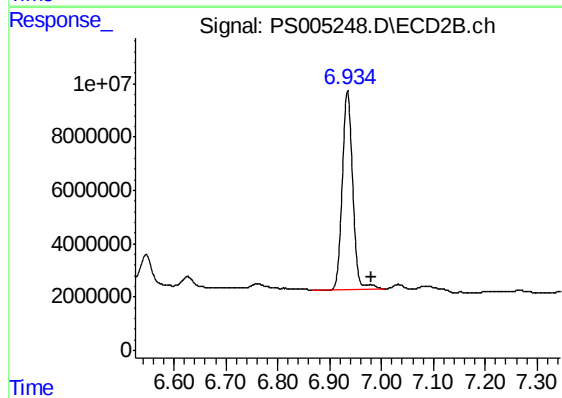

#11 2,4,5-TP (SILVEX)

R.T.: 6.935 min
Delta R.T.: -0.046 min
Response: 104608394
Conc: 19.64 ng/ml