

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
 Data File : PS005251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2019 12:30
 Operator : SM\AJ
 Sample : K3512-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 13:10:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.587	5.302	761.2E6	494.0E6	518.547	492.856
Target Compounds							
1) T	Dalapon	2.097	0.000	50372664	0	27.327	N.D. #
2) T	3,5-DICHL...	4.953	4.621	12516614	241.2E6	6.228	182.870 #
5) T	DICAMBA	0.000	5.409	0	8919795	N.D.	2.383
6) T	MCP	5.941	0.000	8944993	0	2.043	N.D. #
8) T	DICHLORPROP	0.000	5.991	0	13632984	N.D.	14.120
9) T	2,4-D	0.000	6.250	0	11773879	N.D.	10.557
10) T	Pentachlo...	0.000	6.567	0	18445949	N.D.	1.435
11) T	2,4,5-TP ...	0.000	6.956	0	153.0E6	N.D.	28.736
12) T	2,4,5-T	7.611	0.000	254.7E6	0	31.654	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062719\
Data File : PS005251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2019 12:30
Operator : SM\AJ
Sample : K3512-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 13:10:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

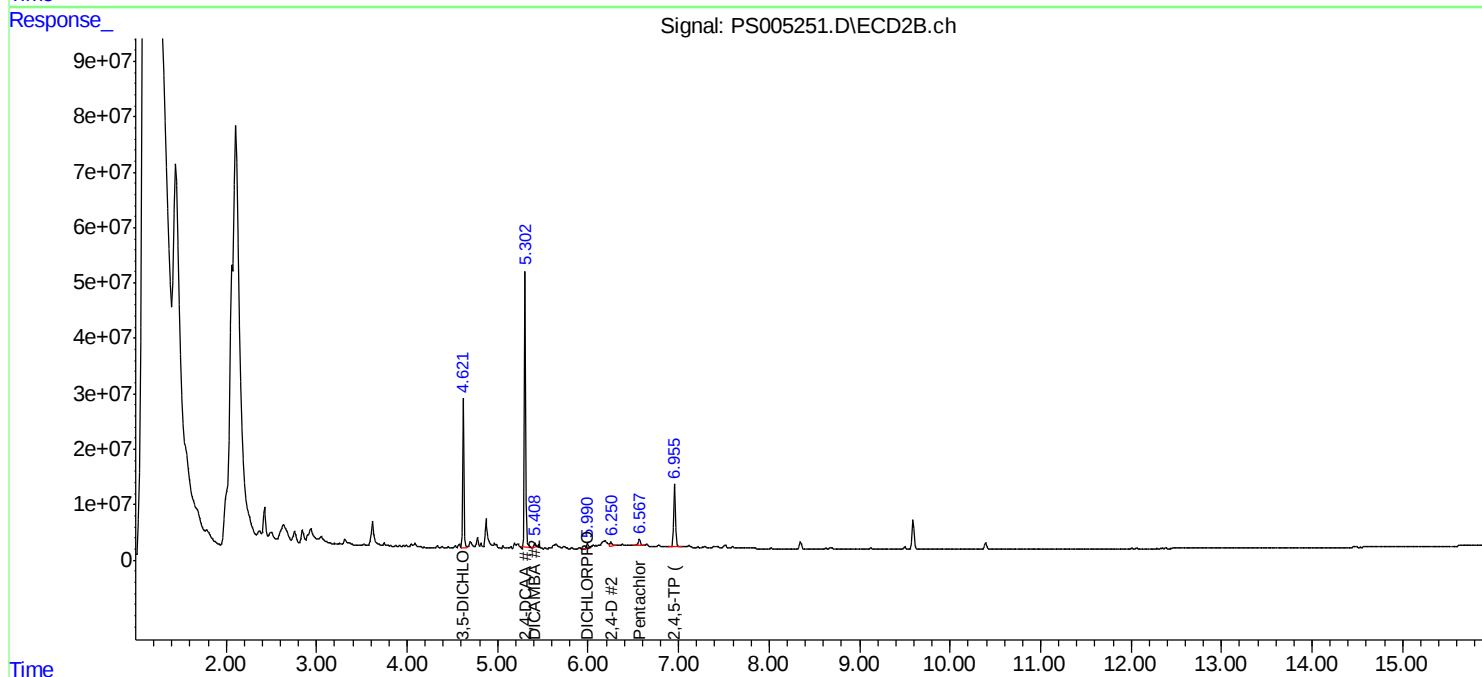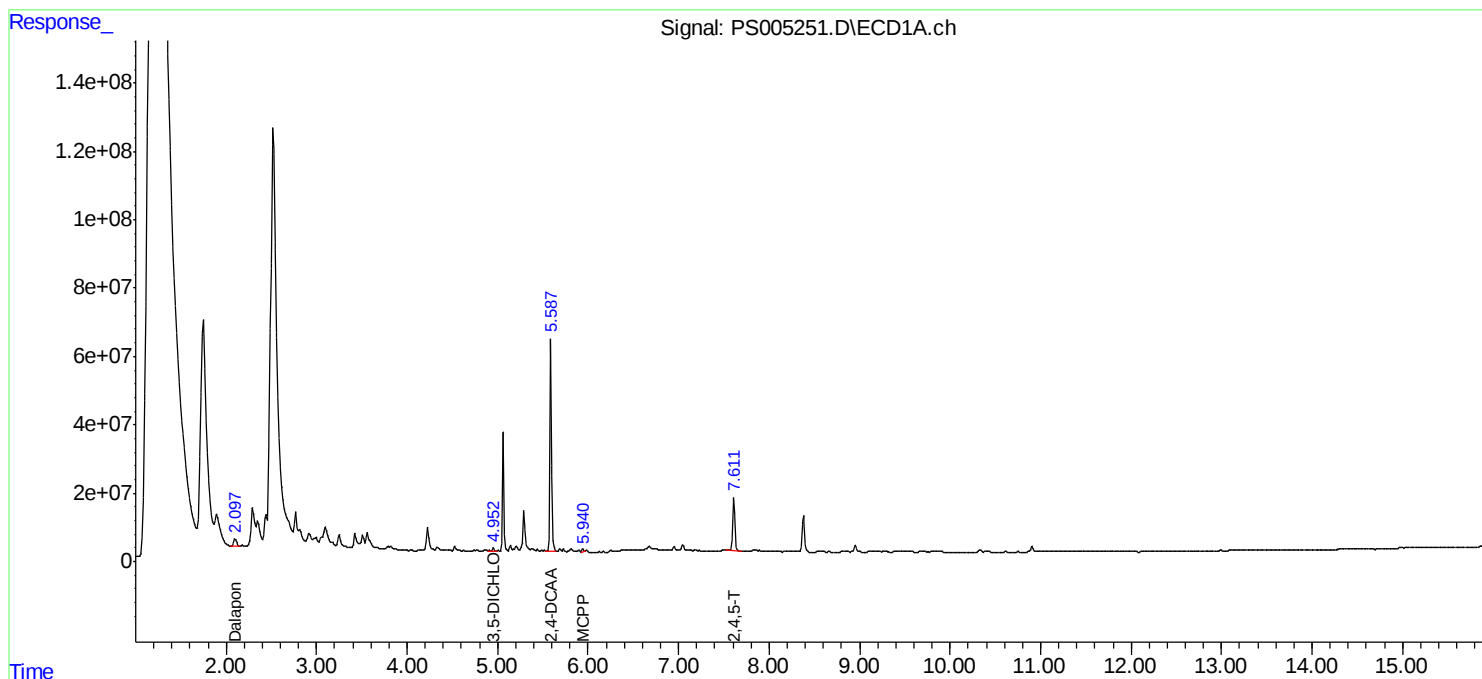


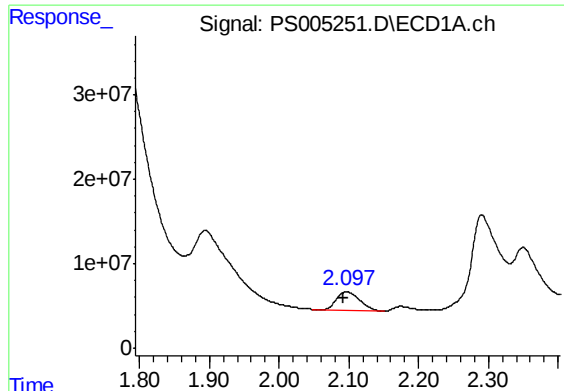

#1 Dalapon


R.T.: 2.097 min
Delta R.T.: 0.005 min
Response: 50372664
Conc: 27.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

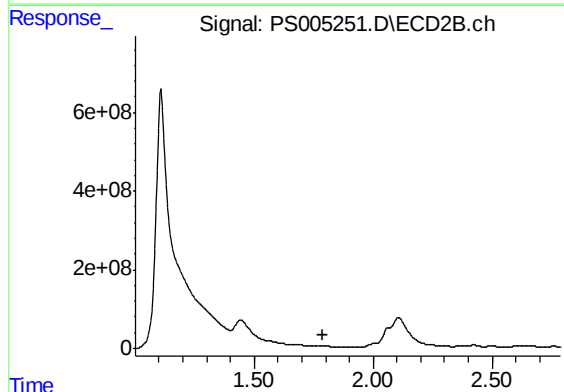


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

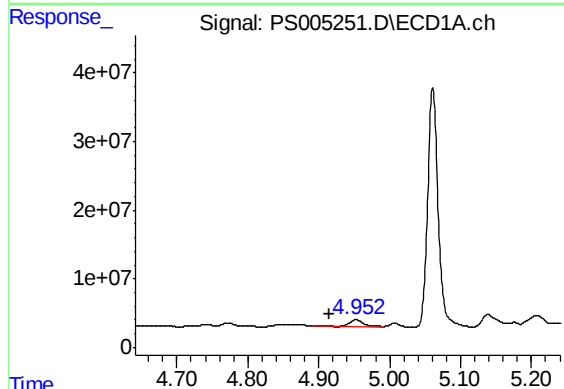


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.953 min
Delta R.T.: 0.038 min
Response: 12516614
Conc: 6.23 ng/ml

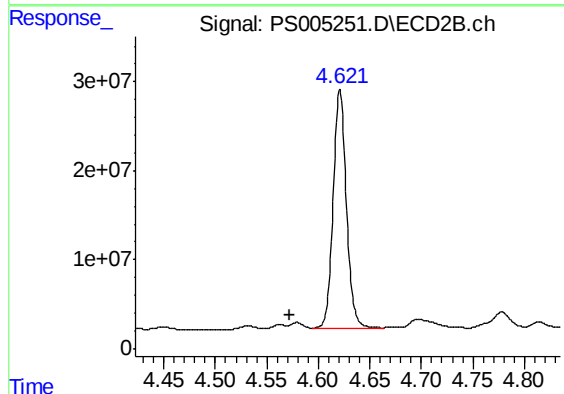

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.621 min
Delta R.T.: 0.048 min
Response: 241151911
Conc: 182.87 ng/ml

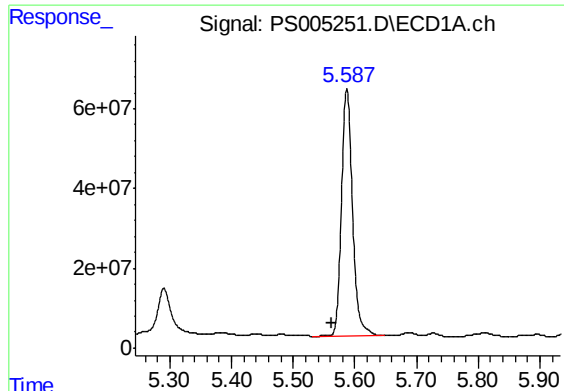

#4 2,4-DCAA


R.T.: 5.587 min
Delta R.T.: 0.023 min
Response: 761171827
Conc: 518.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

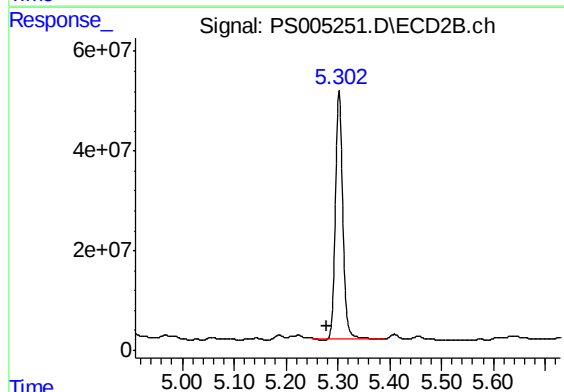


#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: 0.023 min
Response: 494023456
Conc: 492.86 ng/ml

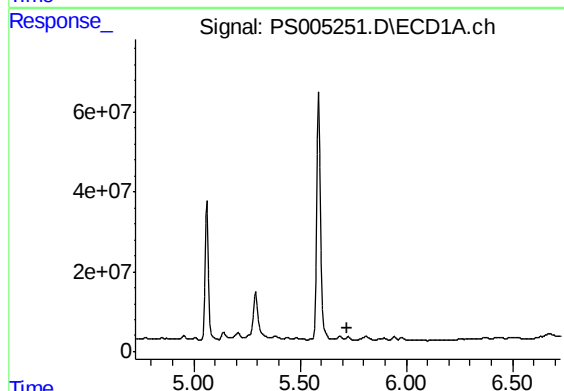


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

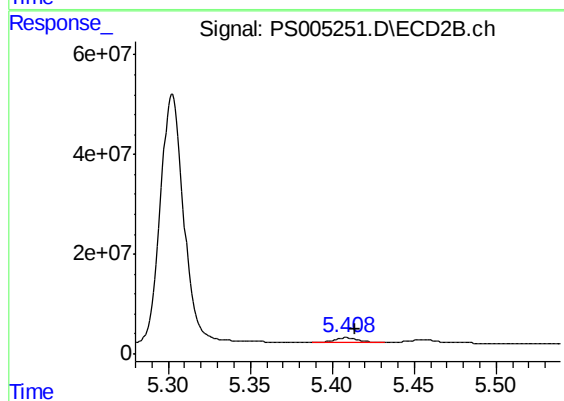

#5 DICAMBA


R.T.: 5.409 min
Delta R.T.: -0.005 min
Response: 8919795
Conc: 2.38 ng/ml

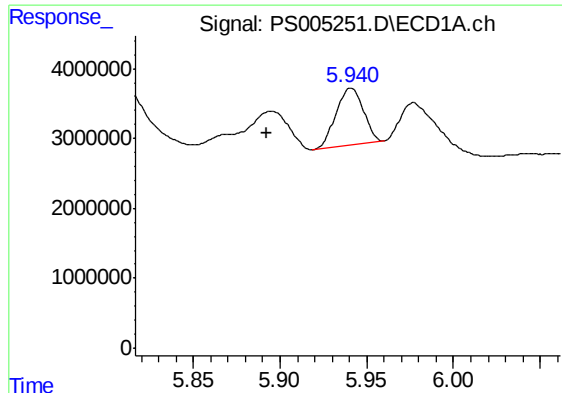

#6 MCP


R.T.: 5.941 min
Delta R.T.: 0.049 min
Response: 8944993
Conc: 2.04 ug/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

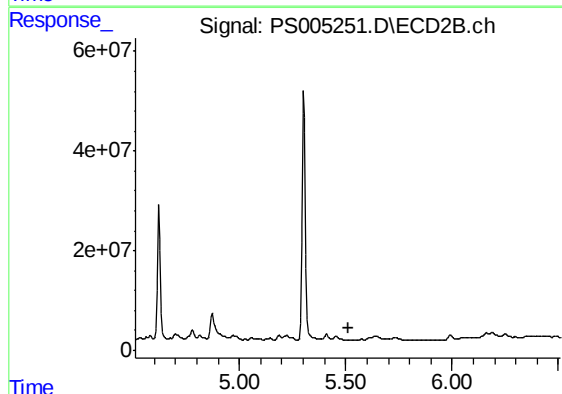


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

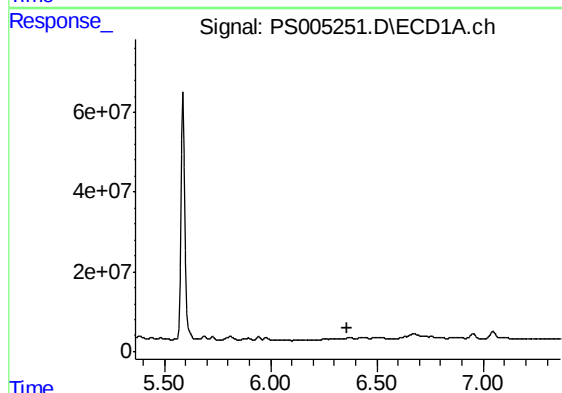


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

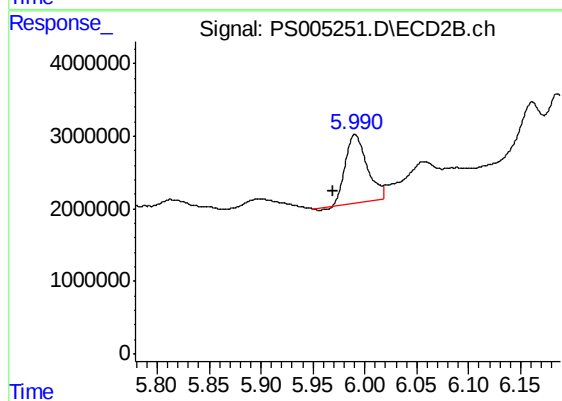

#8 DICHLORPROP


R.T.: 5.991 min
Delta R.T.: 0.022 min
Response: 13632984
Conc: 14.12 ng/ml

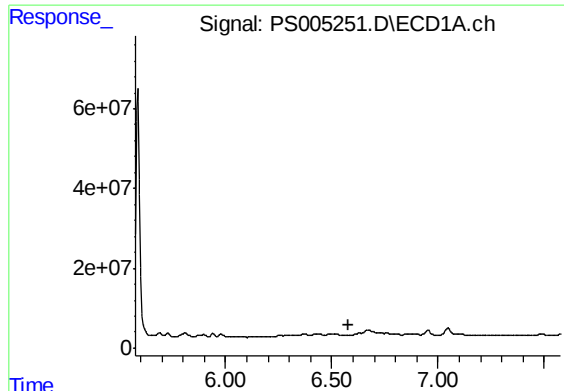

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

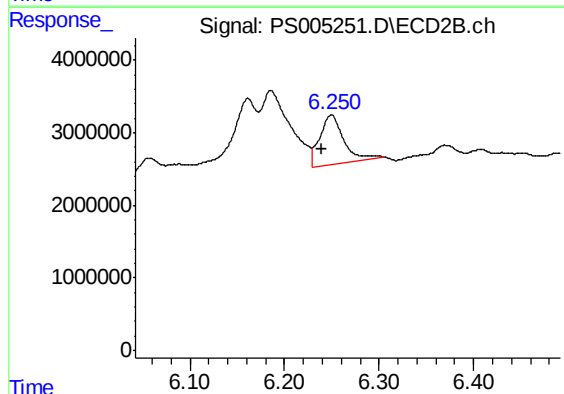


#9 2,4-D

R.T.: 6.250 min
Delta R.T.: 0.010 min
Response: 11773879
Conc: 10.56 ng/ml

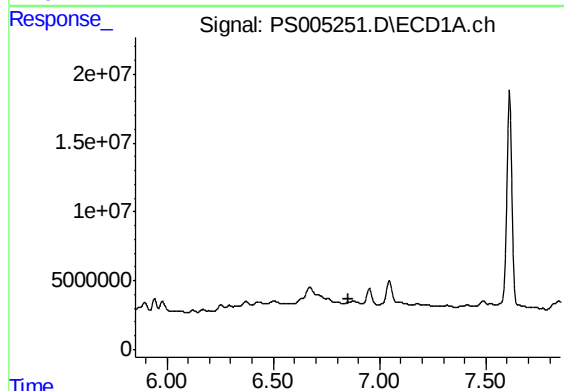


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

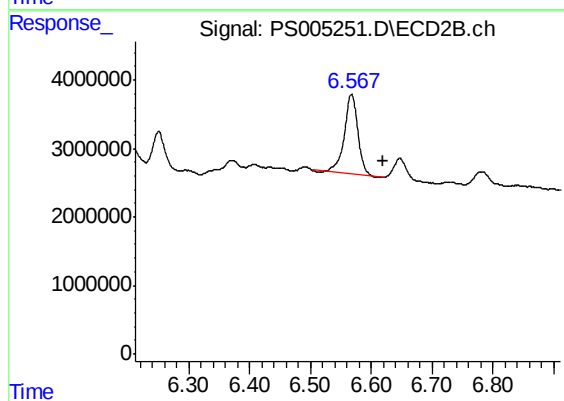

#10 Pentachlorophenol


R.T.: 6.567 min
Delta R.T.: -0.052 min
Response: 18445949
Conc: 1.43 ng/ml

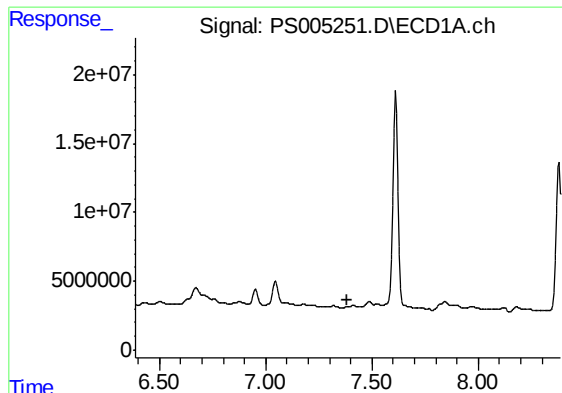

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-8

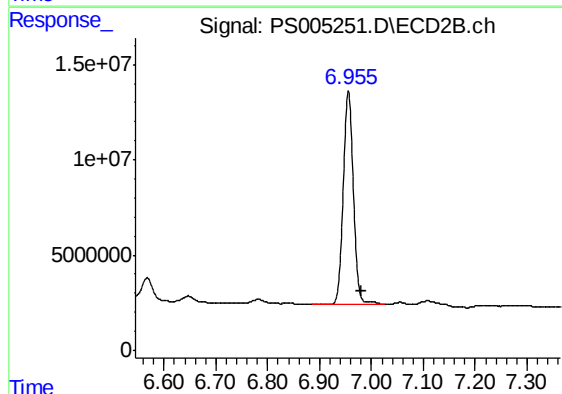


#11 2,4,5-TP (SILVEX)

R.T.: 6.956 min
Delta R.T.: -0.025 min
Response: 153027963
Conc: 28.74 ng/ml

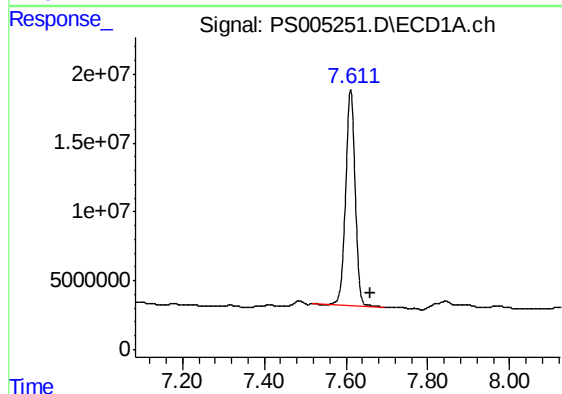

#12 2,4,5-T

R.T.: 7.611 min
Delta R.T.: -0.047 min
Response: 254743086
Conc: 31.65 ng/ml

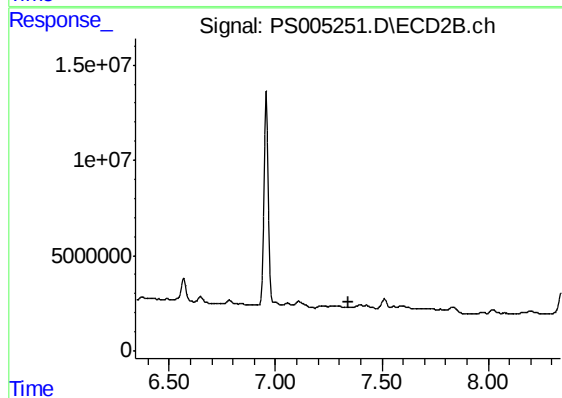

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.