

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 10:44
 Operator : SM\AJ
 Sample : K3530-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-044-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 12:48:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.568	5.283	315.4E6	200.1E6	214.857	199.612
Target Compounds							
2) T	3,5-DICHL...	0.000	4.601	0	217.3E6	N.D.	164.791
3) T	4-Nitroph...	5.370	0.000	27296297	0	37.687	N.D. #
5) T	DICAMBA	5.669	5.389	8346793	21495966	1.463	5.742 #
7) T	MCPA	6.060	5.674	15176859	27479675	2.417	6.784 #
8) T	DICHLORPROP	0.000	5.907	0	16062286	N.D.	16.636
10) T	Pentachlo...	6.852	6.621	24334490	19809856	1.237	1.541
11) T	2,4,5-TP ...	0.000	6.936	0	133.6E6	N.D.	25.080
12) T	2,4,5-T	7.590	0.000	223.0E6	0	27.715	N.D. #
14) T	DINOSEB	0.000	8.143	0	44675000	N.D.	11.049



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 10:44
Operator : SM\AJ
Sample : K3530-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 12:48:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

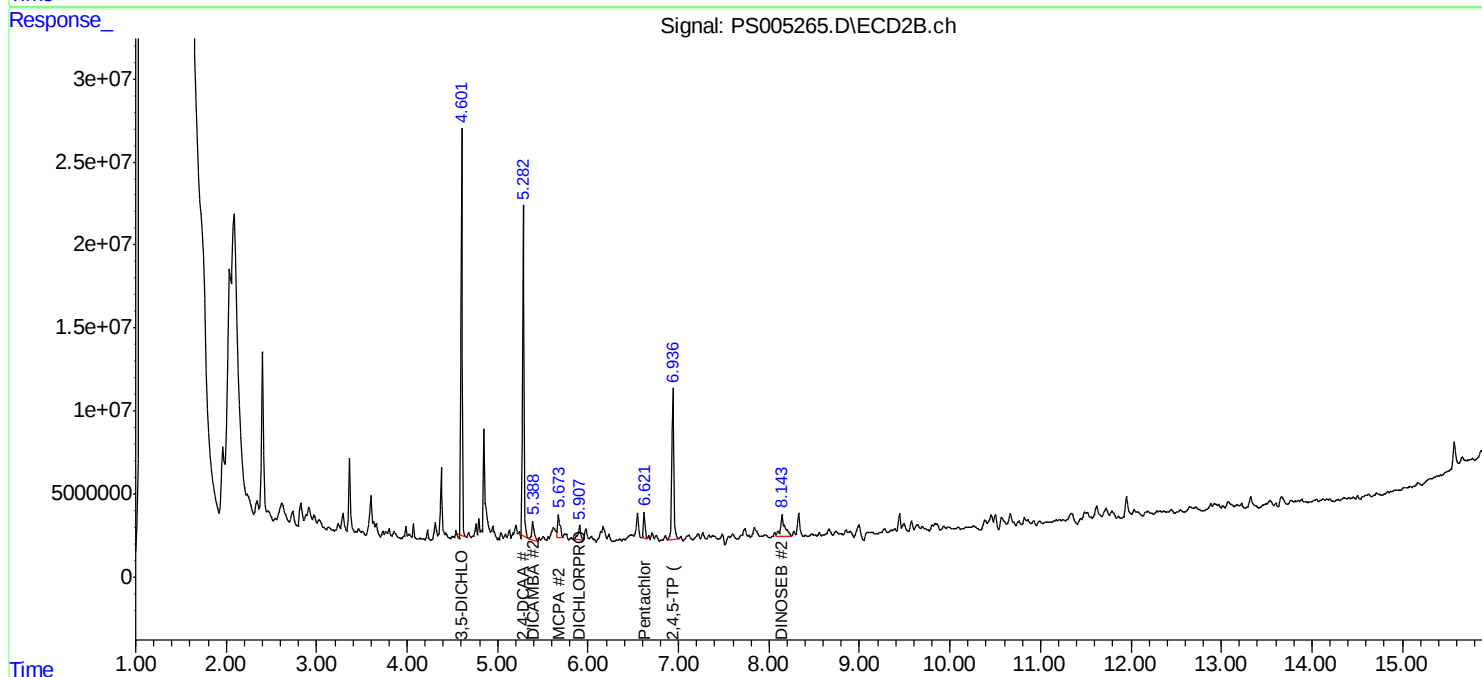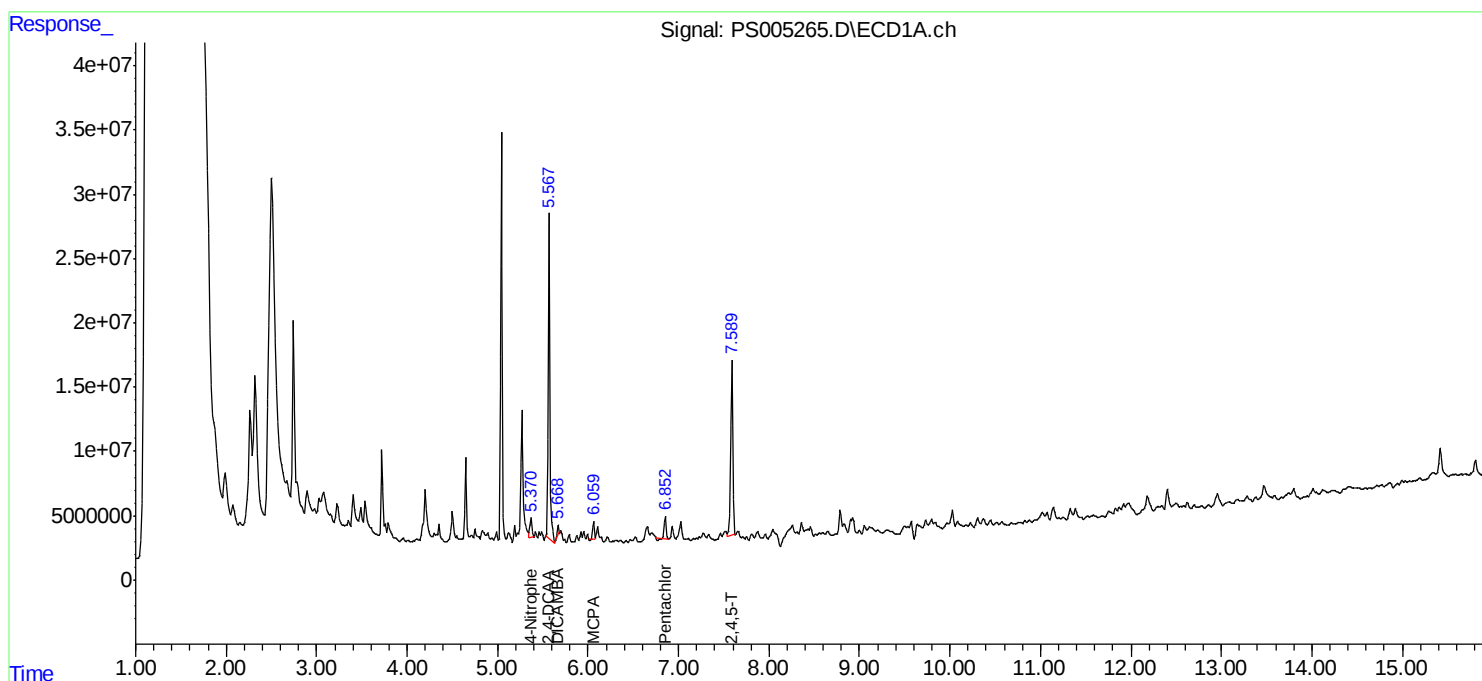


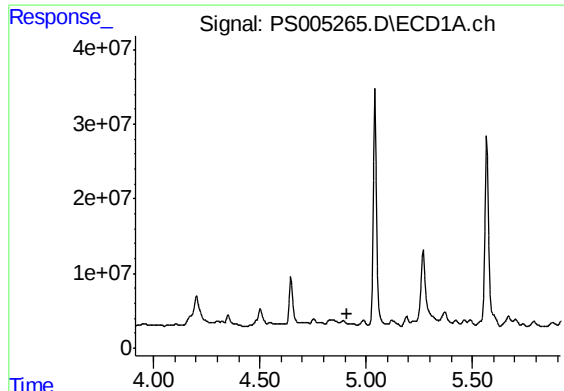

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

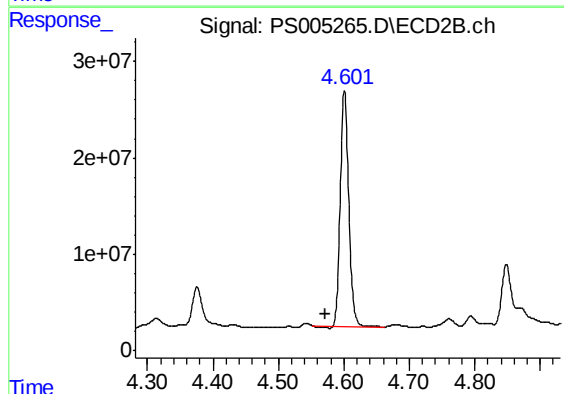


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.601 min
Delta R.T.: 0.029 min
Response: 217311448
Conc: 164.79 ng/ml

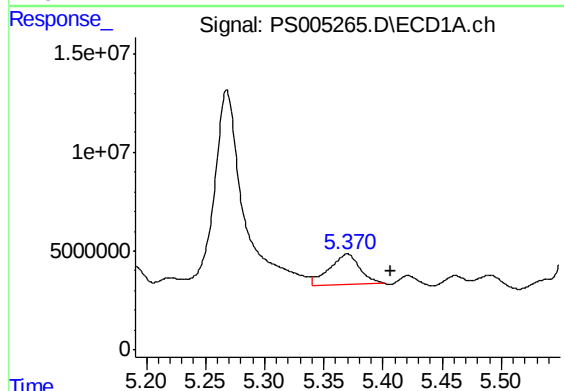


#3 4-Nitrophenol

R.T.: 5.370 min
Delta R.T.: -0.036 min
Response: 27296297
Conc: 37.69 ng/ml

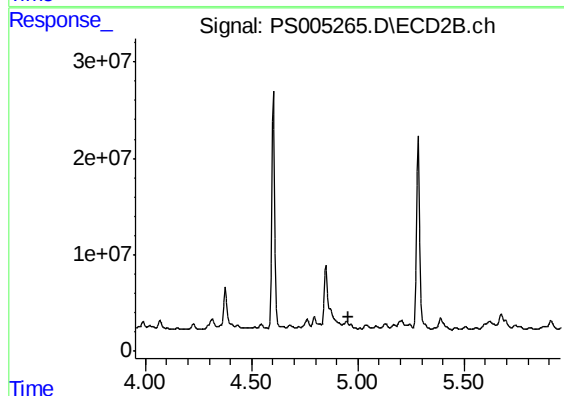

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

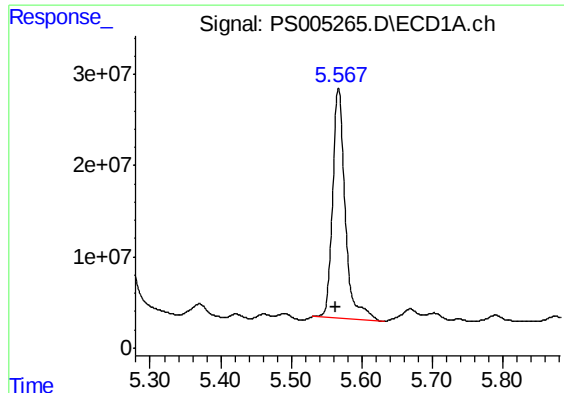

#4 2,4-DCAA


R.T.: 5.568 min
Delta R.T.: 0.004 min
Response: 315387282
Conc: 214.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

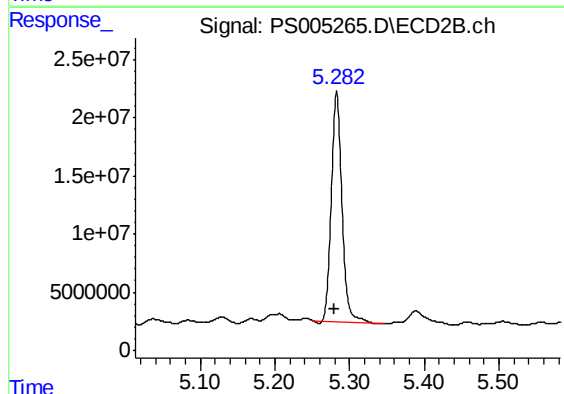


#4 2,4-DCAA

R.T.: 5.283 min
Delta R.T.: 0.003 min
Response: 200084453
Conc: 199.61 ng/ml

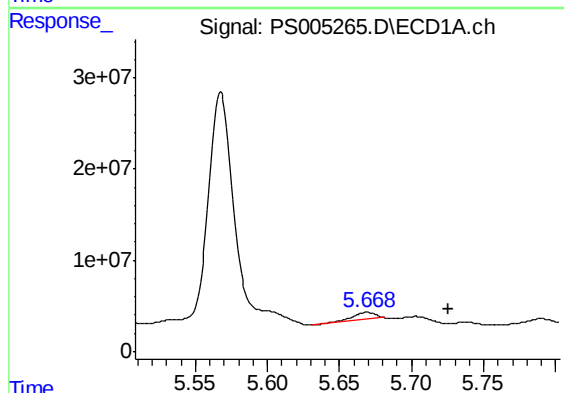


#5 DICAMBA

R.T.: 5.669 min
Delta R.T.: -0.056 min
Response: 8346793
Conc: 1.46 ng/ml

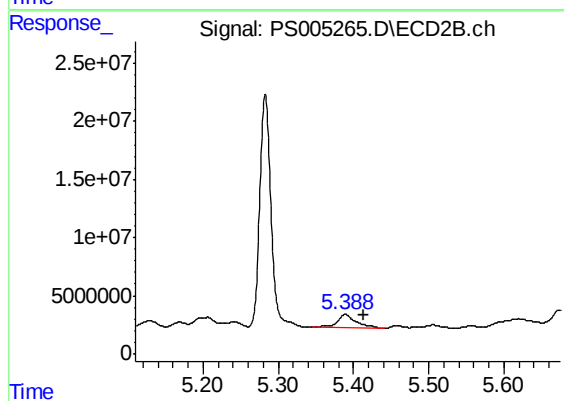

#5 DICAMBA


R.T.: 5.389 min
Delta R.T.: -0.025 min
Response: 21495966
Conc: 5.74 ng/ml

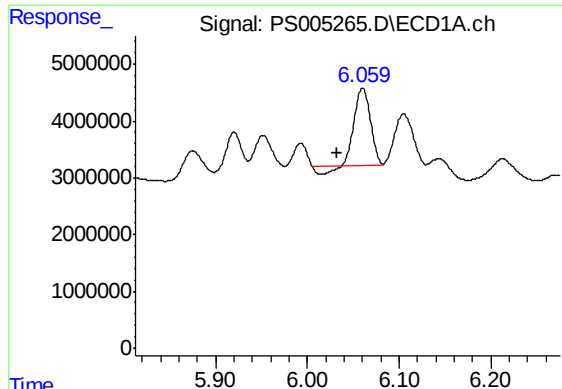

#7 MCPA


R.T.: 6.060 min
Delta R.T.: 0.028 min
Response: 15176859
Conc: 2.42 ug/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

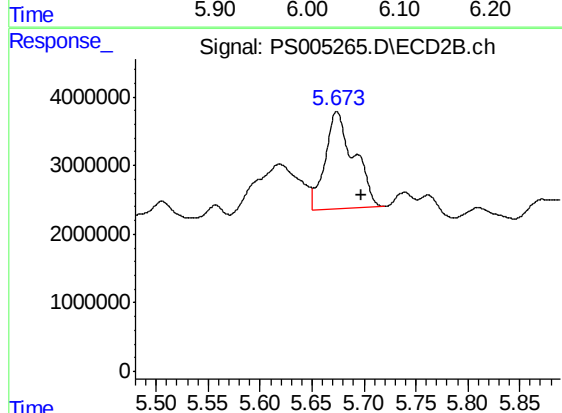


#7 MCPA

R.T.: 5.674 min
Delta R.T.: -0.024 min
Response: 27479675
Conc: 6.78 ug/ml

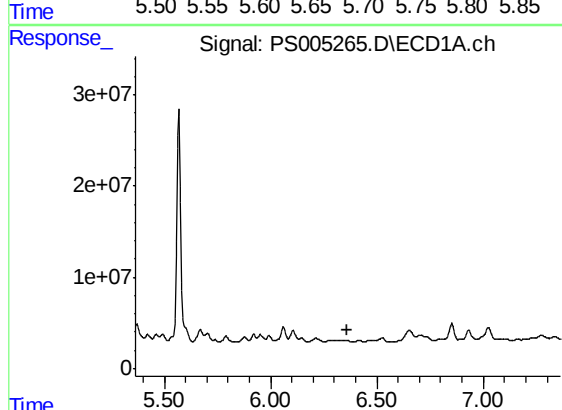


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

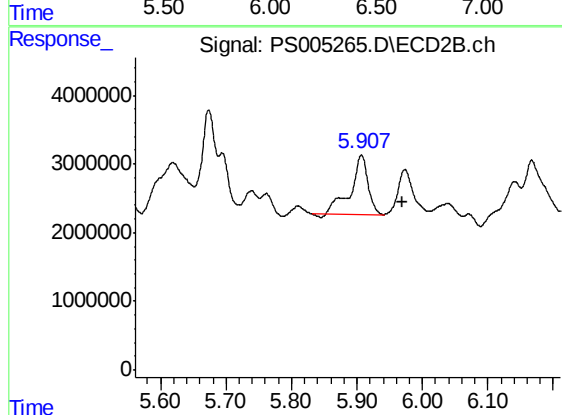

#8 DICHLORPROP


R.T.: 5.907 min
Delta R.T.: -0.062 min
Response: 16062286
Conc: 16.64 ng/ml

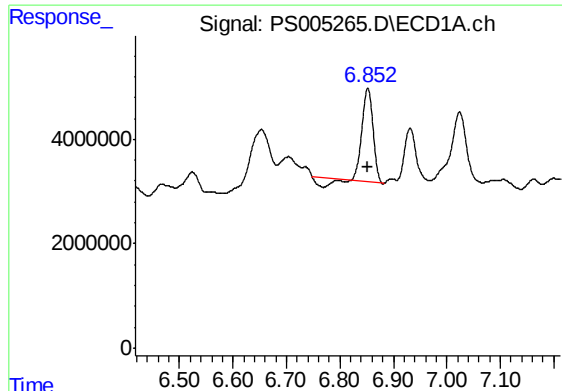

#10 Pentachlorophenol


R.T.: 6.852 min
Delta R.T.: 0.000 min
Response: 24334490
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

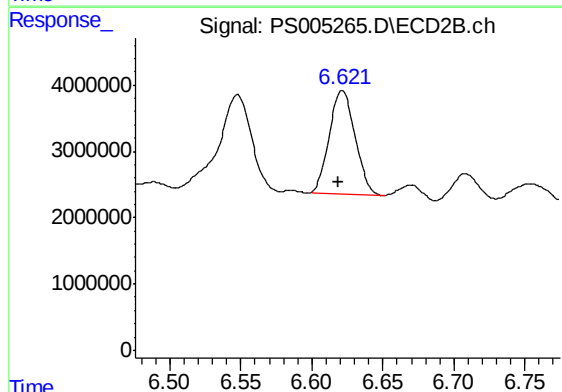


#10 Pentachlorophenol

R.T.: 6.621 min
Delta R.T.: 0.002 min
Response: 19809856
Conc: 1.54 ng/ml

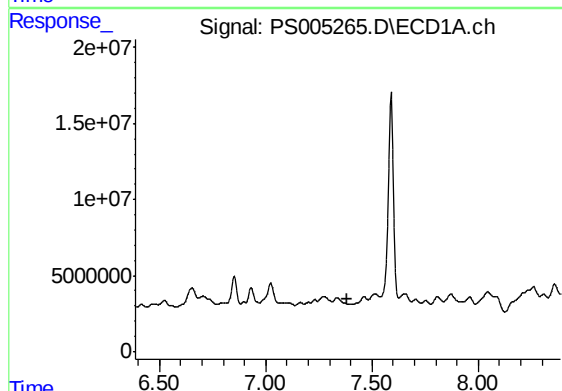


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

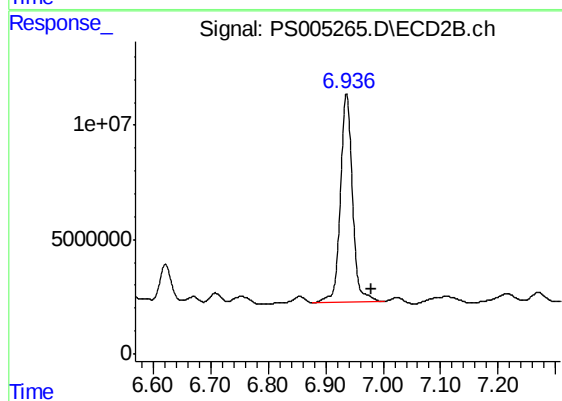

#11 2,4,5-TP (SILVEX)


R.T.: 6.936 min
Delta R.T.: -0.044 min
Response: 133557561
Conc: 25.08 ng/ml

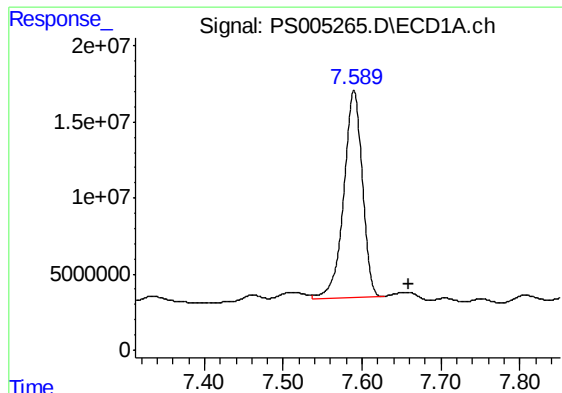

#12 2,4,5-T


R.T.: 7.590 min
Delta R.T.: -0.069 min
Response: 223044771
Conc: 27.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-044-B

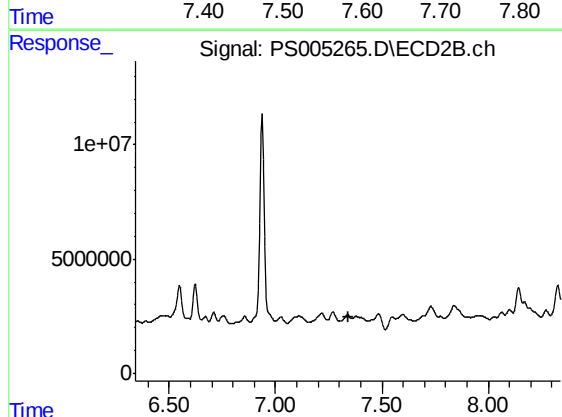


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

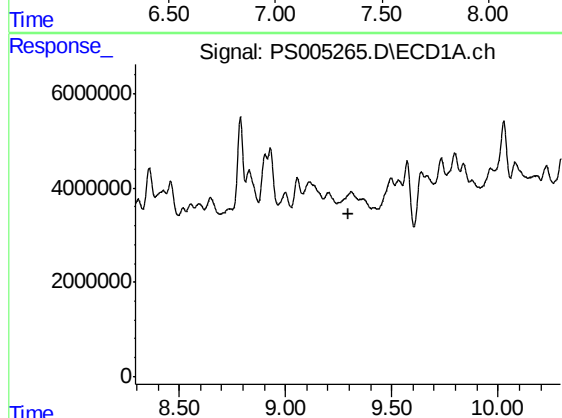

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

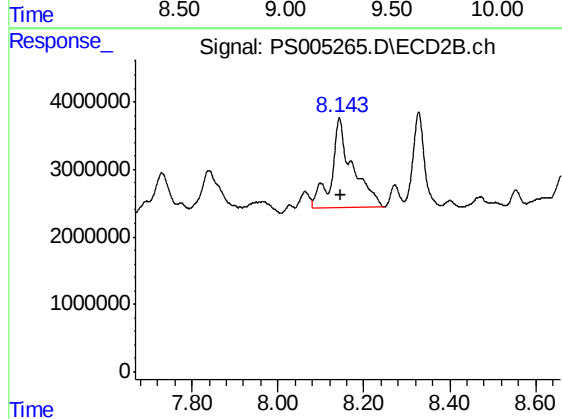

#14 DINOSEB

R.T.: 8.143 min
Delta R.T.: -0.003 min
Response: 44675000
Conc: 11.05 ng/ml