

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 11:06
 Operator : SM\AJ
 Sample : K3531-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-043-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 12:48:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.582	5.297	444.4E6	269.2E6	302.742	268.519
Target Compounds							
2) T	3,5-DICHL...	0.000	4.616	0	169.6E6	N.D.	128.574
3) T	4-Nitroph...	5.384	0.000	12252872	0	16.917	N.D. #
7) T	MCPA	6.075	5.689	5970612	24071934	<MDL	5.942 #
8) T	DICHLORPROP	0.000	5.922	0	31770780	N.D.	32.905
9) T	2,4-D	0.000	6.182	0	15947495	N.D.	14.299
10) T	Pentachlo...	6.867	6.636	28204585	24871840	1.433	1.935 #
11) T	2,4,5-TP ...	0.000	6.951	0	141.8E6	N.D.	26.627
12) T	2,4,5-T	7.605	0.000	240.6E6	0	29.898	N.D. #
14) T	DINOSEB	0.000	8.157	0	40336179	N.D.	9.976



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 11:06
Operator : SM\AJ
Sample : K3531-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 12:48:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

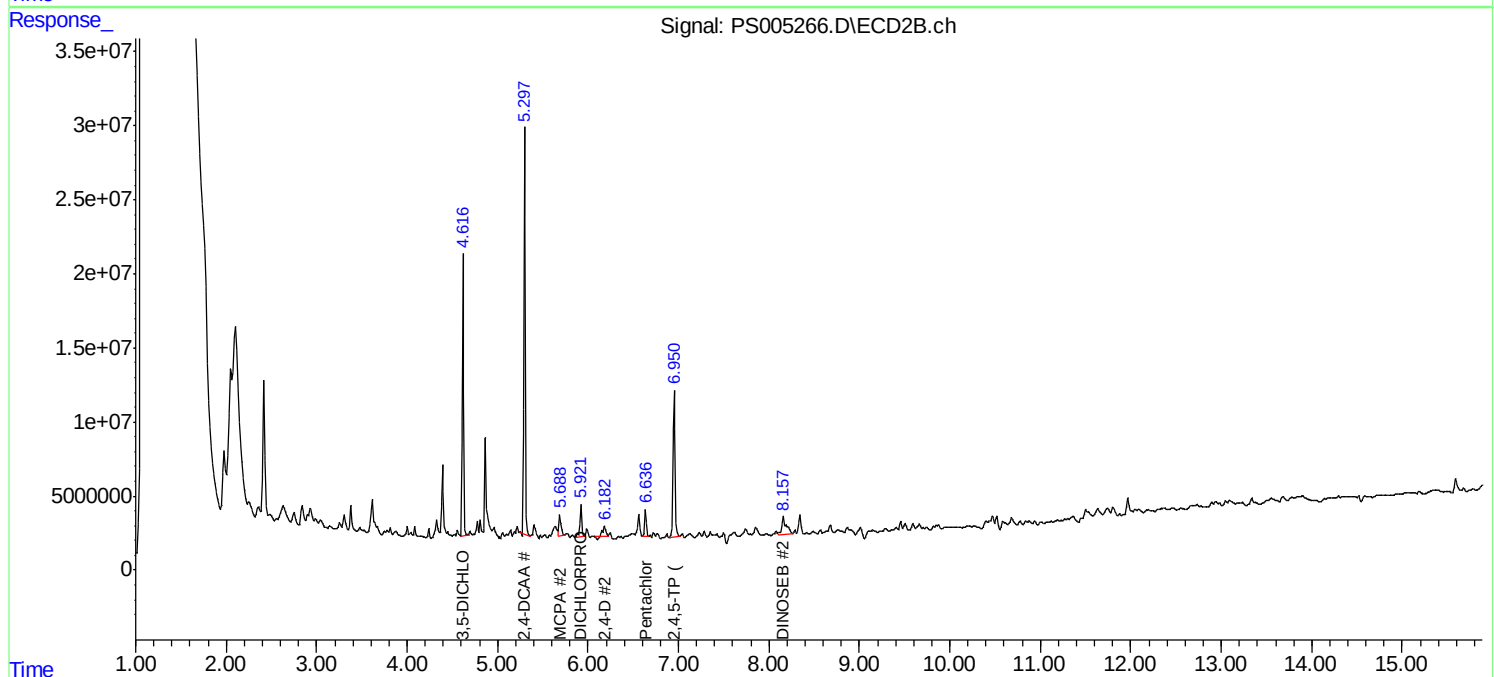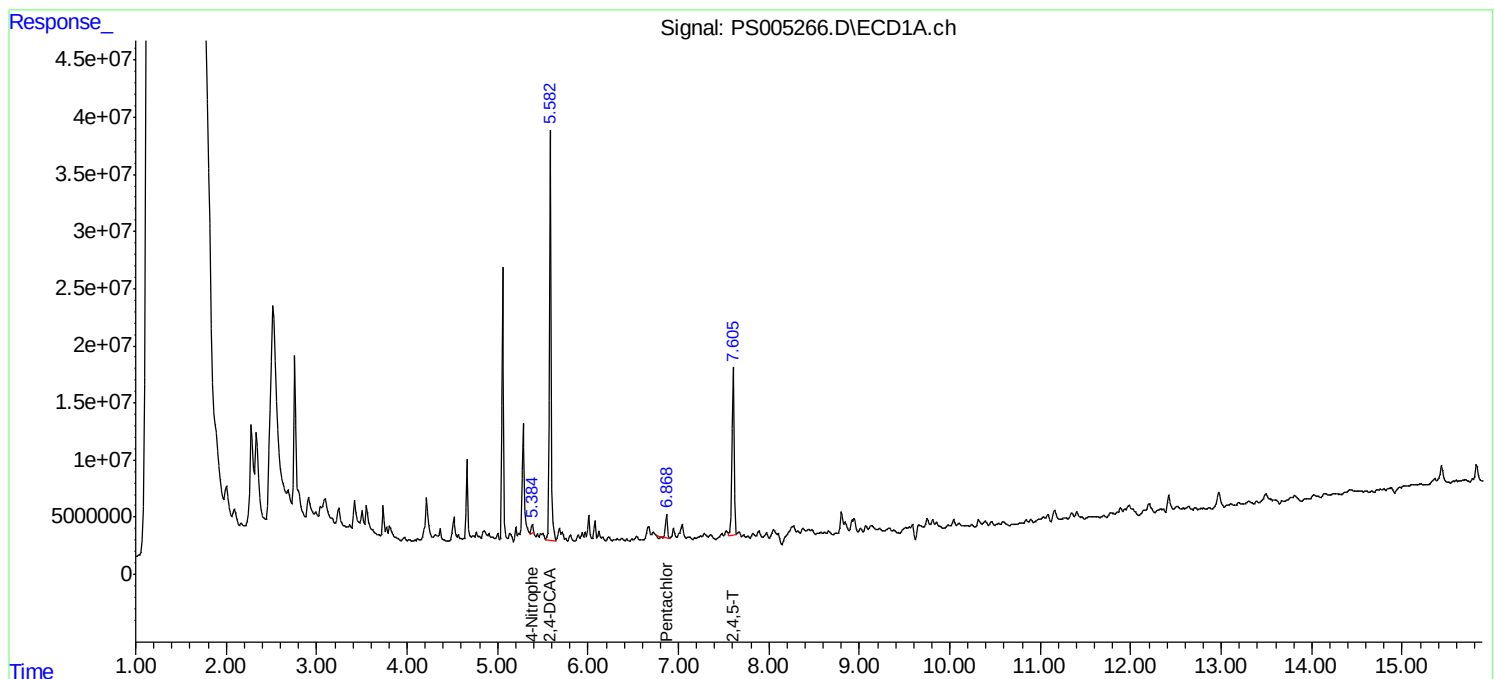


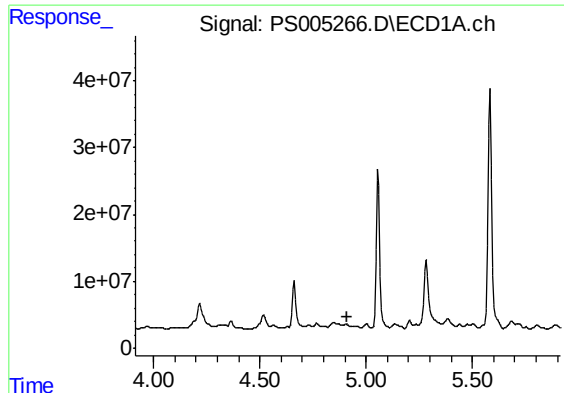

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

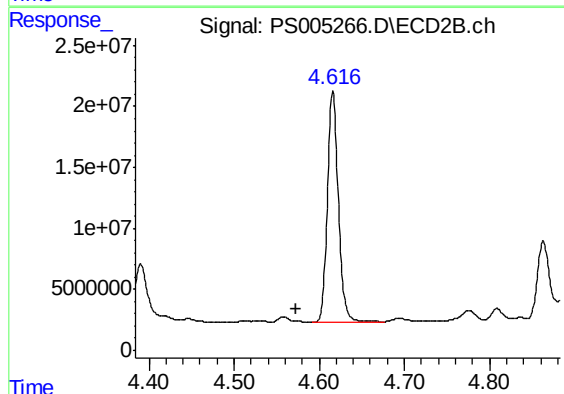


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.616 min
Delta R.T.: 0.044 min
Response: 169551375
Conc: 128.57 ng/ml

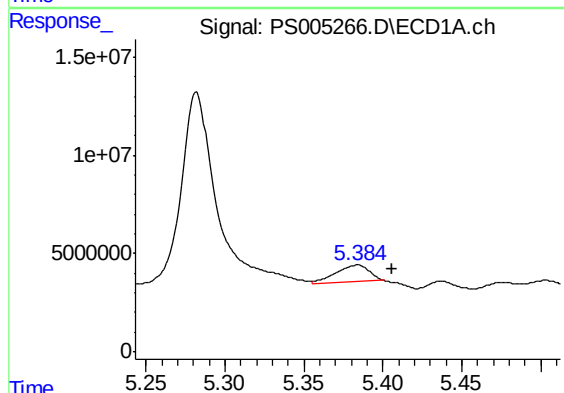


#3 4-Nitrophenol

R.T.: 5.384 min
Delta R.T.: -0.023 min
Response: 12252872
Conc: 16.92 ng/ml

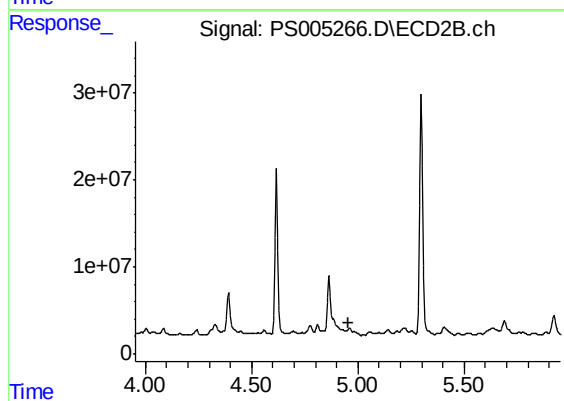

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

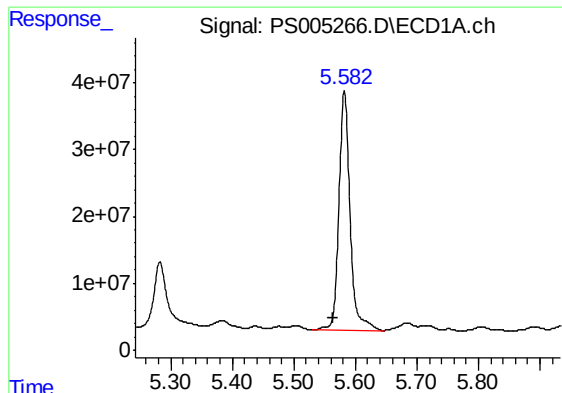

#4 2,4-DCAA


R.T.: 5.582 min
Delta R.T.: 0.018 min
Response: 444393461
Conc: 302.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

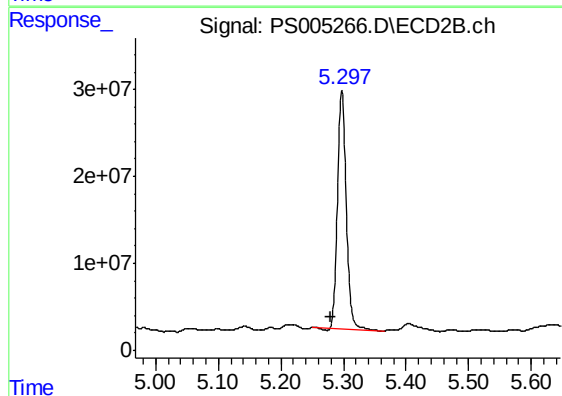


#4 2,4-DCAA

R.T.: 5.297 min
Delta R.T.: 0.018 min
Response: 269155050
Conc: 268.52 ng/ml

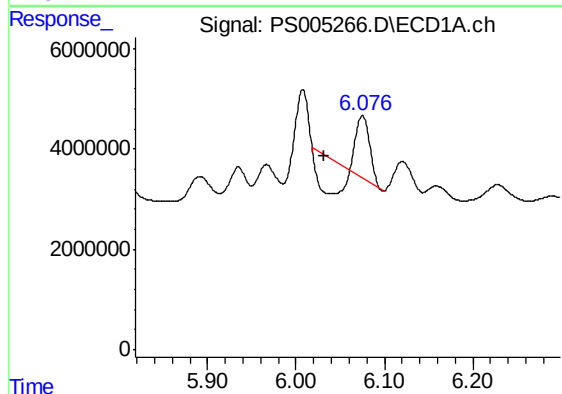


#7 MCPA

R.T.: 6.075 min
Delta R.T.: 0.043 min
Response: 5970612
Conc: N.D.

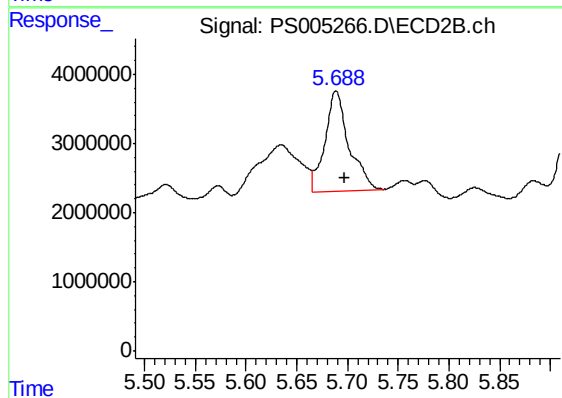

#7 MCPA


R.T.: 5.689 min
Delta R.T.: -0.009 min
Response: 24071934
Conc: 5.94 ug/ml

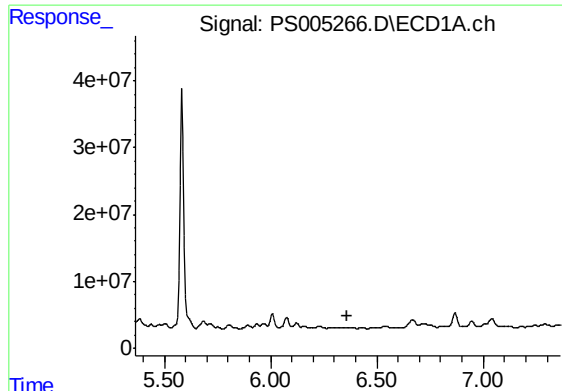

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

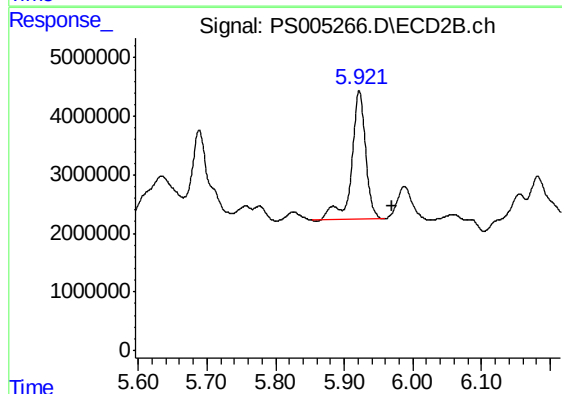


#8 DICHLORPROP

R.T.: 5.922 min
Delta R.T.: -0.047 min
Response: 31770780
Conc: 32.90 ng/ml

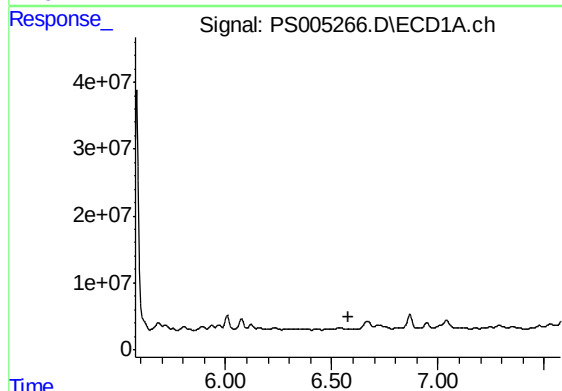


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

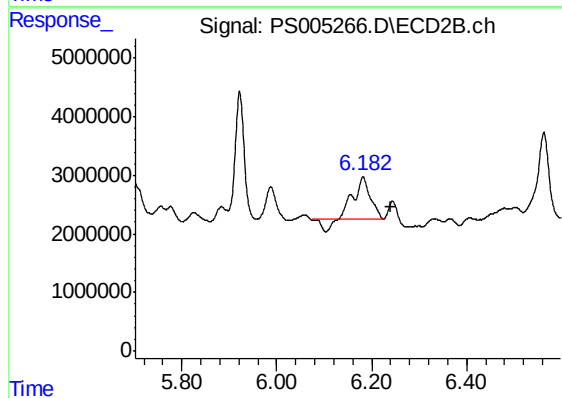

#9 2,4-D


R.T.: 6.182 min
Delta R.T.: -0.058 min
Response: 15947495
Conc: 14.30 ng/ml

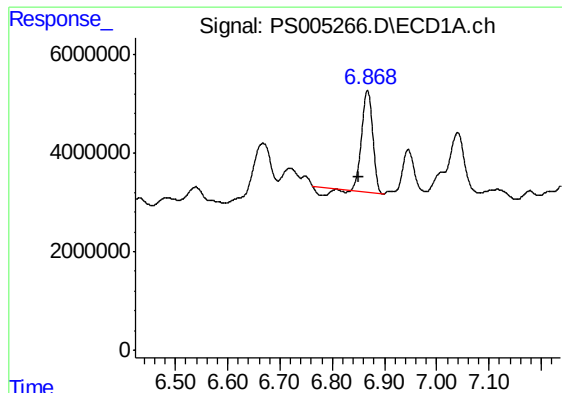

#10 Pentachlorophenol


R.T.: 6.867 min
Delta R.T.: 0.016 min
Response: 28204585
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

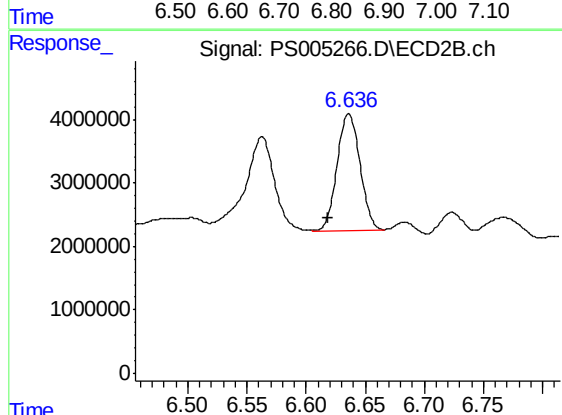


#10 Pentachlorophenol

R.T.: 6.636 min
Delta R.T.: 0.017 min
Response: 24871840
Conc: 1.93 ng/ml

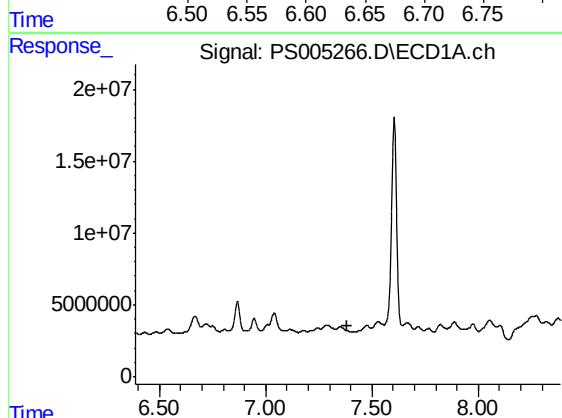


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

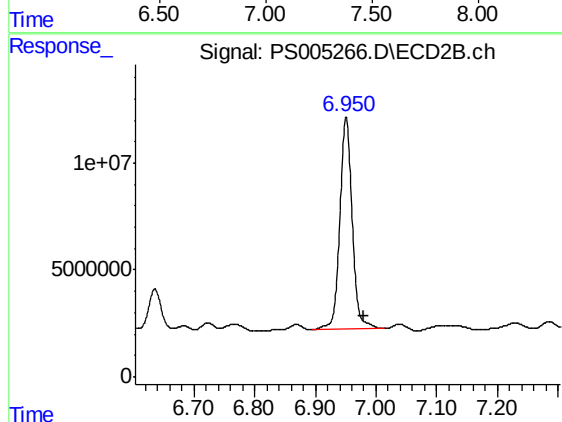

#11 2,4,5-TP (SILVEX)


R.T.: 6.951 min
Delta R.T.: -0.030 min
Response: 141798900
Conc: 26.63 ng/ml

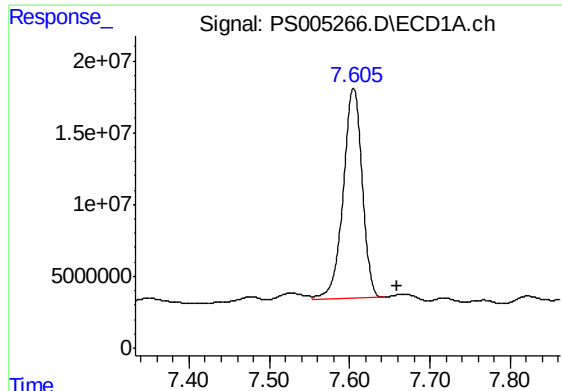

#12 2,4,5-T


R.T.: 7.605 min
Delta R.T.: -0.054 min
Response: 240617716
Conc: 29.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-043-A

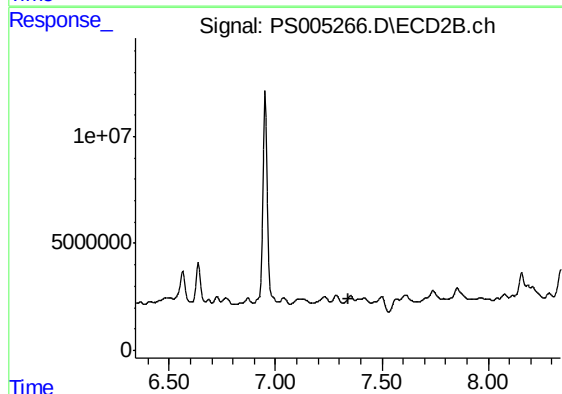


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

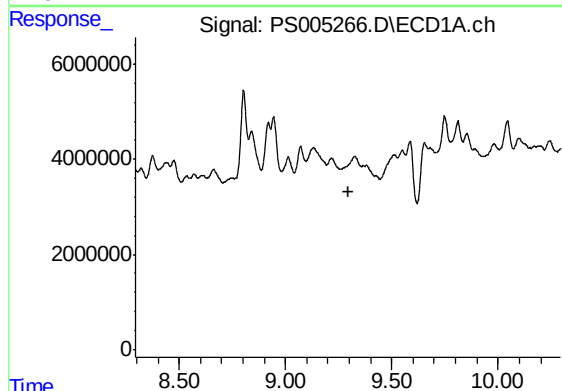

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.294 min
Response: 0
Conc: N.D.

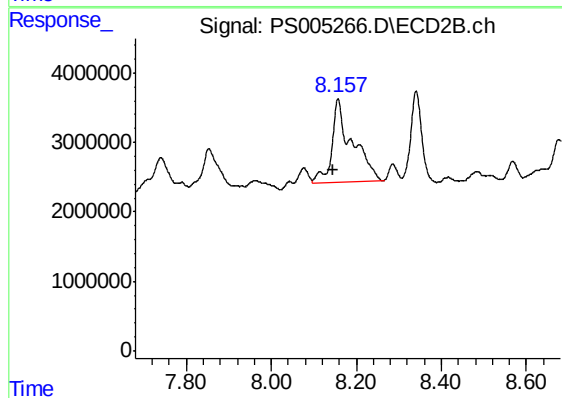

#14 DINOSEB

R.T.: 8.157 min
Delta R.T.: 0.011 min
Response: 40336179
Conc: 9.98 ng/ml