

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 16:44
 Operator : SM\AJ
 Sample : K3157-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-062619-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 17:58:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.570	5.285	697.8E6	461.7E6	475.385	460.578
Target Compounds							
2) T	3,5-DICHL...	0.000	4.604	0	329.0E6	N.D.	249.521
3) T	4-Nitroph...	5.361	4.951	20981604	19522087	28.968	38.931 #
5) T	DICAMBA	5.762	5.391	14832367	20285424	2.600	5.419 #
6) T	MCP	5.923	0.000	16320634	0	3.728	N.D. #
8) T	DICHLORPROP	6.312	5.973	-25326779	39520696	N.D.	40.931
11) T	2,4,5-TP ...	0.000	6.939	0	207.0E6	N.D.	38.863
12) T	2,4,5-T	7.593	0.000	337.1E6	0	41.881	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 16:44
Operator : SM\AJ
Sample : K3157-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 17:58:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

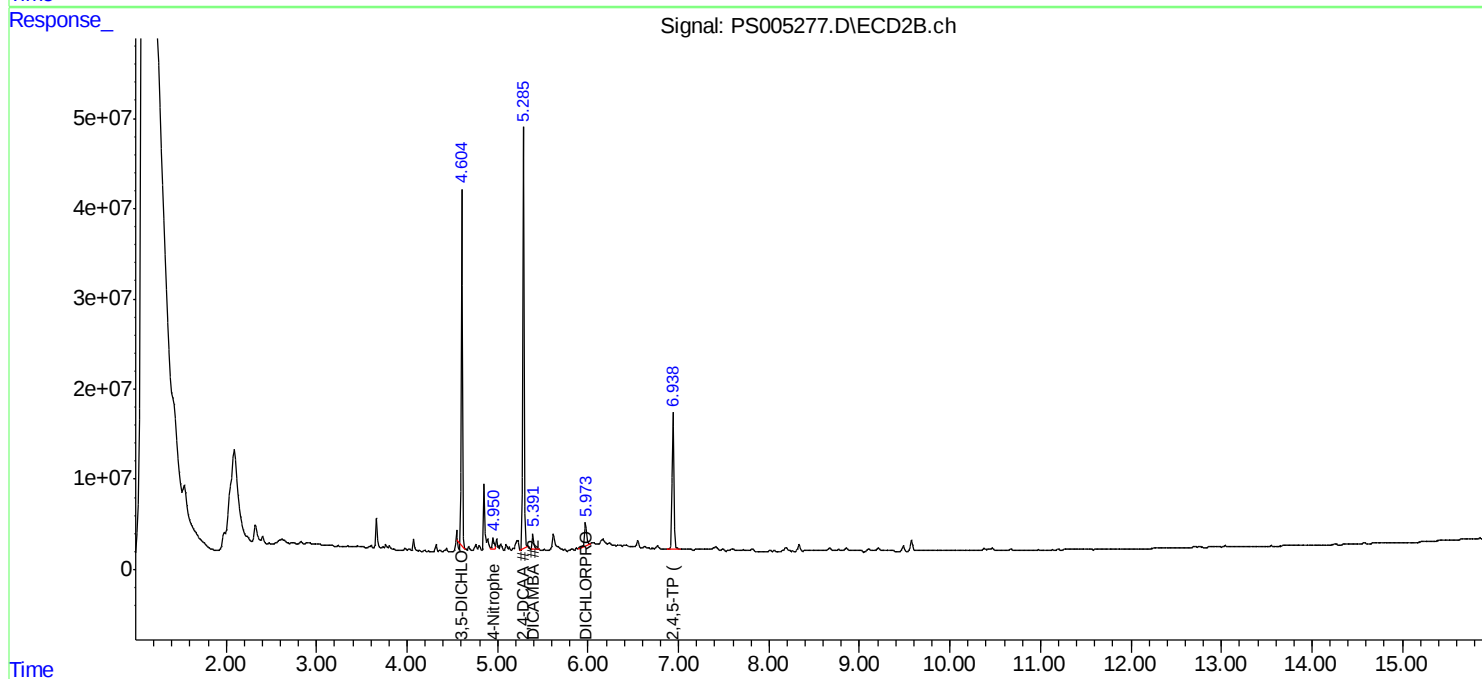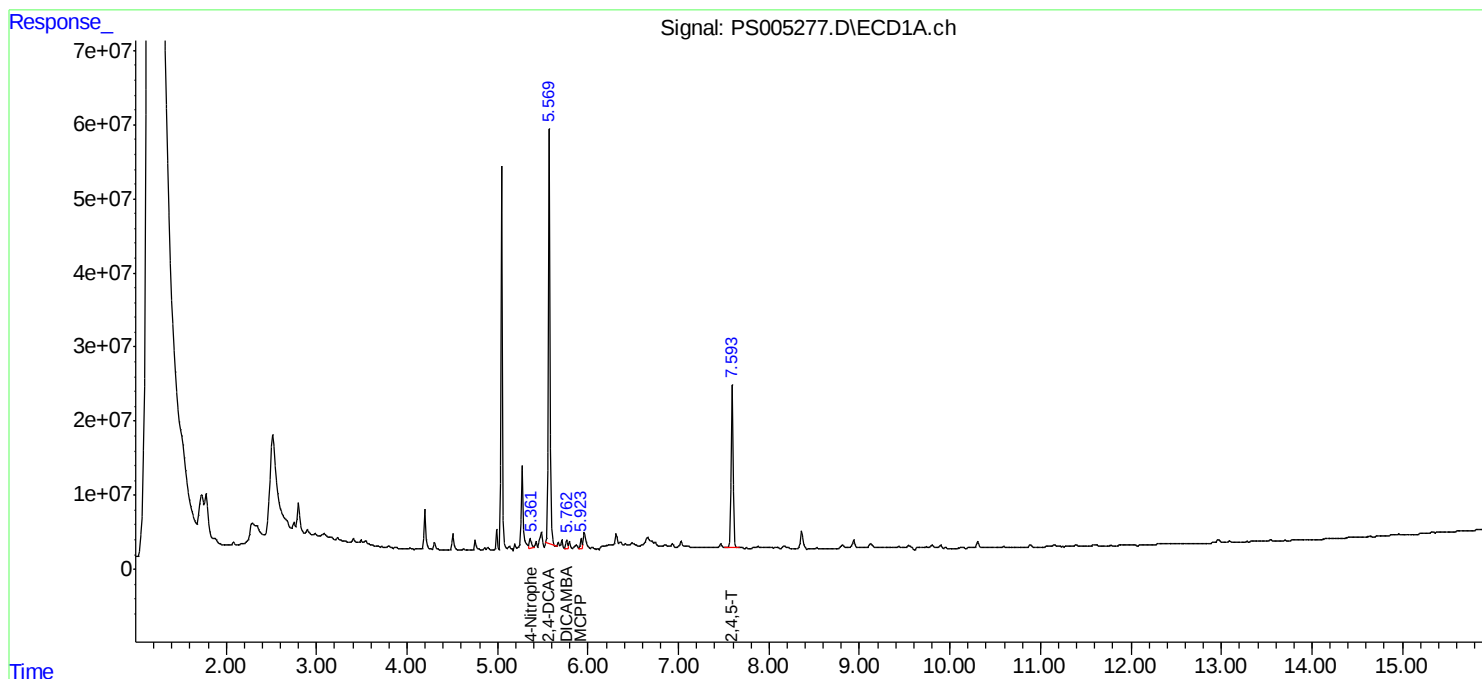


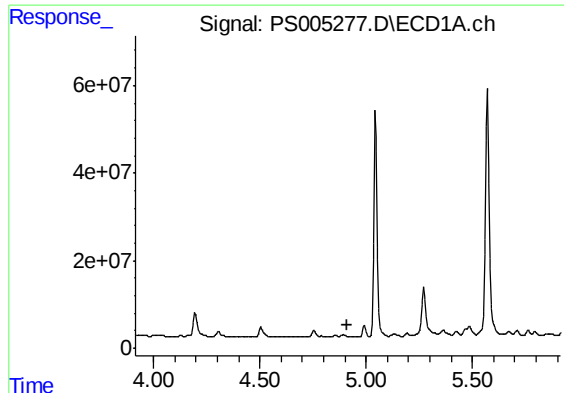

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-A

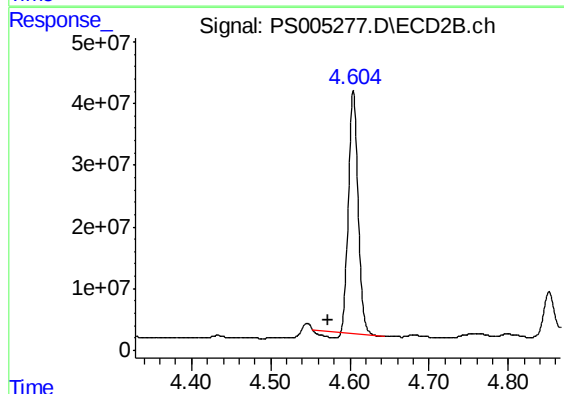


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.604 min
Delta R.T.: 0.032 min
Response: 329045741
Conc: 249.52 ng/ml

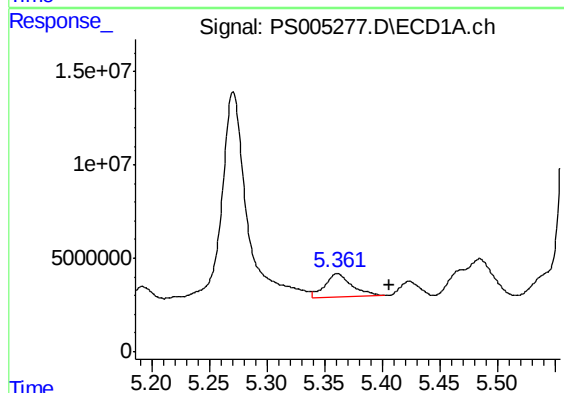


#3 4-Nitrophenol

R.T.: 5.361 min
Delta R.T.: -0.045 min
Response: 20981604
Conc: 28.97 ng/ml

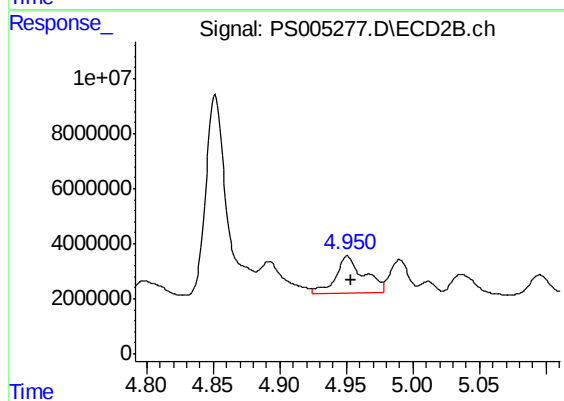

#3 4-Nitrophenol


R.T.: 4.951 min
Delta R.T.: -0.002 min
Response: 19522087
Conc: 38.93 ng/ml

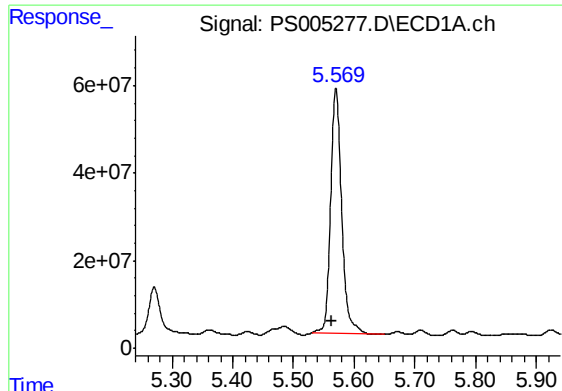

#4 2,4-DCAA


R.T.: 5.570 min
Delta R.T.: 0.006 min
Response: 697814421
Conc: 475.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-A

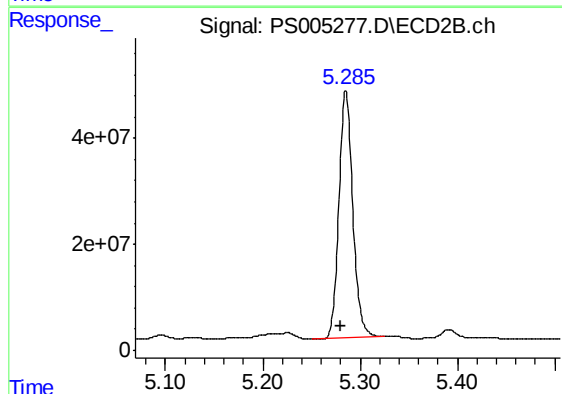


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: 0.006 min
Response: 461669157
Conc: 460.58 ng/ml

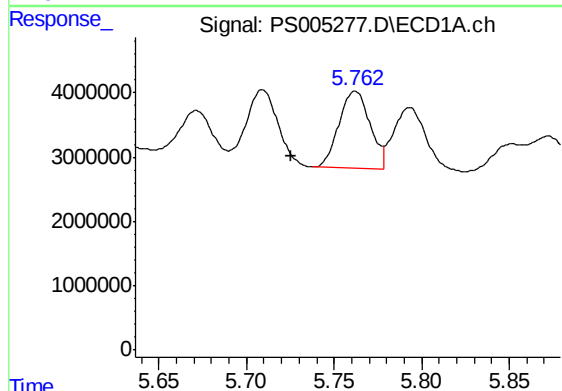


#5 DICAMBA

R.T.: 5.762 min
Delta R.T.: 0.037 min
Response: 14832367
Conc: 2.60 ng/ml

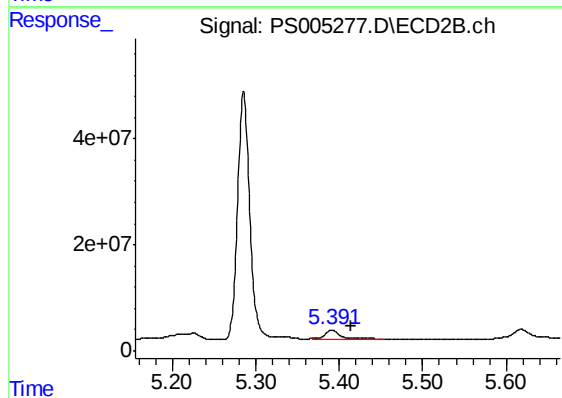

#5 DICAMBA


R.T.: 5.391 min
Delta R.T.: -0.023 min
Response: 20285424
Conc: 5.42 ng/ml

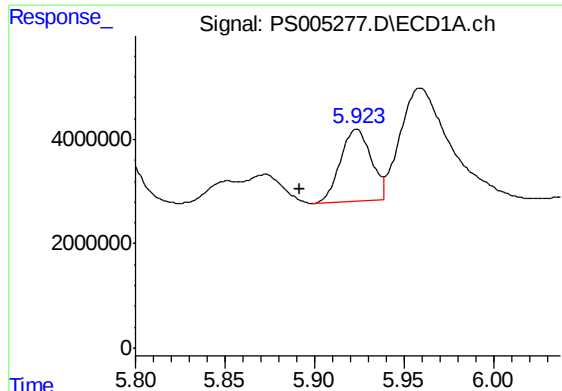

#6 MCP


R.T.: 5.923 min
Delta R.T.: 0.031 min
Response: 16320634
Conc: 3.73 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-A

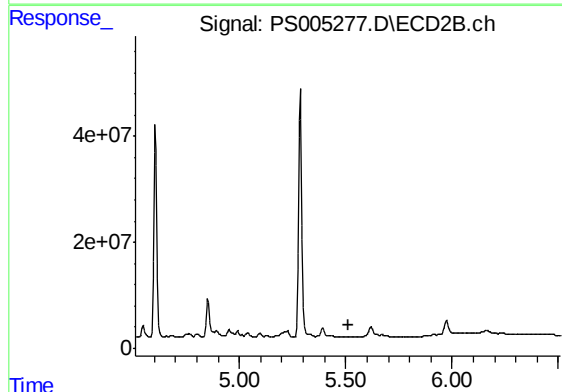


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

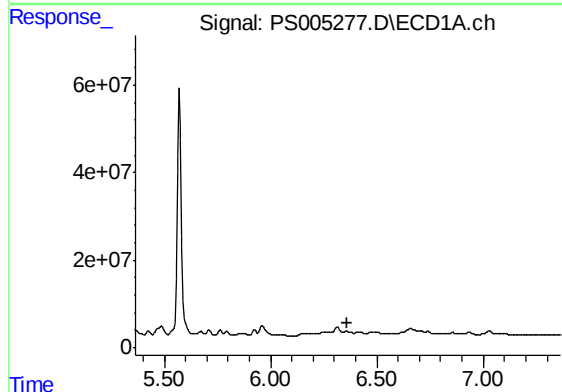


#8 DICHLORPROP

R.T.: 6.312 min
Delta R.T.: -0.051 min
Response: -25326779
Conc: N.D.

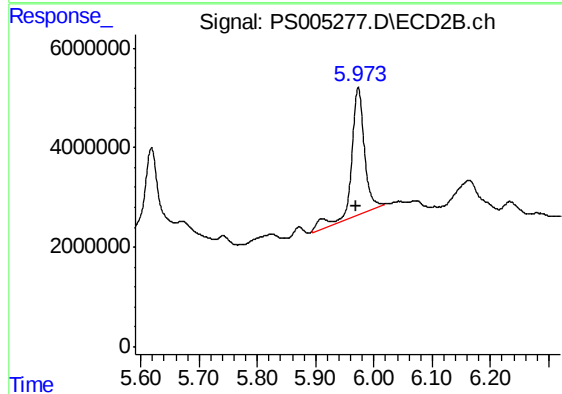

#8 DICHLORPROP


R.T.: 5.973 min
Delta R.T.: 0.004 min
Response: 39520696
Conc: 40.93 ng/ml

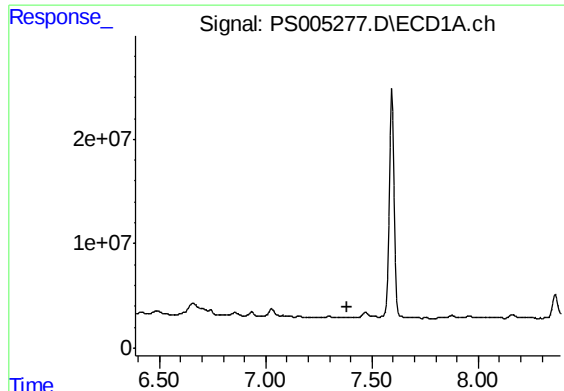

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-A

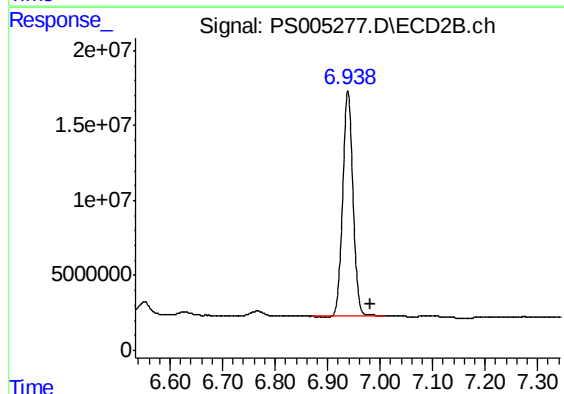


#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.042 min
Response: 206955827
Conc: 38.86 ng/ml

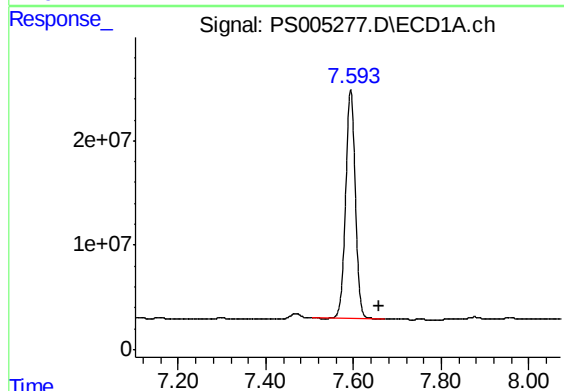

#12 2,4,5-T

R.T.: 7.593 min
Delta R.T.: -0.065 min
Response: 337053351
Conc: 41.88 ng/ml

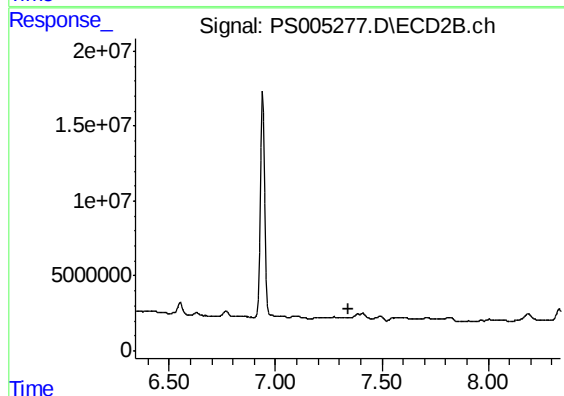

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.