

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 17:28
 Operator : SM\AJ
 Sample : K3157-16
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-062619-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 17:58:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.583	5.299	639.9E6	418.8E6	435.916	417.826
Target Compounds							
2) T	3,5-DICHL...	0.000	4.560	0	13373965	N.D.	10.142
3) T	4-Nitroph...	5.374	5.003	10299399	12574375	14.220	25.076 #
5) T	DICAMBA	5.774	5.405	11654093	13174169	2.043	3.519 #
6) T	MCP	5.936	0.000	12650743	0	2.890	N.D. #
7) T	MCPA	5.975	5.632	17631020	38463011	2.808	9.495 #
8) T	DICHLORPROP	0.000	5.987	0	20106156	N.D.	20.824
10) T	Pentachlo...	0.000	6.564	0	14644504	N.D.	1.139
11) T	2,4,5-TP ...	0.000	6.952	0	167.1E6	N.D.	31.373
12) T	2,4,5-T	7.605	0.000	276.2E6	0	34.317	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 17:28
Operator : SM\AJ
Sample : K3157-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 17:58:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

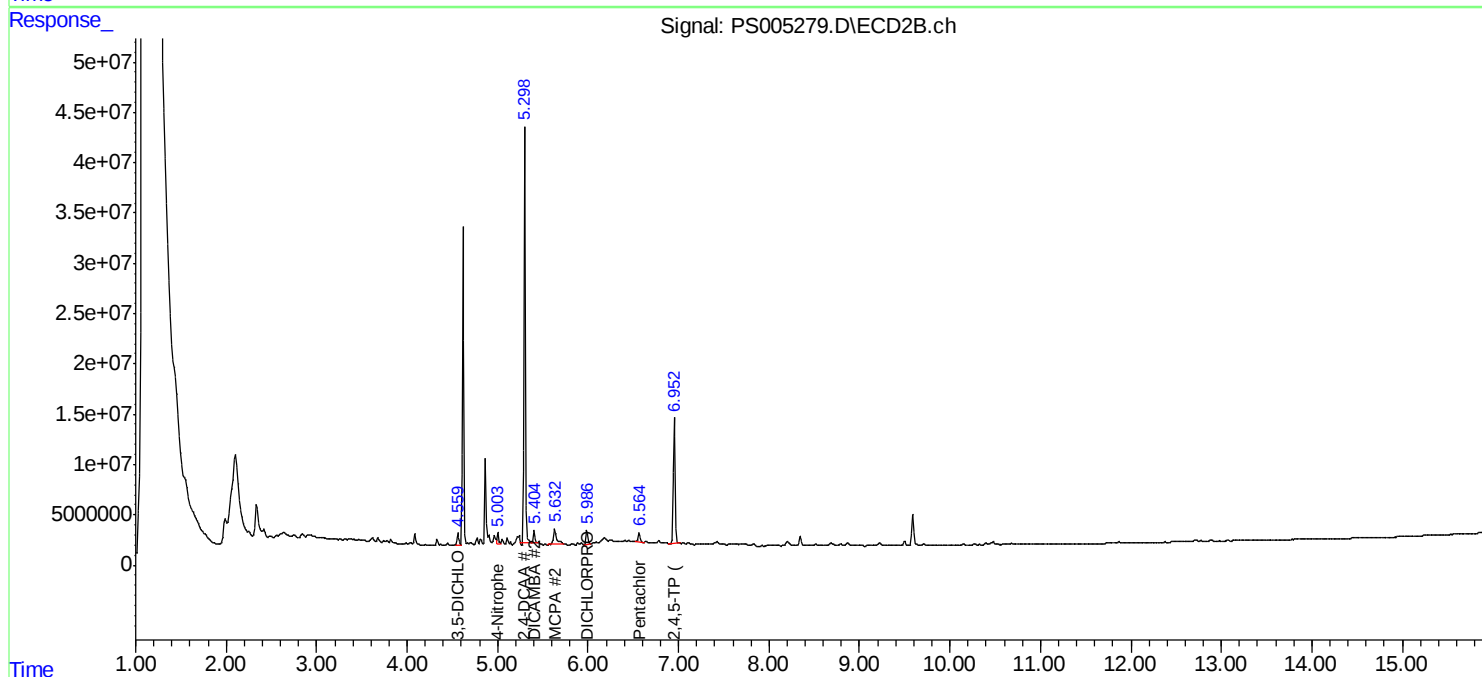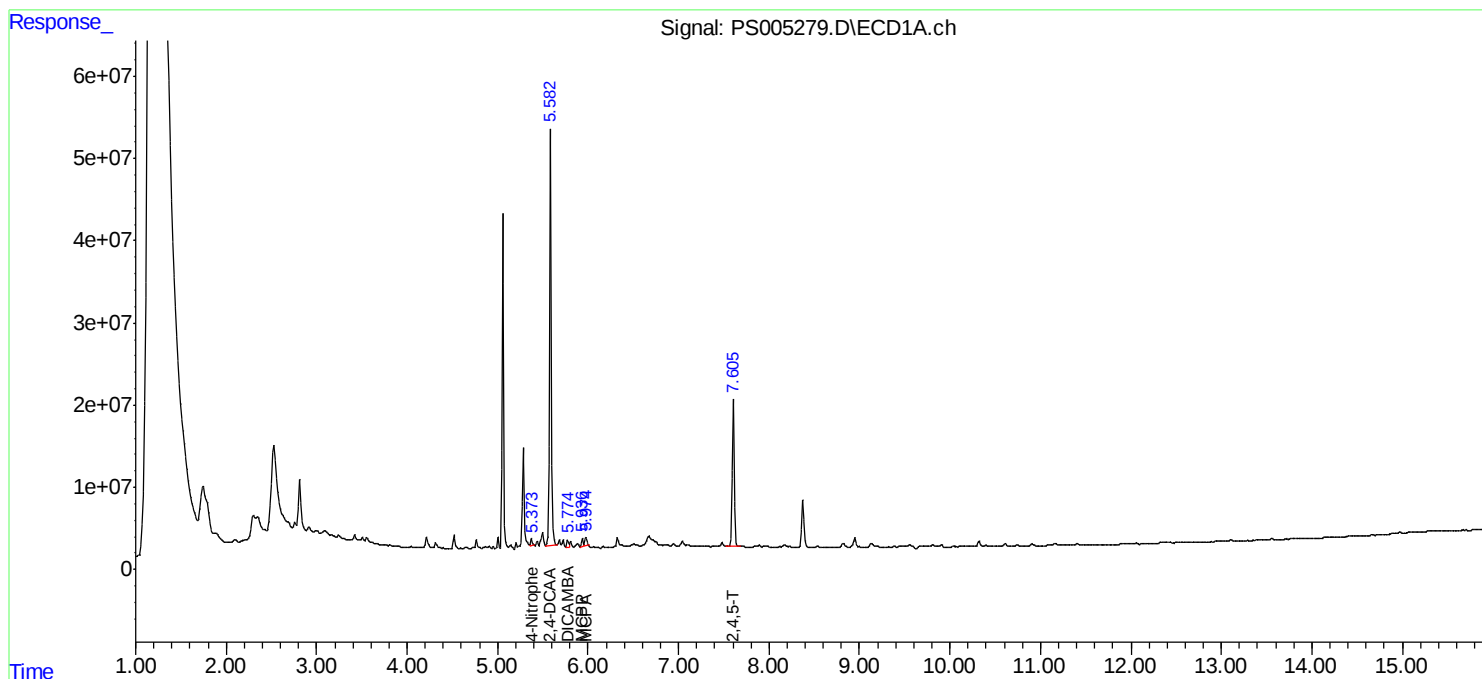


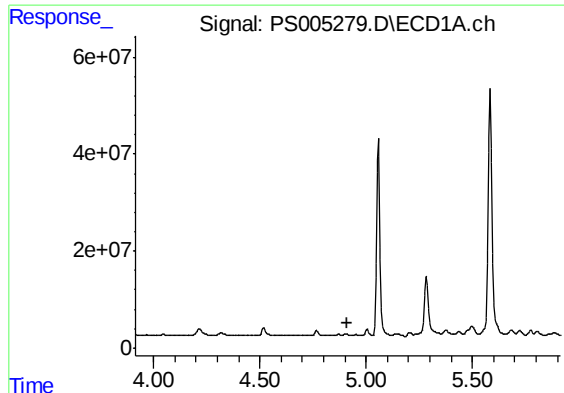

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

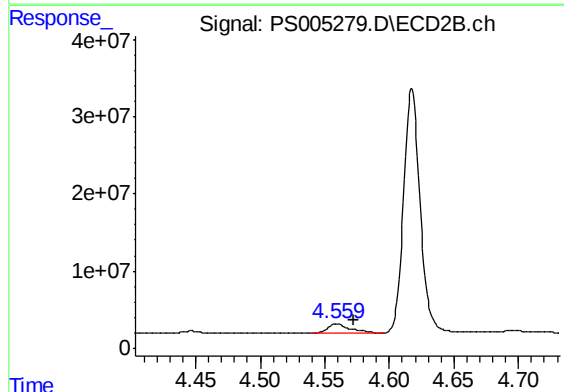


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.560 min
Delta R.T.: -0.013 min
Response: 13373965
Conc: 10.14 ng/ml

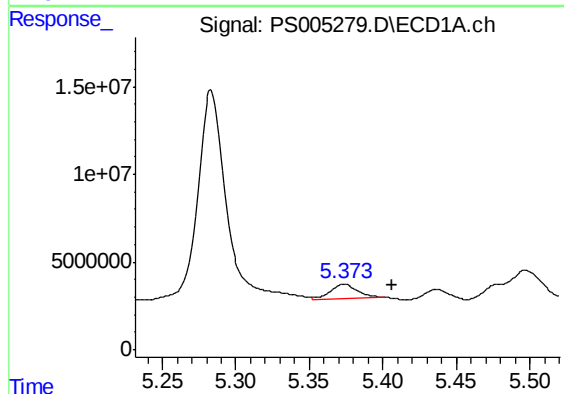


#3 4-Nitrophenol

R.T.: 5.374 min
Delta R.T.: -0.033 min
Response: 10299399
Conc: 14.22 ng/ml

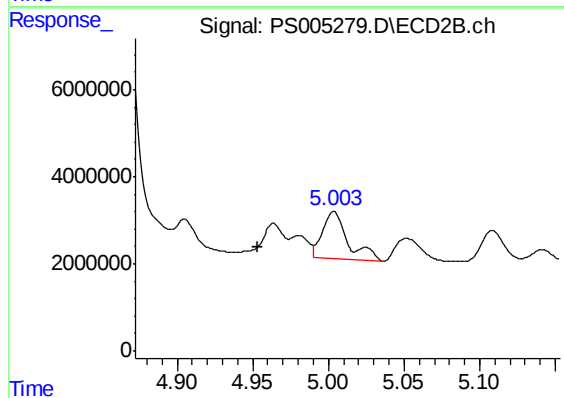

#3 4-Nitrophenol


R.T.: 5.003 min
Delta R.T.: 0.050 min
Response: 12574375
Conc: 25.08 ng/ml

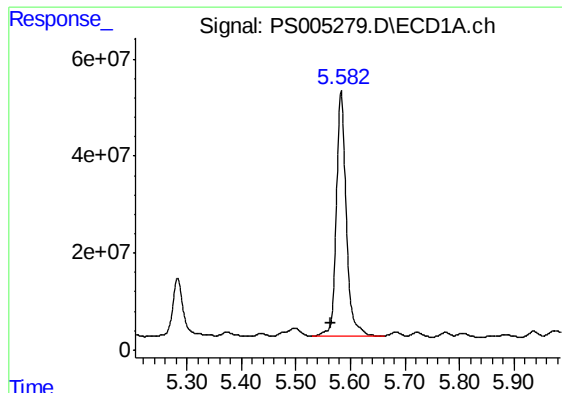

#4 2,4-DCAA


R.T.: 5.583 min
Delta R.T.: 0.019 min
Response: 639877708
Conc: 435.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

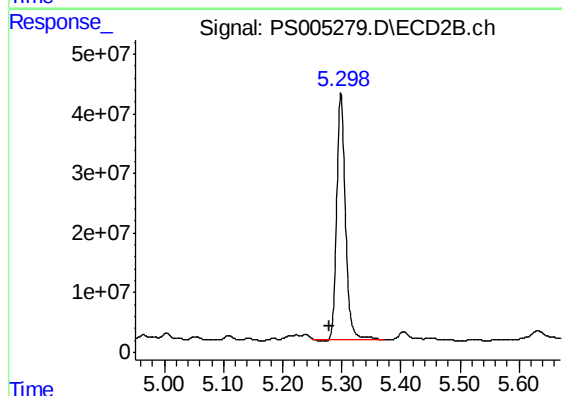


#4 2,4-DCAA

R.T.: 5.299 min
Delta R.T.: 0.019 min
Response: 418815420
Conc: 417.83 ng/ml

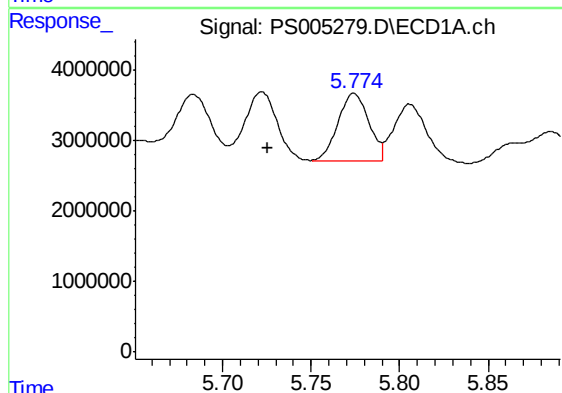


#5 DICAMBA

R.T.: 5.774 min
Delta R.T.: 0.049 min
Response: 11654093
Conc: 2.04 ng/ml

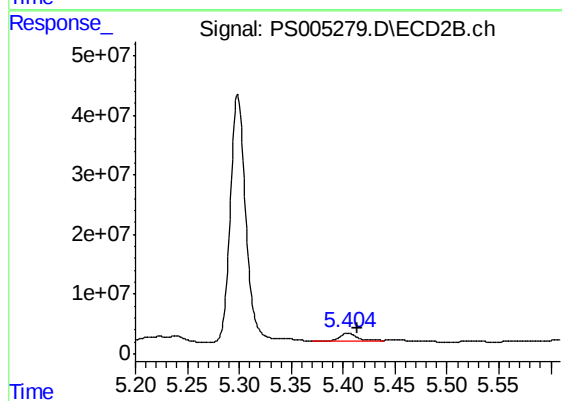

#5 DICAMBA


R.T.: 5.405 min
Delta R.T.: -0.009 min
Response: 13174169
Conc: 3.52 ng/ml

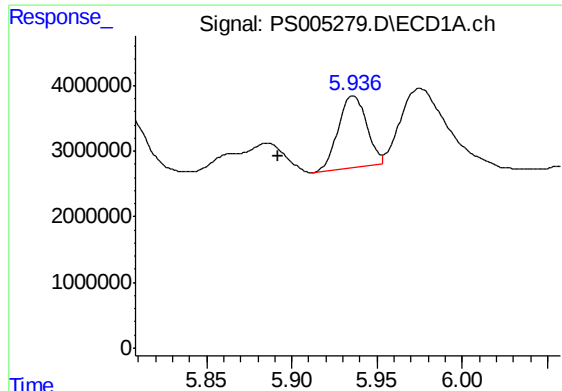

#6 MCPP


R.T.: 5.936 min
Delta R.T.: 0.044 min
Response: 12650743
Conc: 2.89 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

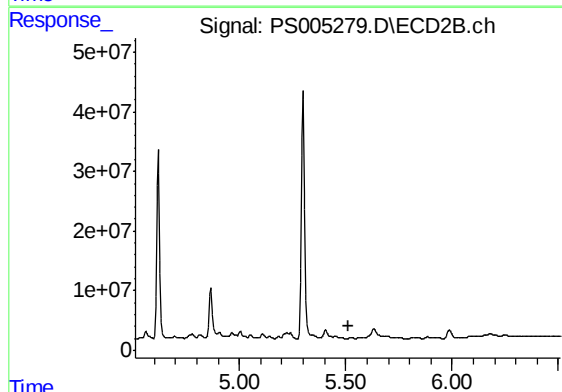


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

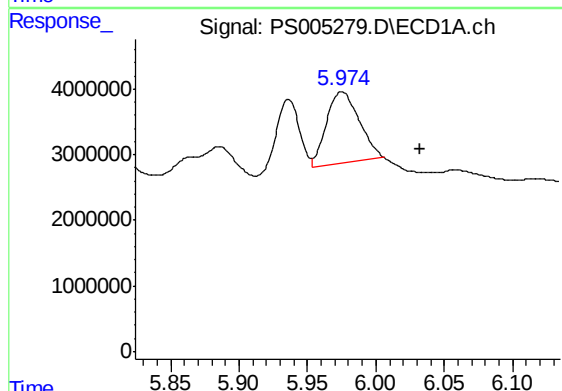


#7 MCPA

R.T.: 5.975 min
Delta R.T.: -0.057 min
Response: 17631020
Conc: 2.81 ug/ml

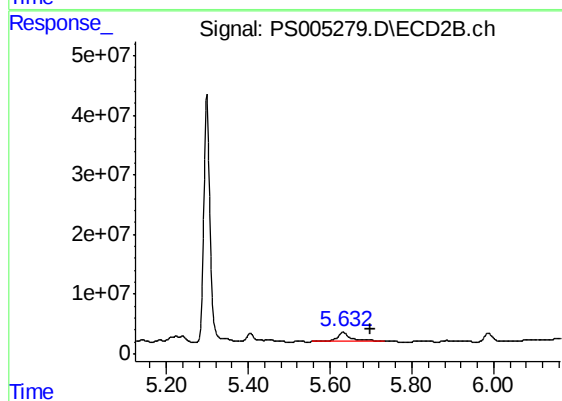

#7 MCPA


R.T.: 5.632 min
Delta R.T.: -0.066 min
Response: 38463011
Conc: 9.50 ug/ml

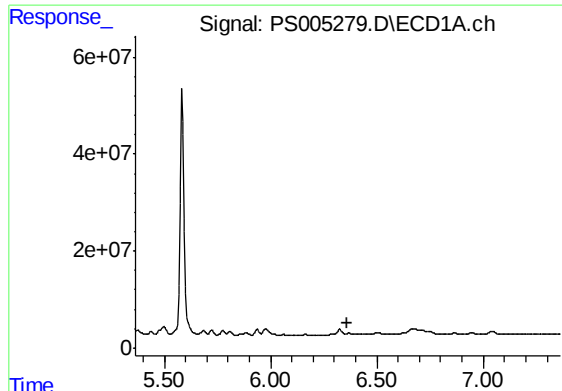

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

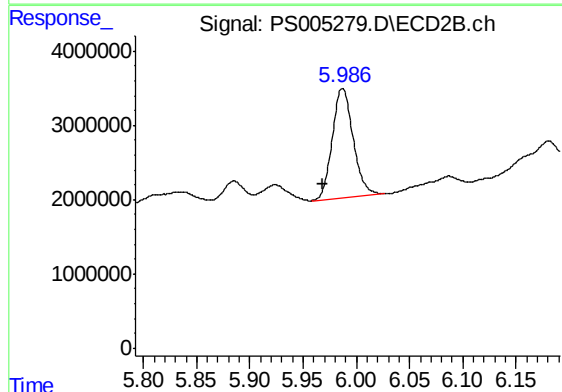


#8 DICHLORPROP

R.T.: 5.987 min
Delta R.T.: 0.018 min
Response: 20106156
Conc: 20.82 ng/ml

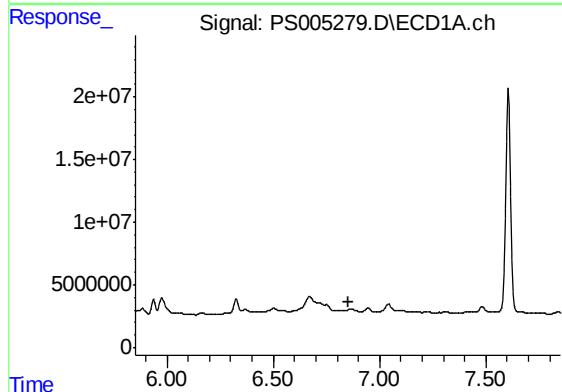


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

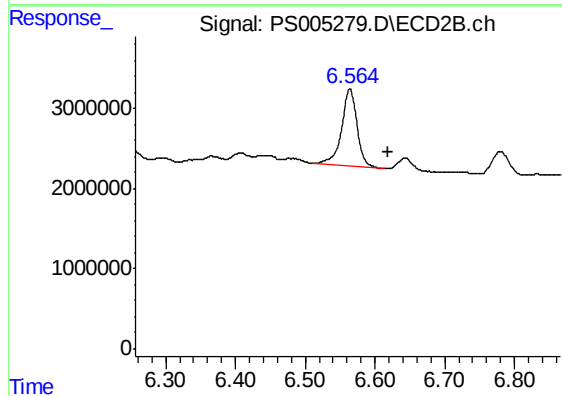

#10 Pentachlorophenol


R.T.: 6.564 min
Delta R.T.: -0.055 min
Response: 14644504
Conc: 1.14 ng/ml

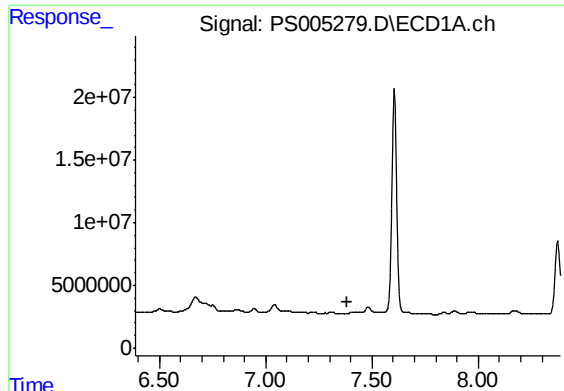

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-C

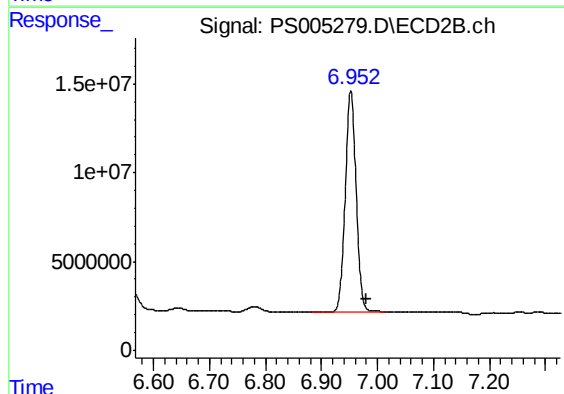


#11 2,4,5-TP (SILVEX)

R.T.: 6.952 min
Delta R.T.: -0.028 min
Response: 167068688
Conc: 31.37 ng/ml

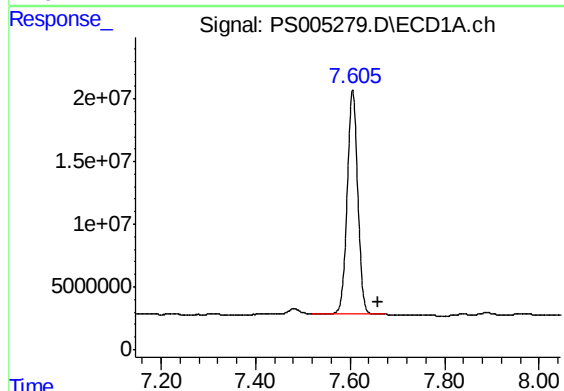

#12 2,4,5-T

R.T.: 7.605 min
Delta R.T.: -0.053 min
Response: 276180165
Conc: 34.32 ng/ml

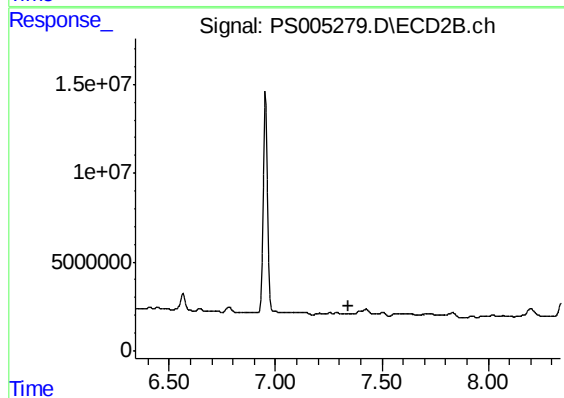

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.