

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 17:50
 Operator : SM\AJ
 Sample : K3157-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CL-02-062619-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 18:27:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.583	5.299	737.6E6	485.7E6	502.466	484.549
Target Compounds							
2) T	3,5-DICHL...	0.000	4.618	0	291.9E6	N.D.	221.370
3) T	4-Nitroph...	5.375	0.000	8129860	0	11.225	N.D. #
5) T	DICAMBA	0.000	5.406	0	14064558	N.D.	3.757
6) T	MCP	5.937	0.000	13649017	0	3.118	N.D. #
7) T	MCPA	5.977	5.633	13194374	35204022	2.101	8.691 #
8) T	DICHLORPROP	0.000	5.988	0	17459879	N.D.	18.083
10) T	Pentachlo...	0.000	6.565	0	15606149	N.D.	1.214
11) T	2,4,5-TP ...	0.000	6.953	0	175.3E6	N.D.	32.920
12) T	2,4,5-T	7.607	0.000	290.5E6	0	36.093	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 17:50
Operator : SM\AJ
Sample : K3157-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 18:27:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

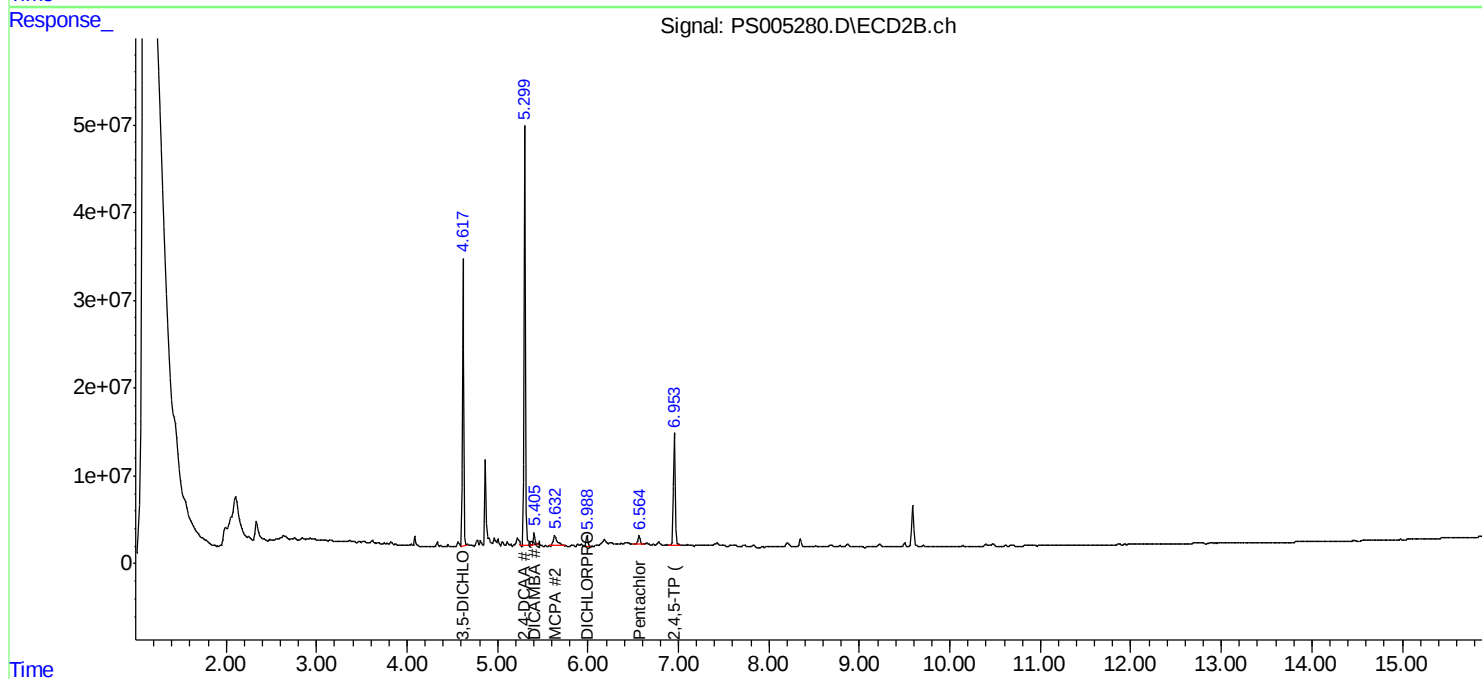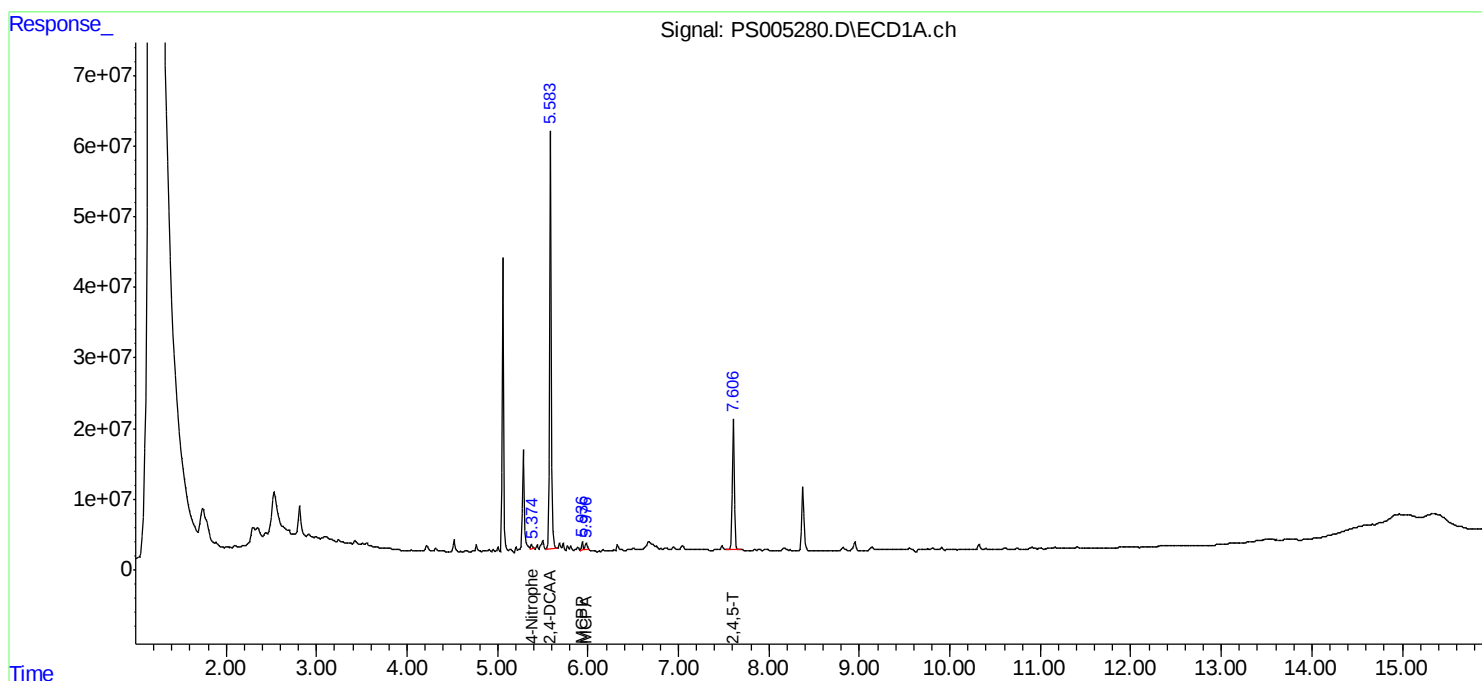


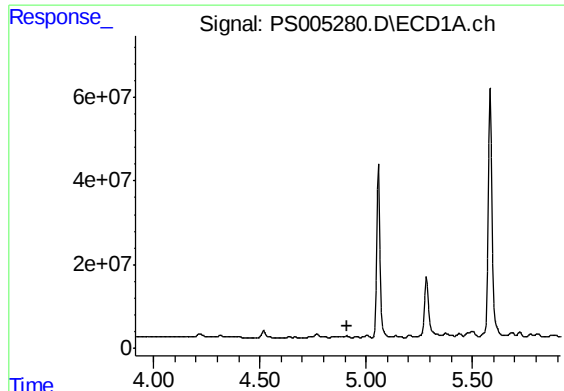

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

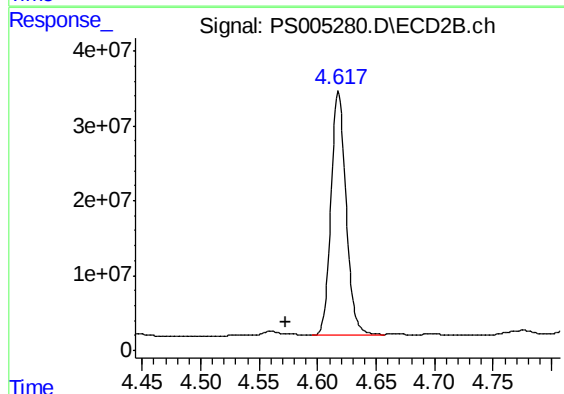


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.618 min
Delta R.T.: 0.045 min
Response: 291922072
Conc: 221.37 ng/ml

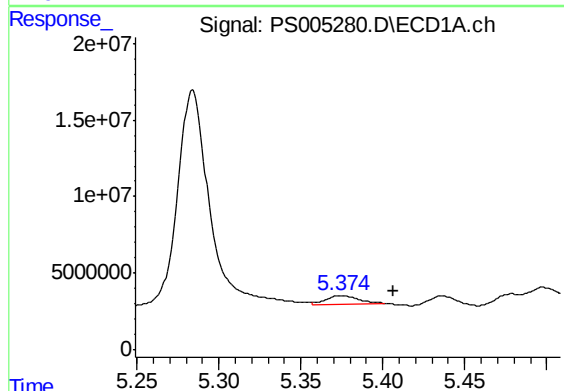


#3 4-Nitrophenol

R.T.: 5.375 min
Delta R.T.: -0.031 min
Response: 8129860
Conc: 11.22 ng/ml

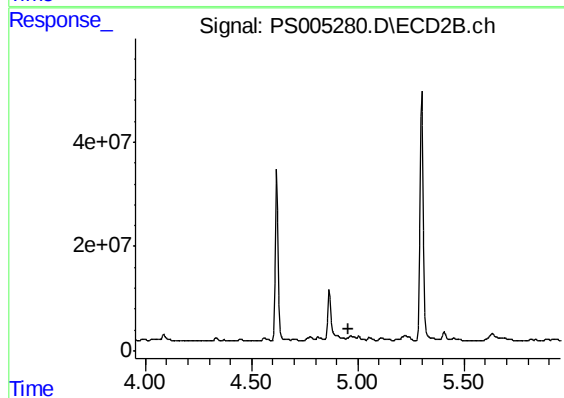

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

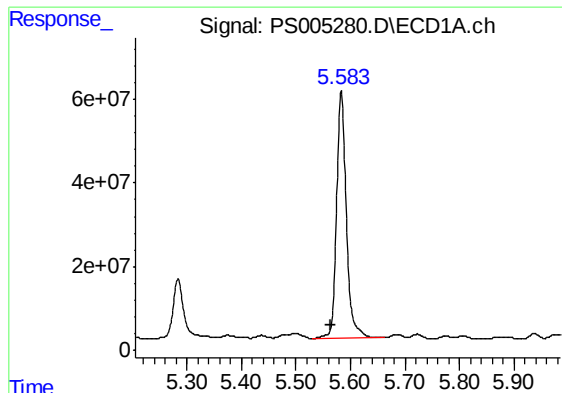

#4 2,4-DCAA


R.T.: 5.583 min
Delta R.T.: 0.020 min
Response: 737566995
Conc: 502.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

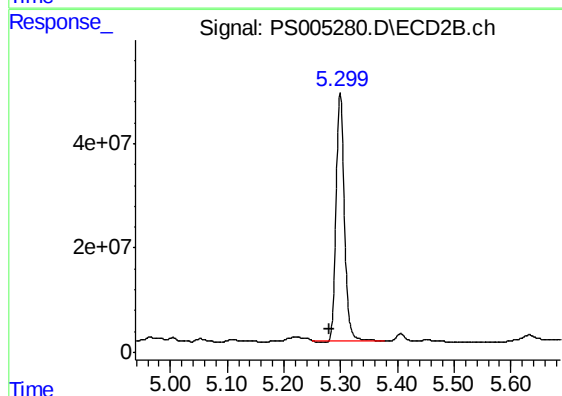


#4 2,4-DCAA

R.T.: 5.299 min
Delta R.T.: 0.020 min
Response: 485696745
Conc: 484.55 ng/ml

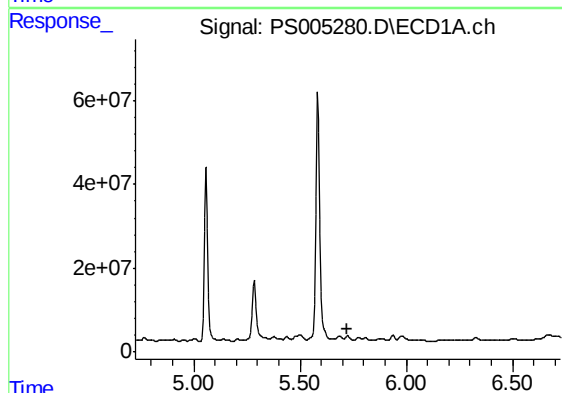


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

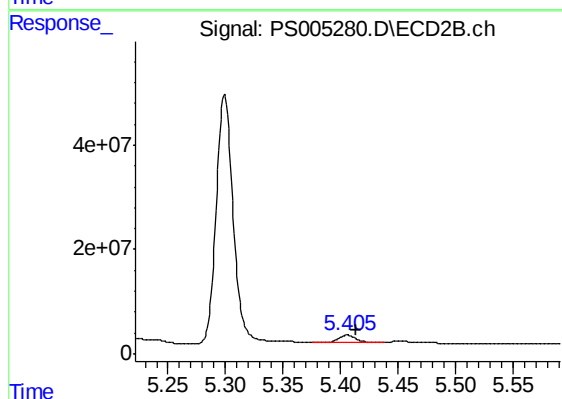

#5 DICAMBA


R.T.: 5.406 min
Delta R.T.: -0.008 min
Response: 14064558
Conc: 3.76 ng/ml

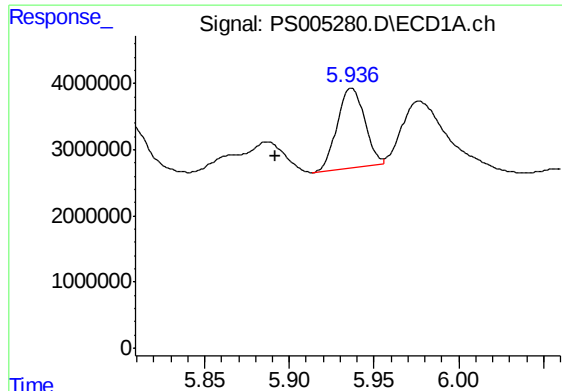

#6 MCPP


R.T.: 5.937 min
Delta R.T.: 0.045 min
Response: 13649017
Conc: 3.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

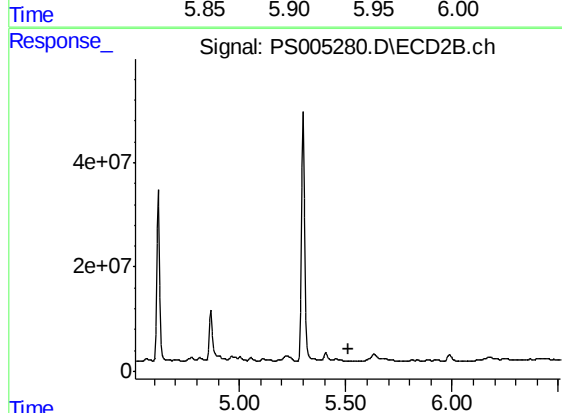


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

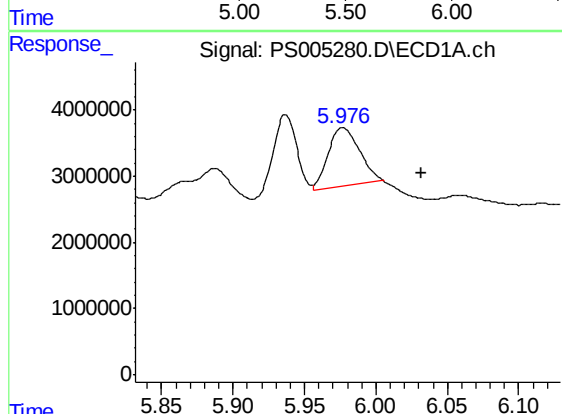


#7 MCPA

R.T.: 5.977 min
Delta R.T.: -0.055 min
Response: 13194374
Conc: 2.10 ug/ml

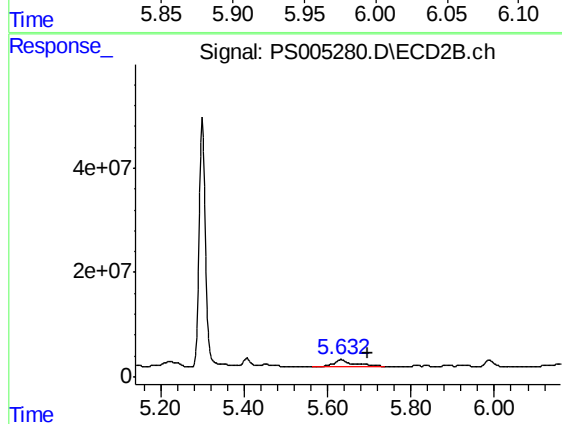

#7 MCPA


R.T.: 5.633 min
Delta R.T.: -0.065 min
Response: 35204022
Conc: 8.69 ug/ml

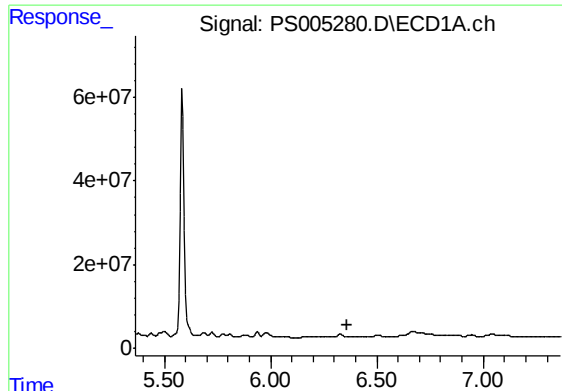

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

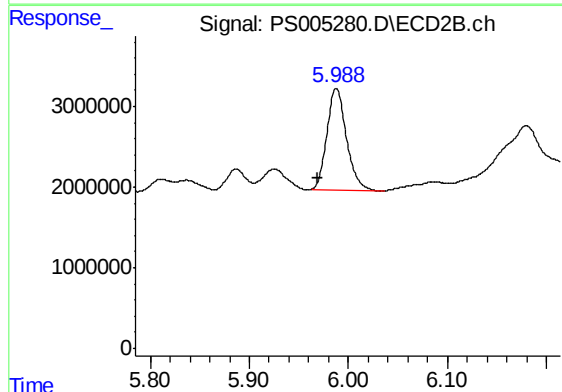


#8 DICHLORPROP

R.T.: 5.988 min
Delta R.T.: 0.019 min
Response: 17459879
Conc: 18.08 ng/ml

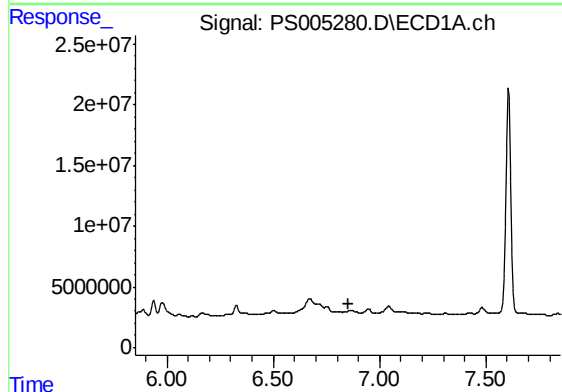


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

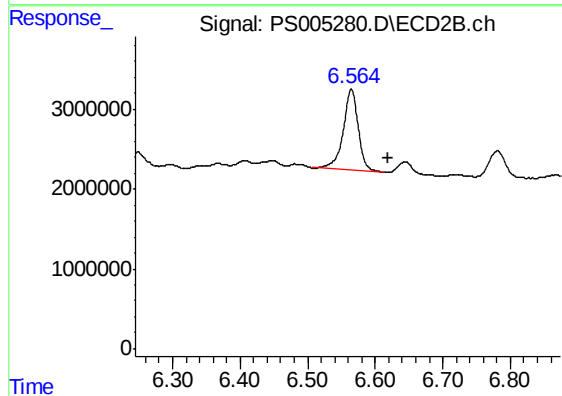

#10 Pentachlorophenol


R.T.: 6.565 min
Delta R.T.: -0.054 min
Response: 15606149
Conc: 1.21 ng/ml

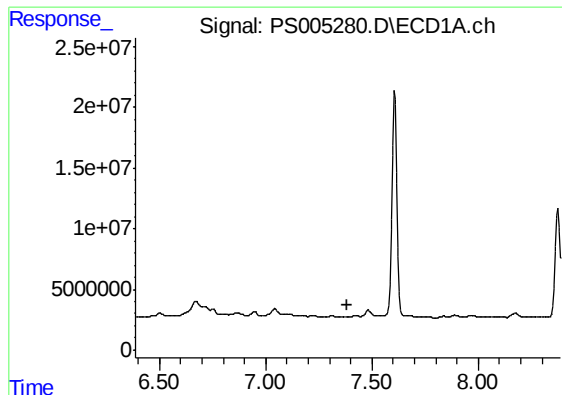

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CL-02-062619-D

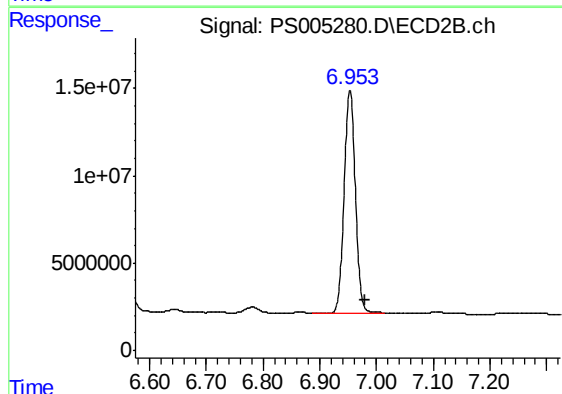


#11 2,4,5-TP (SILVEX)

R.T.: 6.953 min
Delta R.T.: -0.027 min
Response: 175309309
Conc: 32.92 ng/ml

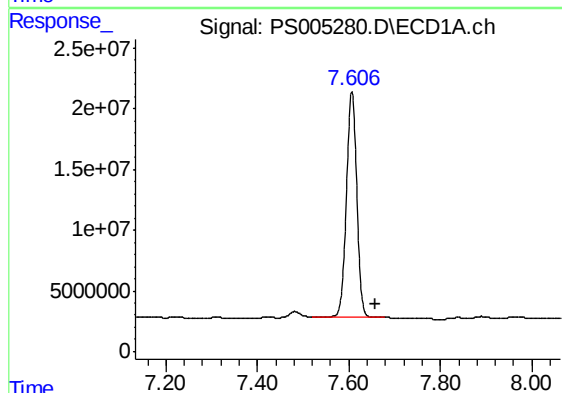

#12 2,4,5-T

R.T.: 7.607 min
Delta R.T.: -0.052 min
Response: 290471719
Conc: 36.09 ng/ml

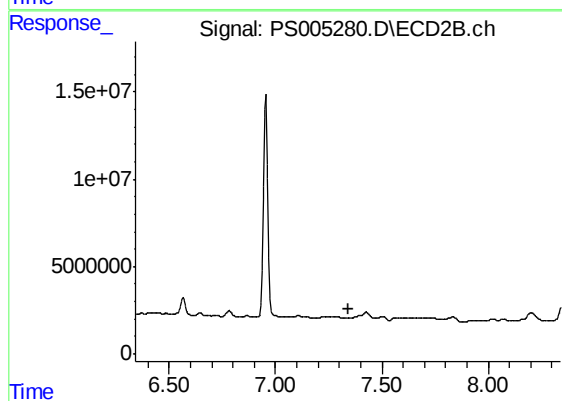

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.