

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 20:46
 Operator : SM\AJ
 Sample : K3509-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SA-06-062619-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 22:48:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.283	695.3E6	482.2E6	473.705	481.013
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0	221.6E6	N.D.	168.080
5) T	DICAMBA	0.000	5.389	0	15315940	N.D.	4.092
6) T	MCP	5.921	0.000	10557597	0	2.412	N.D. #
8) T	DICHLORPROP	0.000	5.972	0	22652697	N.D.	23.461
11) T	2,4,5-TP ...	0.000	6.936	0	163.0E6	N.D.	30.601
12) T	2,4,5-T	7.589	0.000	270.4E6	0	33.594	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 20:46
Operator : SM\AJ
Sample : K3509-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SA-06-062619-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 22:48:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

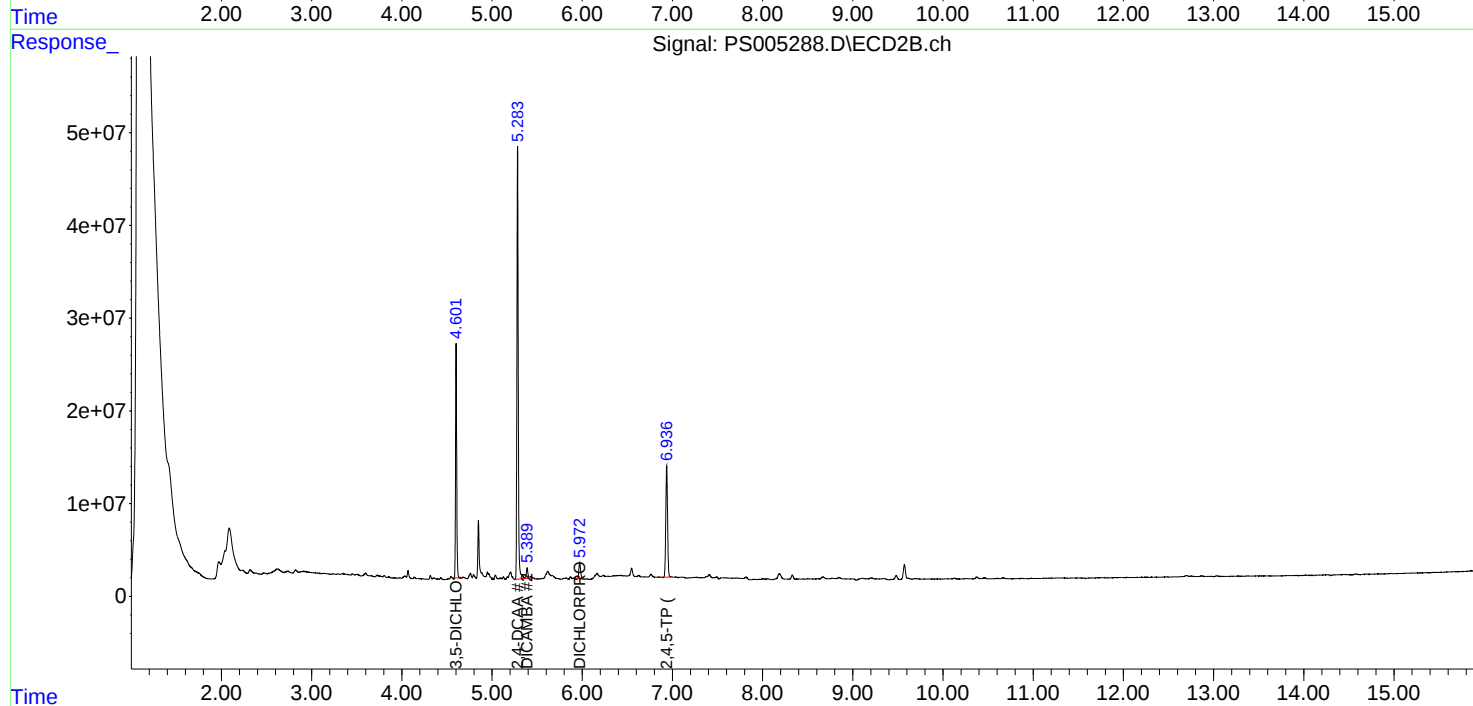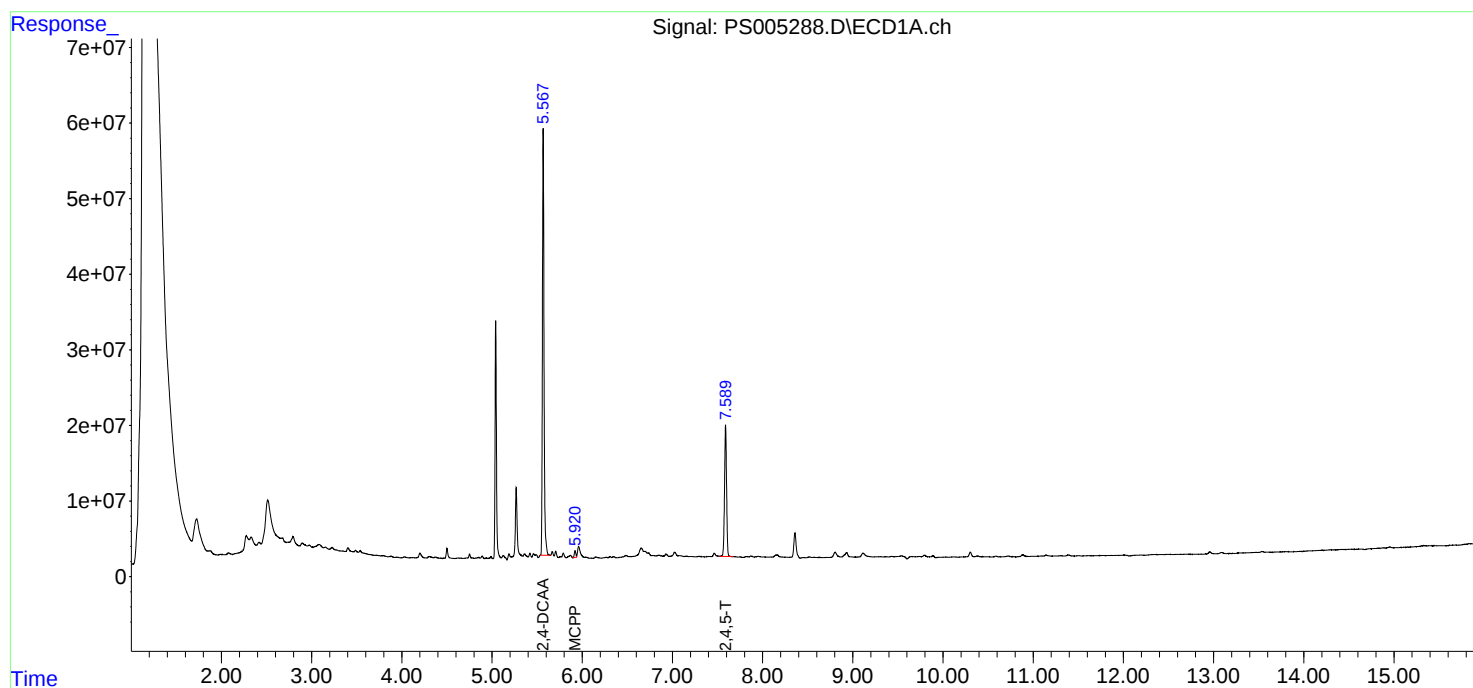


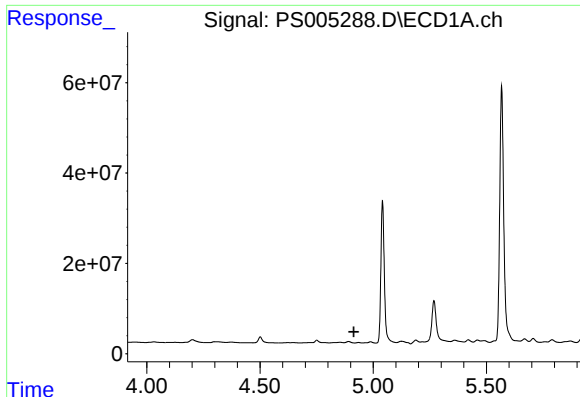

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SA-06-062619-A

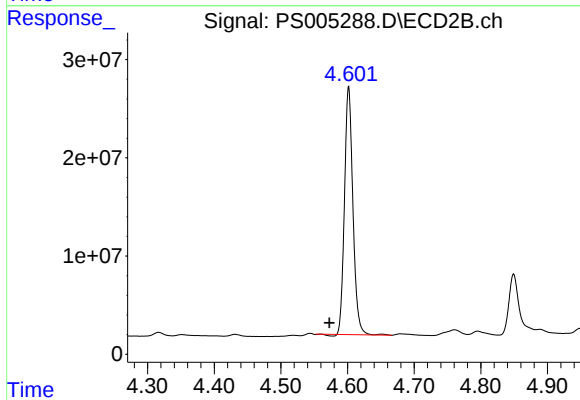


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.029 min
Response: 221648954
Conc: 168.08 ng/ml

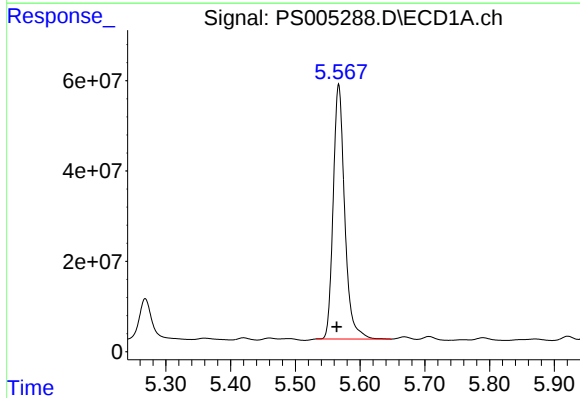


#4 2,4-DCAA

R.T.: 5.567 min
Delta R.T.: 0.003 min
Response: 695348566
Conc: 473.71 ng/ml

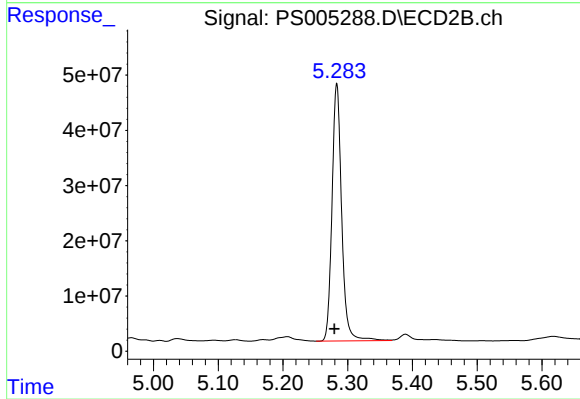

#4 2,4-DCAA


R.T.: 5.283 min
Delta R.T.: 0.004 min
Response: 482152174
Conc: 481.01 ng/ml

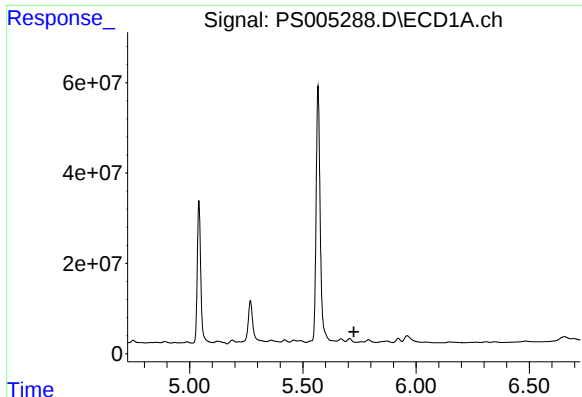

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SA-06-062619-A

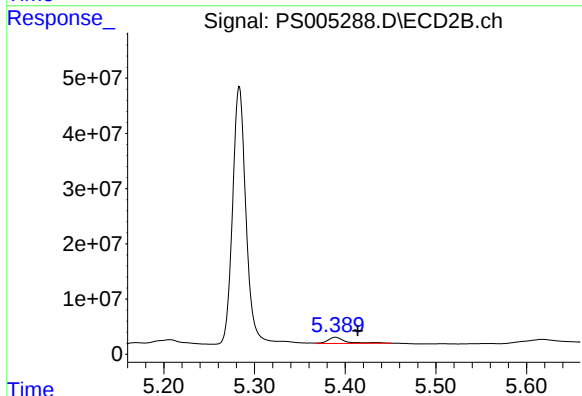


#5 DICAMBA

R.T.: 5.389 min
Delta R.T.: -0.025 min
Response: 15315940
Conc: 4.09 ng/ml

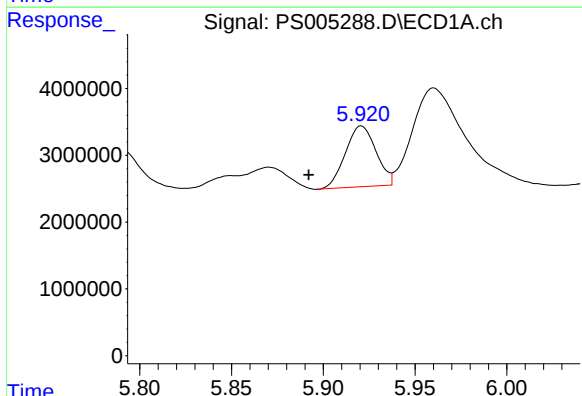


#6 MCP

R.T.: 5.921 min
Delta R.T.: 0.029 min
Response: 10557597
Conc: 2.41 ug/ml

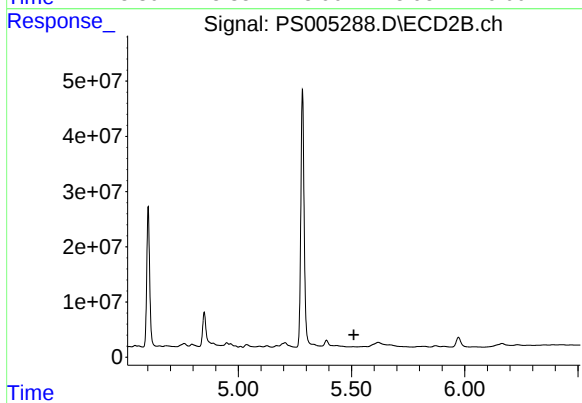

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

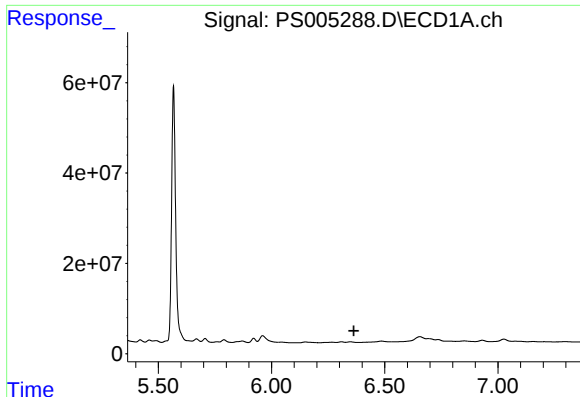

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SA-06-062619-A

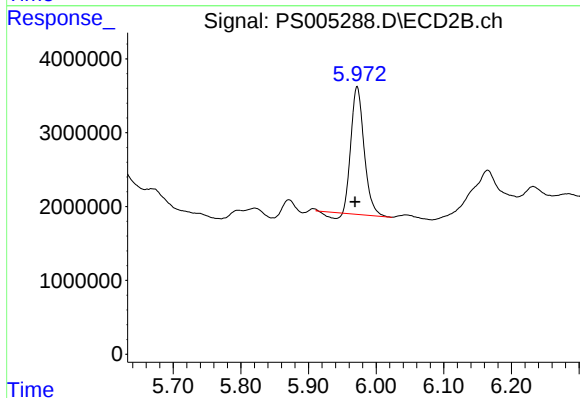


#8 DICHLORPROP

R.T.: 5.972 min
Delta R.T.: 0.003 min
Response: 22652697
Conc: 23.46 ng/ml

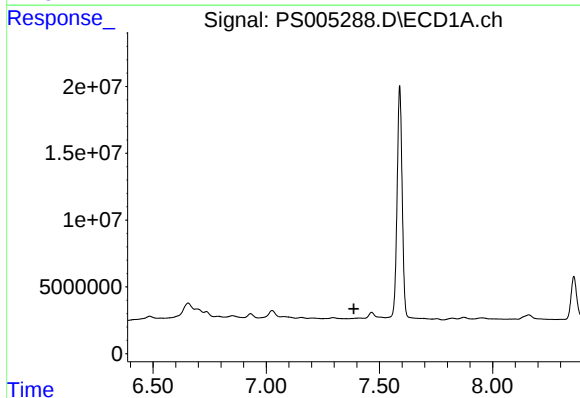


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

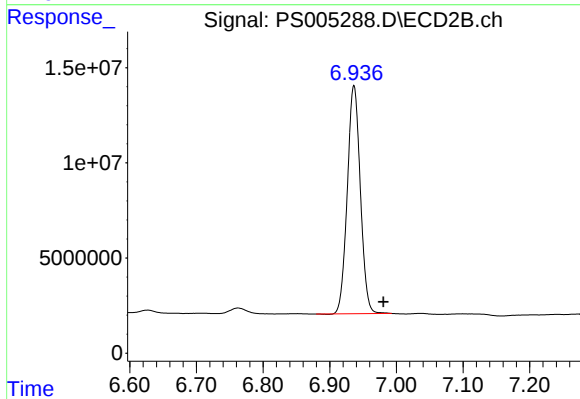

#11 2,4,5-TP (SILVEX)


R.T.: 6.936 min
Delta R.T.: -0.044 min
Response: 162956885
Conc: 30.60 ng/ml

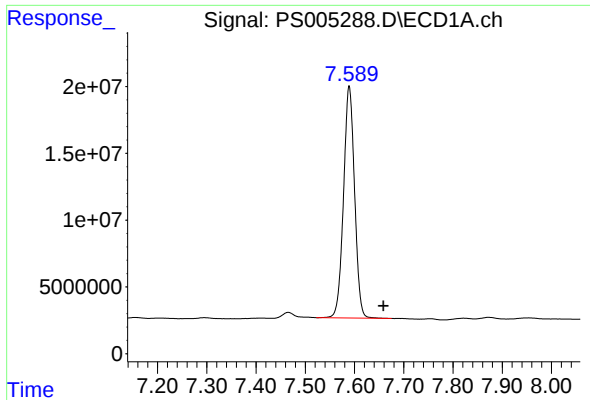

#12 2,4,5-T

R.T.: 7.589 min
Delta R.T.: -0.069 min
Response: 270358164
Conc: 33.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
SA-06-062619-A

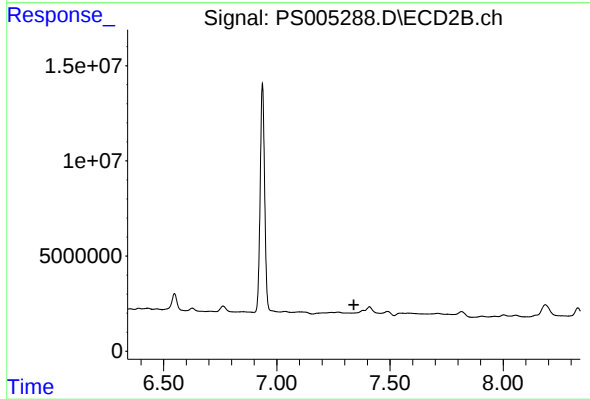

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.