

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 22:36
 Operator : SM\AJ
 Sample : K3532-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SY-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 23:40:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.300	537.0E6	343.0E6	365.825	342.218
Target Compounds							
1) T	Dalapon	2.093	0.000	45663430	0	24.773	N.D. #
2) T	3,5-DICHL...	0.000	4.577	0	14825364	N.D.	11.242
3) T	4-Nitroph...	5.376	0.000	10090578	0	13.932	N.D. #
5) T	DICAMBA	0.000	5.406	0	17531875	N.D.	4.684
6) T	MCPD	5.937	0.000	12418939	0	2.837	N.D. #
7) T	MCPA	5.973	5.634	19770102	15401439	3.148	3.802
8) T	DICHLORPROP	0.000	5.986	0	14006660	N.D.	14.507
10) T	Pentachlo...	0.000	6.564	0	20559452	N.D.	1.599
11) T	2,4,5-TP ...	0.000	6.952	0	187.9E6	N.D.	35.290
12) T	2,4,5-T	7.607	0.000	280.2E6	0	34.819	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 22:36
Operator : SM\AJ
Sample : K3532-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SY-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 23:40:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

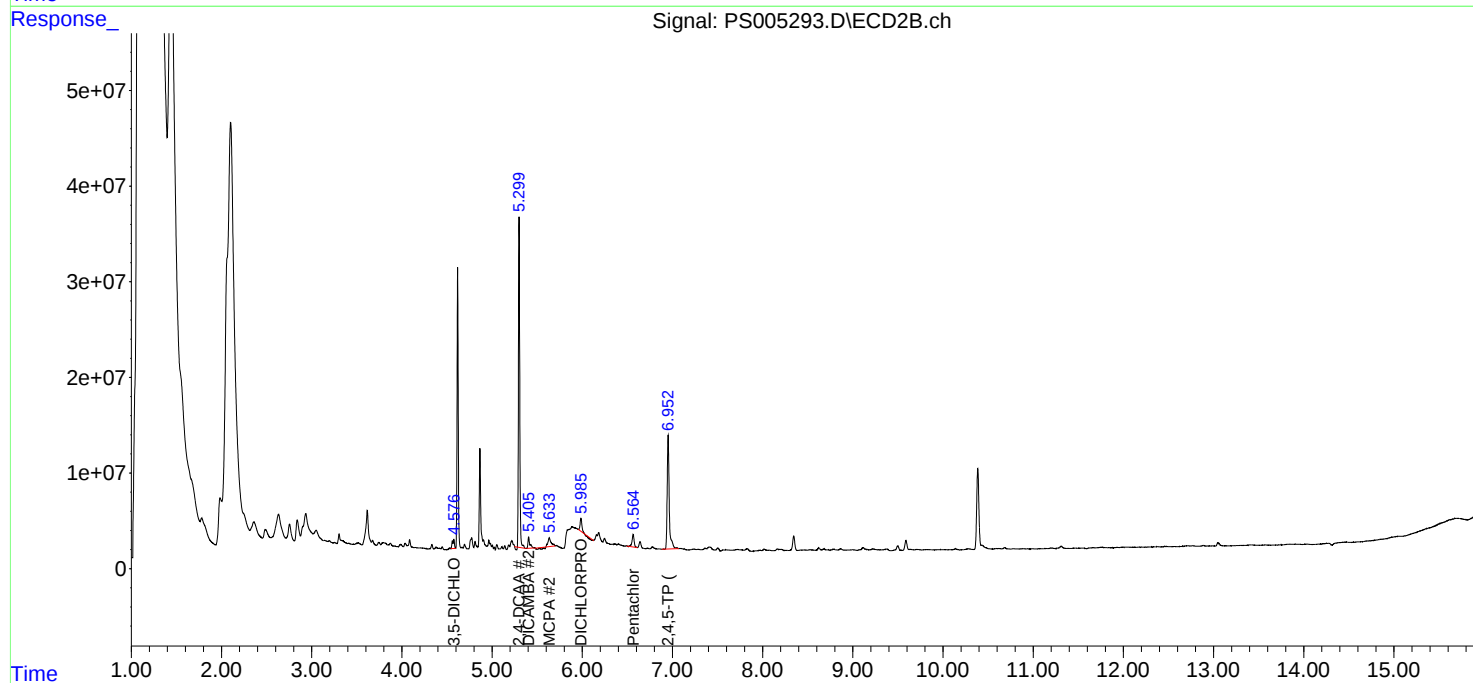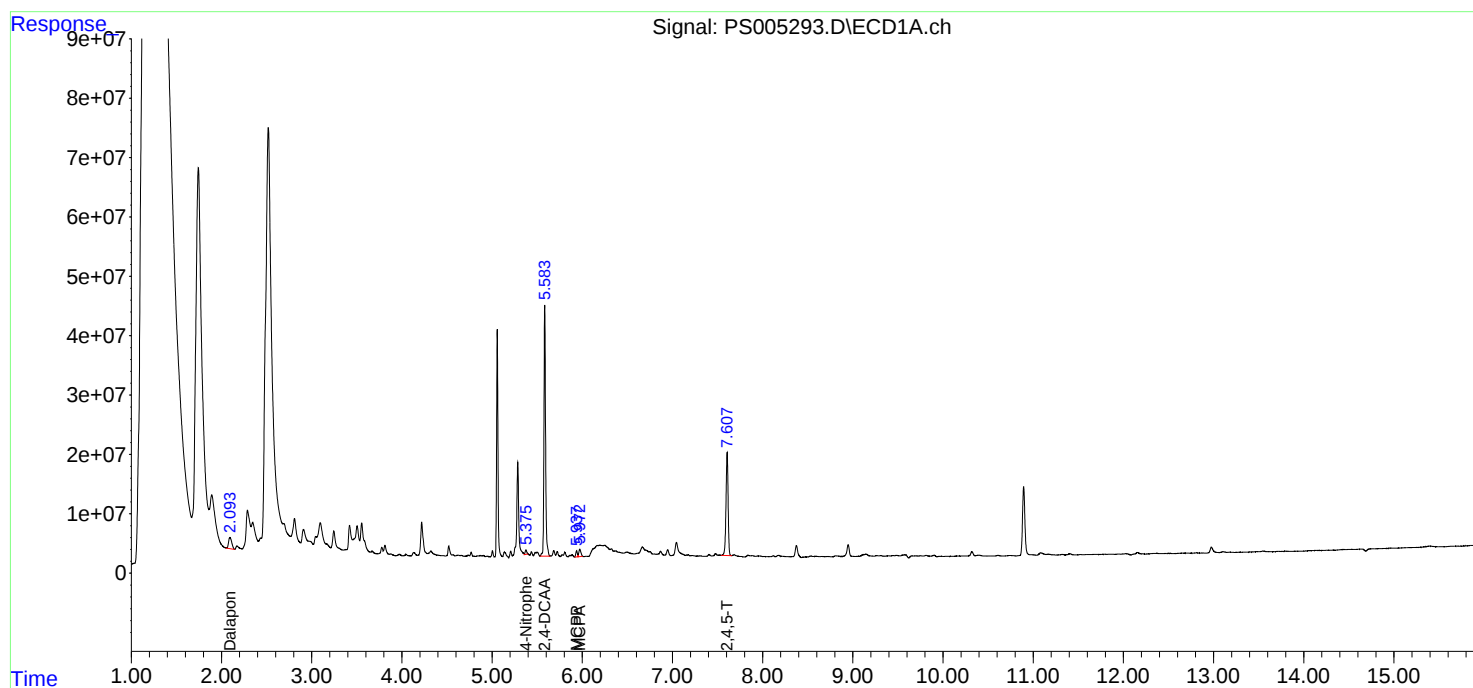


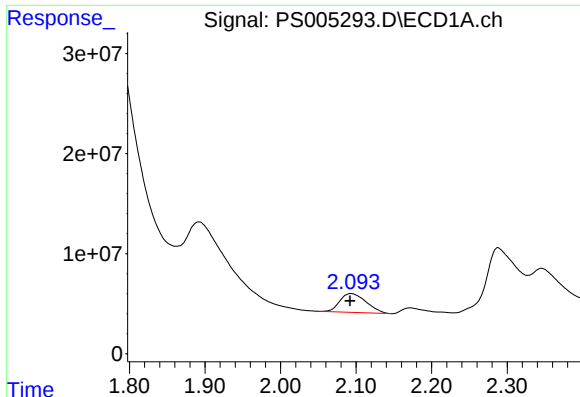

#1 Dalapon


R.T.: 2.093 min
Delta R.T.: 0.001 min
Response: 45663430
Conc: 24.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
SY-6

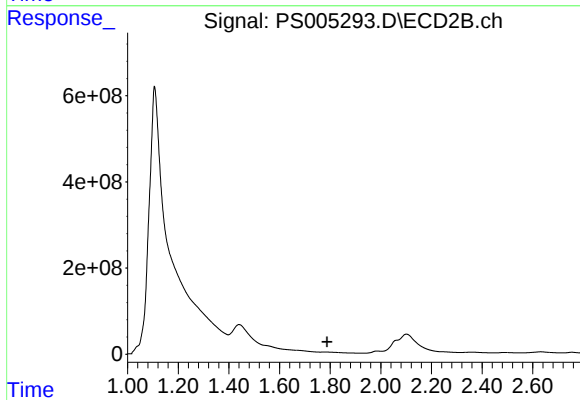


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

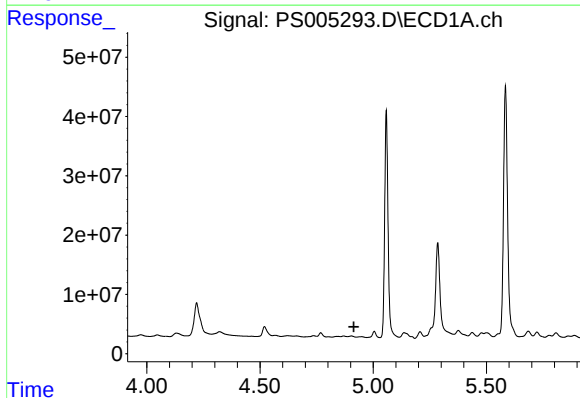


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

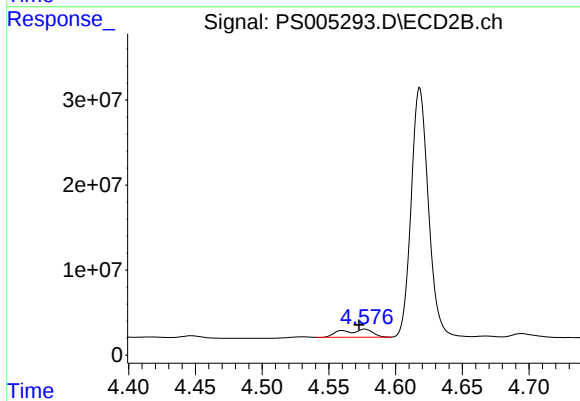

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.577 min
Delta R.T.: 0.004 min
Response: 14825364
Conc: 11.24 ng/ml

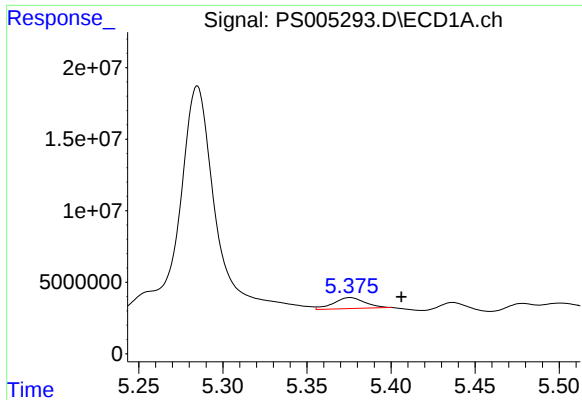

#3 4-Nitrophenol


R.T.: 5.376 min
Delta R.T.: -0.031 min
Response: 10090578
Conc: 13.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
SY-6

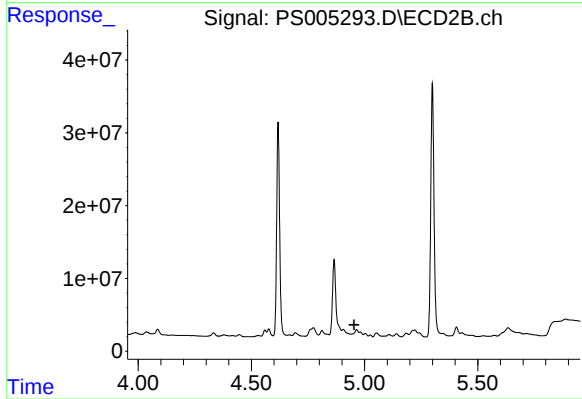


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

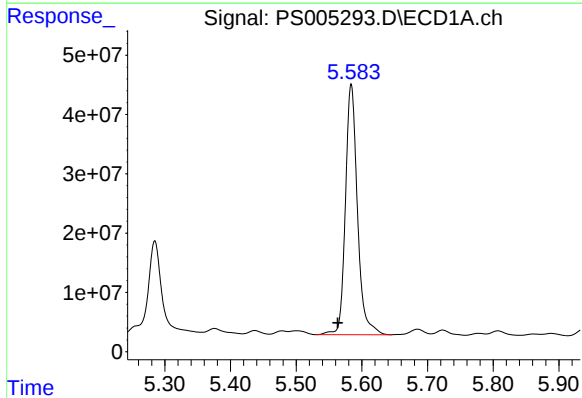


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.020 min
Response: 536992344
Conc: 365.83 ng/ml

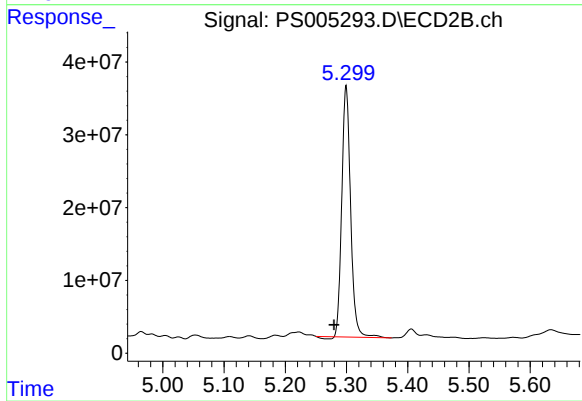

#4 2,4-DCAA


R.T.: 5.300 min
Delta R.T.: 0.020 min
Response: 343028952
Conc: 342.22 ng/ml

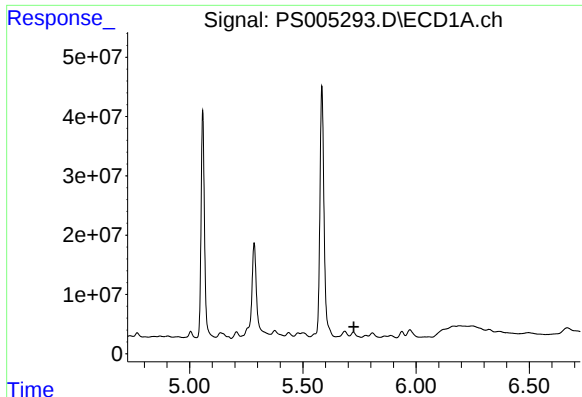

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SY-6

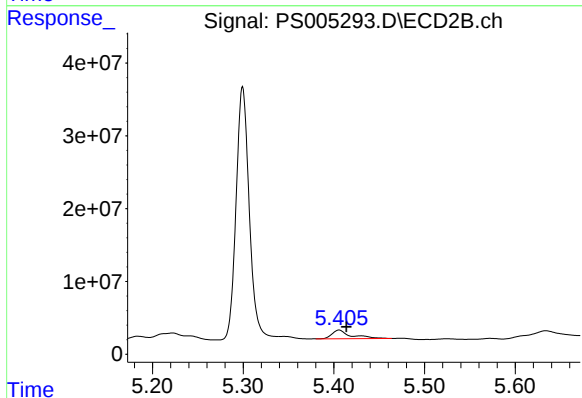


#5 DICAMBA

R.T.: 5.406 min
Delta R.T.: -0.008 min
Response: 17531875
Conc: 4.68 ng/ml

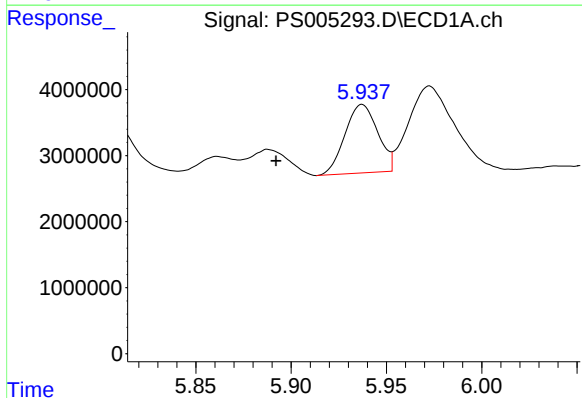


#6 MCPP

R.T.: 5.937 min
Delta R.T.: 0.045 min
Response: 12418939
Conc: 2.84 ug/ml

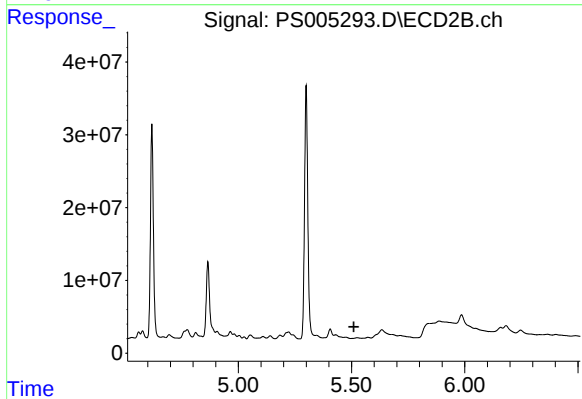

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

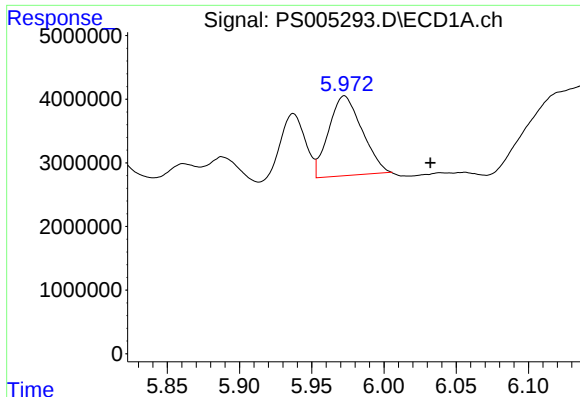

#7 MCPA


R.T.: 5.973 min
Delta R.T.: -0.059 min
Response: 19770102
Conc: 3.15 ug/ml

Instrument :
ECD_S
ClientSampleId :
SY-6

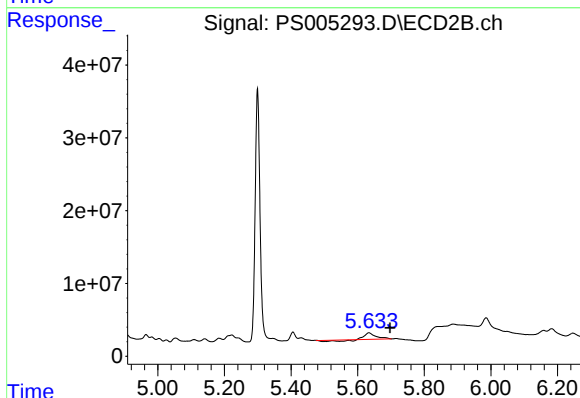


#7 MCPA

R.T.: 5.634 min
Delta R.T.: -0.064 min
Response: 15401439
Conc: 3.80 ug/ml

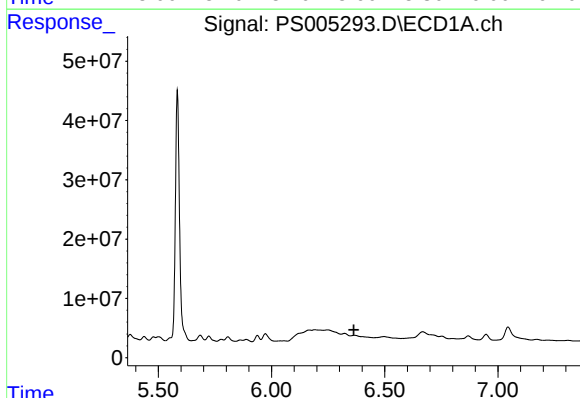


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

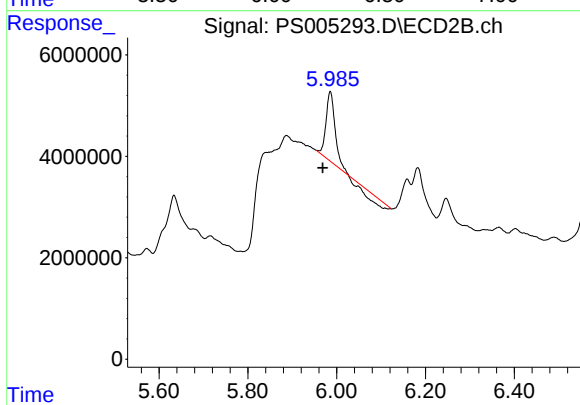

#8 DICHLORPROP


R.T.: 5.986 min
Delta R.T.: 0.017 min
Response: 14006660
Conc: 14.51 ng/ml

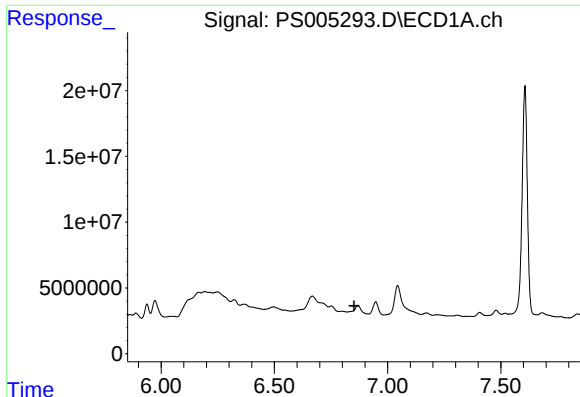

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SY-6

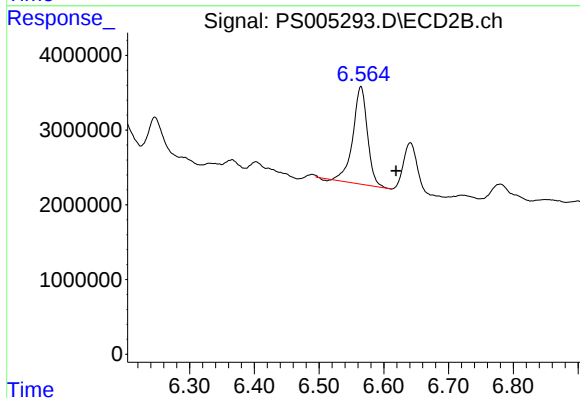


#10 Pentachlorophenol

R.T.: 6.564 min
Delta R.T.: -0.055 min
Response: 20559452
Conc: 1.60 ng/ml

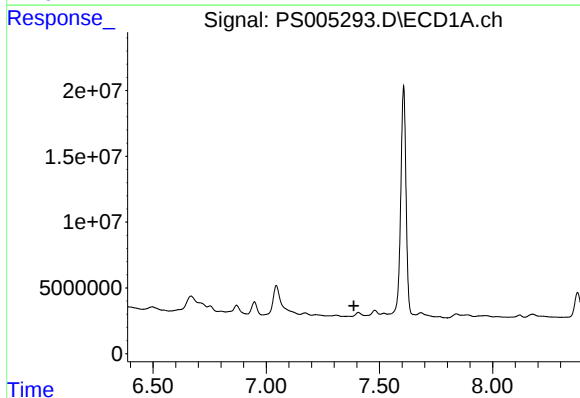


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

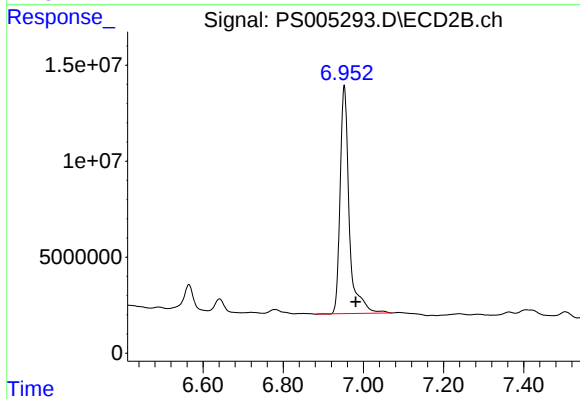

#11 2,4,5-TP (SILVEX)


R.T.: 6.952 min
Delta R.T.: -0.028 min
Response: 187929244
Conc: 35.29 ng/ml

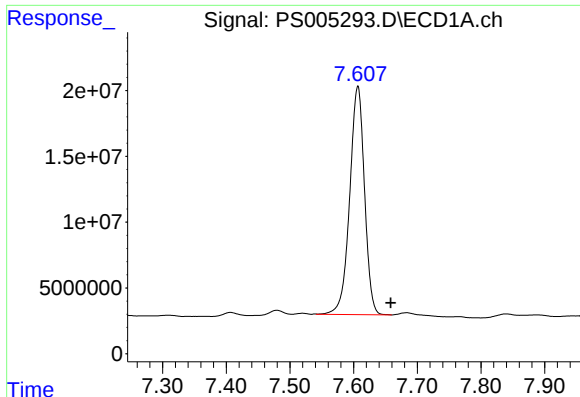

#12 2,4,5-T

R.T.: 7.607 min
Delta R.T.: -0.052 min
Response: 280221606
Conc: 34.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
SY-6

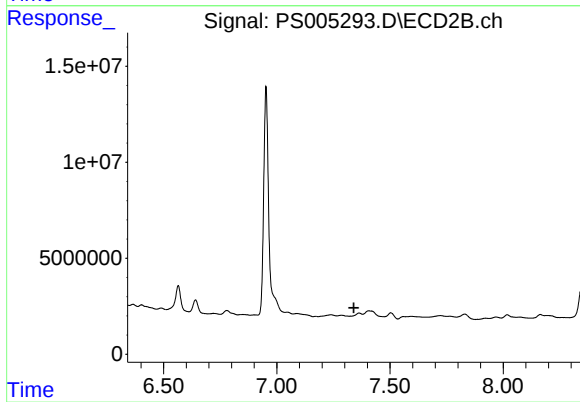

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.