

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
 Data File : PS005271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2019 12:56
 Operator : SM\AJ
 Sample : K3534-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-PS-01-050

Manual Integrations
 APPROVED

Ankita
 7/1/2019 10:06:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 16:26:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.547	5.282	355.4E6	229.7E6	242.136m	229.120
------	----------	-------	-------	---------	---------	----------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062819\
Data File : PS005271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2019 12:56
Operator : SM\AJ
Sample : K3534-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-PS-01-050


Manual Integrations
APPROVED

Ankita
7/1/2019 10:06:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 16:26:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

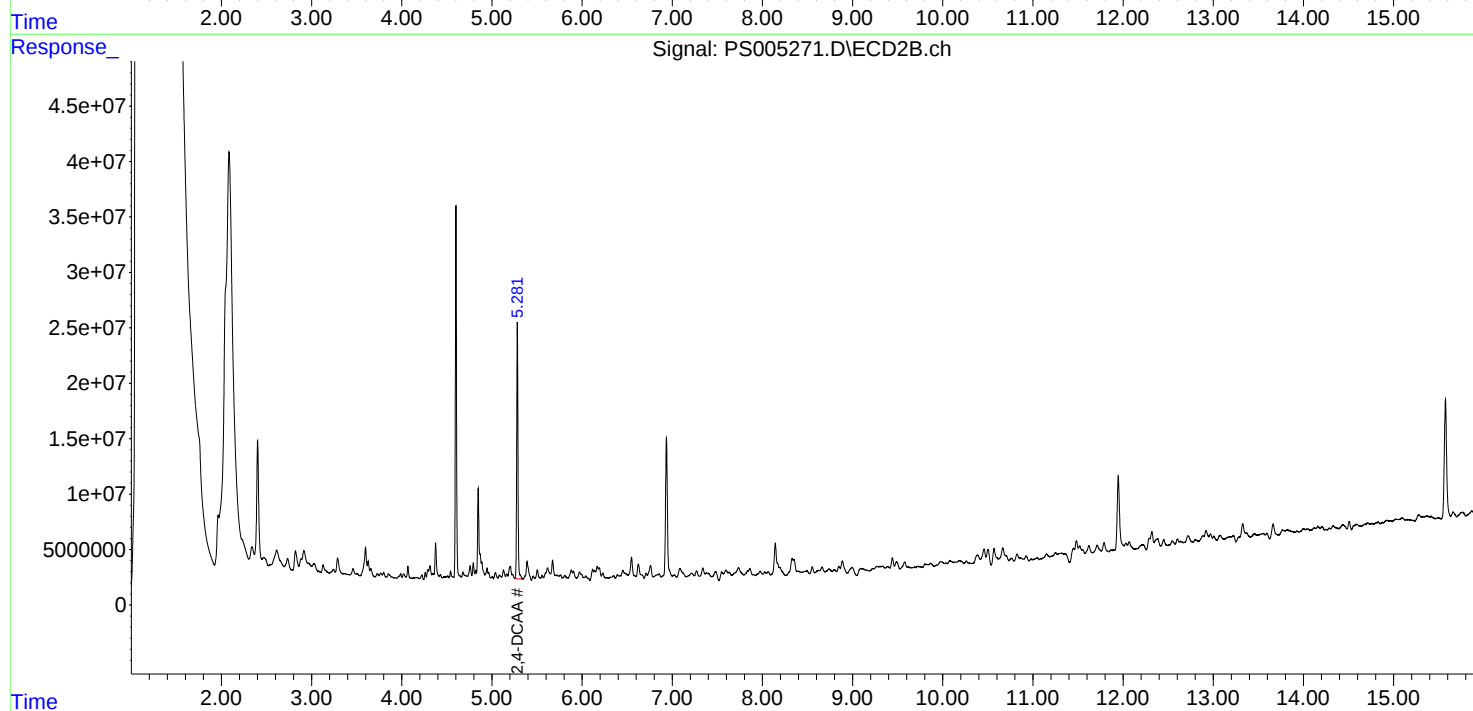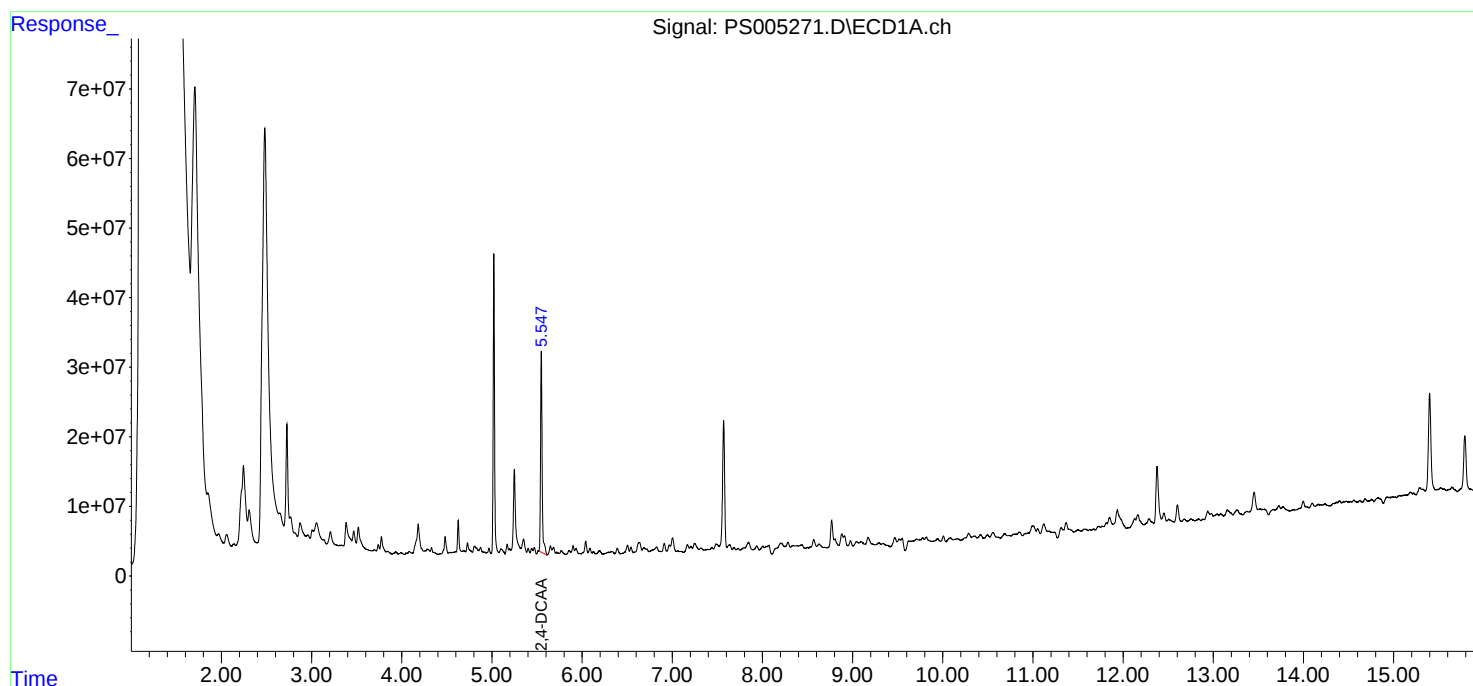

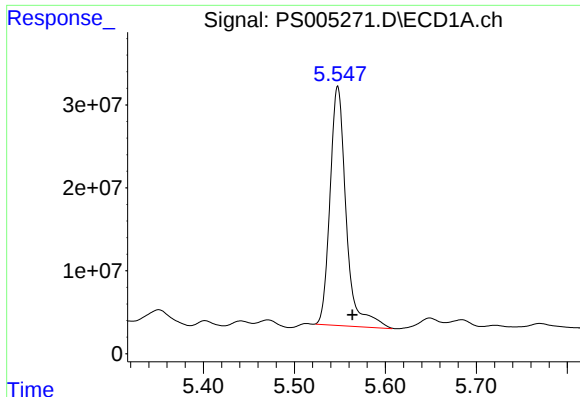


#4 2,4-DCAA

R.T.: 5.547 min
Delta R.T.: -0.016 min
Response: 355429916
Conc: 242.14 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-PS-01-050

Manual Integrations
APPROVED

Ankita
7/1/2019 10:06:28 AM

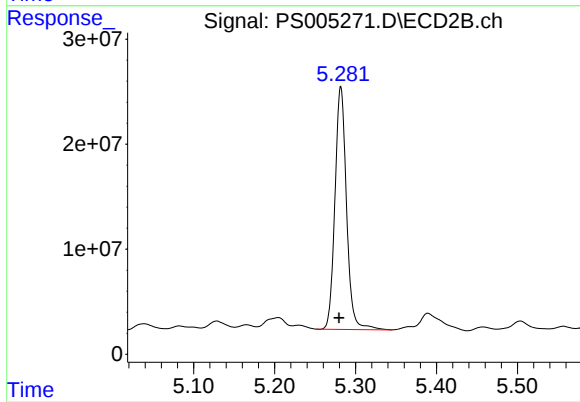

#4 2,4-DCAA

R.T.: 5.282 min
Delta R.T.: 0.002 min
Response: 229663010
Conc: 229.12 ng/ml