

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
 Data File : PS005314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 19:52
 Operator : SM\AJ
 Sample : K3554-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:00:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.569	5.285	1088.4E6	733.6E6	741.463	731.890
Target Compounds							
2) T	3,5-DICHL...	0.000	4.604	0	231.4E6	N.D.	175.495
5) T	DICAMBA	0.000	5.391	0	19782425	N.D.	5.285
6) T	MCP	5.923	0.000	9070738	0	2.072	N.D. #
8) T	DICHLORPROP	6.309	5.974	24418934	11911612	17.075	12.337 #
10) T	Pentachlo...	0.000	6.551	0	13997994	N.D.	1.089
11) T	2,4,5-TP ...	0.000	6.938	0	130.7E6	N.D.	24.542
12) T	2,4,5-T	7.592	0.000	219.8E6	0	27.309	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
Data File : PS005314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 19:52
Operator : SM\AJ
Sample : K3554-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SAMPLE-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:00:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

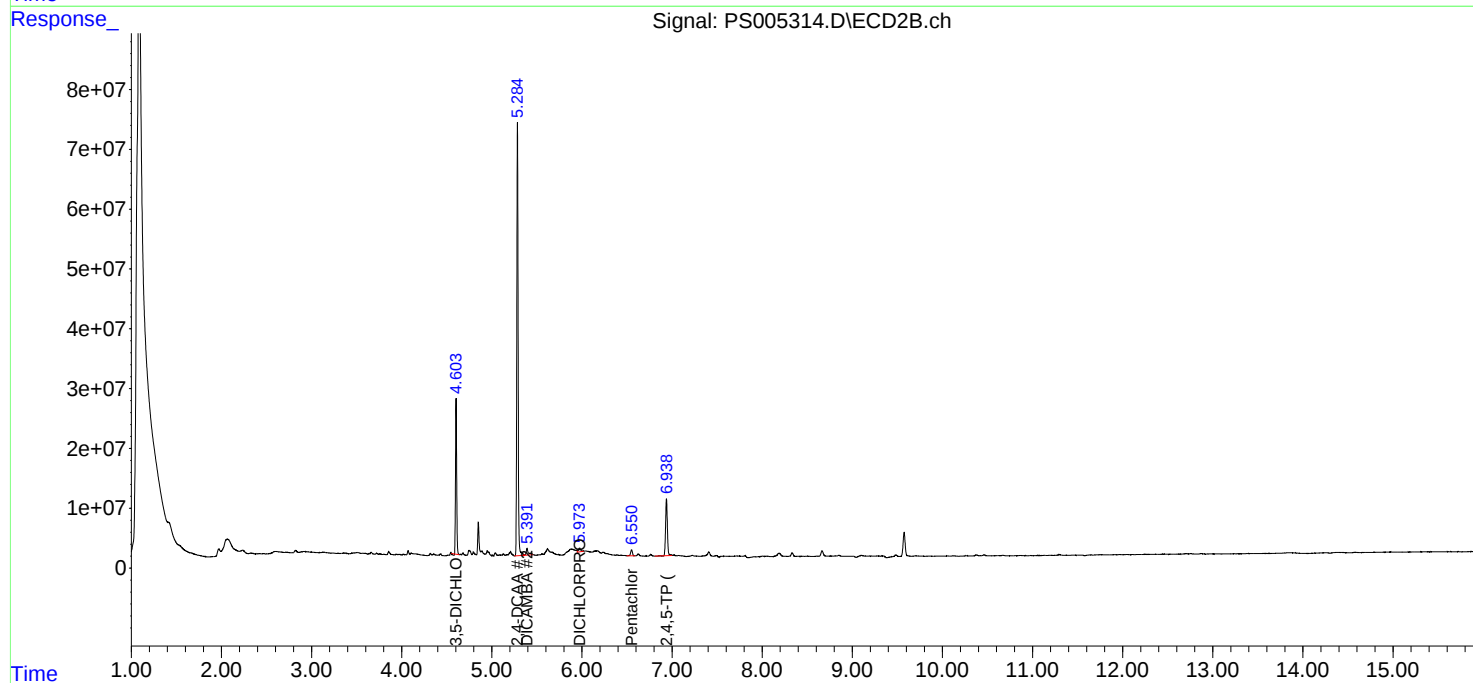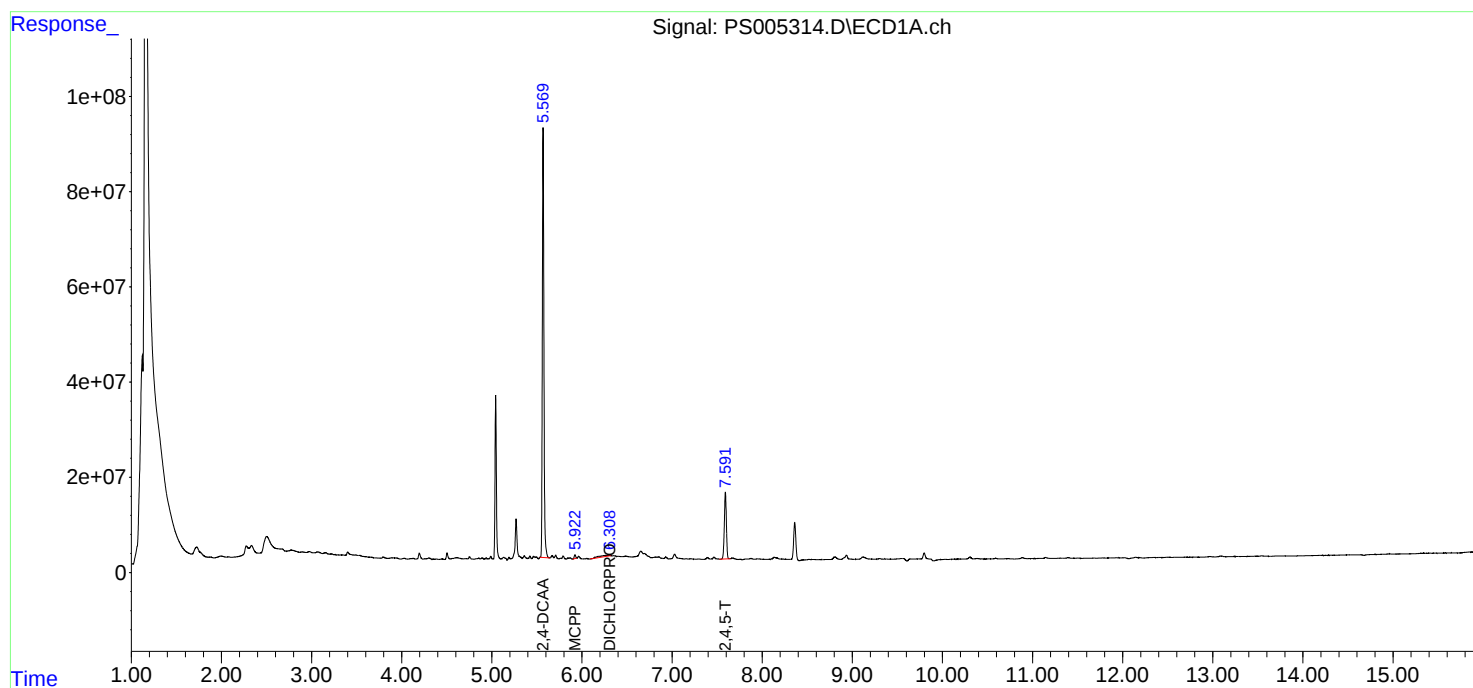


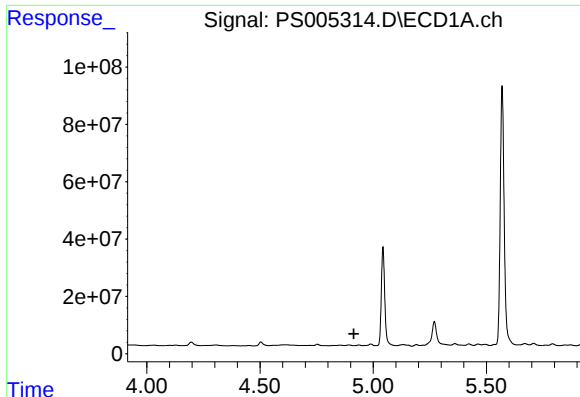

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-11

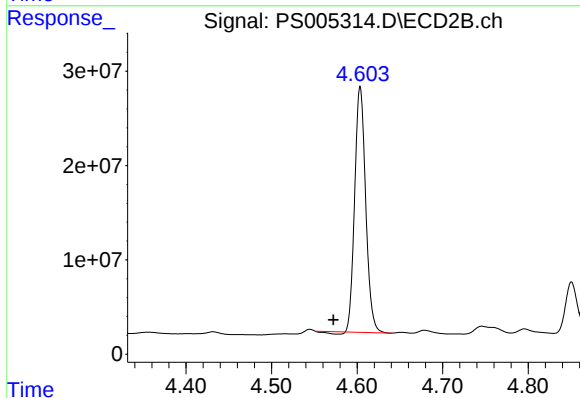


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.604 min
Delta R.T.: 0.031 min
Response: 231426268
Conc: 175.49 ng/ml

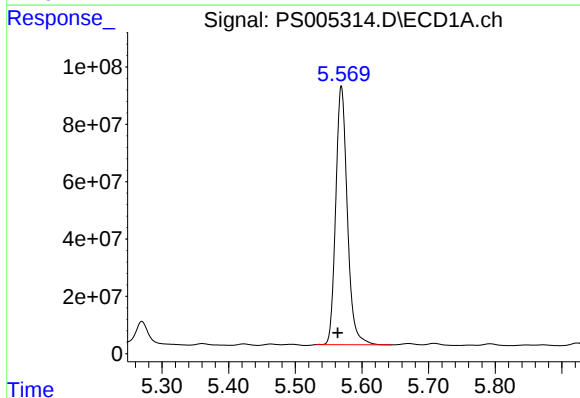


#4 2,4-DCAA

R.T.: 5.569 min
Delta R.T.: 0.006 min
Response: 1088388036
Conc: 741.46 ng/ml

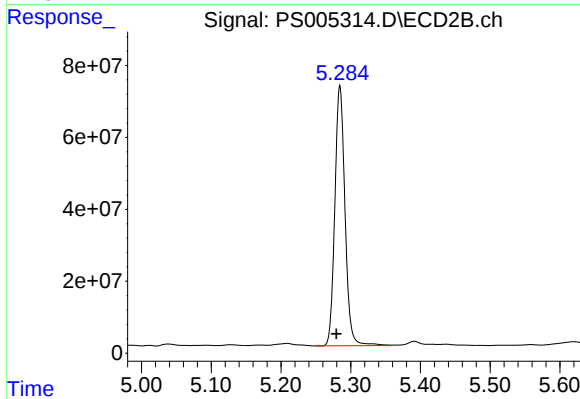

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 733623430
Conc: 731.89 ng/ml

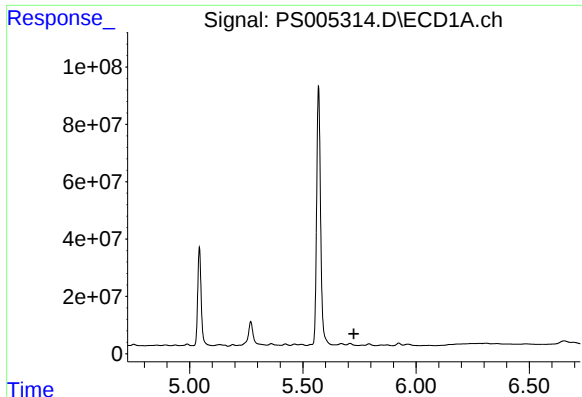

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-11

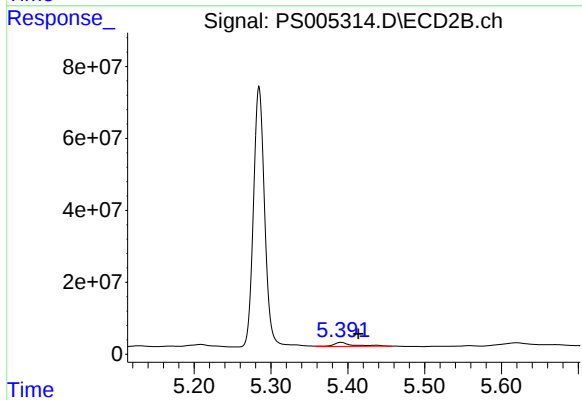


#5 DICAMBA

R.T.: 5.391 min
Delta R.T.: -0.023 min
Response: 19782425
Conc: 5.28 ng/ml

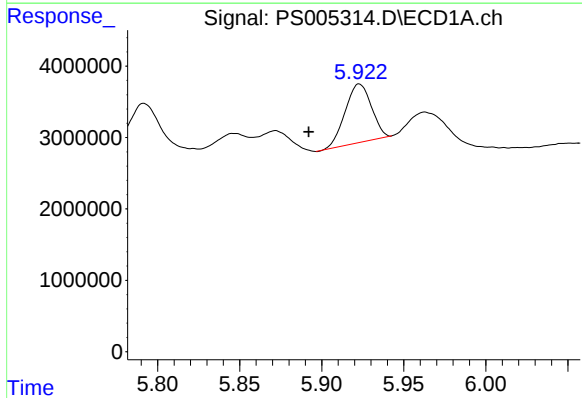


#6 MCP

R.T.: 5.923 min
Delta R.T.: 0.031 min
Response: 9070738
Conc: 2.07 ug/ml

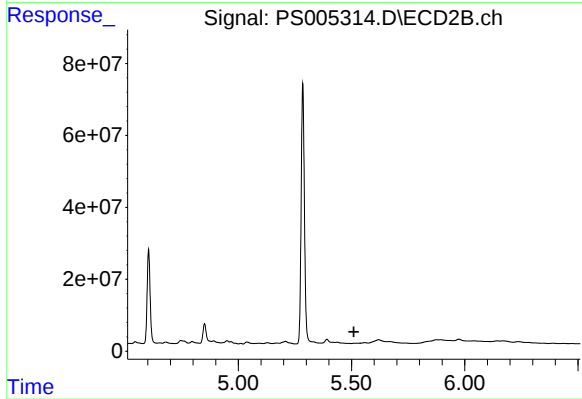

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

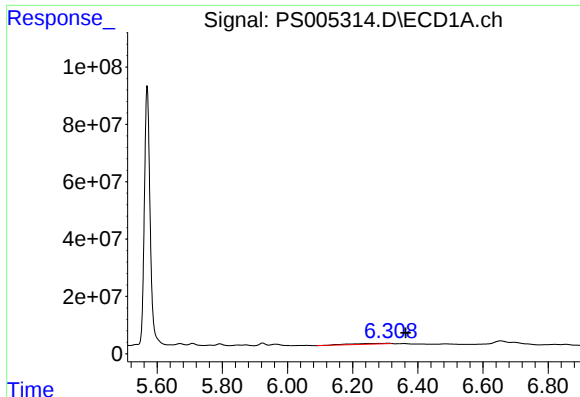

#8 DICHLORPROP


R.T.: 6.309 min
Delta R.T.: -0.054 min
Response: 24418934
Conc: 17.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-11

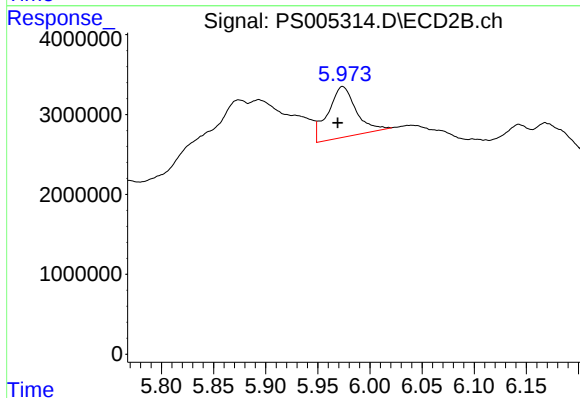


#8 DICHLORPROP

R.T.: 5.974 min
Delta R.T.: 0.005 min
Response: 11911612
Conc: 12.34 ng/ml

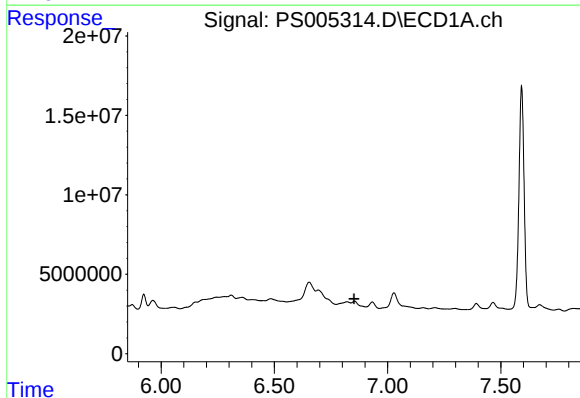


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

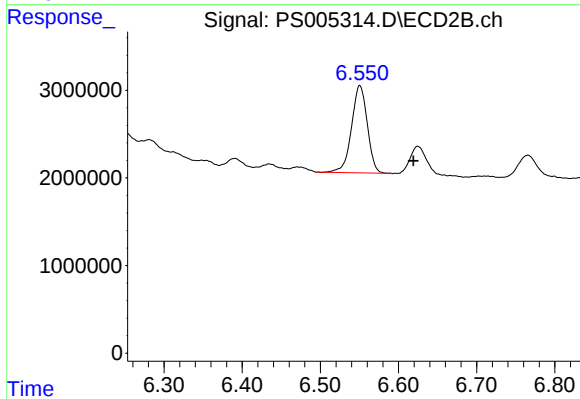

#10 Pentachlorophenol


R.T.: 6.551 min
Delta R.T.: -0.068 min
Response: 13997994
Conc: 1.09 ng/ml

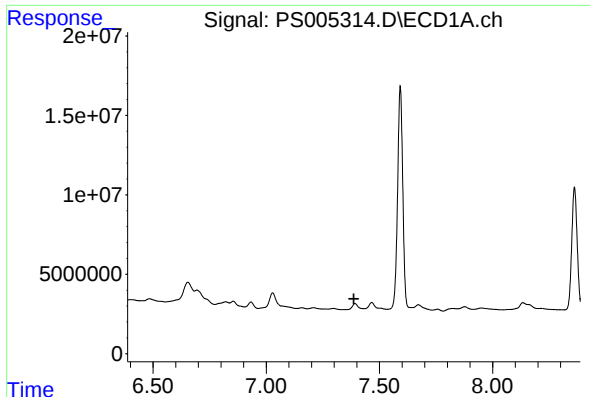

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-11

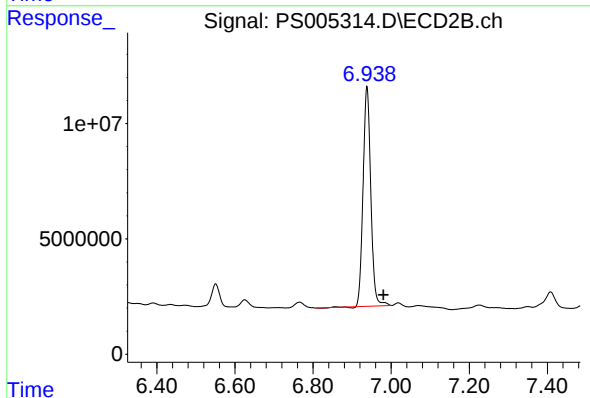


#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.043 min
Response: 130693857
Conc: 24.54 ng/ml

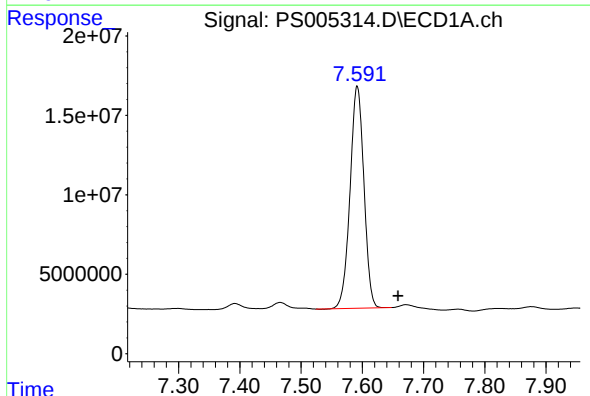

#12 2,4,5-T

R.T.: 7.592 min
Delta R.T.: -0.067 min
Response: 219778506
Conc: 27.31 ng/ml

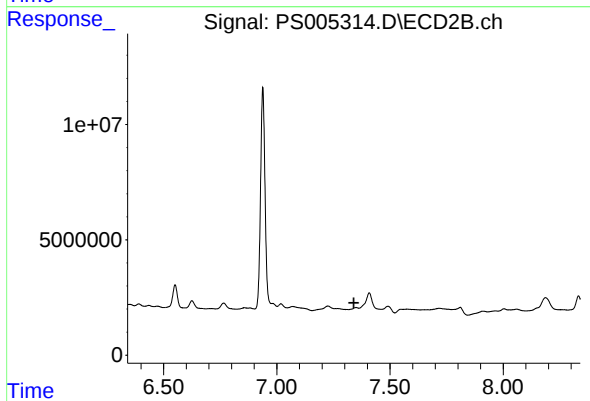

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.