

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
 Data File : PS005322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 22:48
 Operator : SM\AJ
 Sample : K3555-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:07:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.579	5.293	570.6E6	380.8E6	388.738	379.910
Target Compounds							
2) T	3,5-DICHL...	0.000	4.612	0	277.5E6	N.D.	210.428
3) T	4-Nitroph...	5.371	0.000	9564976	0	13.206	N.D. #
5) T	DICAMBA	0.000	5.399	0	11131361	N.D.	2.974
6) T	MCP	5.932	0.000	11732554	0	2.680	N.D. #
8) T	DICHLORPROP	0.000	5.981	0	18100160	N.D.	18.746
11) T	2,4,5-TP ...	0.000	6.946	0	168.3E6	N.D.	31.600
12) T	2,4,5-T	7.601	0.000	282.8E6	0	35.139	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
Data File : PS005322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 22:48
Operator : SM\AJ
Sample : K3555-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SAMPLE-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:07:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

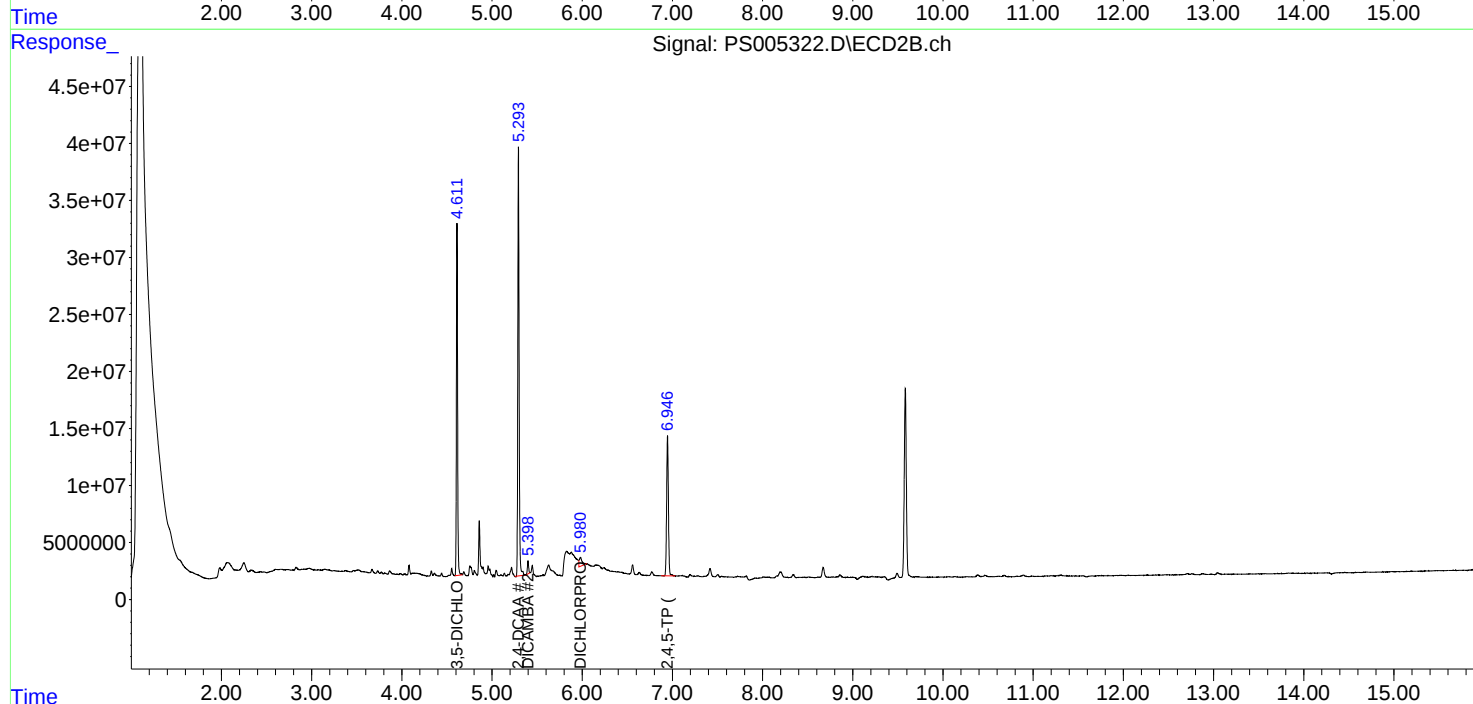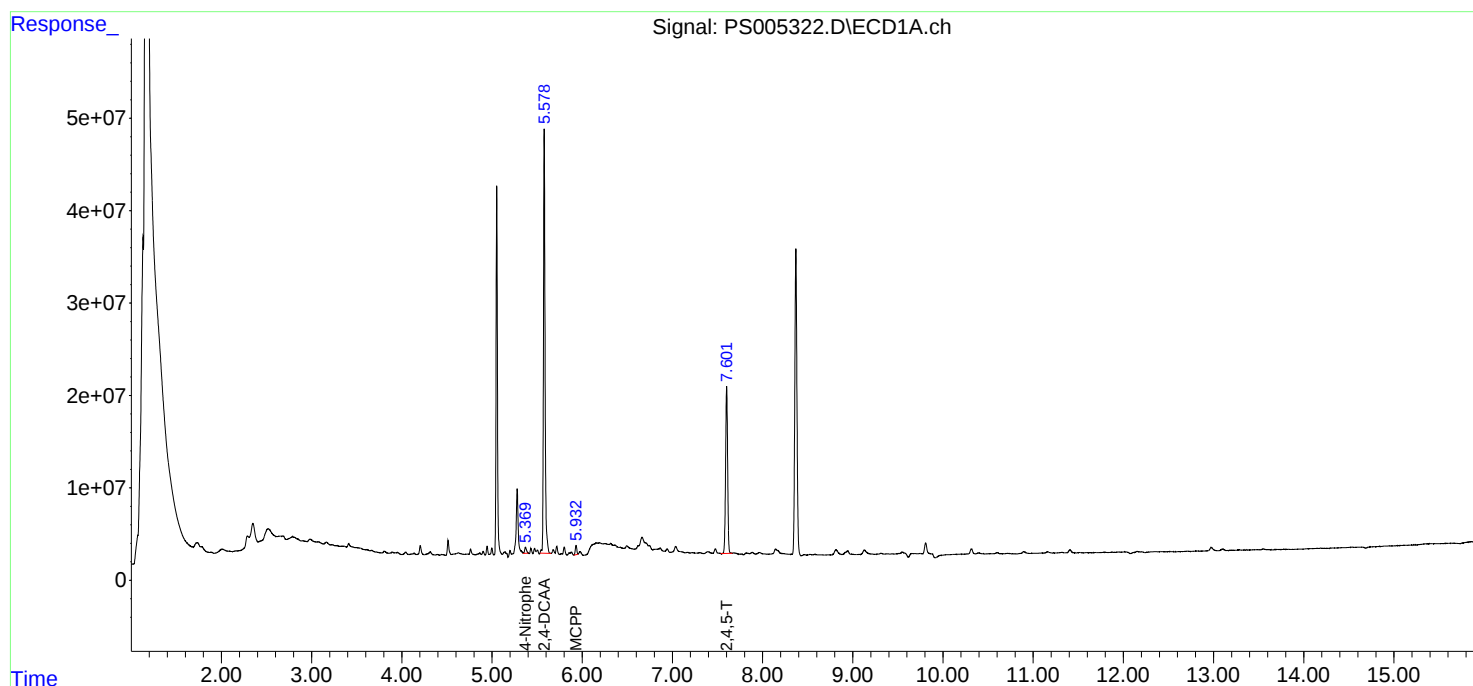


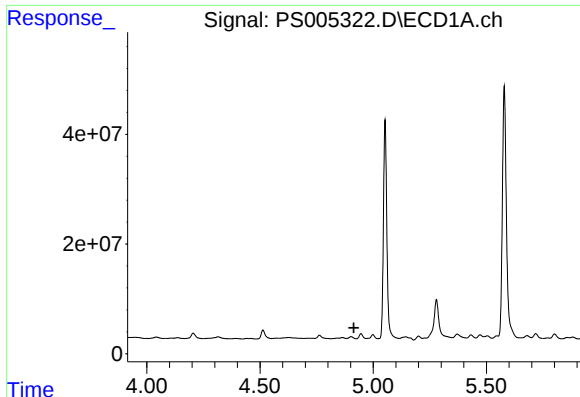

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-13

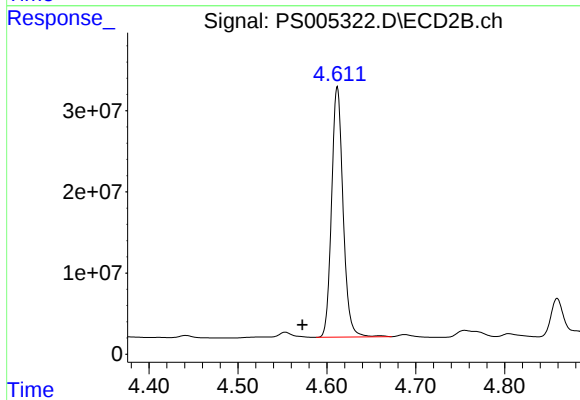


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.612 min
Delta R.T.: 0.039 min
Response: 277493998
Conc: 210.43 ng/ml

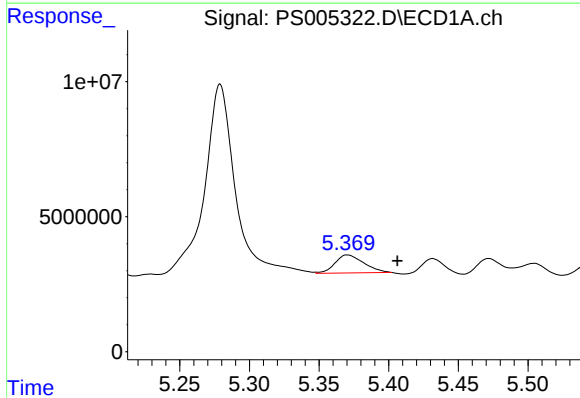


#3 4-Nitrophenol

R.T.: 5.371 min
Delta R.T.: -0.035 min
Response: 9564976
Conc: 13.21 ng/ml

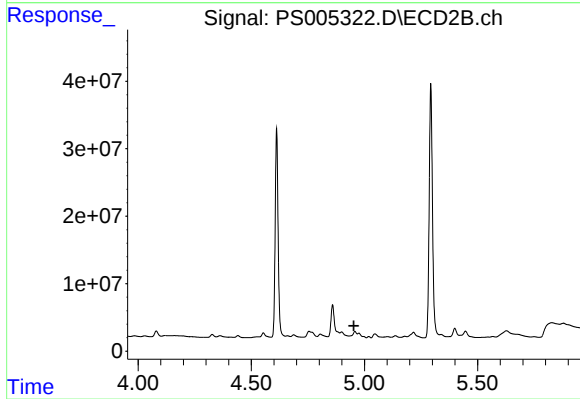

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

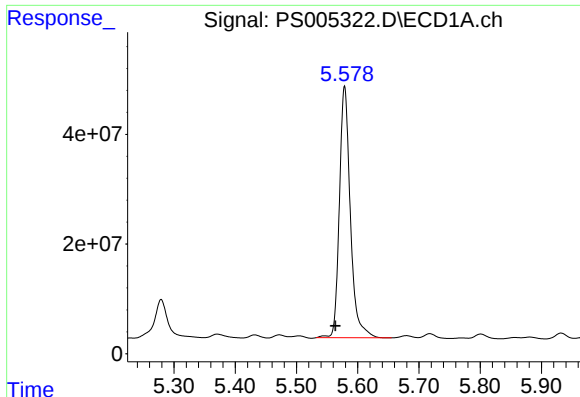

#4 2,4-DCAA


R.T.: 5.579 min
Delta R.T.: 0.015 min
Response: 570626221
Conc: 388.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-13

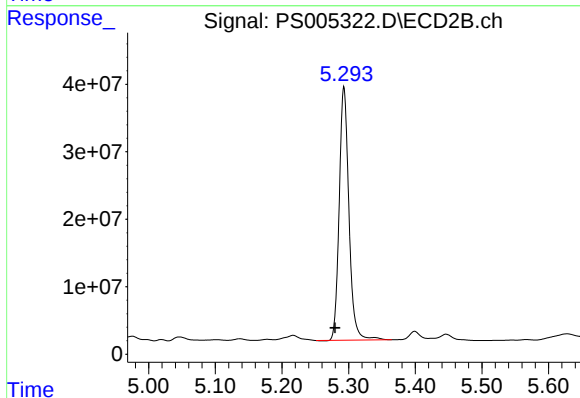


#4 2,4-DCAA

R.T.: 5.293 min
Delta R.T.: 0.013 min
Response: 380810060
Conc: 379.91 ng/ml

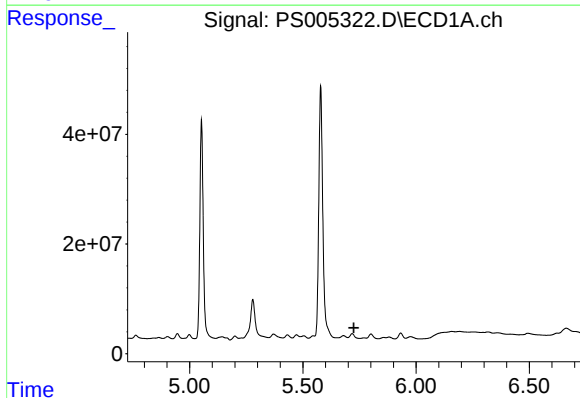


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

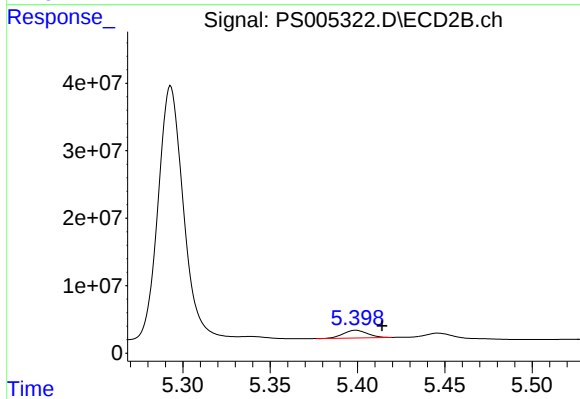

#5 DICAMBA


R.T.: 5.399 min
Delta R.T.: -0.015 min
Response: 11131361
Conc: 2.97 ng/ml

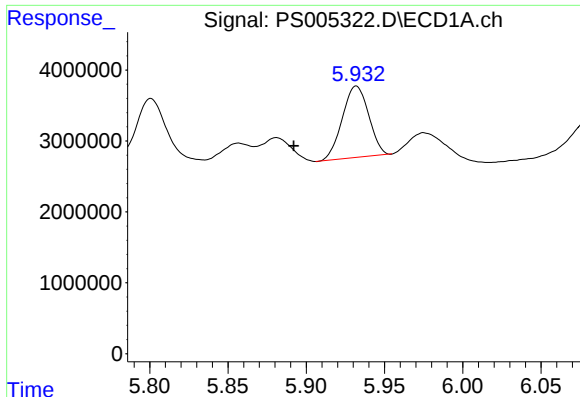

#6 MCP


R.T.: 5.932 min
Delta R.T.: 0.040 min
Response: 11732554
Conc: 2.68 ug/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-13

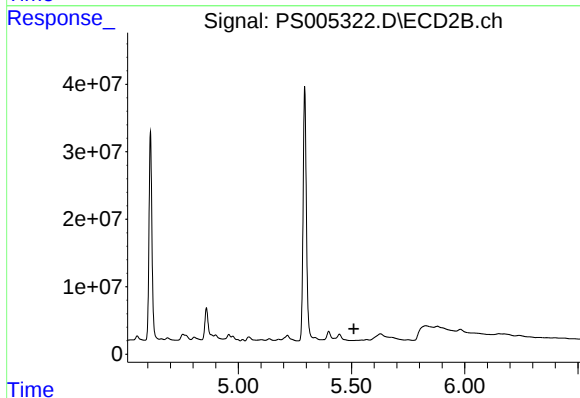


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

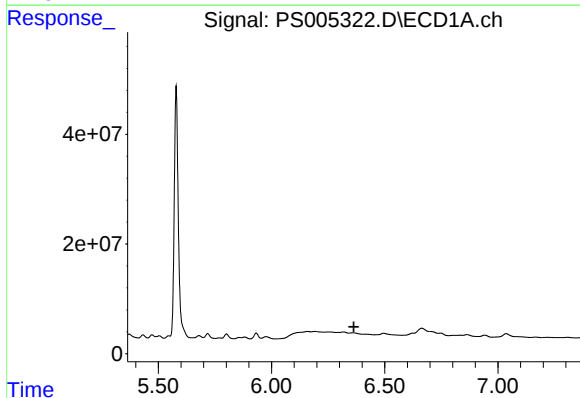


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

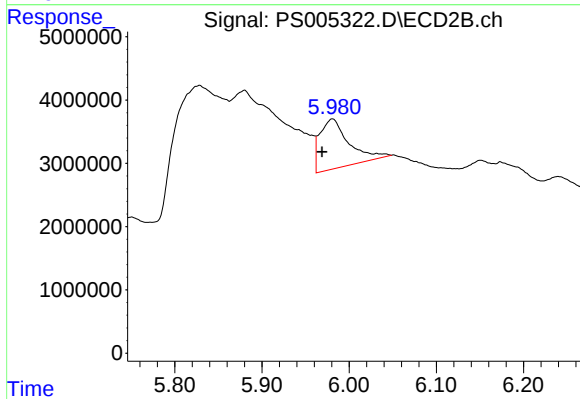

#8 DICHLORPROP


R.T.: 5.981 min
Delta R.T.: 0.012 min
Response: 18100160
Conc: 18.75 ng/ml

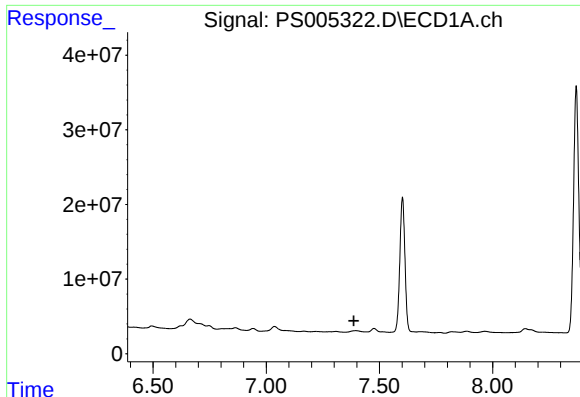

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-13

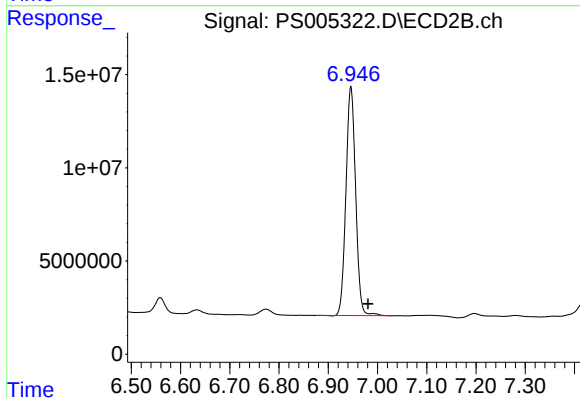


#11 2,4,5-TP (SILVEX)

R.T.: 6.946 min
Delta R.T.: -0.035 min
Response: 168278910
Conc: 31.60 ng/ml

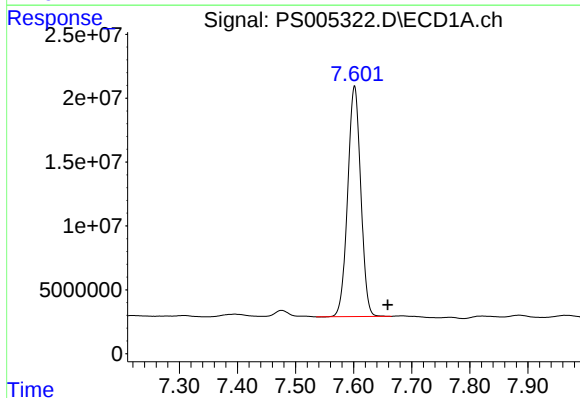

#12 2,4,5-T

R.T.: 7.601 min
Delta R.T.: -0.057 min
Response: 282793478
Conc: 35.14 ng/ml

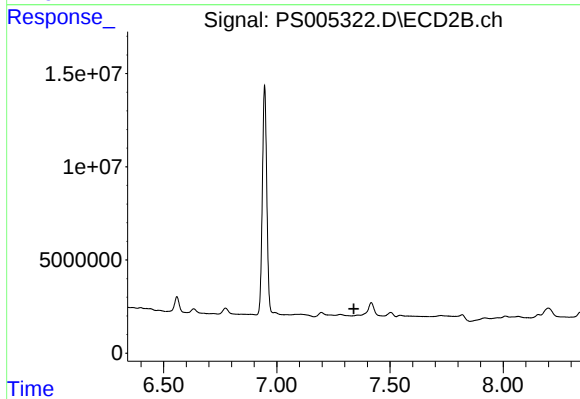

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.