

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
 Data File : PS005335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2019 03:34
 Operator : SM\AJ
 Sample : K3600-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WC-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 05:10:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.287	147.6E6	77771170	100.553	77.587
Target Compounds							
2) T	3,5-DICHL...	0.000	4.607	0	15140903	N.D.	11.482
5) T	DICAMBA	5.671	0.000	6947829	0	1.218	N.D. #
6) T	MCP	5.953	0.000	14827311	0	3.387	N.D. #
7) T	MCPA	6.065	5.677	23614987	29093838	3.761	7.182 #
8) T	DICHLORPROP	0.000	5.911	0	18848210	N.D.	19.521
10) T	Pentachlo...	6.857	6.626	22822975	18088688	1.160	1.407
13) T	2,4-DB	8.234	0.000	50739187	0	43.682	N.D. #
15) T	Picloram	9.108	0.000	36729496	0	3.196	N.D. #
16) T	DCPA	9.579	8.979	43782291	33807893	4.389	4.966



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070119\
Data File : PS005335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2019 03:34
Operator : SM\AJ
Sample : K3600-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WC-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 05:10:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

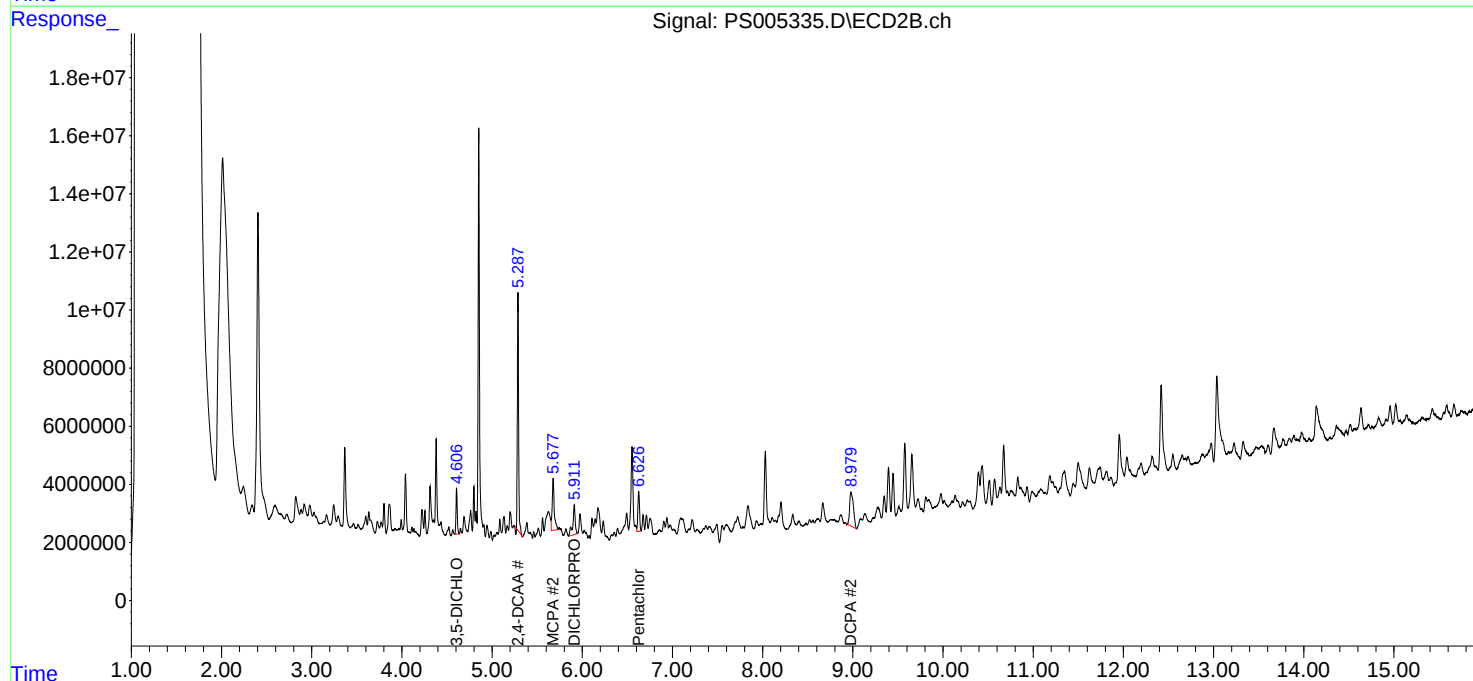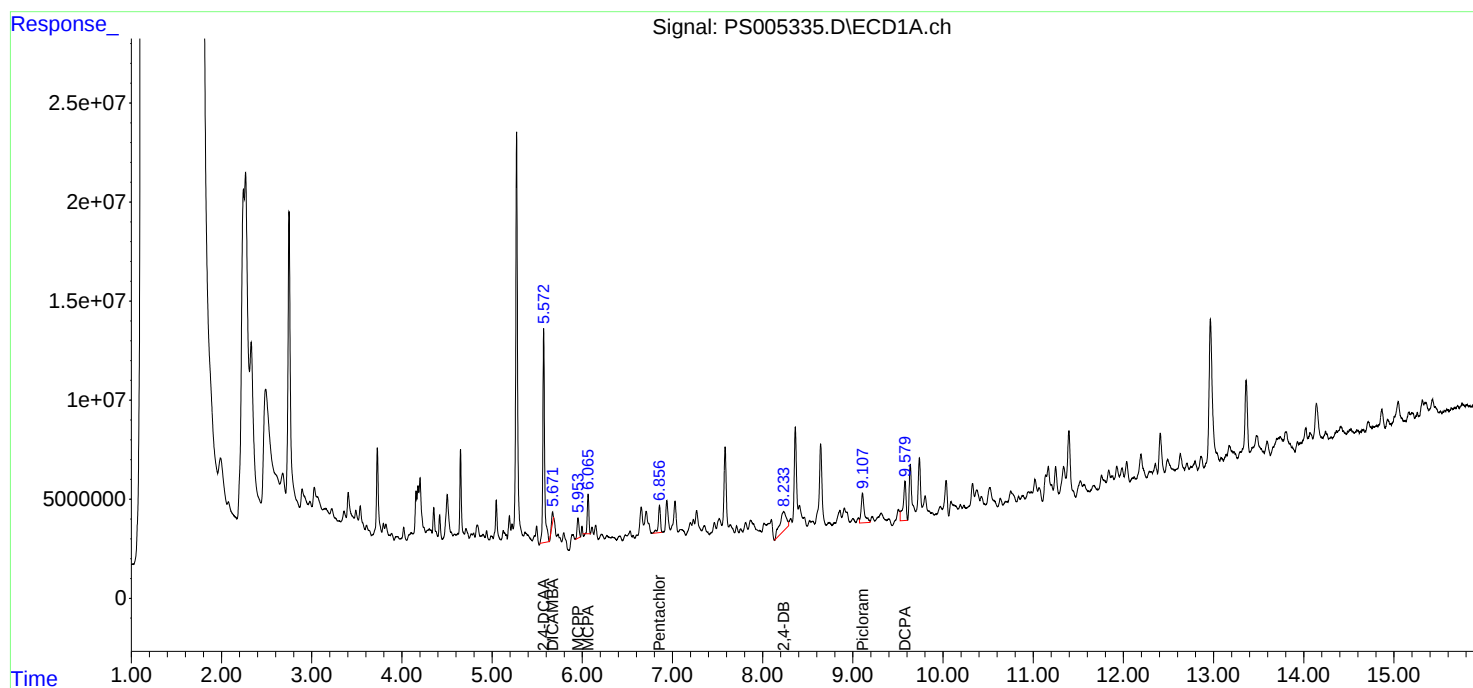


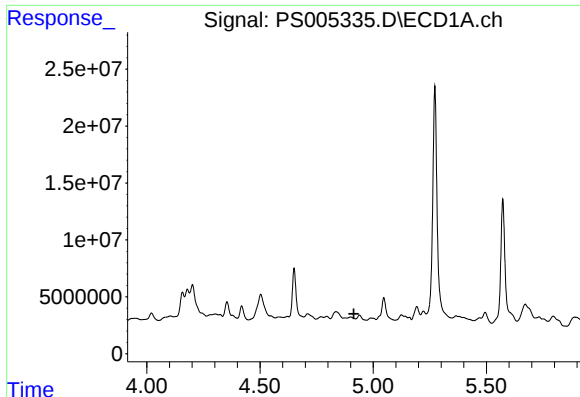

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WC-6

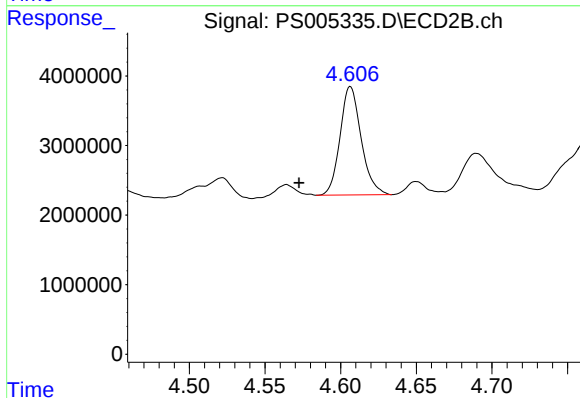


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.607 min
Delta R.T.: 0.034 min
Response: 15140903
Conc: 11.48 ng/ml

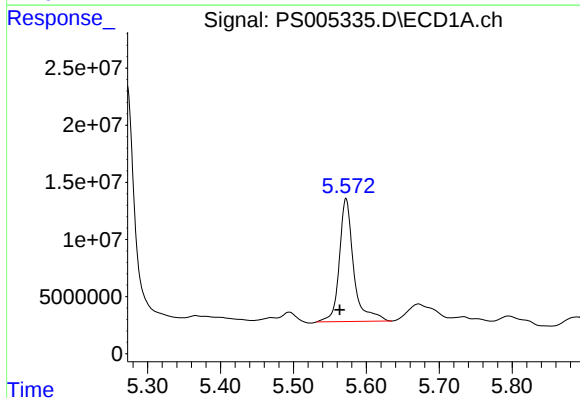


#4 2,4-DCAA

R.T.: 5.572 min
Delta R.T.: 0.009 min
Response: 147601497
Conc: 100.55 ng/ml

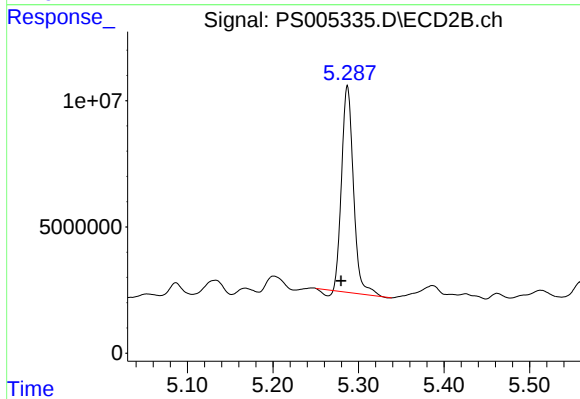

#4 2,4-DCAA


R.T.: 5.287 min
Delta R.T.: 0.007 min
Response: 77771170
Conc: 77.59 ng/ml

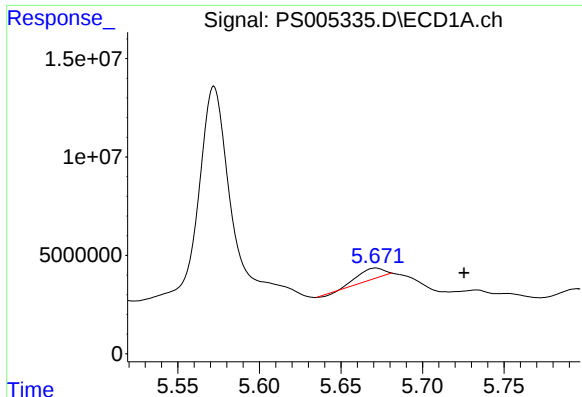

#5 DICAMBA


R.T.: 5.671 min
Delta R.T.: -0.054 min
Response: 6947829
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-6

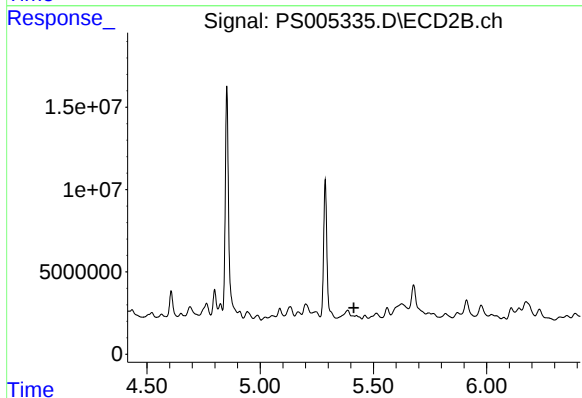


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

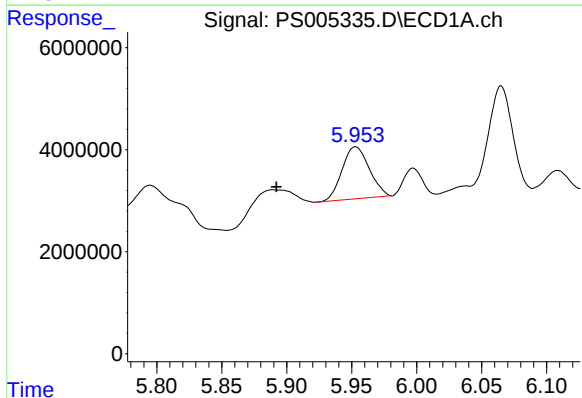


#6 MCP

R.T.: 5.953 min
Delta R.T.: 0.061 min
Response: 14827311
Conc: 3.39 ug/ml

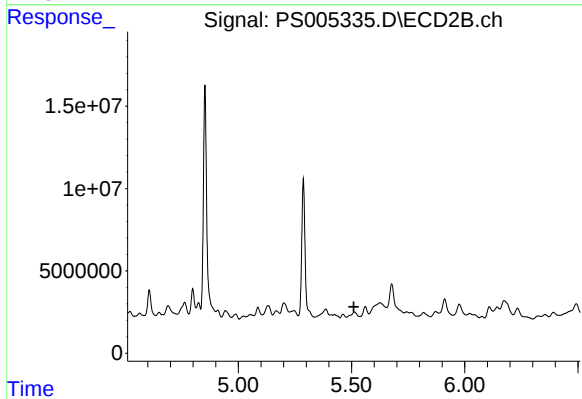

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

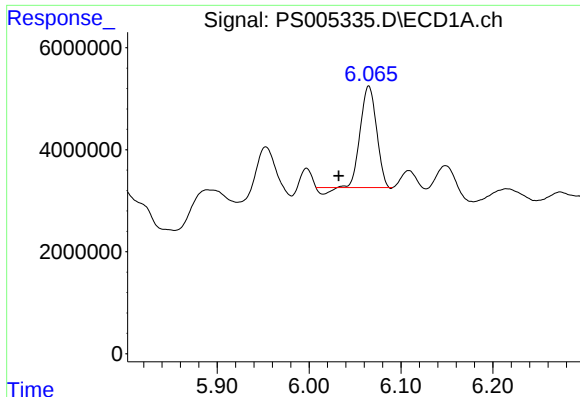

#7 MCPA


R.T.: 6.065 min
Delta R.T.: 0.033 min
Response: 23614987
Conc: 3.76 ug/ml

Instrument :
ECD_S
ClientSampleId :
WC-6

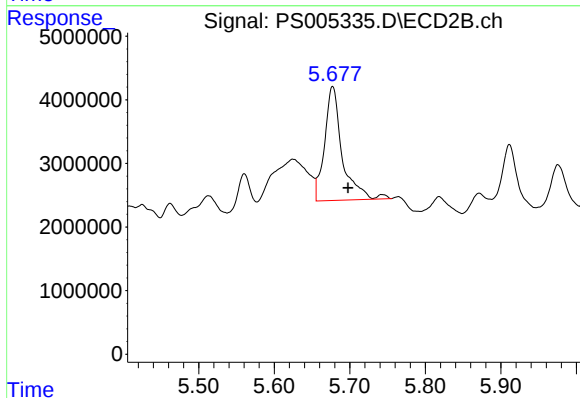


#7 MCPA

R.T.: 5.677 min
Delta R.T.: -0.020 min
Response: 29093838
Conc: 7.18 ug/ml

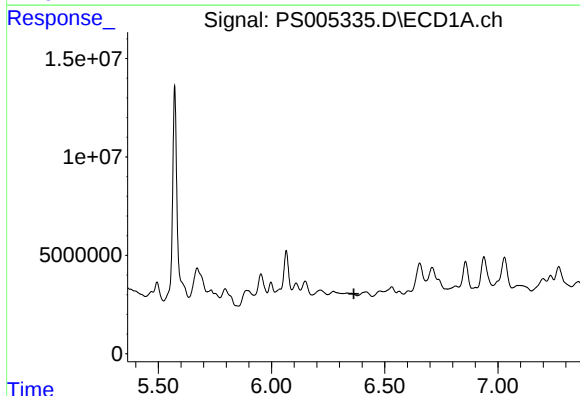


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

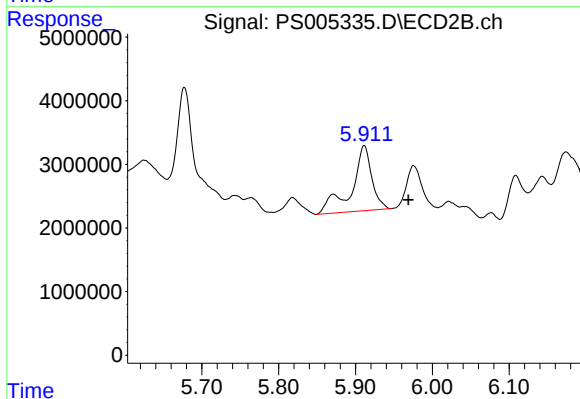

#8 DICHLORPROP


R.T.: 5.911 min
Delta R.T.: -0.058 min
Response: 18848210
Conc: 19.52 ng/ml

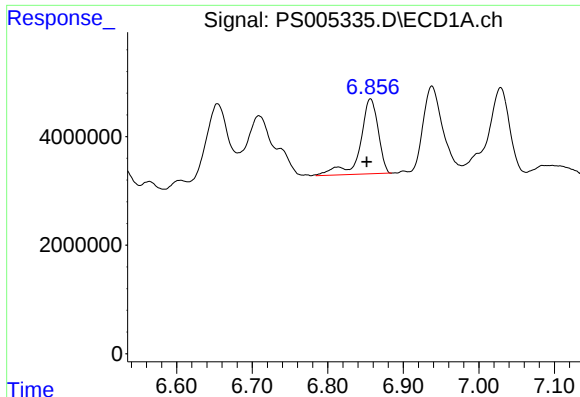

#10 Pentachlorophenol


R.T.: 6.857 min
Delta R.T.: 0.005 min
Response: 22822975
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-6

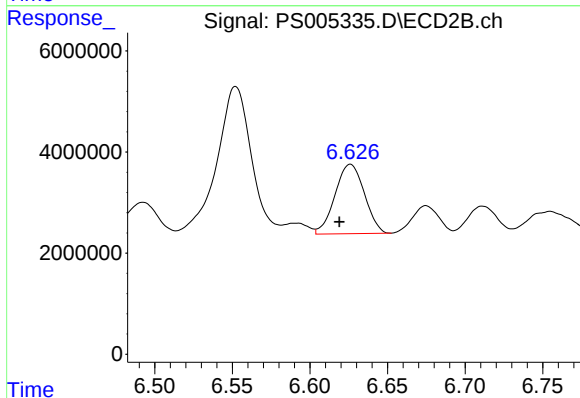


#10 Pentachlorophenol

R.T.: 6.626 min
Delta R.T.: 0.007 min
Response: 18088688
Conc: 1.41 ng/ml

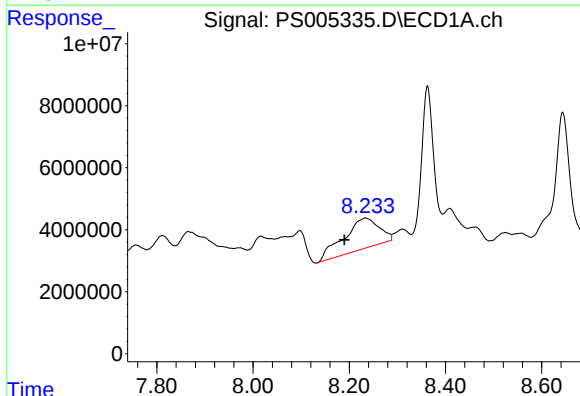


#13 2,4-DB

R.T.: 8.234 min
Delta R.T.: 0.044 min
Response: 50739187
Conc: 43.68 ng/ml

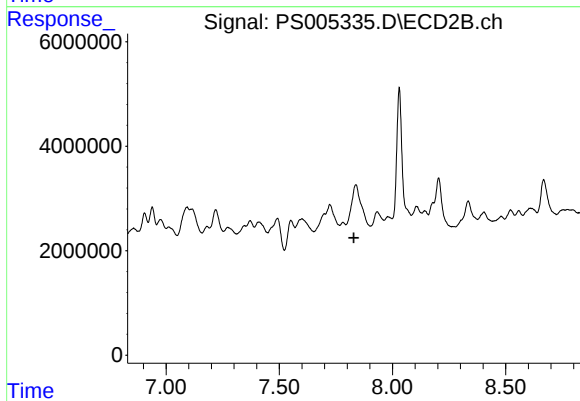

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.830 min
Response: 0
Conc: N.D.

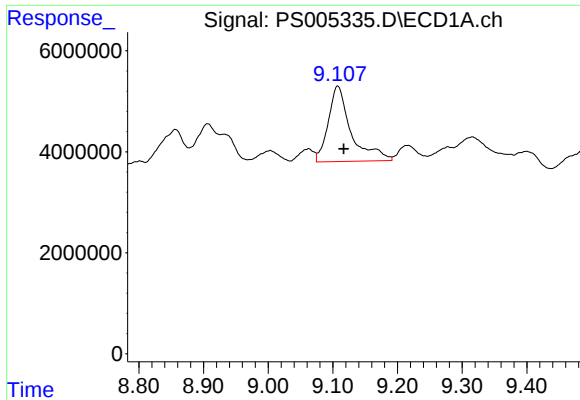

#15 Picloram


R.T.: 9.108 min
Delta R.T.: -0.009 min
Response: 36729496
Conc: 3.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-6

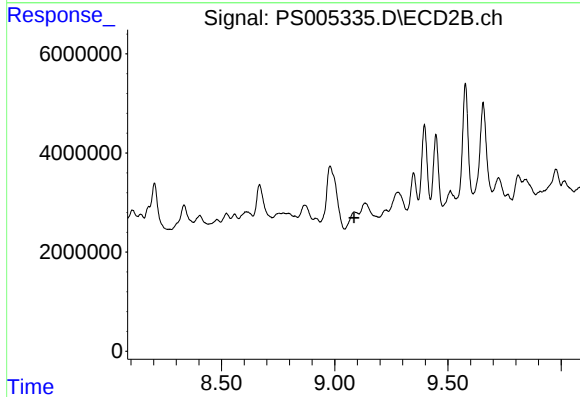


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.

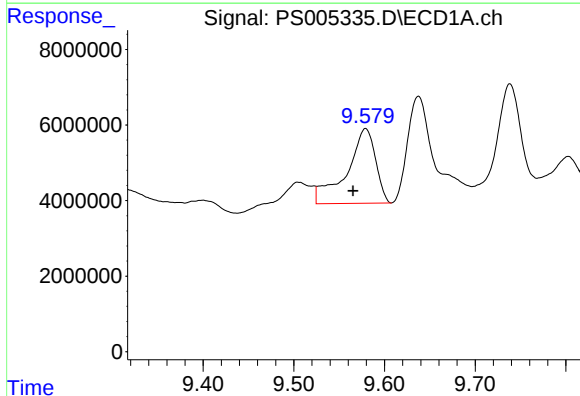

#16 DCPA

R.T.: 9.579 min
Delta R.T.: 0.014 min
Response: 43782291
Conc: 4.39 ng/ml

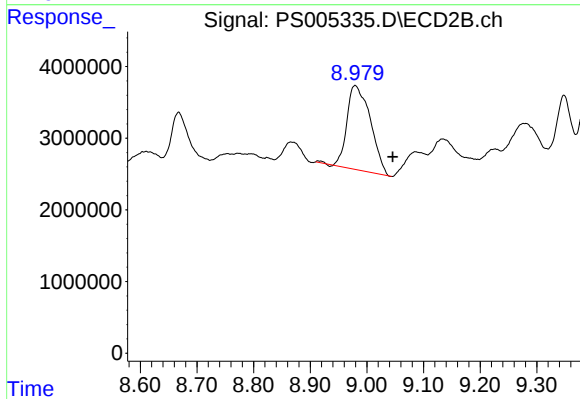

#16 DCPA

R.T.: 8.979 min
Delta R.T.: -0.066 min
Response: 33807893
Conc: 4.97 ng/ml