

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070224\
 Data File : PS027122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2024 19:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:43:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 18 02:58:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	7.753	1307.2E6	1171.3E6	513.647	505.918
Target Compounds							
1) T	Dalapon	2.642	0.000	913476	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.365f	6.696	6884226	516885	1.710	<MDL #
3) T	4-Nitroph...	7.037	0.000	100113	0	<MDL	N.D. #
5) T	DICAMBA	7.412	7.949	110035	5182953	<MDL	<MDL #
6) T	MCPD	7.577	8.058	168015	3449151	<MDL	<MDL #
7) T	MCPA	7.745	8.286	651952	12155591	<MDL	1.168 #
8) T	DICHLORPROP	8.116	8.663	676500	393127	<MDL	<MDL #
9) T	2,4-D	8.341	0.000	18795911	0	6.325	N.D. #
10) T	Pentachlo...	8.649	9.519	709848	831472	<MDL	<MDL #
11) T	2,4,5-TP ...	9.180f	9.901	520884	2564601	<MDL	<MDL #
12) T	2,4,5-T	9.503	10.326	257682	2963765	<MDL	<MDL #
14) T	DINOSEB	11.281	11.270	226947	299894	<MDL	<MDL #
15) T	Picloram	11.062	12.356	1296274	3168912	<MDL	<MDL #
16) T	DCPA	11.567	12.266f	119423	2684415	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070224\
Data File : PS027122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2024 19:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:43:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
Quant Title : 8080.M
QLast Update : Tue Jun 18 02:58:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

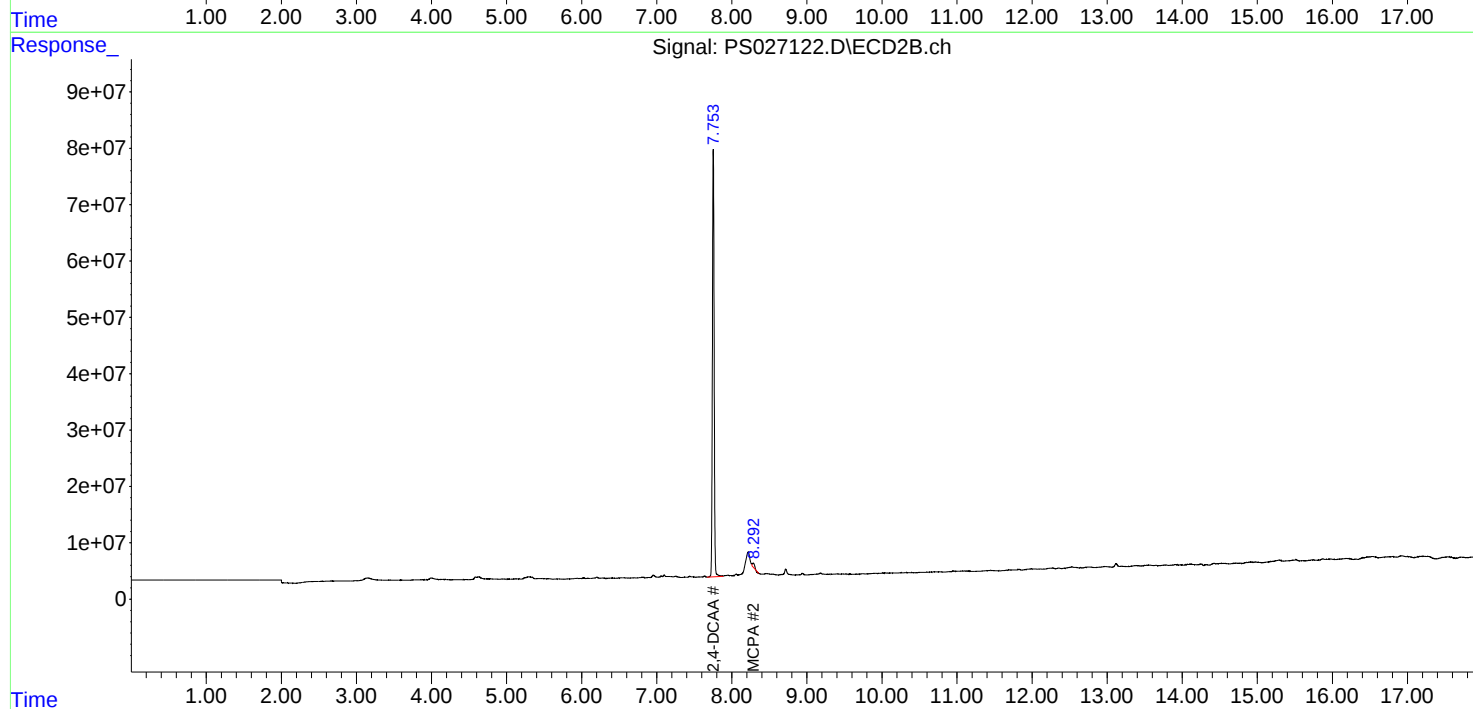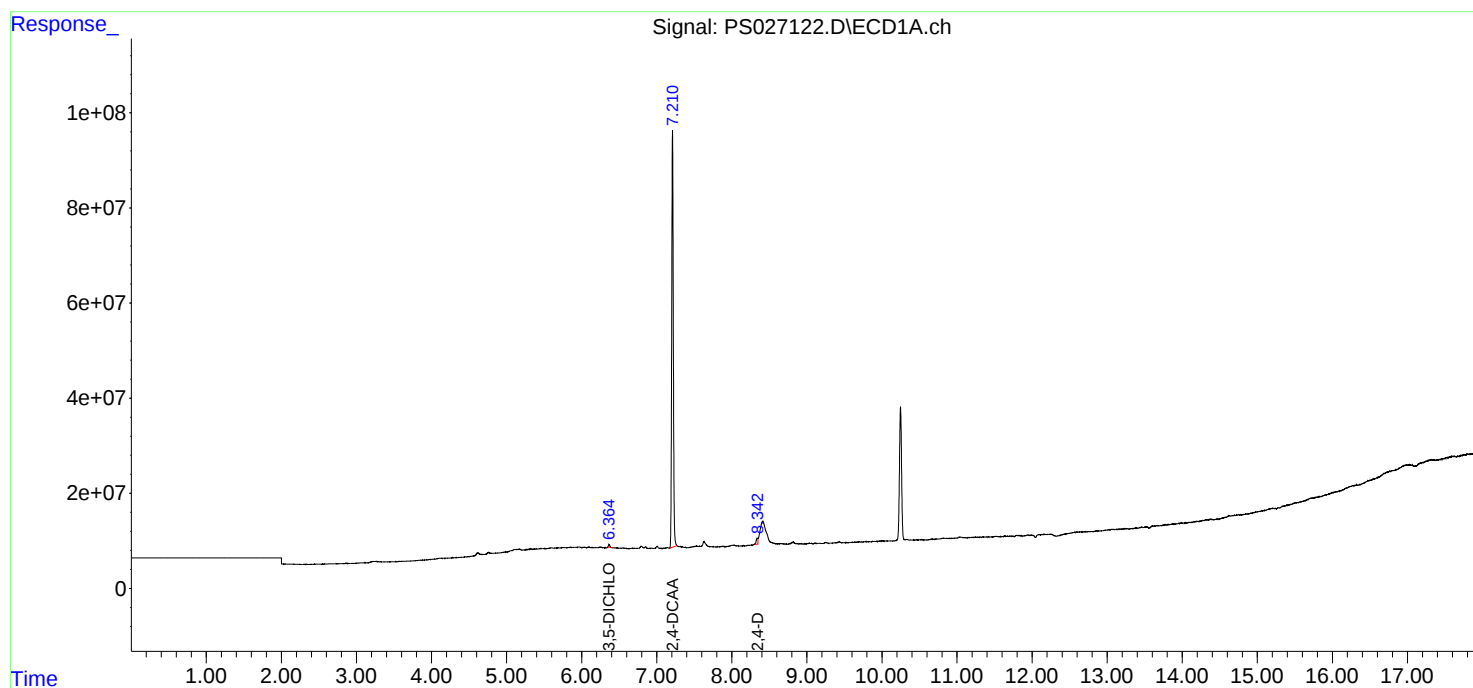


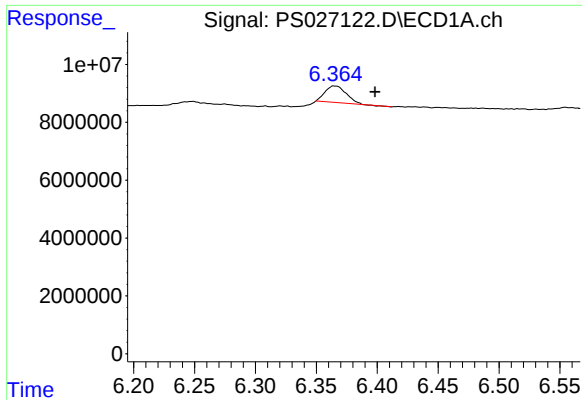

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.365 min
Delta R.T.: -0.033 min
Response: 6884226
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

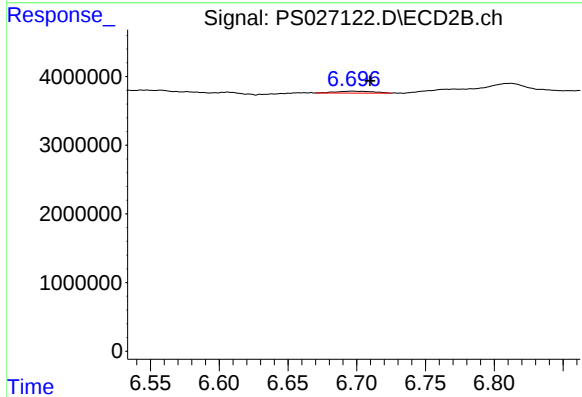


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.696 min
Delta R.T.: -0.013 min
Response: 516885
Conc: N.D.

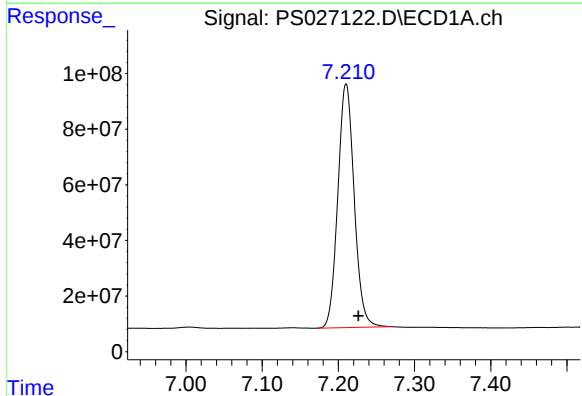


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: -0.016 min
Response: 1307160498
Conc: 513.65 ng/ml

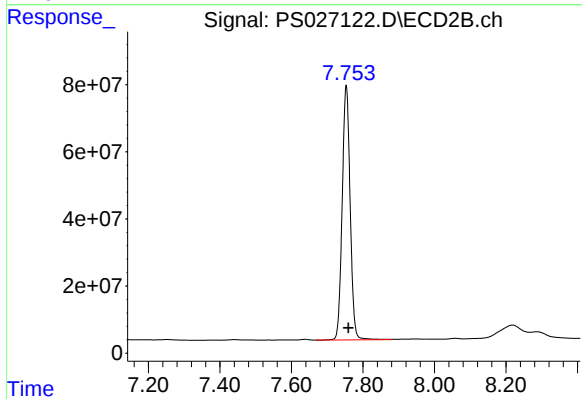

#4 2,4-DCAA


R.T.: 7.753 min
Delta R.T.: -0.006 min
Response: 1171272426
Conc: 505.92 ng/ml

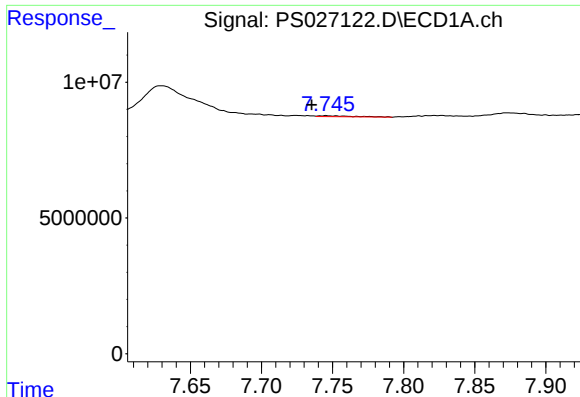

#7 MCPA


R.T.: 7.745 min
Delta R.T.: 0.010 min
Response: 651952
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

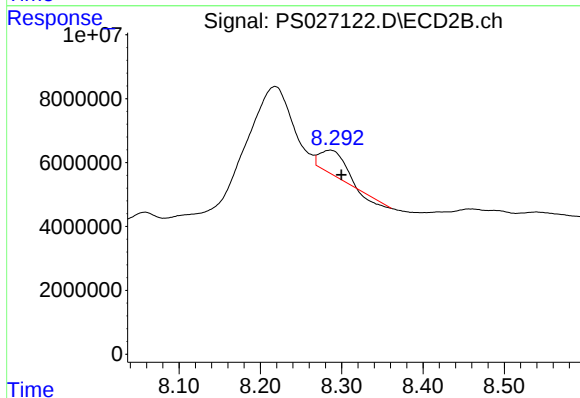


#7 MCPA

R.T.: 8.286 min
Delta R.T.: -0.014 min
Response: 12155591
Conc: 1.17 ug/ml

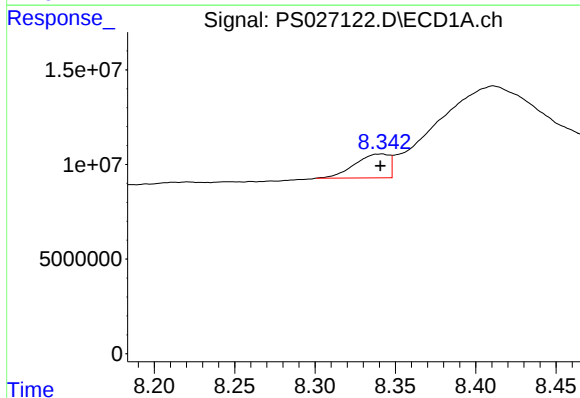

#9 2,4-D

R.T.: 8.341 min
Delta R.T.: 0.000 min
Response: 18795911
Conc: 6.32 ng/ml

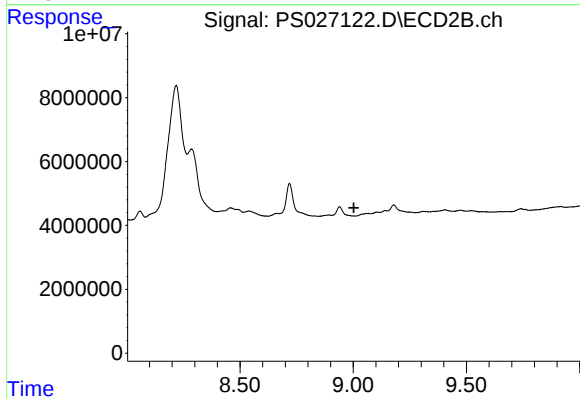

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 9.003 min
Response: 0
Conc: N.D.