

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070224\
Data File : PS027121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2024 19:30
Operator : AR\AJ
Sample : P3135-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-628-COMP-02

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/03/2024
Supervised By :Ankita Jodhani 07/03/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:42:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
Quant Title : 8080.M
QLast Update : Tue Jun 18 02:58:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.210	7.753	598.1E6	388.7E6	235.035m	167.903m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070224\
Data File : PS027121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2024 19:30
Operator : AR\AJ
Sample : P3135-07
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OK-628-COMP-02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/03/2024
Supervised By : Ankita Jodhani 07/03/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:42:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061724.M
Quant Title : 8080.M
QLast Update : Tue Jun 18 02:58:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

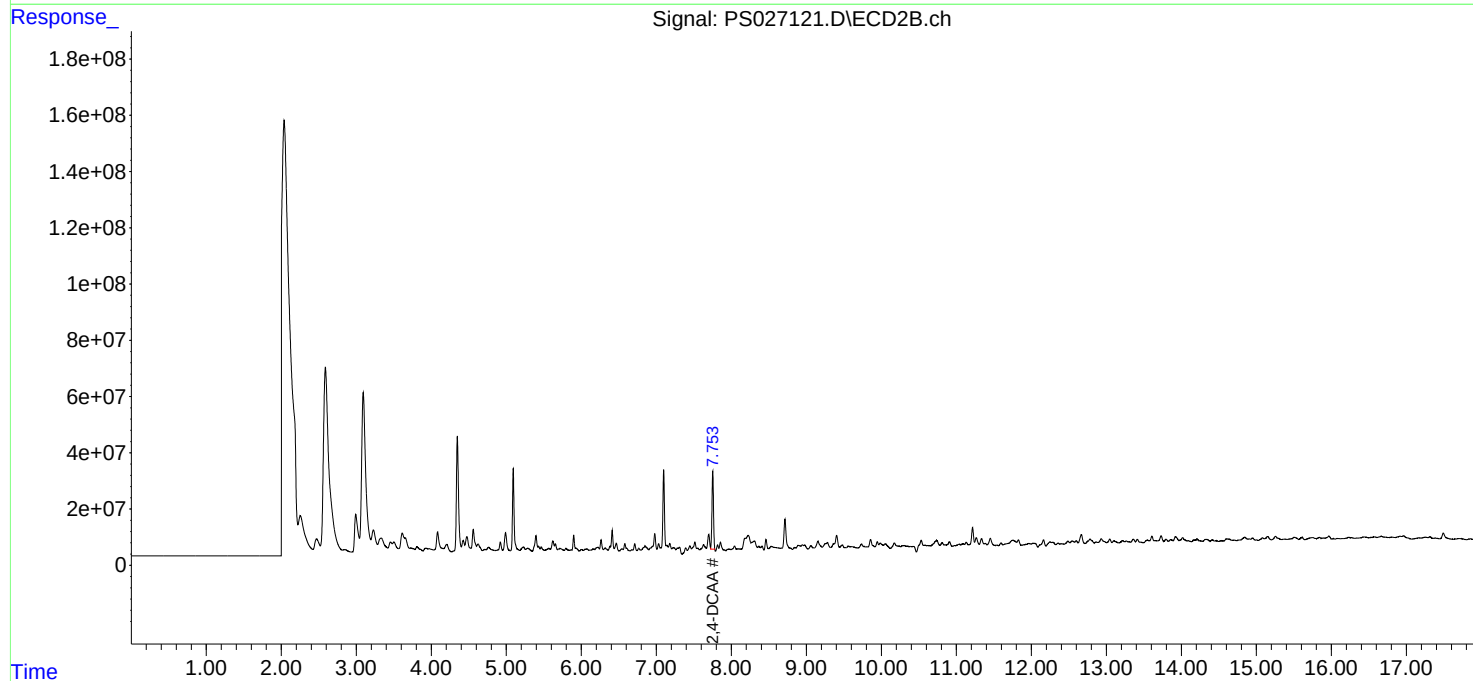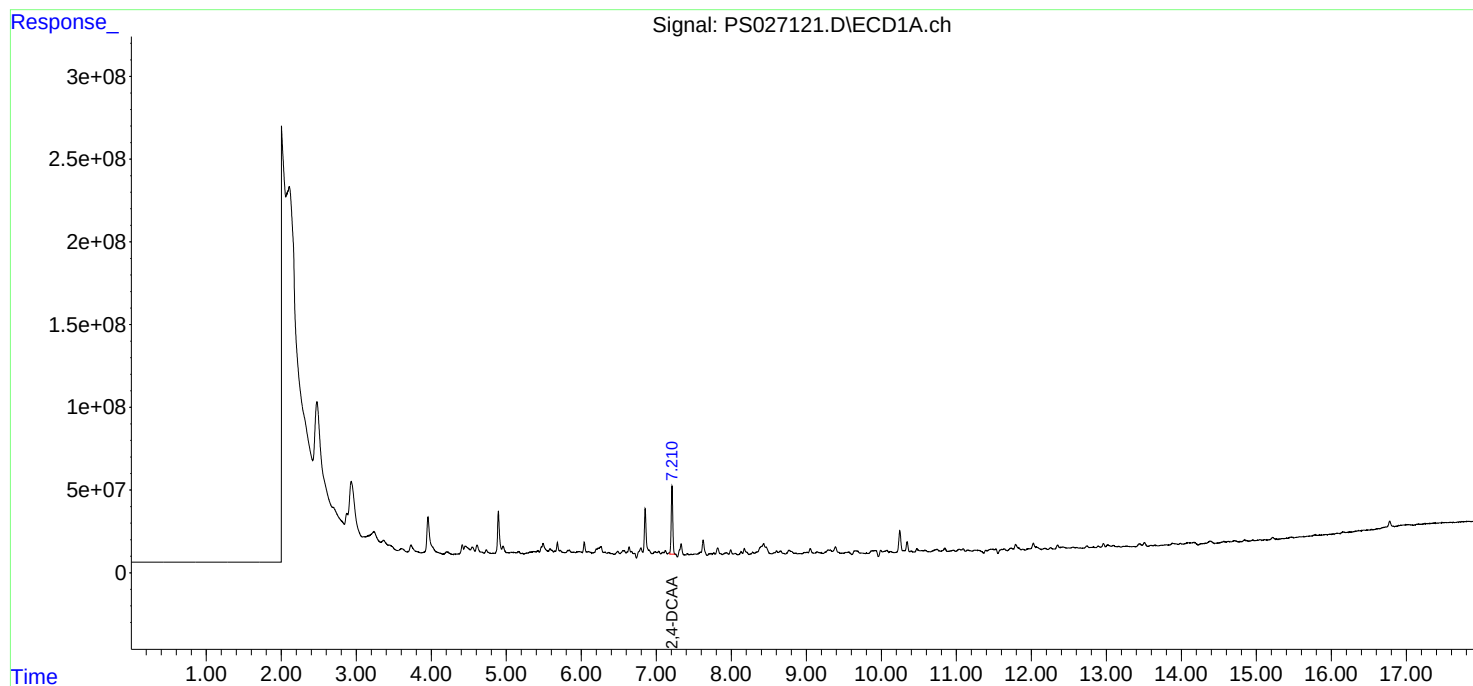

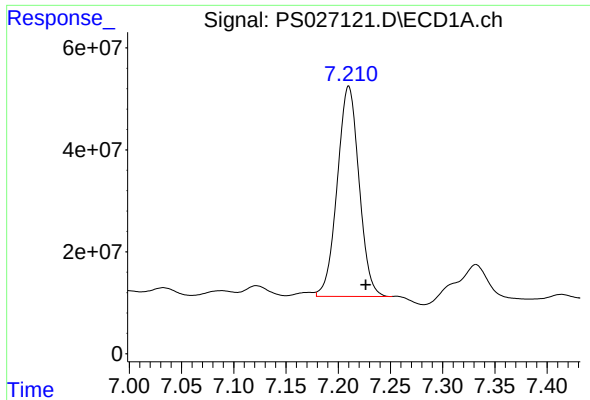


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: -0.017 min
Response: 598131560
Conc: 235.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-628-COMP-02

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/03/2024
Supervised By :Ankita Jodhani 07/03/2024

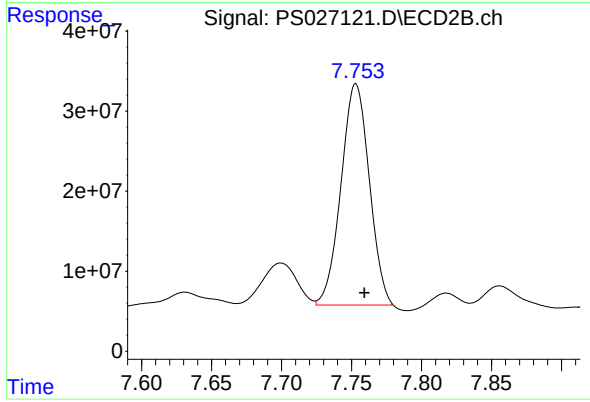

#4 2,4-DCAA

R.T.: 7.753 min
Delta R.T.: -0.007 min
Response: 388719064
Conc: 167.90 ng/ml m