

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
 Data File : PS005371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 10:34
 Operator : SM\AJ
 Sample : PB121021TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121021TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 15:25:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.290	522.9E6	347.3E6	356.253	346.450
Target Compounds							
12) T	2,4,5-T	7.604	7.409	25393848	30387144	3.155	5.957 #
15) T	Picloram	9.162	9.110	203.8E6	149.2E6	17.732	19.768
16) T	DCPA	0.000	9.110	0	149.2E6	N.D.	21.914



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
Data File : PS005371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 10:34
Operator : SM\AJ
Sample : PB121021TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121021TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 15:25:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

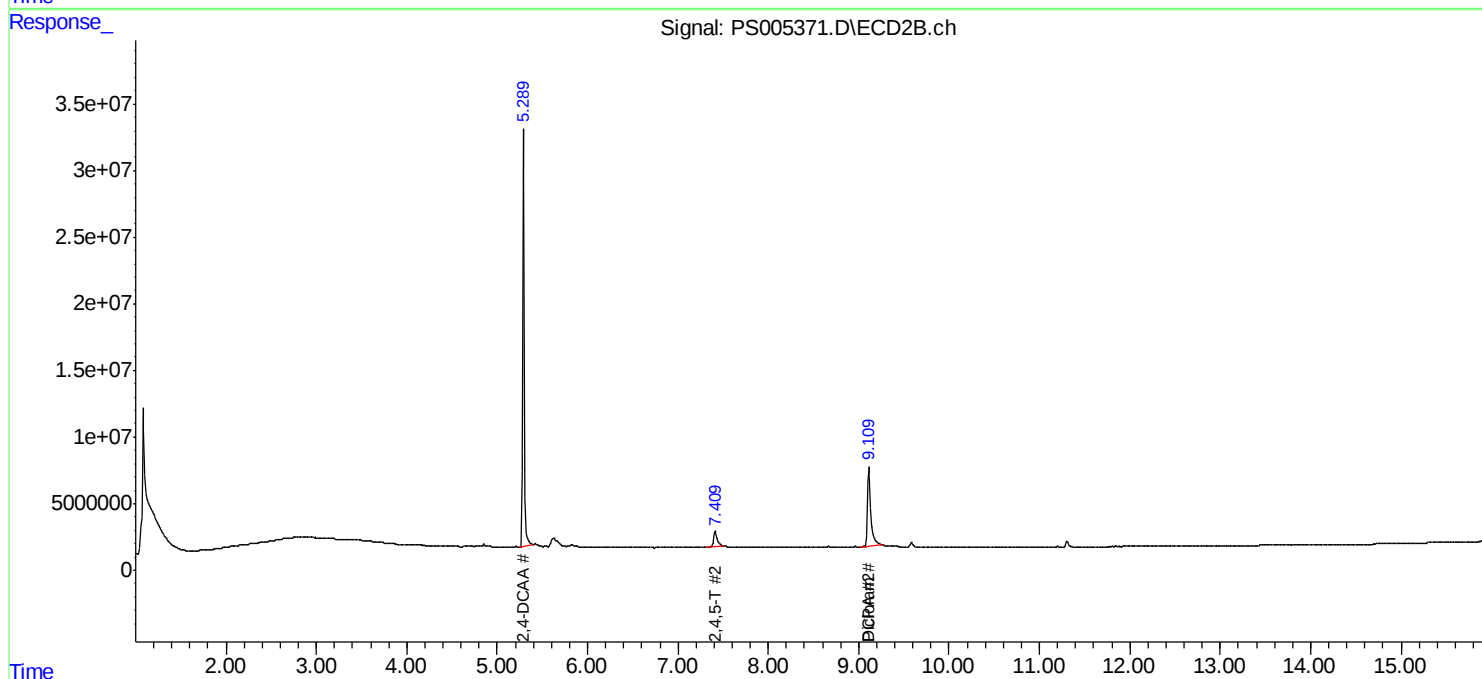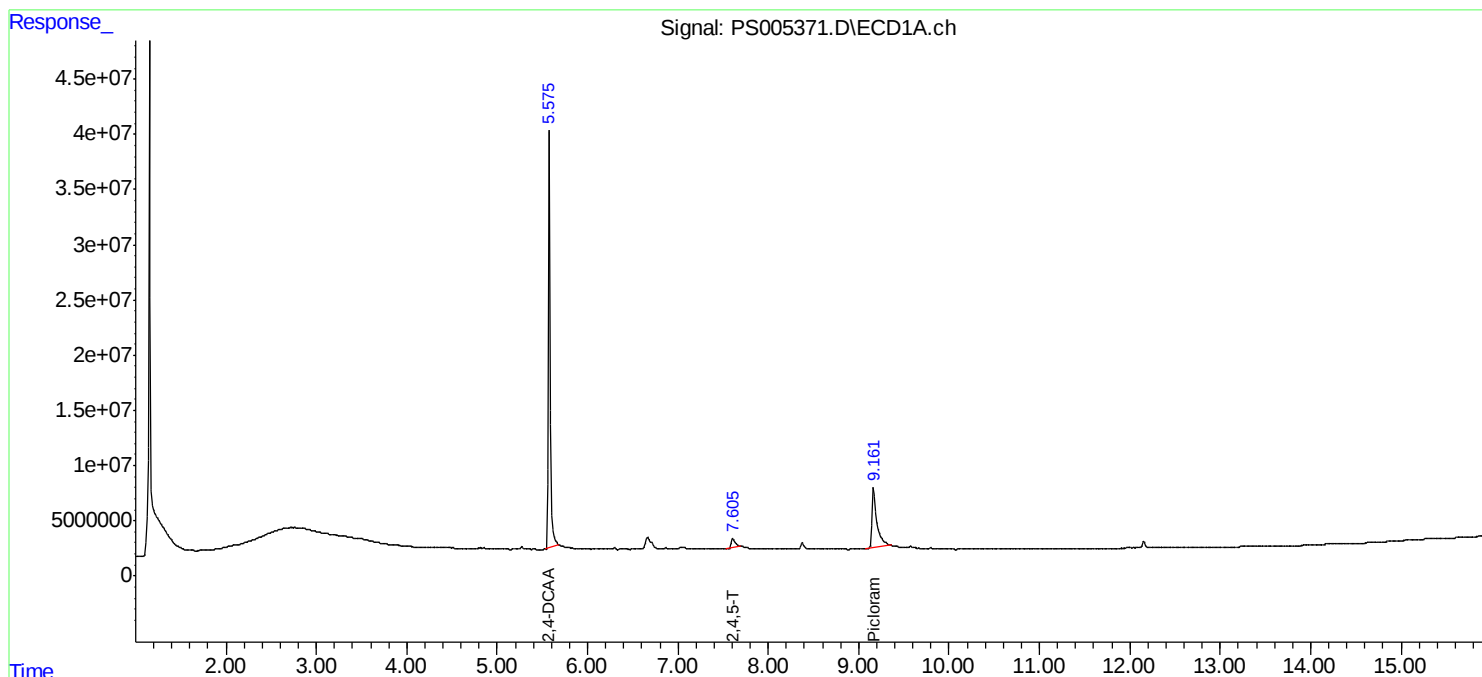


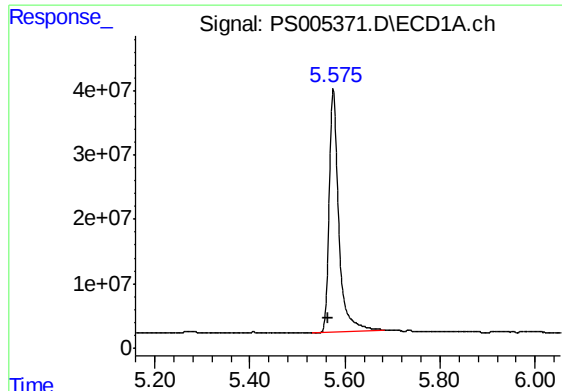

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: 0.012 min
Response: 522941696
Conc: 356.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121021TB

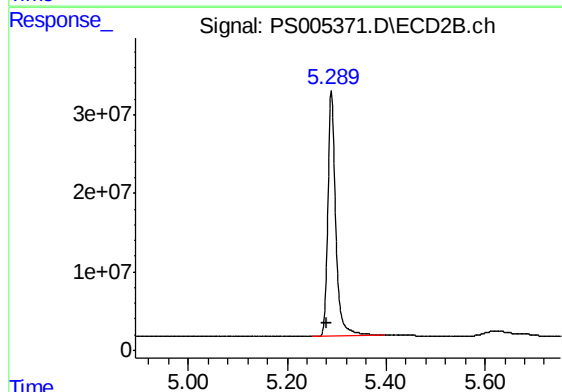


#4 2,4-DCAA

R.T.: 5.290 min
Delta R.T.: 0.010 min
Response: 347270517
Conc: 346.45 ng/ml

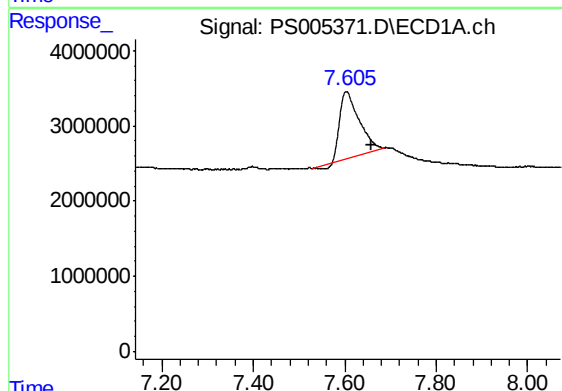


#12 2,4,5-T

R.T.: 7.604 min
Delta R.T.: -0.055 min
Response: 25393848
Conc: 3.16 ng/ml

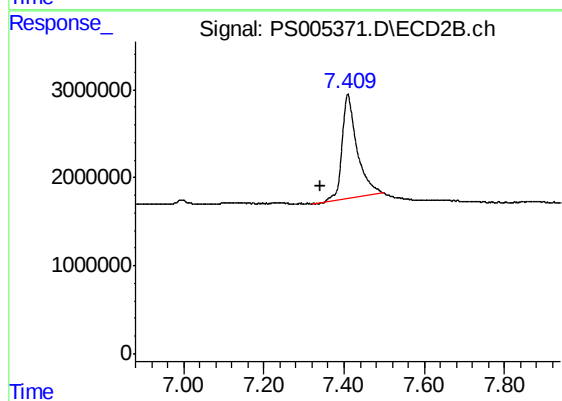

#12 2,4,5-T


R.T.: 7.409 min
Delta R.T.: 0.069 min
Response: 30387144
Conc: 5.96 ng/ml

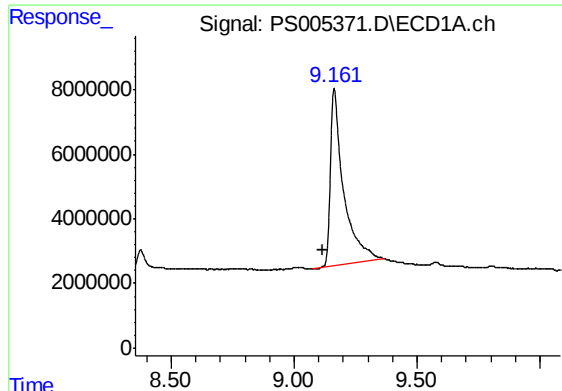

#15 Picloram


R.T.: 9.162 min
Delta R.T.: 0.046 min
Response: 203759991
Conc: 17.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121021TB

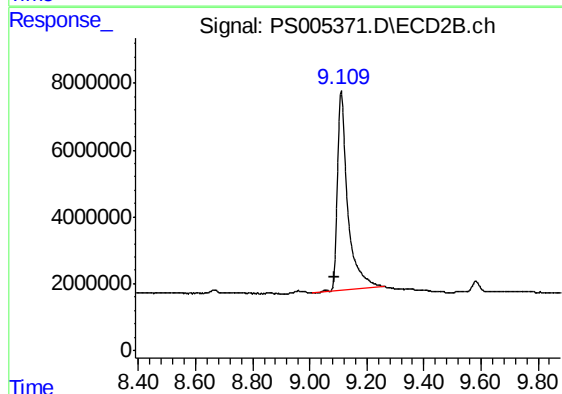


#15 Picloram

R.T.: 9.110 min
Delta R.T.: 0.025 min
Response: 149176792
Conc: 19.77 ng/ml

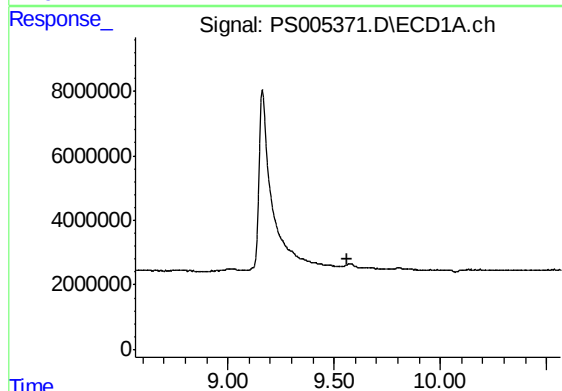

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

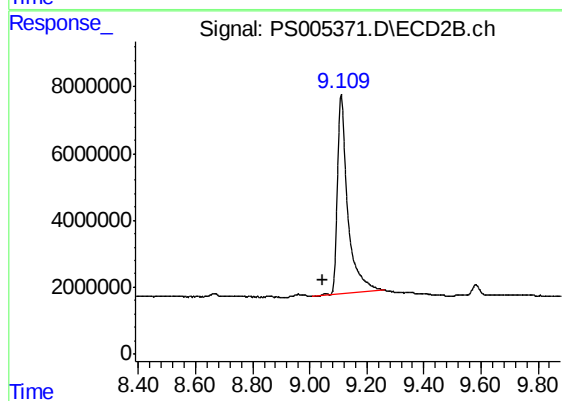

#16 DCPA

R.T.: 9.110 min
Delta R.T.: 0.064 min
Response: 149176792
Conc: 21.91 ng/ml