

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
 Data File : PS005372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 12:08
 Operator : SM\AJ
 Sample : K3634-03RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HJDC-COMP-2RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 15:25:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.605	5.323	307.8E6	205.7E6	209.706	205.225
Target Compounds							
2) T	3,5-DICHL...	0.000	4.641	0	225.9E6	N.D.	171.314
3) T	4-Nitroph...	0.000	4.888	0	55928167	N.D.	111.533
5) T	DICAMBA	0.000	5.429	0	6198128	N.D.	1.656
7) T	MCPA	0.000	5.656	0	9492995	N.D.	2.343
8) T	DICHLORPROP	0.000	6.012	0	33280181	N.D.	34.468
10) T	Pentachlo...	0.000	6.588	0	17602254	N.D.	1.369
11) T	2,4,5-TP ...	0.000	6.975	0	100.5E6	N.D.	18.870
12) T	2,4,5-T	7.624	0.000	286.7E6	0	35.622	N.D. #
15) T	Picloram	9.169	9.133	492.2E6	319.2E6	42.830	42.296



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
Data File : PS005372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 12:08
Operator : SM\AJ
Sample : K3634-03RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 15:25:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

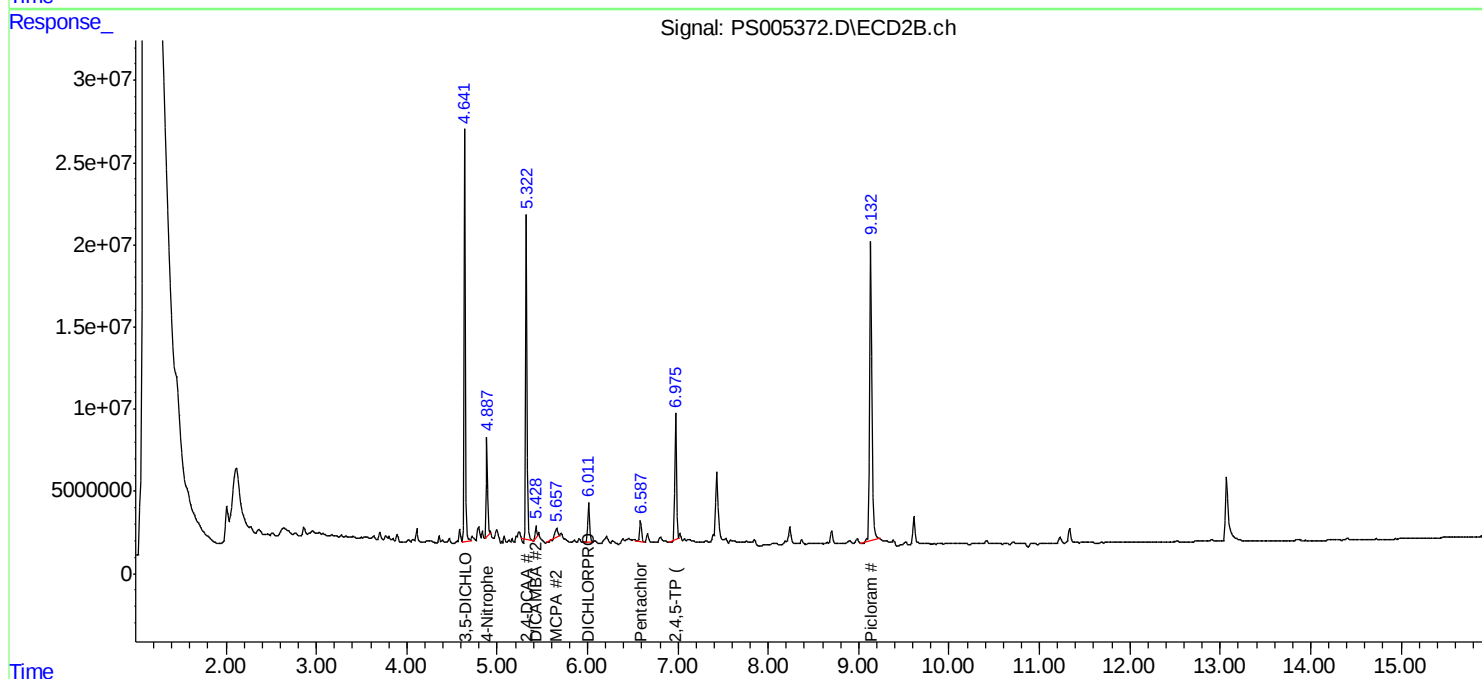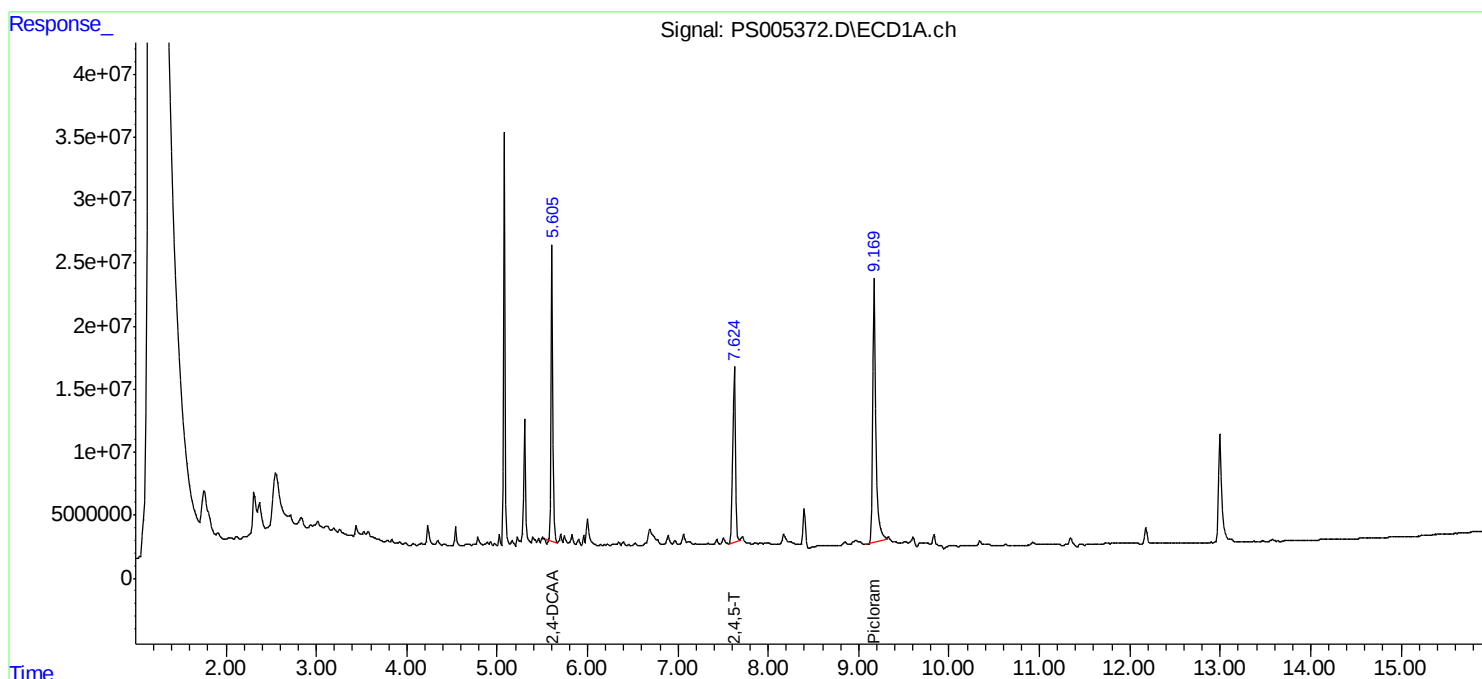


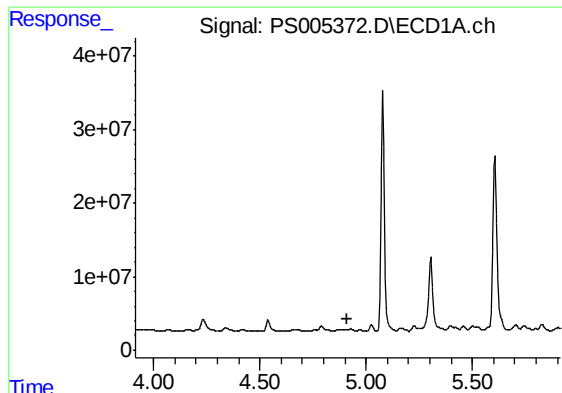

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

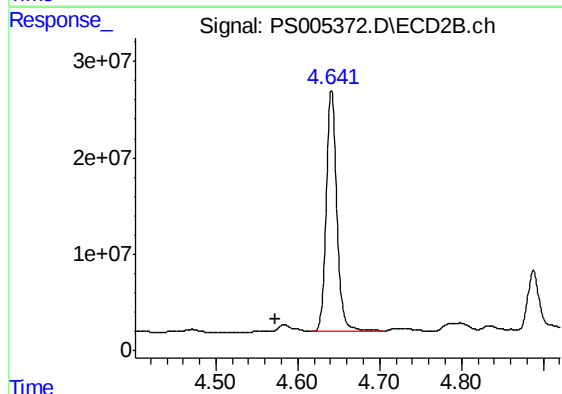


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.641 min
Delta R.T.: 0.069 min
Response: 225913509
Conc: 171.31 ng/ml

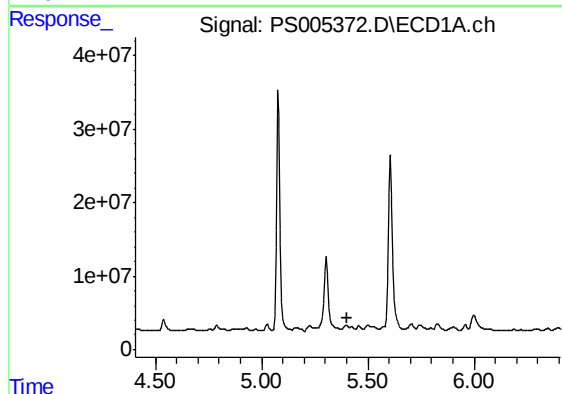


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.406 min
Response: 0
Conc: N.D.

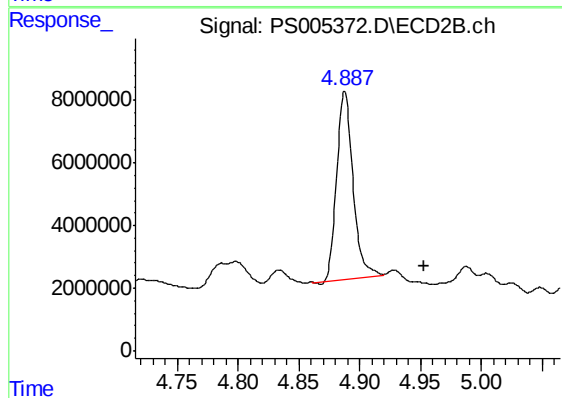

#3 4-Nitrophenol


R.T.: 4.888 min
Delta R.T.: -0.065 min
Response: 55928167
Conc: 111.53 ng/ml

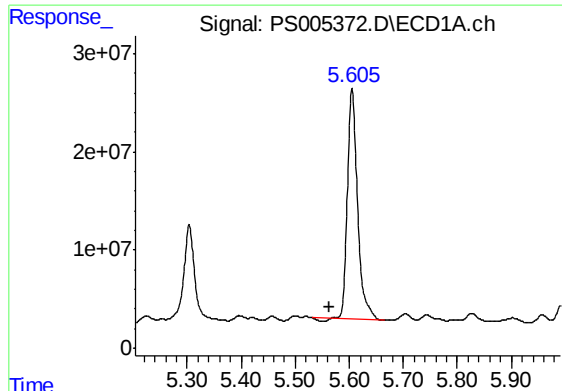

#4 2,4-DCAA


R.T.: 5.605 min
Delta R.T.: 0.042 min
Response: 307825401
Conc: 209.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

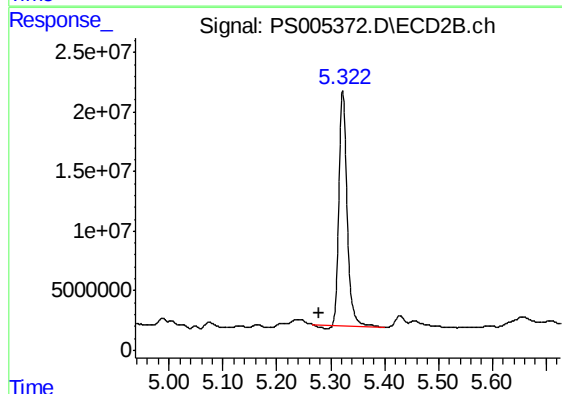


#4 2,4-DCAA

R.T.: 5.323 min
Delta R.T.: 0.043 min
Response: 205711297
Conc: 205.23 ng/ml

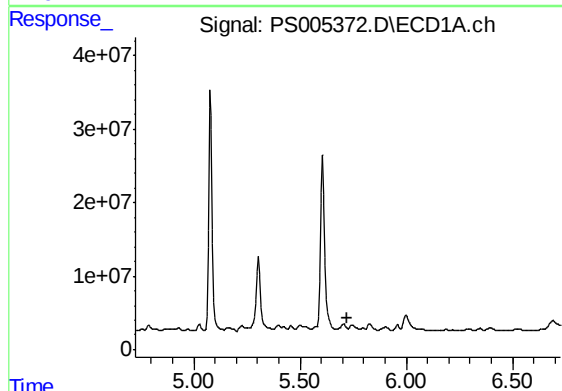


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

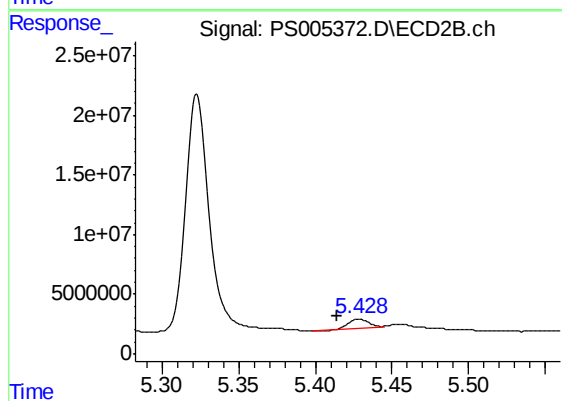

#5 DICAMBA


R.T.: 5.429 min
Delta R.T.: 0.015 min
Response: 6198128
Conc: 1.66 ng/ml

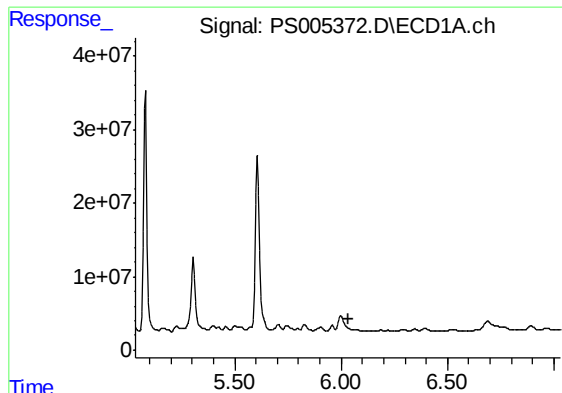

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

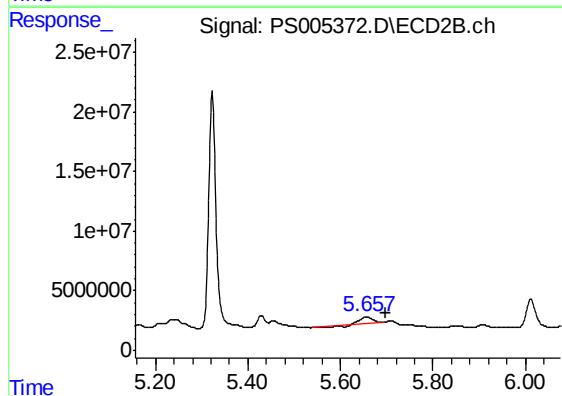


#7 MCPA

R.T.: 5.656 min
Delta R.T.: -0.041 min
Response: 9492995
Conc: 2.34 ug/ml

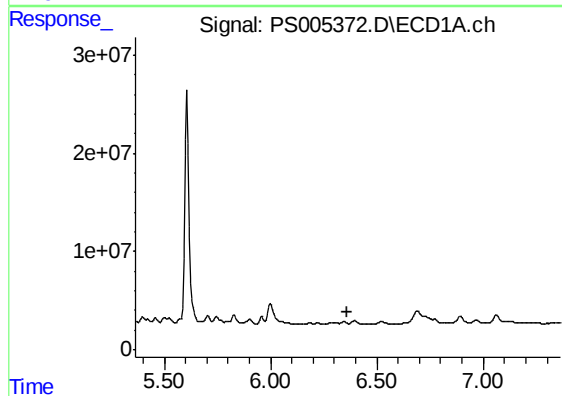


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

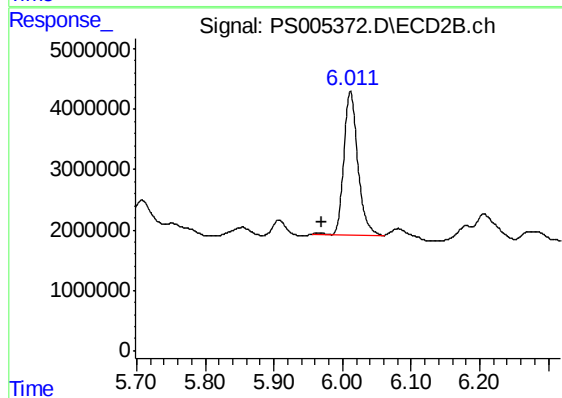

#8 DICHLORPROP


R.T.: 6.012 min
Delta R.T.: 0.043 min
Response: 33280181
Conc: 34.47 ng/ml

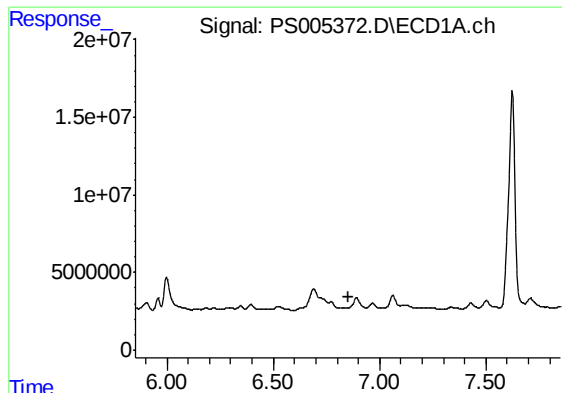

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

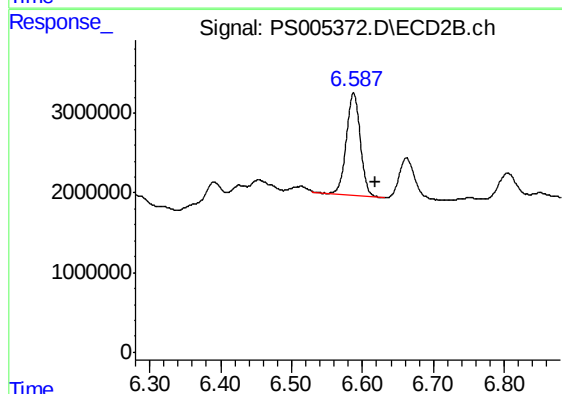


#10 Pentachlorophenol

R.T.: 6.588 min
Delta R.T.: -0.032 min
Response: 17602254
Conc: 1.37 ng/ml

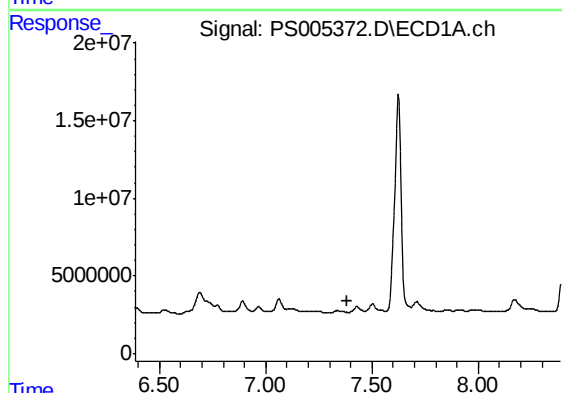


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

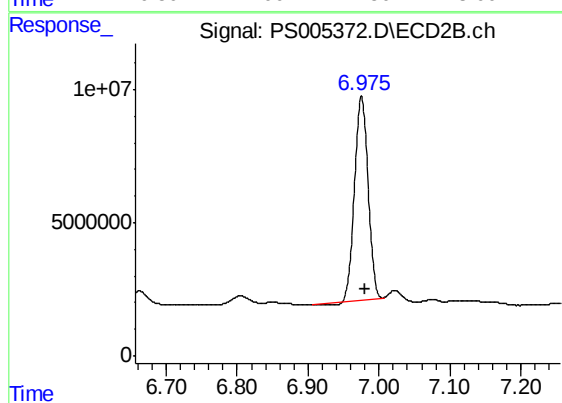

#11 2,4,5-TP (SILVEX)


R.T.: 6.975 min
Delta R.T.: -0.005 min
Response: 100488361
Conc: 18.87 ng/ml

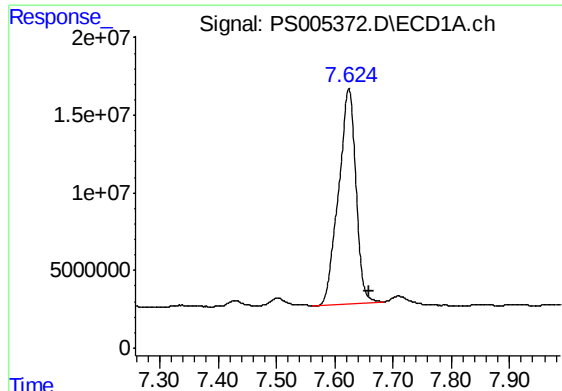

#12 2,4,5-T


R.T.: 7.624 min
Delta R.T.: -0.034 min
Response: 286680004
Conc: 35.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2RE

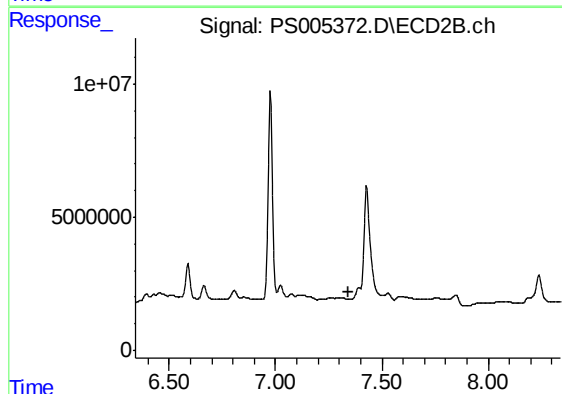


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

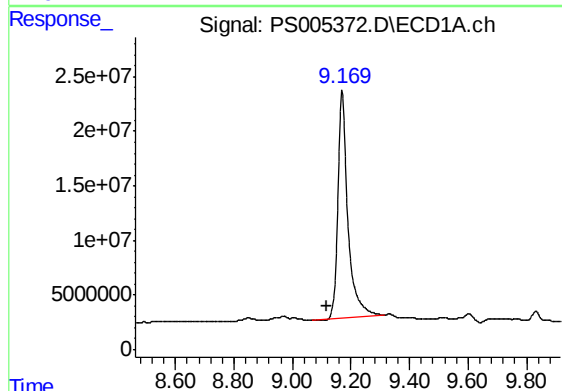

#15 Picloram

R.T.: 9.169 min
Delta R.T.: 0.053 min
Response: 492161928
Conc: 42.83 ng/ml

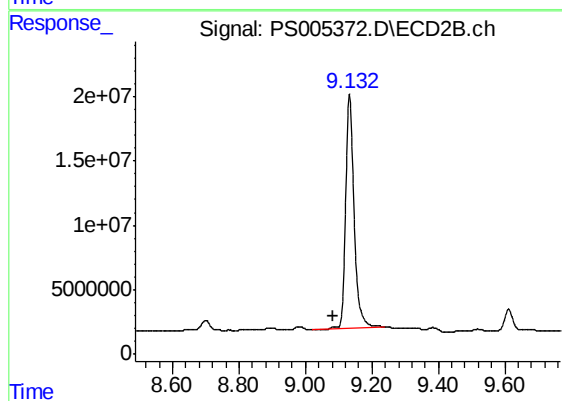

#15 Picloram

R.T.: 9.133 min
Delta R.T.: 0.048 min
Response: 319183052
Conc: 42.30 ng/ml