

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
 Data File : PS005377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 17:07
 Operator : SM\AJ
 Sample : K3628-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VNJ-217-368

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:45:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.585	5.299	372.1E6	215.1E6	253.525	214.552
Target Compounds							
2) T	3,5-DICHL...	0.000	4.618	0 70477455		N.D.	53.444
3) T	4-Nitroph...	5.388	0.000	7667218	0	10.586	N.D. #
5) T	DICAMBA	0.000	5.420	0 21105554		N.D.	5.638
7) T	MCPA	6.077	5.690	14461482	20264242	2.303	5.002 #
8) T	DICHLORPROP	0.000	5.991	0 13006319		N.D.	13.471
9) T	2,4-D	0.000	6.184	0 26198733		N.D.	23.491
10) T	Pentachlo...	6.868	6.641	17732653	11924788	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	6.954	0 28801131		N.D.	5.408
12) T	2,4,5-T	7.683	0.000	29546576	0	3.671	N.D. #
13) T	2,4-DB	8.235	7.870	58129000	34397564	50.045	52.688
15) T	Picloram	0.000	9.119	0 25315895		N.D.	3.355



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
Data File : PS005377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 17:07
Operator : SM\AJ
Sample : K3628-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:45:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

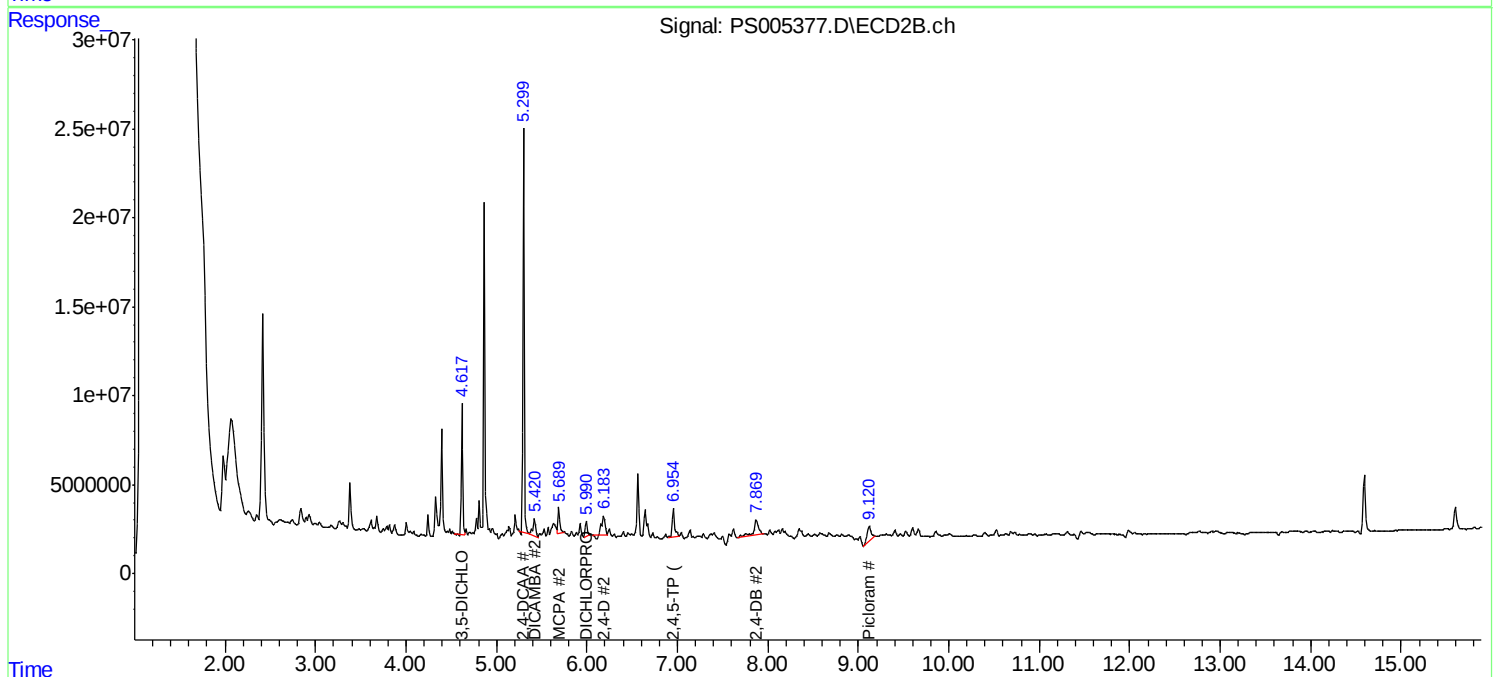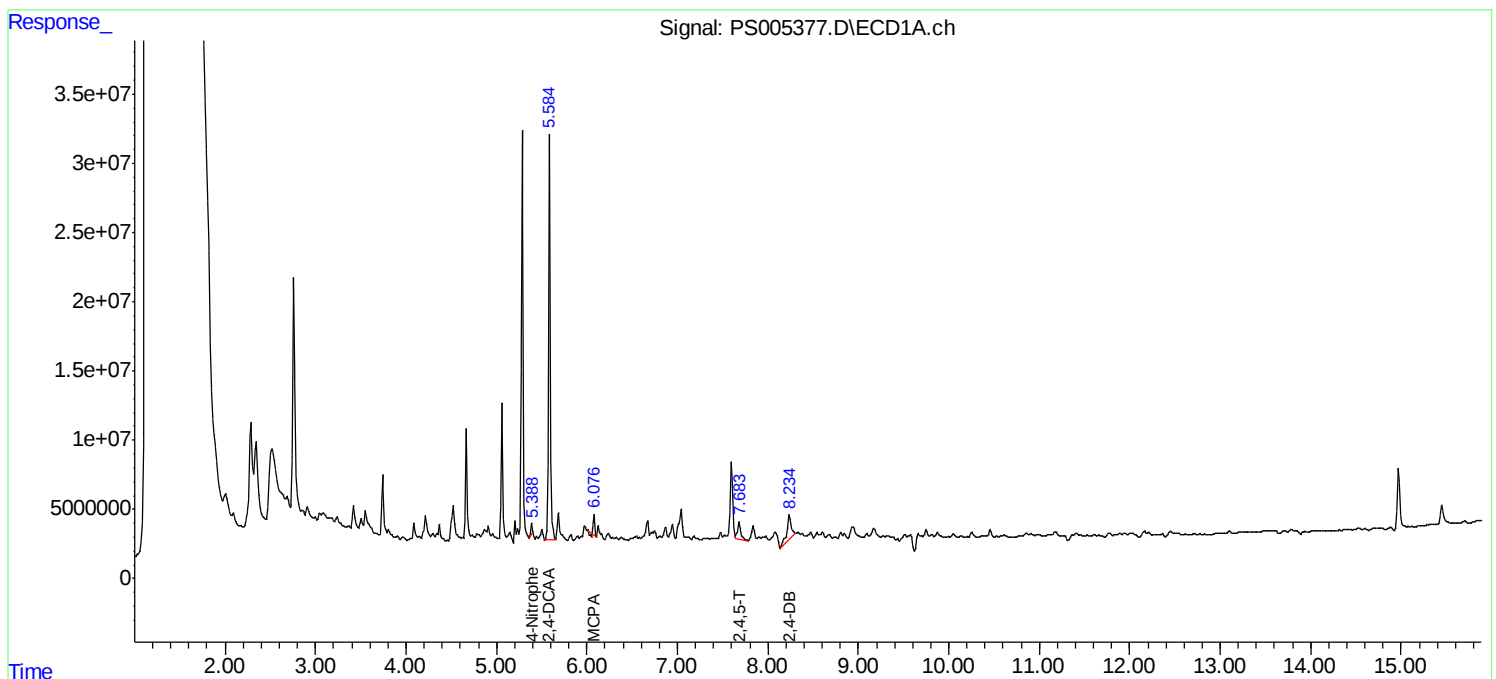


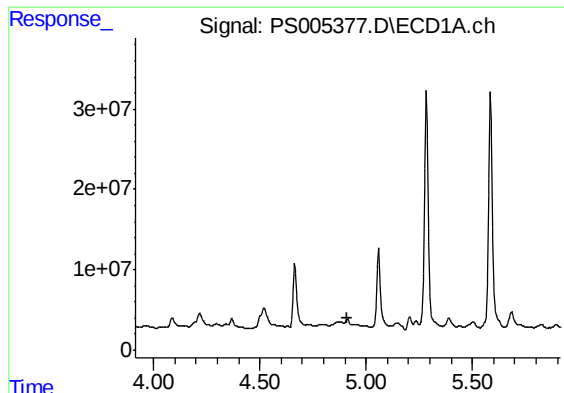

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

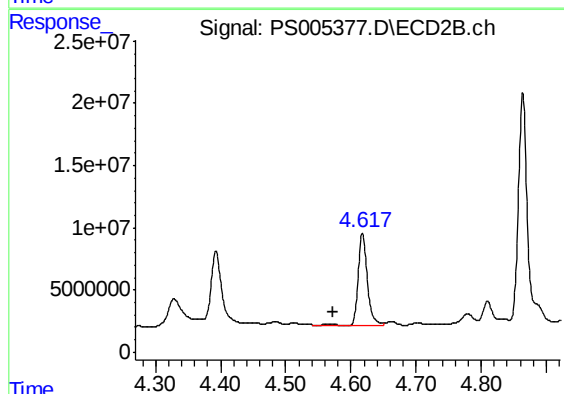


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.618 min
Delta R.T.: 0.045 min
Response: 70477455
Conc: 53.44 ng/ml

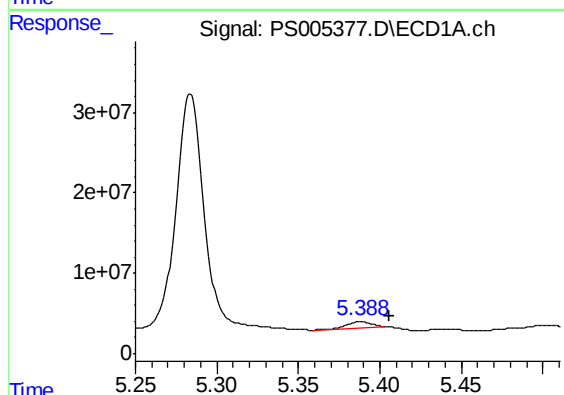


#3 4-Nitrophenol

R.T.: 5.388 min
Delta R.T.: -0.018 min
Response: 7667218
Conc: 10.59 ng/ml

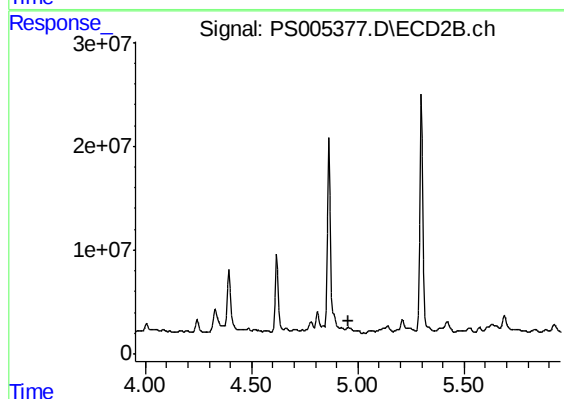

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

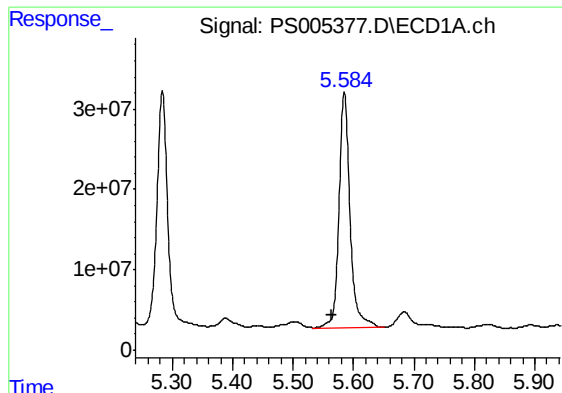

#4 2,4-DCAA


R.T.: 5.585 min
Delta R.T.: 0.021 min
Response: 372148155
Conc: 253.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

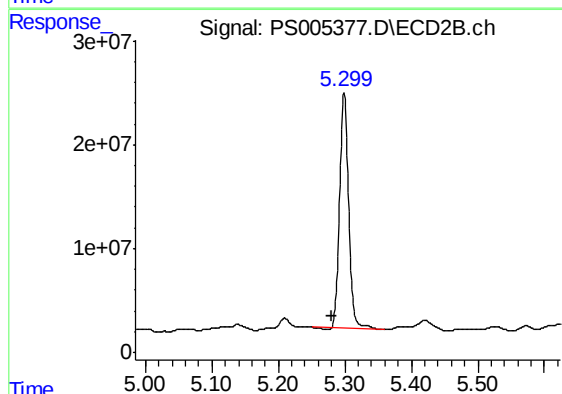


#4 2,4-DCAA

R.T.: 5.299 min
Delta R.T.: 0.019 min
Response: 215059801
Conc: 214.55 ng/ml

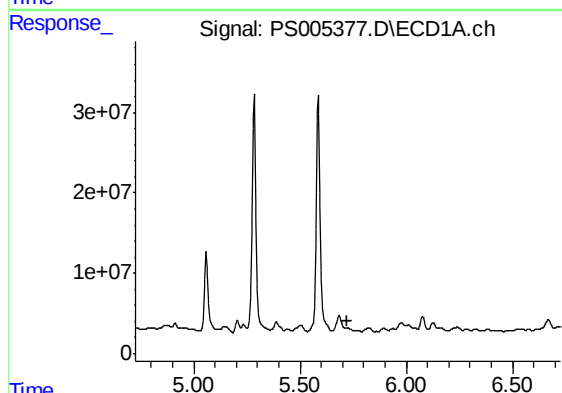


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.725 min
Response: 0
Conc: N.D.

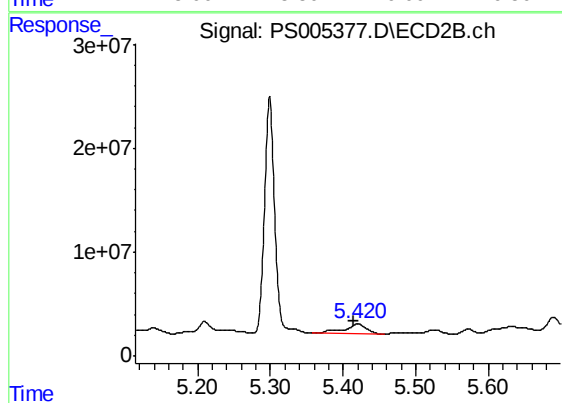

#5 DICAMBA


R.T.: 5.420 min
Delta R.T.: 0.006 min
Response: 21105554
Conc: 5.64 ng/ml

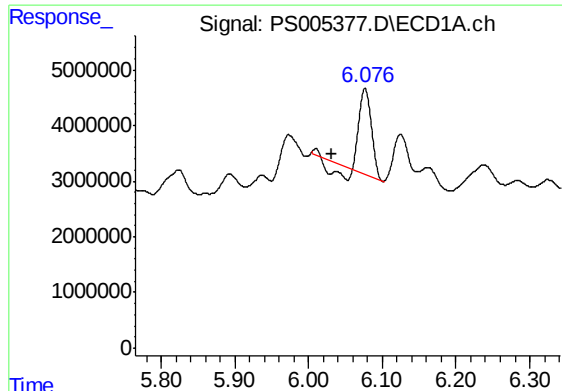

#7 MCPA


R.T.: 6.077 min
Delta R.T.: 0.044 min
Response: 14461482
Conc: 2.30 ug/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

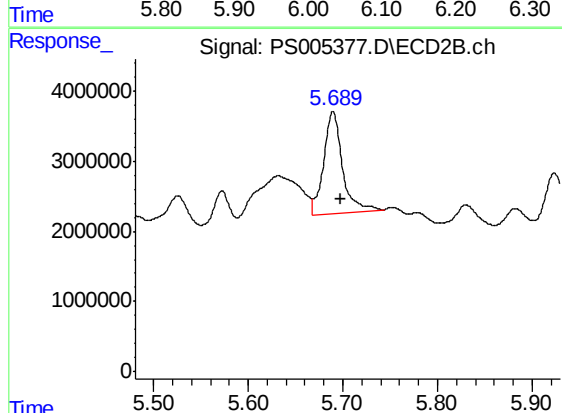


#7 MCPA

R.T.: 5.690 min
Delta R.T.: -0.008 min
Response: 20264242
Conc: 5.00 ug/ml

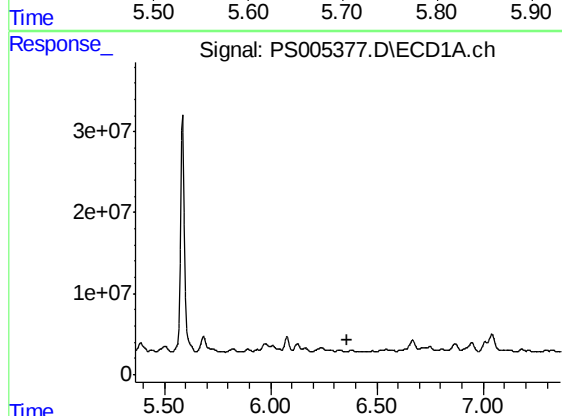


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

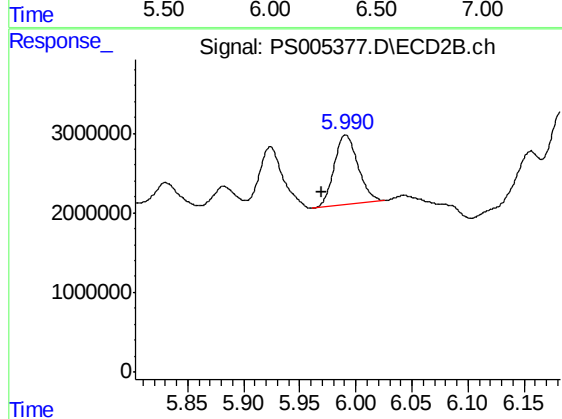

#8 DICHLORPROP


R.T.: 5.991 min
Delta R.T.: 0.022 min
Response: 13006319
Conc: 13.47 ng/ml

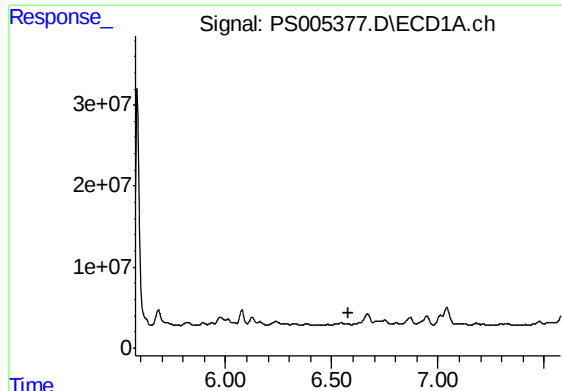

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

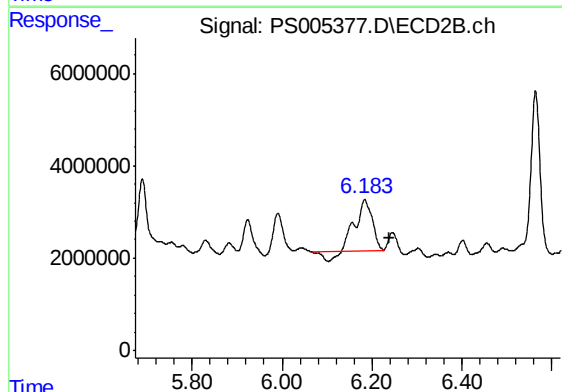


#9 2,4-D

R.T.: 6.184 min
Delta R.T.: -0.056 min
Response: 26198733
Conc: 23.49 ng/ml

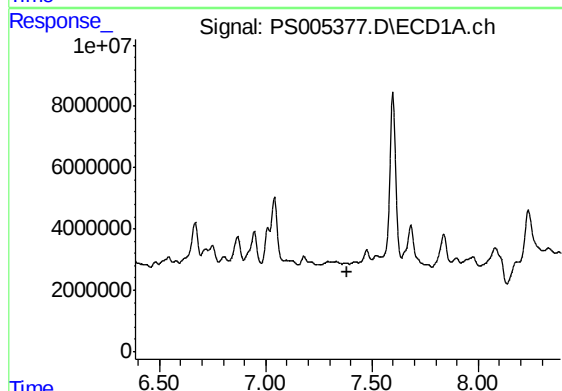


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

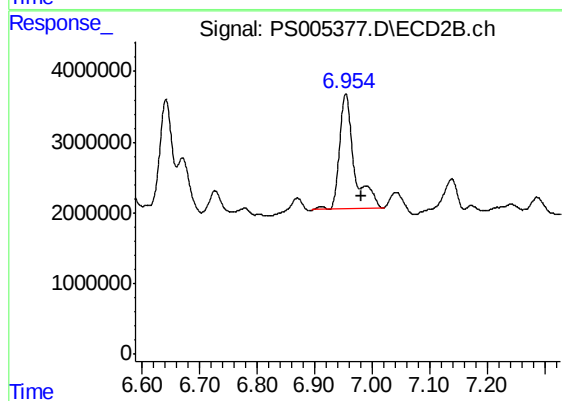

#11 2,4,5-TP (SILVEX)


R.T.: 6.954 min
Delta R.T.: -0.026 min
Response: 28801131
Conc: 5.41 ng/ml

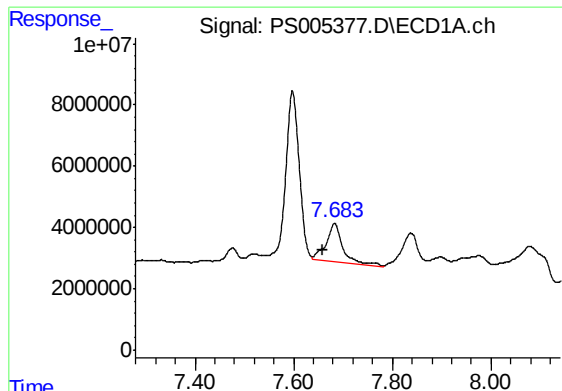

#12 2,4,5-T


R.T.: 7.683 min
Delta R.T.: 0.024 min
Response: 29546576
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

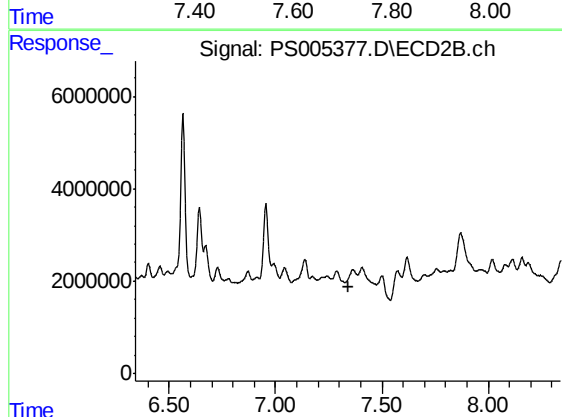


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

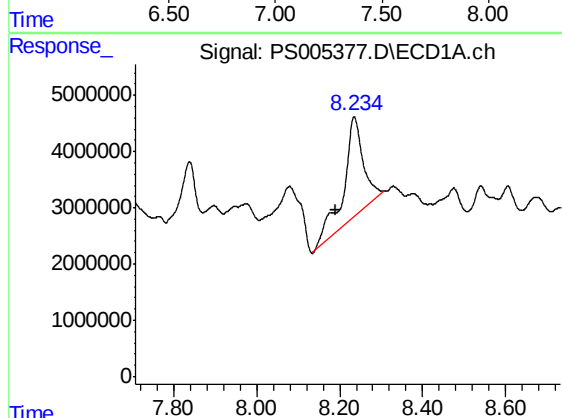


#13 2,4-DB

R.T.: 8.235 min
Delta R.T.: 0.046 min
Response: 58129000
Conc: 50.04 ng/ml

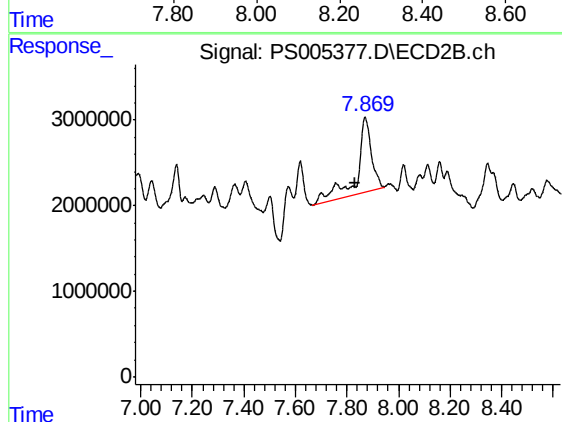

#13 2,4-DB


R.T.: 7.870 min
Delta R.T.: 0.041 min
Response: 34397564
Conc: 52.69 ng/ml

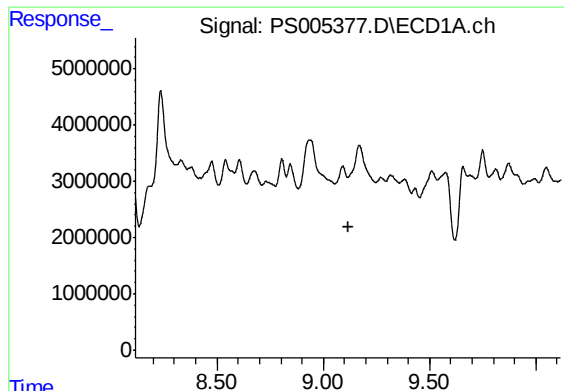

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-217-368

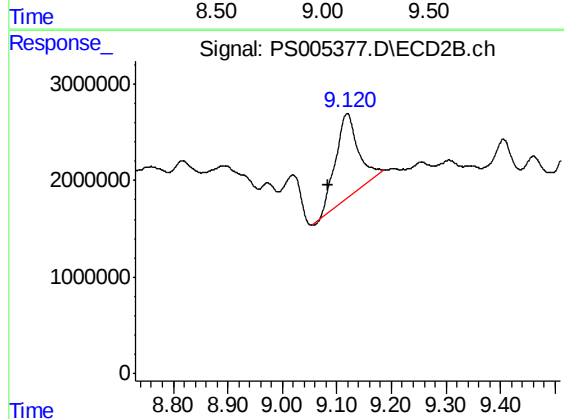

#15 Picloram

R.T.: 9.119 min
Delta R.T.: 0.034 min
Response: 25315895
Conc: 3.35 ng/ml