

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
 Data File : PS005379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 17:51
 Operator : SM\AJ
 Sample : K3628-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VNJ-231-VNJ-236-345

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:45:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.305	444.0E6	260.1E6	302.482	259.515
Target Compounds							
2) T	3,5-DICHL...	0.000	4.623	0	115.8E6	N.D.	87.833
5) T	DICAMBA	0.000	5.425	0	20539556	N.D.	5.487
7) T	MCPA	6.083	5.696	20735021	21874718	3.302	5.400 #
9) T	2,4-D	0.000	6.189	0	32352171	N.D.	29.008
10) T	Pentachlo...	0.000	6.570	0	56827843	N.D.	4.420
11) T	2,4,5-TP ...	0.000	6.960	0	32581726	N.D.	6.118
12) T	2,4,5-T	7.687	0.000	53613097	0	6.662	N.D. #
13) T	2,4-DB	8.243	0.000	67507329	0	58.119	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
Data File : PS005379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 17:51
Operator : SM\AJ
Sample : K3628-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:45:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

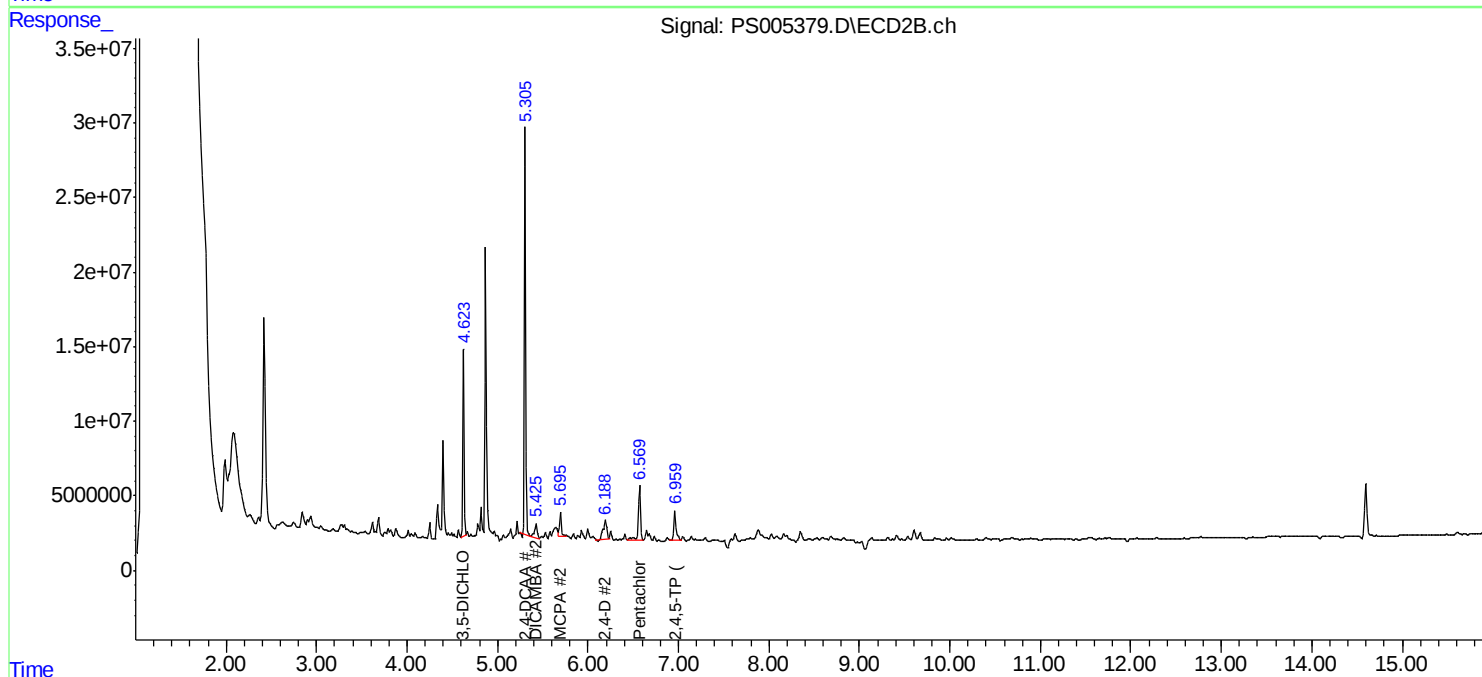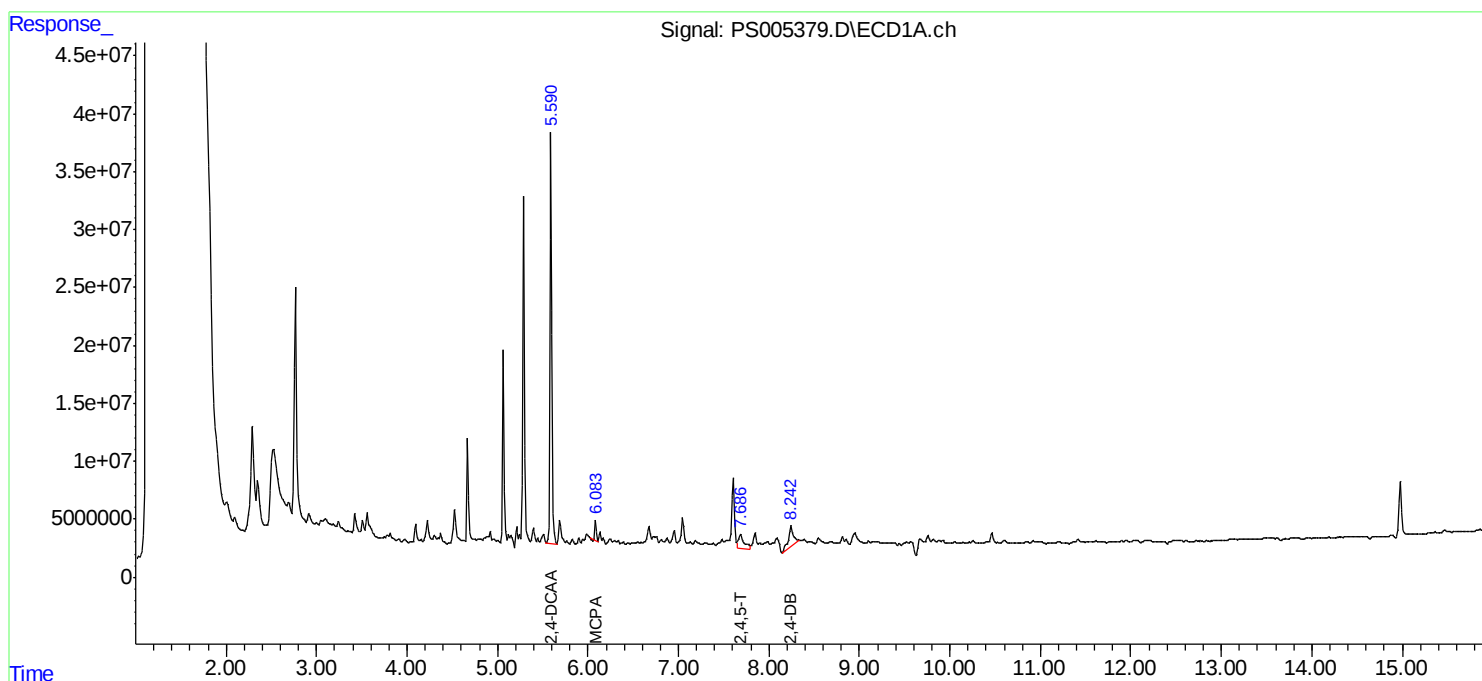


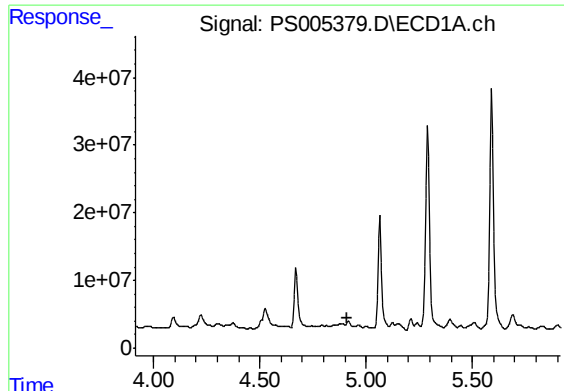

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

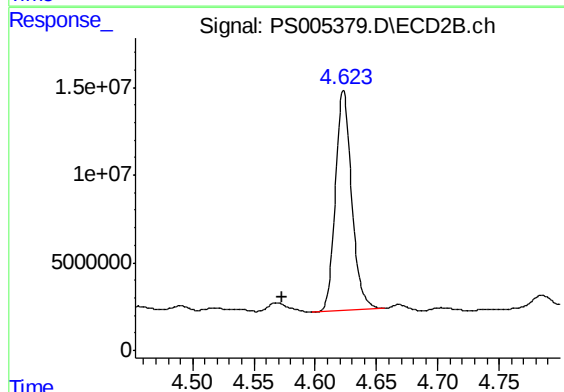


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.623 min
Delta R.T.: 0.051 min
Response: 115826816
Conc: 87.83 ng/ml

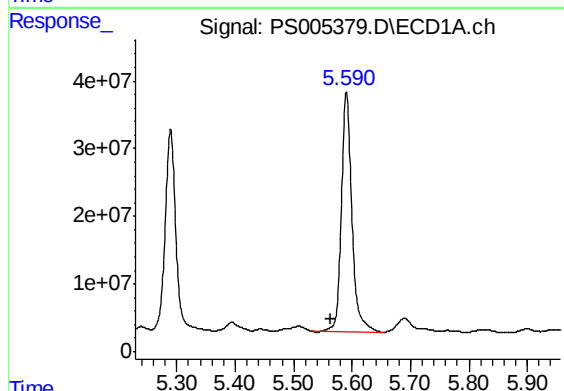


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: 0.027 min
Response: 444011029
Conc: 302.48 ng/ml

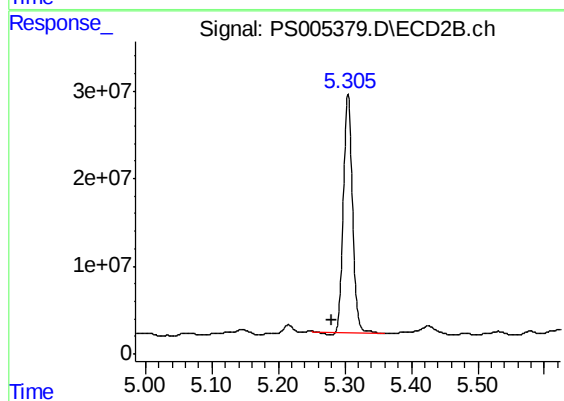

#4 2,4-DCAA


R.T.: 5.305 min
Delta R.T.: 0.025 min
Response: 260129933
Conc: 259.52 ng/ml

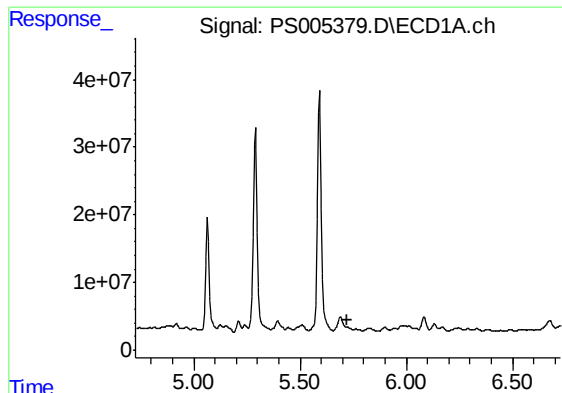

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

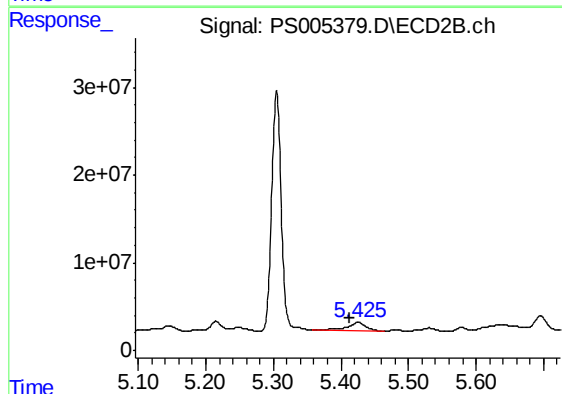


#5 DICAMBA

R.T.: 5.425 min
Delta R.T.: 0.011 min
Response: 20539556
Conc: 5.49 ng/ml

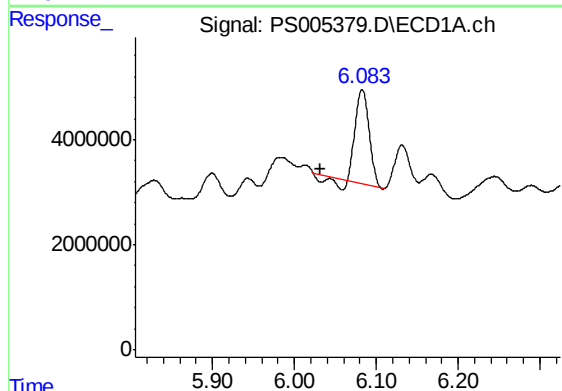


#7 MCPA

R.T.: 6.083 min
Delta R.T.: 0.051 min
Response: 20735021
Conc: 3.30 ug/ml

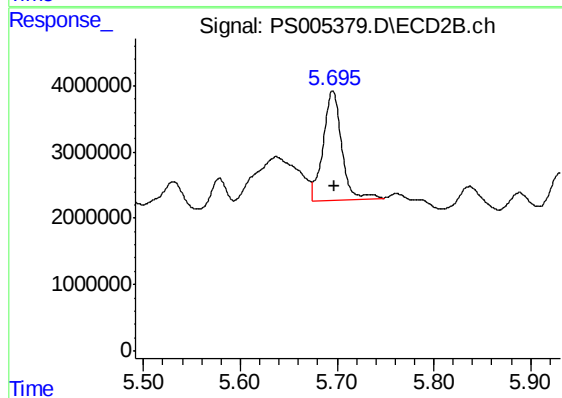

#7 MCPA


R.T.: 5.696 min
Delta R.T.: -0.002 min
Response: 21874718
Conc: 5.40 ug/ml

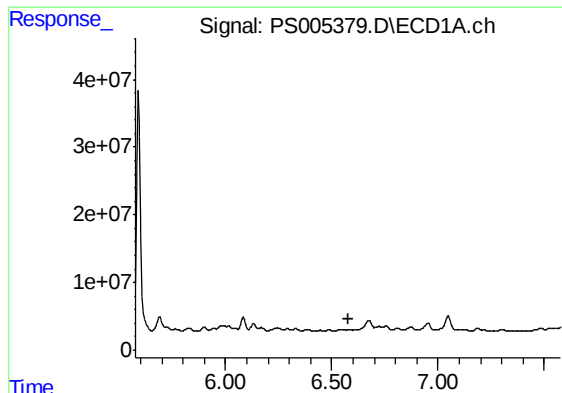

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

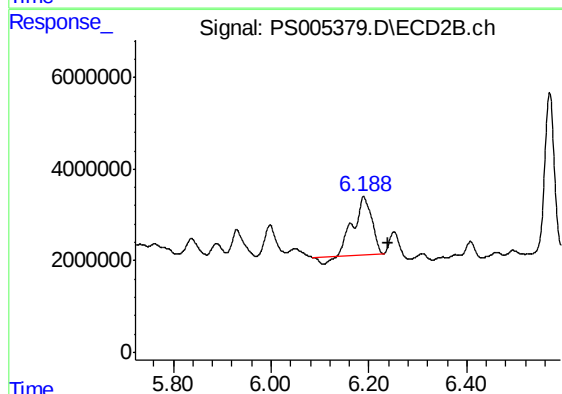


#9 2,4-D

R.T.: 6.189 min
Delta R.T.: -0.050 min
Response: 32352171
Conc: 29.01 ng/ml

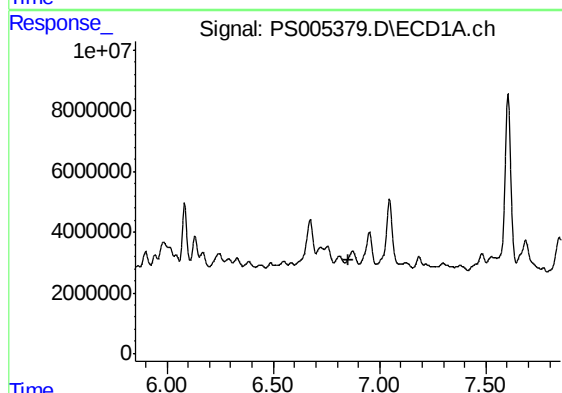


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

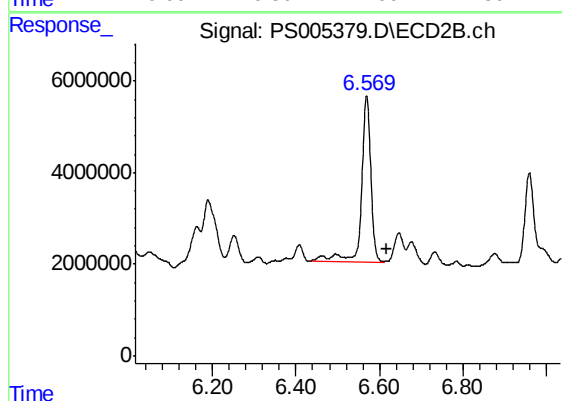

#10 Pentachlorophenol


R.T.: 6.570 min
Delta R.T.: -0.049 min
Response: 56827843
Conc: 4.42 ng/ml

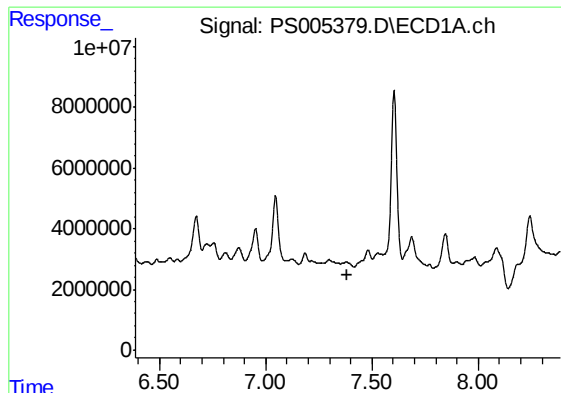

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

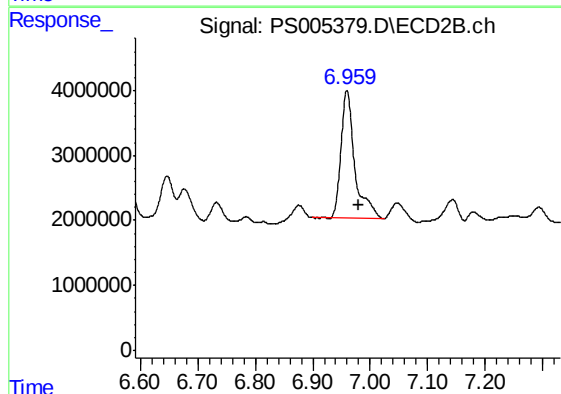


#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.021 min
Response: 32581726
Conc: 6.12 ng/ml

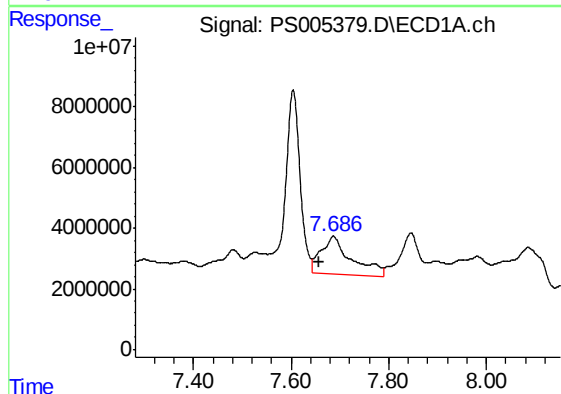


#12 2,4,5-T

R.T.: 7.687 min
Delta R.T.: 0.028 min
Response: 53613097
Conc: 6.66 ng/ml

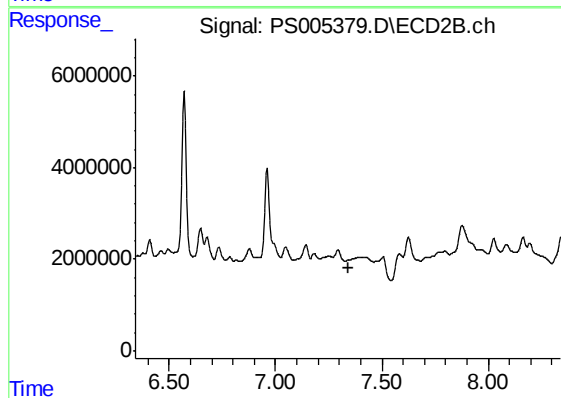

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

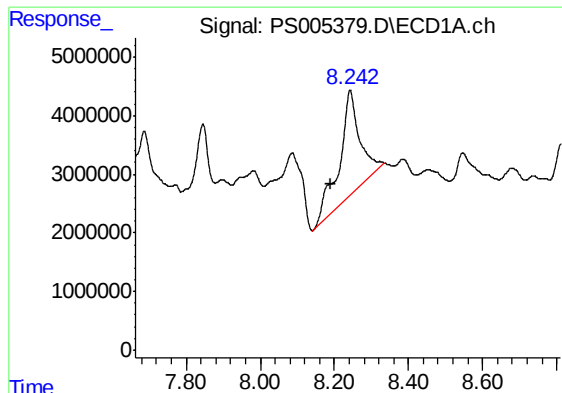

#13 2,4-DB

R.T.: 8.243 min
Delta R.T.: 0.053 min
Response: 67507329
Conc: 58.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-231-VNJ-236-345

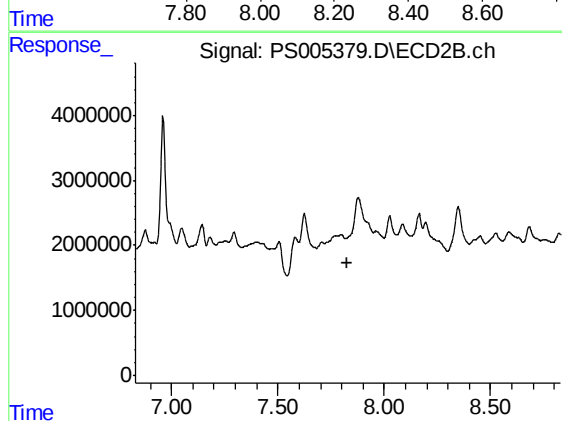

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.830 min
Response: 0
Conc: N.D.