

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
 Data File : PS005378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2019 17:29
 Operator : SM\AJ
 Sample : K3628-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VNJ-226-VNJ-238

Manual Integrations
 APPROVED

Ankita
 7/8/2019 9:57:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 00:45:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.590	5.304	347.0E6	210.0E6	236.367	209.549m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070319\
Data File : PS005378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2019 17:29
Operator : SM\AJ
Sample : K3628-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
VNJ-226-VNJ-238


Manual Integrations
APPROVED

Ankita
7/8/2019 9:57:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 00:45:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

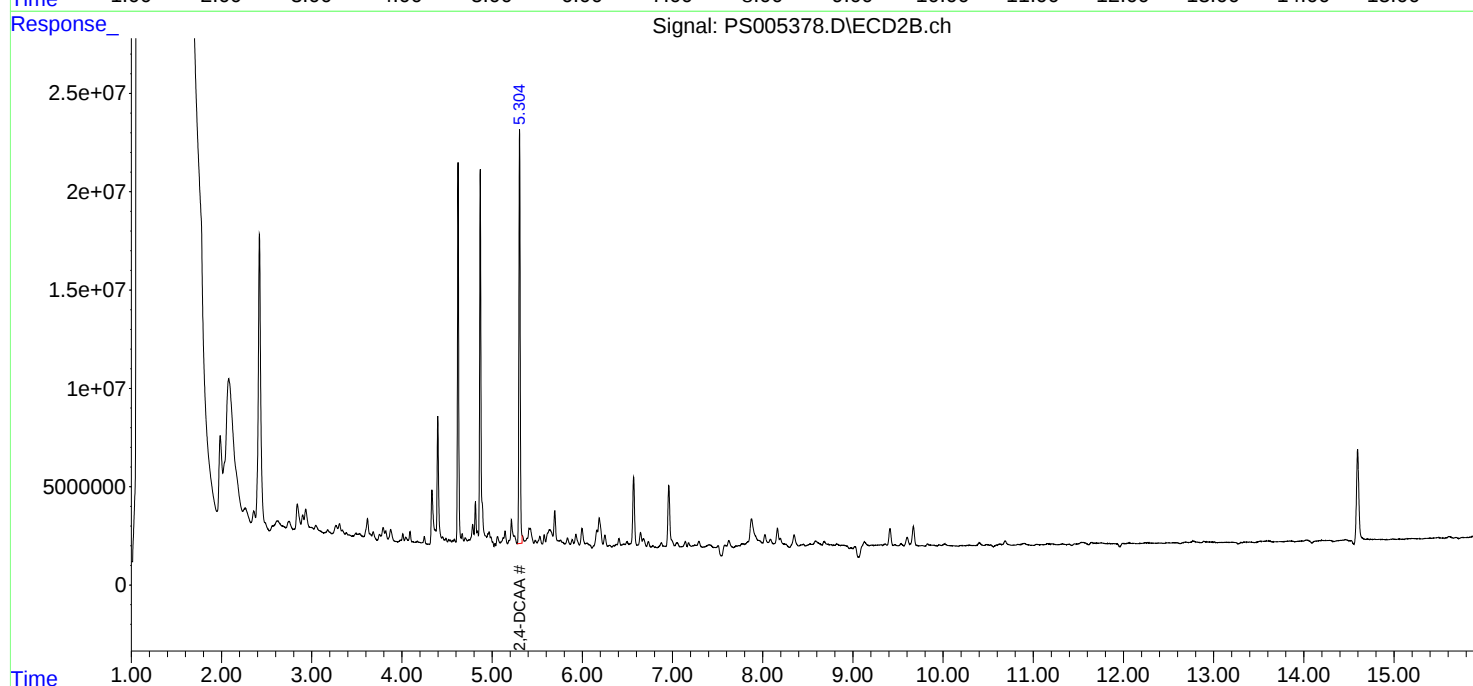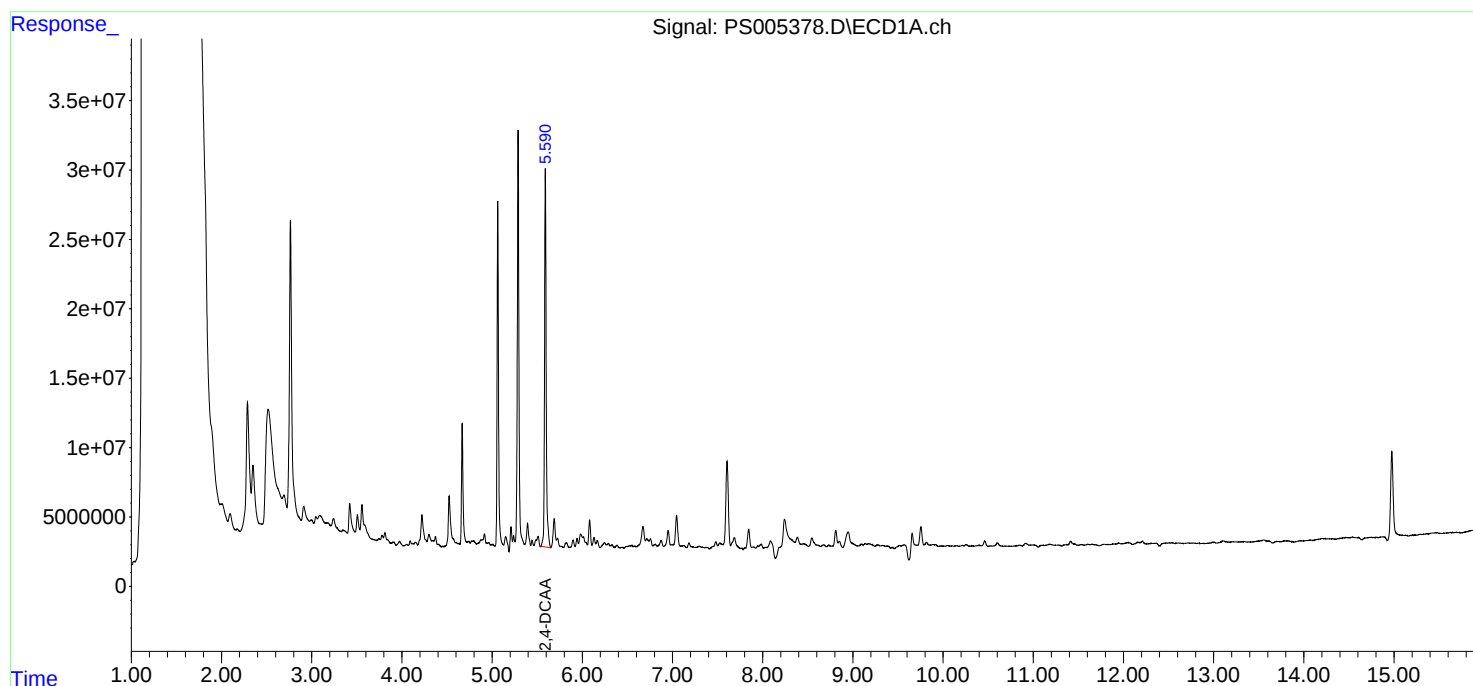

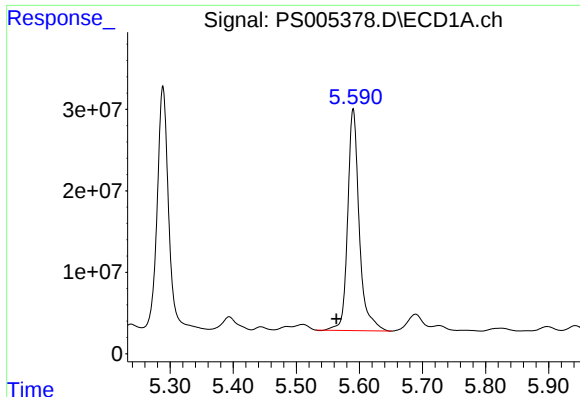


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: 0.027 min
Response: 346961886
Conc: 236.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
VNJ-226-VNJ-238

Manual Integrations
APPROVED

Ankita
7/8/2019 9:57:19 AM

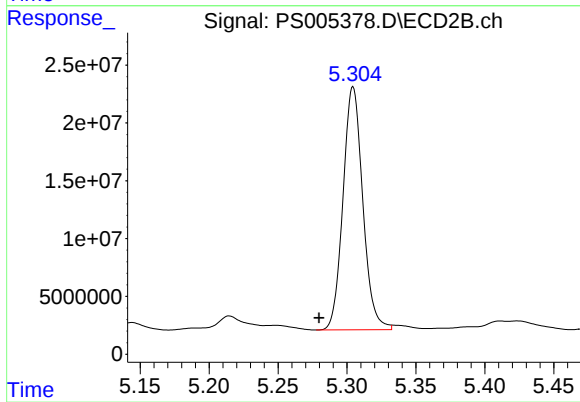

#4 2,4-DCAA

R.T.: 5.304 min
Delta R.T.: 0.024 min
Response: 210045158
Conc: 209.55 ng/ml m