

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 08:53
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 13:24:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.289	528.0E6	350.7E6	359.702	349.904
Target Compounds							
12) T	2,4,5-T	0.000	7.399	0 89025687		N.D.	17.453
14) T	DINOSEB	9.301	0.000	25628941	0	4.010	N.D. #
15) T	Picloram	9.145	9.103	497.8E6	344.1E6	43.317	45.602
16) T	DCPA	0.000	9.103	0 344.1E6		N.D.	50.552



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 08:53
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 13:24:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

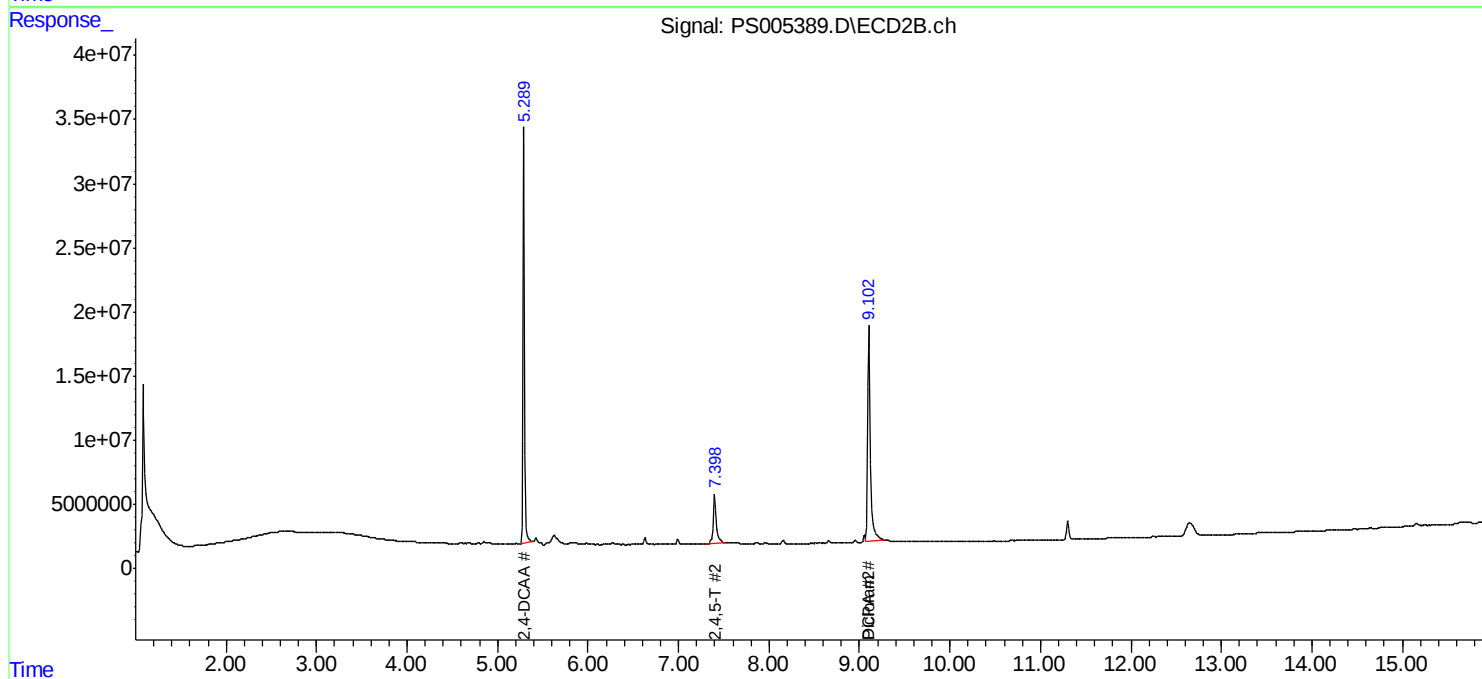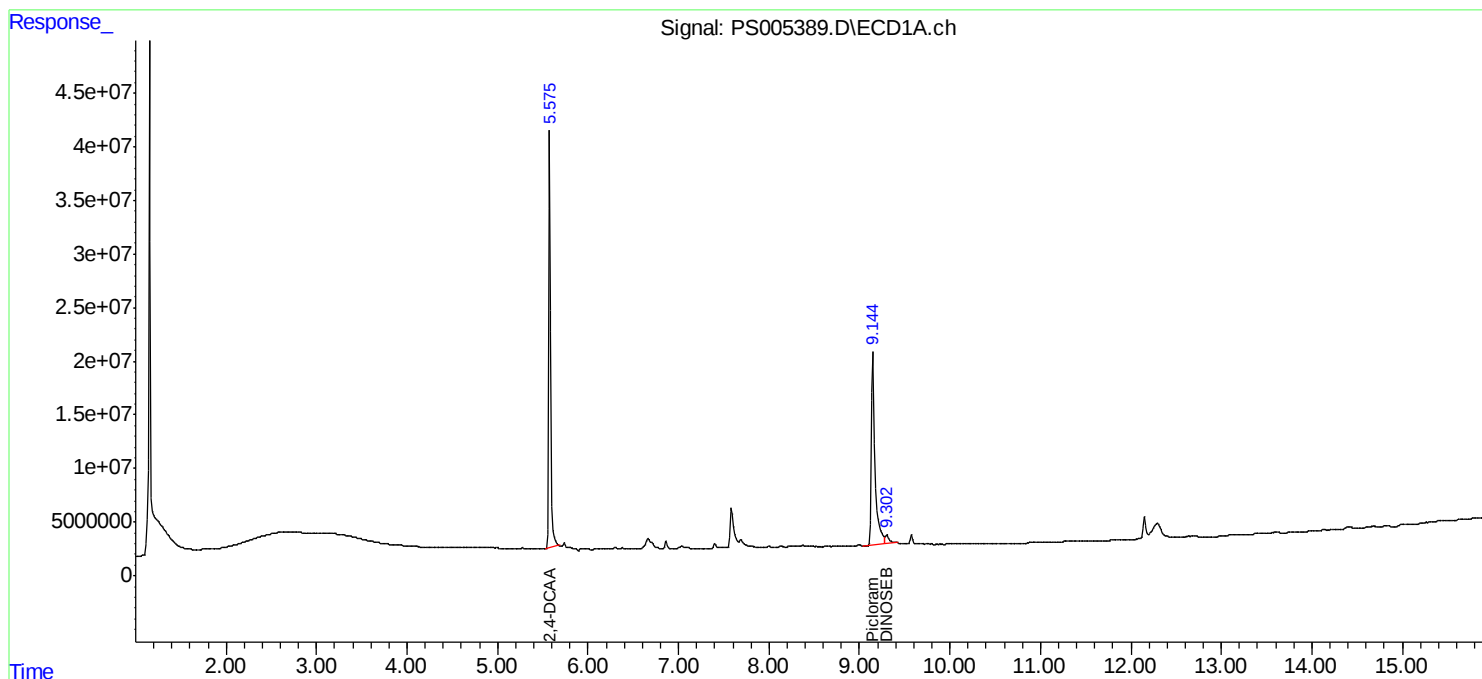


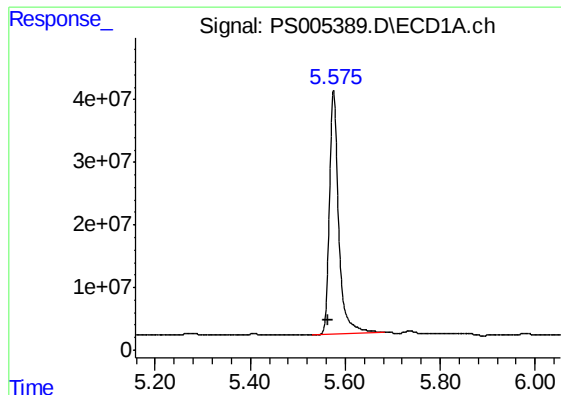

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: 0.012 min
Response: 528003521
Conc: 359.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

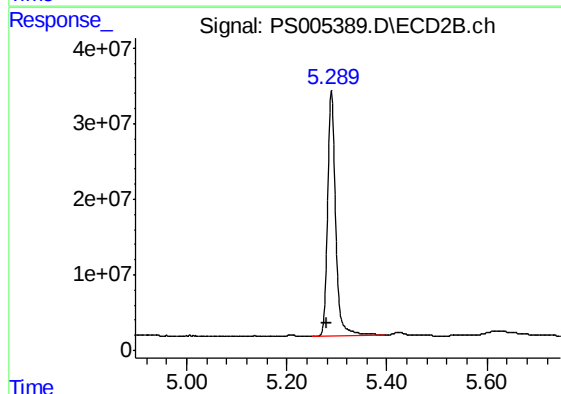


#4 2,4-DCAA

R.T.: 5.289 min
Delta R.T.: 0.009 min
Response: 350732908
Conc: 349.90 ng/ml

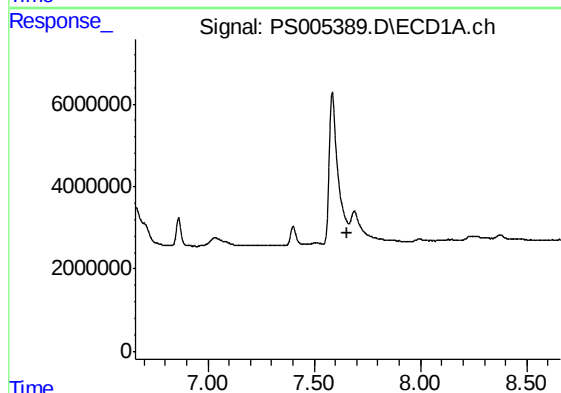


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.659 min
Response: 0
Conc: N.D.

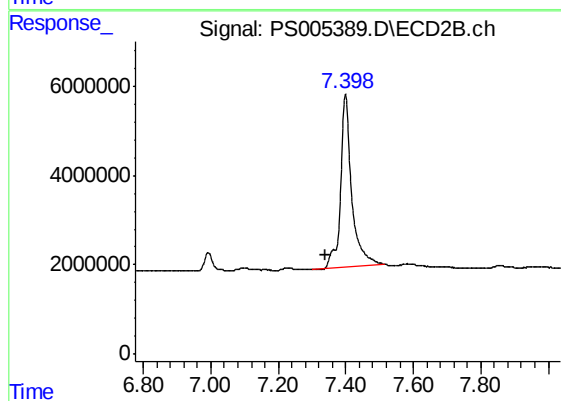

#12 2,4,5-T


R.T.: 7.399 min
Delta R.T.: 0.058 min
Response: 89025687
Conc: 17.45 ng/ml

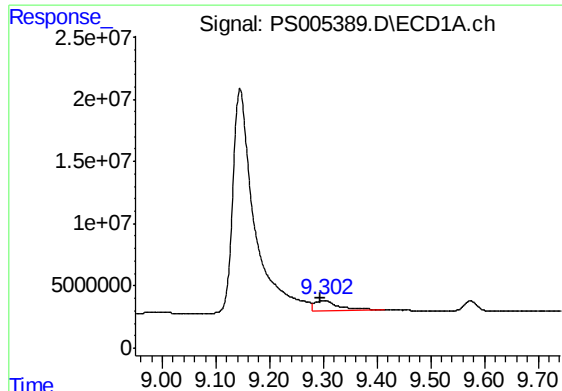

#14 DINOSEB


R.T.: 9.301 min
Delta R.T.: 0.008 min
Response: 25628941
Conc: 4.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

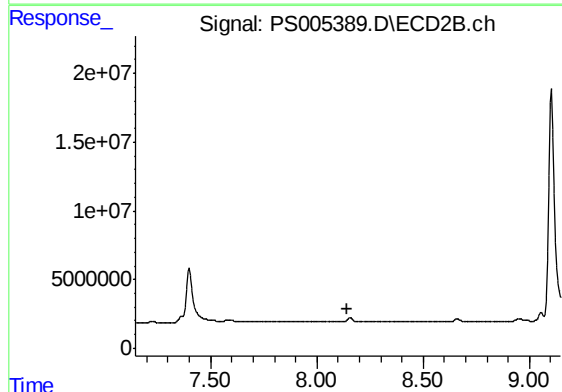


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.146 min
Response: 0
Conc: N.D.

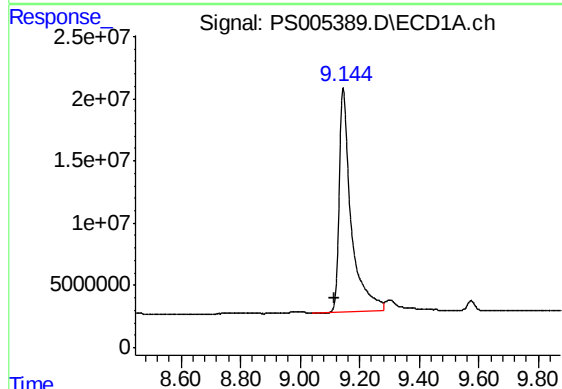


#15 Picloram

R.T.: 9.145 min
Delta R.T.: 0.028 min
Response: 497758296
Conc: 43.32 ng/ml

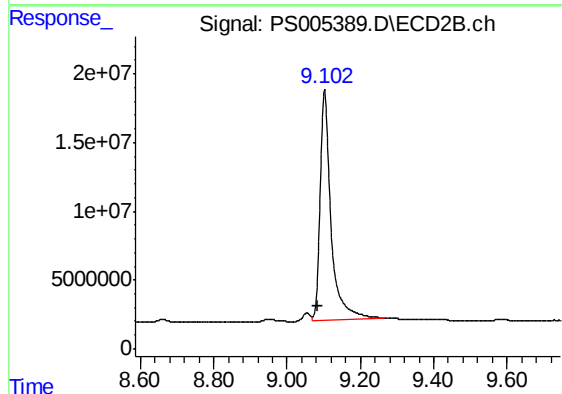

#15 Picloram


R.T.: 9.103 min
Delta R.T.: 0.018 min
Response: 344132023
Conc: 45.60 ng/ml

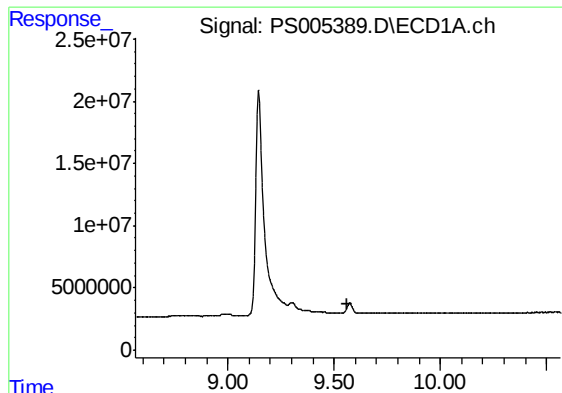

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

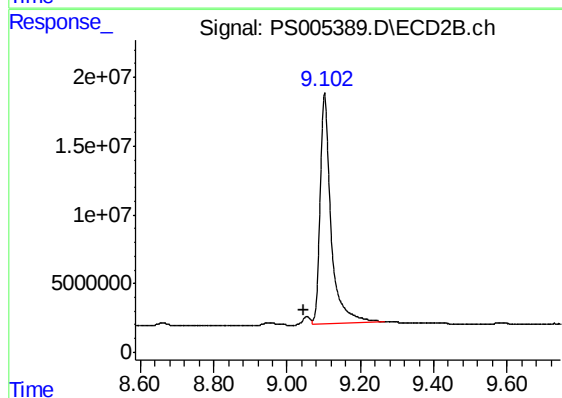

#16 DCPA

R.T.: 9.103 min
Delta R.T.: 0.057 min
Response: 344132023
Conc: 50.55 ng/ml