

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 09:41
 Operator : SM\AJ
 Sample : PB121162BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121162BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 14:10:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.289	825.6E6	548.9E6	562.409	547.581
Target Compounds							
1) T	Dalapon	2.083	0.000	37514051	0	20.352	N.D. #
2) T	3,5-DICHL...	0.000	4.608	0	41991022	N.D.	31.843
5) T	DICAMBA	5.675	0.000	3498885	0	<MDL	N.D. #
7) T	MCPA	6.068	5.679	29730789	29629335	4.734	7.314 #
9) T	2,4-D	0.000	6.173	0	51421175	N.D.	46.106
10) T	Pentachlo...	0.000	6.630	0	17620857	N.D.	1.371
11) T	2,4,5-TP ...	0.000	6.947	0	34729502	N.D.	6.522
12) T	2,4,5-T	0.000	7.396	0	71605584	N.D.	14.038
13) T	2,4-DB	8.232	7.861	105.5E6	54101106	90.825	82.869
15) T	Picloram	9.145	9.101	463.0E6	346.6E6	40.291	45.934
16) T	DCPA	0.000	9.101	0	346.6E6	N.D.	50.920



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 09:41
Operator : SM\AJ
Sample : PB121162BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121162BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 14:10:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

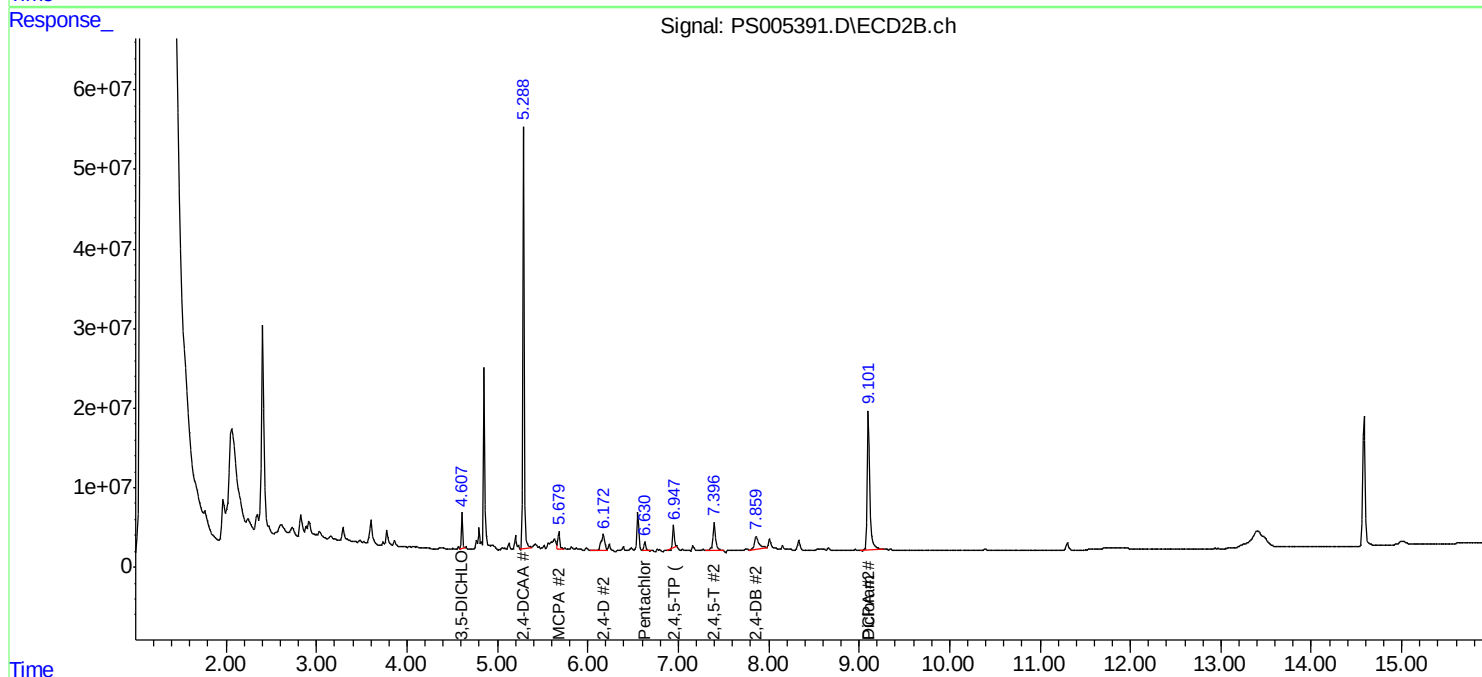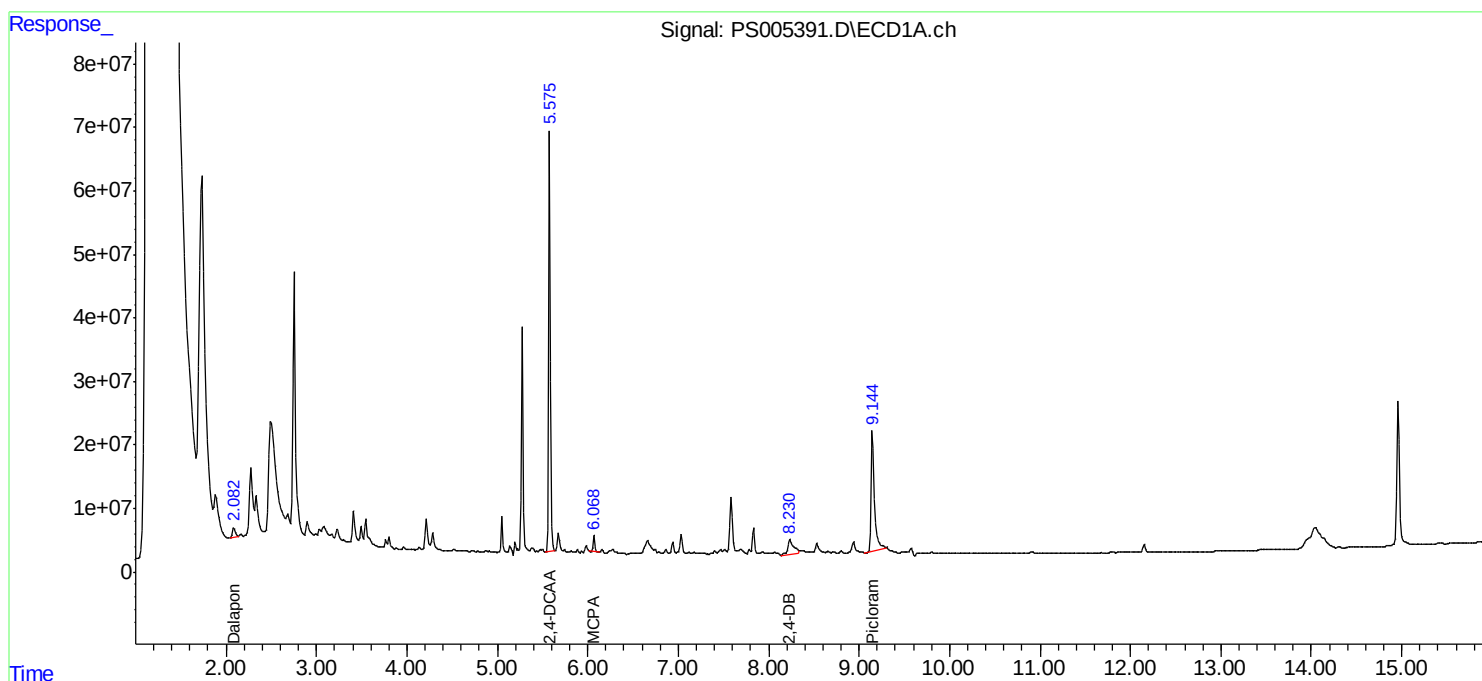


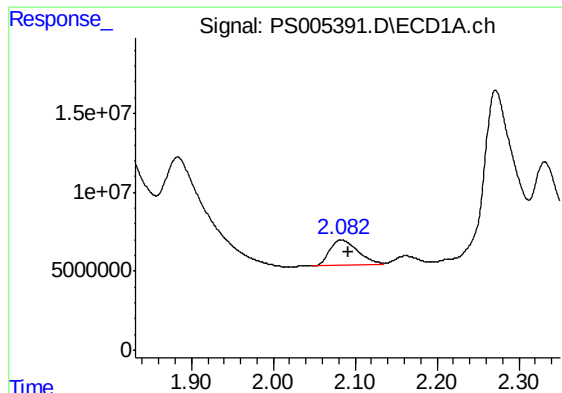

#1 Dalapon


R.T.: 2.083 min
Delta R.T.: -0.009 min
Response: 37514051
Conc: 20.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121162BL

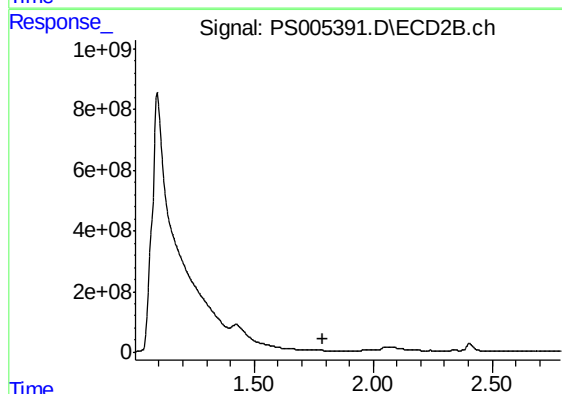


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

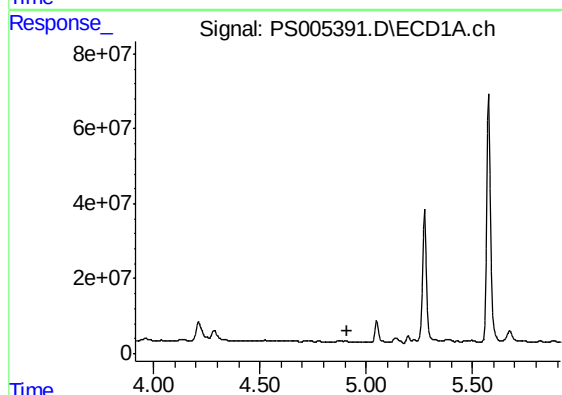


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

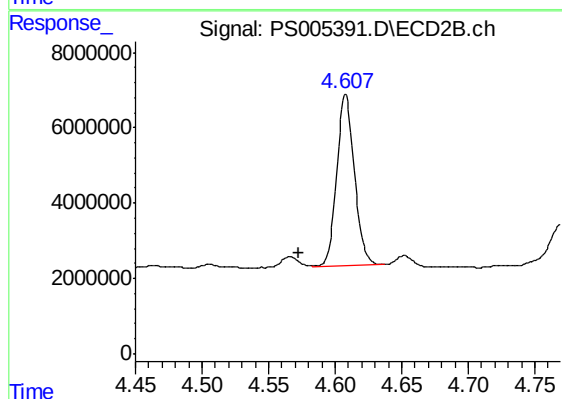

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.608 min
Delta R.T.: 0.035 min
Response: 41991022
Conc: 31.84 ng/ml

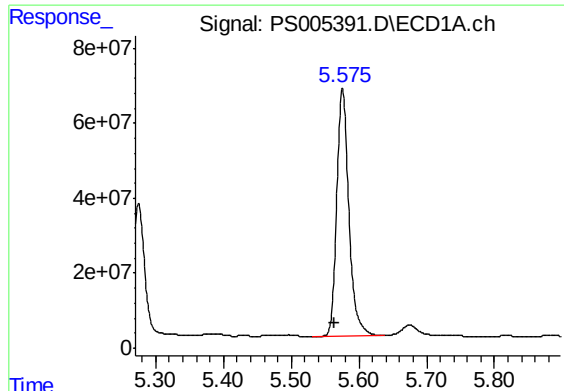

#4 2,4-DCAA


R.T.: 5.576 min
Delta R.T.: 0.012 min
Response: 825555580
Conc: 562.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121162BL

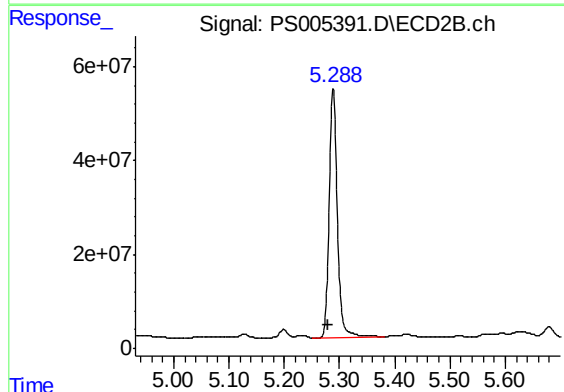


#4 2,4-DCAA

R.T.: 5.289 min
Delta R.T.: 0.009 min
Response: 548878037
Conc: 547.58 ng/ml

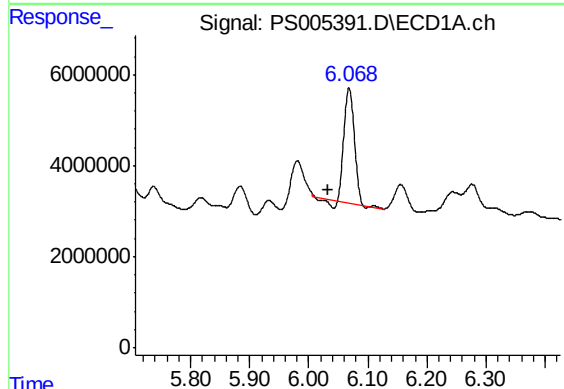


#7 MCPA

R.T.: 6.068 min
Delta R.T.: 0.036 min
Response: 29730789
Conc: 4.73 ug/ml

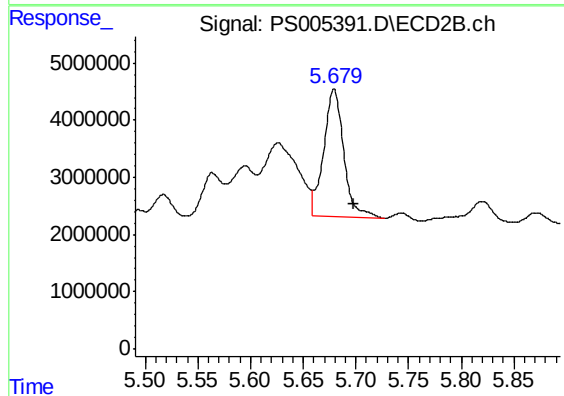

#7 MCPA


R.T.: 5.679 min
Delta R.T.: -0.018 min
Response: 29629335
Conc: 7.31 ug/ml

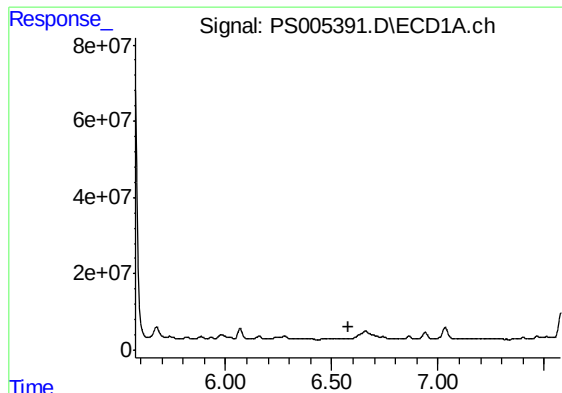

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121162BL

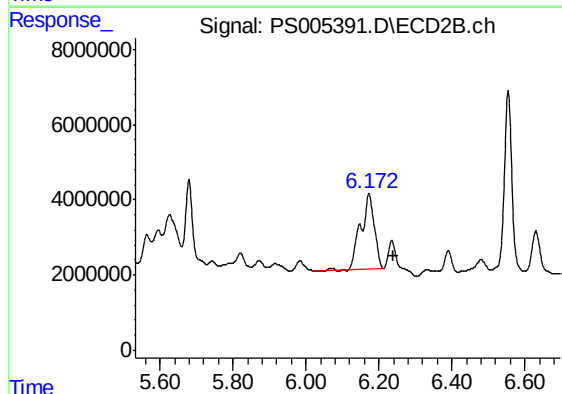


#9 2,4-D

R.T.: 6.173 min
Delta R.T.: -0.067 min
Response: 51421175
Conc: 46.11 ng/ml

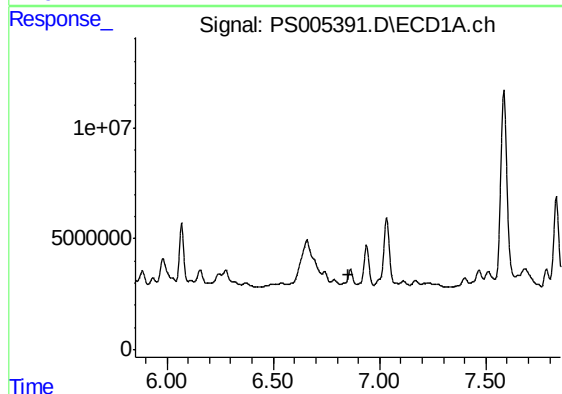


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

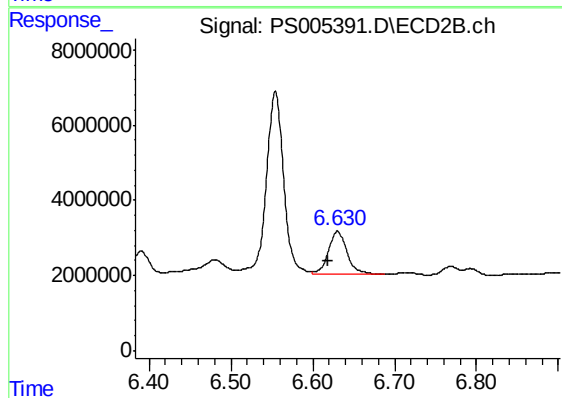

#10 Pentachlorophenol


R.T.: 6.630 min
Delta R.T.: 0.011 min
Response: 17620857
Conc: 1.37 ng/ml

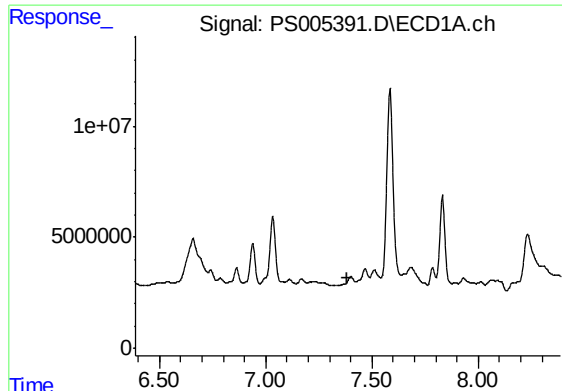

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121162BL

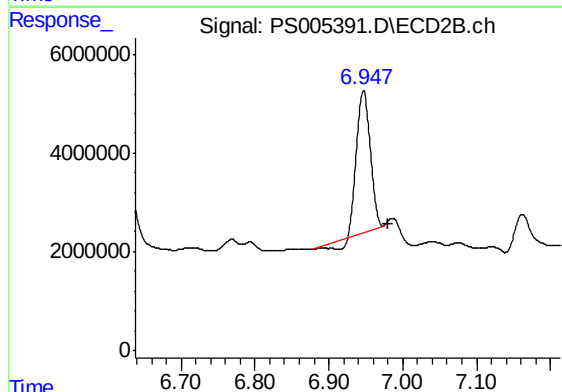


#11 2,4,5-TP (SILVEX)

R.T.: 6.947 min
Delta R.T.: -0.034 min
Response: 34729502
Conc: 6.52 ng/ml

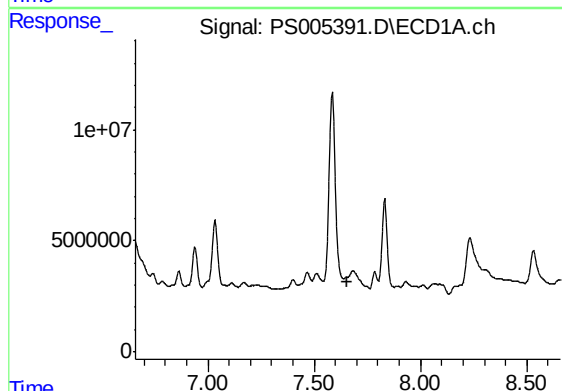


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

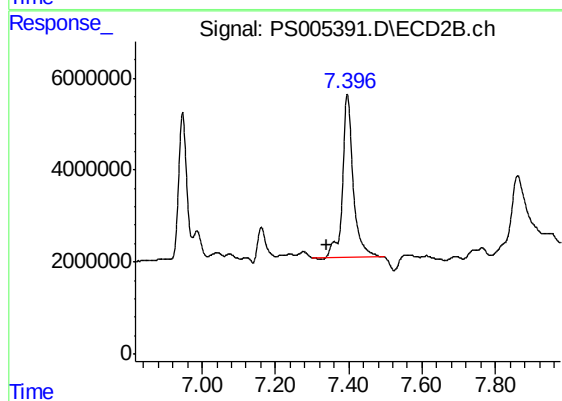

#12 2,4,5-T


R.T.: 7.396 min
Delta R.T.: 0.056 min
Response: 71605584
Conc: 14.04 ng/ml

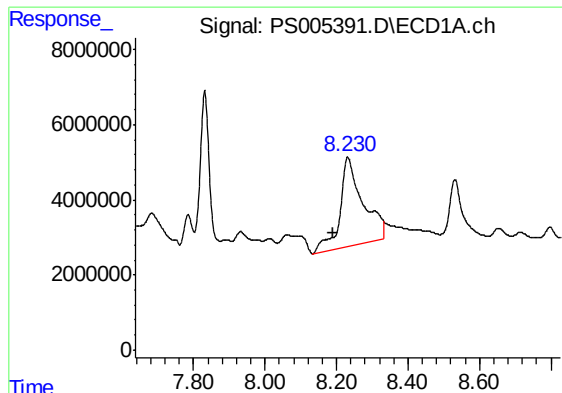

#13 2,4-DB


R.T.: 8.232 min
Delta R.T.: 0.042 min
Response: 105496908
Conc: 90.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121162BL

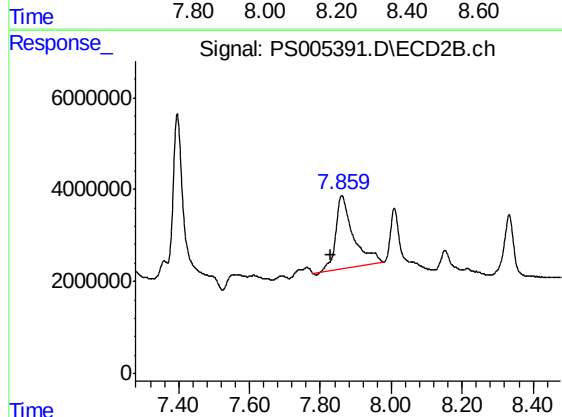


#13 2,4-DB

R.T.: 7.861 min
Delta R.T.: 0.031 min
Response: 54101106
Conc: 82.87 ng/ml

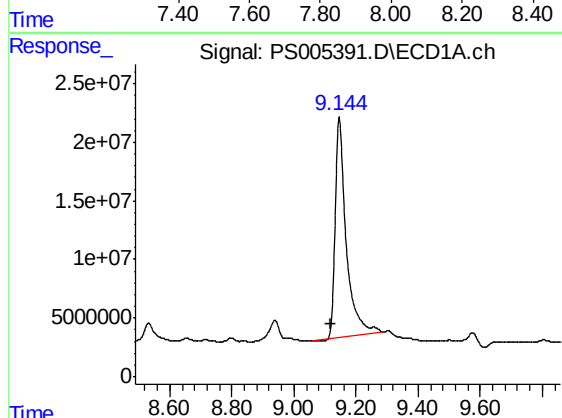


#15 Picloram

R.T.: 9.145 min
Delta R.T.: 0.029 min
Response: 462993218
Conc: 40.29 ng/ml

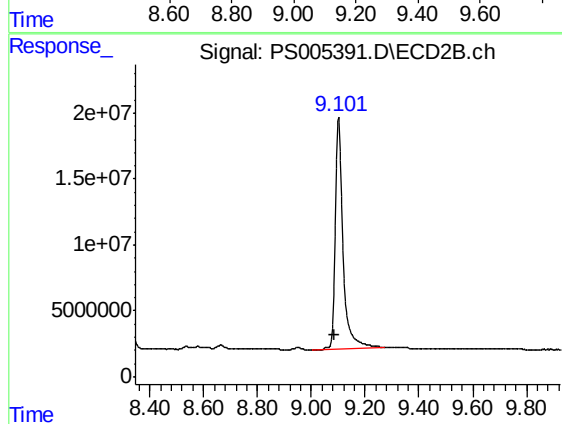

#15 Picloram


R.T.: 9.101 min
Delta R.T.: 0.016 min
Response: 346634854
Conc: 45.93 ng/ml

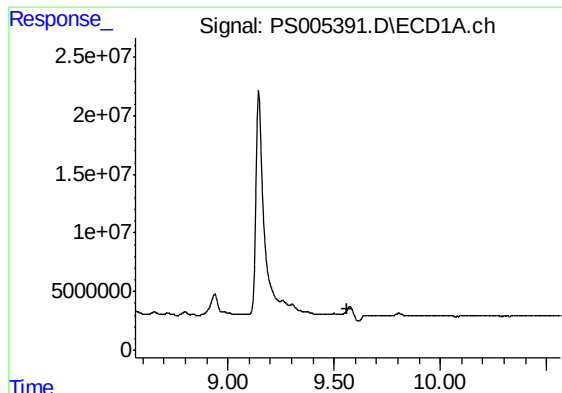

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121162BL

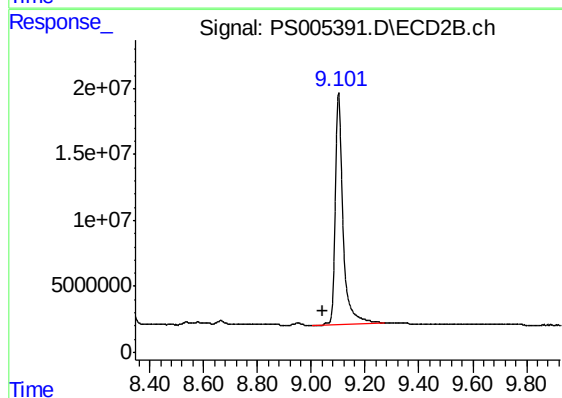

#16 DCPA

R.T.: 9.101 min
Delta R.T.: 0.056 min
Response: 346634854
Conc: 50.92 ng/ml