

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 16:26
 Operator : SM\AJ
 Sample : PB121188BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121188BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 00:39:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.568	5.279	580.6E6	386.1E6	395.519	385.164
Target Compounds							
1) T	Dalapon	2.075	0.000	37200476	0	20.182	N.D. #
2) T	3,5-DICHL...	0.000	4.597	0	150.5E6	N.D.	114.104
3) T	4-Nitroph...	5.371	0.000	25897094	0	35.755	N.D. #
5) T	DICAMBA	5.667	0.000	20243166	0	3.548	N.D. #
7) T	MCPA	6.060	5.670	30026804	21436348	4.782	5.292
11) T	2,4,5-TP ...	0.000	6.936	0	88294052	N.D.	16.580
13) T	2,4-DB	8.227	0.000	93922681	0	80.860	N.D. #
15) T	Picloram	9.148	9.097	97109838	82164728	8.451	10.888 #
16) T	DCPA	0.000	9.097	0	82164728	N.D.	12.070



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 16:26
Operator : SM\AJ
Sample : PB121188BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121188BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 00:39:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

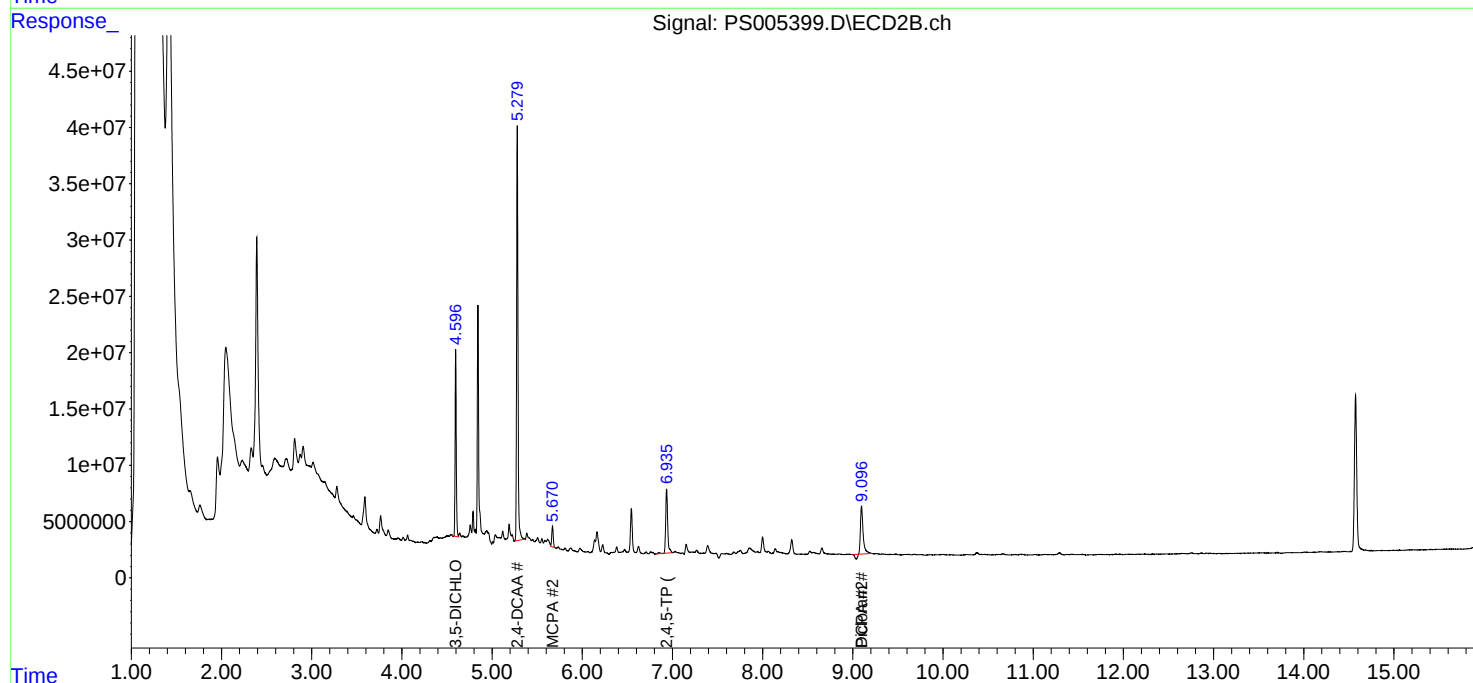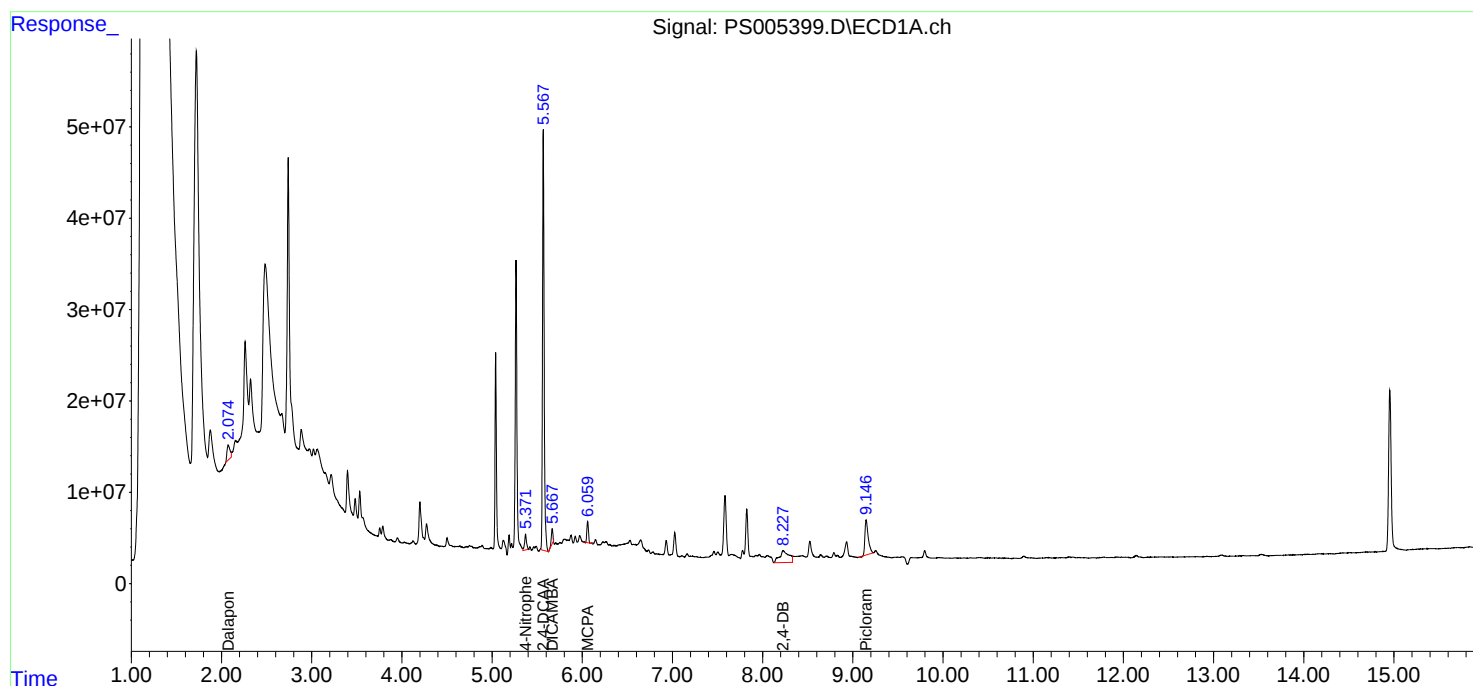


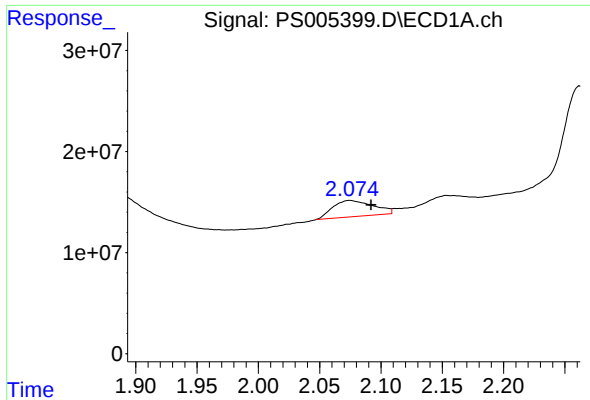

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.017 min
Response: 37200476
Conc: 20.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188BL

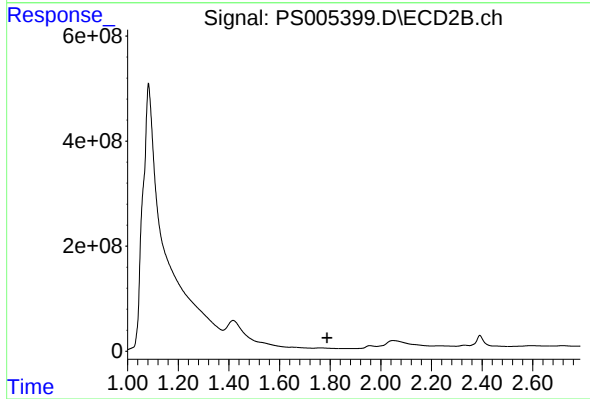


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

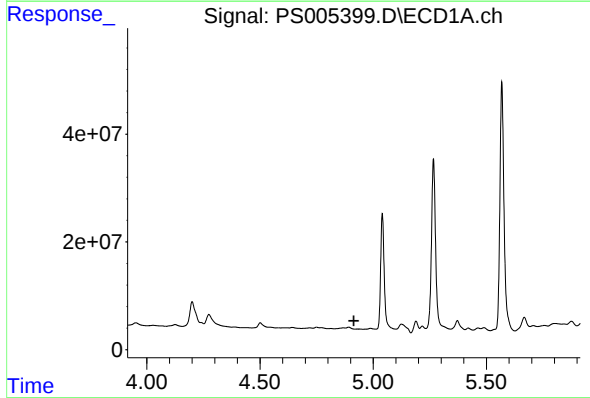


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

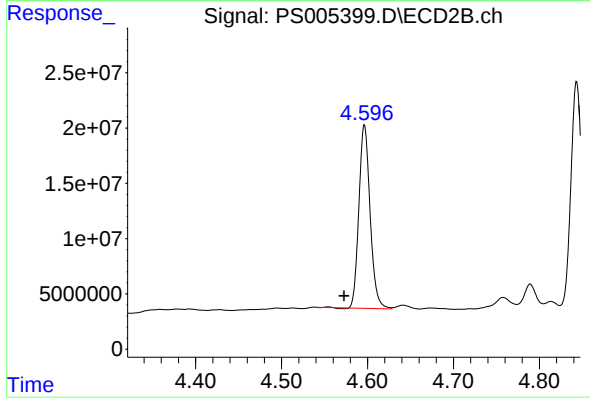

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.597 min
Delta R.T.: 0.024 min
Response: 150470019
Conc: 114.10 ng/ml

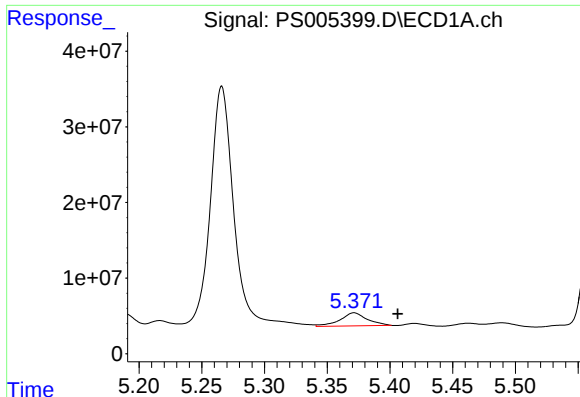

#3 4-Nitrophenol


R.T.: 5.371 min
Delta R.T.: -0.035 min
Response: 25897094
Conc: 35.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188BL

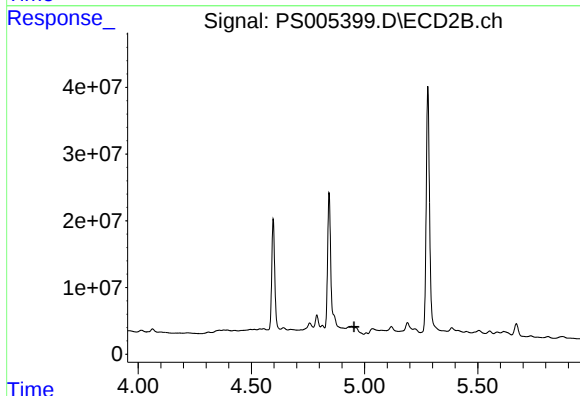


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

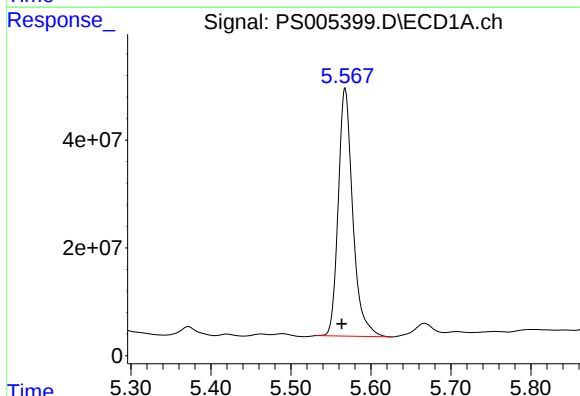


#4 2,4-DCAA

R.T.: 5.568 min
Delta R.T.: 0.004 min
Response: 580579129
Conc: 395.52 ng/ml

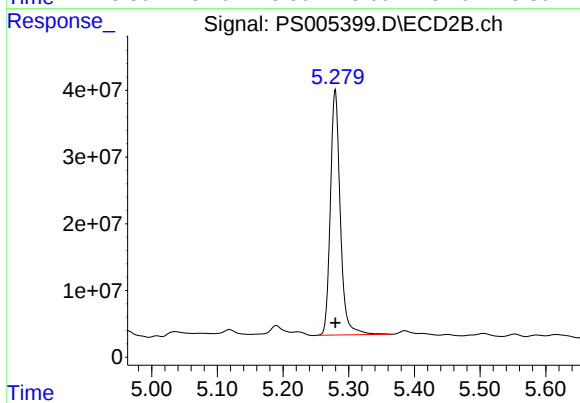

#4 2,4-DCAA


R.T.: 5.279 min
Delta R.T.: 0.000 min
Response: 386076465
Conc: 385.16 ng/ml

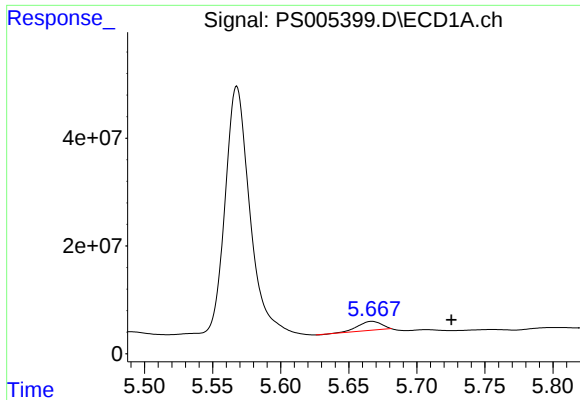

#5 DICAMBA


R.T.: 5.667 min
Delta R.T.: -0.058 min
Response: 20243166
Conc: 3.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188BL

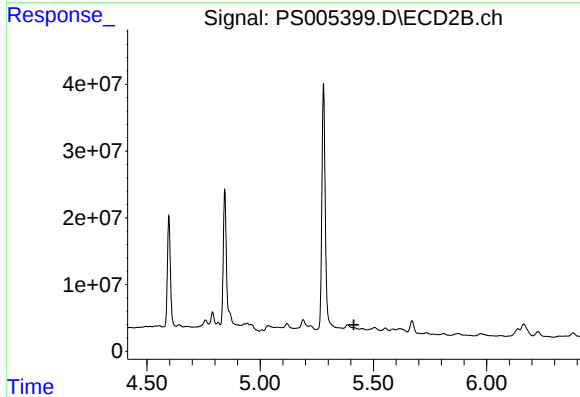


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

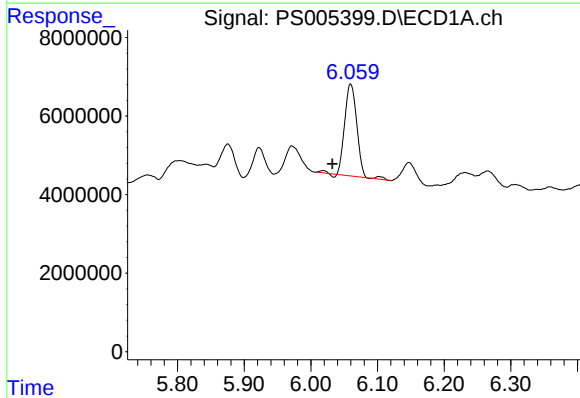


#7 MCPA

R.T.: 6.060 min
Delta R.T.: 0.028 min
Response: 30026804
Conc: 4.78 ug/ml

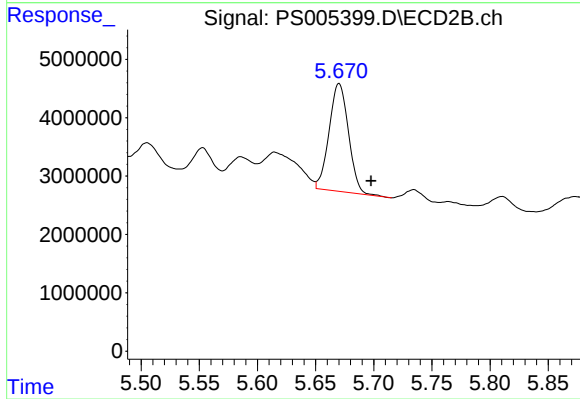

#7 MCPA


R.T.: 5.670 min
Delta R.T.: -0.028 min
Response: 21436348
Conc: 5.29 ug/ml

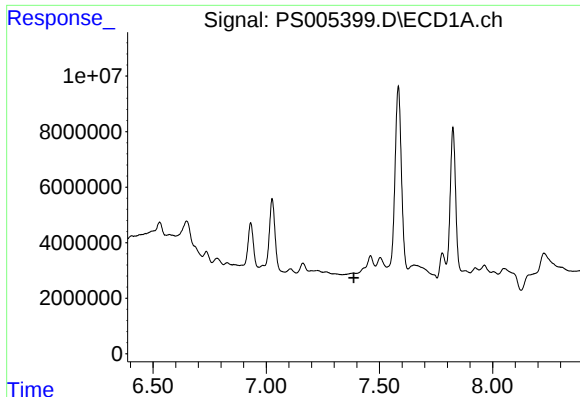

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121188BL

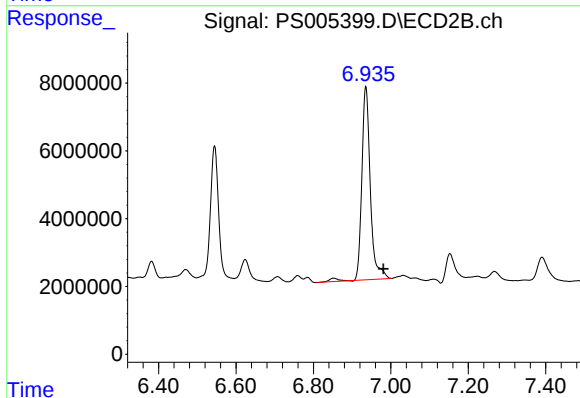


#11 2,4,5-TP (SILVEX)

R.T.: 6.936 min
Delta R.T.: -0.045 min
Response: 88294052
Conc: 16.58 ng/ml

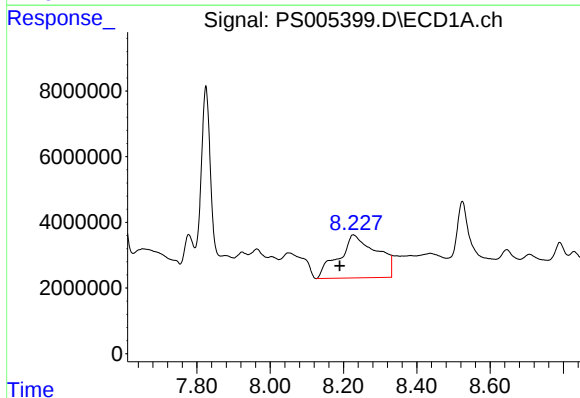


#13 2,4-DB

R.T.: 8.227 min
Delta R.T.: 0.037 min
Response: 93922681
Conc: 80.86 ng/ml

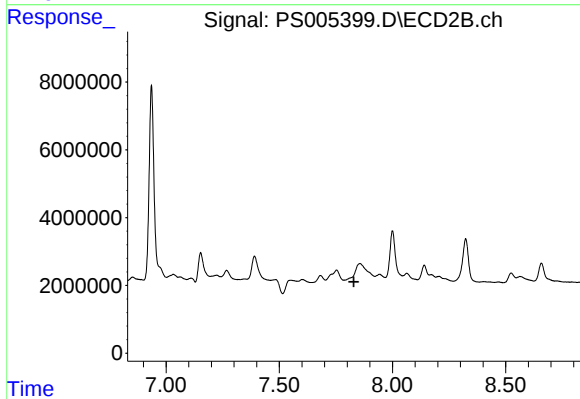

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.830 min
Response: 0
Conc: N.D.

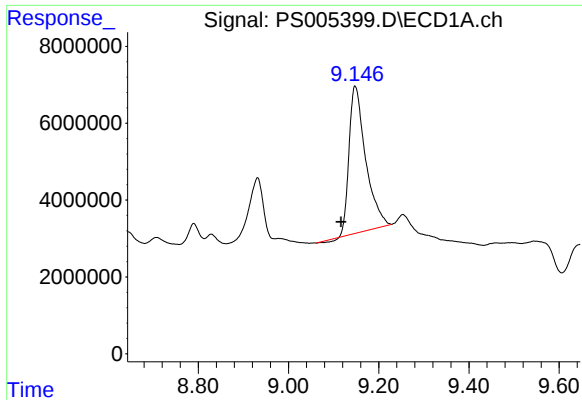

#15 Picloram


R.T.: 9.148 min
Delta R.T.: 0.032 min
Response: 97109838
Conc: 8.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188BL

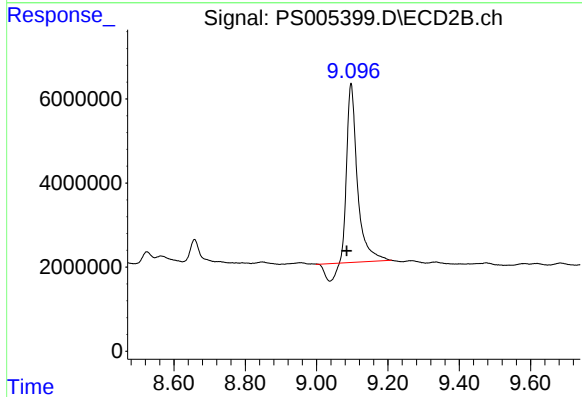


#15 Picloram

R.T.: 9.097 min
Delta R.T.: 0.012 min
Response: 82164728
Conc: 10.89 ng/ml

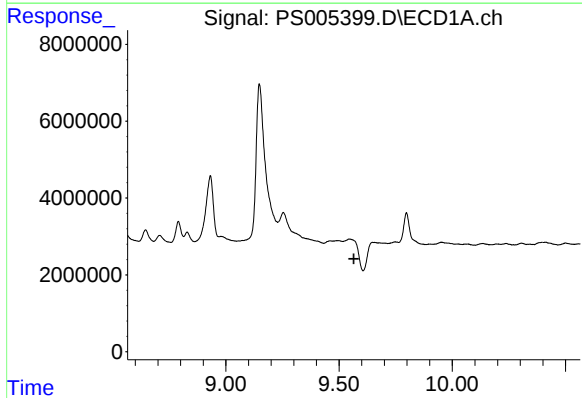

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

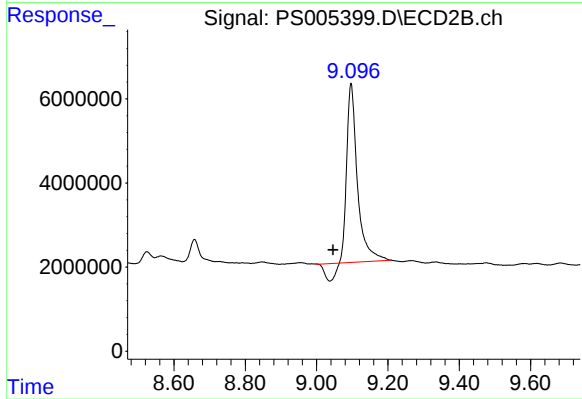

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.051 min
Response: 82164728
Conc: 12.07 ng/ml