

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 17:09
 Operator : SM\AJ
 Sample : PB121188TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121188TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 00:39:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.285	587.4E6	398.1E6	400.179	397.135
Target Compounds							
1) T	Dalapon	2.077	0.000	36612694	0	19.863	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	153.4E6	N.D.	116.298
3) T	4-Nitroph...	5.373	0.000	24634535	0	34.012	N.D. #
5) T	DICAMBA	5.668	0.000	17818443	0	3.123	N.D. #
7) T	MCPA	6.062	5.675	31900790	27840758	5.080	6.873 #
10) T	Pentachlo...	0.000	6.549	0	52197137	N.D.	4.060
11) T	2,4,5-TP ...	0.000	6.941	0	85043358	N.D.	15.970
13) T	2,4-DB	8.229	0.000	95306340	0	82.051	N.D. #
15) T	Picloram	0.000	9.113	0	20559552	N.D.	2.724
16) T	DCPA	0.000	9.113	0	20559552	N.D.	3.020



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 17:09
Operator : SM\AJ
Sample : PB121188TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121188TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 00:39:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

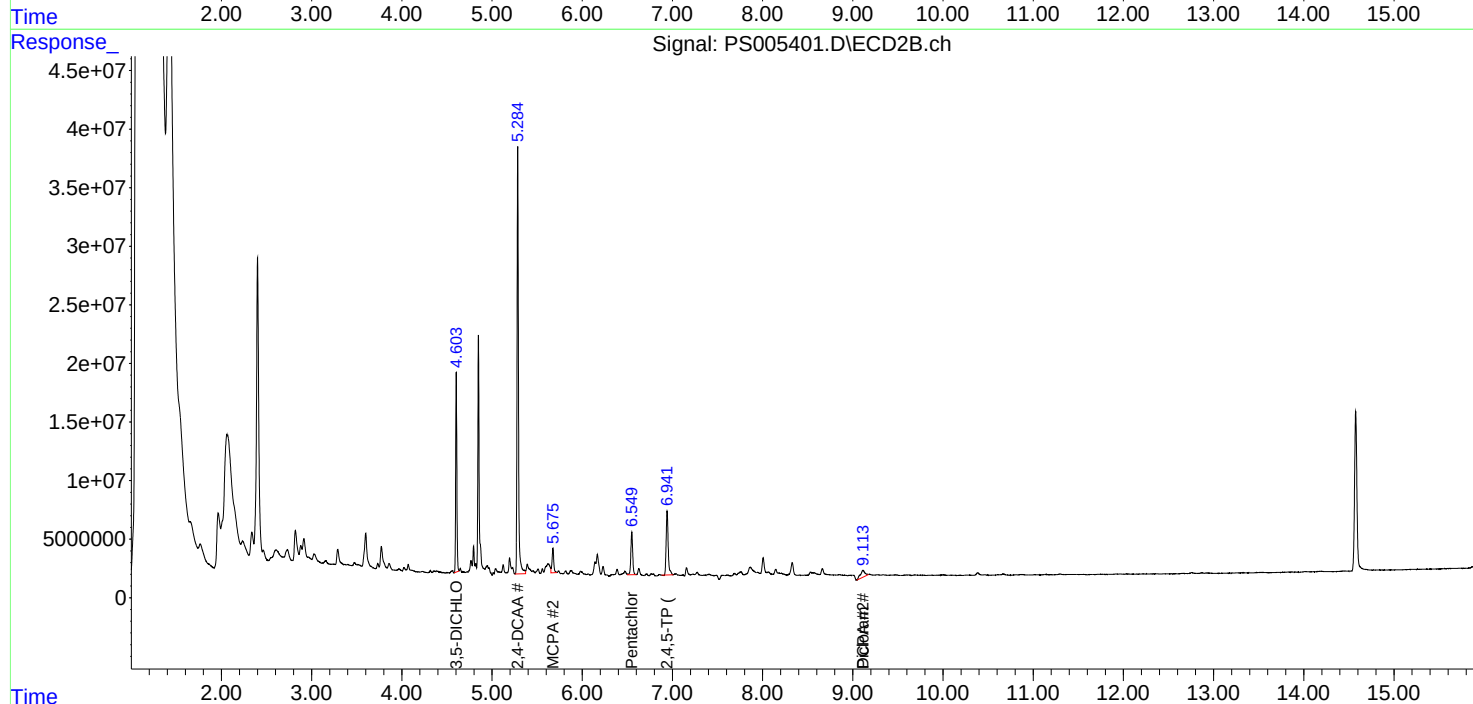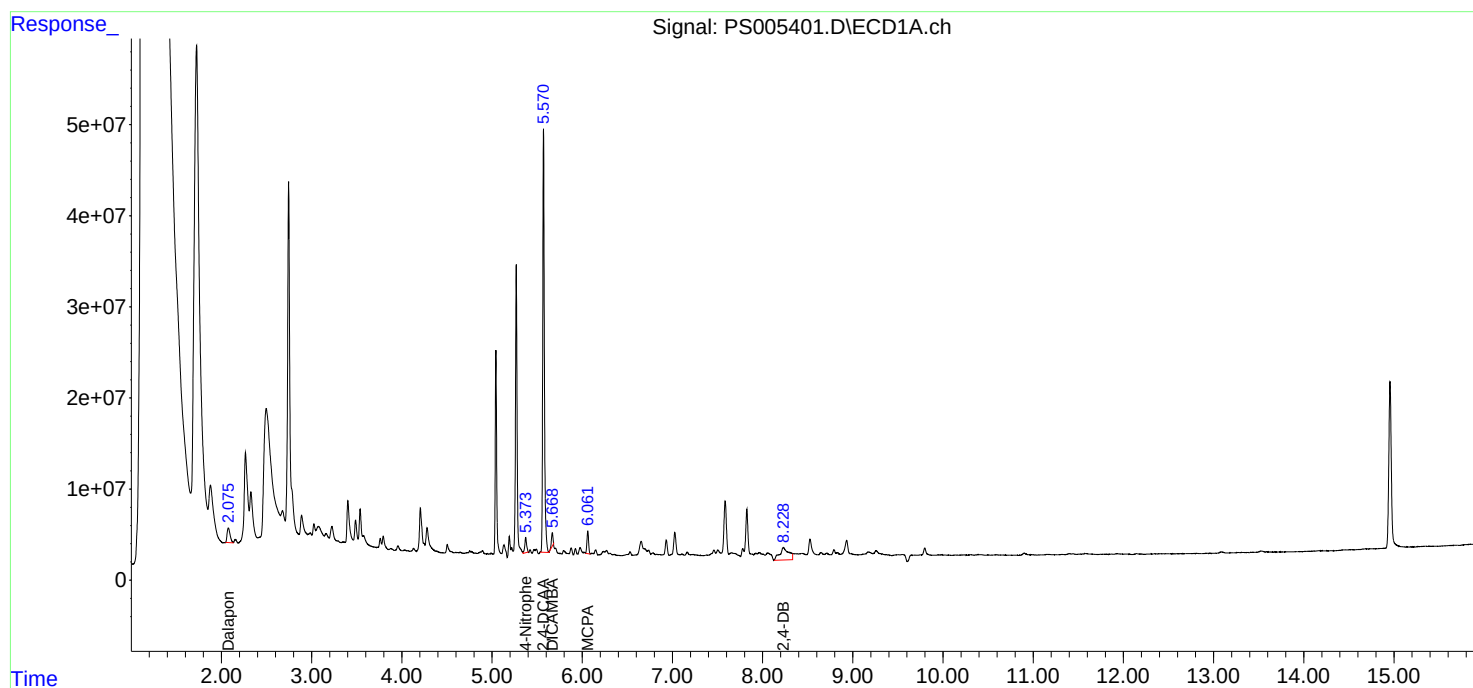


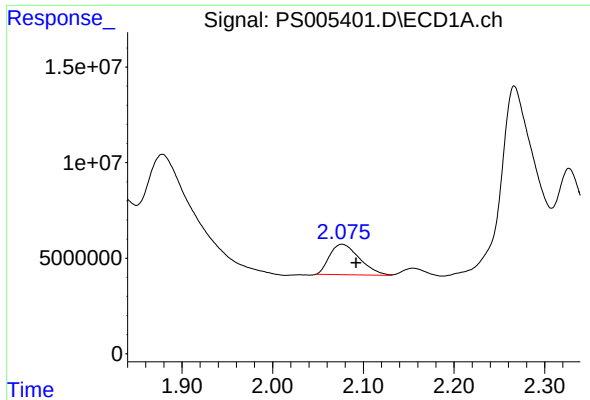

#1 Dalapon


R.T.: 2.077 min
Delta R.T.: -0.015 min
Response: 36612694
Conc: 19.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188TB

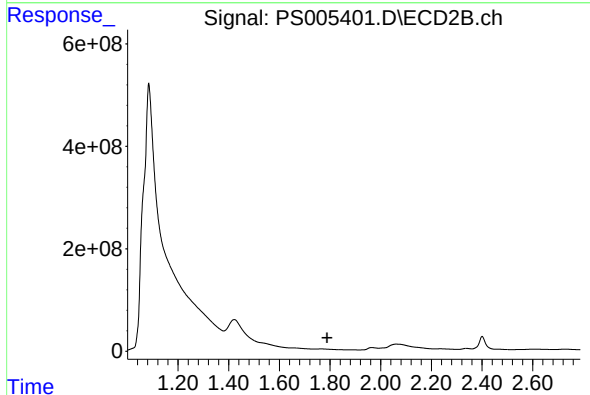


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

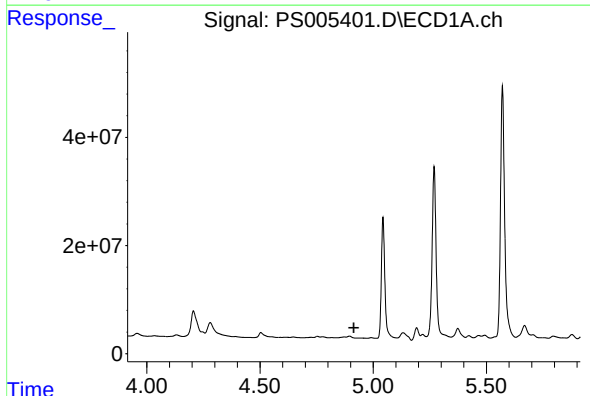


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

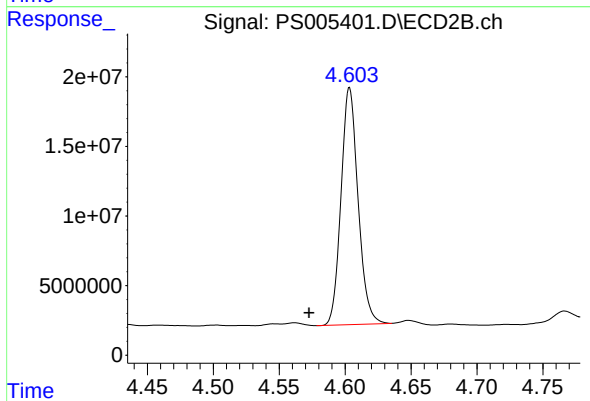

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.031 min
Response: 153362984
Conc: 116.30 ng/ml

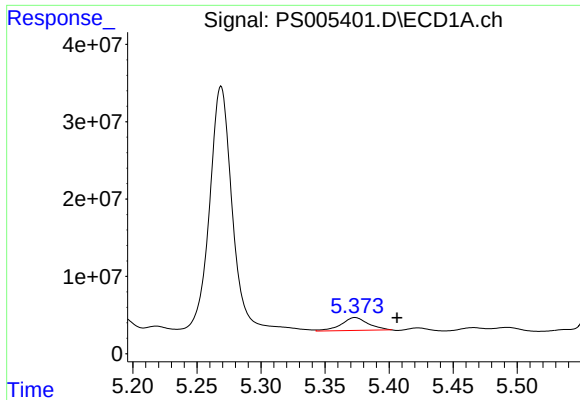

#3 4-Nitrophenol


R.T.: 5.373 min
Delta R.T.: -0.033 min
Response: 24634535
Conc: 34.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188TB

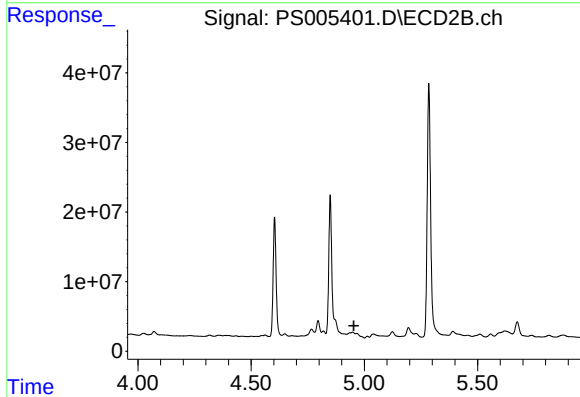


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

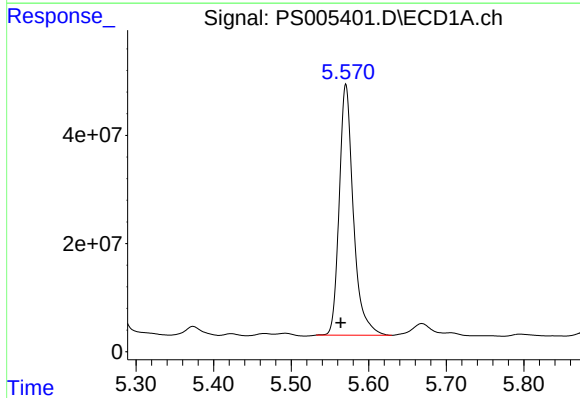


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: 0.007 min
Response: 587420302
Conc: 400.18 ng/ml

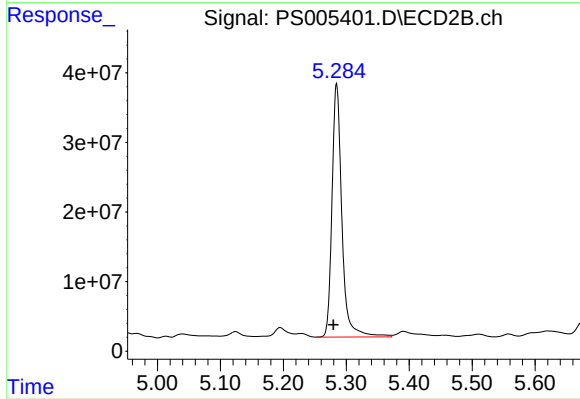

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 398076104
Conc: 397.14 ng/ml

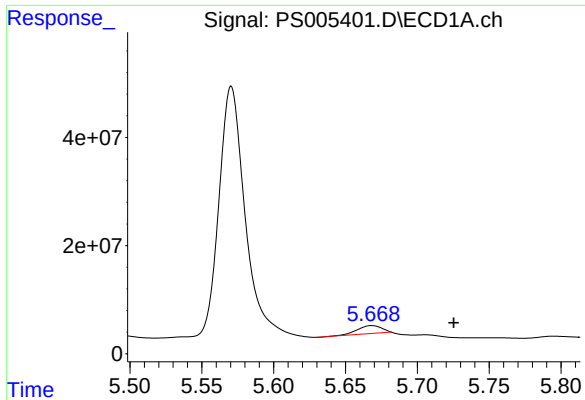

#5 DICAMBA


R.T.: 5.668 min
Delta R.T.: -0.057 min
Response: 17818443
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188TB

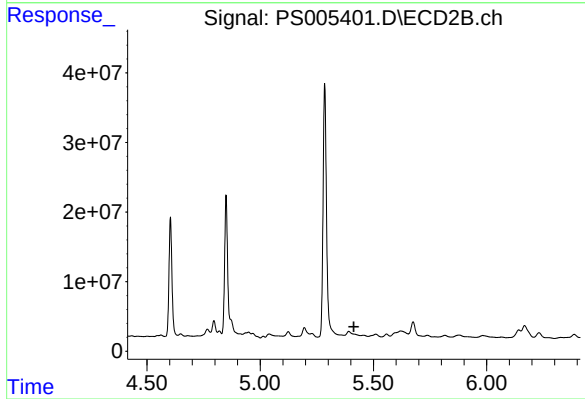


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

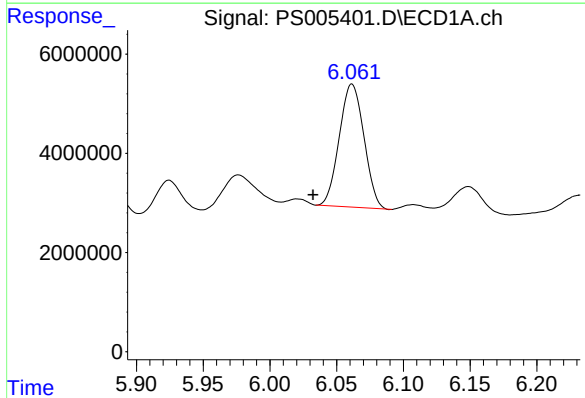


#7 MCPA

R.T.: 6.062 min
Delta R.T.: 0.029 min
Response: 31900790
Conc: 5.08 ug/ml

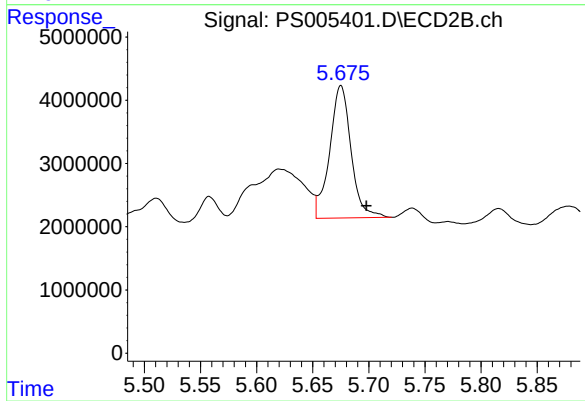

#7 MCPA


R.T.: 5.675 min
Delta R.T.: -0.023 min
Response: 27840758
Conc: 6.87 ug/ml

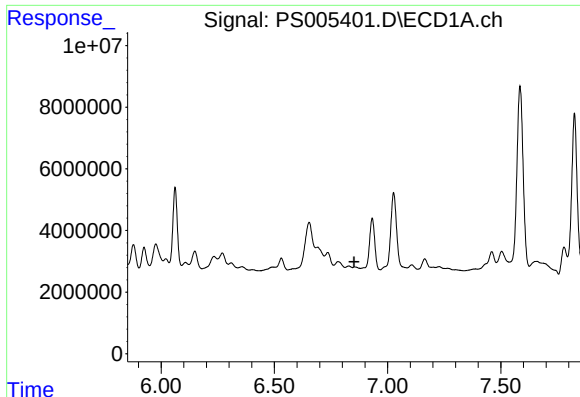

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121188TB

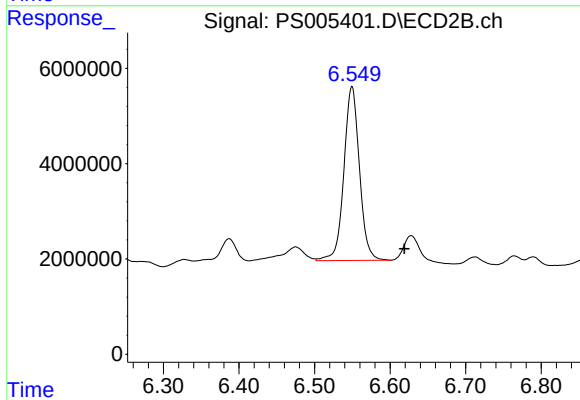


#10 Pentachlorophenol

R.T.: 6.549 min
Delta R.T.: -0.070 min
Response: 52197137
Conc: 4.06 ng/ml

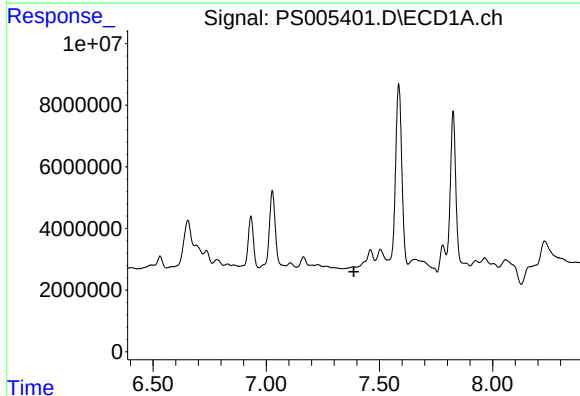


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

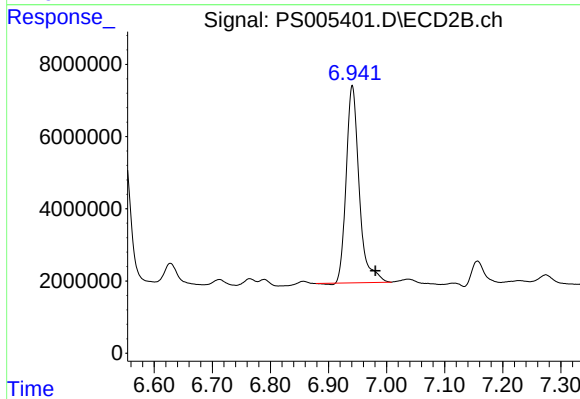

#11 2,4,5-TP (SILVEX)


R.T.: 6.941 min
Delta R.T.: -0.040 min
Response: 85043358
Conc: 15.97 ng/ml

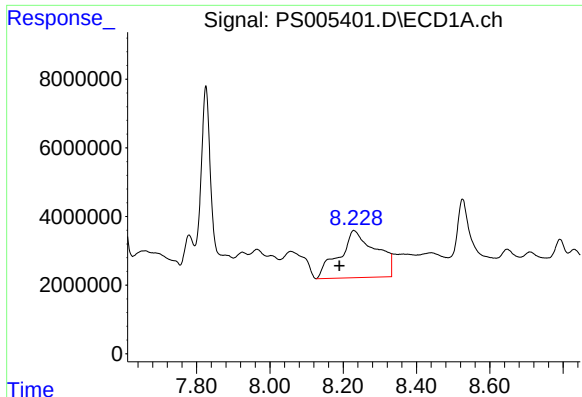

#13 2,4-DB


R.T.: 8.229 min
Delta R.T.: 0.040 min
Response: 95306340
Conc: 82.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121188TB

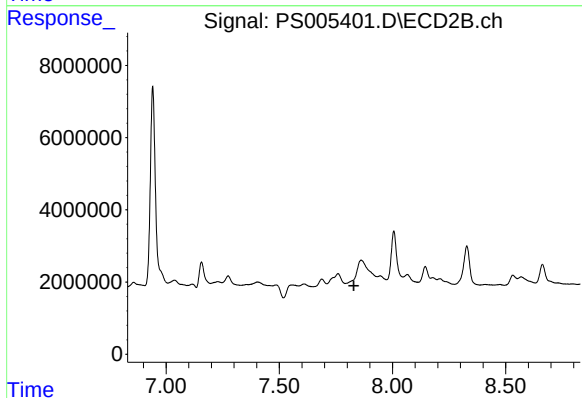


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.830 min
Response: 0
Conc: N.D.

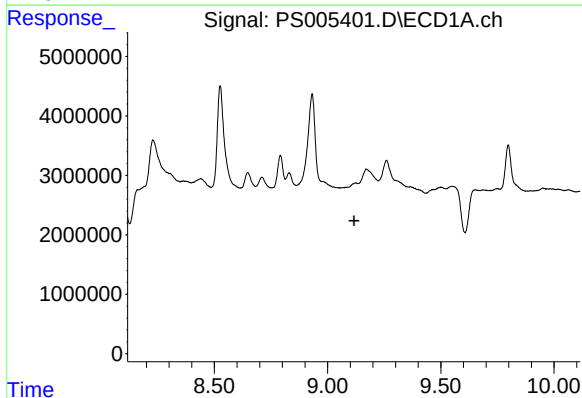


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.117 min
Response: 0
Conc: N.D.

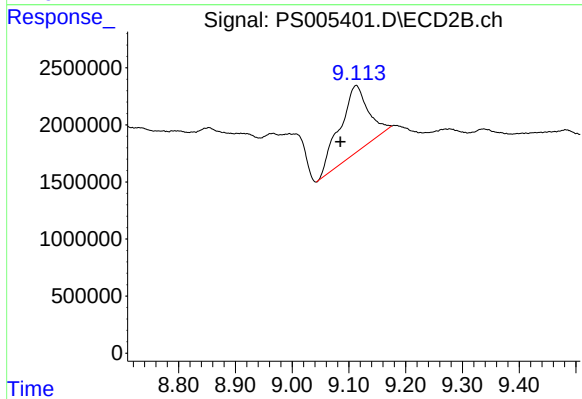

#15 Picloram


R.T.: 9.113 min
Delta R.T.: 0.028 min
Response: 20559552
Conc: 2.72 ng/ml

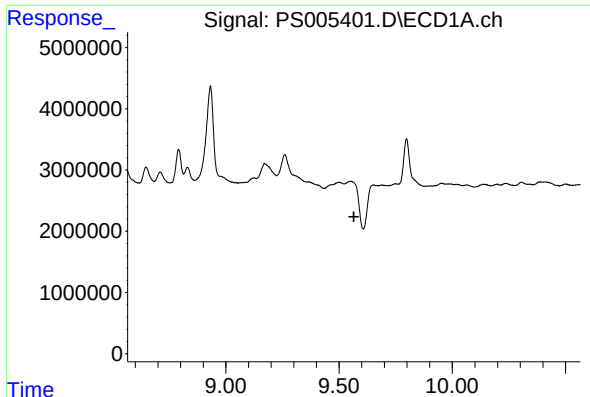

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121188TB

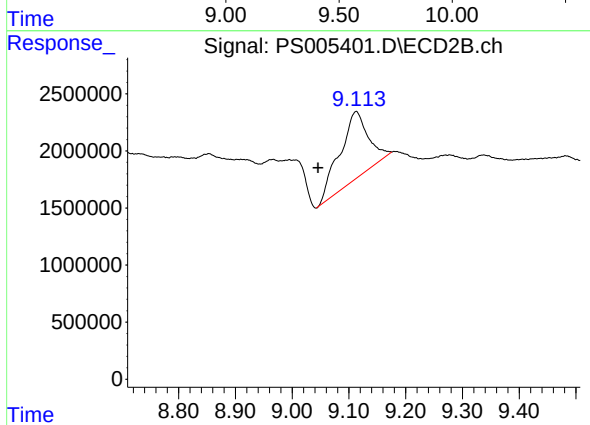

#16 DCPA

R.T.: 9.113 min
Delta R.T.: 0.067 min
Response: 20559552
Conc: 3.02 ng/ml