

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 17:31
 Operator : SM\AJ
 Sample : K3622-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-02-070319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 00:40:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.567	5.291	201.8E6	142.5E6	137.489	142.176
Target Compounds							
1) T	Dalapon	2.073	0.000	30983511	0	16.809	N.D. #
2) T	3,5-DICHL...	0.000	4.568	0	11446028	N.D.	8.680
5) T	DICAMBA	5.665	5.397	15705216	16037275	2.753	4.284 #
6) T	MCP	5.919	0.000	10947327	0	2.501	N.D. #
8) T	DICHLORPROP	0.000	5.983	0	15653930	N.D.	16.213
9) T	2,4-D	0.000	6.237	0	46800802	N.D.	41.963
10) T	Pentachlo...	0.000	6.556	0	34016783	N.D.	2.646
11) T	2,4,5-TP ...	0.000	6.944	0	94053068	N.D.	17.662



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 17:31
Operator : SM\AJ
Sample : K3622-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 00:40:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

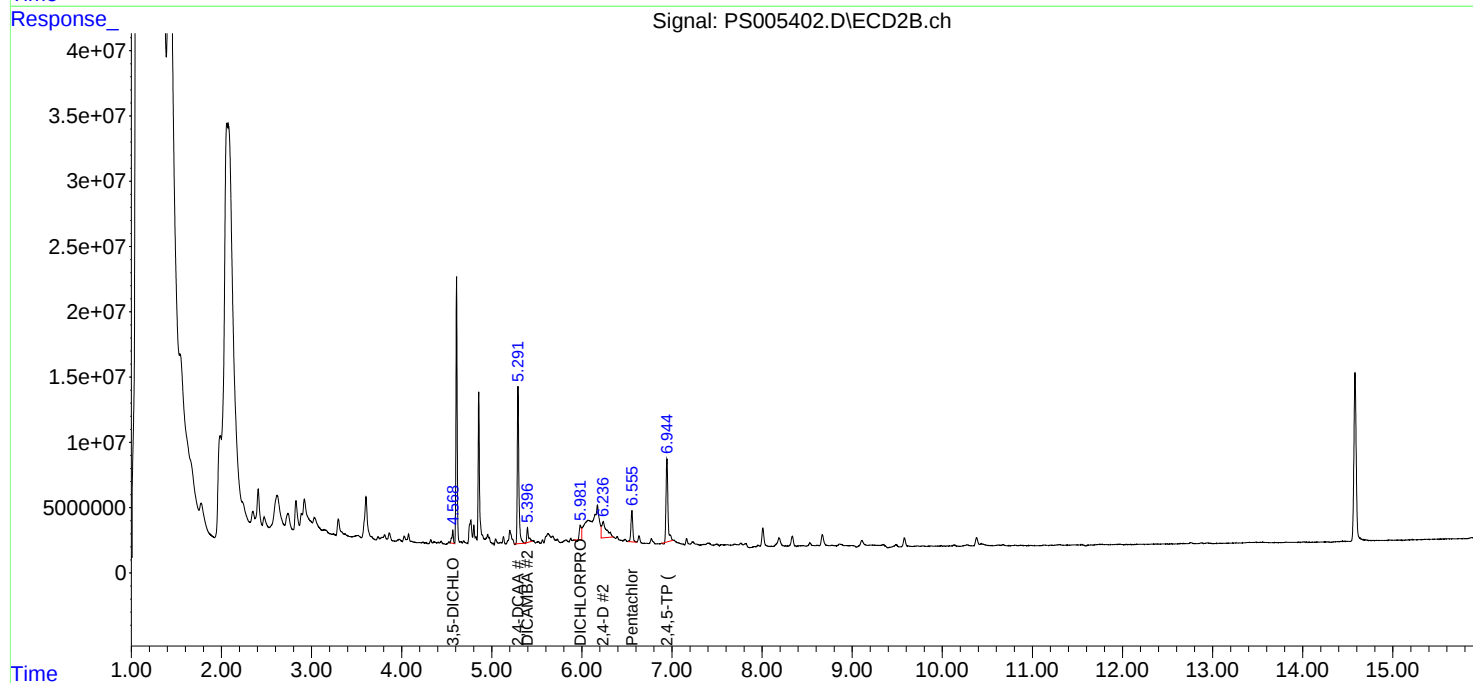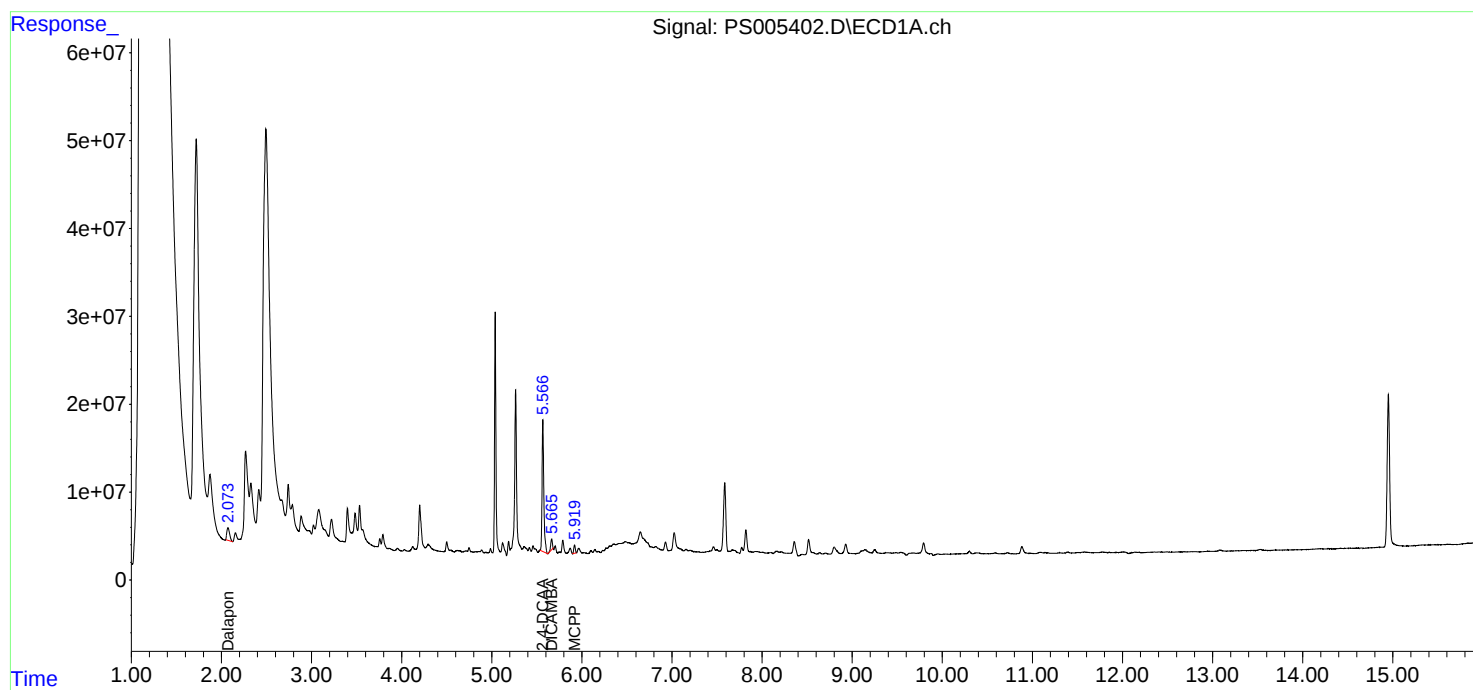


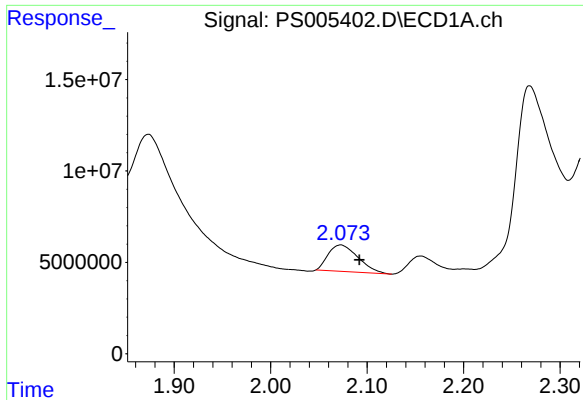

#1 Dalapon


R.T.: 2.073 min
Delta R.T.: -0.019 min
Response: 30983511
Conc: 16.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

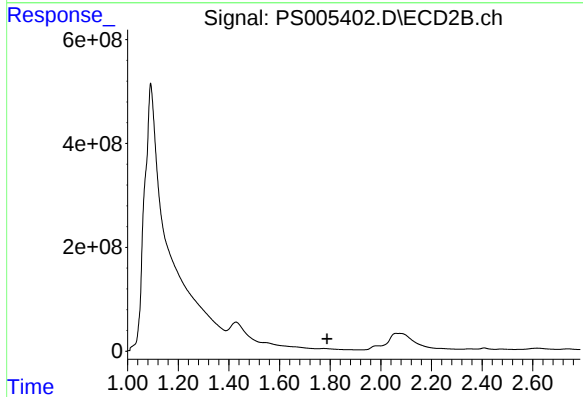


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

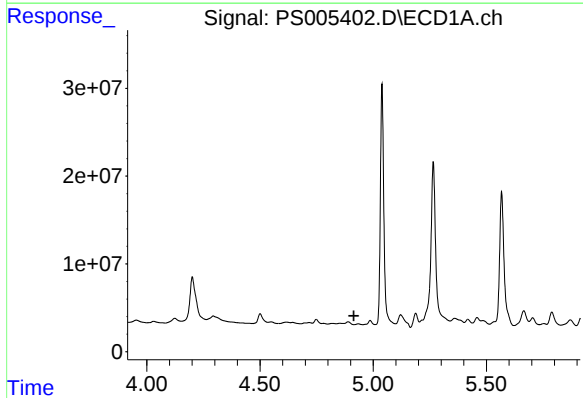


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

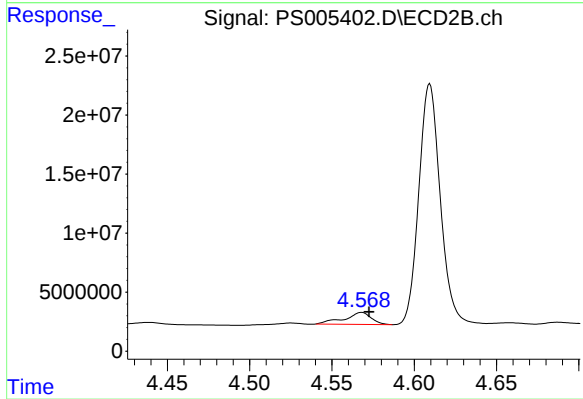

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.568 min
Delta R.T.: -0.005 min
Response: 11446028
Conc: 8.68 ng/ml

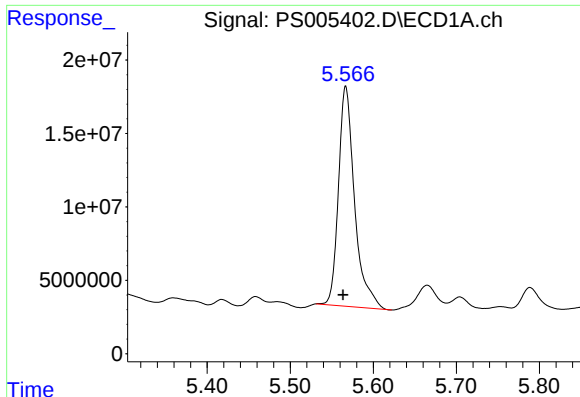

#4 2,4-DCAA


R.T.: 5.567 min
Delta R.T.: 0.003 min
Response: 201819741
Conc: 137.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

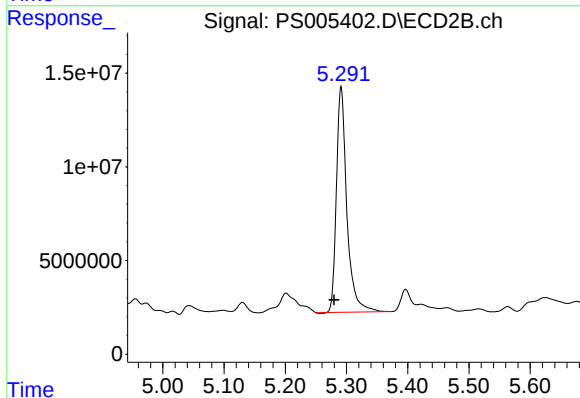


#4 2,4-DCAA

R.T.: 5.291 min
Delta R.T.: 0.012 min
Response: 142512875
Conc: 142.18 ng/ml

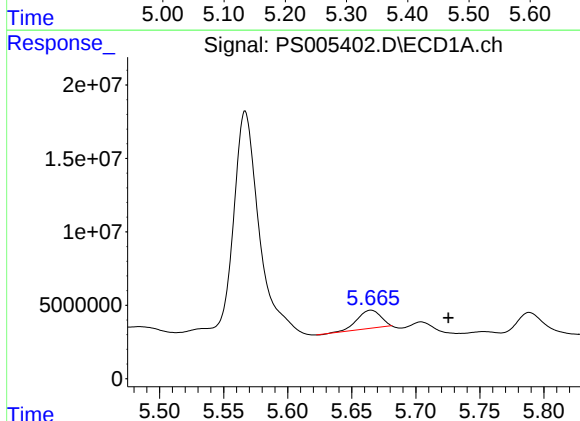


#5 DICAMBA

R.T.: 5.665 min
Delta R.T.: -0.061 min
Response: 15705216
Conc: 2.75 ng/ml

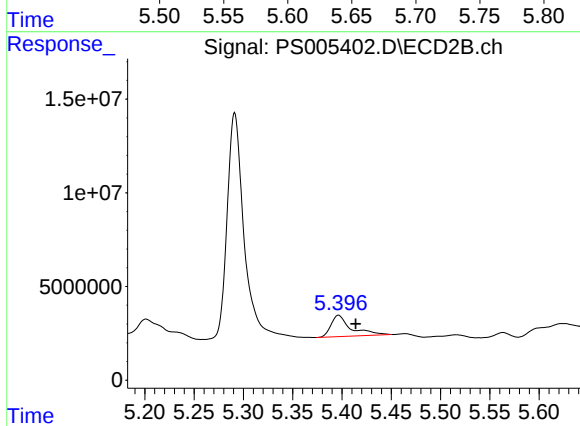

#5 DICAMBA


R.T.: 5.397 min
Delta R.T.: -0.017 min
Response: 16037275
Conc: 4.28 ng/ml

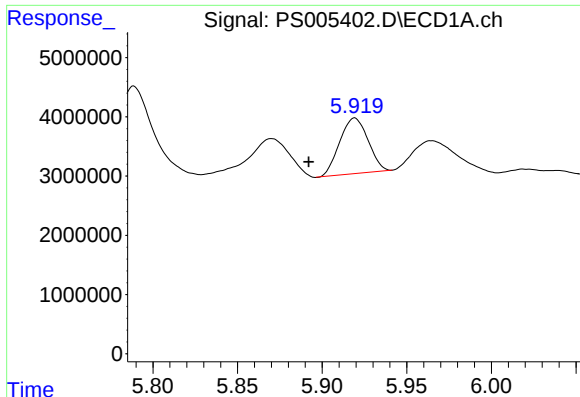

#6 MCP


R.T.: 5.919 min
Delta R.T.: 0.027 min
Response: 10947327
Conc: 2.50 ug/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

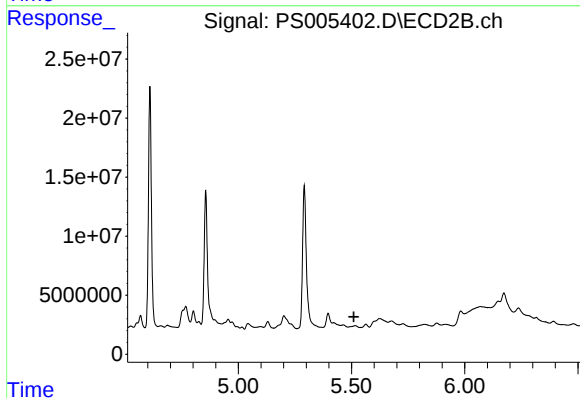


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

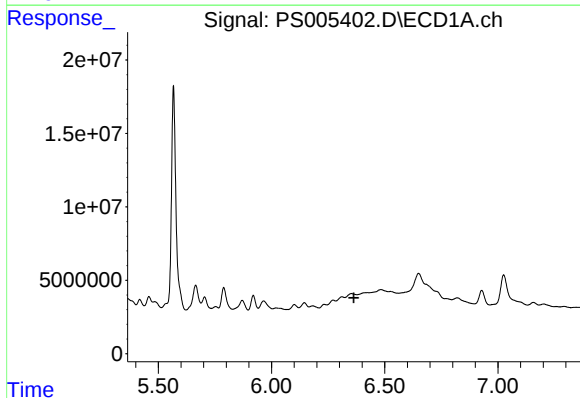


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

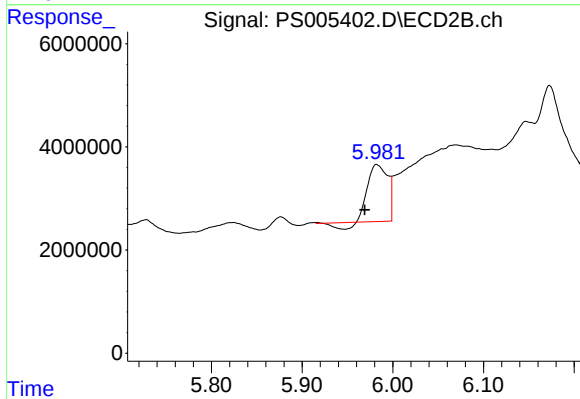

#8 DICHLORPROP


R.T.: 5.983 min
Delta R.T.: 0.014 min
Response: 15653930
Conc: 16.21 ng/ml

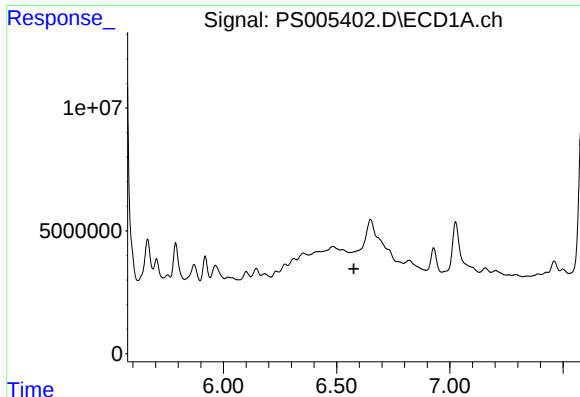

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

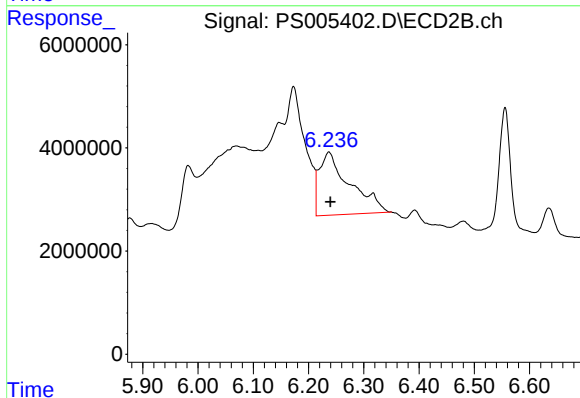


#9 2,4-D

R.T.: 6.237 min
Delta R.T.: -0.003 min
Response: 46800802
Conc: 41.96 ng/ml

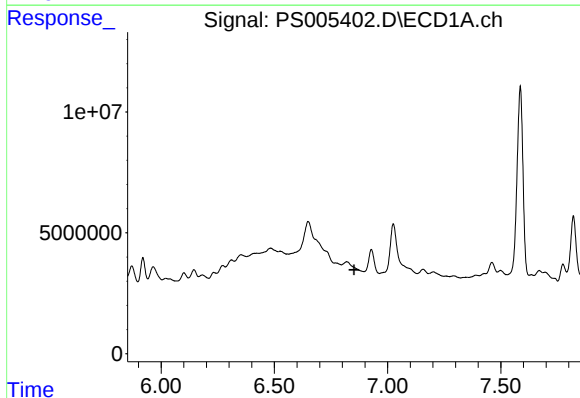


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

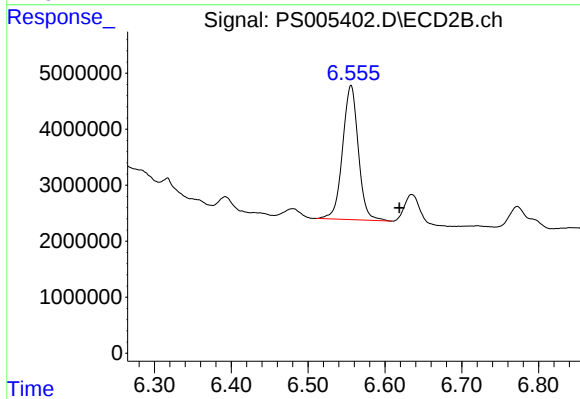

#10 Pentachlorophenol

R.T.: 6.556 min
Delta R.T.: -0.063 min
Response: 34016783
Conc: 2.65 ng/ml

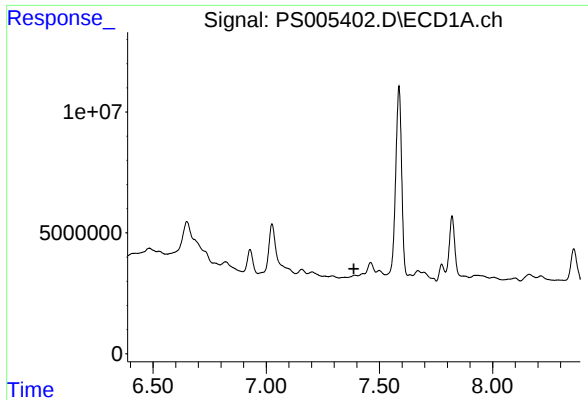

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min

Exp R.T.: 7.387 min

Response: 0

Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-02-070319-A

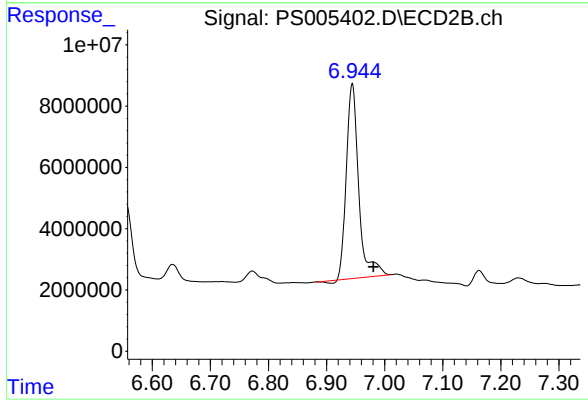

#11 2,4,5-TP (SILVEX)

R.T.: 6.944 min

Delta R.T.: -0.036 min

Response: 94053068

Conc: 17.66 ng/ml