

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 18:59
 Operator : SM\AJ
 Sample : K3624-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PL-01-070319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 00:41:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.572	5.287	239.8E6	164.5E6	163.394	164.140
Target Compounds							
1) T	Dalapon	2.078	0.000	38186913	0	20.717	N.D. #
2) T	3,5-DICHL...	0.000	4.564	0	9186993	N.D.	6.967
5) T	DICAMBA	5.670	0.000	13016983	0	2.282	N.D. #
8) T	DICHLORPROP	0.000	5.980	0	45523904	N.D.	47.149
10) T	Pentachlo...	0.000	6.551	0	40966289	N.D.	3.186
11) T	2,4,5-TP ...	0.000	6.940	0	102.1E6	N.D.	19.171
12) T	2,4,5-T	7.590	0.000	149.5E6	0	18.571	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 18:59
Operator : SM\AJ
Sample : K3624-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 00:41:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

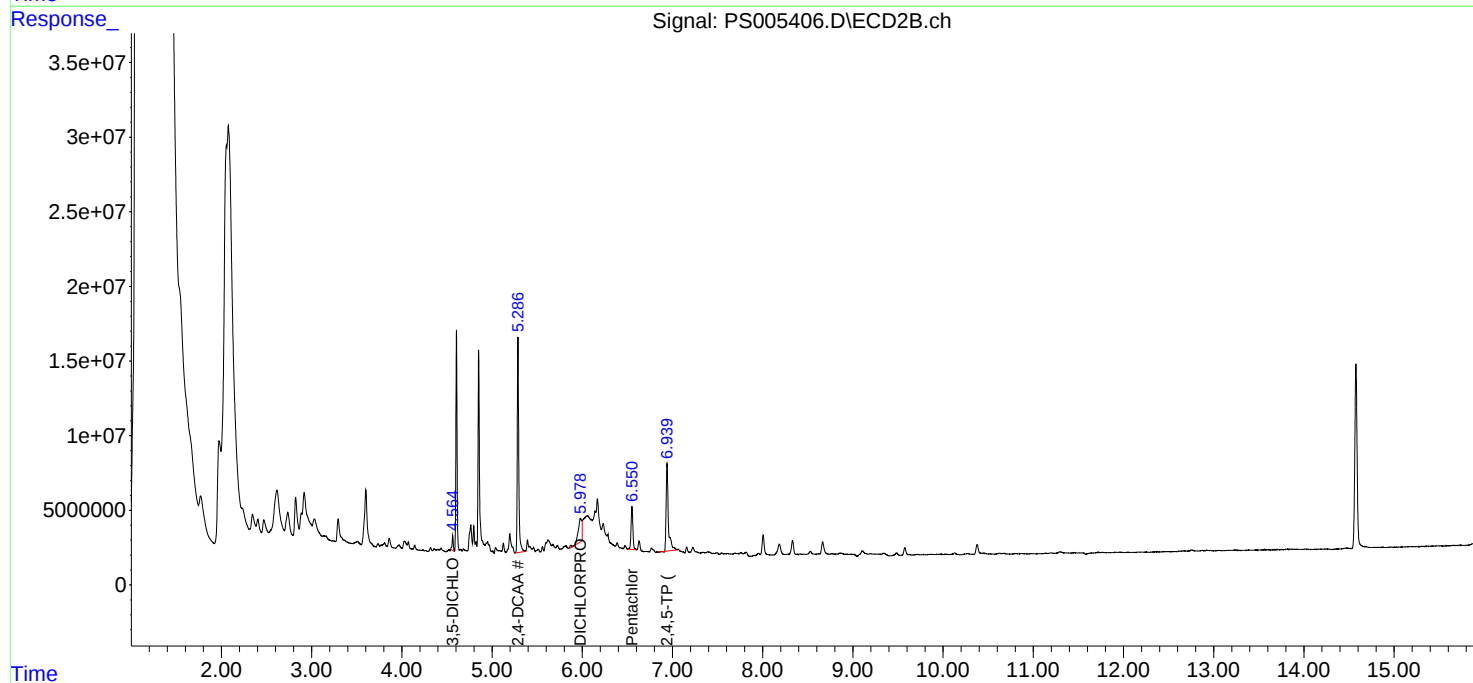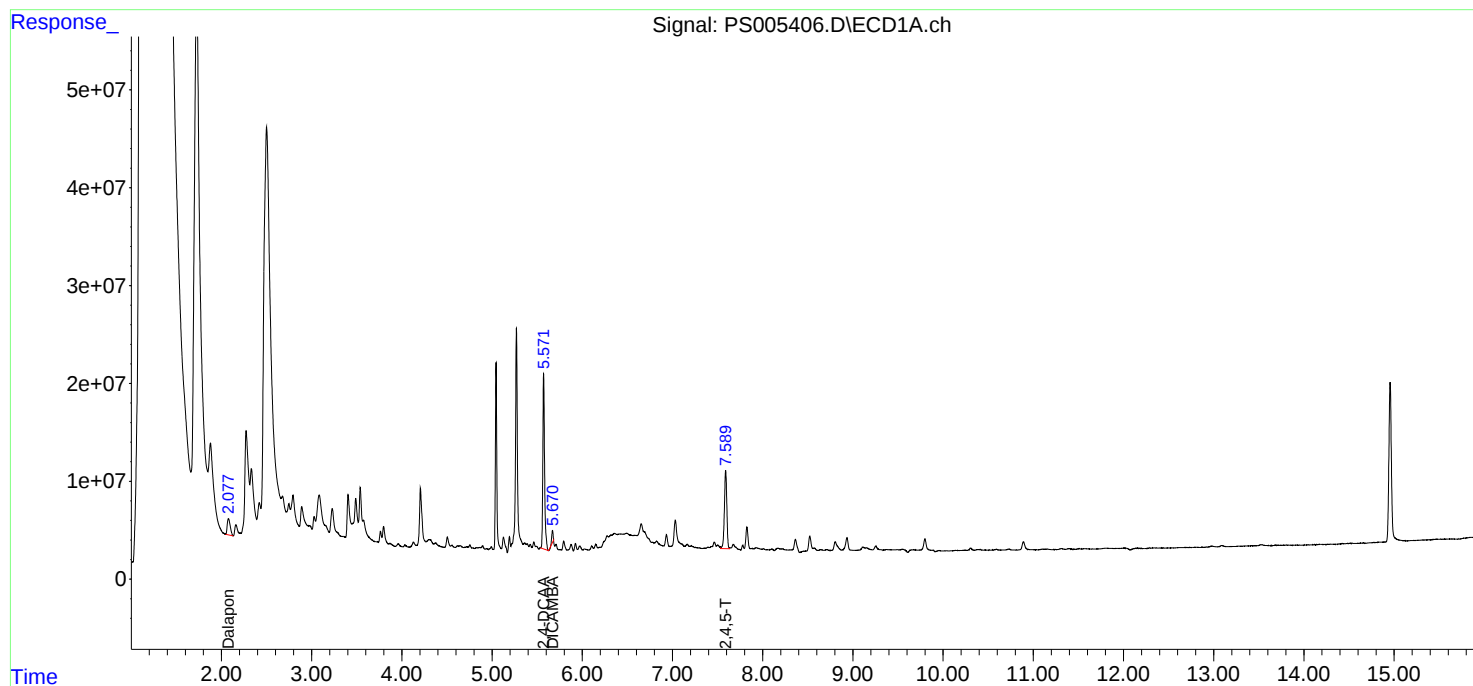


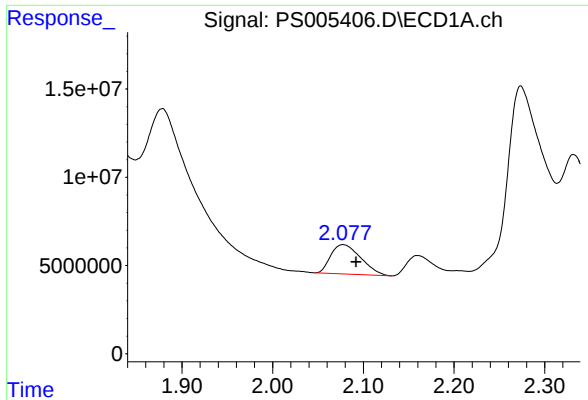

#1 Dalapon


R.T.: 2.078 min
Delta R.T.: -0.014 min
Response: 38186913
Conc: 20.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-A

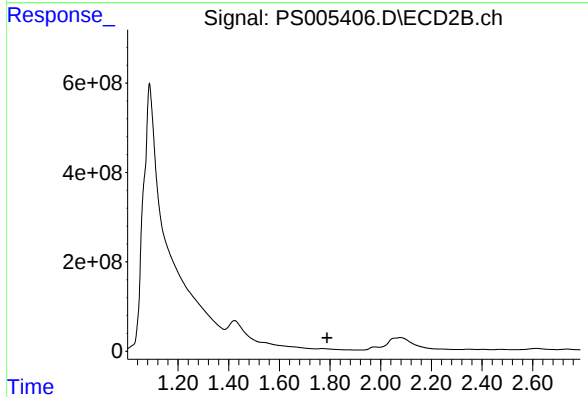


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

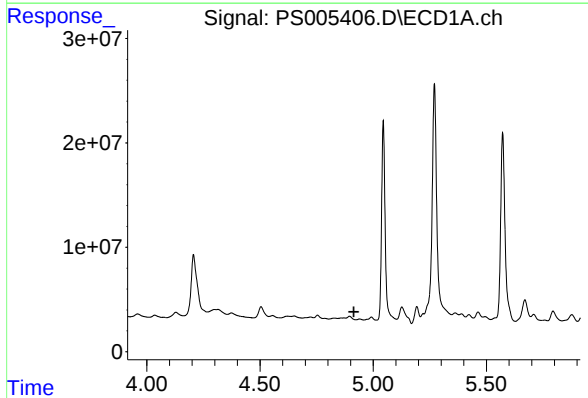


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

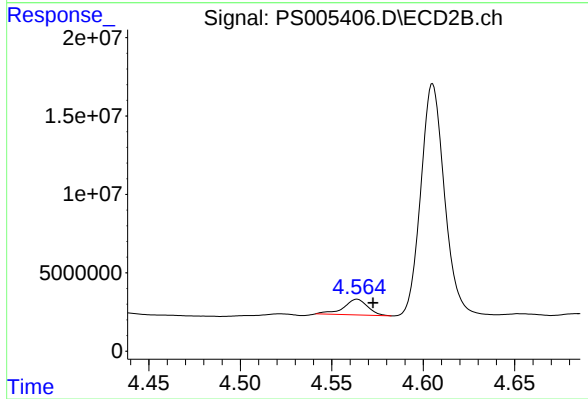

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.564 min
Delta R.T.: -0.009 min
Response: 9186993
Conc: 6.97 ng/ml

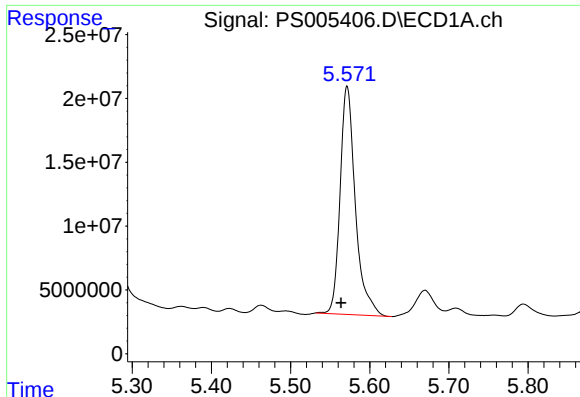

#4 2,4-DCAA


R.T.: 5.572 min
Delta R.T.: 0.008 min
Response: 239844250
Conc: 163.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-A

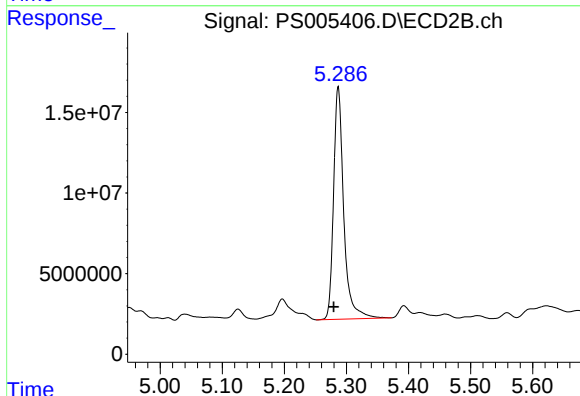


#4 2,4-DCAA

R.T.: 5.287 min
Delta R.T.: 0.007 min
Response: 164528702
Conc: 164.14 ng/ml

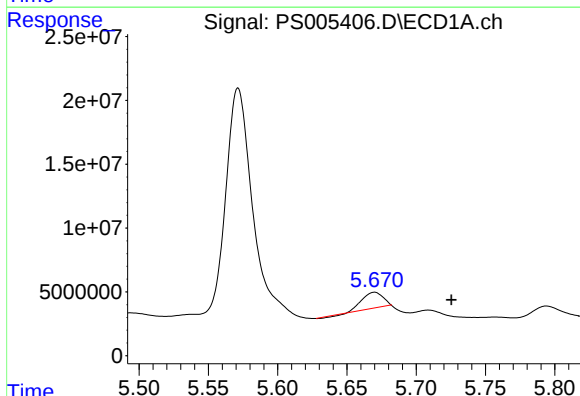


#5 DICAMBA

R.T.: 5.670 min
Delta R.T.: -0.056 min
Response: 13016983
Conc: 2.28 ng/ml

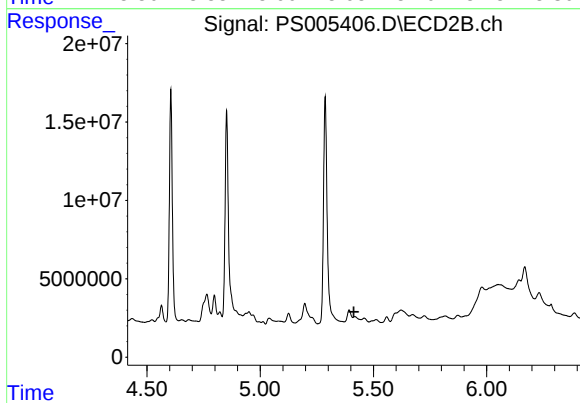

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

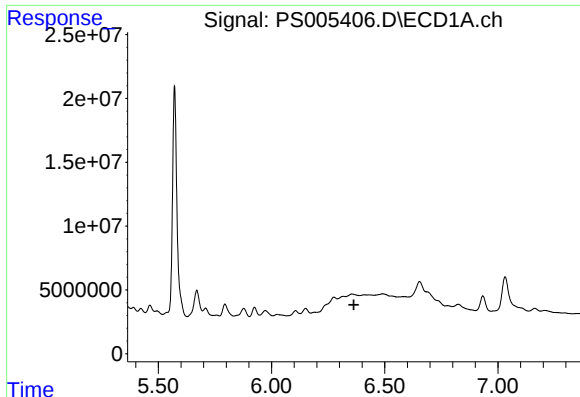

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-A

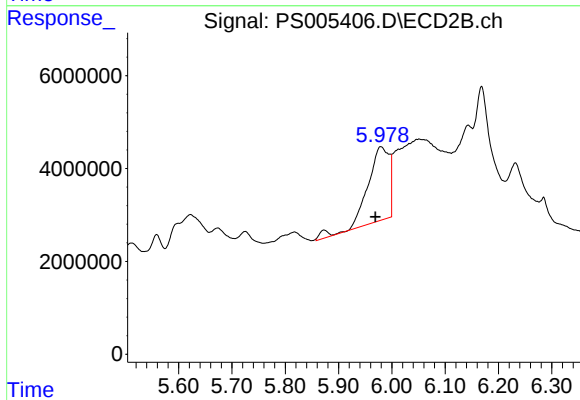


#8 DICHLORPROP

R.T.: 5.980 min
Delta R.T.: 0.011 min
Response: 45523904
Conc: 47.15 ng/ml

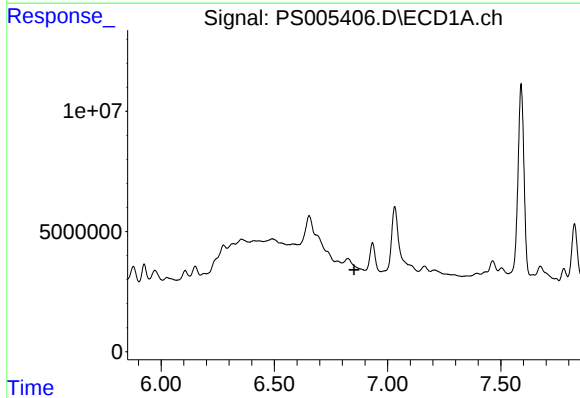


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

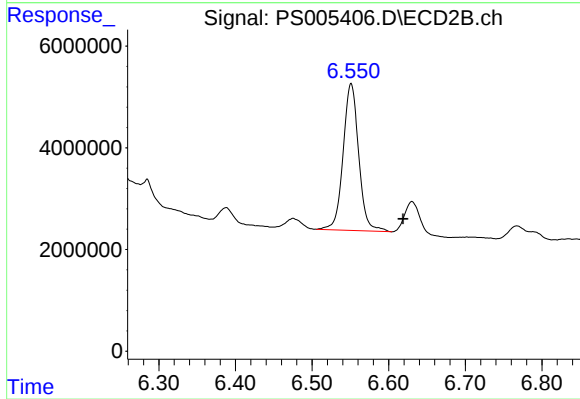

#10 Pentachlorophenol


R.T.: 6.551 min
Delta R.T.: -0.068 min
Response: 40966289
Conc: 3.19 ng/ml

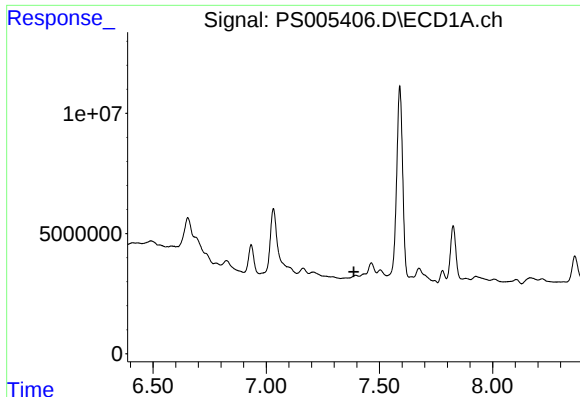

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-A

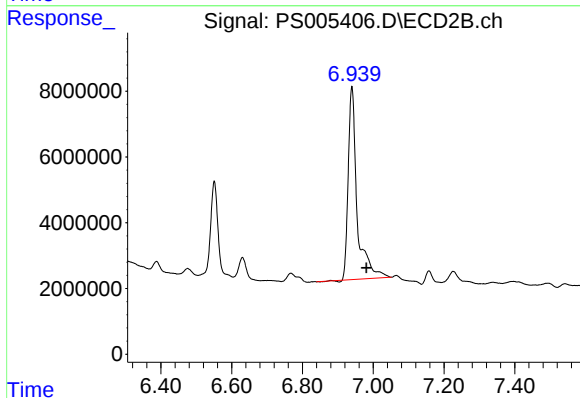


#11 2,4,5-TP (SILVEX)

R.T.: 6.940 min
Delta R.T.: -0.041 min
Response: 102092776
Conc: 19.17 ng/ml

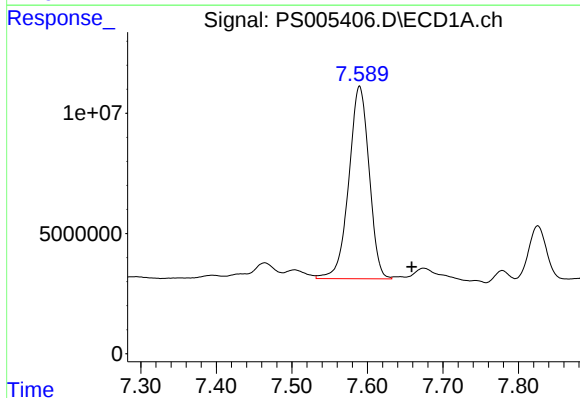

#12 2,4,5-T

R.T.: 7.590 min
Delta R.T.: -0.069 min
Response: 149456809
Conc: 18.57 ng/ml

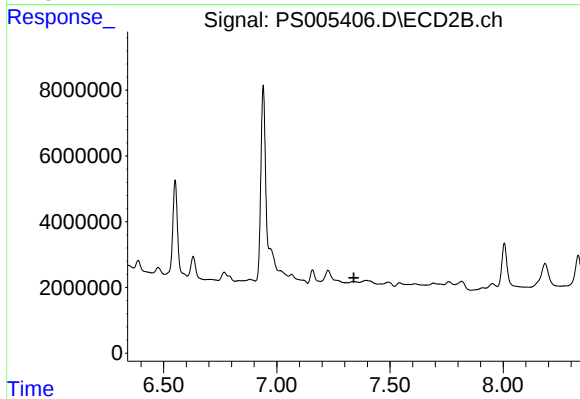

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.