

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
 Data File : PS005410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2019 20:27
 Operator : SM\AJ
 Sample : K3624-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PL-01-070319-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 00:42:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.588	5.304	264.8E6	171.7E6	180.384	171.261
Target Compounds							
1) T	Dalapon	2.096	0.000	31110179	0	16.877	N.D. #
2) T	3,5-DICHL...	0.000	4.622	0	155.2E6	N.D.	117.705
9) T	2,4-D	0.000	6.186	0	26952589	N.D.	24.167
10) T	Pentachlo...	0.000	6.567	0	30630720	N.D.	2.383
11) T	2,4,5-TP ...	0.000	6.957	0	89582039	N.D.	16.822
12) T	2,4,5-T	7.606	0.000	153.6E6	0	19.080	N.D. #
15) T	Picloram	9.161	9.117	112.3E6	89508935	9.770	11.861



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070819\
Data File : PS005410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2019 20:27
Operator : SM\AJ
Sample : K3624-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PL-01-070319-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 00:42:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

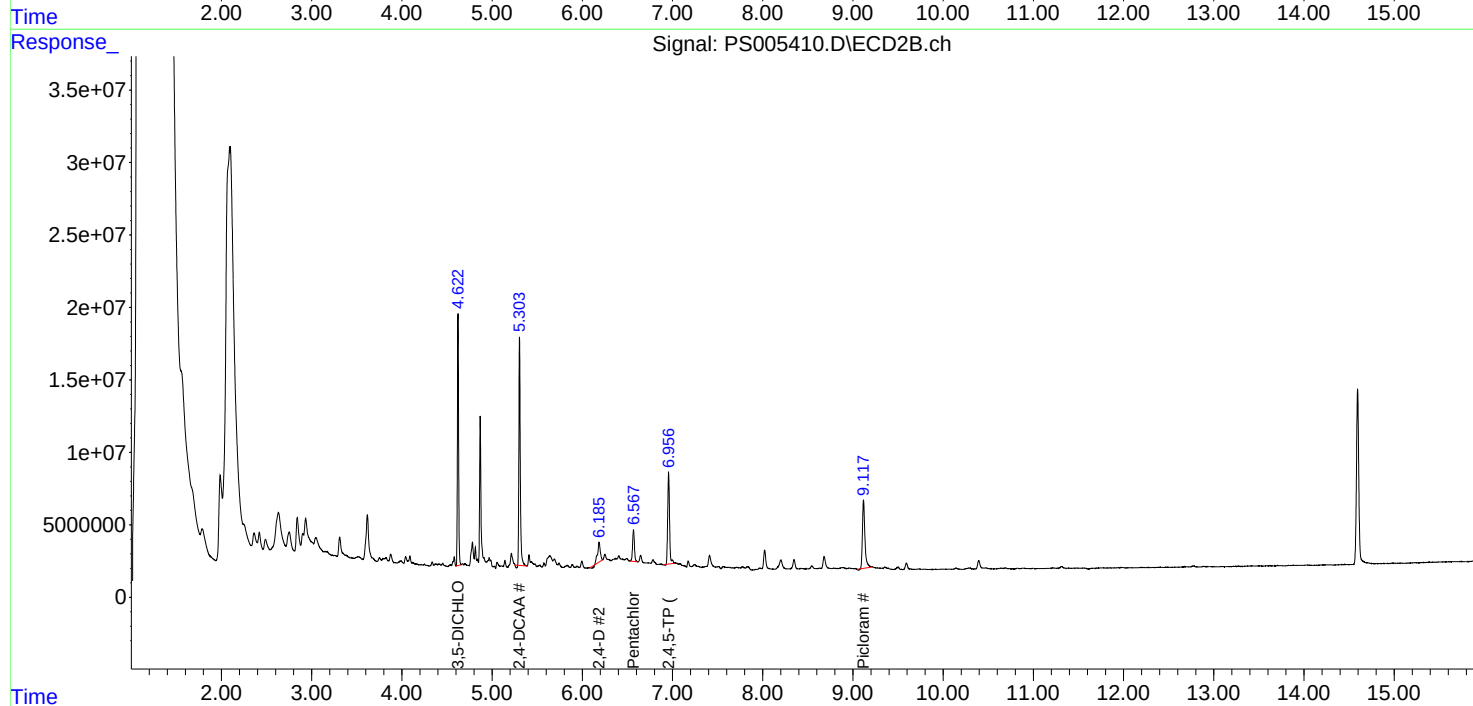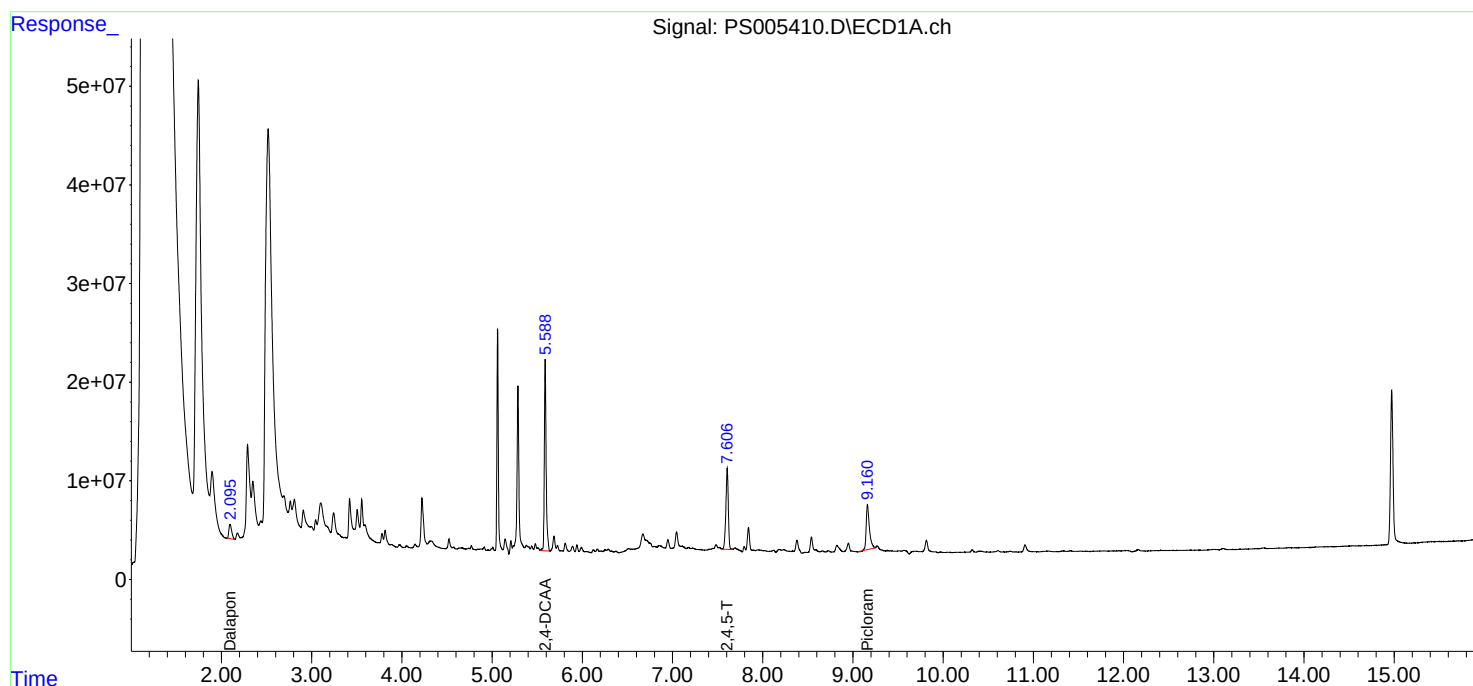


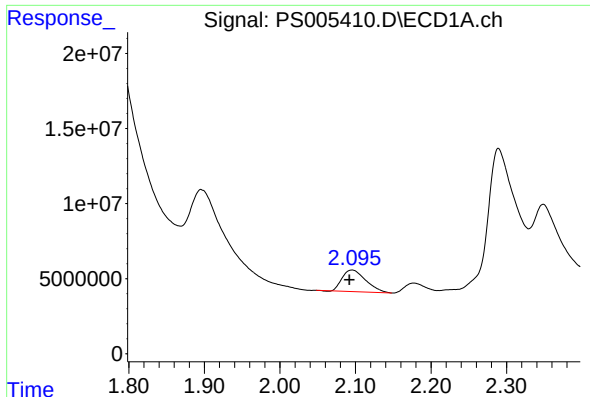

#1 Dalapon


R.T.: 2.096 min
Delta R.T.: 0.004 min
Response: 31110179
Conc: 16.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-C

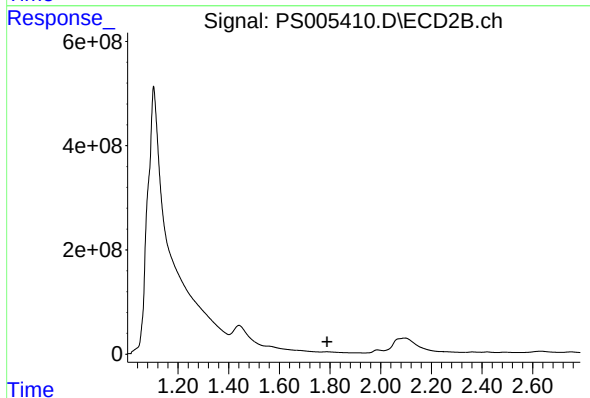


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

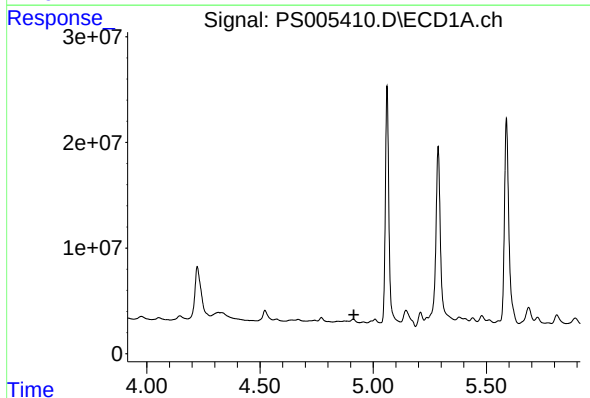


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

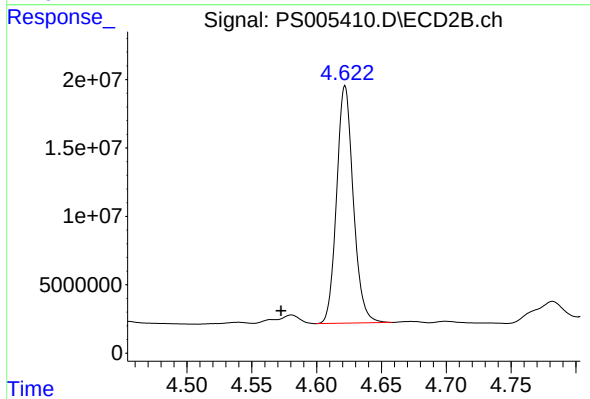

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.622 min
Delta R.T.: 0.049 min
Response: 155219009
Conc: 117.71 ng/ml

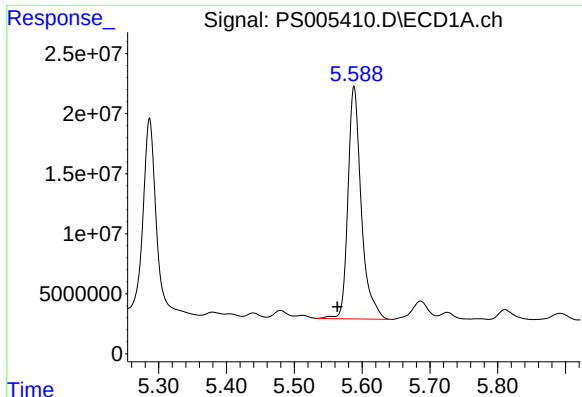

#4 2,4-DCAA


R.T.: 5.588 min
Delta R.T.: 0.025 min
Response: 264784195
Conc: 180.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-C

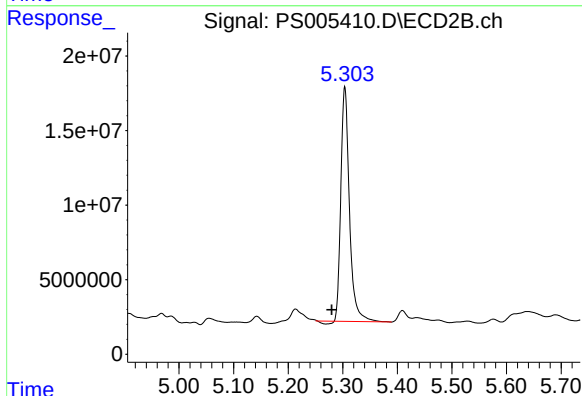


#4 2,4-DCAA

R.T.: 5.304 min
Delta R.T.: 0.024 min
Response: 171666415
Conc: 171.26 ng/ml

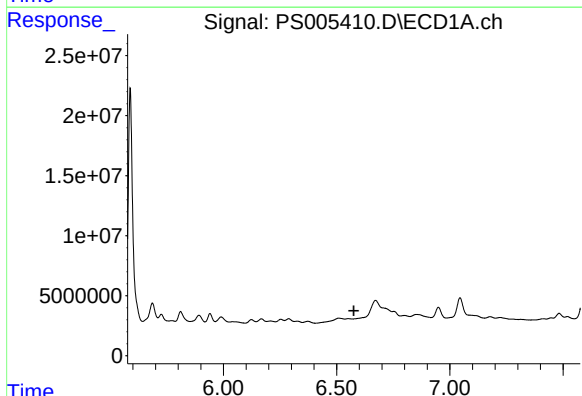


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.576 min
Response: 0
Conc: N.D.

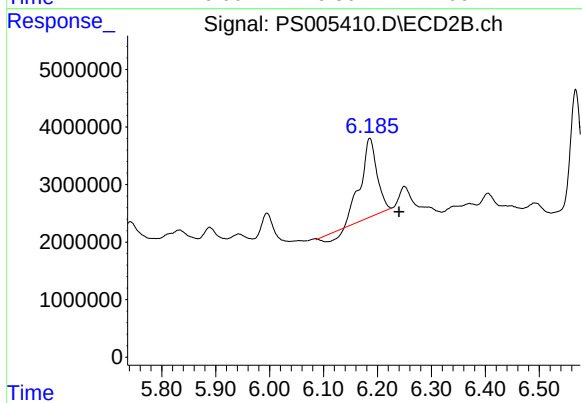

#9 2,4-D


R.T.: 6.186 min
Delta R.T.: -0.054 min
Response: 26952589
Conc: 24.17 ng/ml

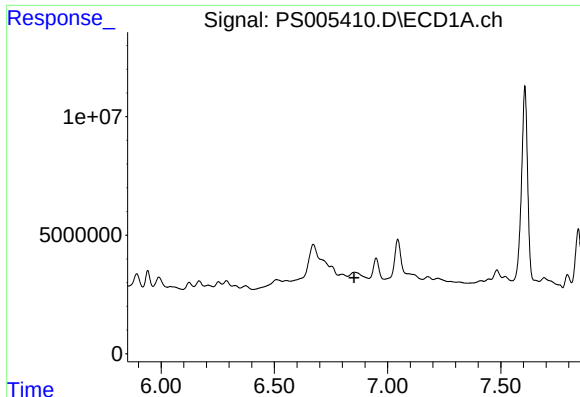

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-C

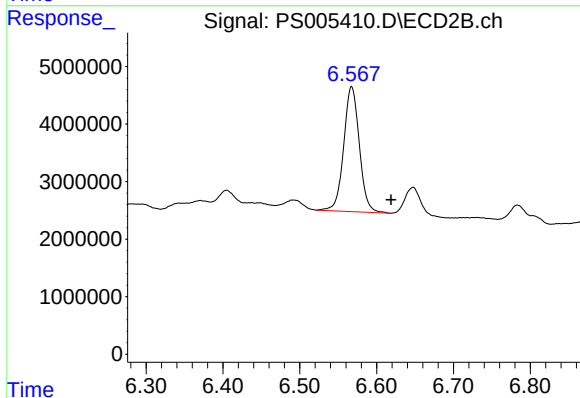


#10 Pentachlorophenol

R.T.: 6.567 min
Delta R.T.: -0.052 min
Response: 30630720
Conc: 2.38 ng/ml

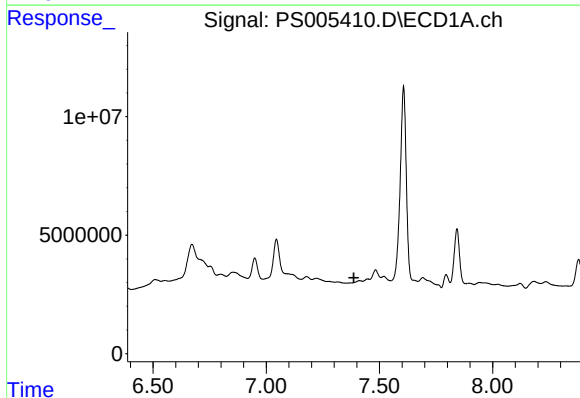


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

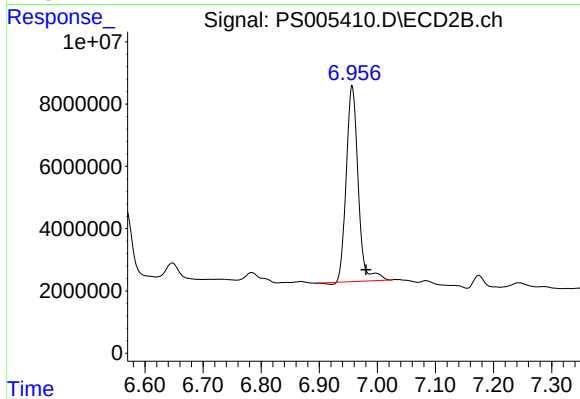

#11 2,4,5-TP (SILVEX)


R.T.: 6.957 min
Delta R.T.: -0.024 min
Response: 89582039
Conc: 16.82 ng/ml

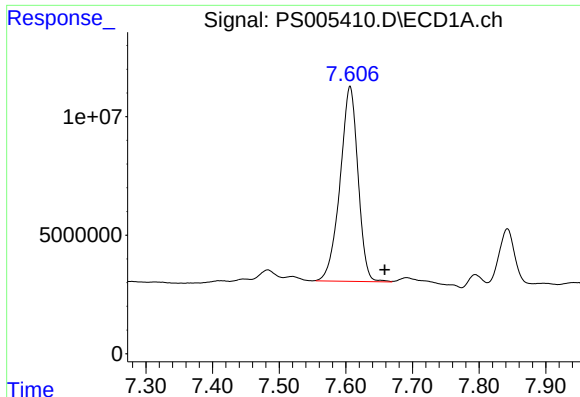

#12 2,4,5-T


R.T.: 7.606 min
Delta R.T.: -0.052 min
Response: 153555946
Conc: 19.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-070319-C

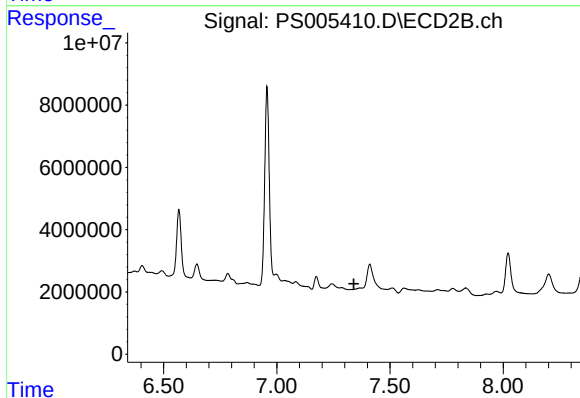


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

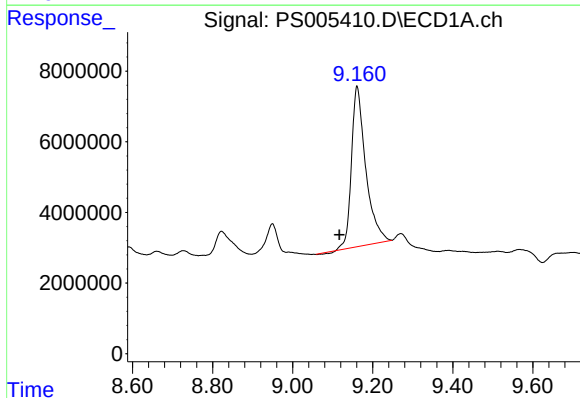

#15 Picloram

R.T.: 9.161 min
Delta R.T.: 0.044 min
Response: 112273445
Conc: 9.77 ng/ml

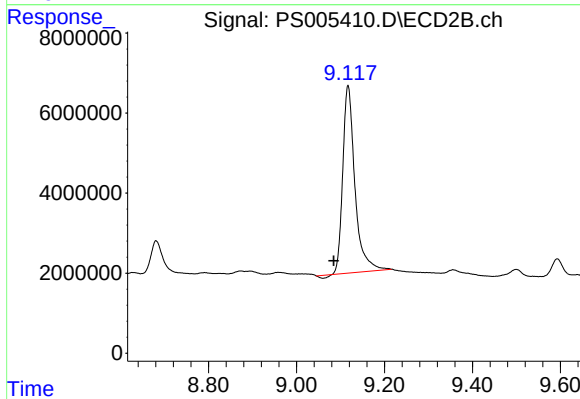

#15 Picloram

R.T.: 9.117 min
Delta R.T.: 0.032 min
Response: 89508935
Conc: 11.86 ng/ml