

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070919\
 Data File : PS005420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2019 09:54
 Operator : SM\AJ
 Sample : K3555-12
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SAMPLE-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 12:04:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.287	582.3E6	385.8E6	396.673	384.847
Target Compounds							
2) T	3,5-DICHL...	0.000	4.606	0	187.1E6	N.D.	141.870
5) T	DICAMBA	0.000	5.393	0	7405073	N.D.	1.978
11) T	2,4,5-TP ...	0.000	6.940	0	85278844	N.D.	16.014
12) T	2,4,5-T	7.596	7.397	170.1E6	24308372	21.140	4.766 #
15) T	Picloram	9.150	9.101	143.5E6	103.4E6	12.484	13.697
16) T	DCPA	0.000	9.101	0	103.4E6	N.D.	15.184



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070919\
Data File : PS005420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2019 09:54
Operator : SM\AJ
Sample : K3555-12
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SAMPLE-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 12:04:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

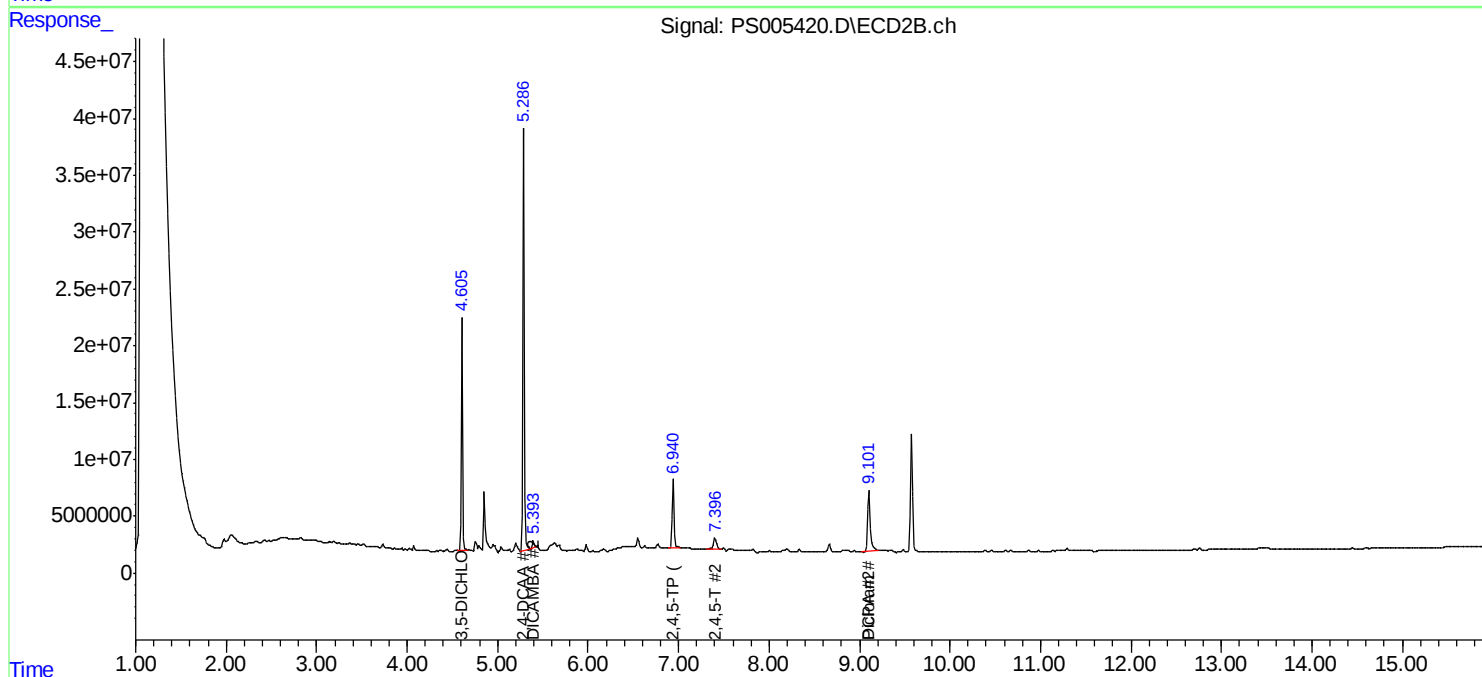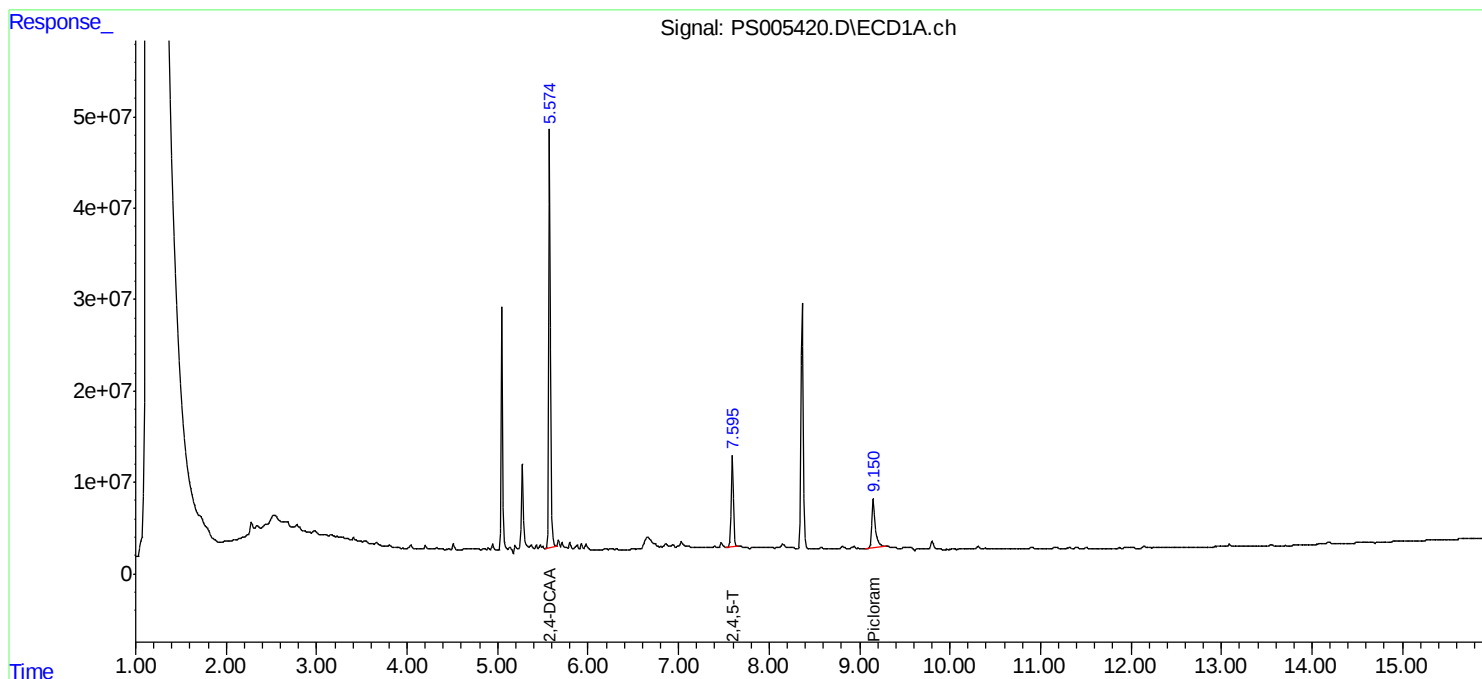


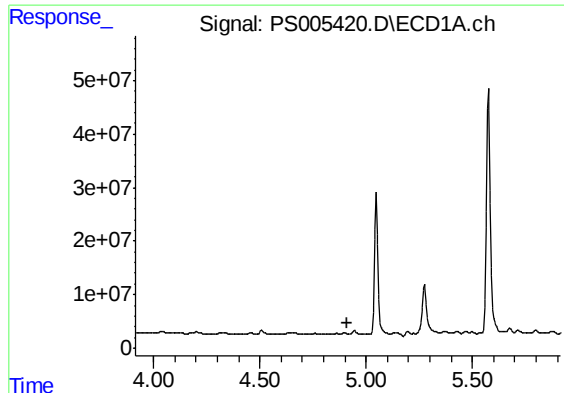

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-9

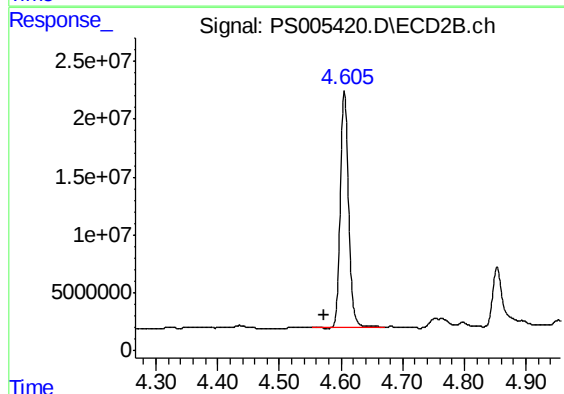


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.606 min
Delta R.T.: 0.033 min
Response: 187085303
Conc: 141.87 ng/ml

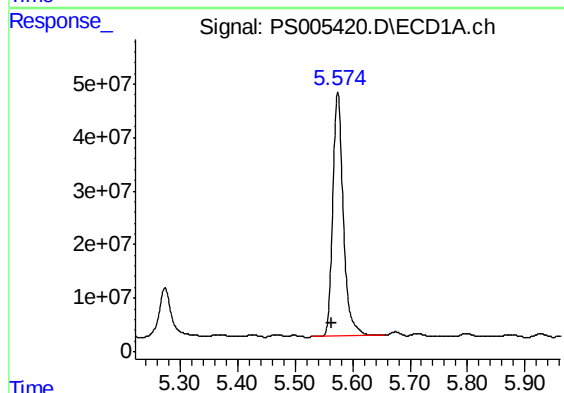


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: 0.011 min
Response: 582273833
Conc: 396.67 ng/ml

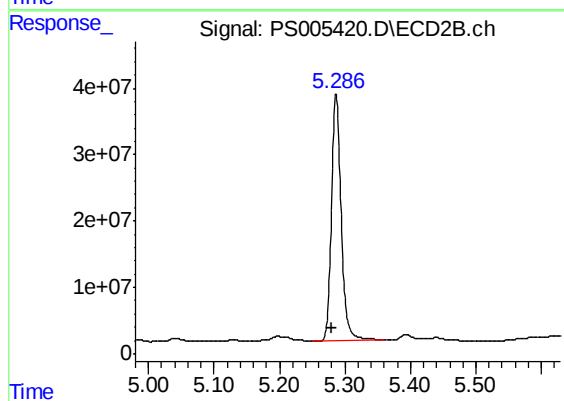

#4 2,4-DCAA


R.T.: 5.287 min
Delta R.T.: 0.007 min
Response: 385758997
Conc: 384.85 ng/ml

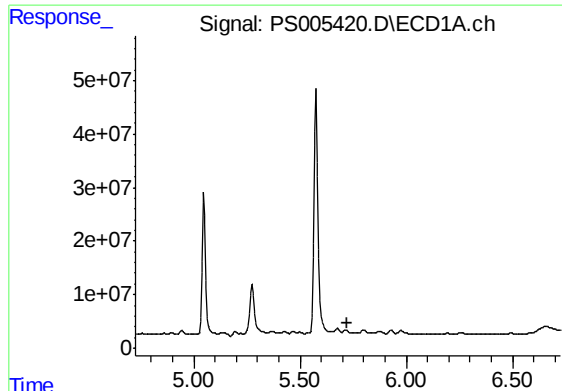

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-9

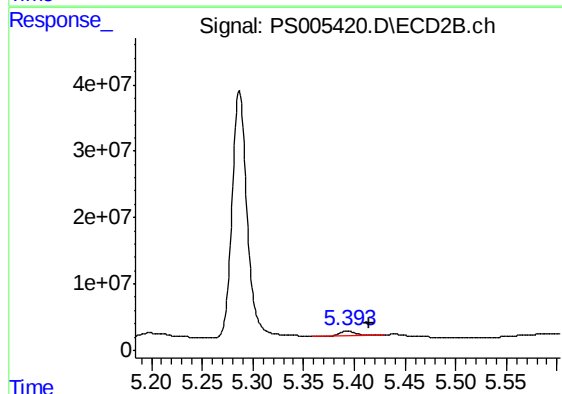


#5 DICAMBA

R.T.: 5.393 min
Delta R.T.: -0.021 min
Response: 7405073
Conc: 1.98 ng/ml

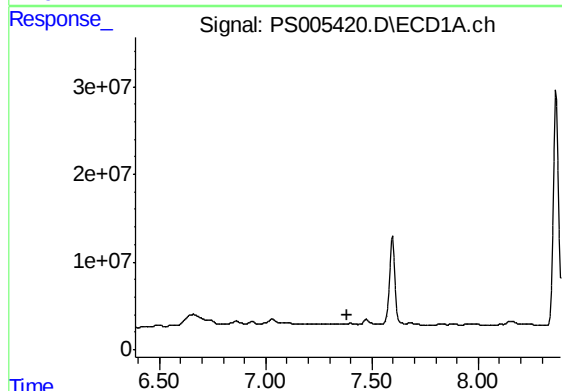


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

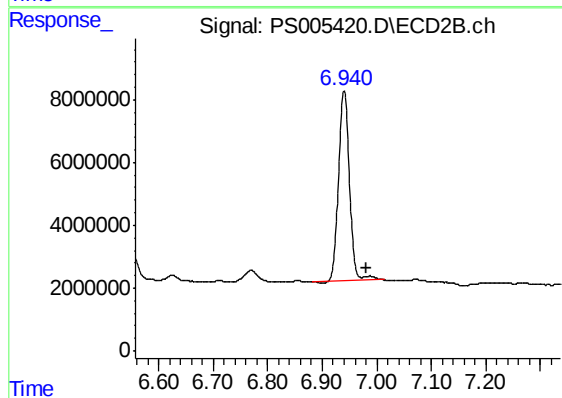

#11 2,4,5-TP (SILVEX)


R.T.: 6.940 min
Delta R.T.: -0.041 min
Response: 85278844
Conc: 16.01 ng/ml

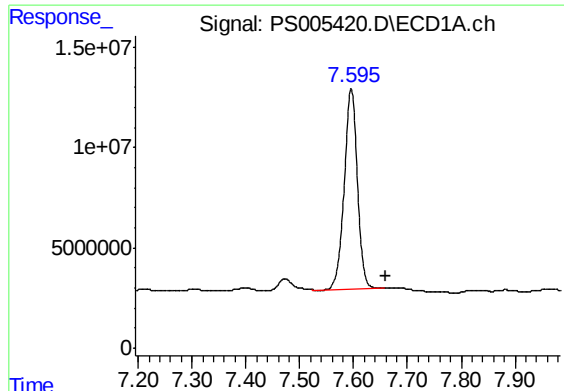

#12 2,4,5-T


R.T.: 7.596 min
Delta R.T.: -0.063 min
Response: 170130211
Conc: 21.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
SAMPLE-9

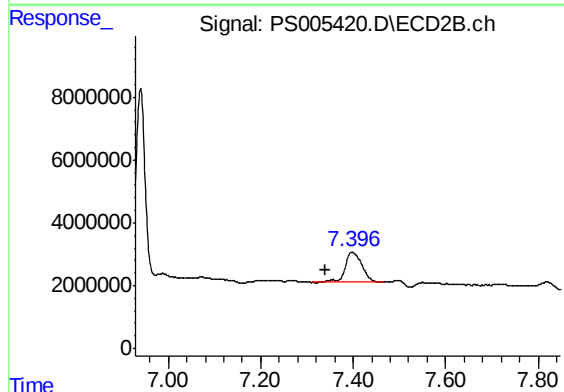


#12 2,4,5-T

R.T.: 7.397 min
Delta R.T.: 0.057 min
Response: 24308372
Conc: 4.77 ng/ml

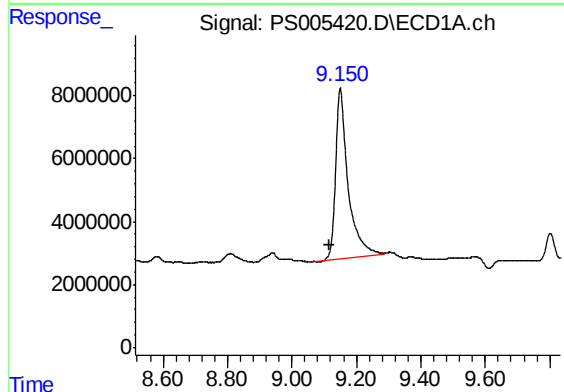


#15 Picloram

R.T.: 9.150 min
Delta R.T.: 0.033 min
Response: 143458057
Conc: 12.48 ng/ml

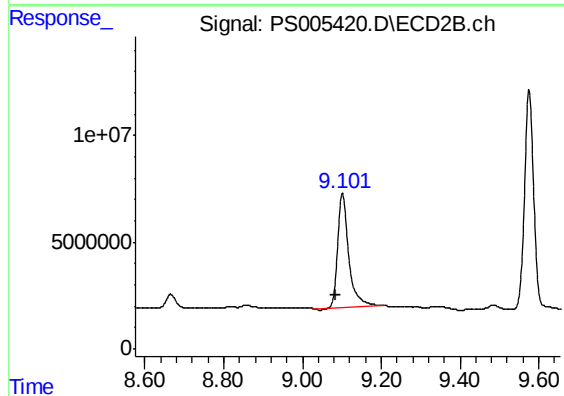

#15 Picloram


R.T.: 9.101 min
Delta R.T.: 0.016 min
Response: 103366322
Conc: 13.70 ng/ml

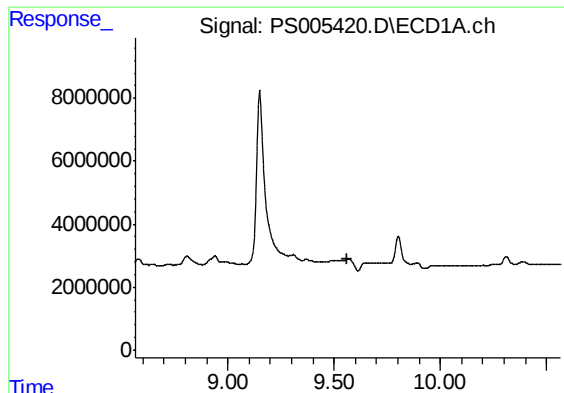

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SAMPLE-9

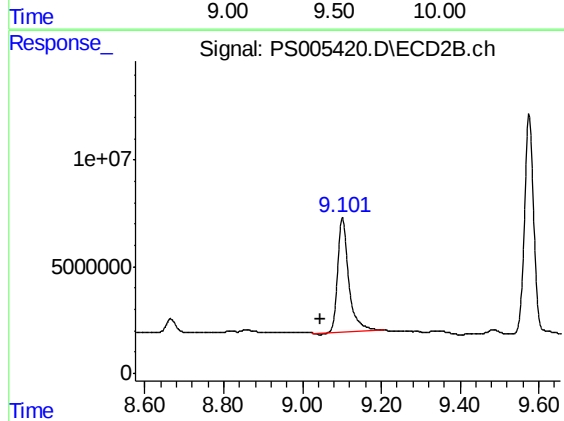

#16 DCPA

R.T.: 9.101 min
Delta R.T.: 0.056 min
Response: 103366322
Conc: 15.18 ng/ml