

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 11:47
 Operator : SM\AJ
 Sample : K3740-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:33:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.600	5.285	108.5E6	60258175	73.895	60.116
Target Compounds							
1) T	Dalapon	2.108	0.000	28218660	0	15.309	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	93809454	N.D.	71.137
5) T	DICAMBA	5.699	0.000	27641661	0	4.845	N.D. #
6) T	MCPD	5.908	0.000	12184439	0	2.783	N.D. #
7) T	MCPA	6.090	5.674	23224621	37369191	3.698	9.225 #
10) T	Pentachlo...	6.884	6.621	77374319	54374798	3.932	4.229
12) T	2,4,5-T	7.609	0.000	81135530	0	10.082	N.D. #
13) T	2,4-DB	8.252	7.850	50062007	52420313	43.099	80.294 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 11:47
Operator : SM\AJ
Sample : K3740-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:33:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

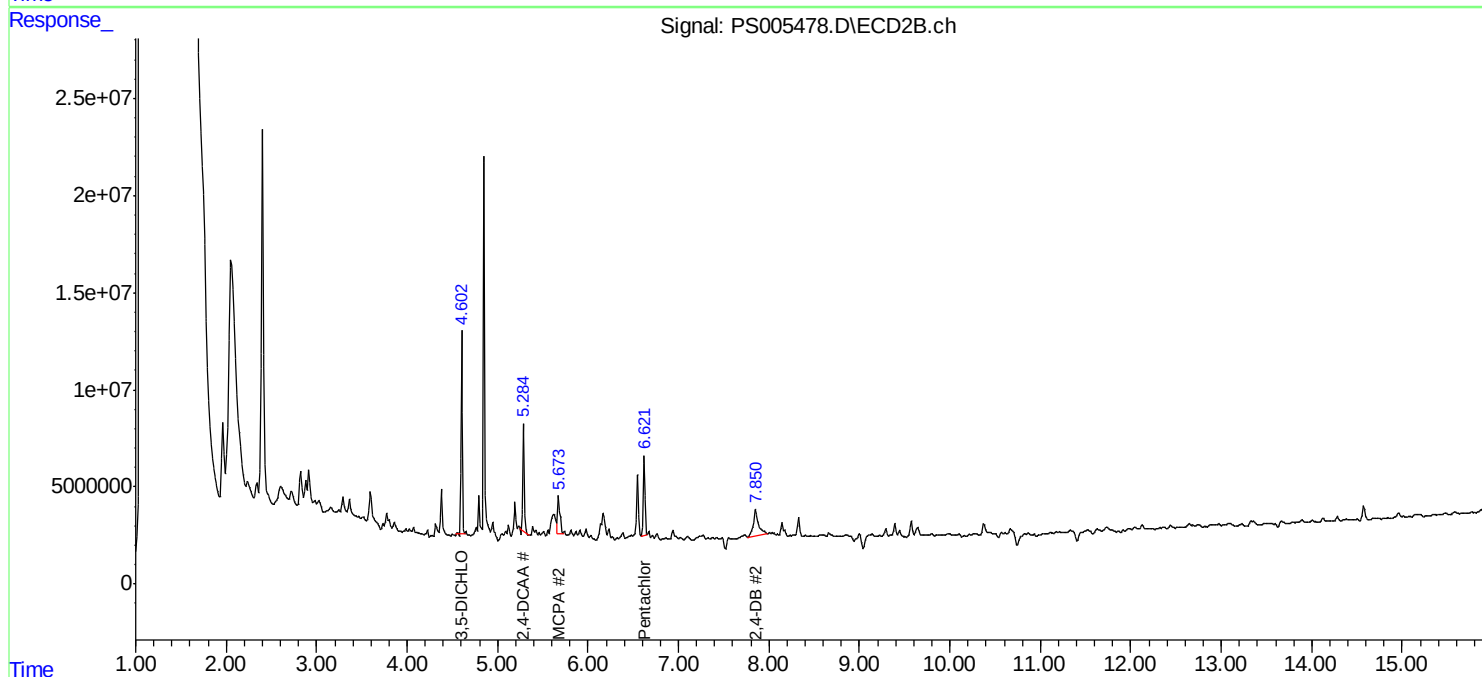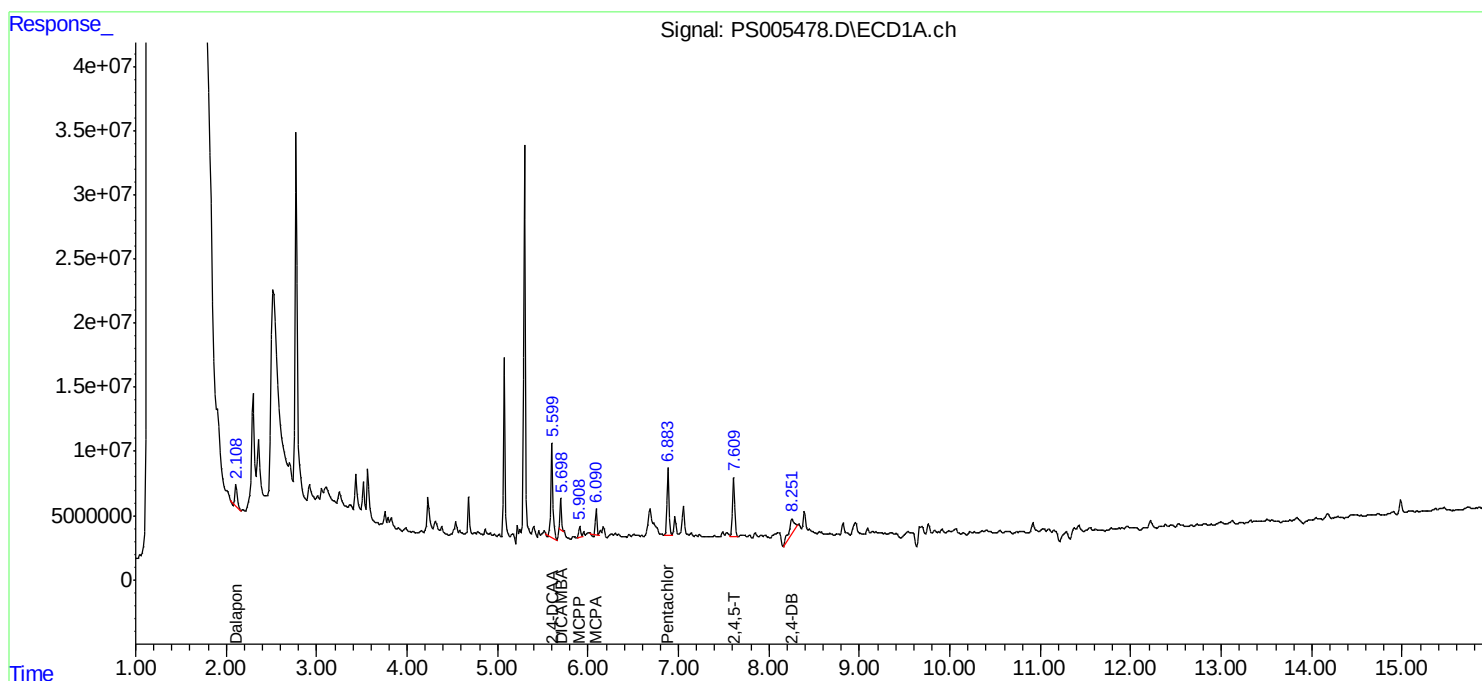


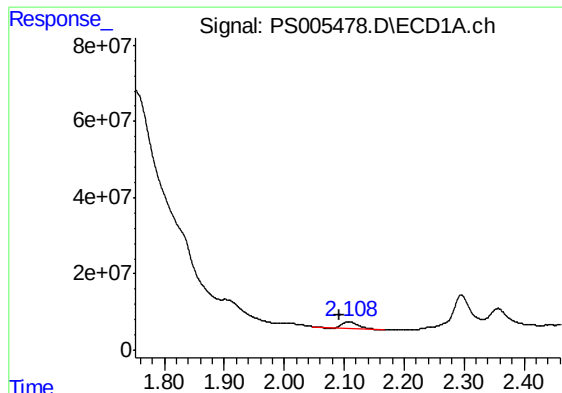

#1 Dalapon


R.T.: 2.108 min
Delta R.T.: 0.016 min
Response: 28218660
Conc: 15.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

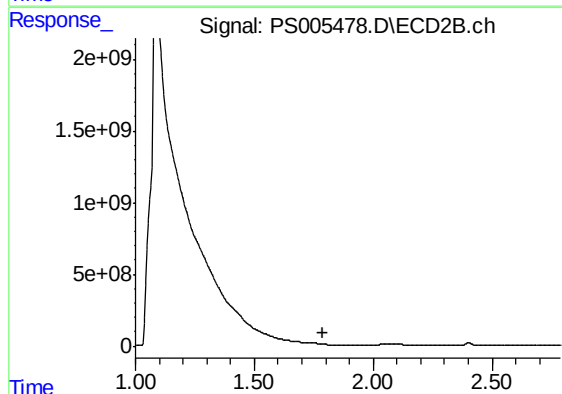


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

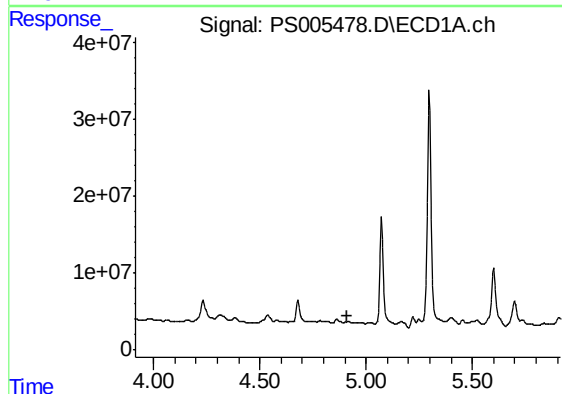


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

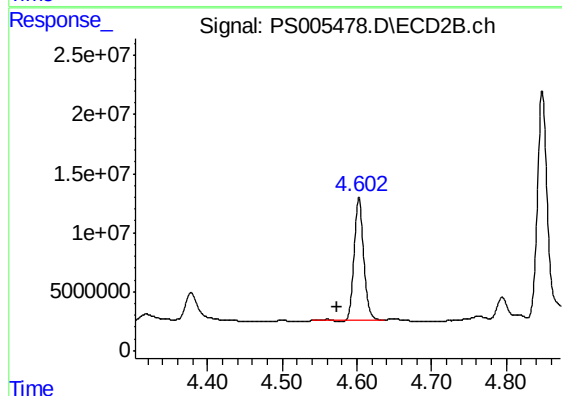

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.030 min
Response: 93809454
Conc: 71.14 ng/ml

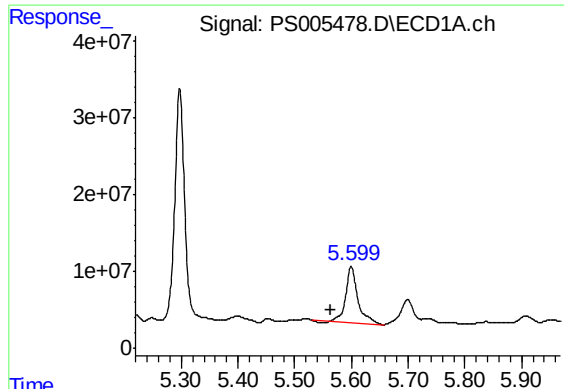

#4 2,4-DCAA


R.T.: 5.600 min
Delta R.T.: 0.036 min
Response: 108470082
Conc: 73.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

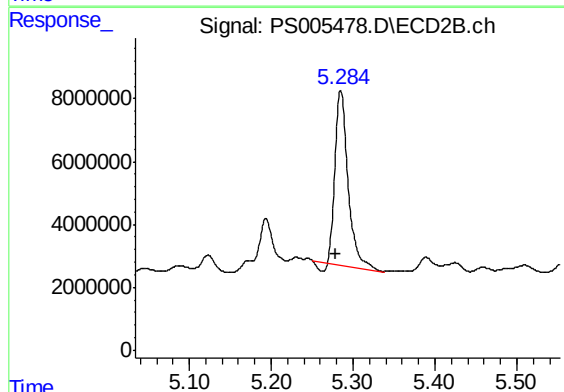


#4 2,4-DCAA

R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 60258175
Conc: 60.12 ng/ml

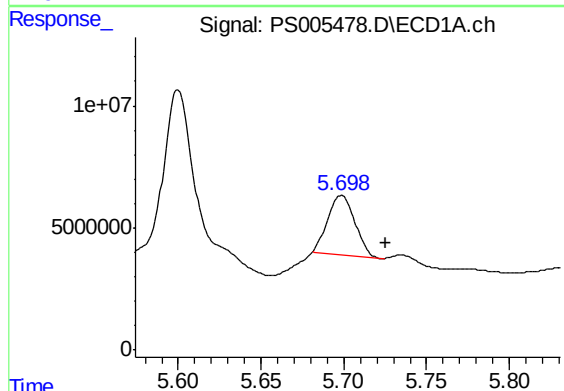


#5 DICAMBA

R.T.: 5.699 min
Delta R.T.: -0.027 min
Response: 27641661
Conc: 4.85 ng/ml

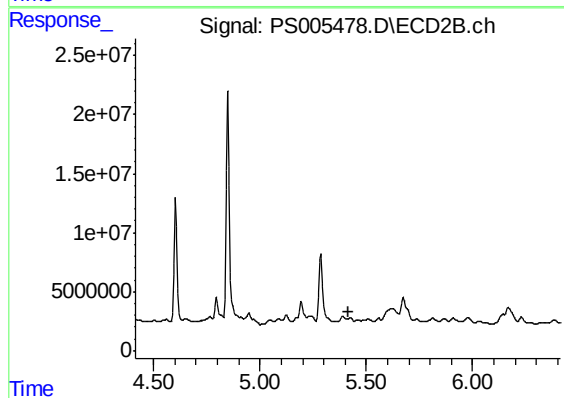

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

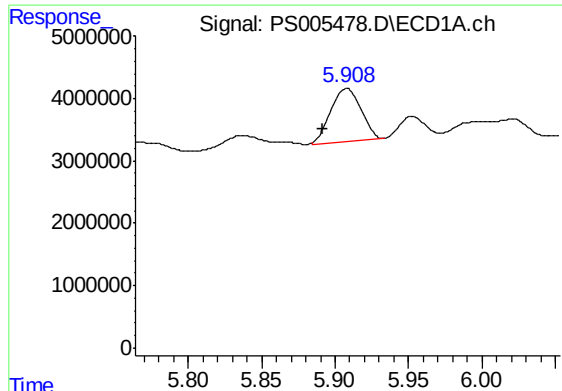

#6 MCPP


R.T.: 5.908 min
Delta R.T.: 0.016 min
Response: 12184439
Conc: 2.78 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

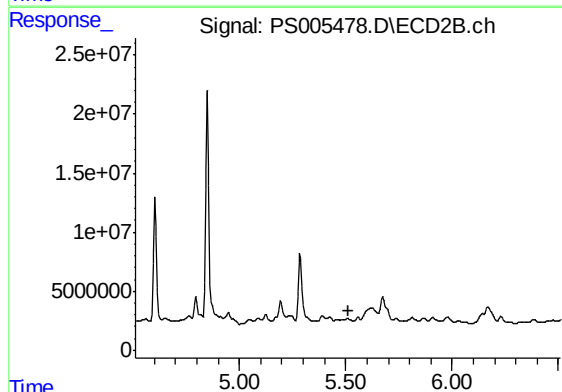


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.511 min
Response: 0
Conc: N.D.

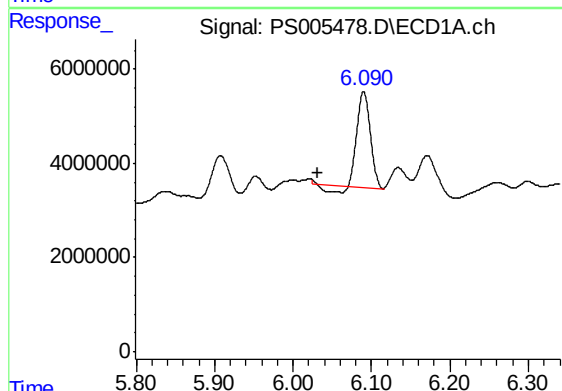


#7 MCPA

R.T.: 6.090 min
Delta R.T.: 0.058 min
Response: 23224621
Conc: 3.70 ug/ml

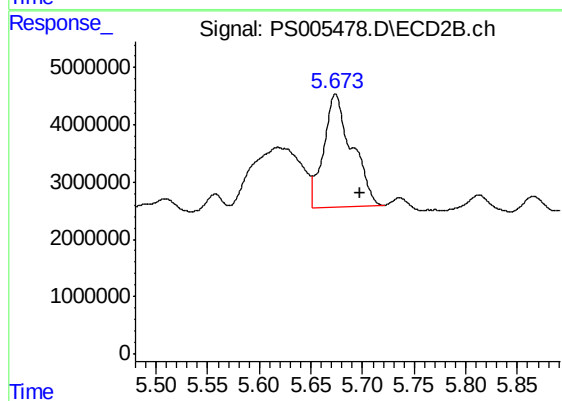

#7 MCPA


R.T.: 5.674 min
Delta R.T.: -0.024 min
Response: 37369191
Conc: 9.23 ug/ml

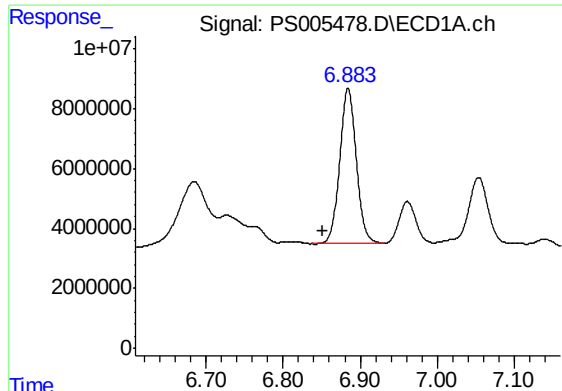

#10 Pentachlorophenol


R.T.: 6.884 min
Delta R.T.: 0.032 min
Response: 77374319
Conc: 3.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

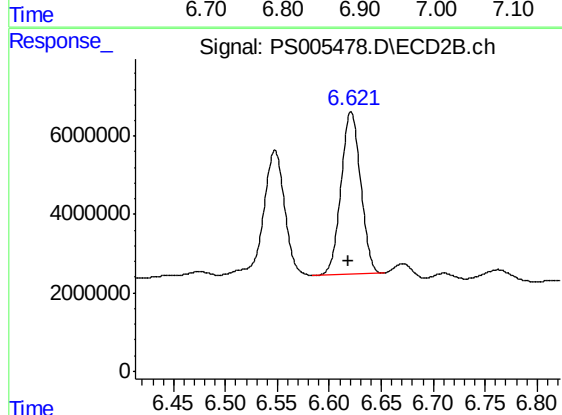


#10 Pentachlorophenol

R.T.: 6.621 min
Delta R.T.: 0.002 min
Response: 54374798
Conc: 4.23 ng/ml

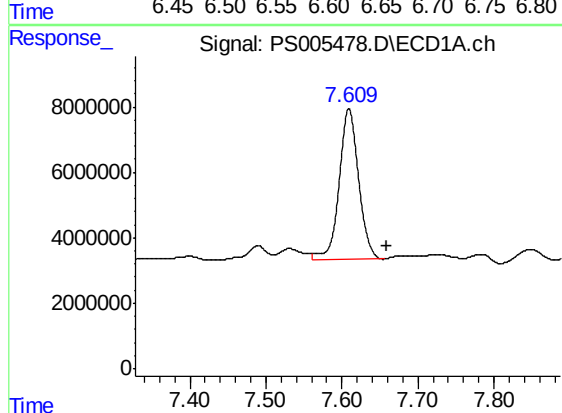


#12 2,4,5-T

R.T.: 7.609 min
Delta R.T.: -0.049 min
Response: 81135530
Conc: 10.08 ng/ml

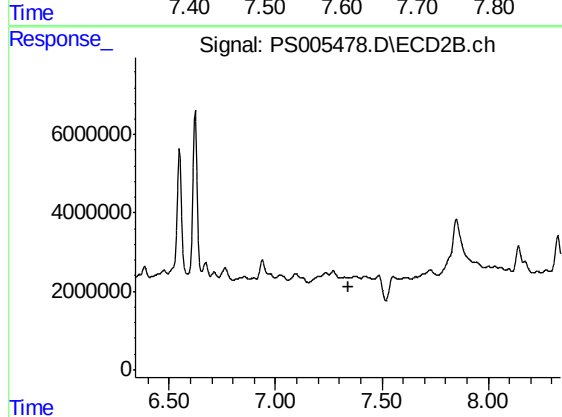

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

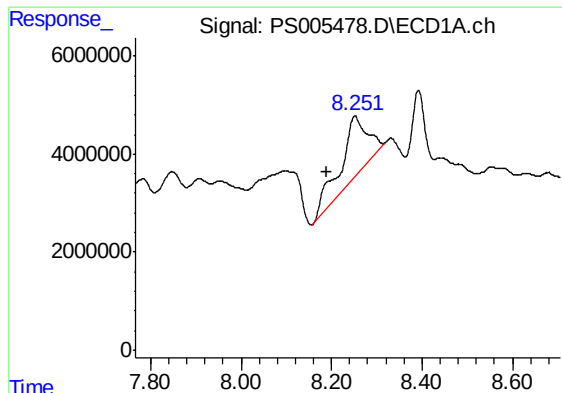

#13 2,4-DB

R.T.: 8.252 min
Delta R.T.: 0.062 min
Response: 50062007
Conc: 43.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

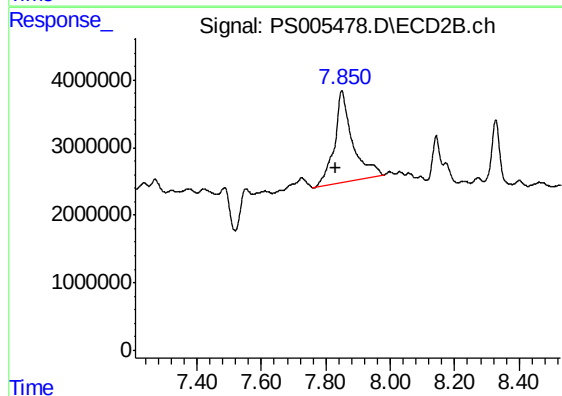

#13 2,4-DB

R.T.: 7.850 min
Delta R.T.: 0.020 min
Response: 52420313
Conc: 80.29 ng/ml