

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005482.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 16:37
 Operator : SM\AJ
 Sample : PB121343BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121343BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:16:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.568	5.280	806.3E6	519.9E6	549.291	518.702
Target Compounds							
1) T	Dalapon	2.075	1.771	102.3E6	15391086	55.476	11.668 #
2) T	3,5-DICHL...	0.000	4.597	0	82240720	N.D.	62.365
3) T	4-Nitroph...	5.374	0.000	25784901	0	35.600	N.D. #
5) T	DICAMBA	5.668	0.000	27751440	0	4.865	N.D. #
7) T	MCPA	6.061	5.671	24073980	17888411	3.834	4.416
12) T	2,4,5-T	0.000	7.388	0	40632038	N.D.	7.966
15) T	Picloram	9.143	9.095	237.6E6	171.4E6	20.679	22.707
16) T	DCPA	0.000	9.095	0	171.4E6	N.D.	25.172



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005482.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 16:37
Operator : SM\AJ
Sample : PB121343BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB121343BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:16:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

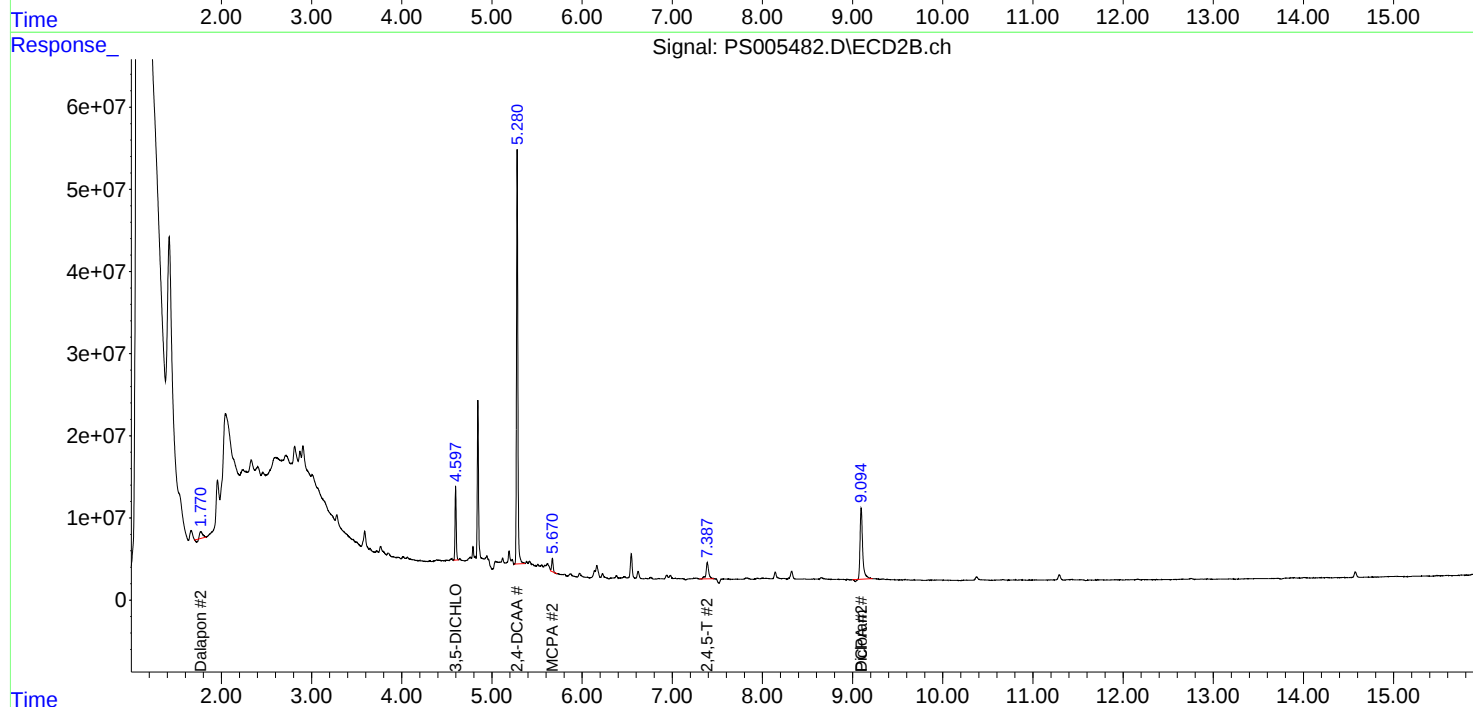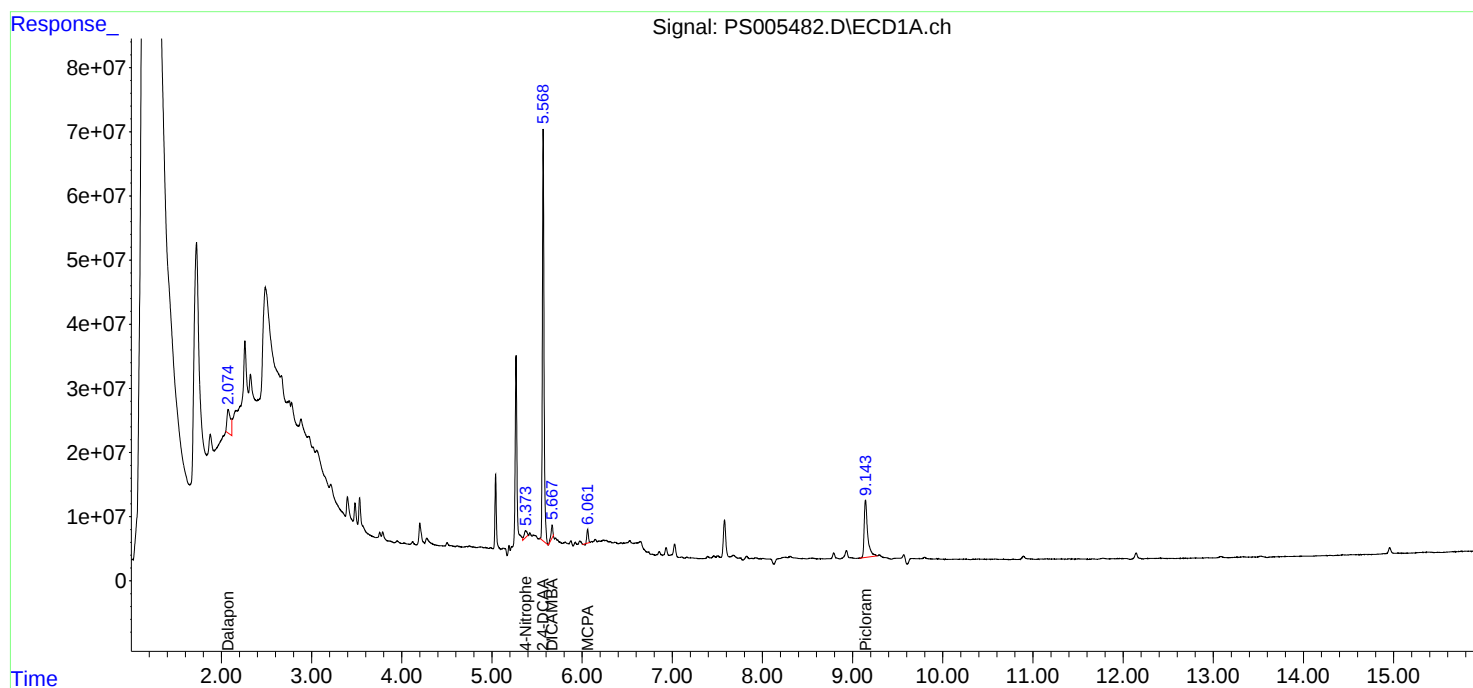


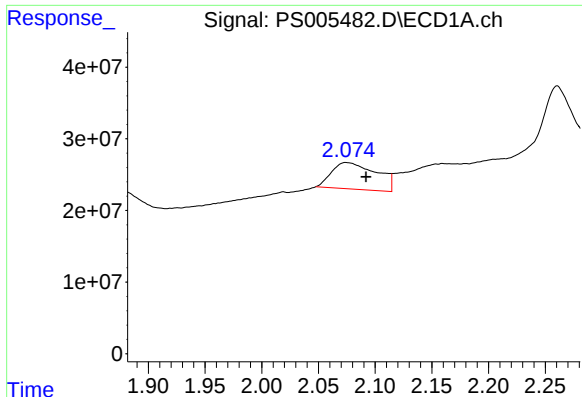

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.017 min
Response: 102258301
Conc: 55.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121343BL

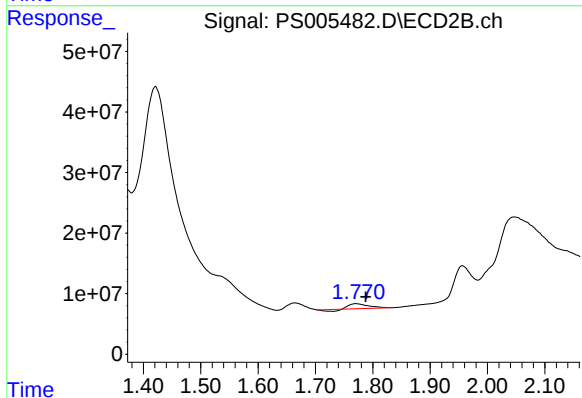


#1 Dalapon

R.T.: 1.771 min
Delta R.T.: -0.017 min
Response: 15391086
Conc: 11.67 ng/ml

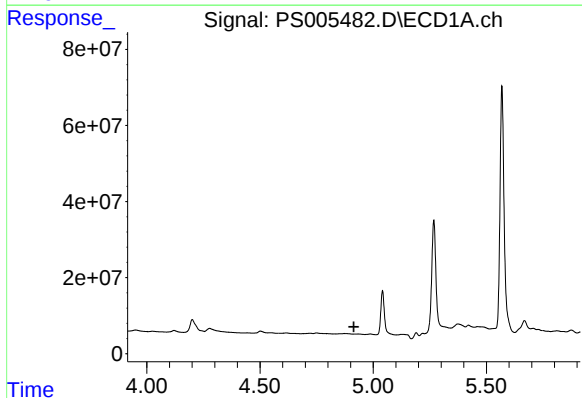


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

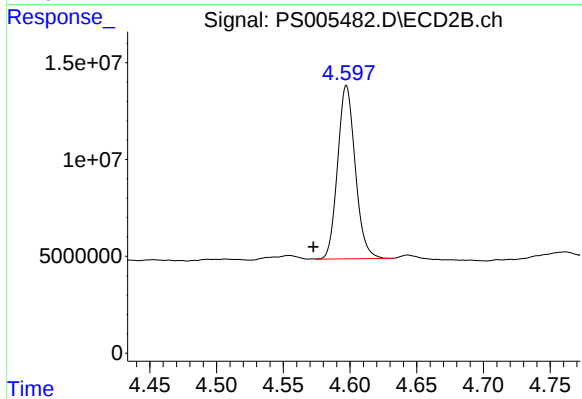

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.597 min
Delta R.T.: 0.025 min
Response: 82240720
Conc: 62.36 ng/ml

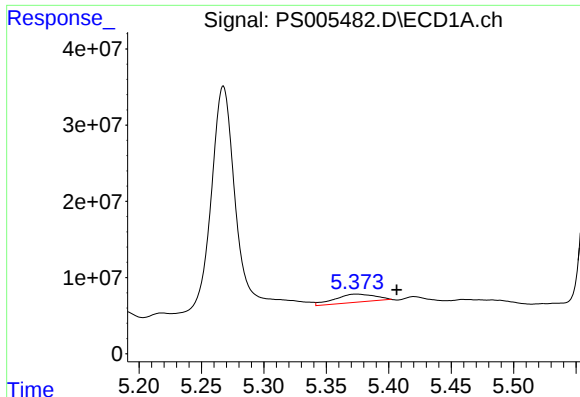

#3 4-Nitrophenol


R.T.: 5.374 min
Delta R.T.: -0.032 min
Response: 25784901
Conc: 35.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121343BL

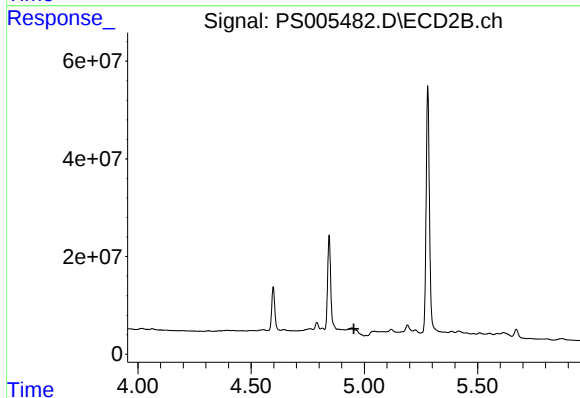


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

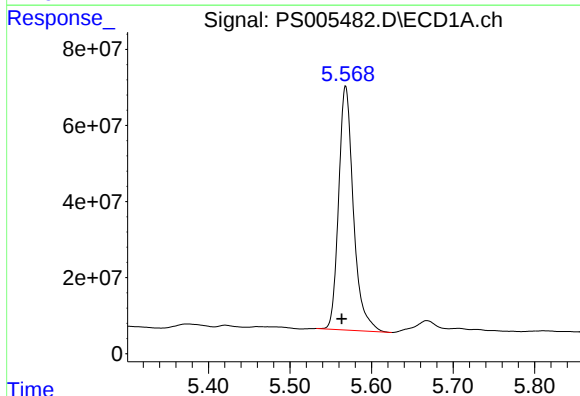


#4 2,4-DCAA

R.T.: 5.568 min
Delta R.T.: 0.005 min
Response: 806300986
Conc: 549.29 ng/ml

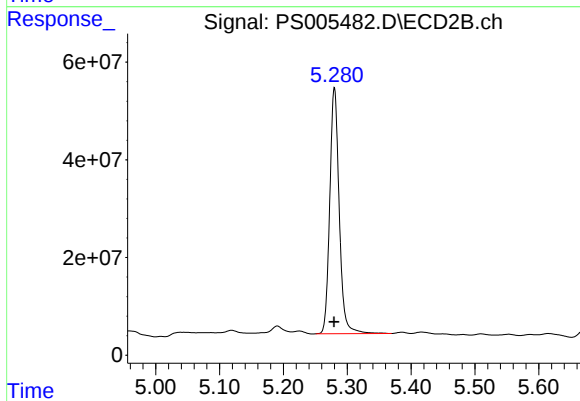

#4 2,4-DCAA


R.T.: 5.280 min
Delta R.T.: 0.000 min
Response: 519930726
Conc: 518.70 ng/ml

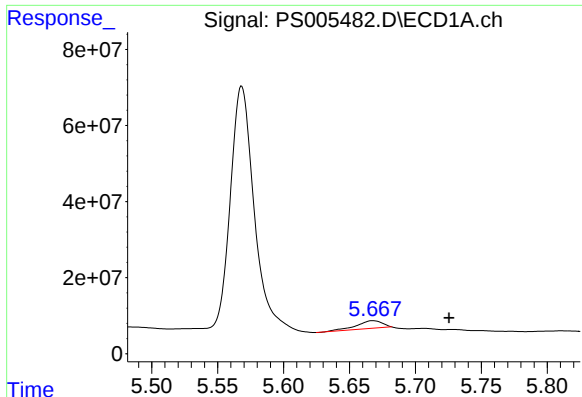

#5 DICAMBA


R.T.: 5.668 min
Delta R.T.: -0.057 min
Response: 27751440
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121343BL

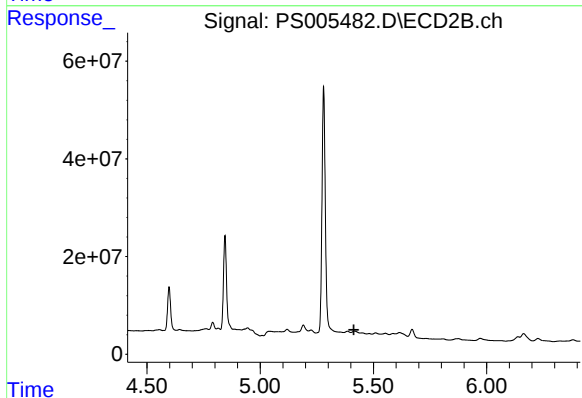


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

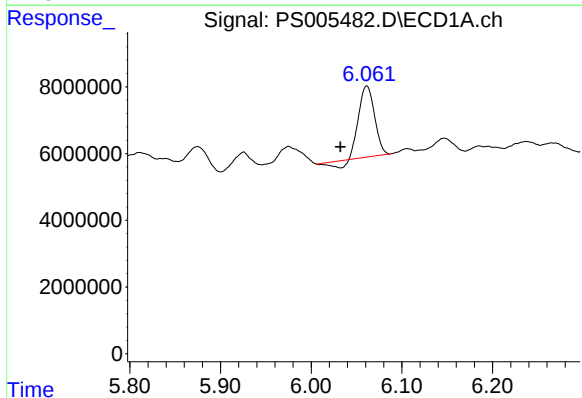


#7 MCPA

R.T.: 6.061 min
Delta R.T.: 0.029 min
Response: 24073980
Conc: 3.83 ug/ml

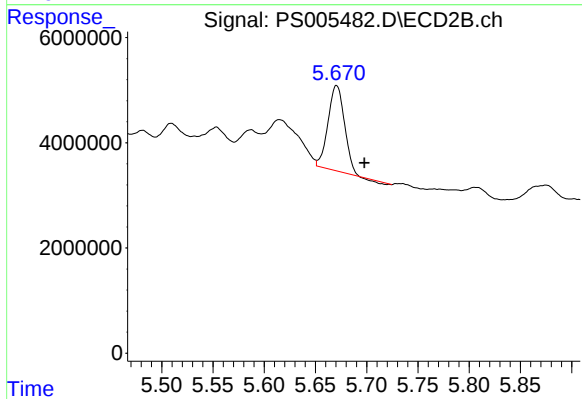

#7 MCPA


R.T.: 5.671 min
Delta R.T.: -0.027 min
Response: 17888411
Conc: 4.42 ug/ml

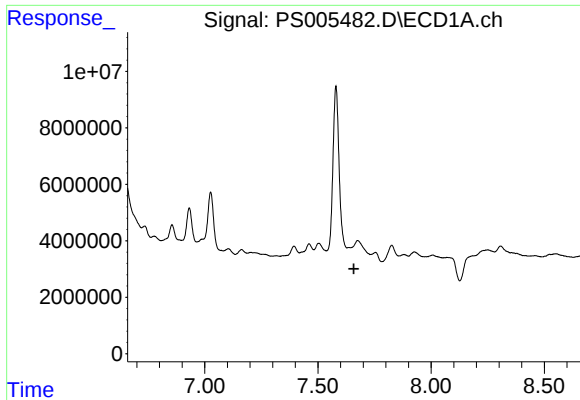

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121343BL

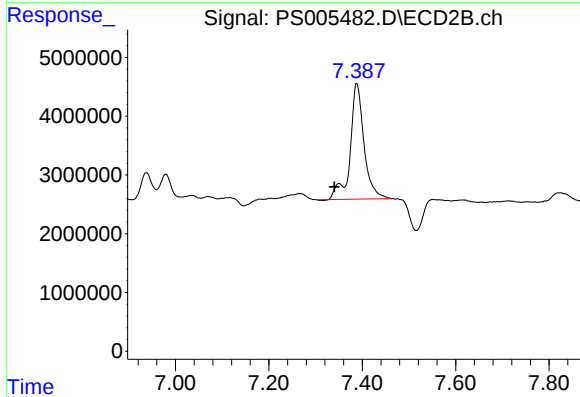


#12 2,4,5-T

R.T.: 7.388 min
Delta R.T.: 0.048 min
Response: 40632038
Conc: 7.97 ng/ml

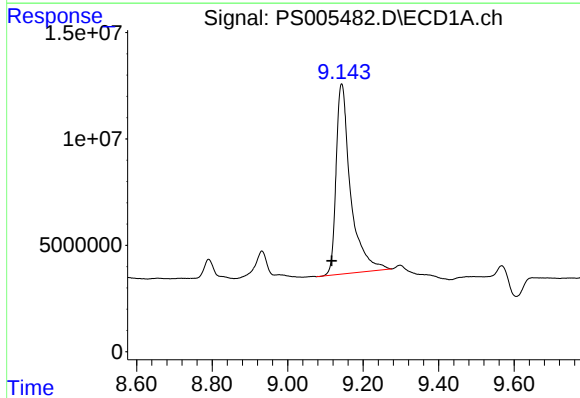


#15 Picloram

R.T.: 9.143 min
Delta R.T.: 0.026 min
Response: 237626725
Conc: 20.68 ng/ml

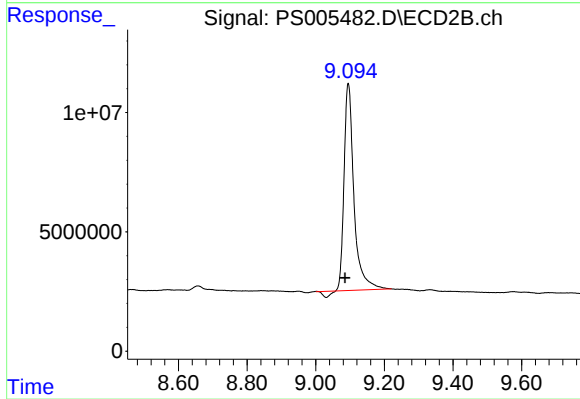

#15 Picloram


R.T.: 9.095 min
Delta R.T.: 0.010 min
Response: 171354547
Conc: 22.71 ng/ml

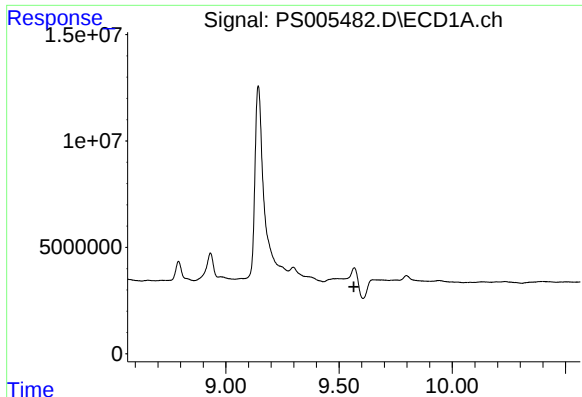

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121343BL

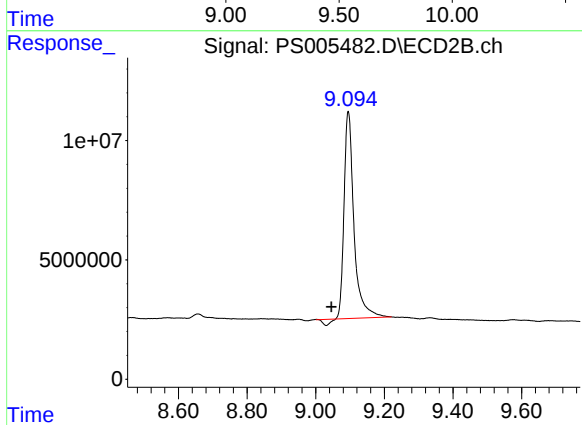

#16 DCPA

R.T.: 9.095 min
Delta R.T.: 0.049 min
Response: 171354547
Conc: 25.17 ng/ml