

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 17:44
 Operator : SM\AJ
 Sample : K3618-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HD-02-071119

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:17:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.566	5.282	467.2E6	326.4E6	318.264	325.603
Target Compounds							
1) T	Dalapon	2.075	0.000	63151542	0	34.260	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	230.3E6	N.D.	174.672
3) T	4-Nitroph...	5.357	4.997	15625601	15808403	21.574	31.525 #
5) T	DICAMBA	5.666	5.387	17762504	19261774	3.114	5.146 #
6) T	MCP	5.920	0.000	15095003	0	3.448	N.D. #
8) T	DICHLORPROP	0.000	5.972	0	14609341	N.D.	15.131
11) T	2,4,5-TP ...	0.000	6.935	0	133.3E6	N.D.	25.027
14) T	DINOSEB	0.000	8.180	0	85425652	N.D.	21.128
15) T	Picloram	9.104	0.000	29870291	0	2.599	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 17:44
Operator : SM\AJ
Sample : K3618-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
HD-02-071119

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:17:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

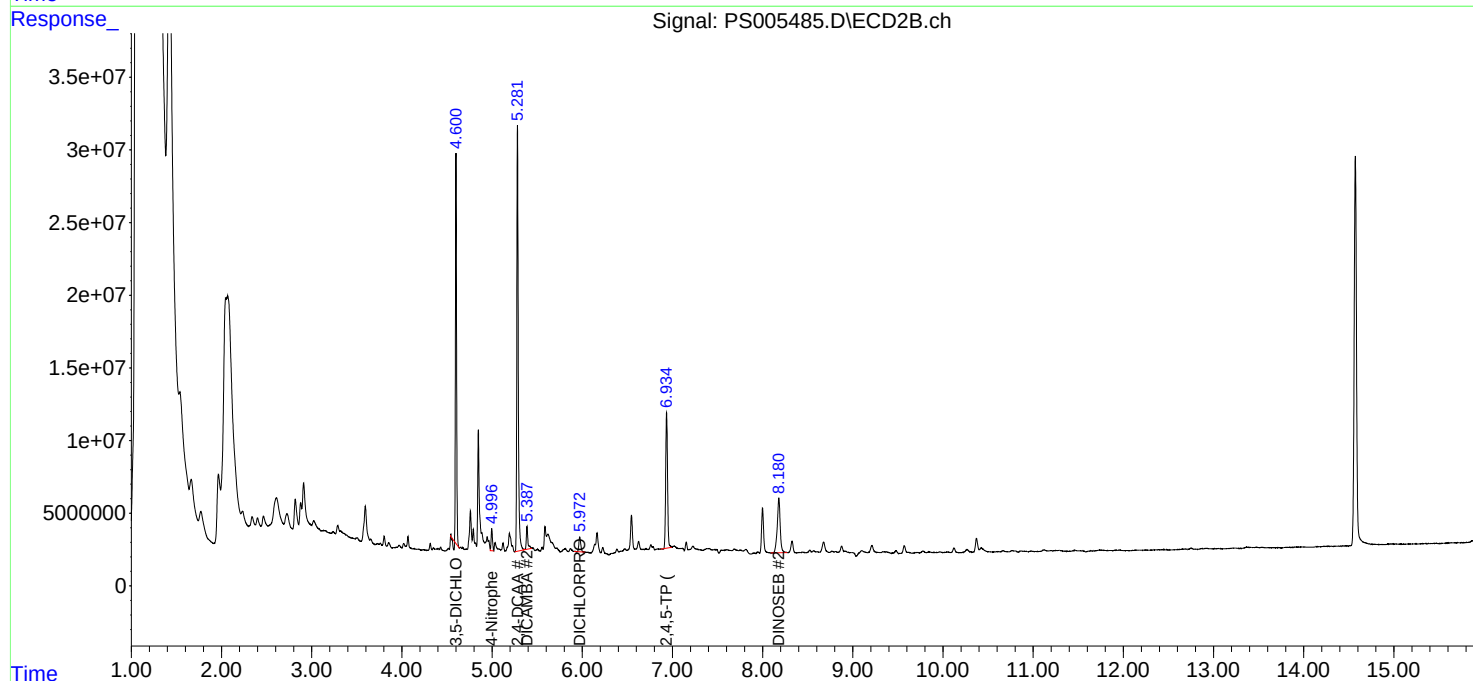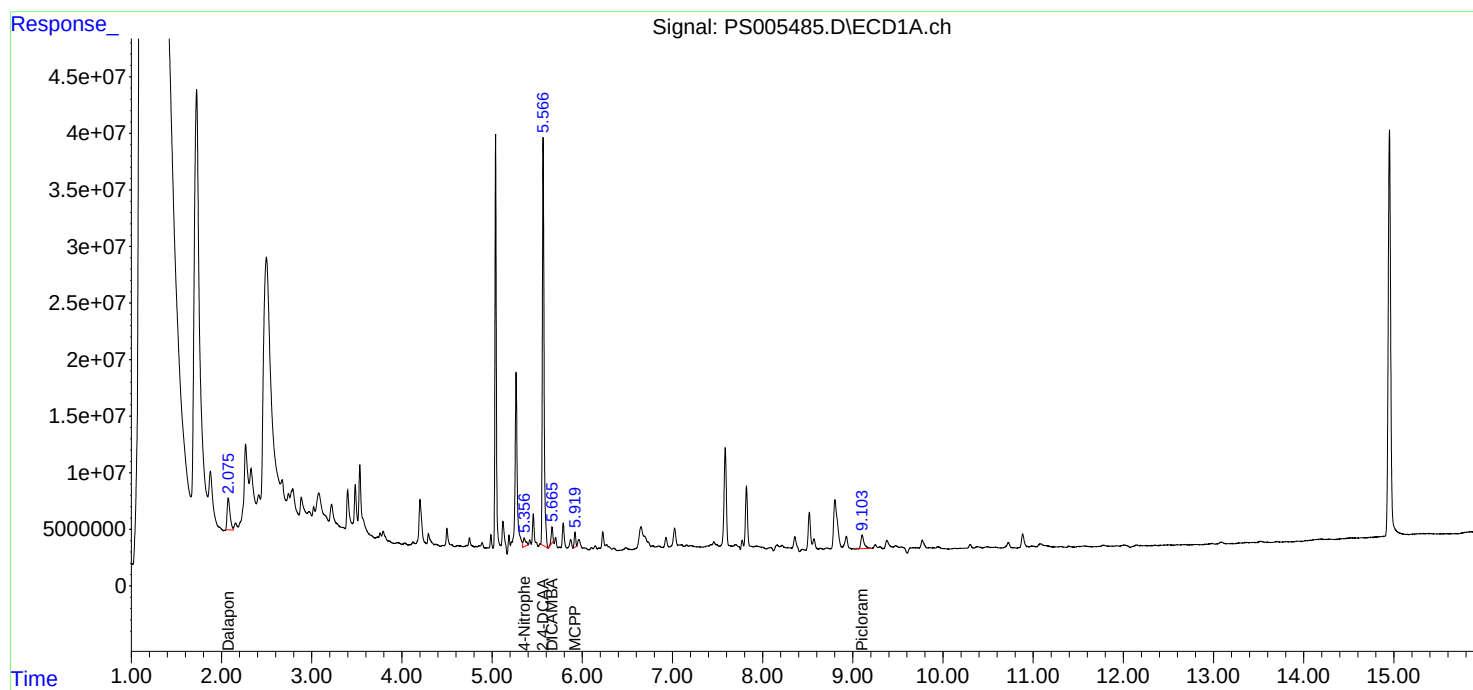


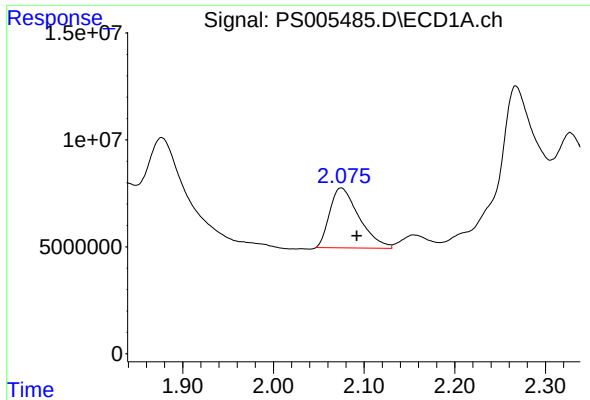

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.017 min
Response: 63151542
Conc: 34.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-071119

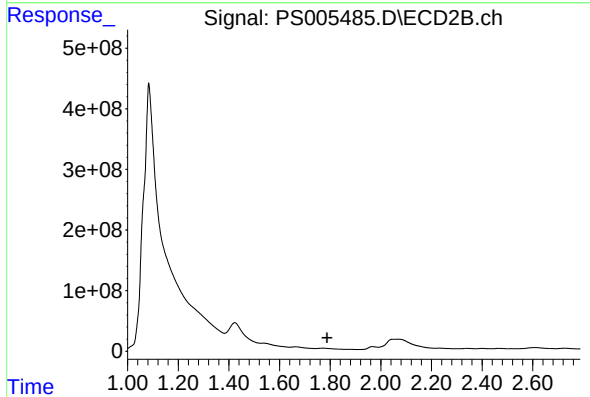


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

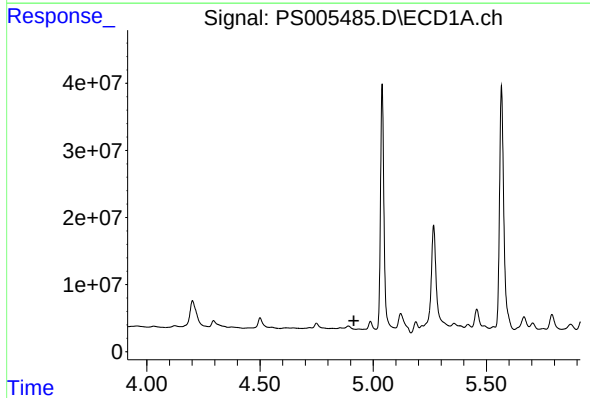


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

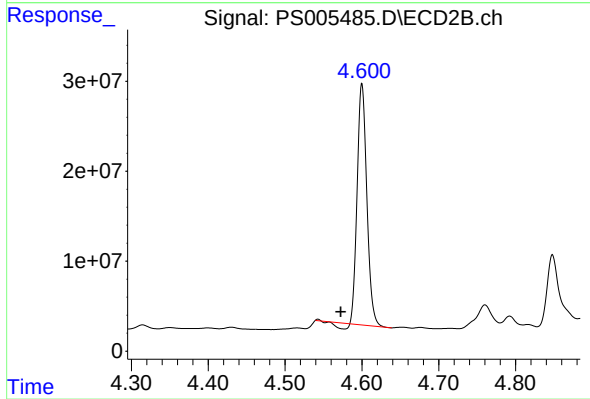

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.028 min
Response: 230341802
Conc: 174.67 ng/ml

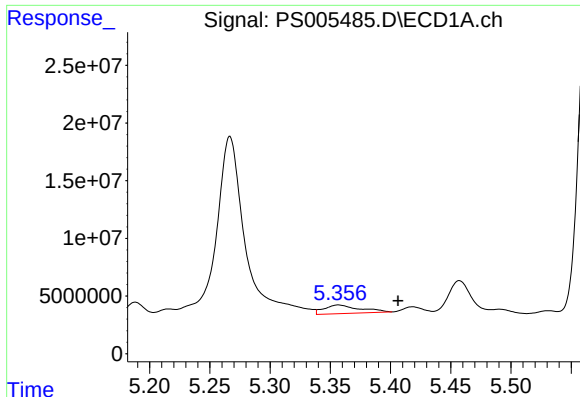

#3 4-Nitrophenol


R.T.: 5.357 min
Delta R.T.: -0.049 min
Response: 15625601
Conc: 21.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-071119

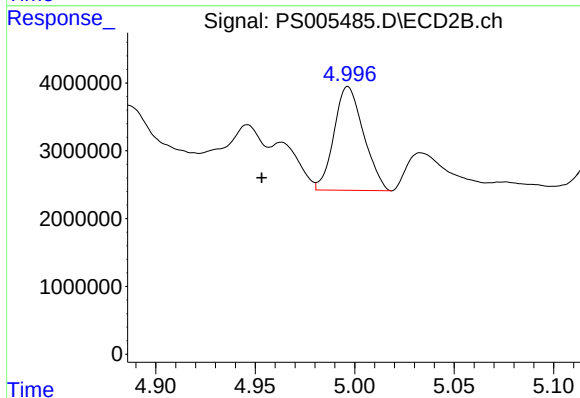


#3 4-Nitrophenol

R.T.: 4.997 min
Delta R.T.: 0.044 min
Response: 15808403
Conc: 31.53 ng/ml

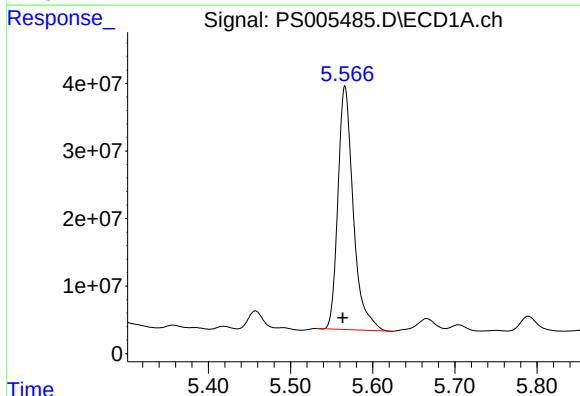


#4 2,4-DCAA

R.T.: 5.566 min
Delta R.T.: 0.003 min
Response: 467177441
Conc: 318.26 ng/ml

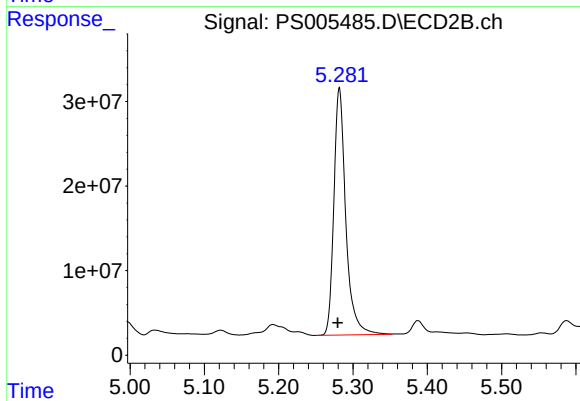

#4 2,4-DCAA


R.T.: 5.282 min
Delta R.T.: 0.002 min
Response: 326374009
Conc: 325.60 ng/ml

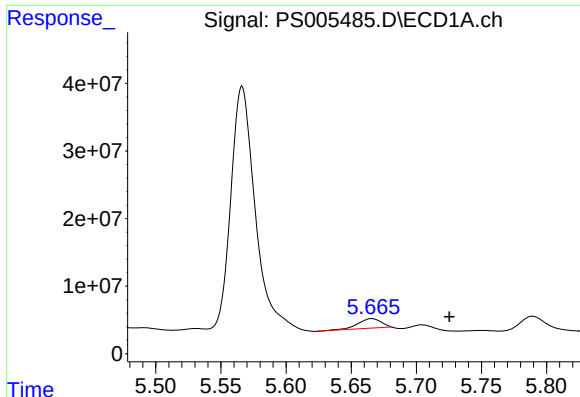

#5 DICAMBA


R.T.: 5.666 min
Delta R.T.: -0.060 min
Response: 17762504
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HD-02-071119

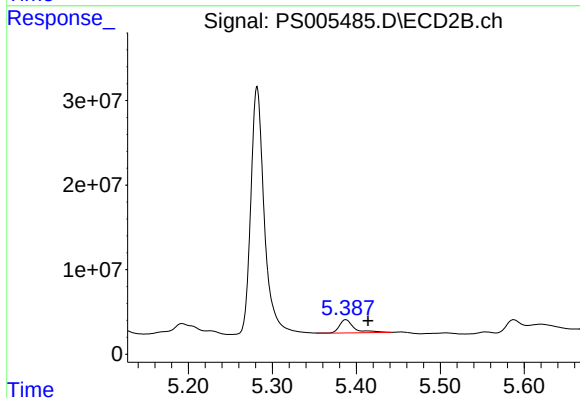


#5 DICAMBA

R.T.: 5.387 min
Delta R.T.: -0.027 min
Response: 19261774
Conc: 5.15 ng/ml

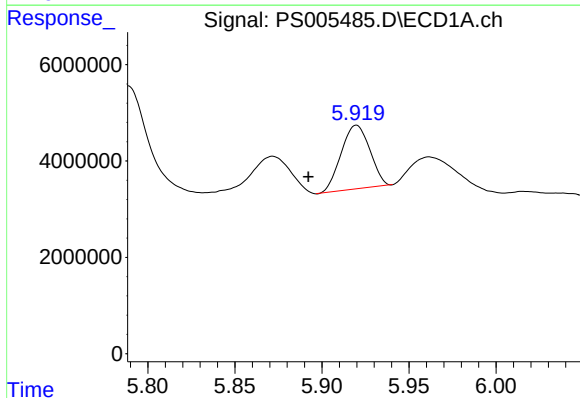


#6 MCP

R.T.: 5.920 min
Delta R.T.: 0.028 min
Response: 15095003
Conc: 3.45 ug/ml

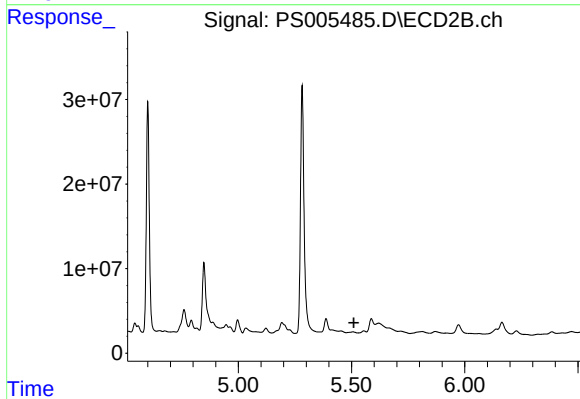

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

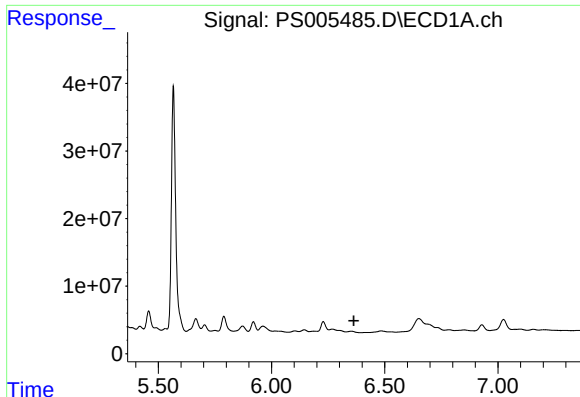

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-071119

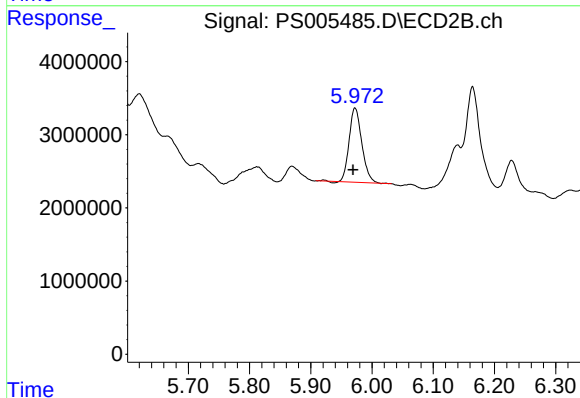


#8 DICHLORPROP

R.T.: 5.972 min
Delta R.T.: 0.003 min
Response: 14609341
Conc: 15.13 ng/ml

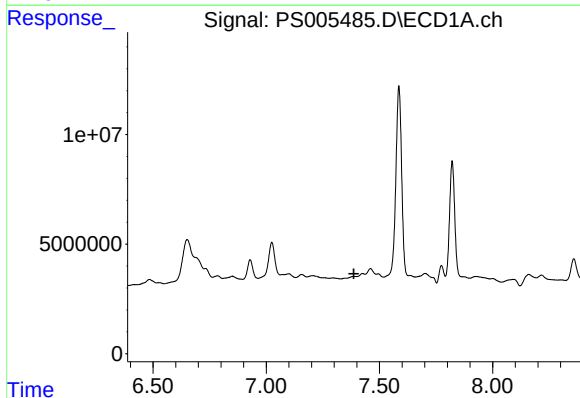


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

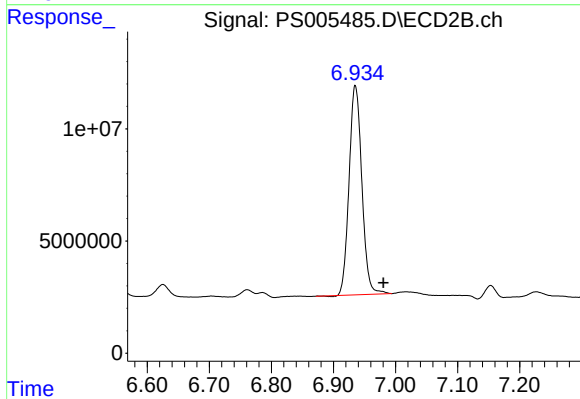

#11 2,4,5-TP (SILVEX)


R.T.: 6.935 min
Delta R.T.: -0.045 min
Response: 133273385
Conc: 25.03 ng/ml

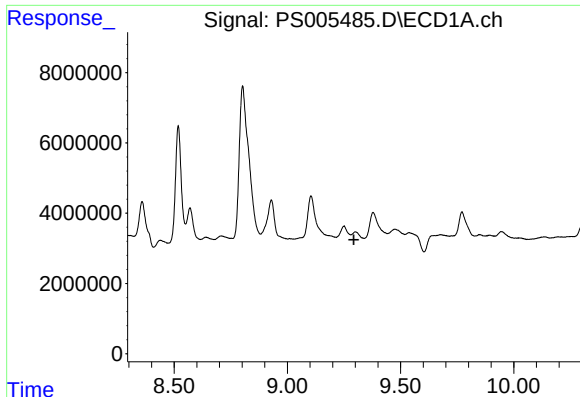

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HD-02-071119

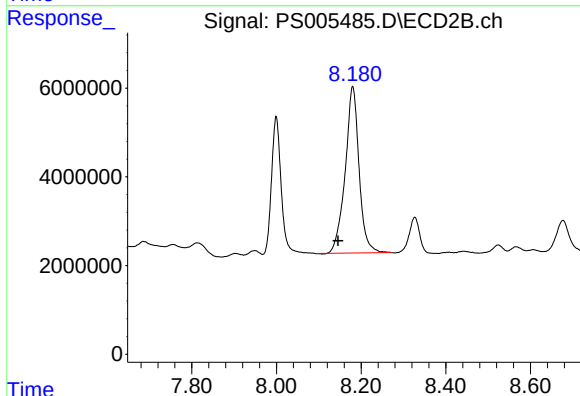


#14 DINOSEB

R.T.: 8.180 min
Delta R.T.: 0.034 min
Response: 85425652
Conc: 21.13 ng/ml

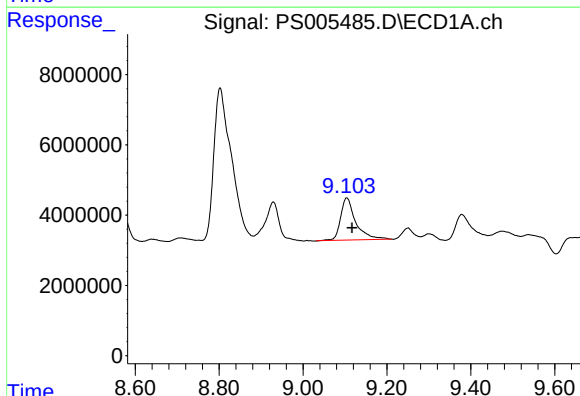

#15 Picloram

R.T.: 9.104 min
Delta R.T.: -0.012 min
Response: 29870291
Conc: 2.60 ng/ml

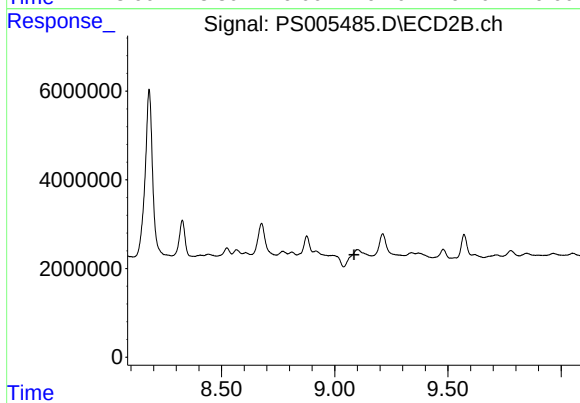

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.085 min
Response: 0
Conc: N.D.