

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 19:34
 Operator : SM\AJ
 Sample : K3626-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-04-071119-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:18:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.585	5.285	467.9E6	318.1E6	318.779	317.376
Target Compounds							
1) T	Dalapon	2.094	0.000	53081563	0	28.797	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	213.4E6	N.D.	161.801
3) T	4-Nitroph...	5.375	5.000	5748986	13950637	7.937	27.821 #
5) T	DICAMBA	0.000	5.390	0	16577098	N.D.	4.428
6) T	MCP	5.938	0.000	15980531	0	3.651	N.D. #
11) T	2,4,5-TP ...	0.000	6.938	0	116.8E6	N.D.	21.926
12) T	2,4,5-T	7.604	0.000	134.5E6	0	16.718	N.D. #
14) T	DINOSEB	0.000	8.182	0	68347036	N.D.	16.904
15) T	Picloram	9.124	0.000	20280759	0	1.765	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 19:34
Operator : SM\AJ
Sample : K3626-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:18:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

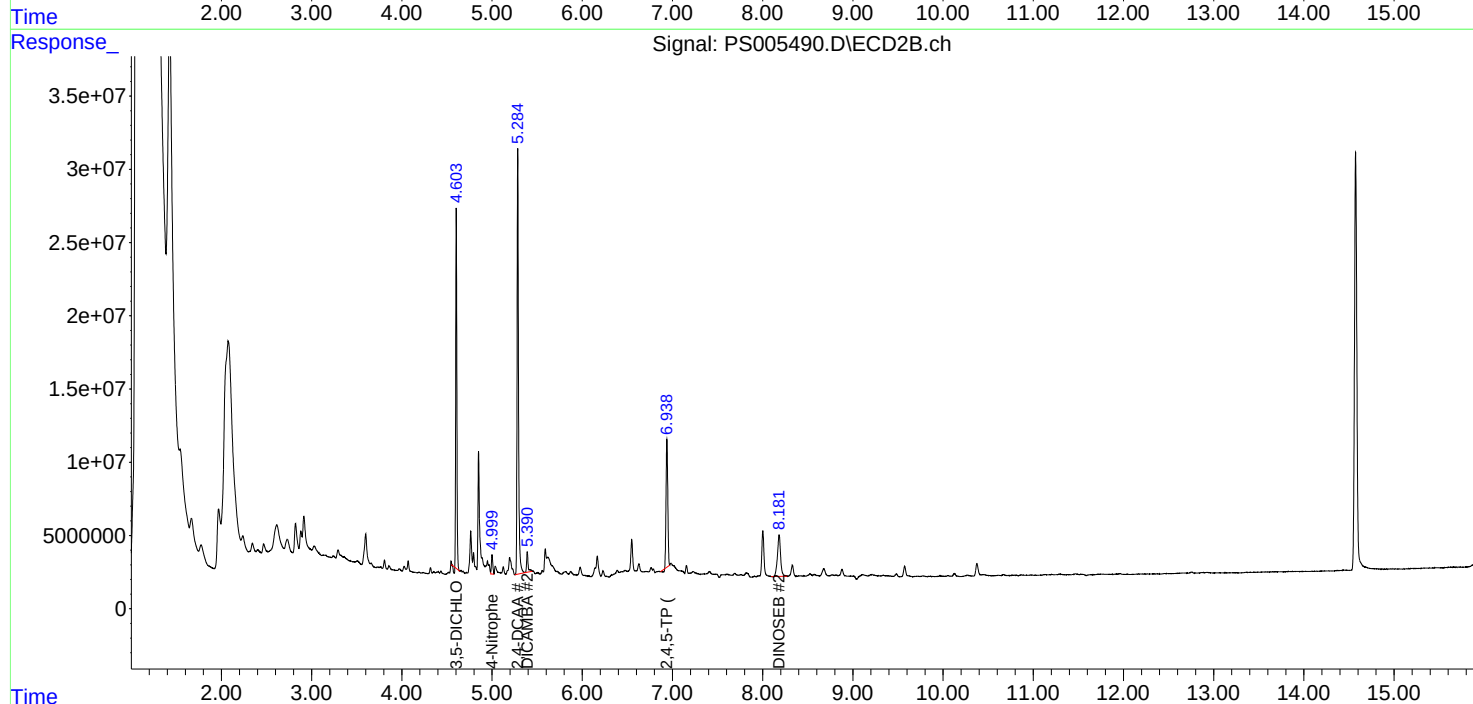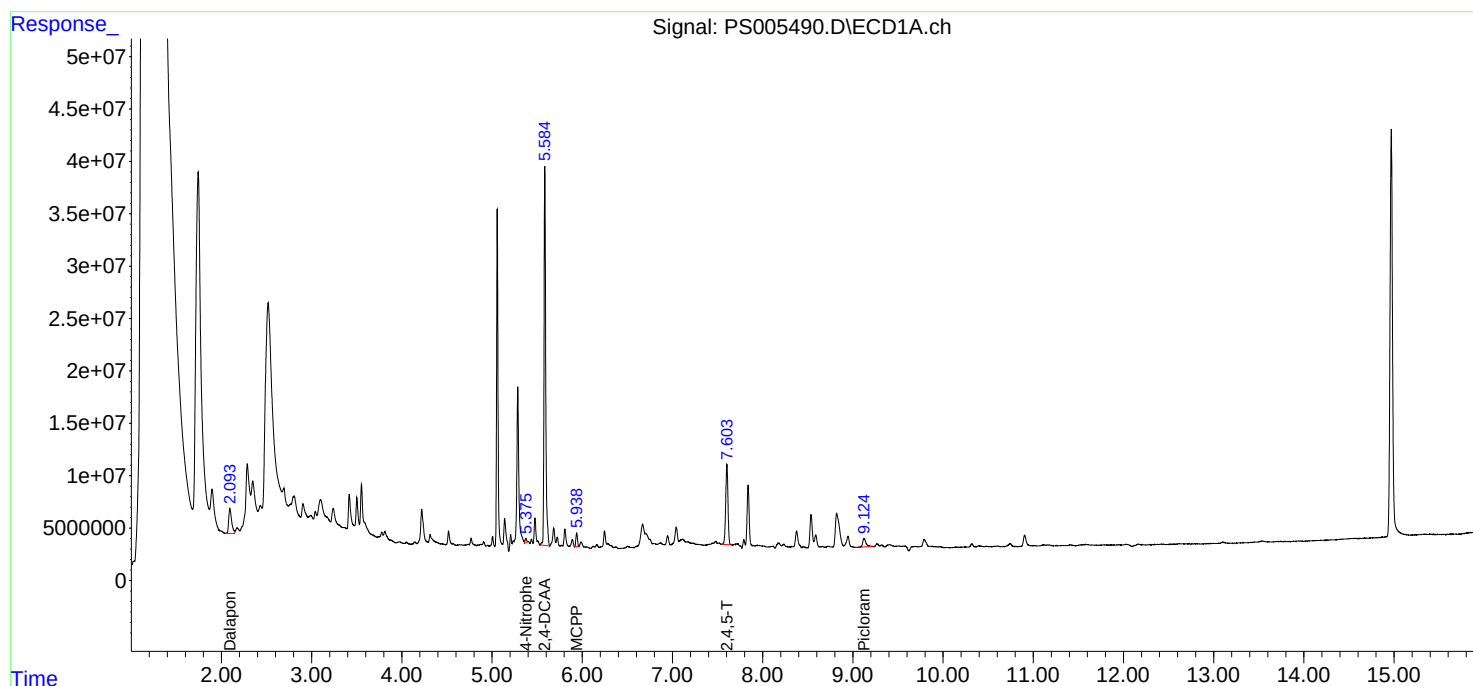


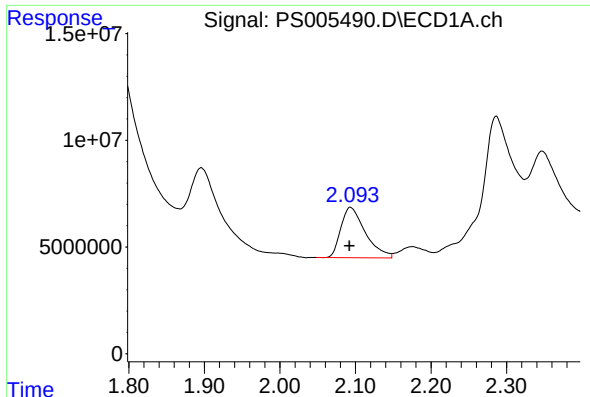

#1 Dalapon


R.T.: 2.094 min
Delta R.T.: 0.002 min
Response: 53081563
Conc: 28.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

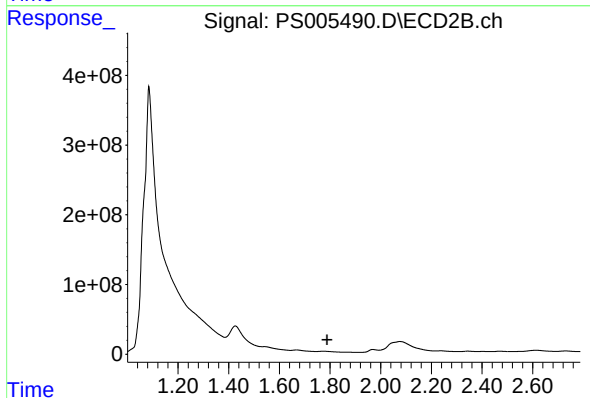


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

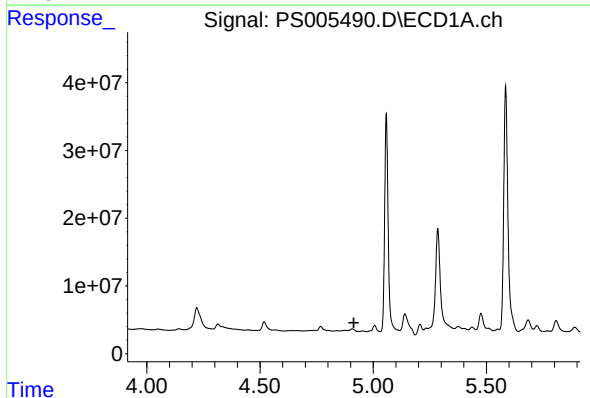


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

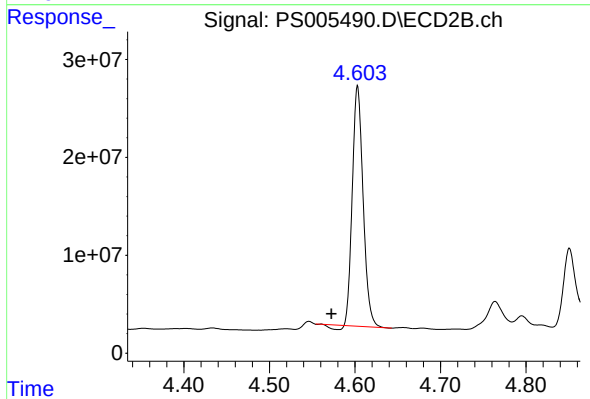

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.031 min
Response: 213369131
Conc: 161.80 ng/ml

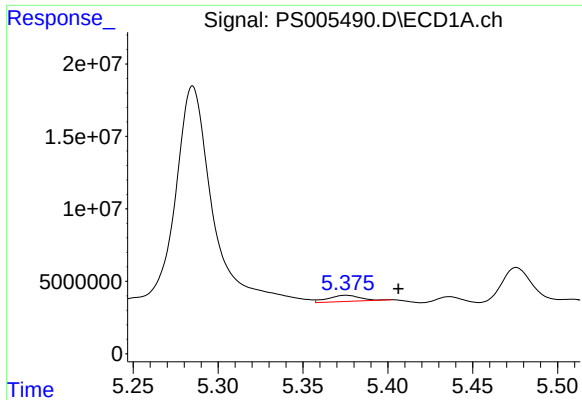

#3 4-Nitrophenol


R.T.: 5.375 min
Delta R.T.: -0.031 min
Response: 5748986
Conc: 7.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

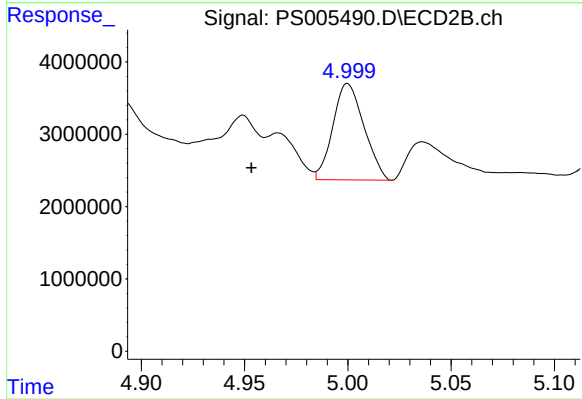


#3 4-Nitrophenol

R.T.: 5.000 min
Delta R.T.: 0.047 min
Response: 13950637
Conc: 27.82 ng/ml

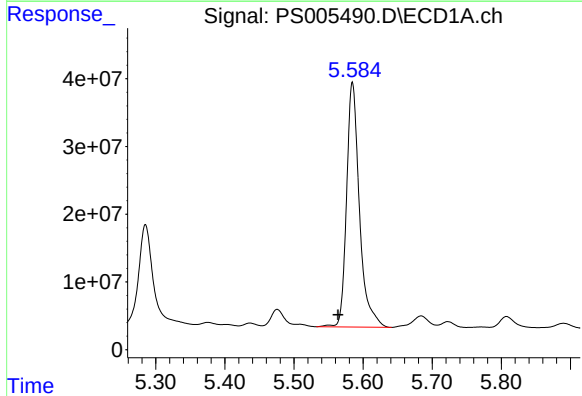


#4 2,4-DCAA

R.T.: 5.585 min
Delta R.T.: 0.021 min
Response: 467933027
Conc: 318.78 ng/ml

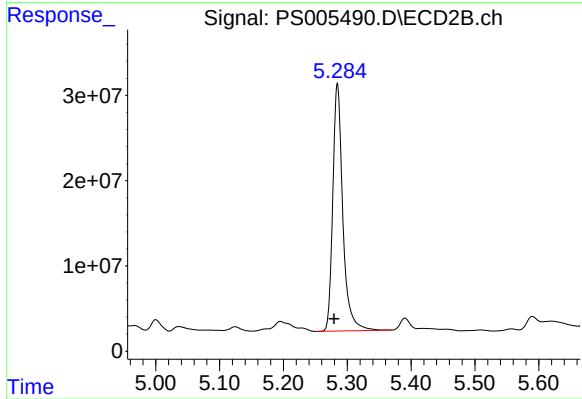

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 318127571
Conc: 317.38 ng/ml

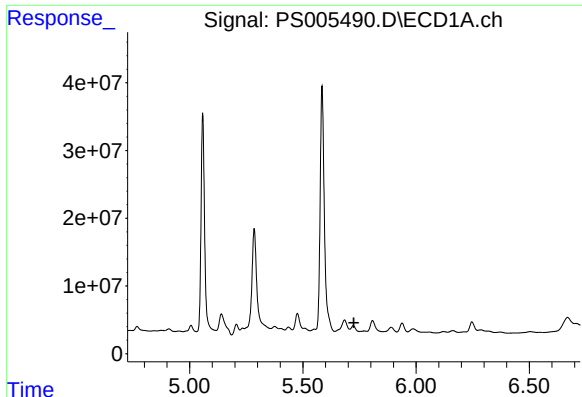

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

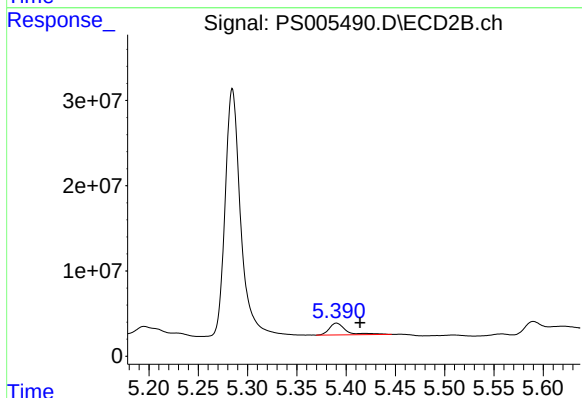


#5 DICAMBA

R.T.: 5.390 min
Delta R.T.: -0.024 min
Response: 16577098
Conc: 4.43 ng/ml

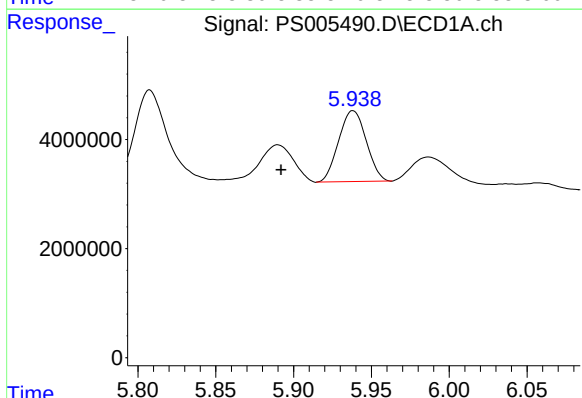


#6 MCP

R.T.: 5.938 min
Delta R.T.: 0.046 min
Response: 15980531
Conc: 3.65 ug/ml

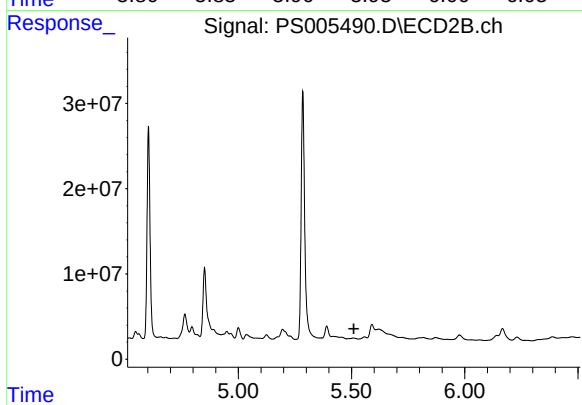

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

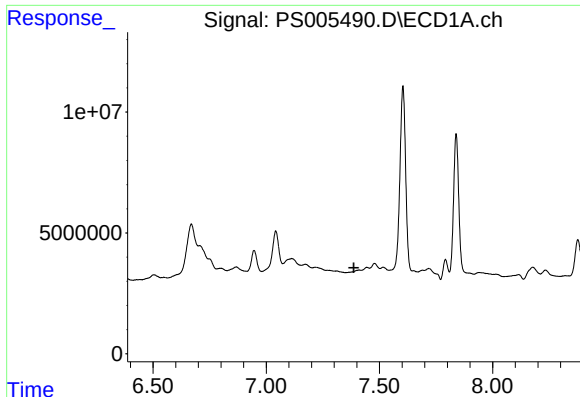

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

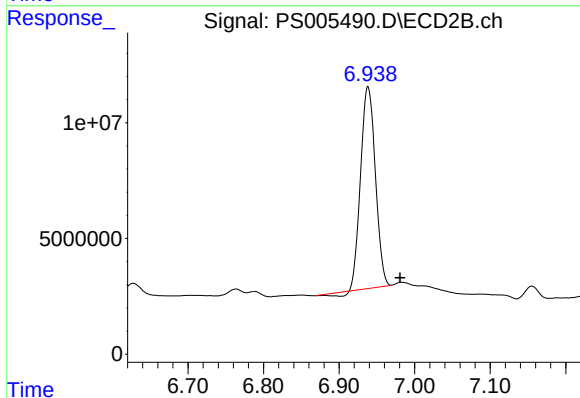


#11 2,4,5-TP (SILVEX)

R.T.: 6.938 min
Delta R.T.: -0.042 min
Response: 116764195
Conc: 21.93 ng/ml

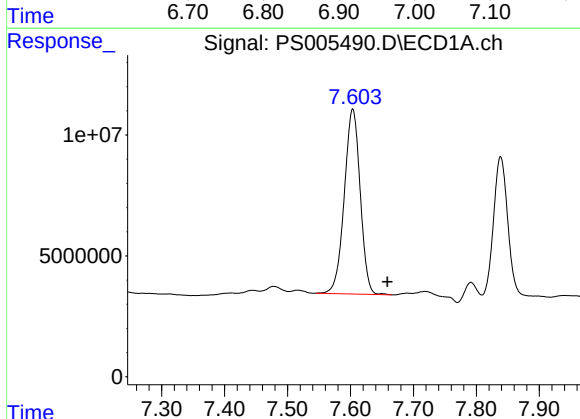


#12 2,4,5-T

R.T.: 7.604 min
Delta R.T.: -0.055 min
Response: 134545457
Conc: 16.72 ng/ml

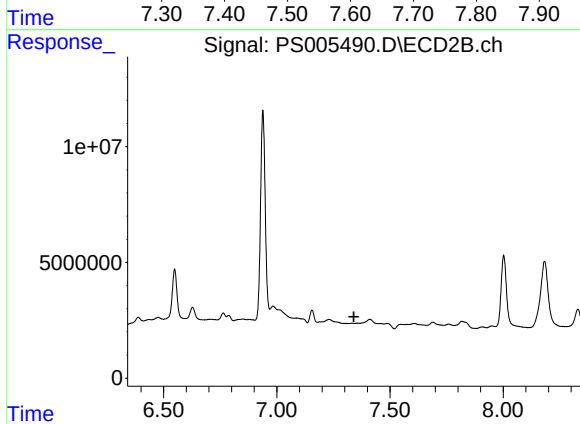

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.

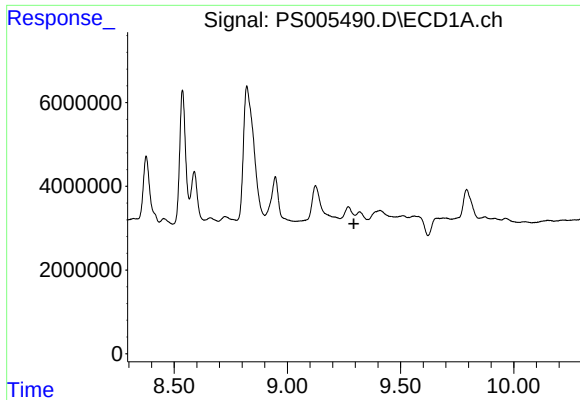

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-04-071119-A

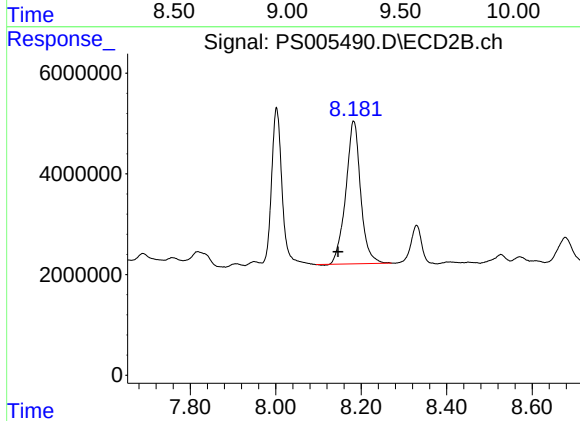


#14 DINOSEB

R.T.: 8.182 min
Delta R.T.: 0.036 min
Response: 68347036
Conc: 16.90 ng/ml

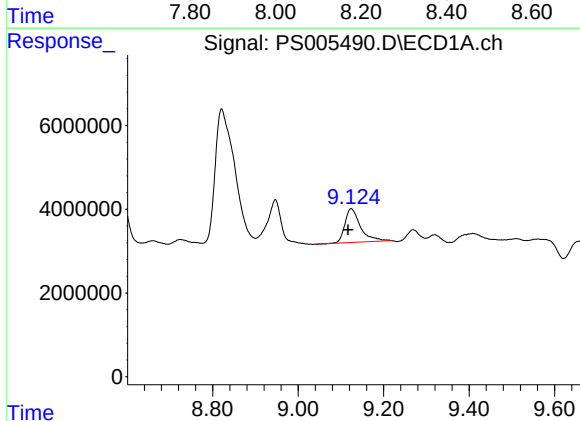

#15 Picloram

R.T.: 9.124 min
Delta R.T.: 0.008 min
Response: 20280759
Conc: 1.76 ng/ml

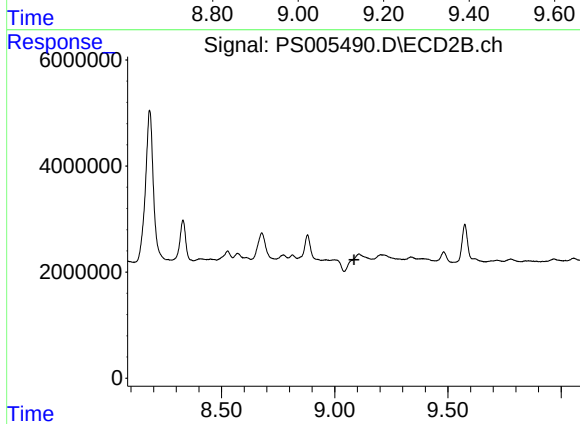

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.085 min
Response: 0
Conc: N.D.