

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 21:03
 Operator : SM\AJ
 Sample : K3740-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-22

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:19:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.565	5.281	539.6E6	366.3E6	367.619	365.419
Target Compounds							
1) T	Dalapon	2.074	0.000	56455383	0	30.627	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	114.9E6	N.D.	87.153
3) T	4-Nitroph...	5.355	0.000	3199186	0	4.417	N.D. #
5) T	DICAMBA	5.664	0.000	21922504	0	3.843	N.D. #
8) T	DICHLORPROP	0.000	5.972	0	13030172	N.D.	13.495
10) T	Pentachlo...	6.851	6.620	27789327	23826045	1.412	1.853 #
11) T	2,4,5-TP ...	0.000	6.933	0	29801379	N.D.	5.596
12) T	2,4,5-T	0.000	7.387	0	47665463	N.D.	9.345
15) T	Picloram	9.136	9.094	246.9E6	169.6E6	21.490	22.472
16) T	DCPA	0.000	9.094	0	169.6E6	N.D.	24.912



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 21:03
Operator : SM\AJ
Sample : K3740-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
COMP-22

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:19:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

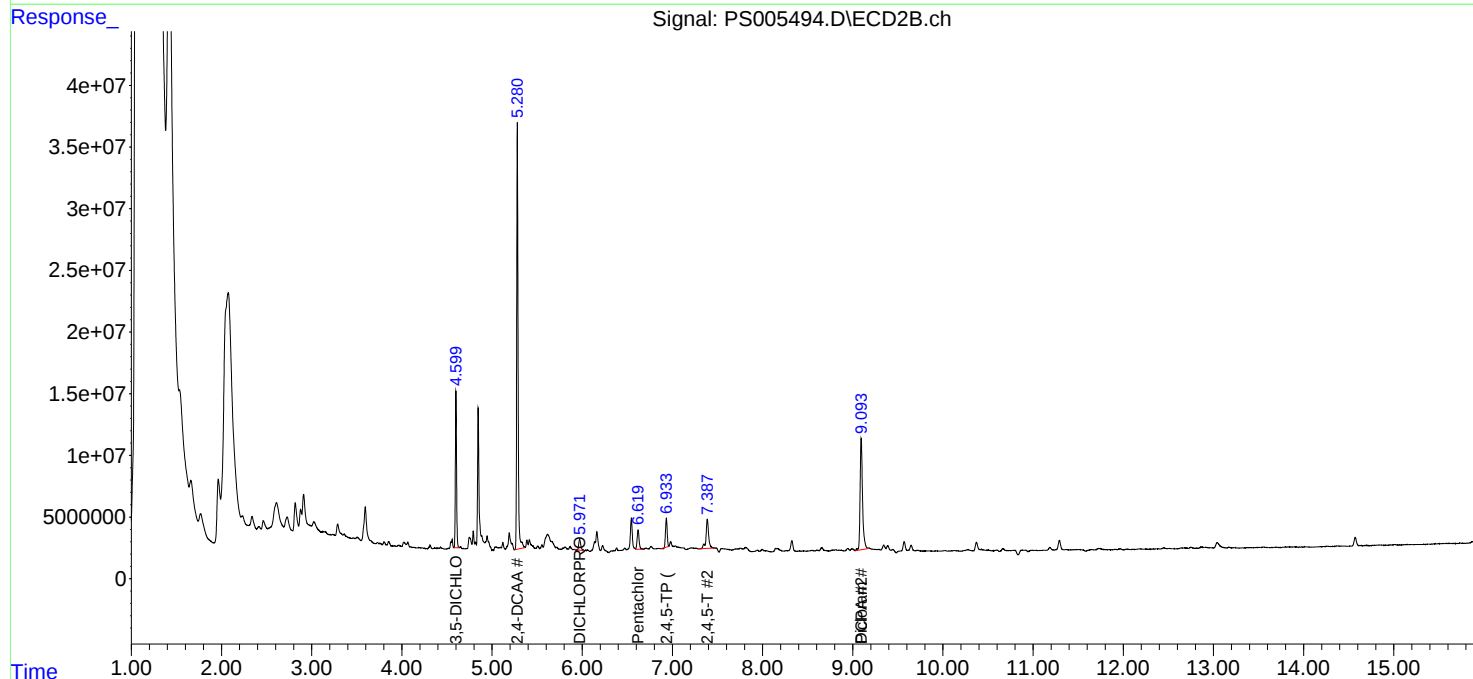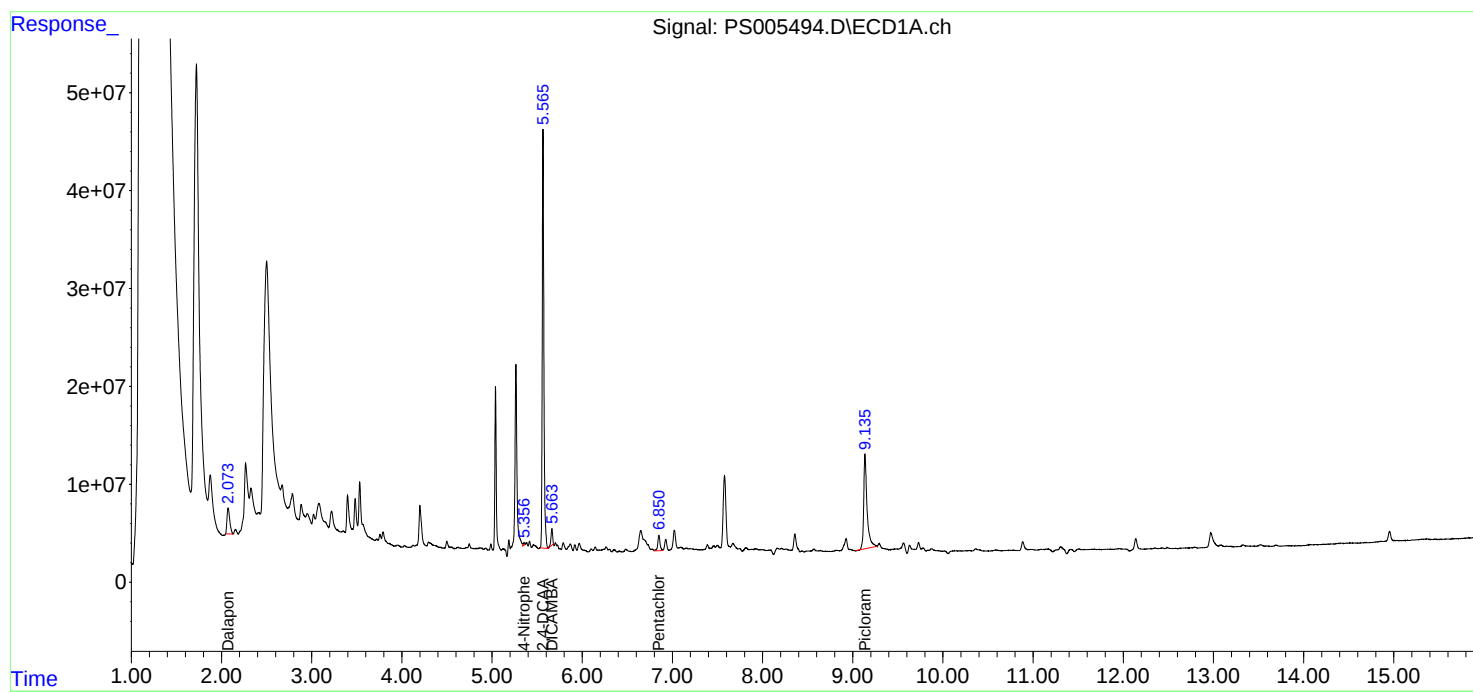


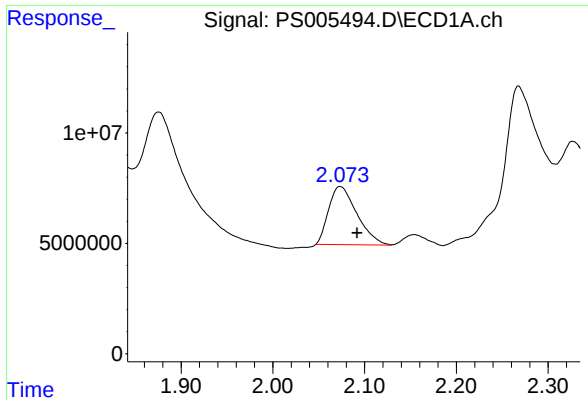

#1 Dalapon


R.T.: 2.074 min
Delta R.T.: -0.018 min
Response: 56455383
Conc: 30.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-22

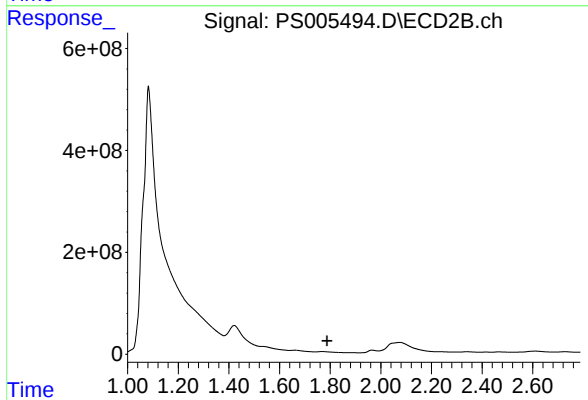


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

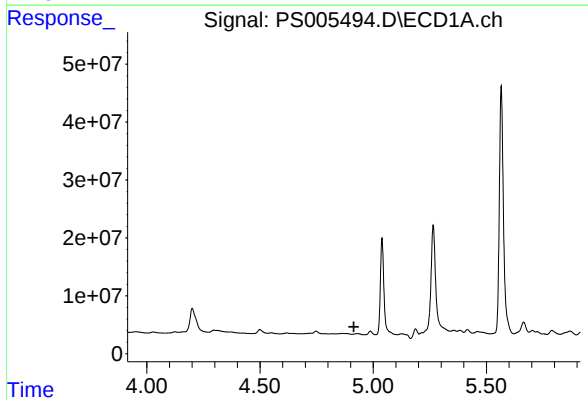


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

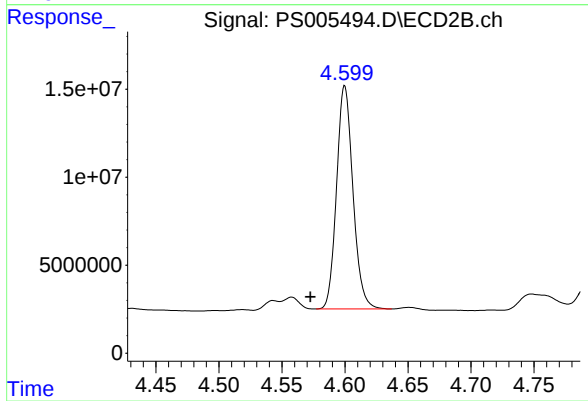

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.027 min
Response: 114929539
Conc: 87.15 ng/ml

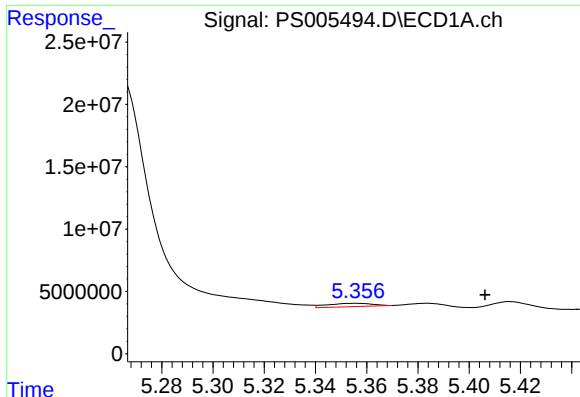

#3 4-Nitrophenol


R.T.: 5.355 min
Delta R.T.: -0.051 min
Response: 3199186
Conc: 4.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-22

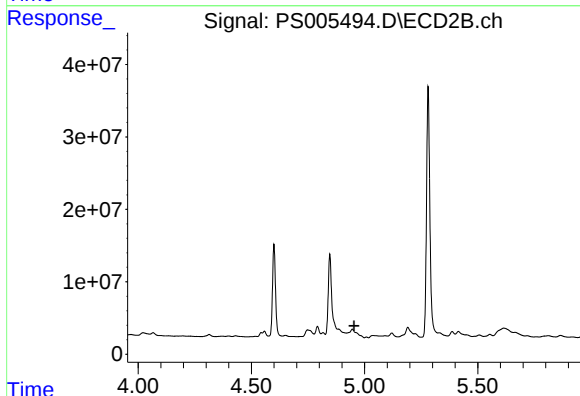


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

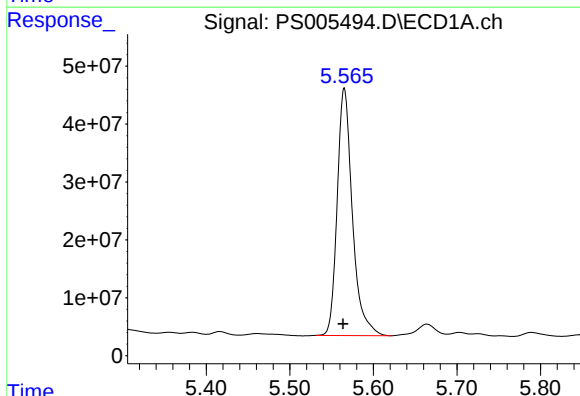


#4 2,4-DCAA

R.T.: 5.565 min
Delta R.T.: 0.002 min
Response: 539624710
Conc: 367.62 ng/ml

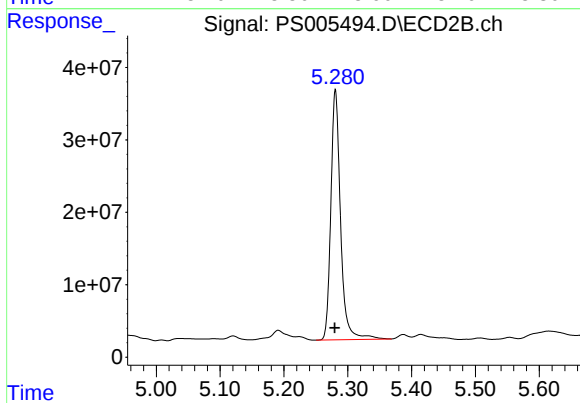

#4 2,4-DCAA


R.T.: 5.281 min
Delta R.T.: 0.001 min
Response: 366284116
Conc: 365.42 ng/ml

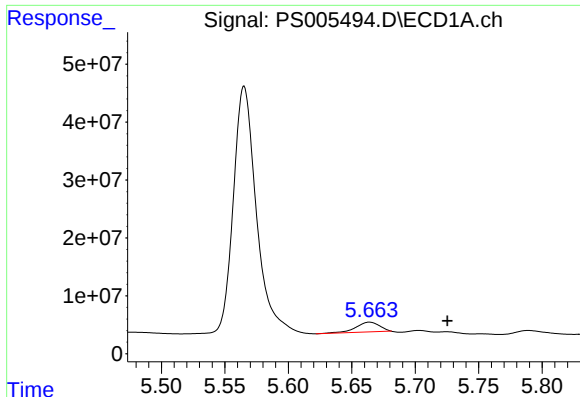

#5 DICAMBA


R.T.: 5.664 min
Delta R.T.: -0.061 min
Response: 21922504
Conc: 3.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-22

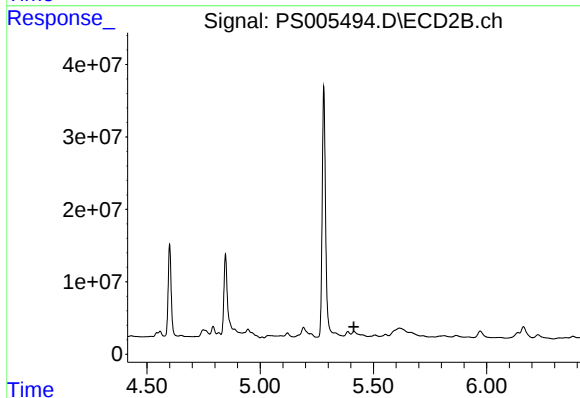


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

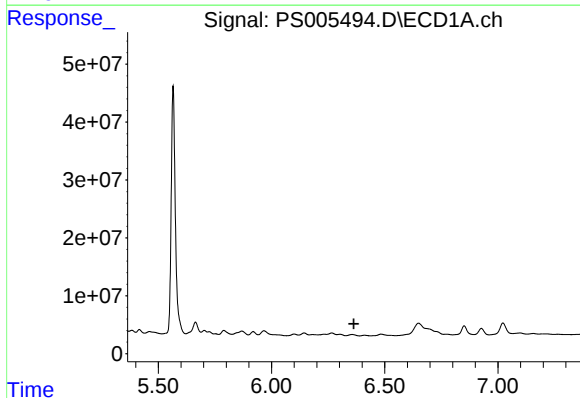


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

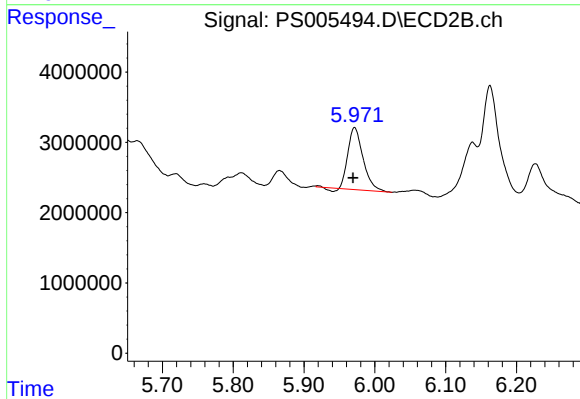

#8 DICHLORPROP


R.T.: 5.972 min
Delta R.T.: 0.002 min
Response: 13030172
Conc: 13.50 ng/ml

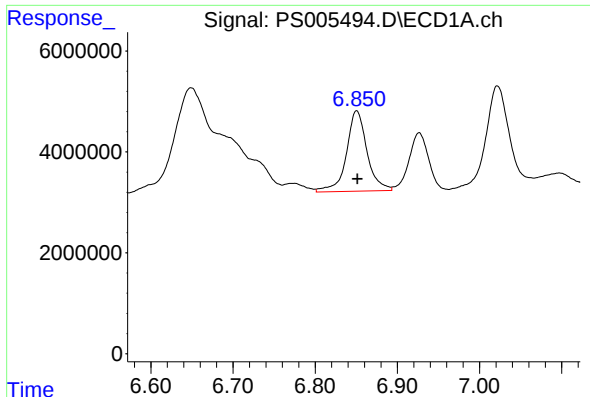

#10 Pentachlorophenol


R.T.: 6.851 min
Delta R.T.: -0.001 min
Response: 27789327
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-22

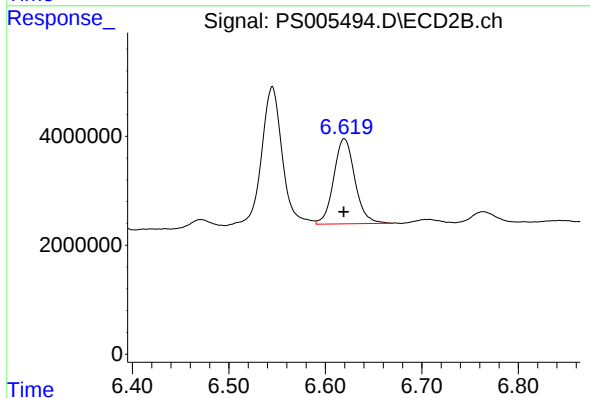


#10 Pentachlorophenol

R.T.: 6.620 min
Delta R.T.: 0.000 min
Response: 23826045
Conc: 1.85 ng/ml

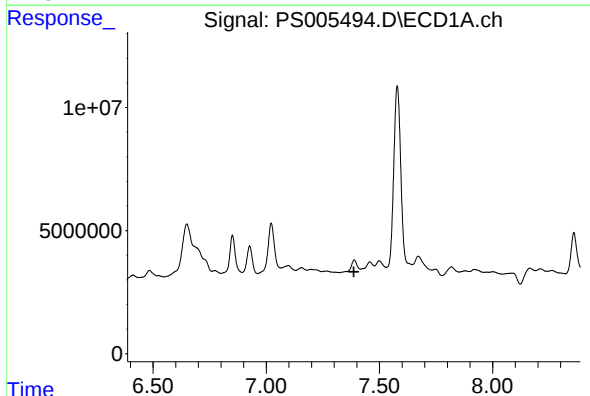


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

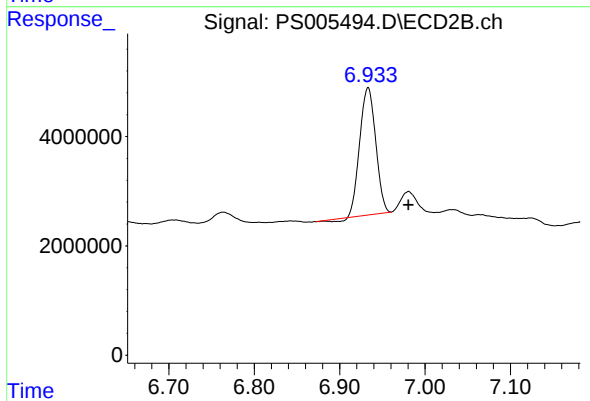

#11 2,4,5-TP (SILVEX)


R.T.: 6.933 min
Delta R.T.: -0.047 min
Response: 29801379
Conc: 5.60 ng/ml

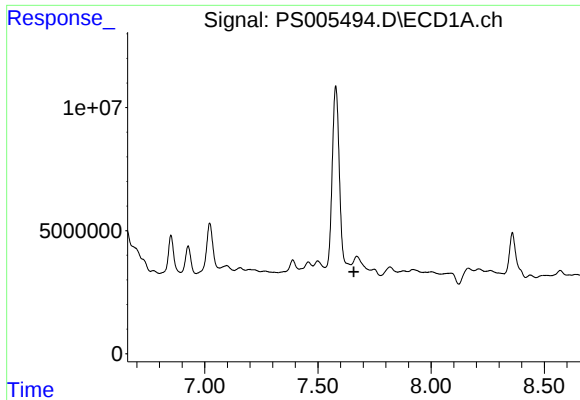

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.659 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-22

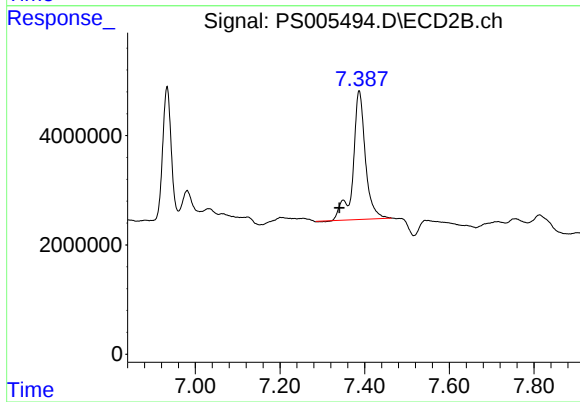


#12 2,4,5-T

R.T.: 7.387 min
Delta R.T.: 0.047 min
Response: 47665463
Conc: 9.34 ng/ml

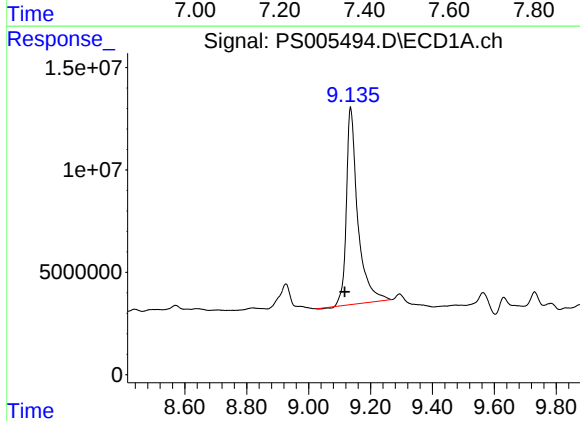


#15 Picloram

R.T.: 9.136 min
Delta R.T.: 0.019 min
Response: 246949734
Conc: 21.49 ng/ml

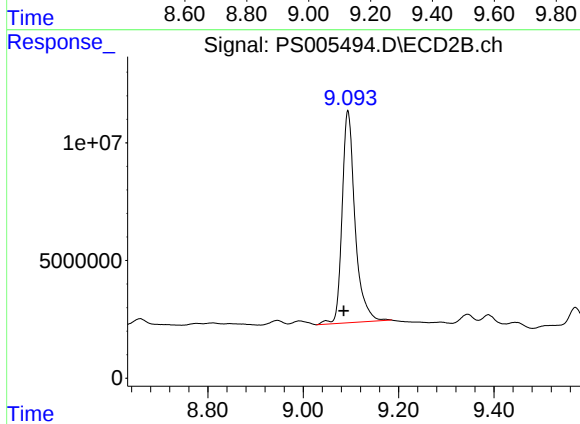

#15 Picloram


R.T.: 9.094 min
Delta R.T.: 0.009 min
Response: 169586222
Conc: 22.47 ng/ml

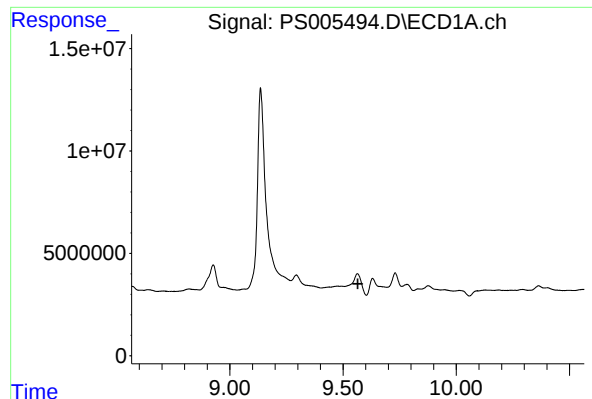

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-22

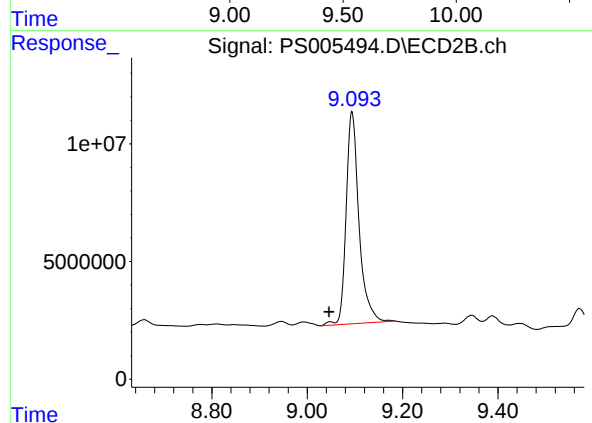

#16 DCPA

R.T.: 9.094 min
Delta R.T.: 0.048 min
Response: 169586222
Conc: 24.91 ng/ml