

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 21:25
 Operator : SM\AJ
 Sample : K3740-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:20:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.569	5.285	417.7E6	281.2E6	284.551	280.514
Target Compounds							
1) T	Dalapon	2.077	0.000	58858452	0	31.931	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	95322223	N.D.	72.284
3) T	4-Nitroph...	5.358	0.000	3103903	0	4.285	N.D. #
5) T	DICAMBA	5.668	0.000	18118041	0	3.176	N.D. #
7) T	MCPA	5.968	0.000	20104399	0	3.201	N.D. #
8) T	DICHLORPROP	0.000	5.976	0	15338832	N.D.	15.886
10) T	Pentachlo...	6.854	6.624	15813746	15328909	<MDL	1.192 #
11) T	2,4,5-TP ...	0.000	6.936	0	27631400	N.D.	5.189
16) T	DCPA	9.633	0.000	30984584	0	3.106	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 21:25
Operator : SM\AJ
Sample : K3740-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:20:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

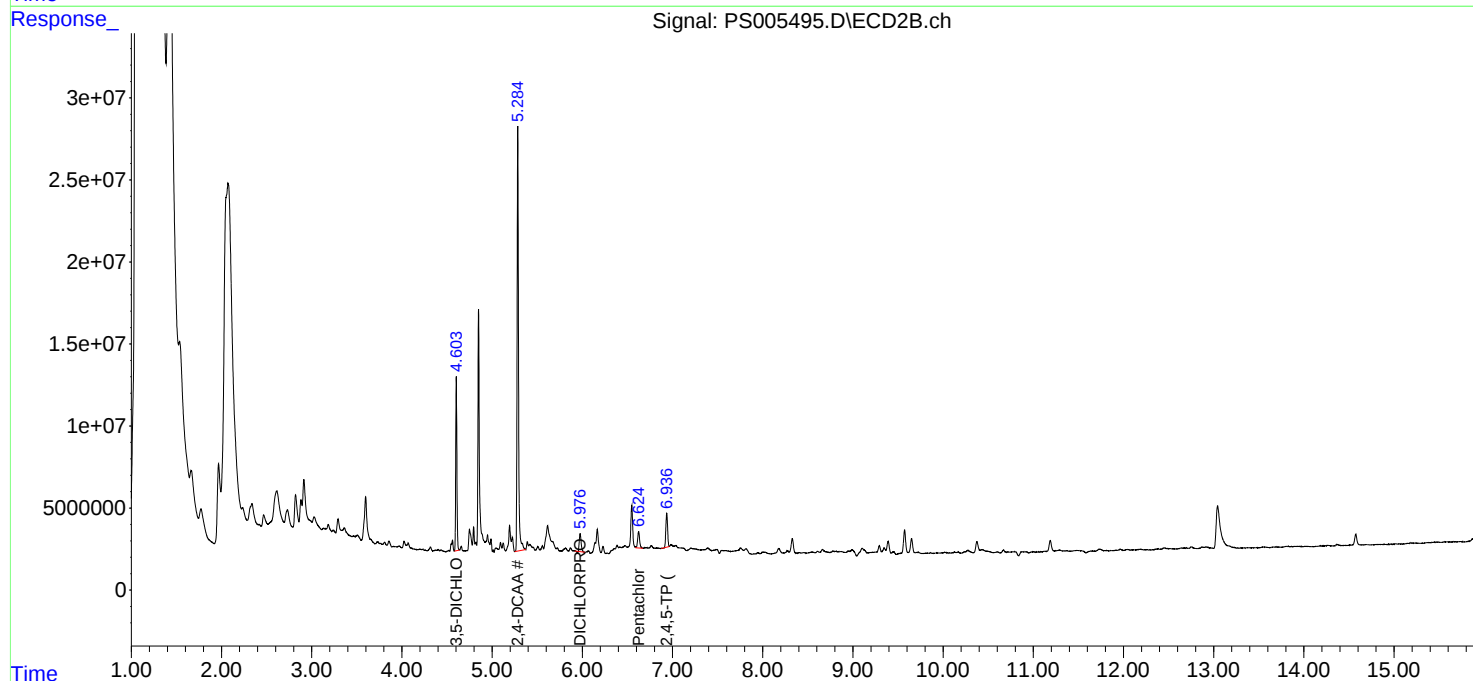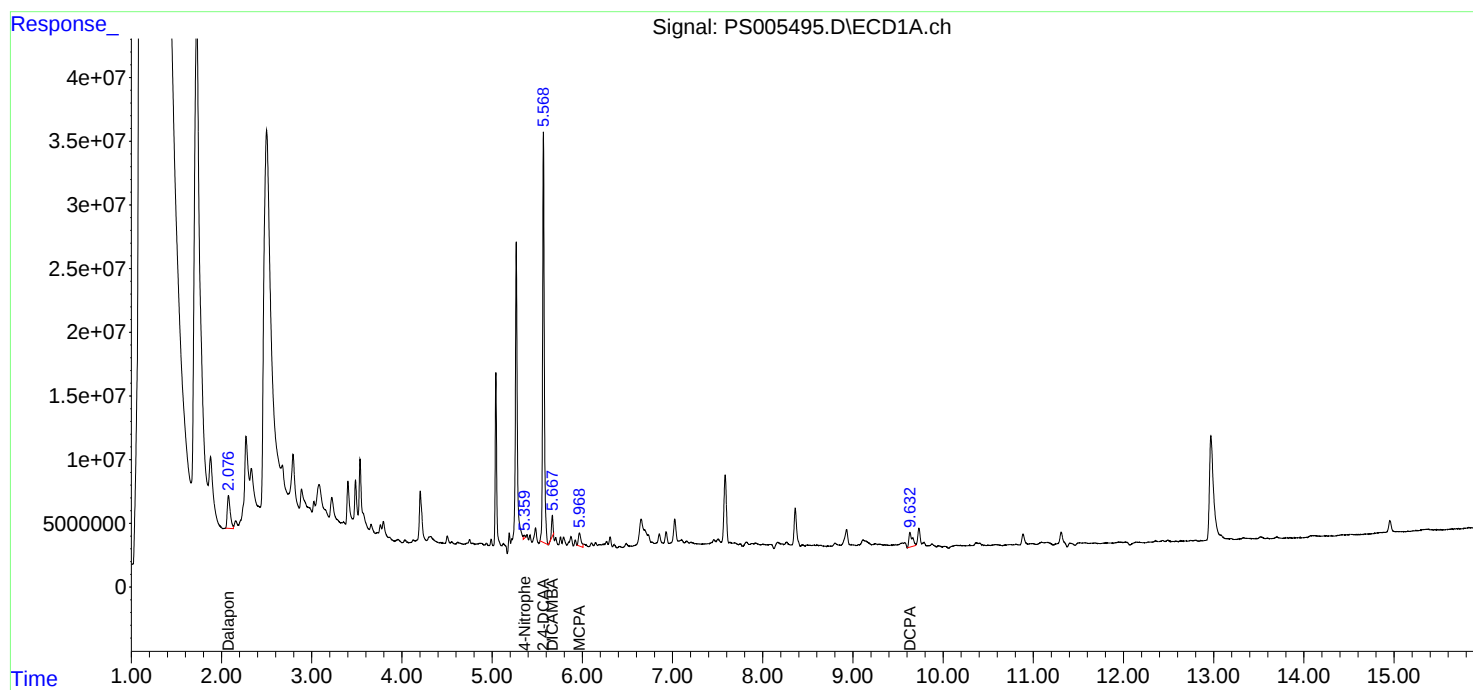


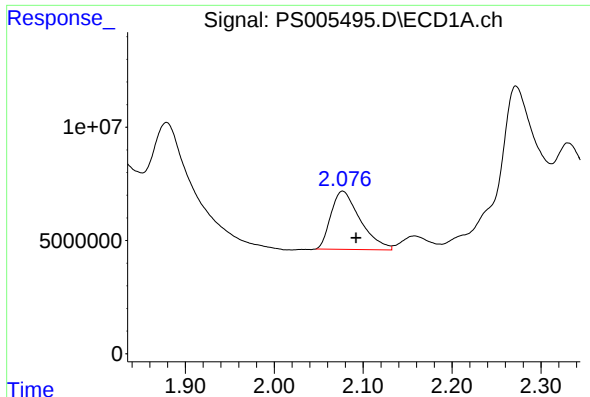

#1 Dalapon


R.T.: 2.077 min
Delta R.T.: -0.015 min
Response: 58858452
Conc: 31.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

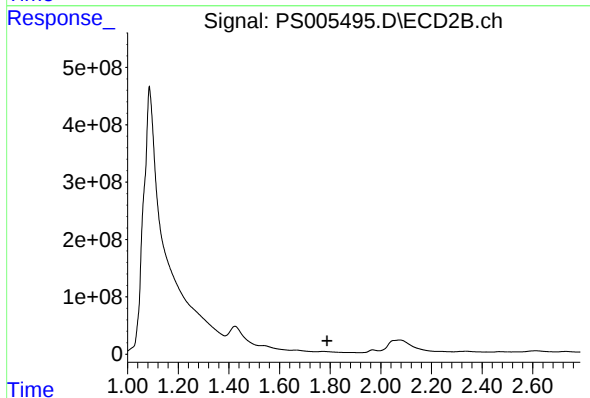


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

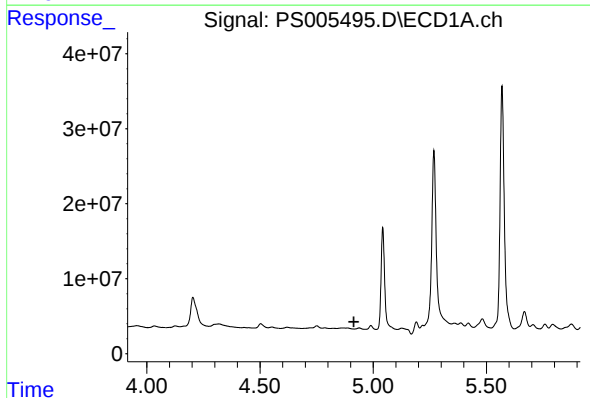


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

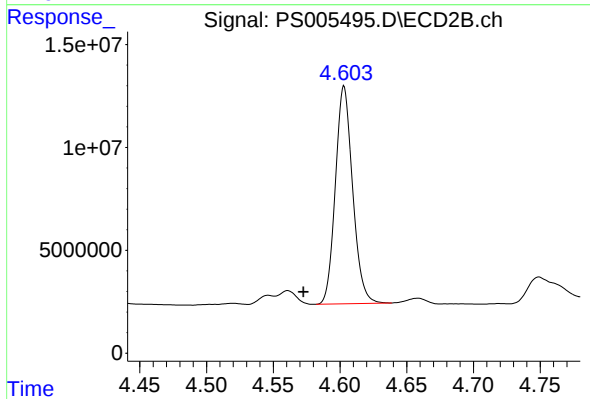

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.031 min
Response: 95322223
Conc: 72.28 ng/ml

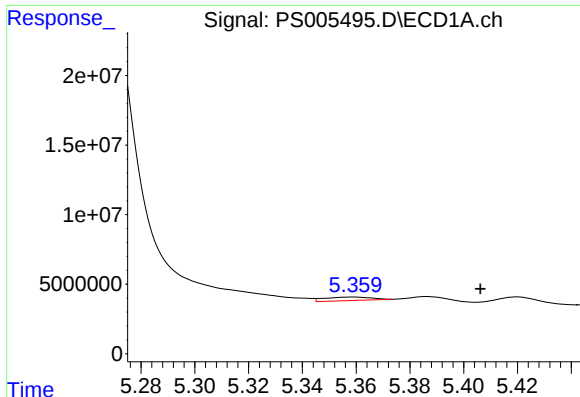

#3 4-Nitrophenol


R.T.: 5.358 min
Delta R.T.: -0.048 min
Response: 3103903
Conc: 4.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

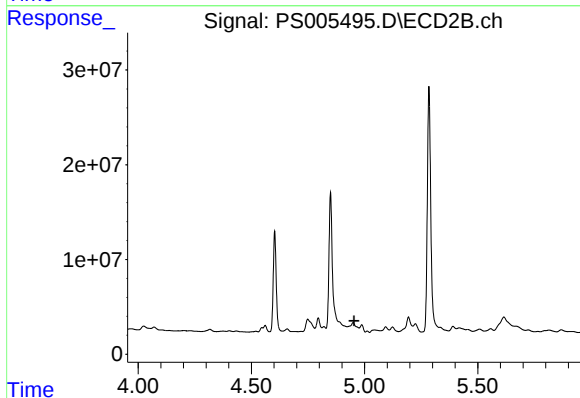


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

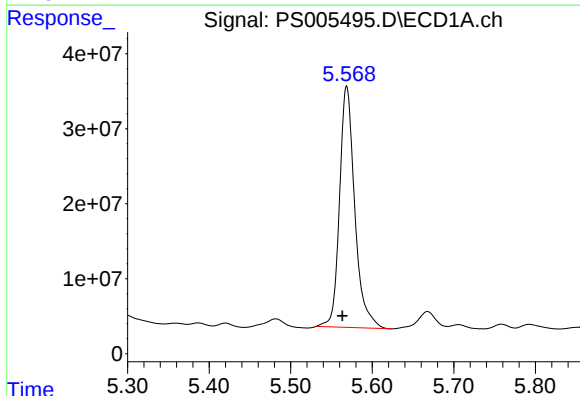


#4 2,4-DCAA

R.T.: 5.569 min
Delta R.T.: 0.005 min
Response: 417690306
Conc: 284.55 ng/ml

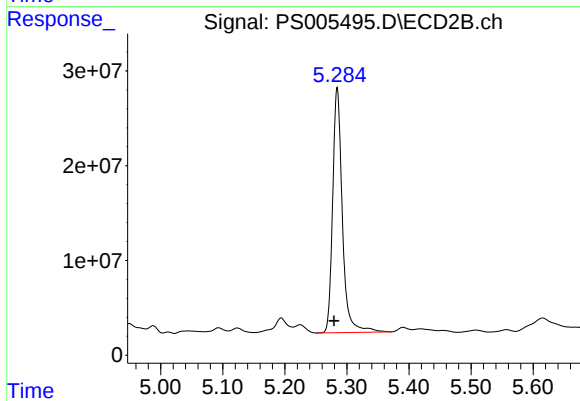

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 281178380
Conc: 280.51 ng/ml

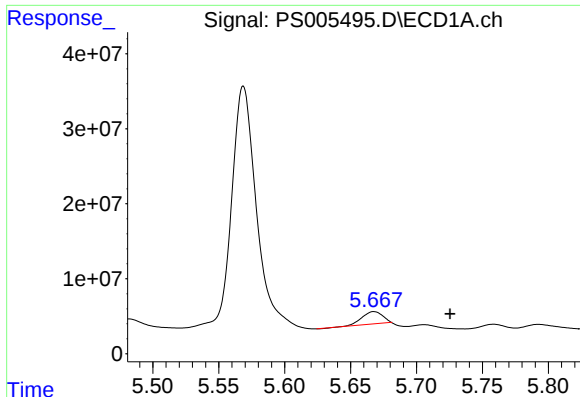

#5 DICAMBA


R.T.: 5.668 min
Delta R.T.: -0.058 min
Response: 18118041
Conc: 3.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-23

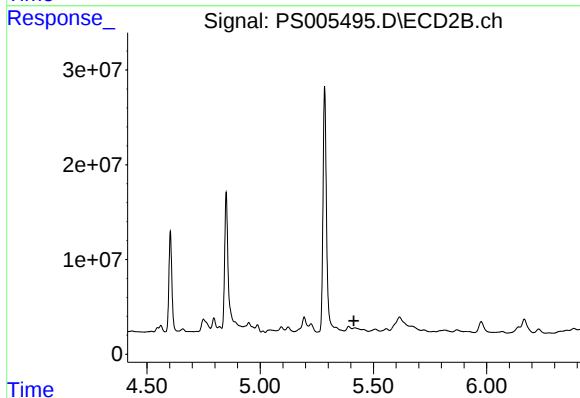


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

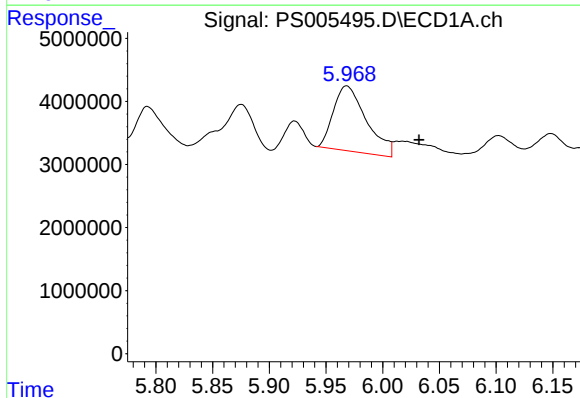


#7 MCPA

R.T.: 5.968 min
Delta R.T.: -0.064 min
Response: 20104399
Conc: 3.20 ug/ml

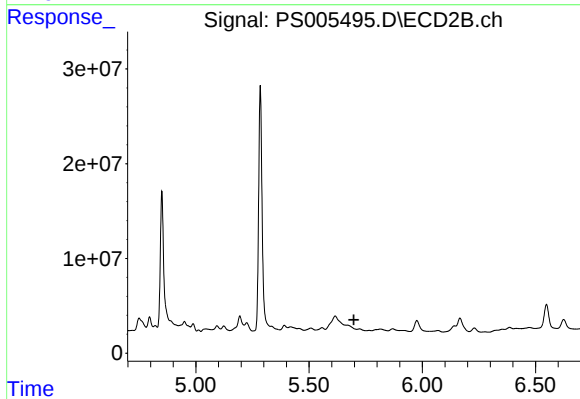

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.698 min
Response: 0
Conc: N.D.

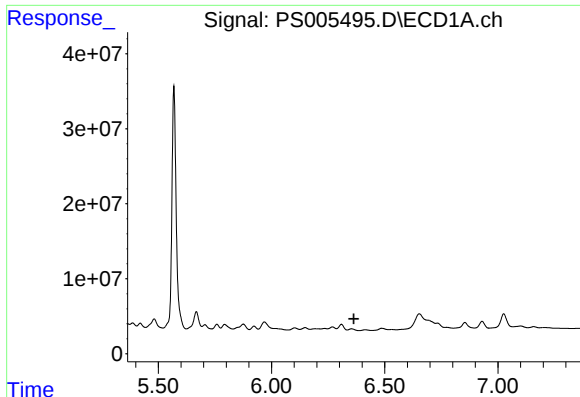

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-23

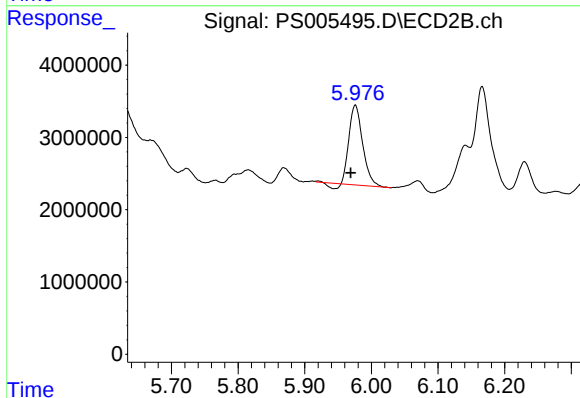


#8 DICHLORPROP

R.T.: 5.976 min
Delta R.T.: 0.007 min
Response: 15338832
Conc: 15.89 ng/ml

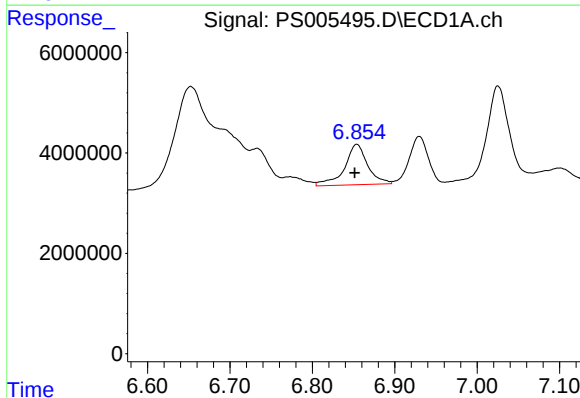


#10 Pentachlorophenol

R.T.: 6.854 min
Delta R.T.: 0.002 min
Response: 15813746
Conc: N.D.

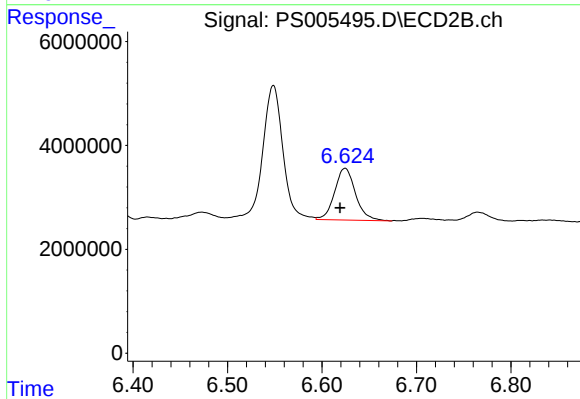

#10 Pentachlorophenol


R.T.: 6.624 min
Delta R.T.: 0.005 min
Response: 15328909
Conc: 1.19 ng/ml

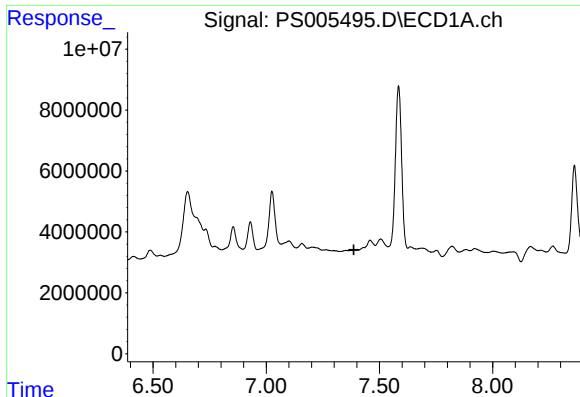

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-23

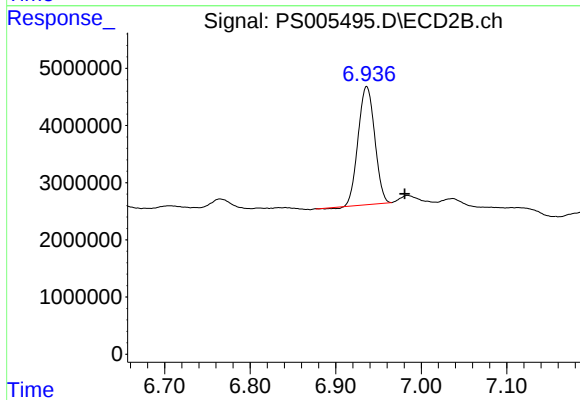


#11 2,4,5-TP (SILVEX)

R.T.: 6.936 min
Delta R.T.: -0.044 min
Response: 27631400
Conc: 5.19 ng/ml

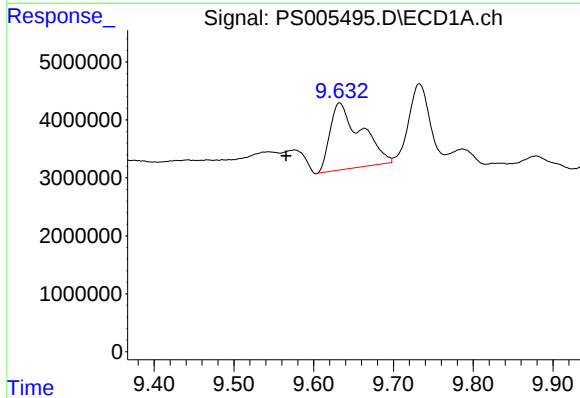

#16 DCPA

R.T.: 9.633 min
Delta R.T.: 0.067 min
Response: 30984584
Conc: 3.11 ng/ml

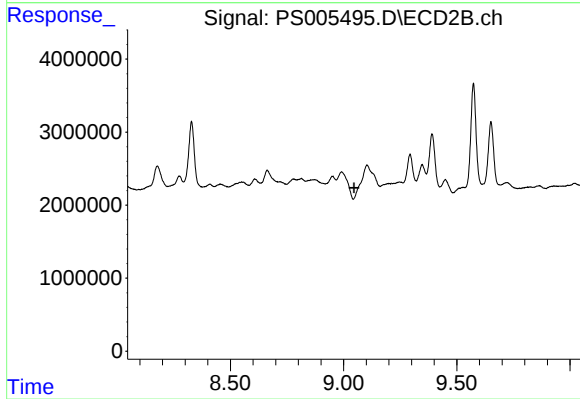

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.046 min
Response: 0
Conc: N.D.