

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
 Data File : PS005489.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 19:12
 Operator : SM\AJ
 Sample : K3621-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-071019-B

Manual Integrations
 APPROVED

Ankita
 7/16/2019 8:42:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:18:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.584	5.300	499.7E6	335.5E6	340.393	334.707m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071219\
Data File : PS005489.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 19:12
Operator : SM\AJ
Sample : K3621-04
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OK-03-071019-B


Manual Integrations
APPROVED

Ankita
7/16/2019 8:42:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:18:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

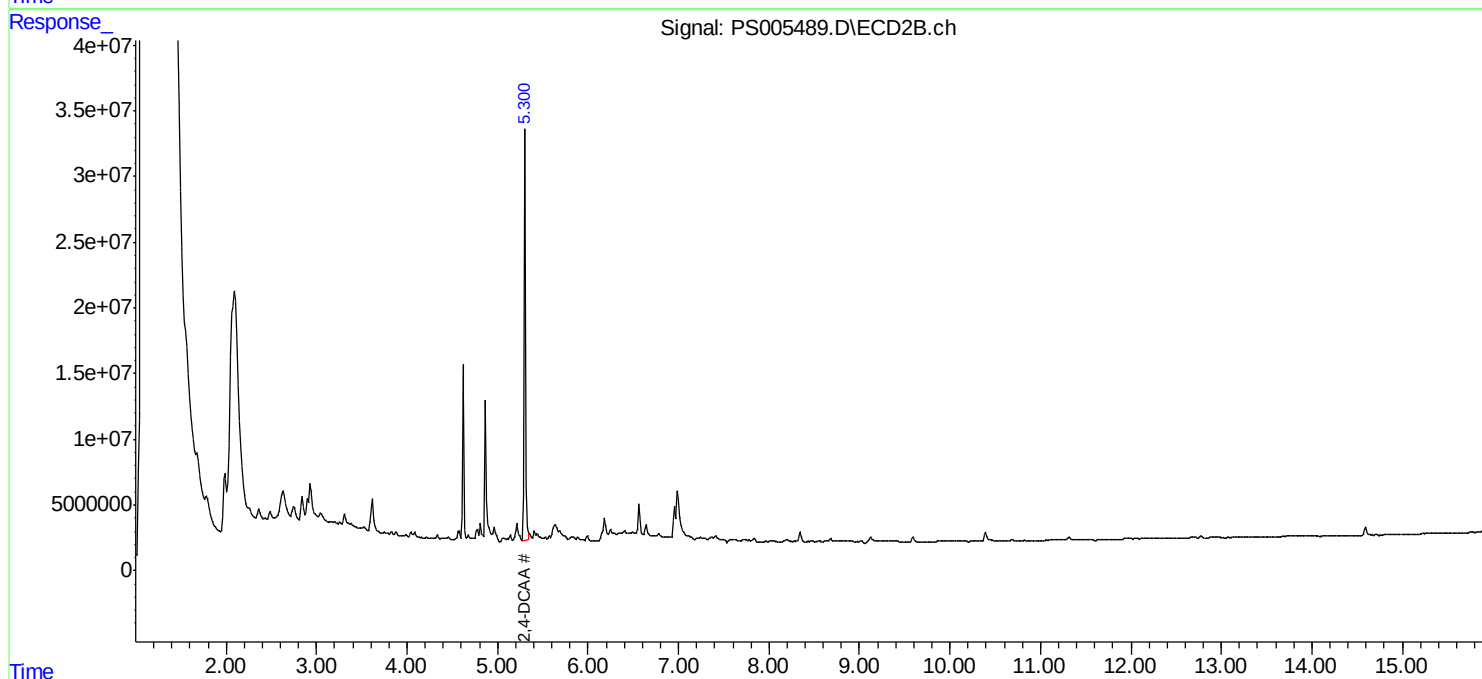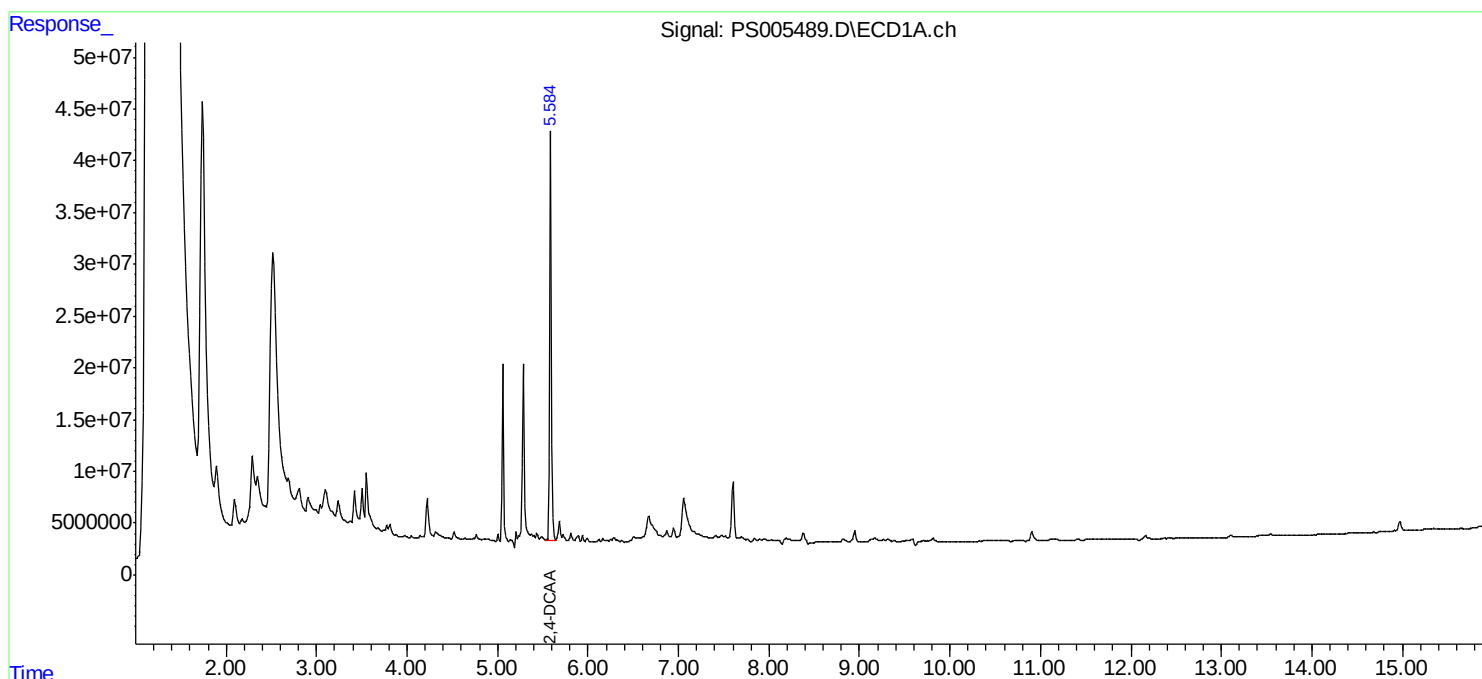

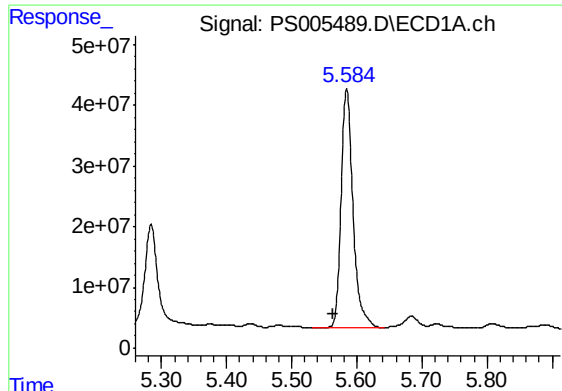


#4 2,4-DCAA

R.T.: 5.584 min
Delta R.T.: 0.021 min
Response: 499659923
Conc: 340.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-071019-B

Manual Integrations
APPROVED

Ankita
7/16/2019 8:42:14 AM

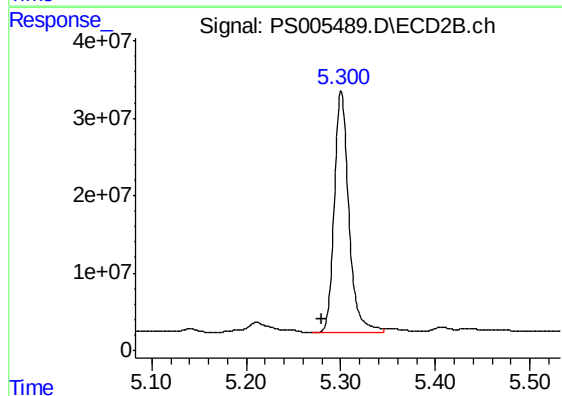

#4 2,4-DCAA

R.T.: 5.300 min
Delta R.T.: 0.020 min
Response: 335500216
Conc: 334.71 ng/ml m